

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110718\
 Data File : PS002365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2018 12:22
 Operator : EI\SJ
 Sample : J5819-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BES48_WC

Manual Integrations
 APPROVED

SOHIL
 11/12/2018 6:15:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 12:50:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	11.423	10.893	34373193	38856121	109.230m	108.205m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110718\
Data File : PS002365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2018 12:22
Operator : EI\SJ
Sample : J5819-09
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
BES48_WC


Manual Integrations
APPROVED

SOHIL
11/12/2018 6:15:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 12:50:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

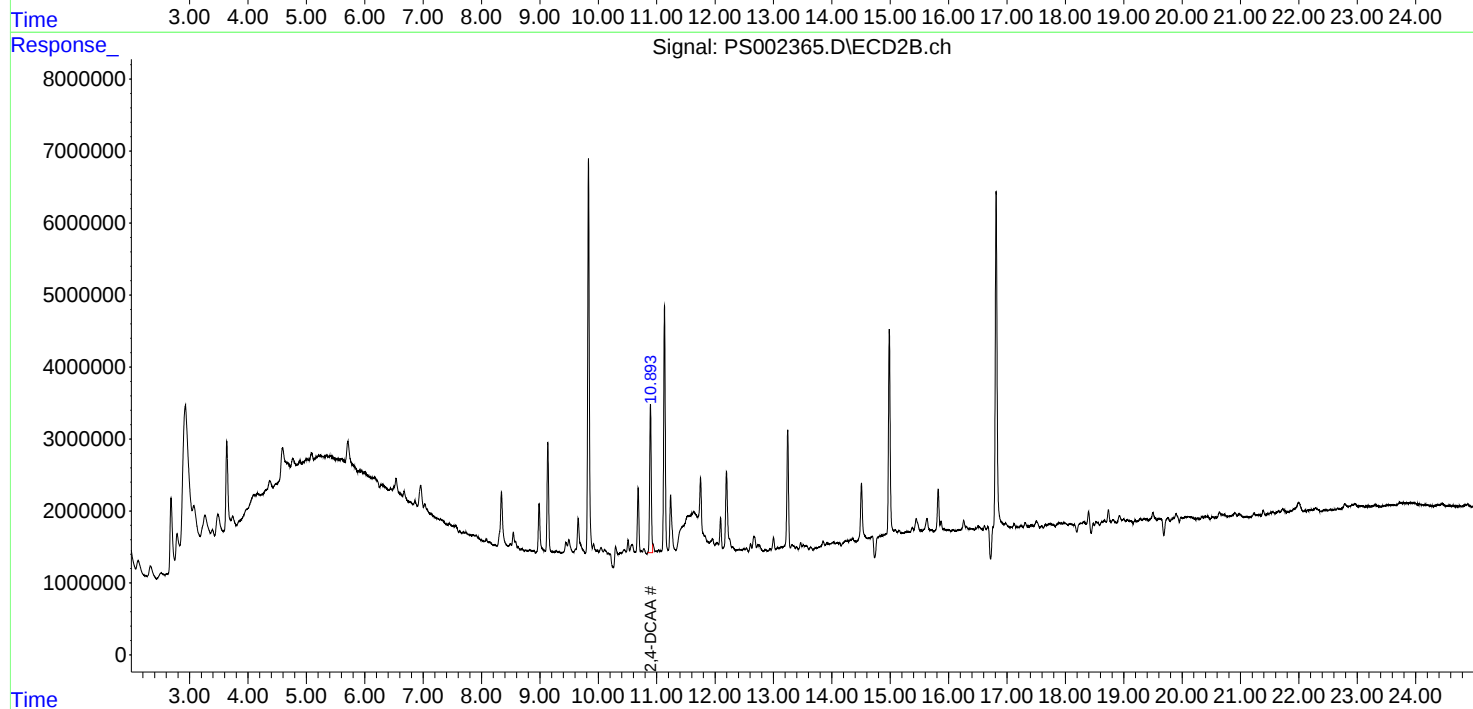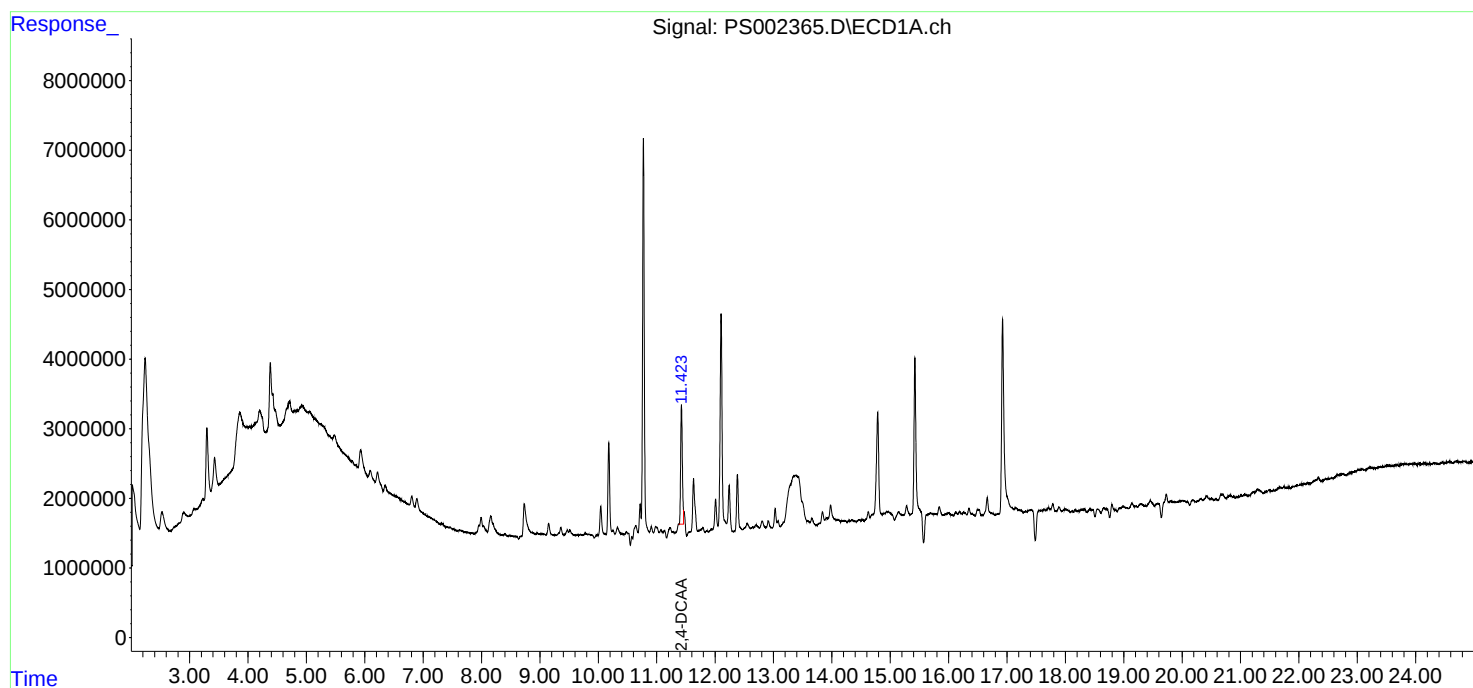

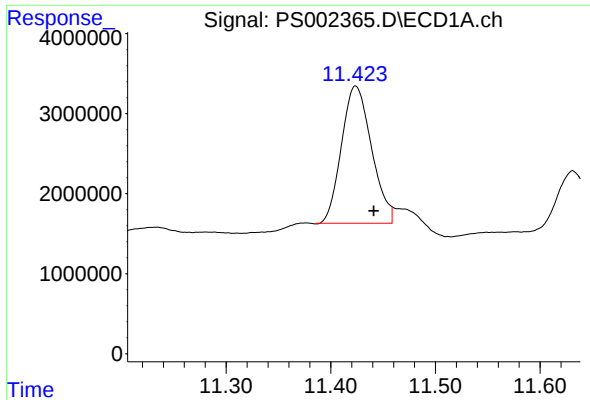


#4 2,4-DCAA

R.T.: 11.423 min
Delta R.T.: -0.018 min
Response: 34373193
Conc: 109.23 ng/ml m

Instrument :
ECD_S
ClientSampleId :
BES48_WC

Manual Integrations
APPROVED

SOHIL
11/12/2018 6:15:29 AM

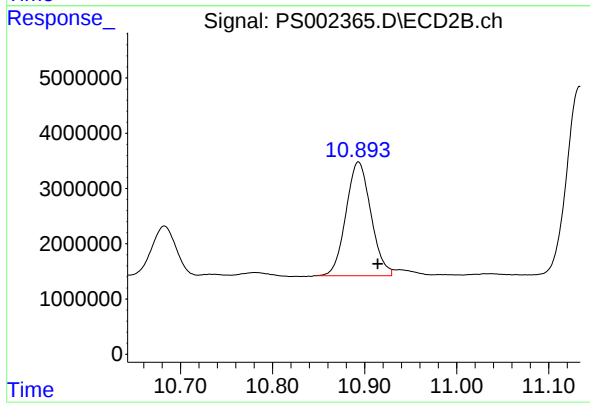

#4 2,4-DCAA

R.T.: 10.893 min
Delta R.T.: -0.022 min
Response: 38856121
Conc: 108.20 ng/ml m