

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110719\
 Data File : PS007633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2019 17:29
 Operator : SM\AJ
 Sample : PB124610BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB124610BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 01:21:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.436	5.159	554.2E6	302.6E6	402.420	430.727
Target Compounds							
1) T	Dalapon	1.998	1.704	104.8E6	254.7E6	57.943	214.531 #
2) T	3,5-DICHL...	0.000	4.493	0	65887952	N.D.	72.931
5) T	DICAMBA	5.526	0.000	34915462	0	6.863	N.D. #
7) T	MCPA	0.000	5.528	0	21351041	N.D.	7.104
9) T	2,4-D	0.000	6.062	0	6823145	N.D.	8.461
10) T	Pentachlo...	0.000	6.371	0	21388739	N.D.	2.184
11) T	2,4,5-TP ...	0.000	6.756	0	25274684	N.D.	6.454
14) T	DINOSEB	0.000	7.949	0	13812884	N.D.	4.751



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110719\
Data File : PS007633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2019 17:29
Operator : SM\AJ
Sample : PB124610BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB124610BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:21:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

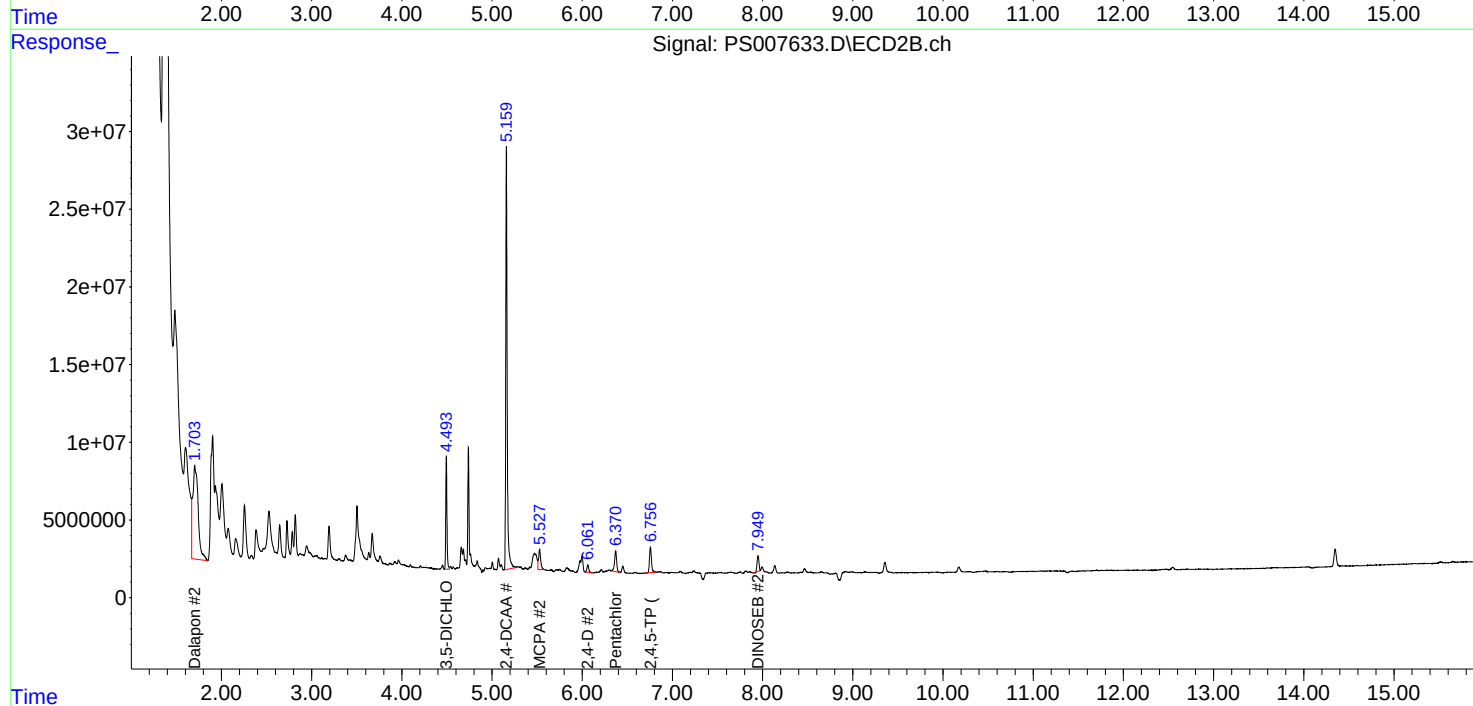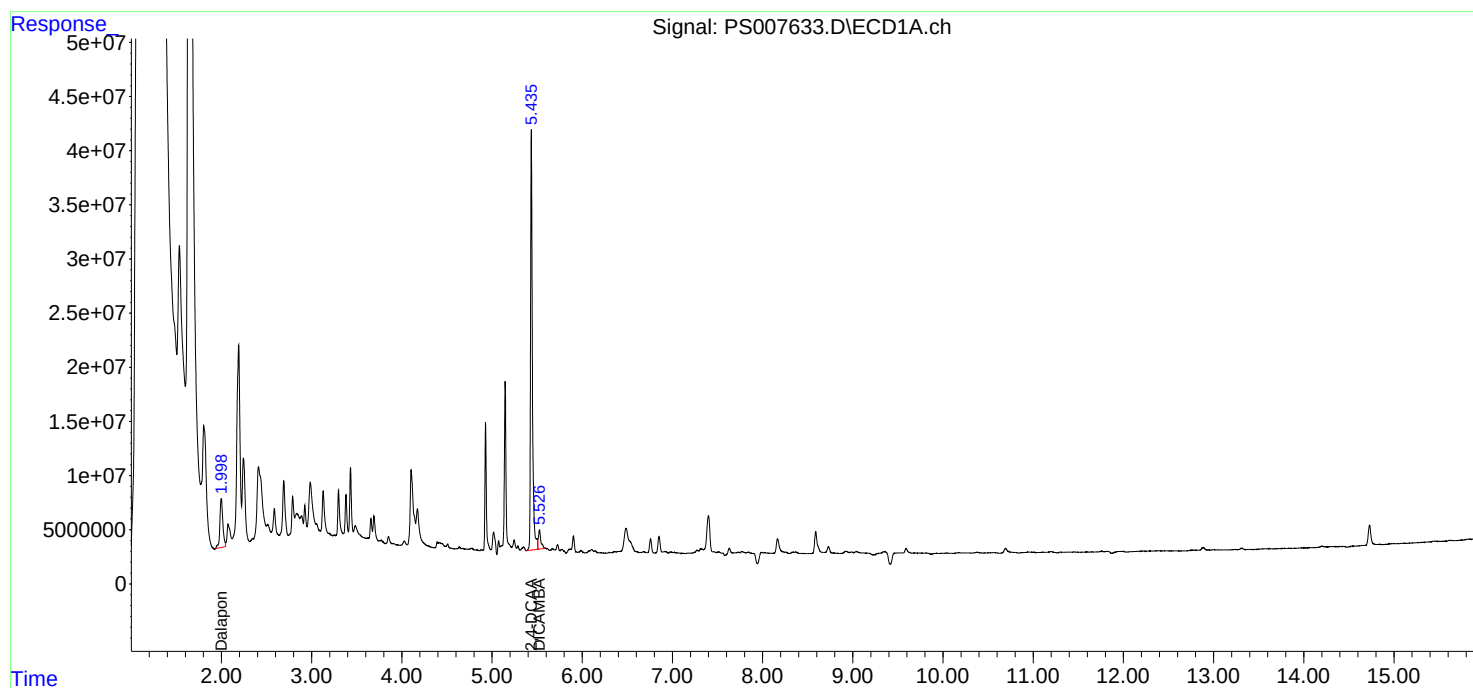


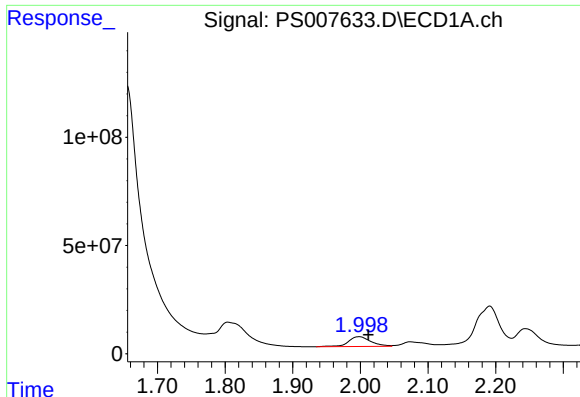

#1 Dalapon


R.T.: 1.998 min
Delta R.T.: -0.014 min
Response: 104829235
Conc: 57.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124610BL

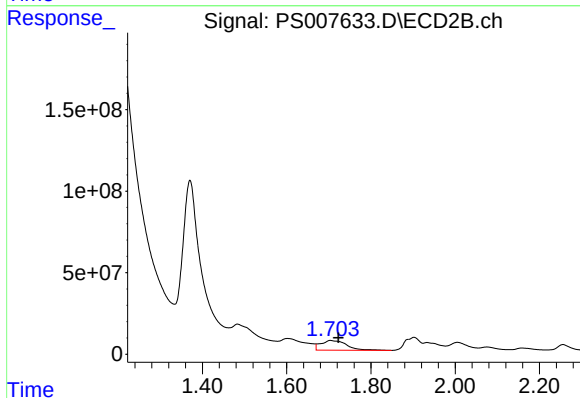


#1 Dalapon

R.T.: 1.704 min
Delta R.T.: -0.019 min
Response: 254734596
Conc: 214.53 ng/ml

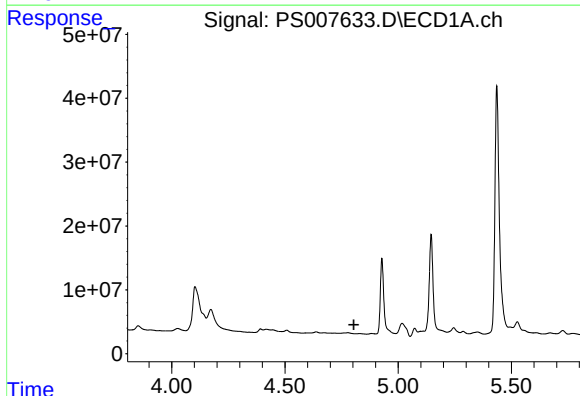


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

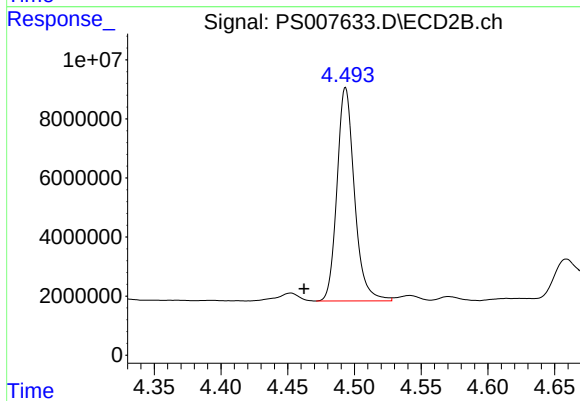

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.493 min
Delta R.T.: 0.031 min
Response: 65887952
Conc: 72.93 ng/ml

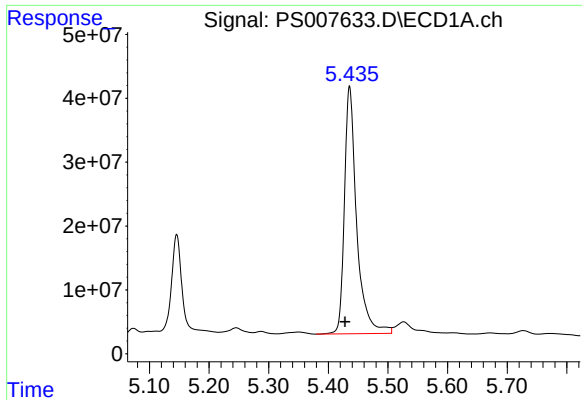

#4 2,4-DCAA


R.T.: 5.436 min
Delta R.T.: 0.007 min
Response: 554206418
Conc: 402.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124610BL

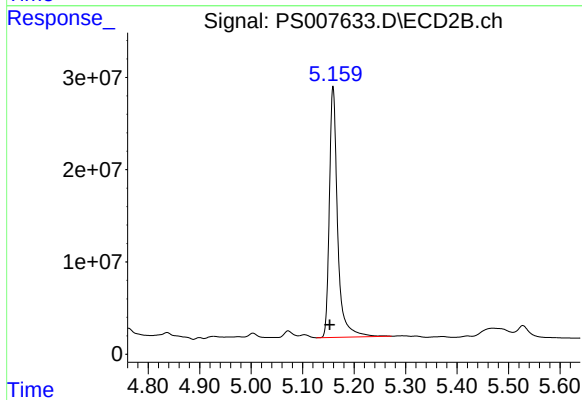


#4 2,4-DCAA

R.T.: 5.159 min
Delta R.T.: 0.007 min
Response: 302613062
Conc: 430.73 ng/ml

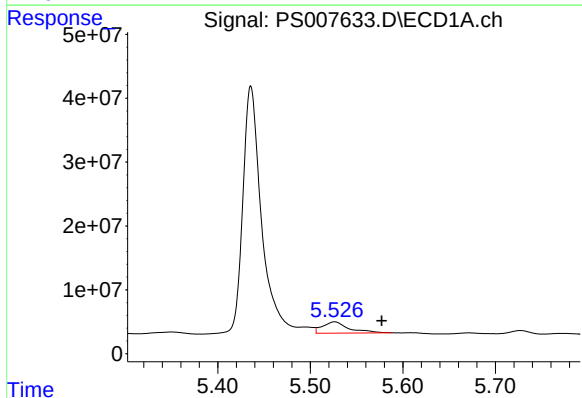


#5 DICAMBA

R.T.: 5.526 min
Delta R.T.: -0.051 min
Response: 34915462
Conc: 6.86 ng/ml

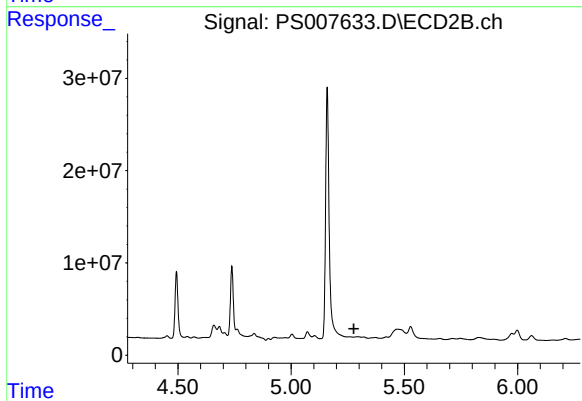

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

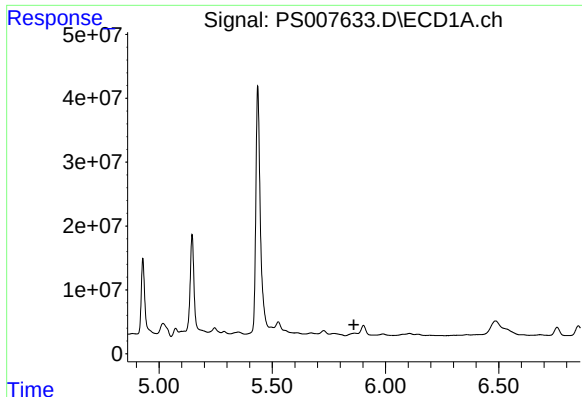

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.860 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124610BL

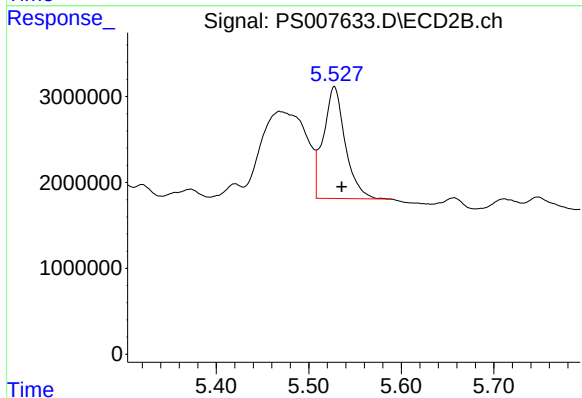


#7 MCPA

R.T.: 5.528 min
Delta R.T.: -0.008 min
Response: 21351041
Conc: 7.10 ug/ml

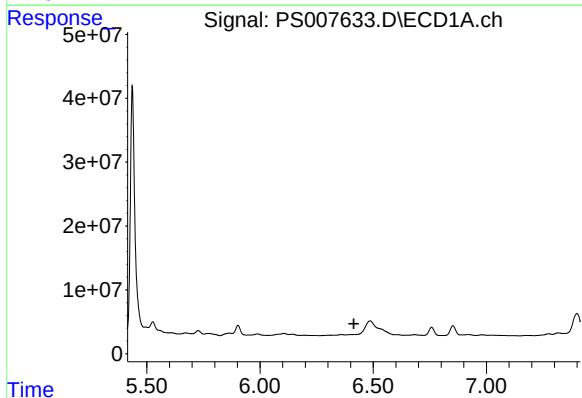


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.414 min
Response: 0
Conc: N.D.

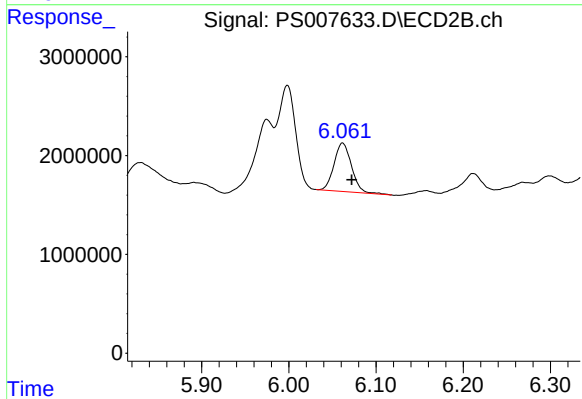

#9 2,4-D


R.T.: 6.062 min
Delta R.T.: -0.010 min
Response: 6823145
Conc: 8.46 ng/ml

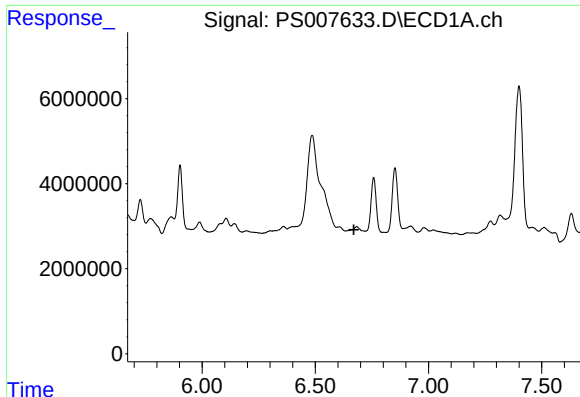

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124610BL

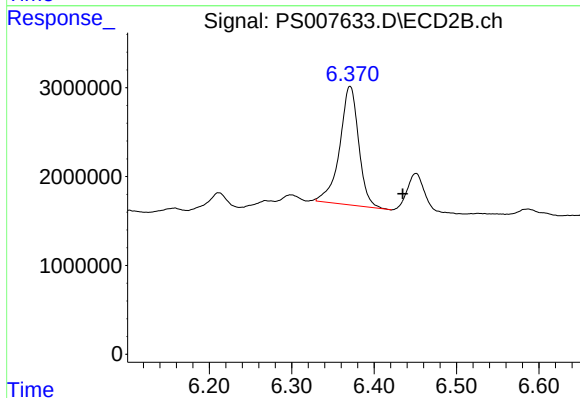


#10 Pentachlorophenol

R.T.: 6.371 min
Delta R.T.: -0.064 min
Response: 21388739
Conc: 2.18 ng/ml

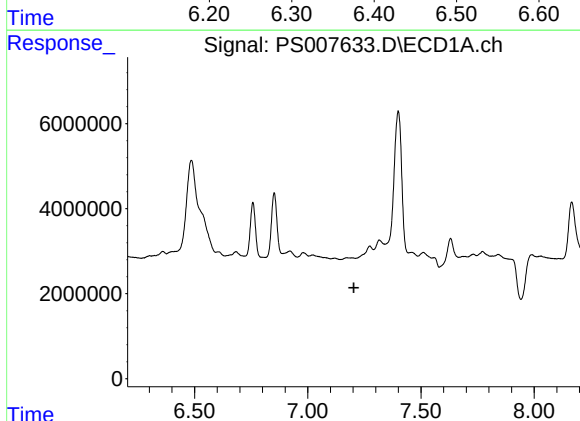


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

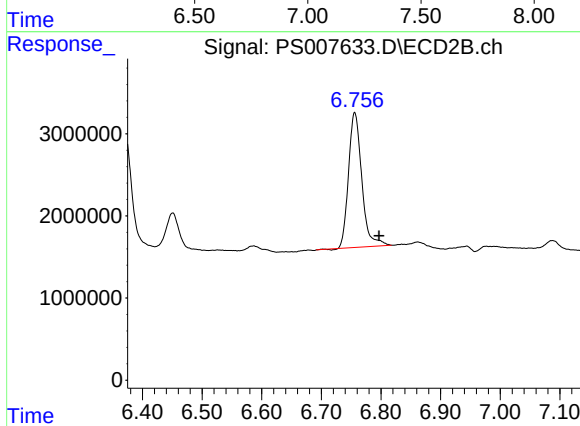

#11 2,4,5-TP (SILVEX)


R.T.: 6.756 min
Delta R.T.: -0.041 min
Response: 25274684
Conc: 6.45 ng/ml

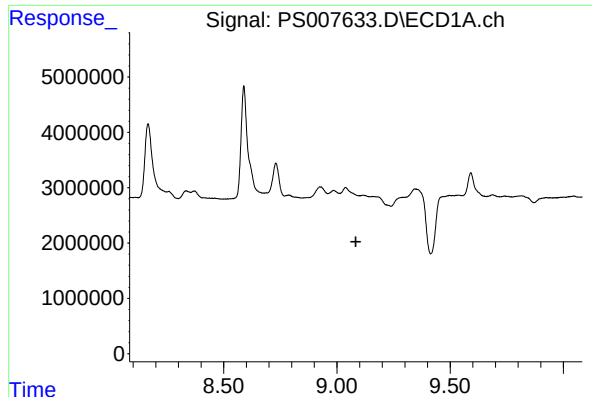

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124610BL

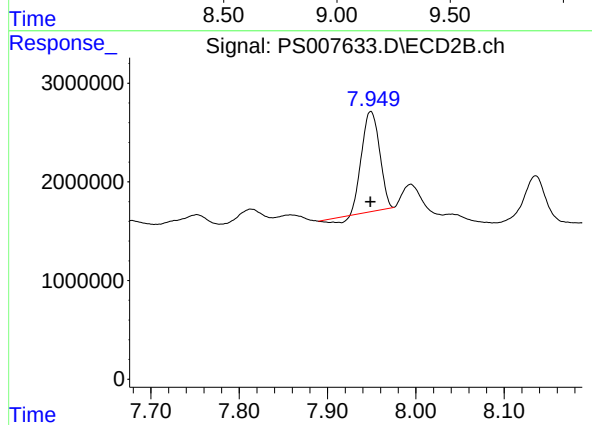

#14 DINOSEB

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 13812884
Conc: 4.75 ng/ml