

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110723\
 Data File : PS024782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 13:00
 Operator : AR\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 14:31:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.357	6.776	1519.7E6	502.8E6	744.422	745.307
Target Compounds							
1) T	Dalapon	2.480	2.539	1667.5E6	712.0E6	692.226	675.794
2) T	3,5-DICHL...	5.732	5.964	2173.1E6	746.3E6	692.779	697.036
3) T	4-Nitroph...	6.195	6.391	895.4E6	299.5E6	690.762	681.970
5) T	DICAMBA	6.499	6.937	6372.4E6	2076.3E6	712.190	714.599
6) T	MCPD	6.650	7.034	448.4E6	140.0E6	71.979	72.142
7) T	MCPA	6.772	7.240	617.9E6	212.0E6	70.435	68.765
8) T	DICHLORPROP	7.086	7.551	1637.4E6	516.6E6	699.886	707.237
9) T	2,4-D	7.284	7.834	1926.8E6	632.4E6	700.954	706.450
10) T	Pentachlo...	7.512	8.258	23843.8E6	7670.3E6	731.922	721.803
11) T	2,4,5-TP ...	8.034	8.616	9968.0E6	2970.0E6	716.910	722.589
12) T	2,4,5-T	8.289	8.986	9362.7E6	2878.2E6	716.064	721.324
13) T	2,4-DB	8.795	9.489	1505.1E6	362.6E6	715.751	743.698
14) T	DINOSEB	9.847	9.817	7078.7E6	2077.0E6	717.774	728.482
15) T	Picloram	9.673	10.767	12506.0E6	4261.3E6	703.107	701.325
16) T	DCPA	10.113	10.738	12321.5E6	3701.8E6	720.006	736.575



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110723\
Data File : PS024782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 13:00
Operator : AR\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 14:31:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

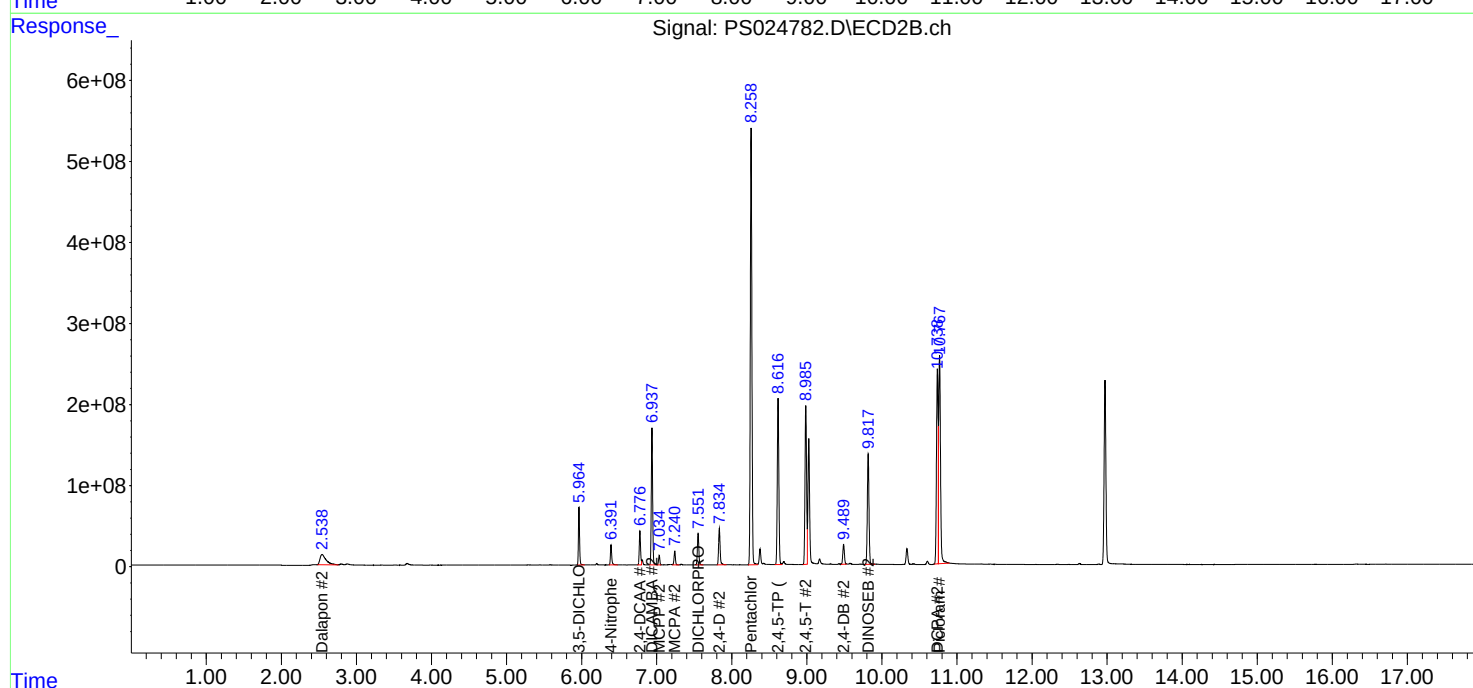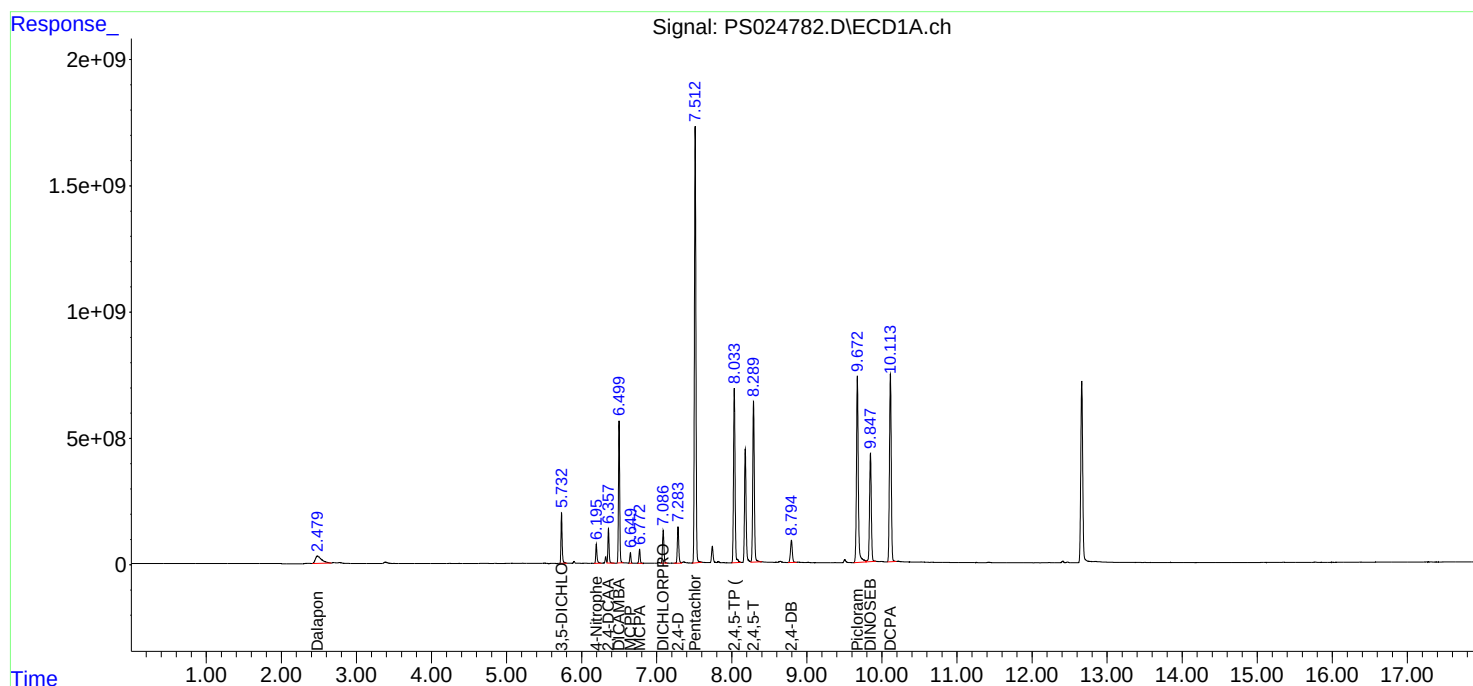


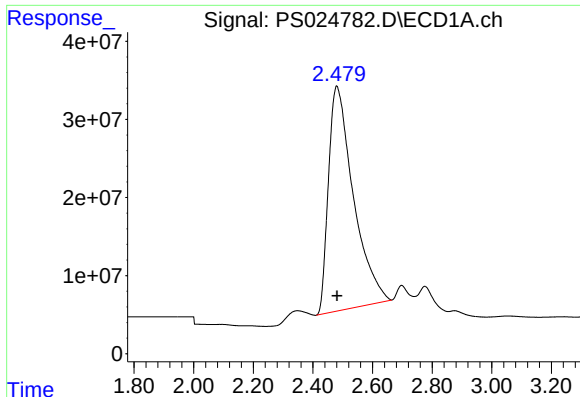

#1 Dalapon


R.T.: 2.480 min
Delta R.T.: -0.001 min
Response: 1667525354
Conc: 692.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

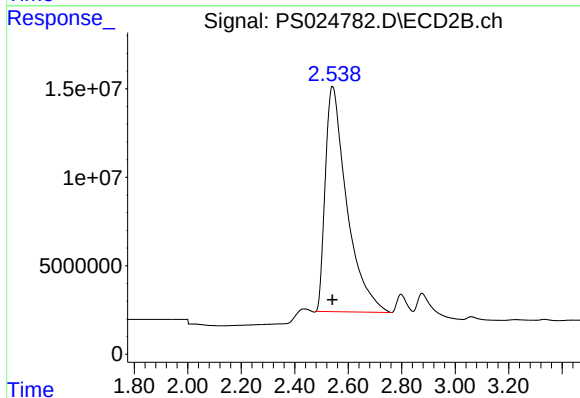


#1 Dalapon

R.T.: 2.539 min
Delta R.T.: -0.001 min
Response: 711986369
Conc: 675.79 ng/ml

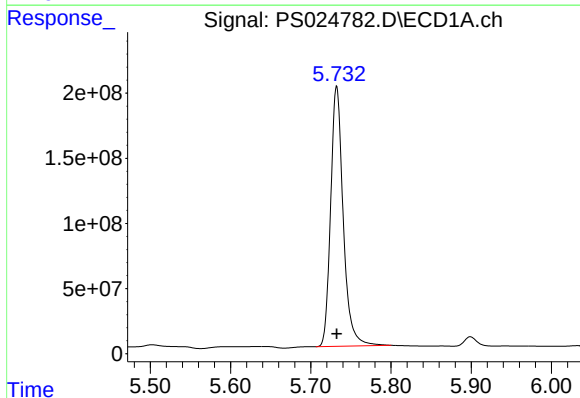


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.732 min
Delta R.T.: 0.000 min
Response: 2173101769
Conc: 692.78 ng/ml

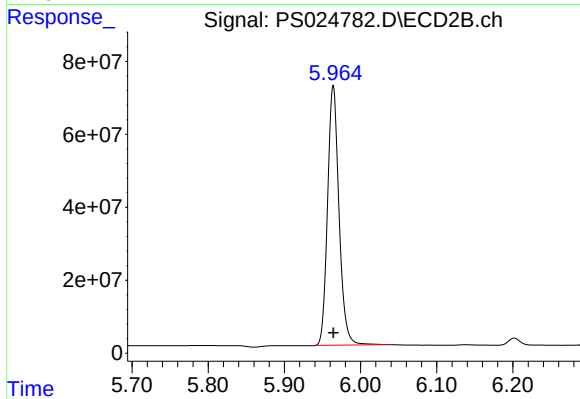

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.964 min
Delta R.T.: 0.000 min
Response: 746285270
Conc: 697.04 ng/ml

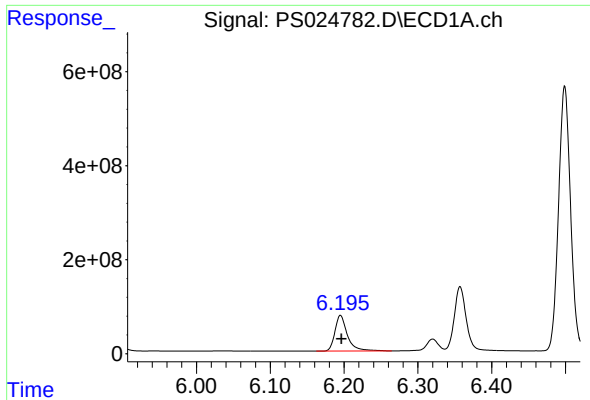

#3 4-Nitrophenol


R.T.: 6.195 min
Delta R.T.: -0.001 min
Response: 895380271
Conc: 690.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

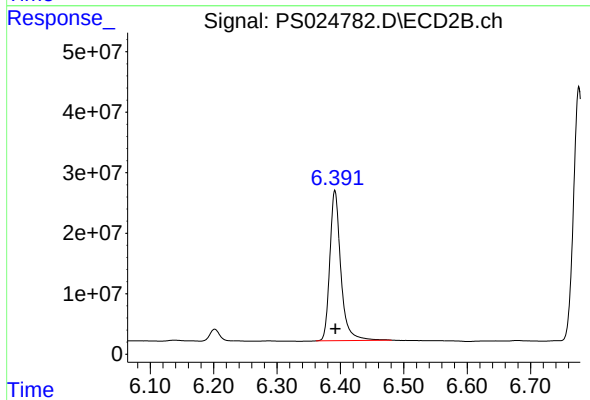


#3 4-Nitrophenol

R.T.: 6.391 min
Delta R.T.: 0.000 min
Response: 299450718
Conc: 681.97 ng/ml

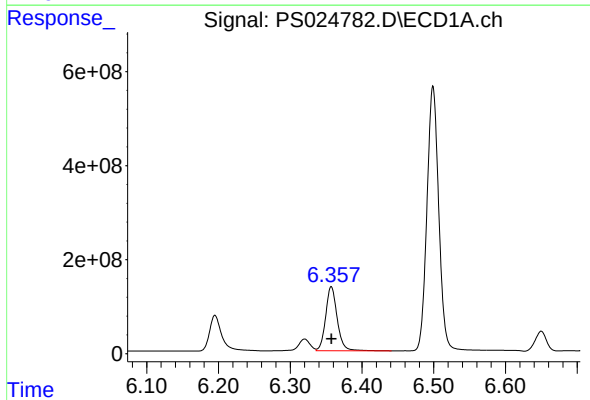


#4 2,4-DCAA

R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 1519740259
Conc: 744.42 ng/ml

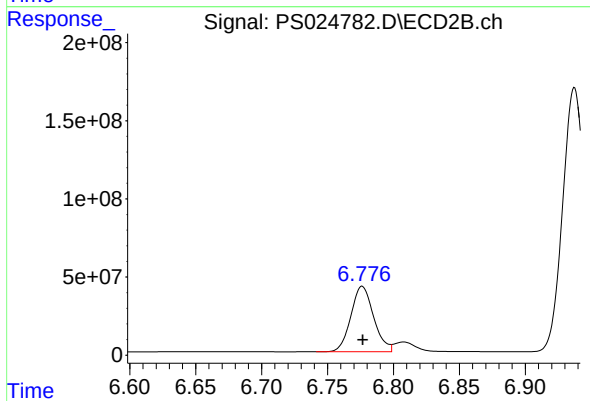

#4 2,4-DCAA


R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 502783119
Conc: 745.31 ng/ml

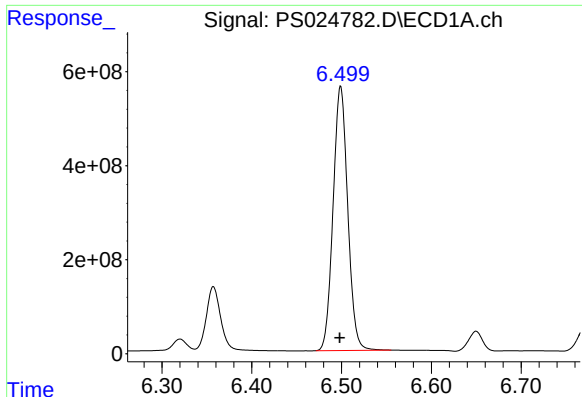

#5 DICAMBA


R.T.: 6.499 min
Delta R.T.: 0.000 min
Response: 6372426508
Conc: 712.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

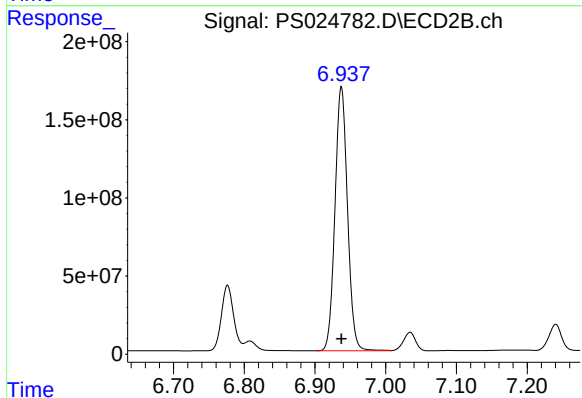


#5 DICAMBA

R.T.: 6.937 min
Delta R.T.: 0.000 min
Response: 2076274029
Conc: 714.60 ng/ml

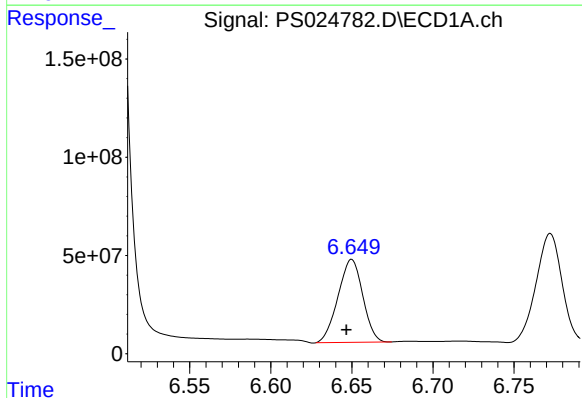


#6 MCP

R.T.: 6.650 min
Delta R.T.: 0.003 min
Response: 448427495
Conc: 71.98 ug/ml

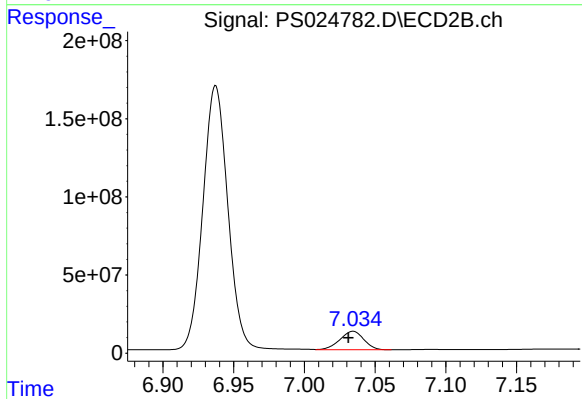

#6 MCP


R.T.: 7.034 min
Delta R.T.: 0.003 min
Response: 139980218
Conc: 72.14 ug/ml

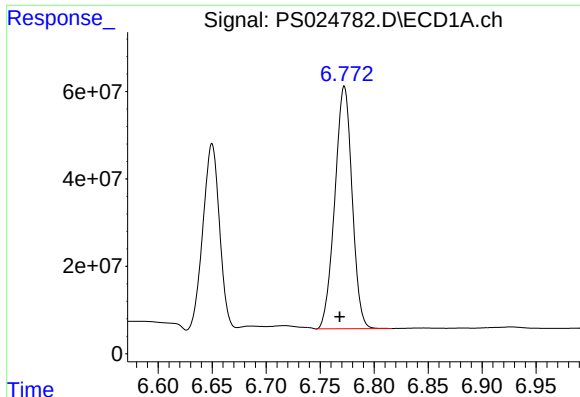

#7 MCPA


R.T.: 6.772 min
Delta R.T.: 0.004 min
Response: 617936330
Conc: 70.43 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

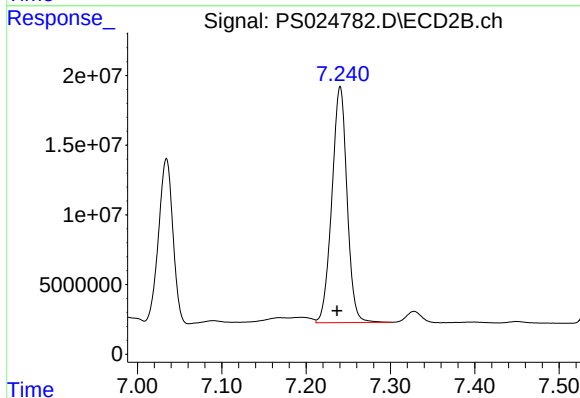


#7 MCPA

R.T.: 7.240 min
Delta R.T.: 0.004 min
Response: 212000678
Conc: 68.77 ug/ml

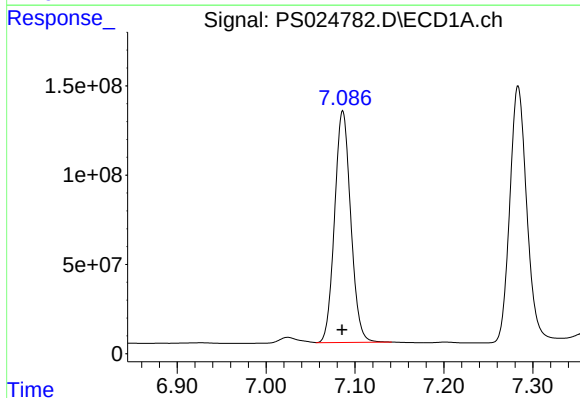


#8 DICHLORPROP

R.T.: 7.086 min
Delta R.T.: 0.000 min
Response: 1637395763
Conc: 699.89 ng/ml

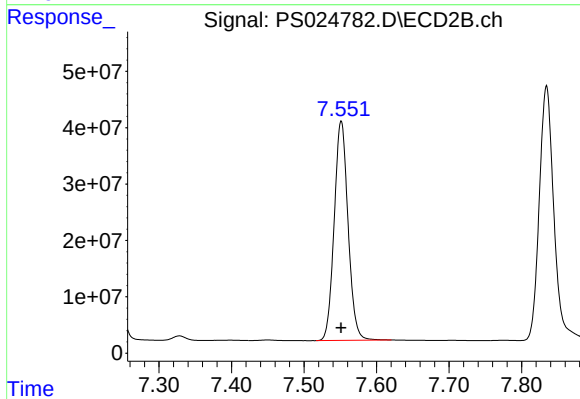

#8 DICHLORPROP


R.T.: 7.551 min
Delta R.T.: 0.000 min
Response: 516638669
Conc: 707.24 ng/ml

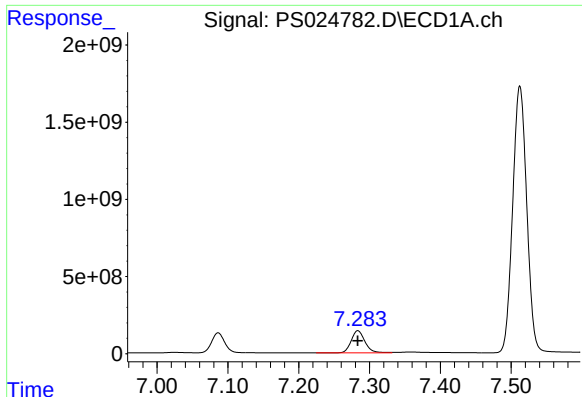

#9 2,4-D


R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 1926785816
Conc: 700.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

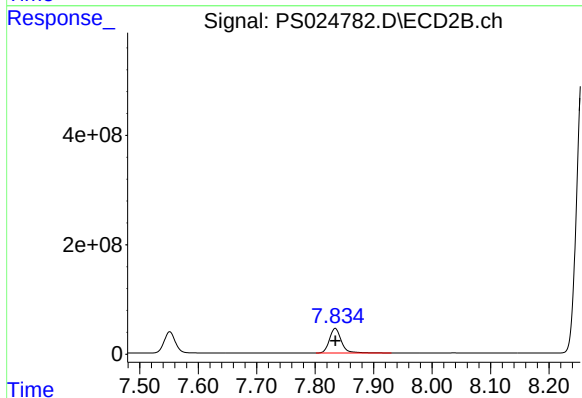


#9 2,4-D

R.T.: 7.834 min
Delta R.T.: 0.000 min
Response: 632356774
Conc: 706.45 ng/ml

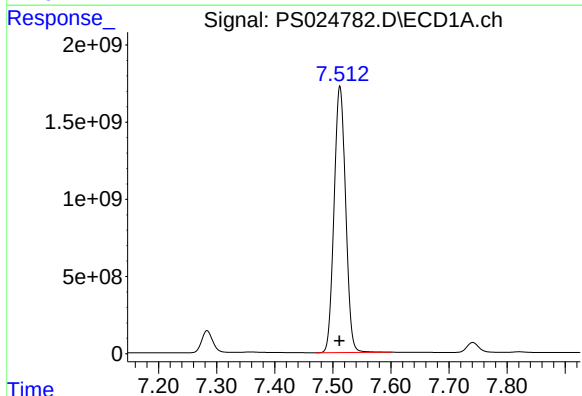


#10 Pentachlorophenol

R.T.: 7.512 min
Delta R.T.: 0.000 min
Response: 23843813771
Conc: 731.92 ng/ml

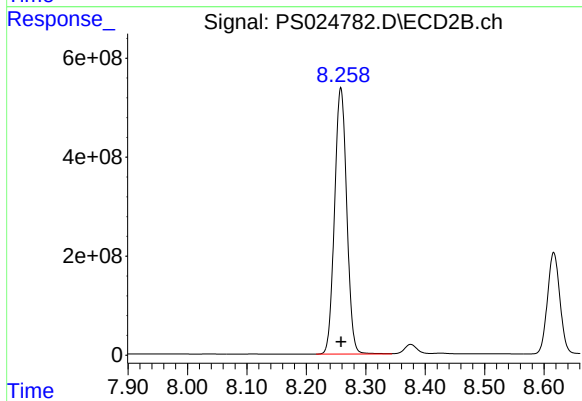

#10 Pentachlorophenol


R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 7670346147
Conc: 721.80 ng/ml

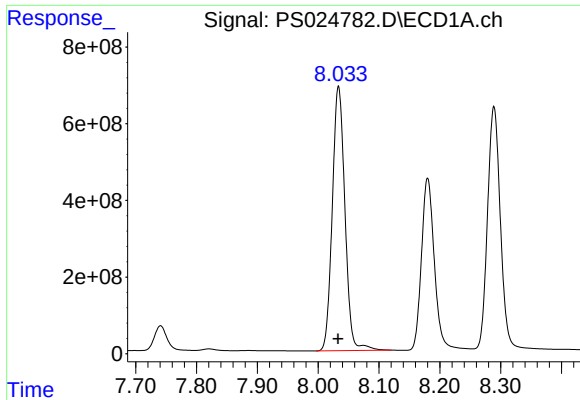

#11 2,4,5-TP (SILVEX)


R.T.: 8.034 min
Delta R.T.: 0.000 min
Response: 9968018811
Conc: 716.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

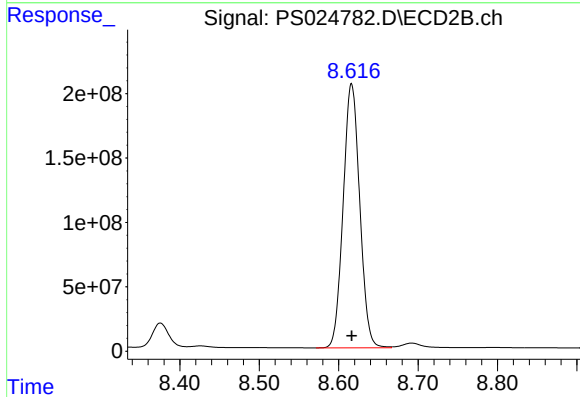


#11 2,4,5-TP (SILVEX)

R.T.: 8.616 min
Delta R.T.: 0.000 min
Response: 2969991217
Conc: 722.59 ng/ml

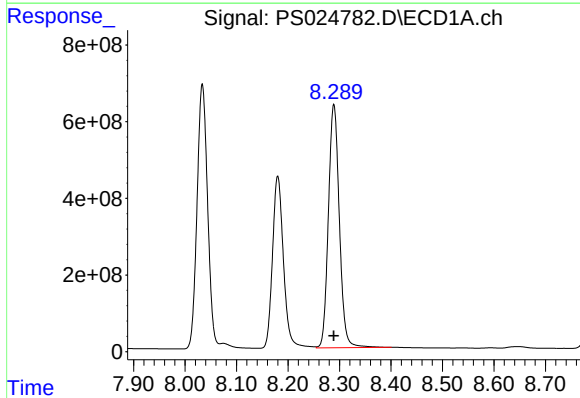


#12 2,4,5-T

R.T.: 8.289 min
Delta R.T.: 0.000 min
Response: 9362706650
Conc: 716.06 ng/ml

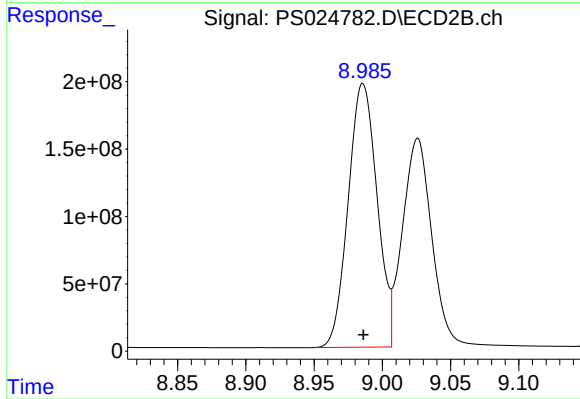

#12 2,4,5-T


R.T.: 8.986 min
Delta R.T.: 0.000 min
Response: 2878164729
Conc: 721.32 ng/ml

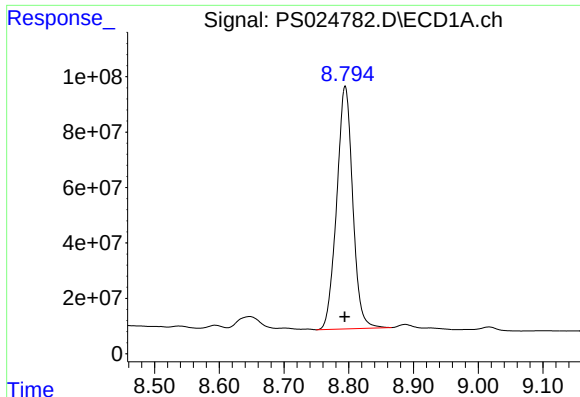

#13 2,4-DB


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 1505116192
Conc: 715.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

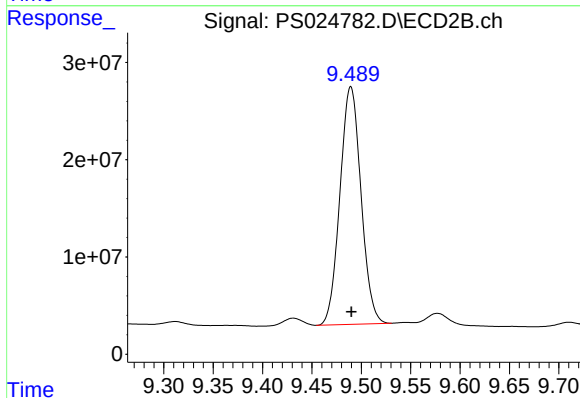


#13 2,4-DB

R.T.: 9.489 min
Delta R.T.: 0.000 min
Response: 362595530
Conc: 743.70 ng/ml

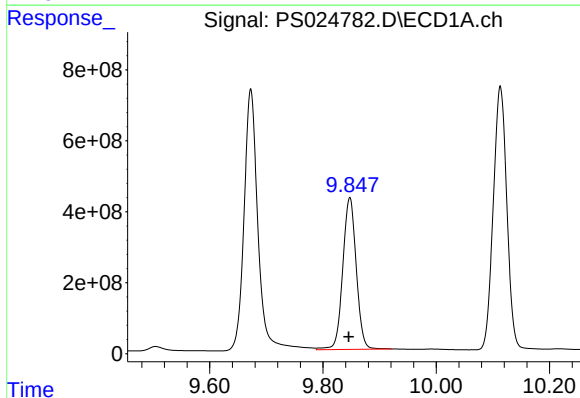


#14 DINOSEB

R.T.: 9.847 min
Delta R.T.: 0.002 min
Response: 7078738982
Conc: 717.77 ng/ml

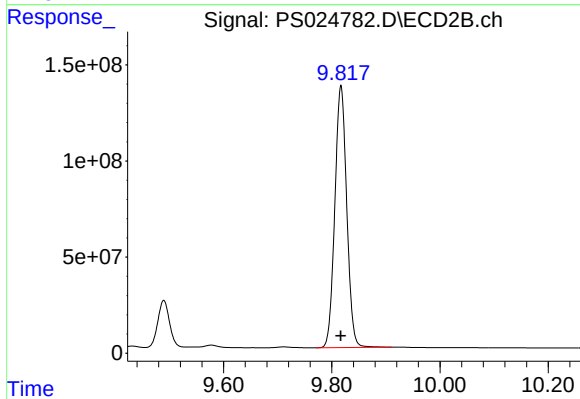

#14 DINOSEB


R.T.: 9.817 min
Delta R.T.: 0.000 min
Response: 2076991049
Conc: 728.48 ng/ml

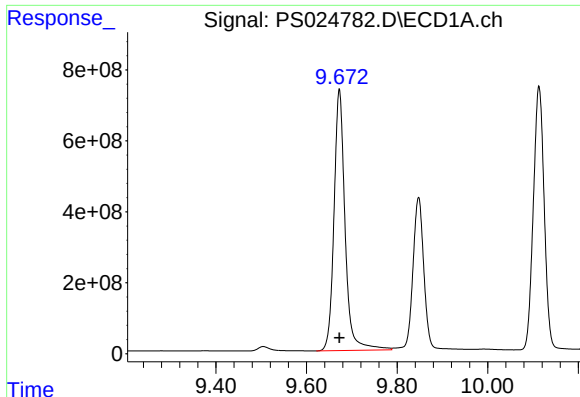

#15 Picloram


R.T.: 9.673 min
Delta R.T.: 0.000 min
Response: 12506007081
Conc: 703.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

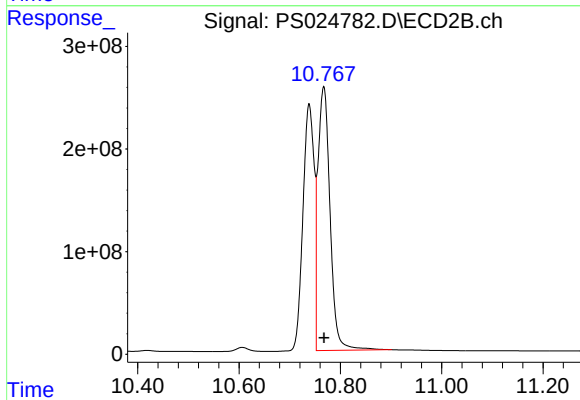


#15 Picloram

R.T.: 10.767 min
Delta R.T.: 0.000 min
Response: 4261253436
Conc: 701.33 ng/ml

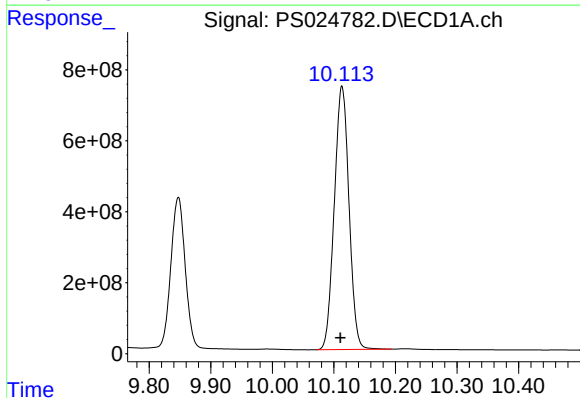

#16 DCPA

R.T.: 10.113 min
Delta R.T.: 0.002 min
Response: 12321465330
Conc: 720.01 ng/ml

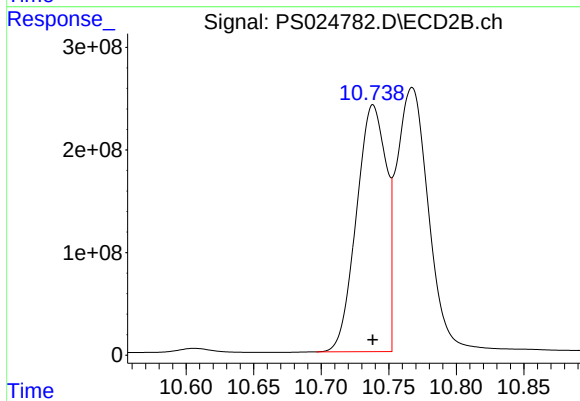

#16 DCPA

R.T.: 10.738 min
Delta R.T.: 0.000 min
Response: 3701772965
Conc: 736.58 ng/ml