

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
 Data File : PS028245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 06:36
 Operator : AR\AJ
 Sample : PB164393TB
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 06:39:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 00:14:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.264	7.766	489.7E6	275.6E6	271.583	176.248 #
Target Compounds							
1) T	Dalapon	2.618f	2.683f	49978168	383.0E6	15.688	138.380 #
2) T	3,5-DICHL...	6.419	6.747f	9751582	4104162	3.479	1.752 #
3) T	4-Nitroph...	7.051	0.000	5225825	0	4.409	N.D. #
5) T	DICAMBA	7.487f	7.953	-1152575	4225772	N.D.	<MDL
6) T	MCPD	7.626	8.063	4163418	4310239	<MDL	<MDL #
7) T	MCPA	0.000	8.301	0	28054681	N.D.	3.911
8) T	DICHLORPROP	8.179	0.000	9730526	0	5.386	N.D. #
9) T	2,4-D	0.000	9.011	0	4362034	N.D.	2.237
10) T	Pentachlo...	8.697	9.557	11064812	10682944	<MDL	<MDL #
11) T	2,4,5-TP ...	9.279	9.936	2447634	15537246	<MDL	1.445 #
12) T	2,4,5-T	0.000	10.323	0	45501561	N.D.	4.253
13) T	2,4-DB	10.164	10.957f	22246409	-826679	13.490	N.D. #
14) T	DINOSEB	11.383	11.260f	21375166	3284555	2.845	<MDL #
15) T	Picloram	11.166	12.393	50417659	24925740	2.889	1.518 #
16) T	DCPA	11.633f	12.347	31614202	11588696	2.539	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
Data File : PS028245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 06:36
Operator : AR\AJ
Sample : PB164393TB
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 06:39:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 00:14:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

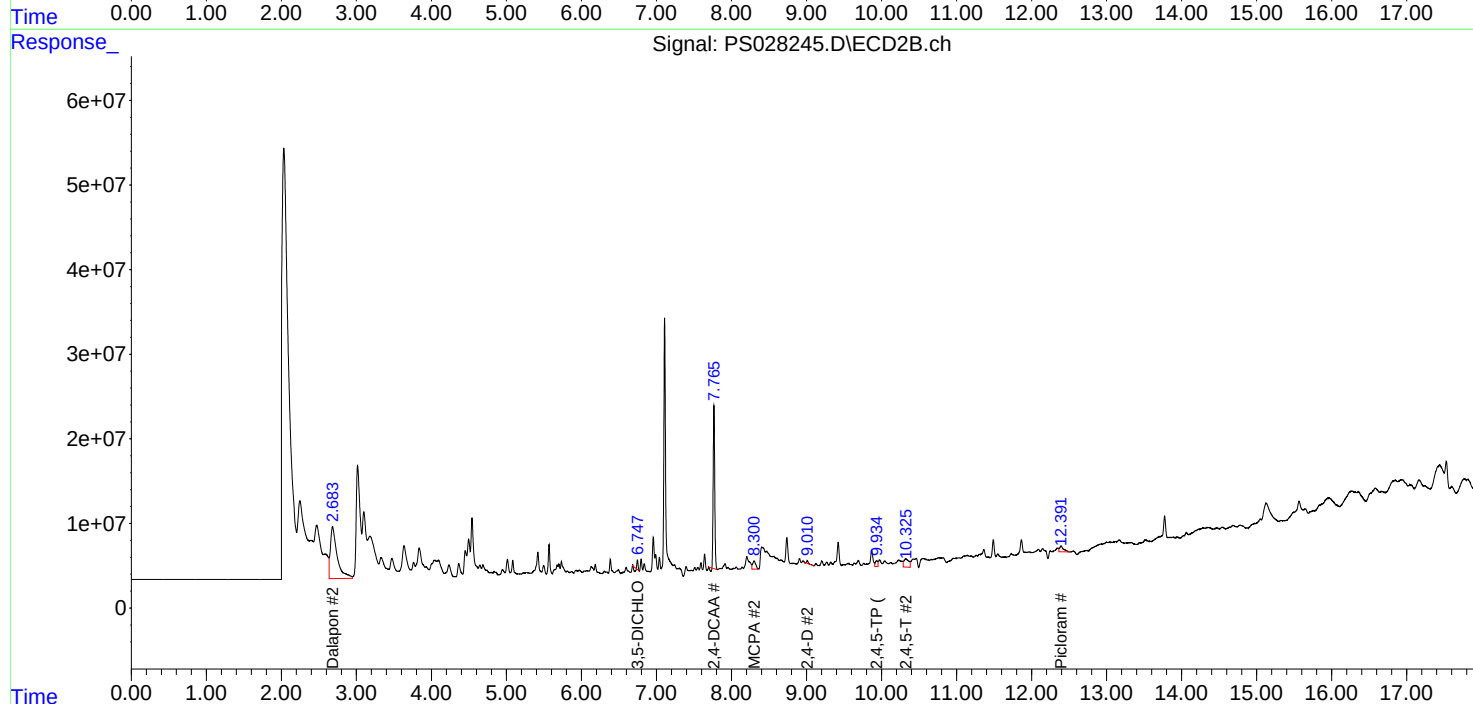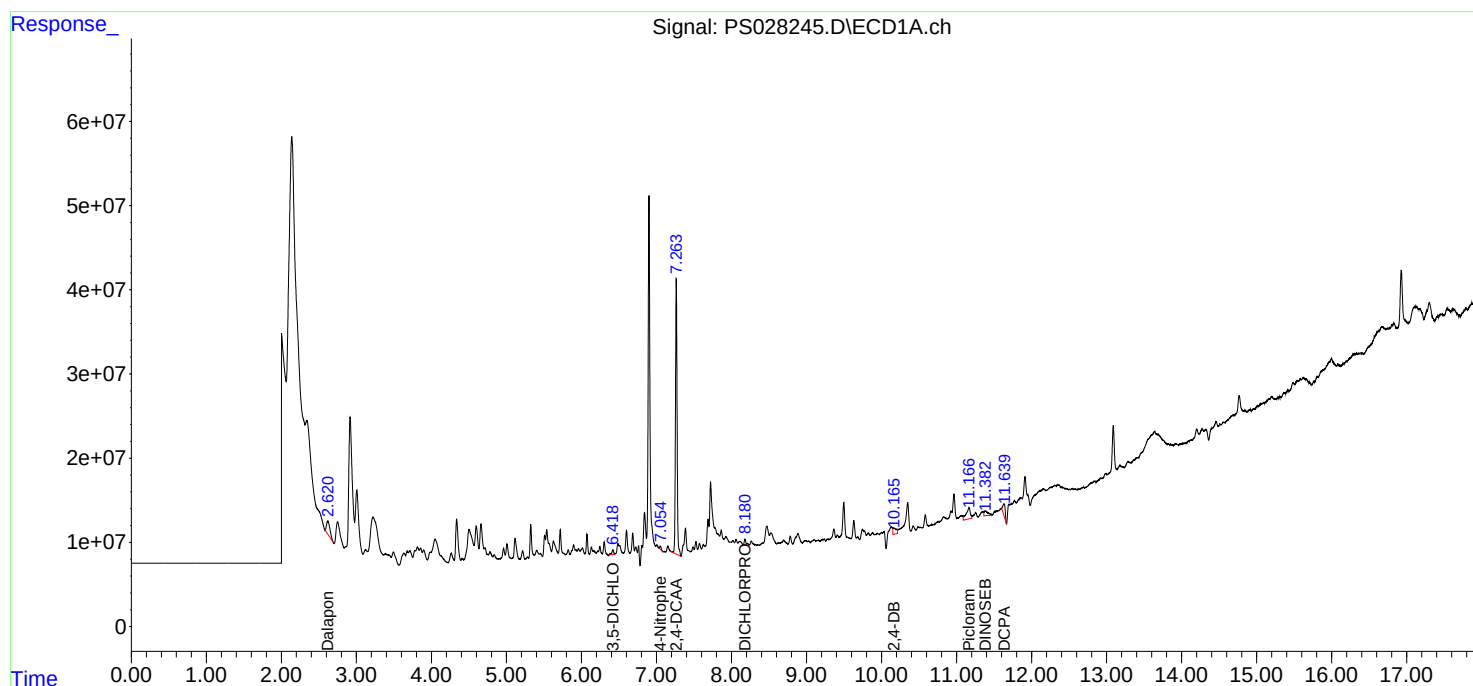


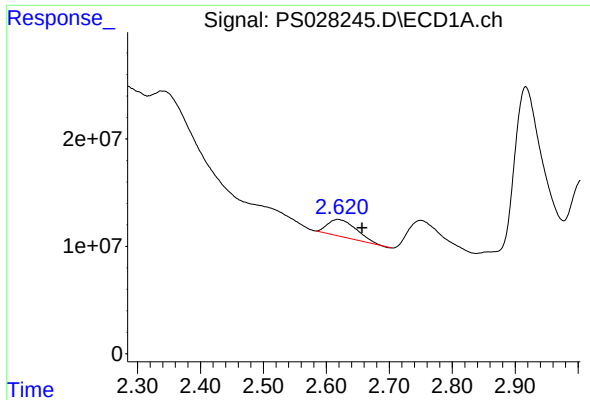

#1 Dalapon


R.T.: 2.618 min
Delta R.T.: -0.039 min
Response: 49978168
Conc: 15.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

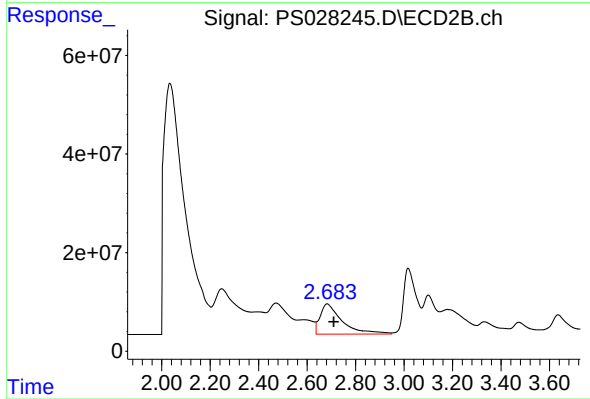


#1 Dalapon

R.T.: 2.683 min
Delta R.T.: -0.028 min
Response: 382982329
Conc: 138.38 ng/ml

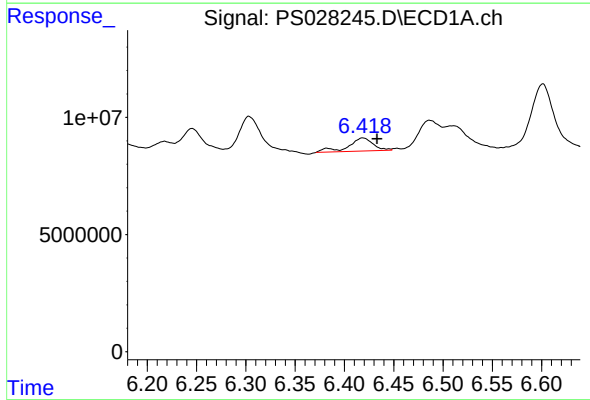


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.419 min
Delta R.T.: -0.014 min
Response: 9751582
Conc: 3.48 ng/ml

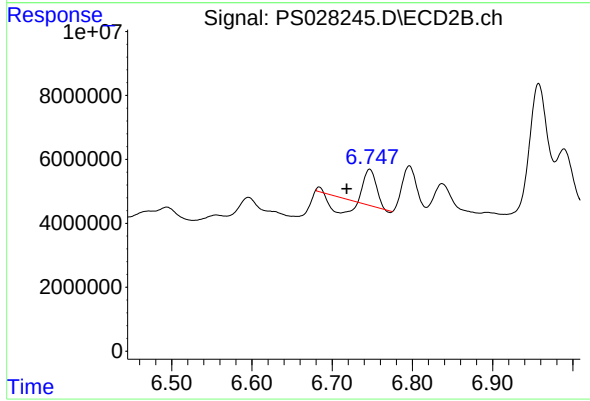

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.747 min
Delta R.T.: 0.029 min
Response: 4104162
Conc: 1.75 ng/ml

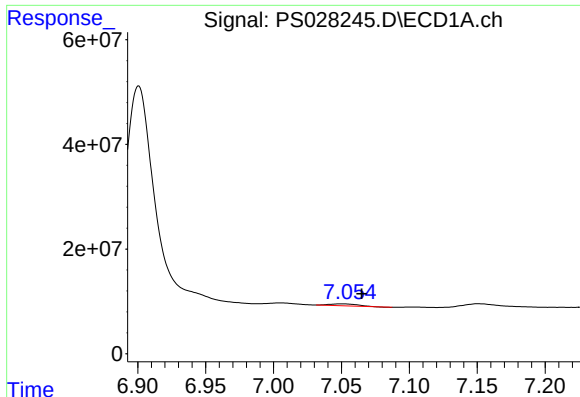

#3 4-Nitrophenol


R.T.: 7.051 min
Delta R.T.: -0.014 min
Response: 5225825
Conc: 4.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

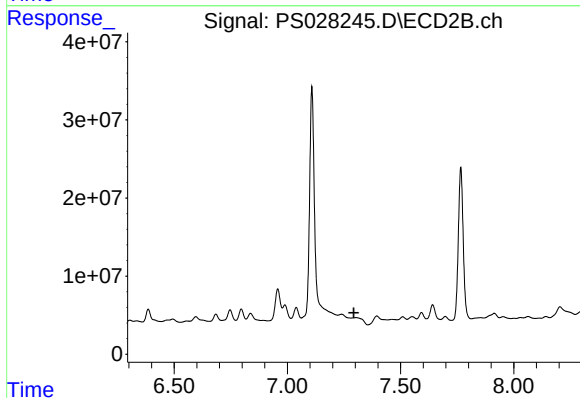


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.293 min
Response: 0
Conc: N.D.

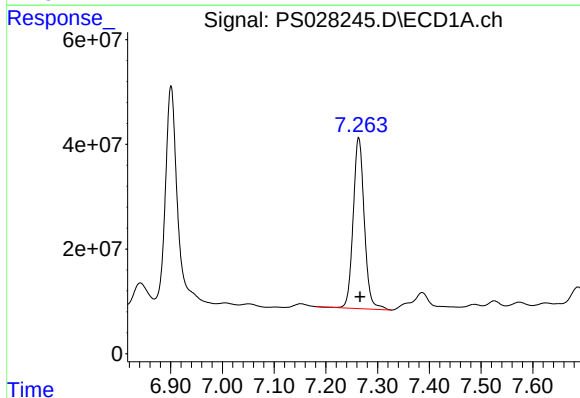


#4 2,4-DCAA

R.T.: 7.264 min
Delta R.T.: -0.002 min
Response: 489672701
Conc: 271.58 ng/ml

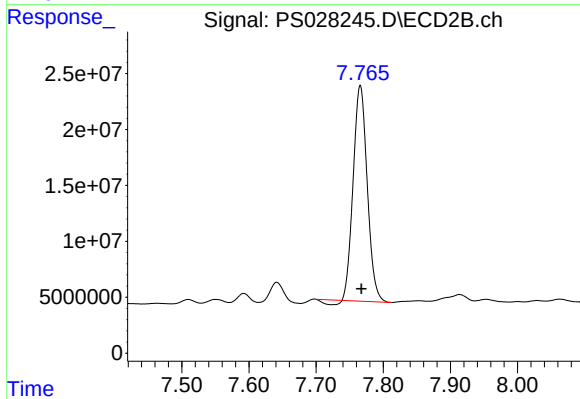

#4 2,4-DCAA


R.T.: 7.766 min
Delta R.T.: -0.002 min
Response: 275632568
Conc: 176.25 ng/ml

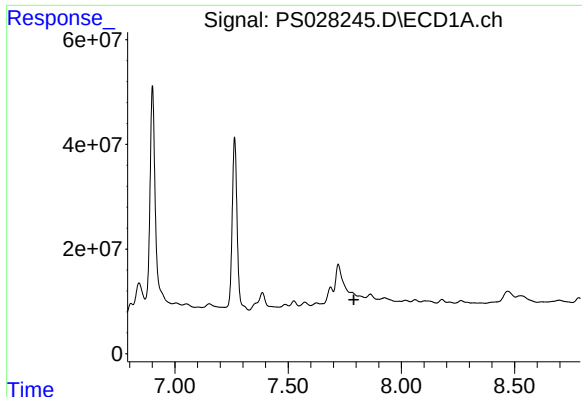

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

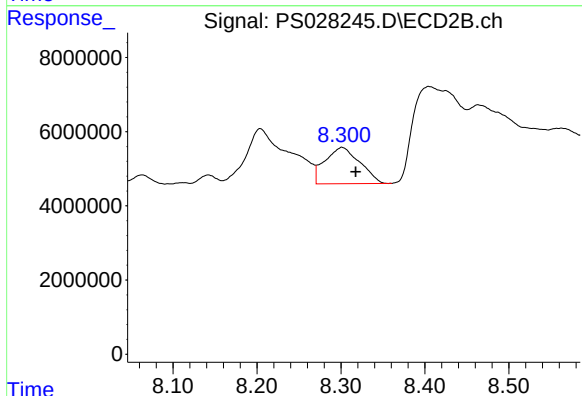


#7 MCPA

R.T.: 8.301 min
Delta R.T.: -0.016 min
Response: 28054681
Conc: 3.91 ug/ml

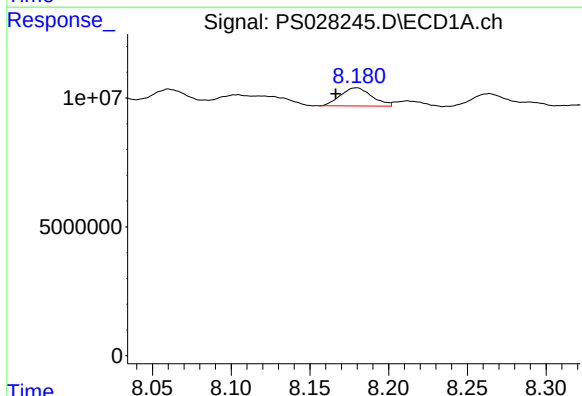


#8 DICHLORPROP

R.T.: 8.179 min
Delta R.T.: 0.013 min
Response: 9730526
Conc: 5.39 ng/ml

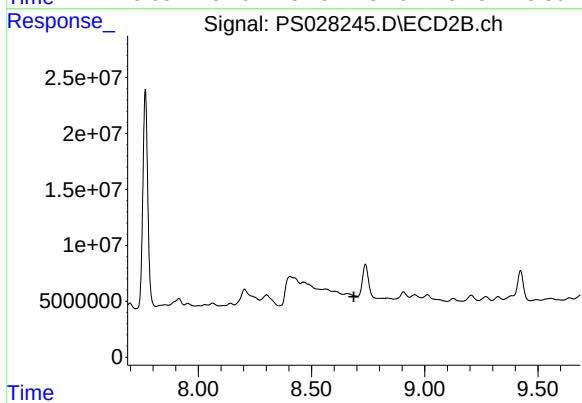

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.687 min
Response: 0
Conc: N.D.

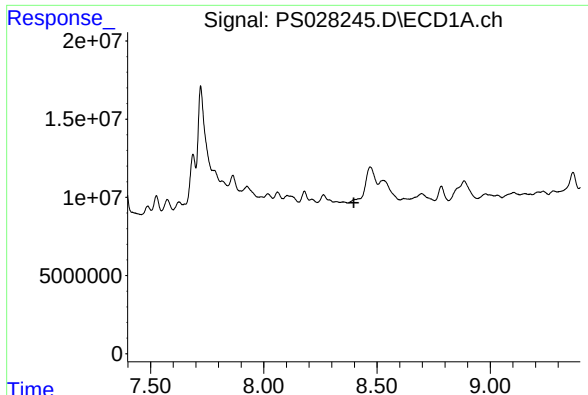

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

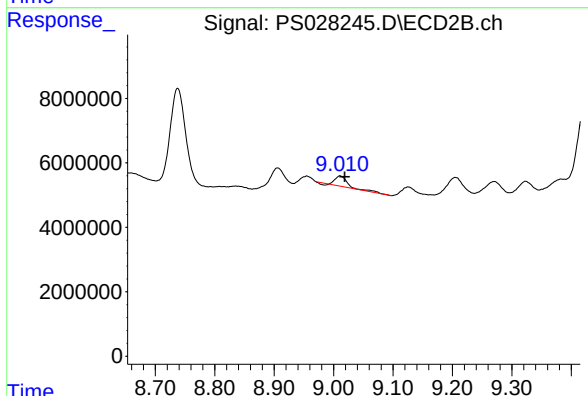


#9 2,4-D

R.T.: 9.011 min
Delta R.T.: -0.007 min
Response: 4362034
Conc: 2.24 ng/ml

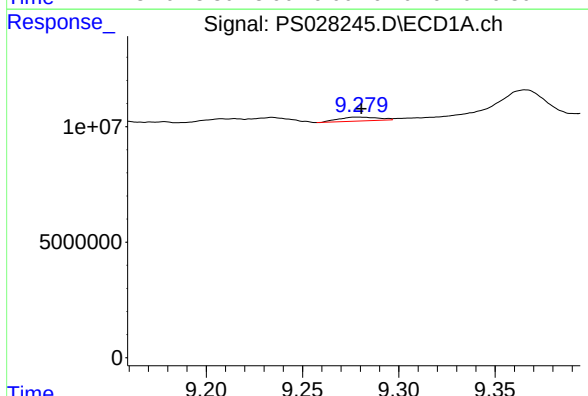


#11 2,4,5-TP (SILVEX)

R.T.: 9.279 min
Delta R.T.: -0.001 min
Response: 2447634
Conc: N.D.

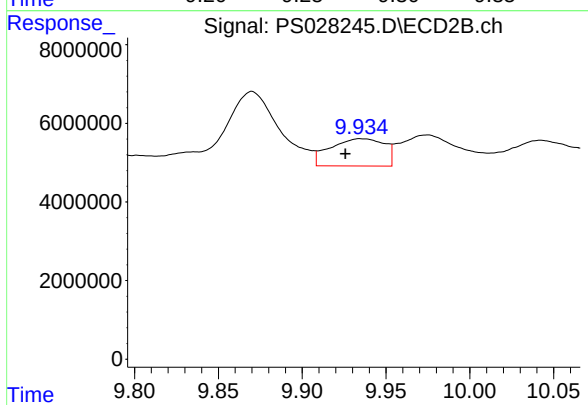

#11 2,4,5-TP (SILVEX)


R.T.: 9.936 min
Delta R.T.: 0.010 min
Response: 15537246
Conc: 1.45 ng/ml

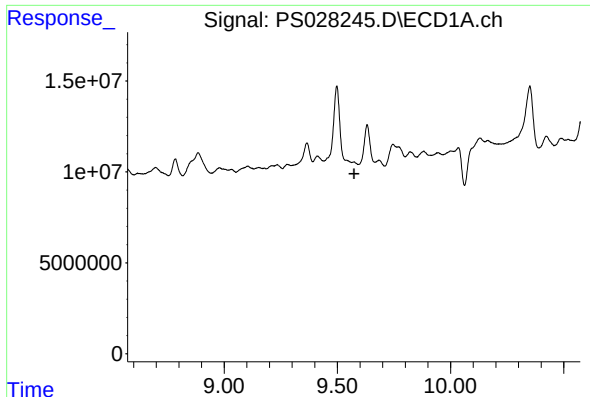

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

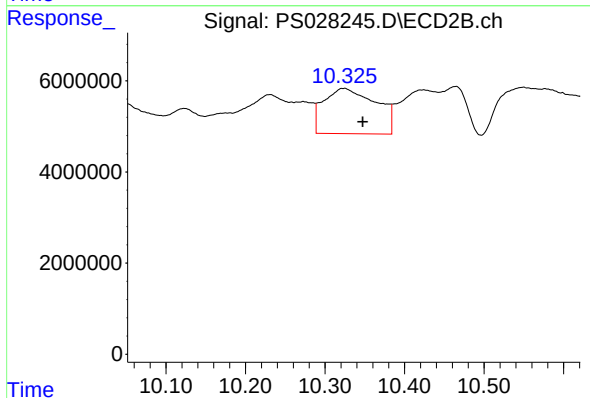


#12 2,4,5-T

R.T.: 10.323 min
Delta R.T.: -0.024 min
Response: 45501561
Conc: 4.25 ng/ml

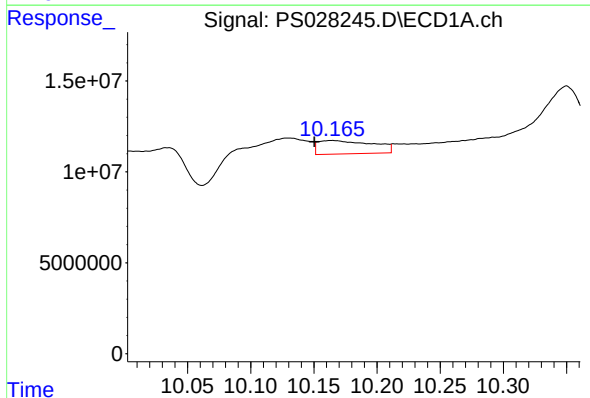


#13 2,4-DB

R.T.: 10.164 min
Delta R.T.: 0.014 min
Response: 22246409
Conc: 13.49 ng/ml

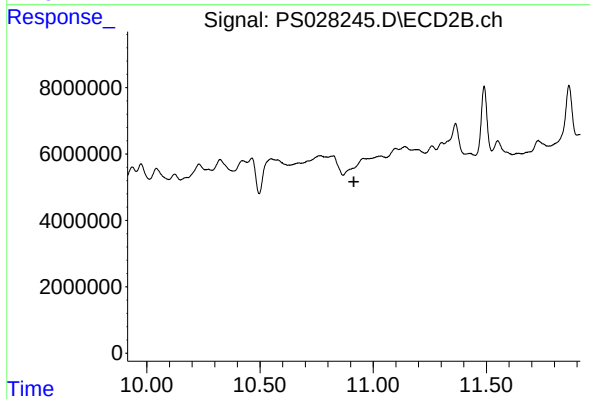

#13 2,4-DB


R.T.: 10.957 min
Delta R.T.: 0.042 min
Response: -826679
Conc: N.D.

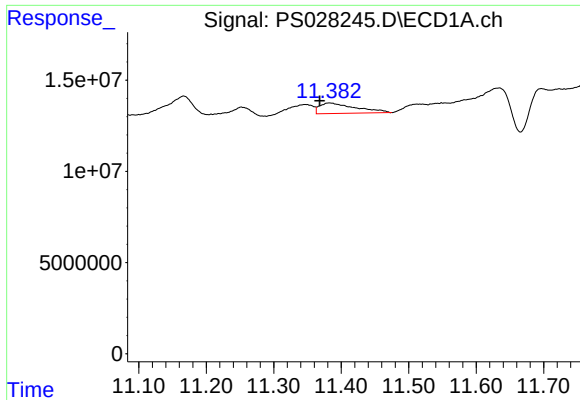

#14 DINOSEB


R.T.: 11.383 min
Delta R.T.: 0.014 min
Response: 21375166
Conc: 2.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

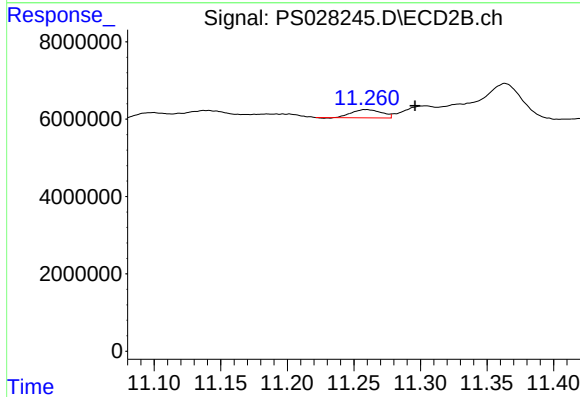


#14 DINOSEB

R.T.: 11.260 min
Delta R.T.: -0.037 min
Response: 3284555
Conc: N.D.

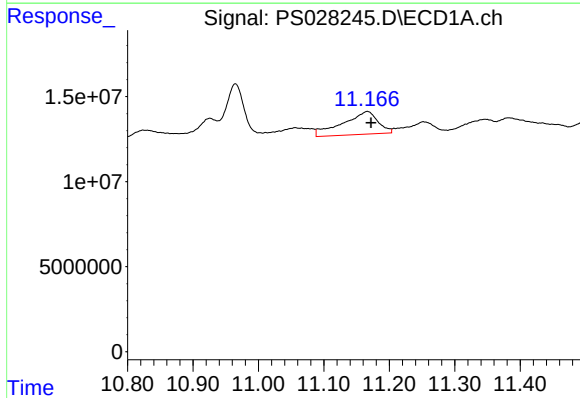


#15 Picloram

R.T.: 11.166 min
Delta R.T.: -0.006 min
Response: 50417659
Conc: 2.89 ng/ml

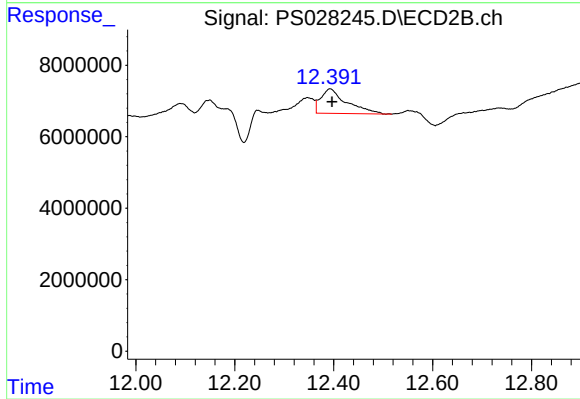

#15 Picloram


R.T.: 12.393 min
Delta R.T.: -0.004 min
Response: 24925740
Conc: 1.52 ng/ml

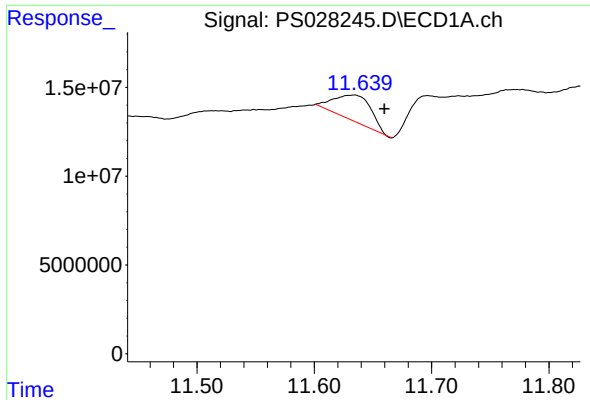

#16 DCPA

R.T.: 11.633 min
Delta R.T.: -0.027 min
Response: 31614202
Conc: 2.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

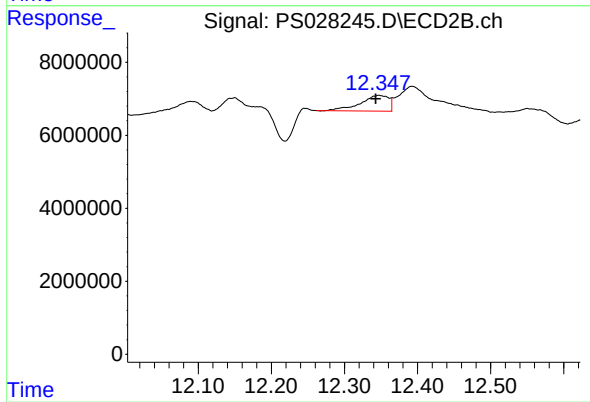

#16 DCPA

R.T.: 12.347 min
Delta R.T.: 0.004 min
Response: 11588696
Conc: N.D.