

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
 Data File : PS028247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 07:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 07:11:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 00:14:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.262	7.765	1225.9E6	841.7E6	679.918	538.236
Target Compounds							
1) T	Dalapon	2.656	0.000	592928	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.418	0.000	824919	0	<MDL	N.D. #
3) T	4-Nitroph...	7.055	0.000	4831879	0	4.077	N.D. #
6) T	MCP	0.000	8.114f	0	27558683	N.D.	5.326
7) T	MCPA	0.000	8.285f	0	7893015	N.D.	1.100
8) T	DICHLORPROP	0.000	8.736f	0	6560581	N.D.	3.769
10) T	Pentachlo...	8.742f	0.000	983841	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.941	0	29434241	N.D.	2.737
12) T	2,4,5-T	0.000	10.347	0	1447294	N.D.	<MDL
13) T	2,4-DB	10.101f	0.000	592323	0	<MDL	N.D. #
15) T	Picloram	11.152	12.395	10542888	15534355	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
Data File : PS028247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 07:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 07:11:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 00:14:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

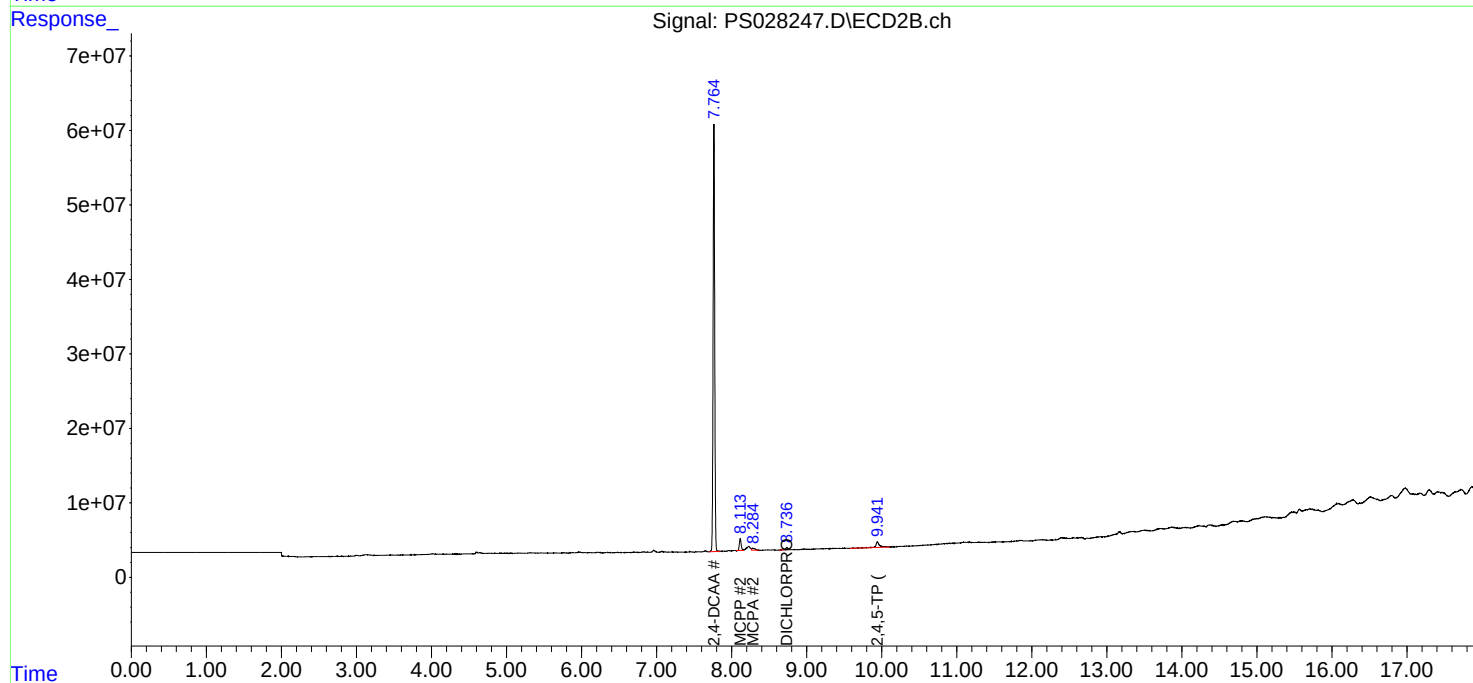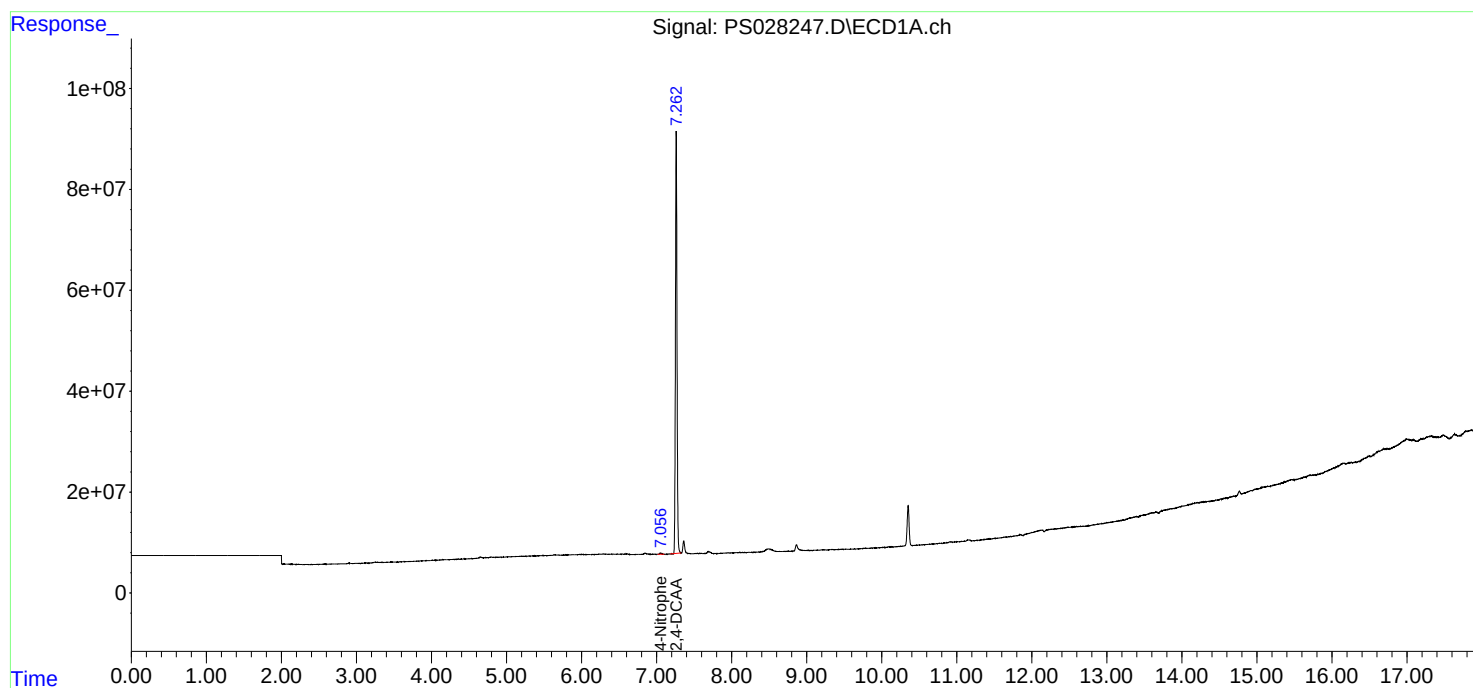


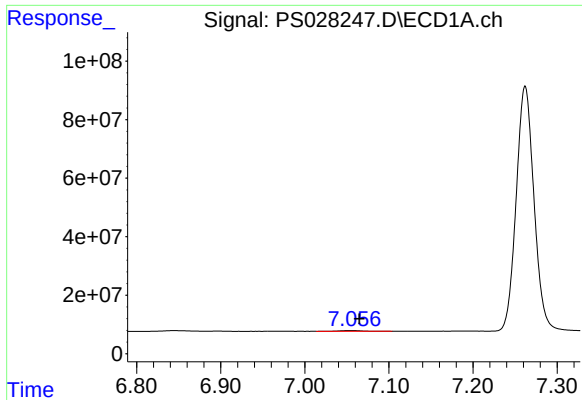

#3 4-Nitrophenol


R.T.: 7.055 min
Delta R.T.: -0.010 min
Response: 4831879
Conc: 4.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

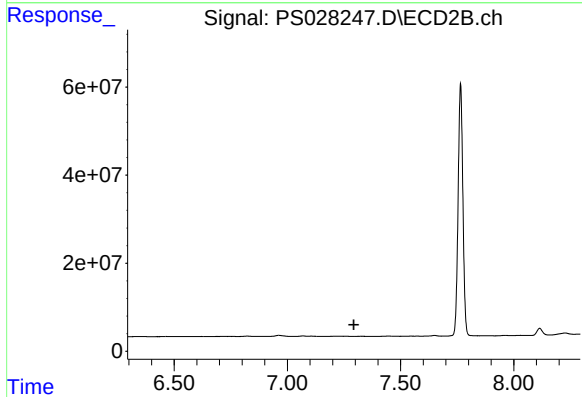


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.293 min
Response: 0
Conc: N.D.

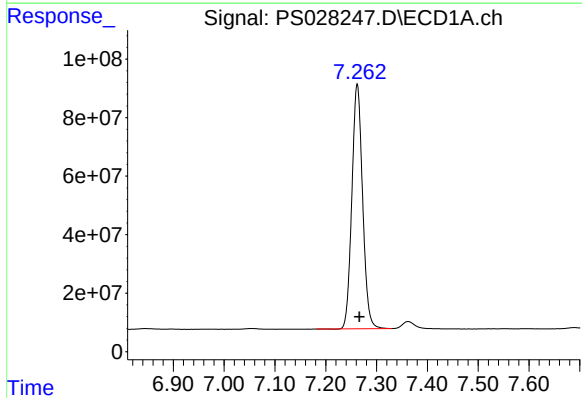


#4 2,4-DCAA

R.T.: 7.262 min
Delta R.T.: -0.004 min
Response: 1225913682
Conc: 679.92 ng/ml

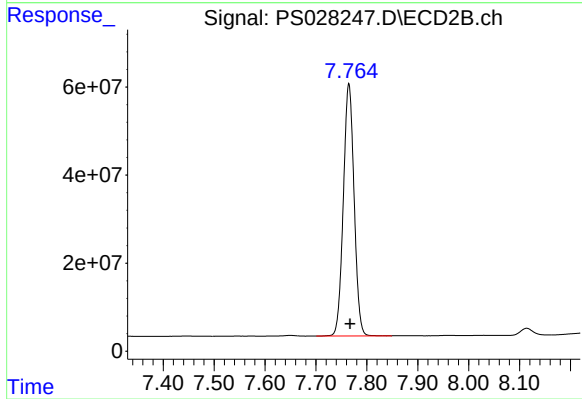

#4 2,4-DCAA


R.T.: 7.765 min
Delta R.T.: -0.003 min
Response: 841741685
Conc: 538.24 ng/ml

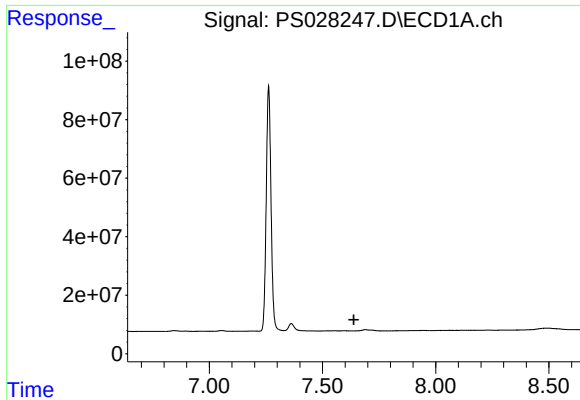

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.639 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

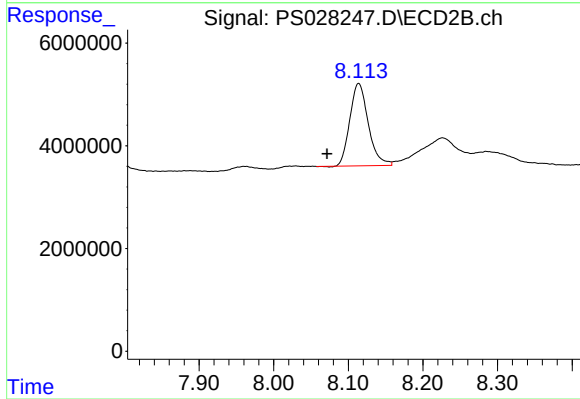


#6 MCPP

R.T.: 8.114 min
Delta R.T.: 0.042 min
Response: 27558683
Conc: 5.33 ug/ml

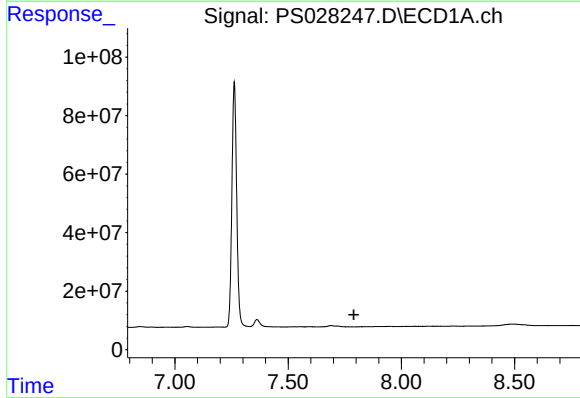


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.790 min
Response: 0
Conc: N.D.

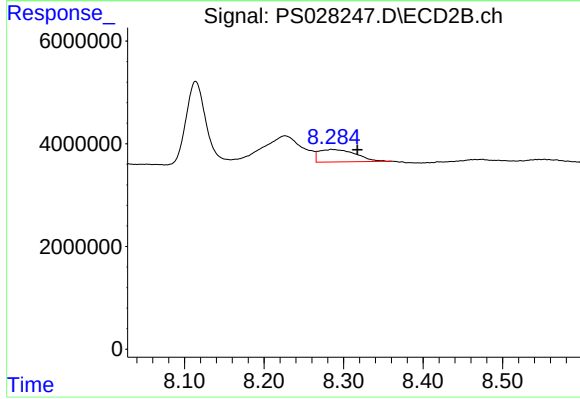

#7 MCPA


R.T.: 8.285 min
Delta R.T.: -0.033 min
Response: 7893015
Conc: 1.10 ug/ml

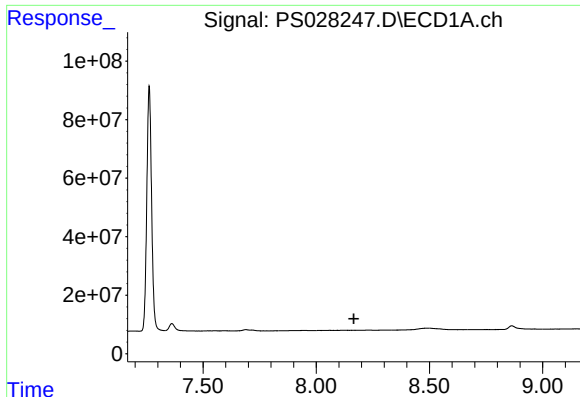

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.166 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

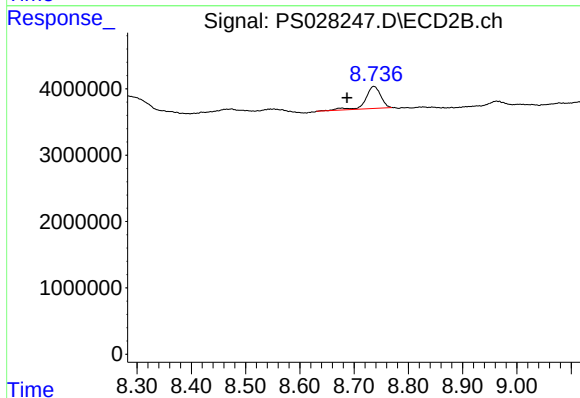


#8 DICHLORPROP

R.T.: 8.736 min
Delta R.T.: 0.050 min
Response: 6560581
Conc: 3.77 ng/ml

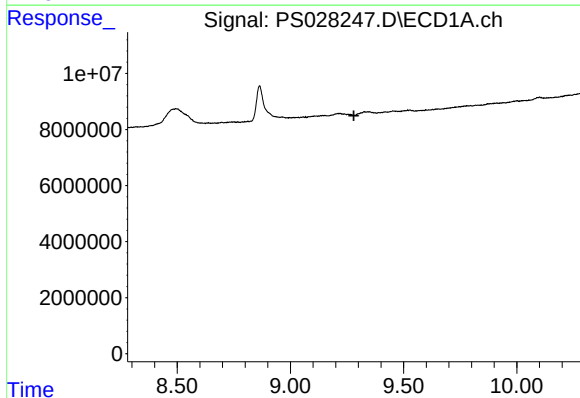

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.281 min
Response: 0
Conc: N.D.

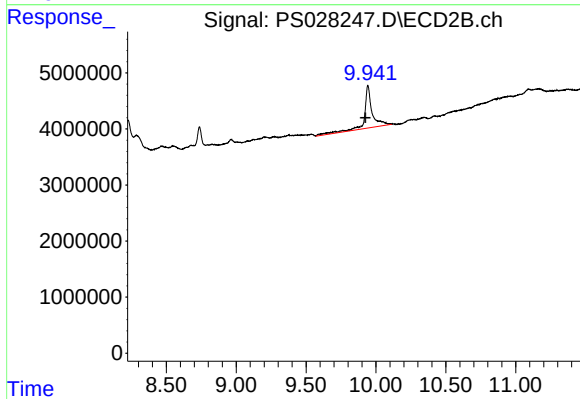

#11 2,4,5-TP (SILVEX)

R.T.: 9.941 min
Delta R.T.: 0.016 min
Response: 29434241
Conc: 2.74 ng/ml