

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110724\
 Data File : PS028333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 19:53
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 04:36:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 11:48:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.691f	0.000	6275610	0	1.763	N.D.	#
2) T	3,5-DICHL...	6.407	0.000	22457622	0	5.991	N.D.	#
3) T	4-Nitroph...	7.037	0.000	13612640	0	8.262	N.D.	#
5) T	DICAMBA	0.000	7.952	0	2748318	N.D.	<MDL	
6) T	MCP	7.678f	8.068	30308939	7022184	3.997	1.157	#
7) T	MCPA	0.000	8.279f	0	12385512	N.D.	1.485	
8) T	DICHLORPROP	8.192f	8.729f	948733	19403930	<MDL	9.657	#
9) T	2,4-D	8.403	0.000	102.8E6	0	32.562	N.D.	#
10) T	Pentachlo...	8.695	0.000	3389066	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.272	9.939	177128	6968724	<MDL	<MDL	#
12) T	2,4,5-T	9.566	0.000	2085944	0	<MDL	N.D.	#
15) T	Picloram	11.131f	12.383	74924600	35805475	2.584	1.986	
16) T	DCPA	11.635	12.383f	2235634	35805475	<MDL	2.556	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110724\
Data File : PS028333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 19:53
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 04:36:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 11:48:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

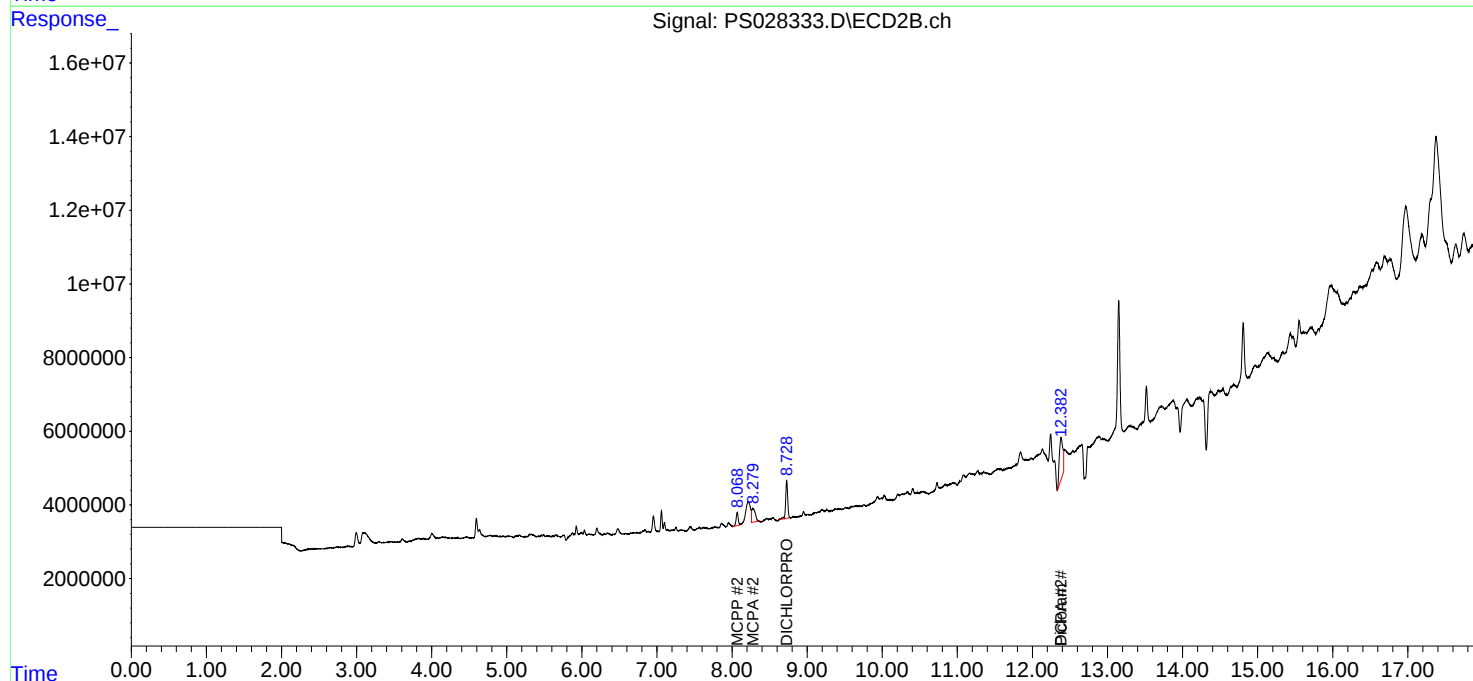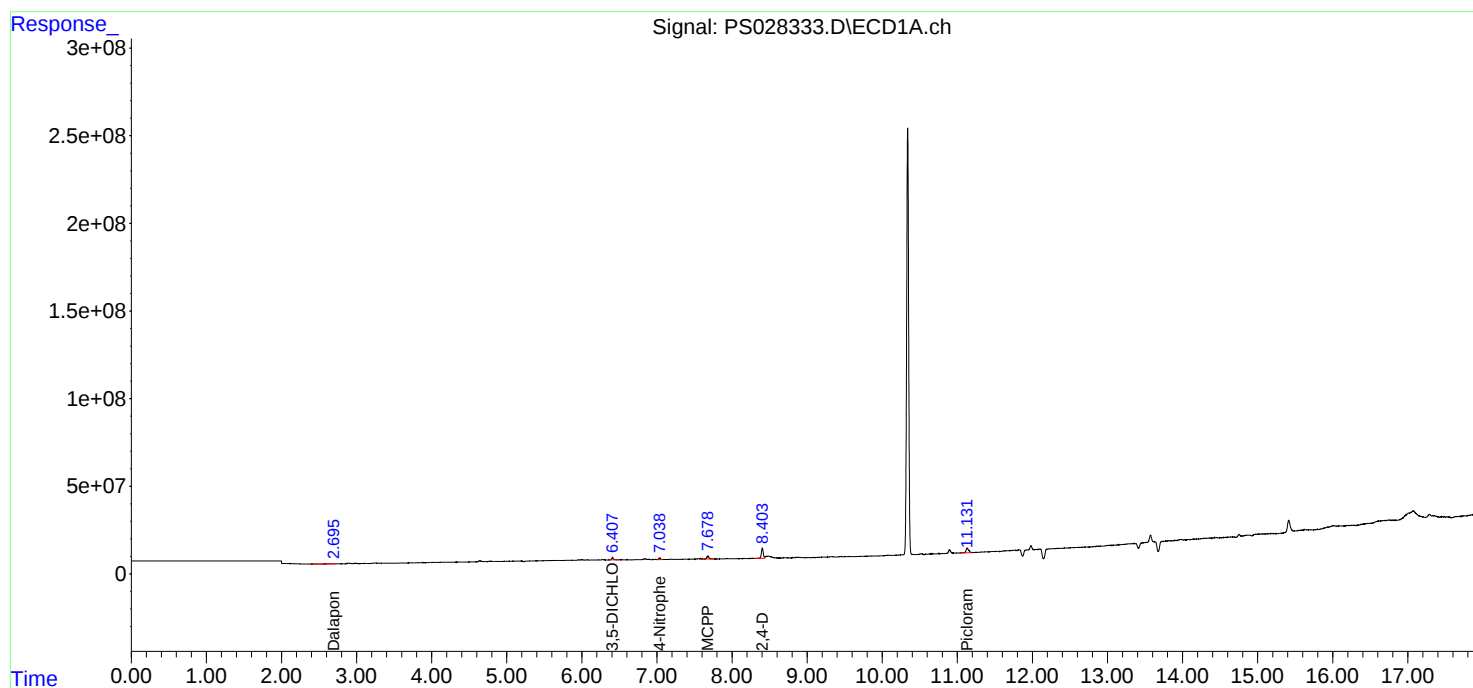


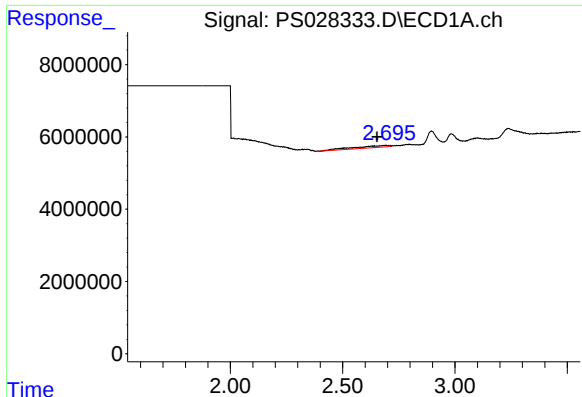

#1 Dalapon


R.T.: 2.691 min
Delta R.T.: 0.037 min
Response: 6275610
Conc: 1.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

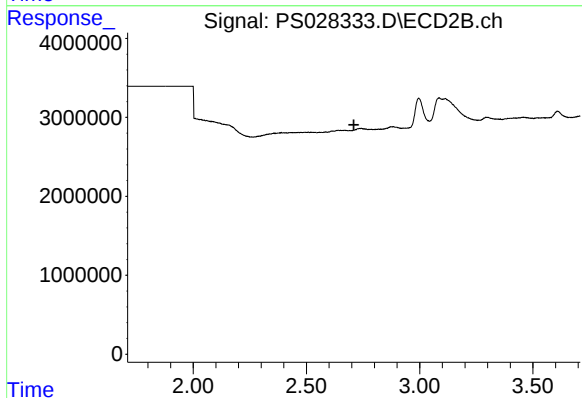


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.710 min
Response: 0
Conc: N.D.

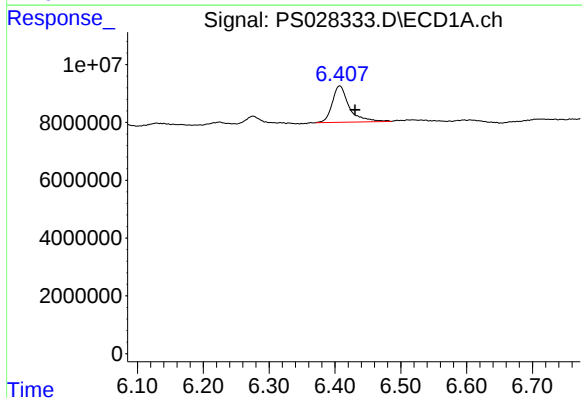


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.407 min
Delta R.T.: -0.023 min
Response: 22457622
Conc: 5.99 ng/ml

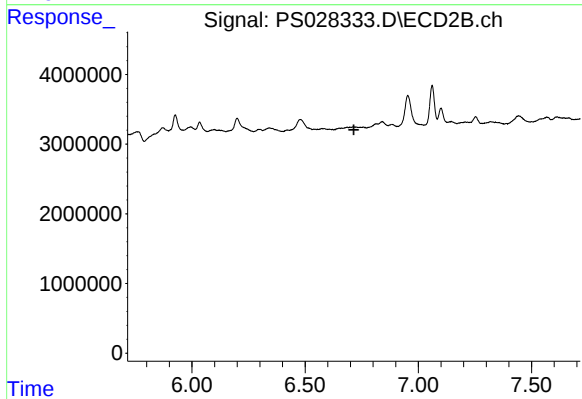

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 6.716 min
Response: 0
Conc: N.D.

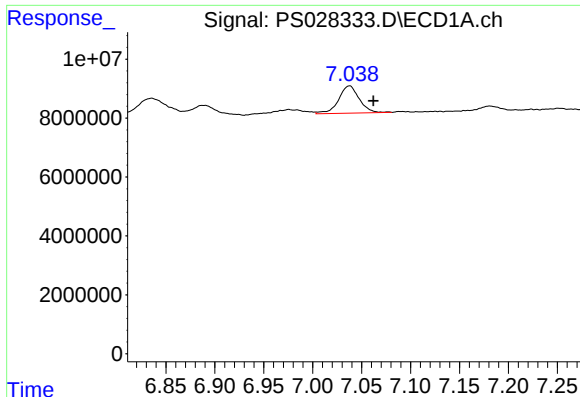

#3 4-Nitrophenol


R.T.: 7.037 min
Delta R.T.: -0.025 min
Response: 13612640
Conc: 8.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

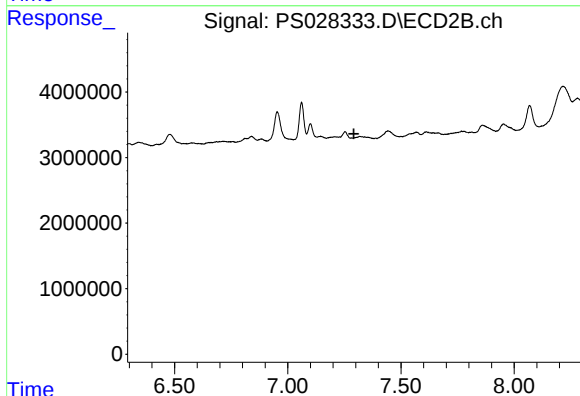


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.292 min
Response: 0
Conc: N.D.

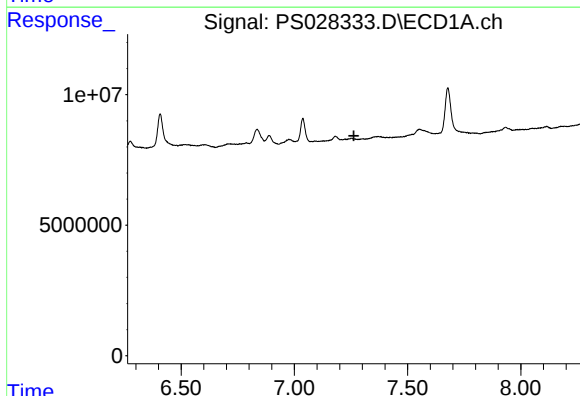


#4 2,4-DCAA

R.T.: 7.252 min
Delta R.T.: -0.010 min
Response: -1461694
Conc: N.D.

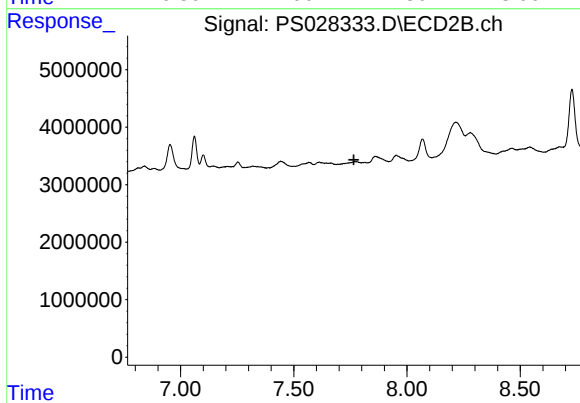

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.765 min
Response: 0
Conc: N.D.

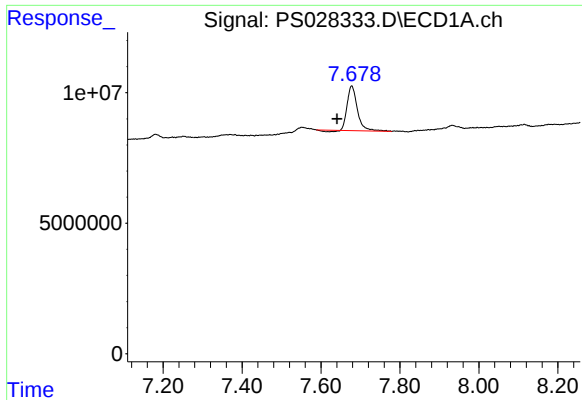

#6 MCPP


R.T.: 7.678 min
Delta R.T.: 0.037 min
Response: 30308939
Conc: 4.00 ug/ml

Instrument :
ECD_S
ClientSampleId :

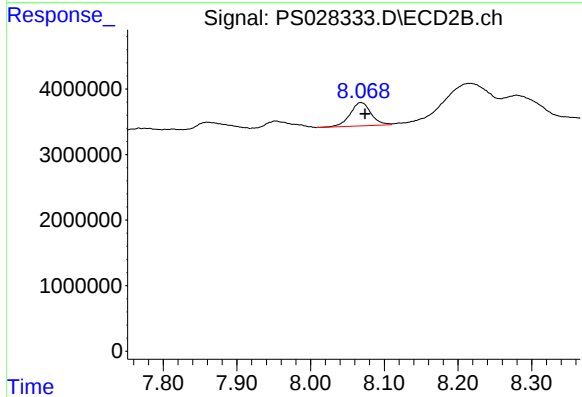


#6 MCPP

R.T.: 8.068 min
Delta R.T.: -0.006 min
Response: 7022184
Conc: 1.16 ug/ml

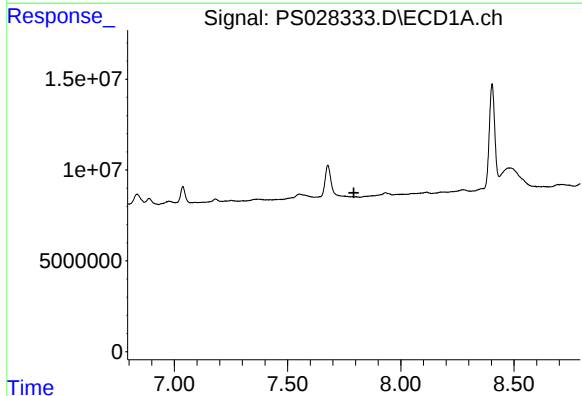


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.793 min
Response: 0
Conc: N.D.

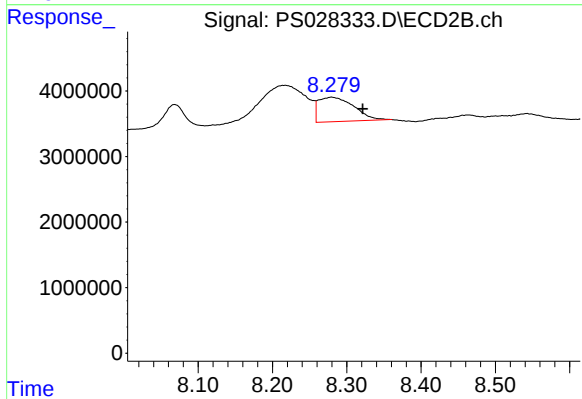

#7 MCPA


R.T.: 8.279 min
Delta R.T.: -0.042 min
Response: 12385512
Conc: 1.49 ug/ml

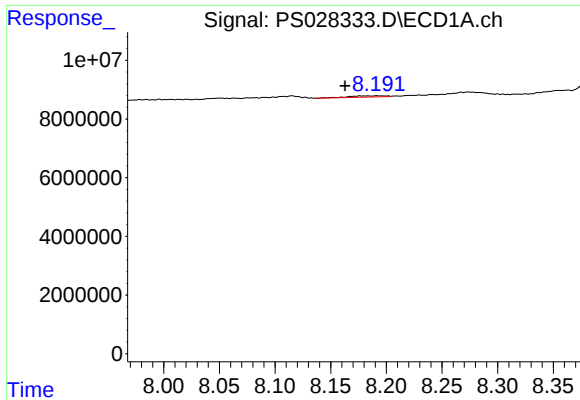

#8 DICHLORPROP


R.T.: 8.192 min
Delta R.T.: 0.029 min
Response: 948733
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

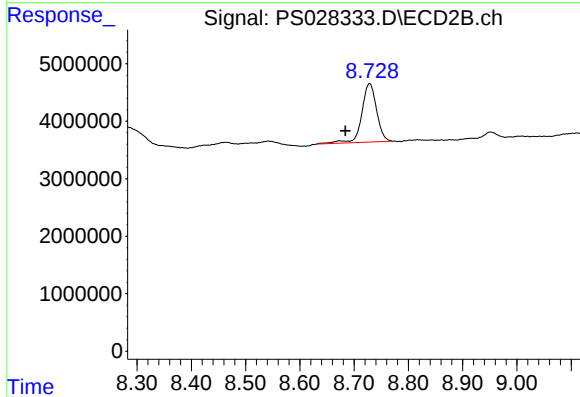


#8 DICHLORPROP

R.T.: 8.729 min
Delta R.T.: 0.045 min
Response: 19403930
Conc: 9.66 ng/ml

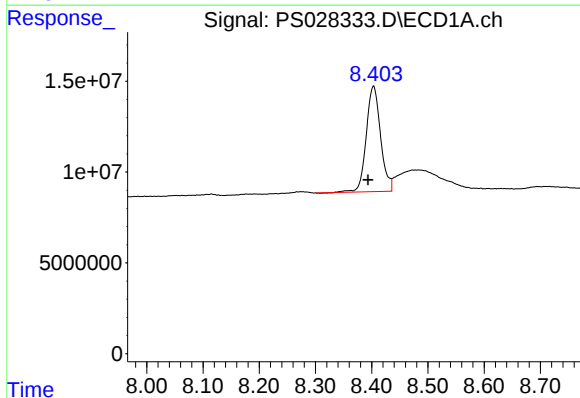


#9 2,4-D

R.T.: 8.403 min
Delta R.T.: 0.009 min
Response: 102770773
Conc: 32.56 ng/ml

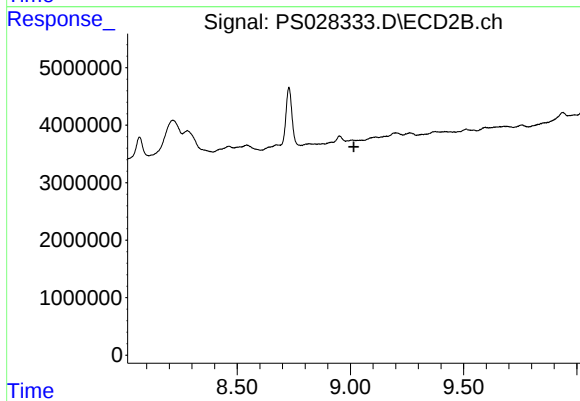

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 9.015 min
Response: 0
Conc: N.D.

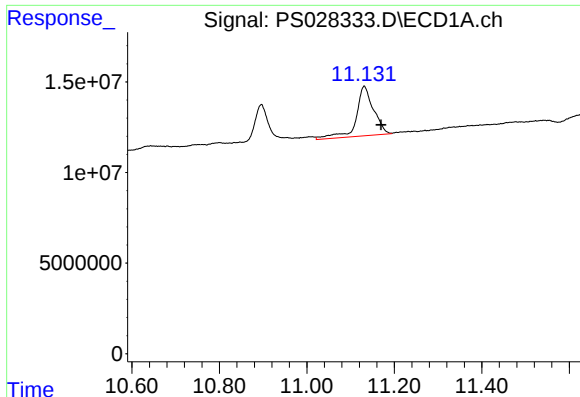

#15 Picloram


R.T.: 11.131 min
Delta R.T.: -0.038 min
Response: 74924600
Conc: 2.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

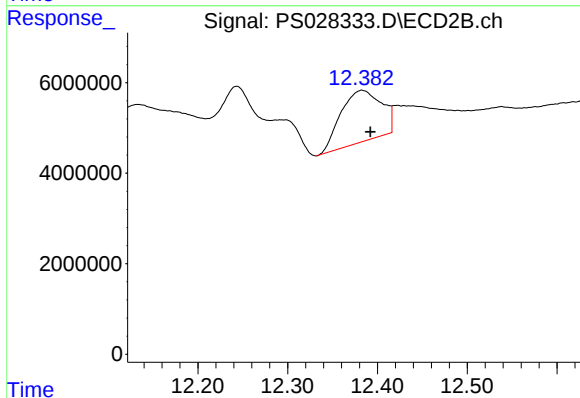


#15 Picloram

R.T.: 12.383 min
Delta R.T.: -0.010 min
Response: 35805475
Conc: 1.99 ng/ml

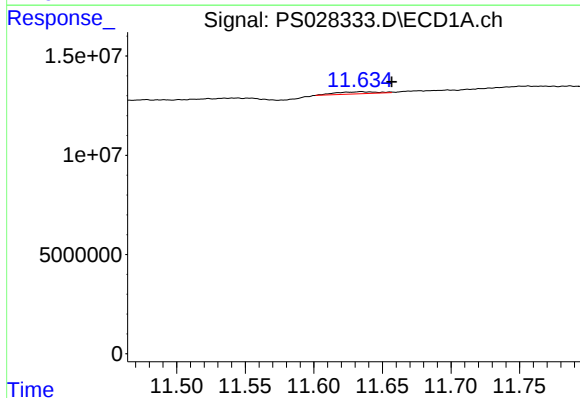

#16 DCPA

R.T.: 11.635 min
Delta R.T.: -0.022 min
Response: 2235634
Conc: N.D.

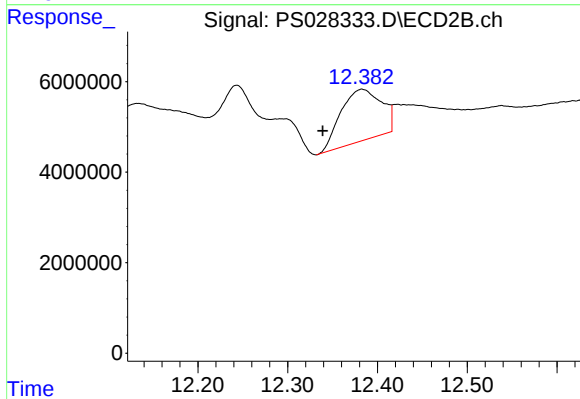

#16 DCPA

R.T.: 12.383 min
Delta R.T.: 0.044 min
Response: 35805475
Conc: 2.56 ng/ml