

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110724\
 Data File : PS028334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 20:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 04:36:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 11:48:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.253	7.758	1389.6E6	824.4E6	542.520	473.294
Target Compounds							
2) T	3,5-DICHL...	6.407	0.000	393515	0	<MDL	N.D. #
3) T	4-Nitroph...	7.045	0.000	6433444	0	3.905	N.D. #
6) T	MCP	7.680f	8.109f	6656551	1133382	<MDL	<MDL #
7) T	MCPA	0.000	8.284f	0	11669303	N.D.	1.399
8) T	DICHLORPROP	0.000	8.729f	0	5018895	N.D.	2.498
10) T	Pentachlo...	8.688	0.000	1218566	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.938	0	9943922	N.D.	<MDL
12) T	2,4,5-T	9.565	0.000	1994908	0	<MDL	N.D. #
15) T	Picloram	11.157	12.384	30190671	25154454	1.041	1.395 #
16) T	DCPA	11.643	12.384f	1324673	25154454	<MDL	1.795 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110724\
Data File : PS028334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 20:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 04:36:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 11:48:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

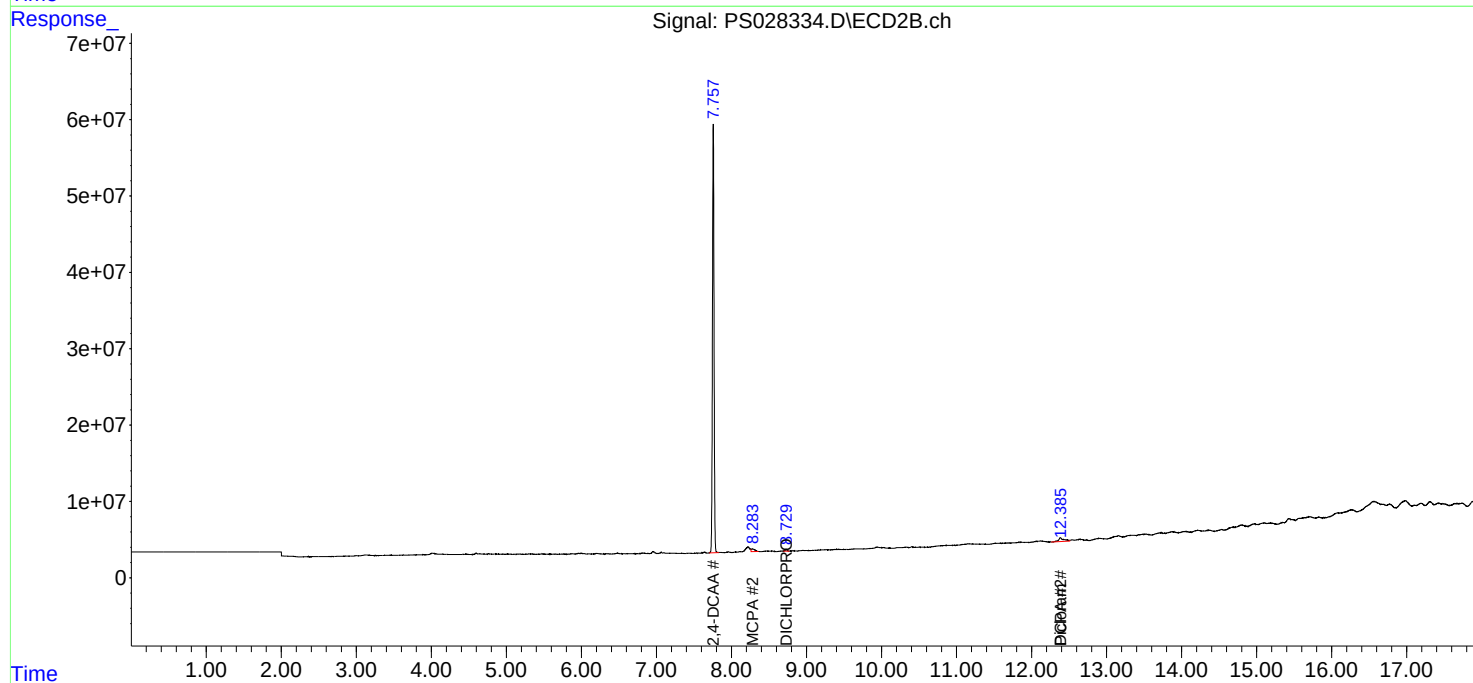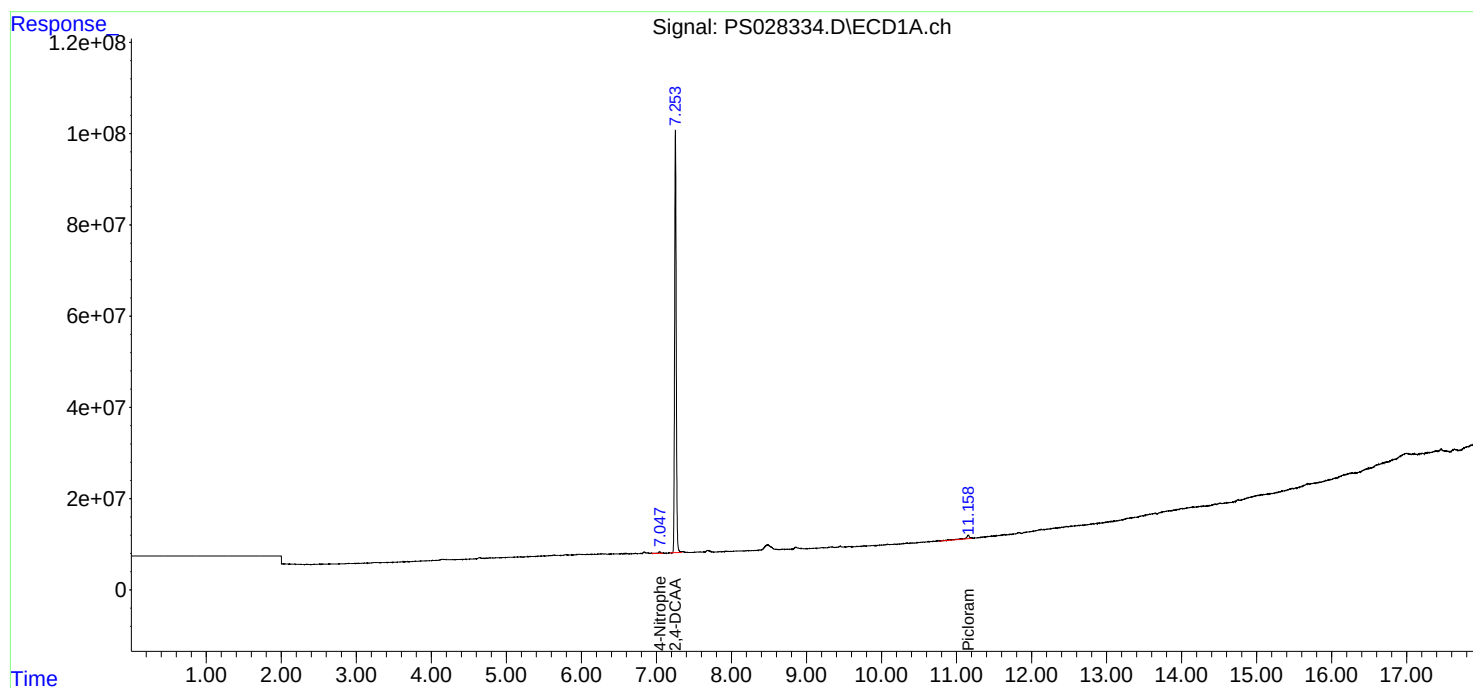


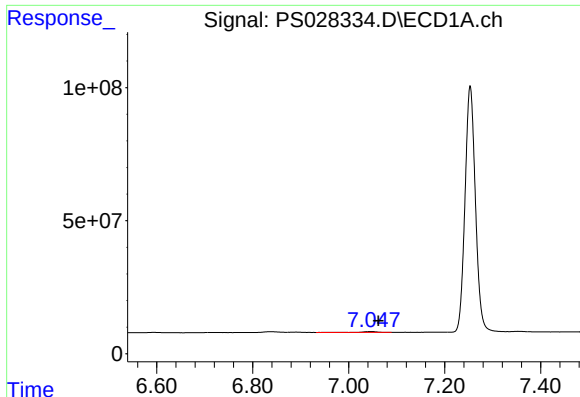

#3 4-Nitrophenol


R.T.: 7.045 min
Delta R.T.: -0.017 min
Response: 6433444
Conc: 3.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

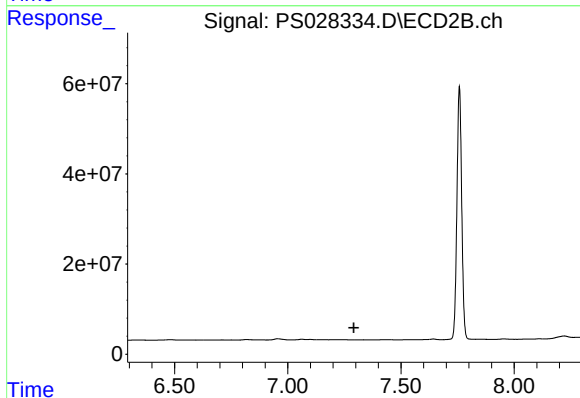


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.292 min
Response: 0
Conc: N.D.

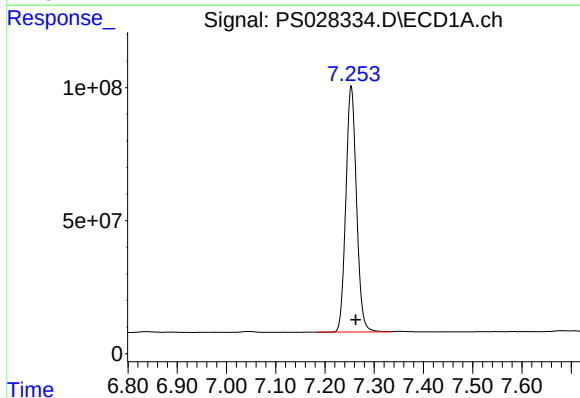


#4 2,4-DCAA

R.T.: 7.253 min
Delta R.T.: -0.009 min
Response: 1389618211
Conc: 542.52 ng/ml

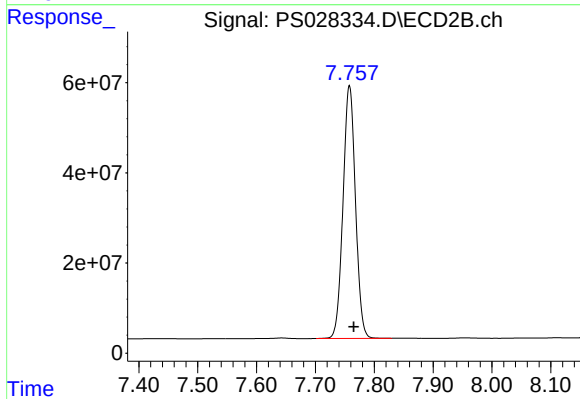

#4 2,4-DCAA


R.T.: 7.758 min
Delta R.T.: -0.007 min
Response: 824374873
Conc: 473.29 ng/ml

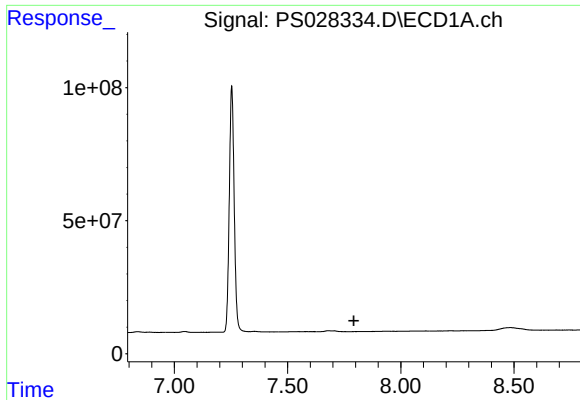

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

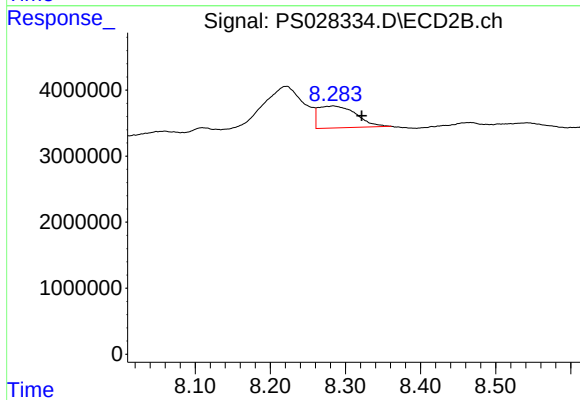


#7 MCPA

R.T.: 8.284 min
Delta R.T.: -0.038 min
Response: 11669303
Conc: 1.40 ug/ml

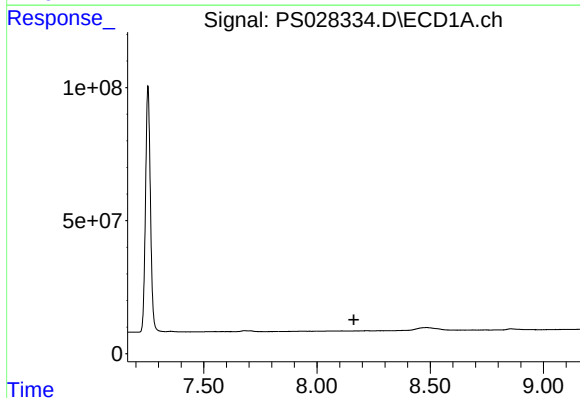


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.163 min
Response: 0
Conc: N.D.

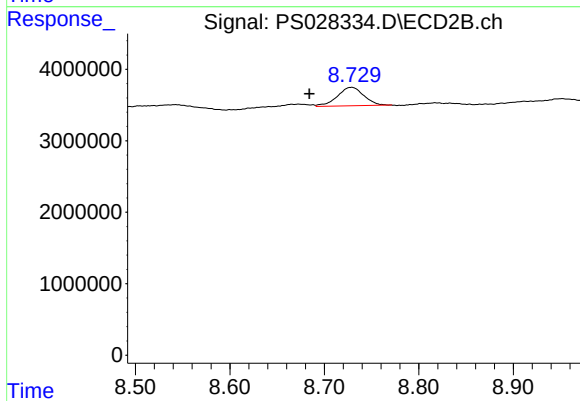

#8 DICHLORPROP


R.T.: 8.729 min
Delta R.T.: 0.045 min
Response: 5018895
Conc: 2.50 ng/ml

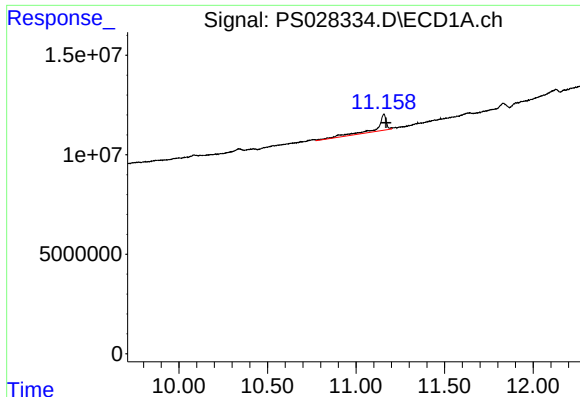

#15 Picloram


R.T.: 11.157 min
Delta R.T.: -0.012 min
Response: 30190671
Conc: 1.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

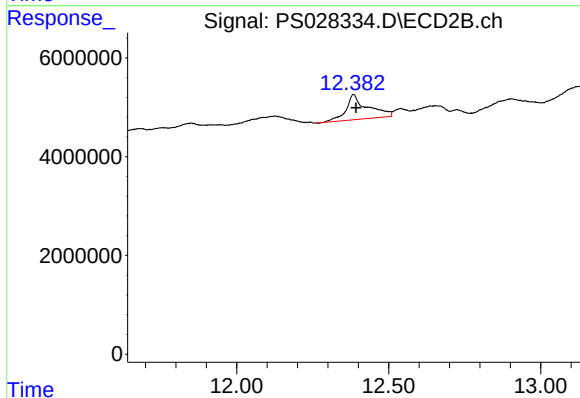


#15 Picloram

R.T.: 12.384 min
Delta R.T.: -0.008 min
Response: 25154454
Conc: 1.39 ng/ml

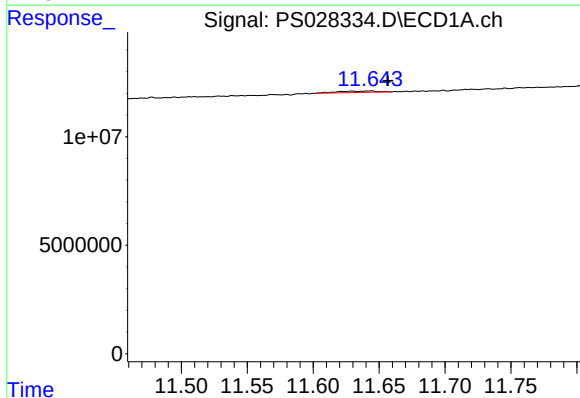

#16 DCPA

R.T.: 11.643 min
Delta R.T.: -0.014 min
Response: 1324673
Conc: N.D.

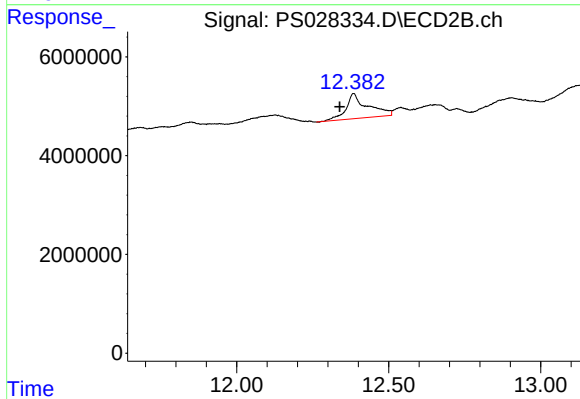

#16 DCPA

R.T.: 12.384 min
Delta R.T.: 0.045 min
Response: 25154454
Conc: 1.80 ng/ml