

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110725\
 Data File : PS032308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2025 01:49
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 05:49:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.288	0.000	613699	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.448	0.000	33286814	0	5.148	N.D. #
3) T	4-Nitroph...	7.120	0.000	138756	0	<MDL	N.D. #
5) T	DICAMBA	7.460	0.000	144536	0	<MDL	N.D. #
6) T	MCP	7.645	7.918	446654	22598759	<MDL	1.699 #
7) T	MCPA	7.799	8.109f	754375	1992719	<MDL	<MDL #
8) T	DICHLORPROP	8.180	0.000	645948	0	<MDL	N.D. #
9) T	2,4-D	8.406	0.000	1215912	0	<MDL	N.D. #
10) T	Pentachlo...	8.708	9.375	2090297	6461044	<MDL	<MDL #
11) T	2,4,5-TP ...	9.279	9.790f	671775	5559367	<MDL	<MDL #
12) T	2,4,5-T	9.584	0.000	487710	0	<MDL	N.D. #
13) T	2,4-DB	10.138	0.000	1790443	0	<MDL	N.D. #
14) T	DINOSEB	11.362	11.126	9610568	3000460	<MDL	<MDL #
15) T	Picloram	11.169	12.212	472342	21079044	<MDL	<MDL #
16) T	DCPA	11.658	0.000	5840703	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110725\
Data File : PS032308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2025 01:49
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 05:49:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

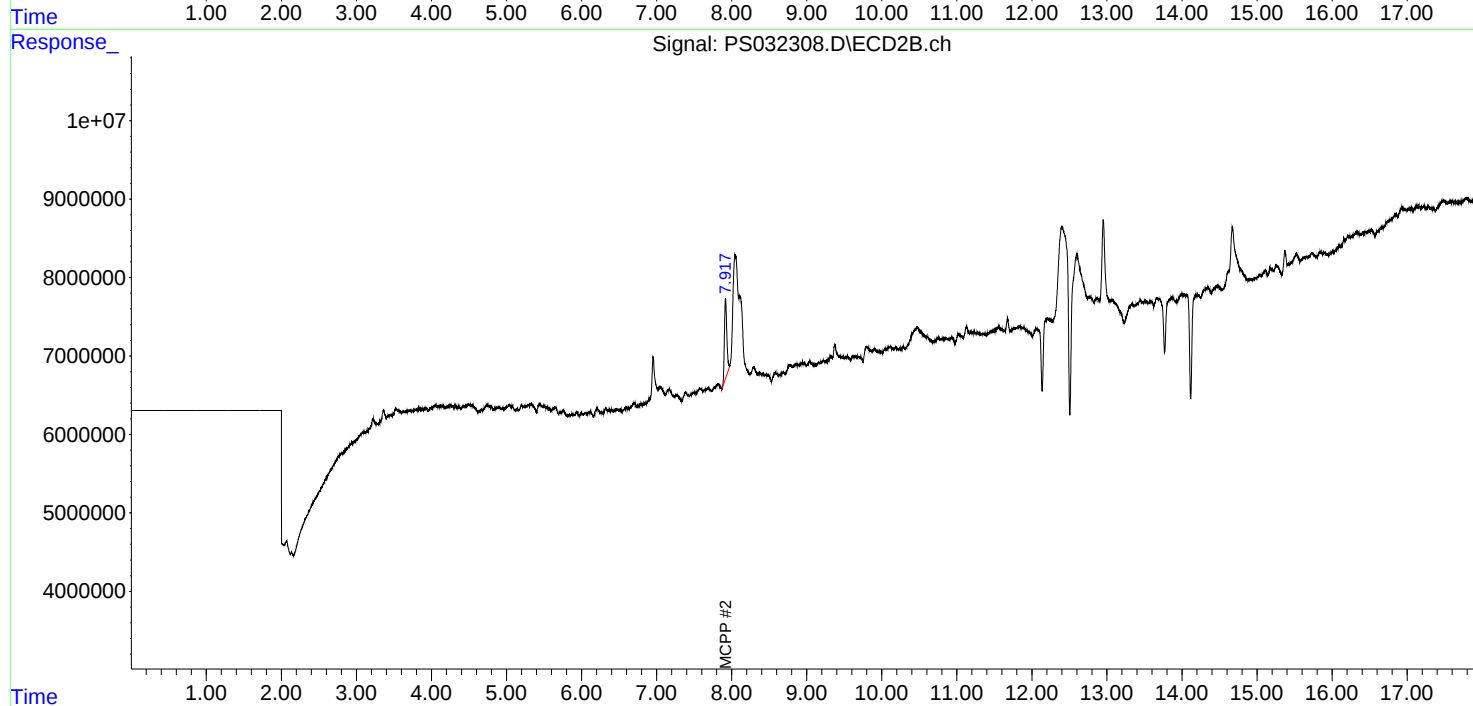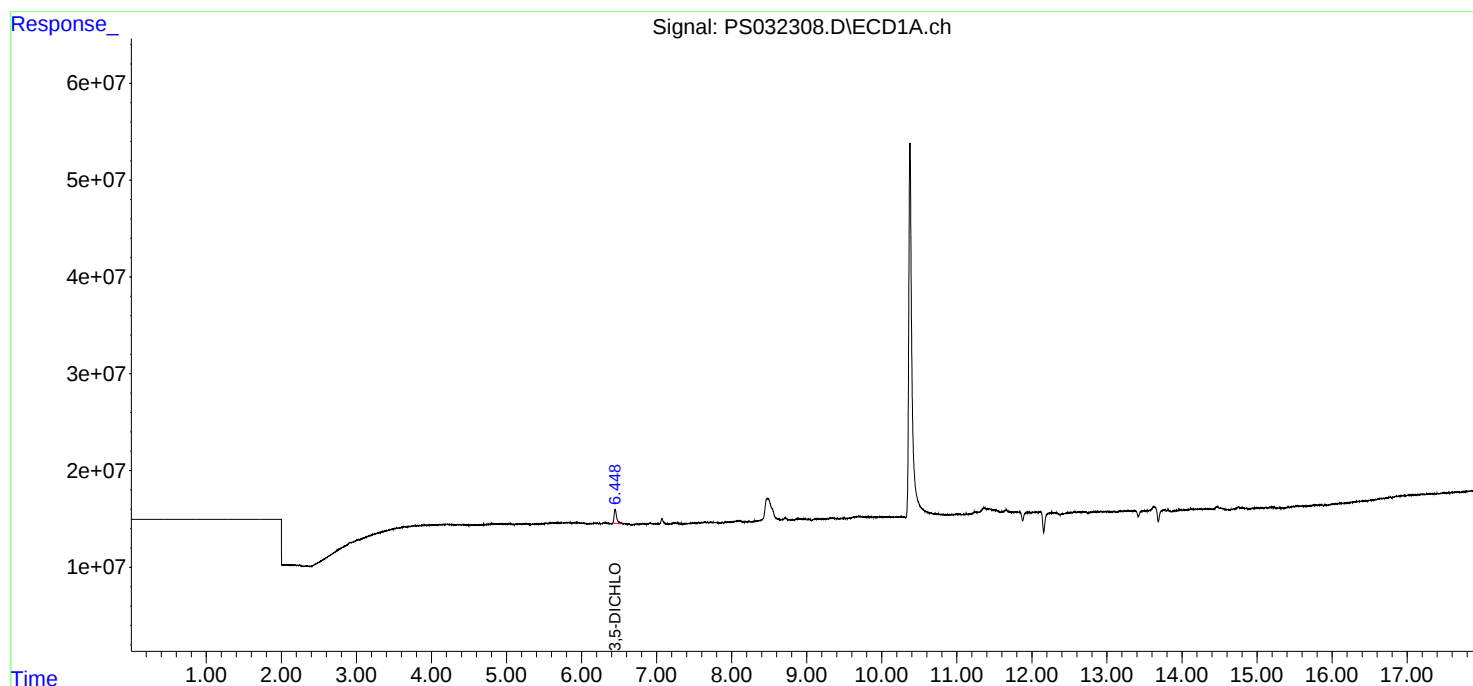


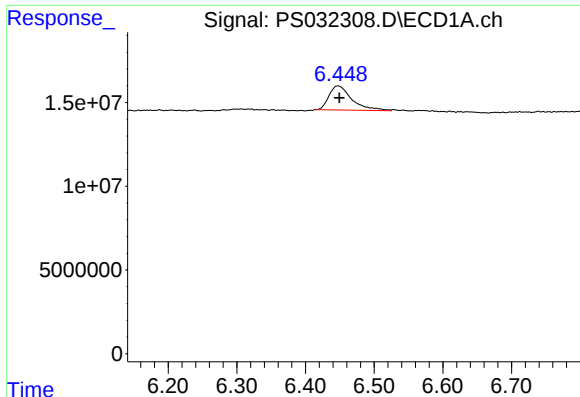

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.448 min
Delta R.T.: -0.002 min
Response: 33286814
Conc: 5.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

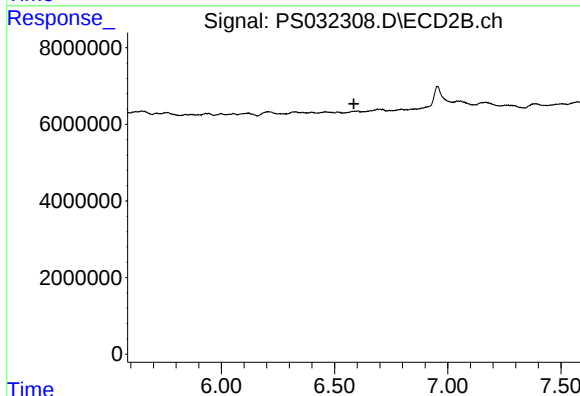


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

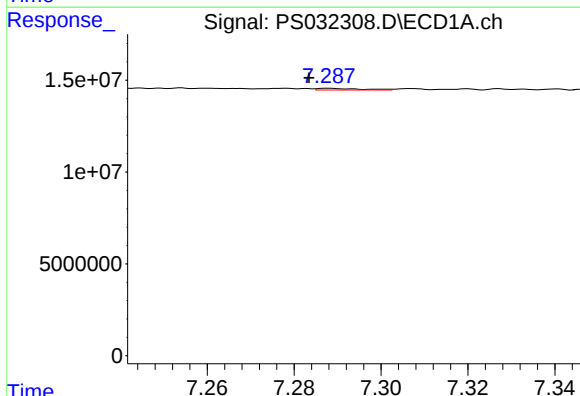


#4 2,4-DCAA

R.T.: 7.288 min
Delta R.T.: 0.005 min
Response: 613699
Conc: N.D.

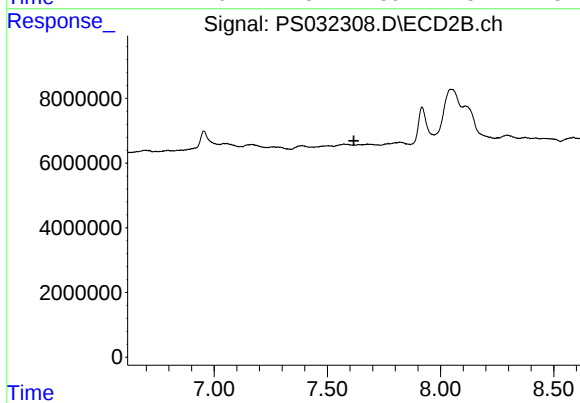

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.617 min
Response: 0
Conc: N.D.

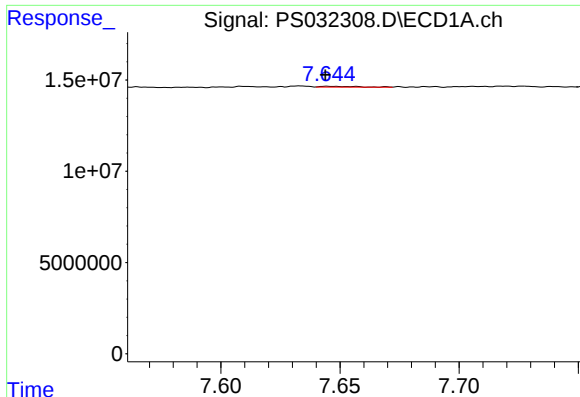

#6 MCPP

R.T.: 7.645 min
Delta R.T.: 0.000 min
Response: 446654
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

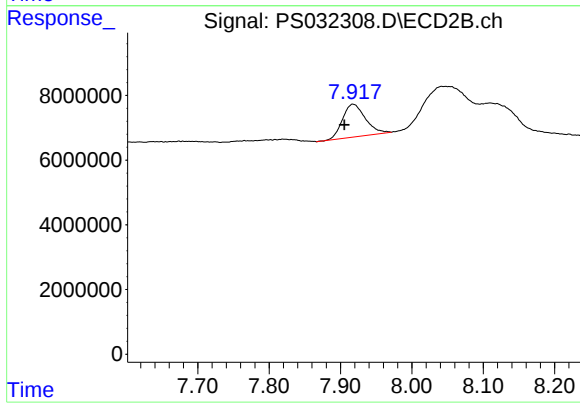

#6 MCPP

R.T.: 7.918 min
Delta R.T.: 0.012 min
Response: 22598759
Conc: 1.70 ug/ml