

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110725\
 Data File : PS032309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2025 02:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 05:50:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.290	7.627	1819.7E6	2098.0E6	401.587	575.501	#
Target Compounds								
2) T	3,5-DICHL...	6.448	0.000	30611242	0	4.734	N.D.	#
3) T	4-Nitroph...	7.077	0.000	4222320	0	3.145	N.D.	#
6) T	MCP	7.632	7.917	-318038	58209499	N.D.	4.376	
7) T	MCPA	7.763f	0.000	1457780	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.174	0.000	257514	0	<MDL	N.D.	#
10) T	Pentachlo...	8.724	9.377	7284101	5294295	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.283	0.000	4795332	0	<MDL	N.D.	#
12) T	2,4,5-T	9.606f	10.143f	4042911	3871885	<MDL	<MDL	#
14) T	DINOSEB	11.371f	11.126	10812173	1208560	<MDL	<MDL	#
15) T	Picloram	0.000	12.232	0	1334298	N.D.	<MDL	
16) T	DCPA	11.652	0.000	6849084	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110725\
Data File : PS032309.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2025 02:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 05:50:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

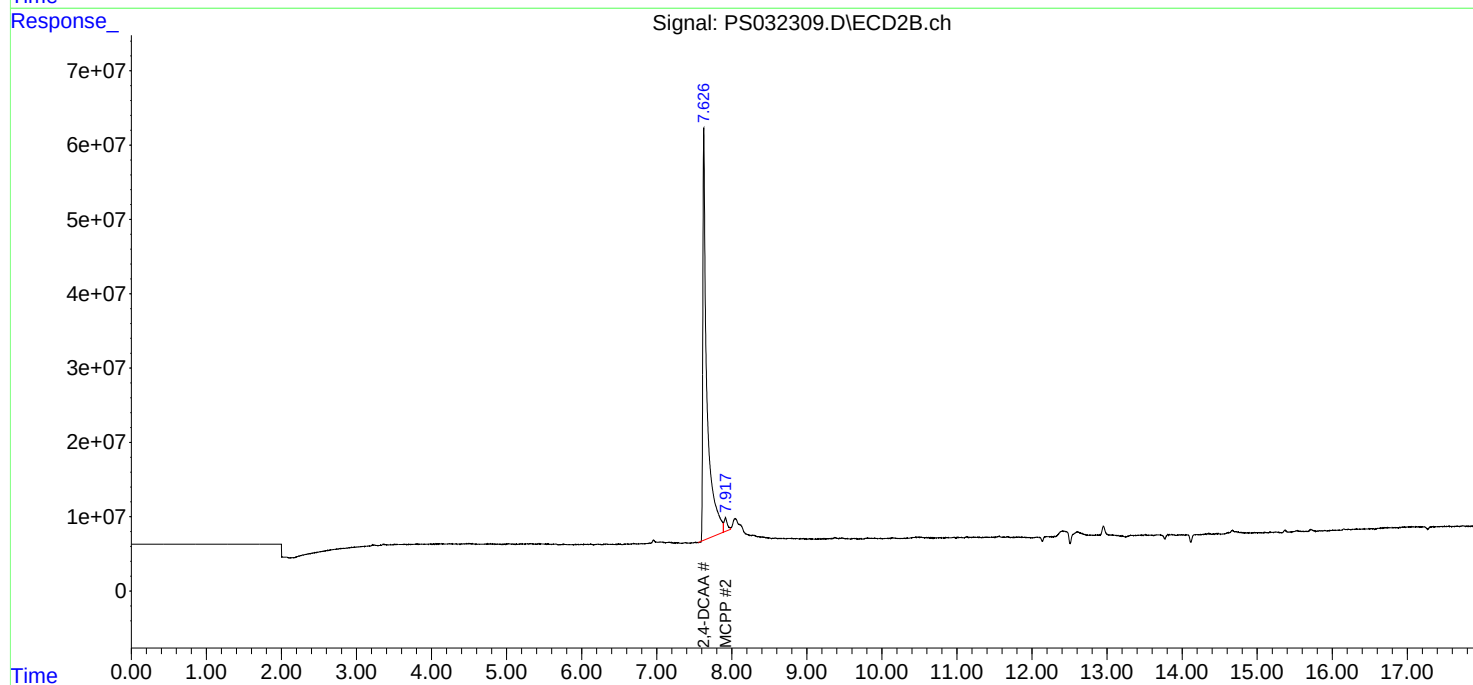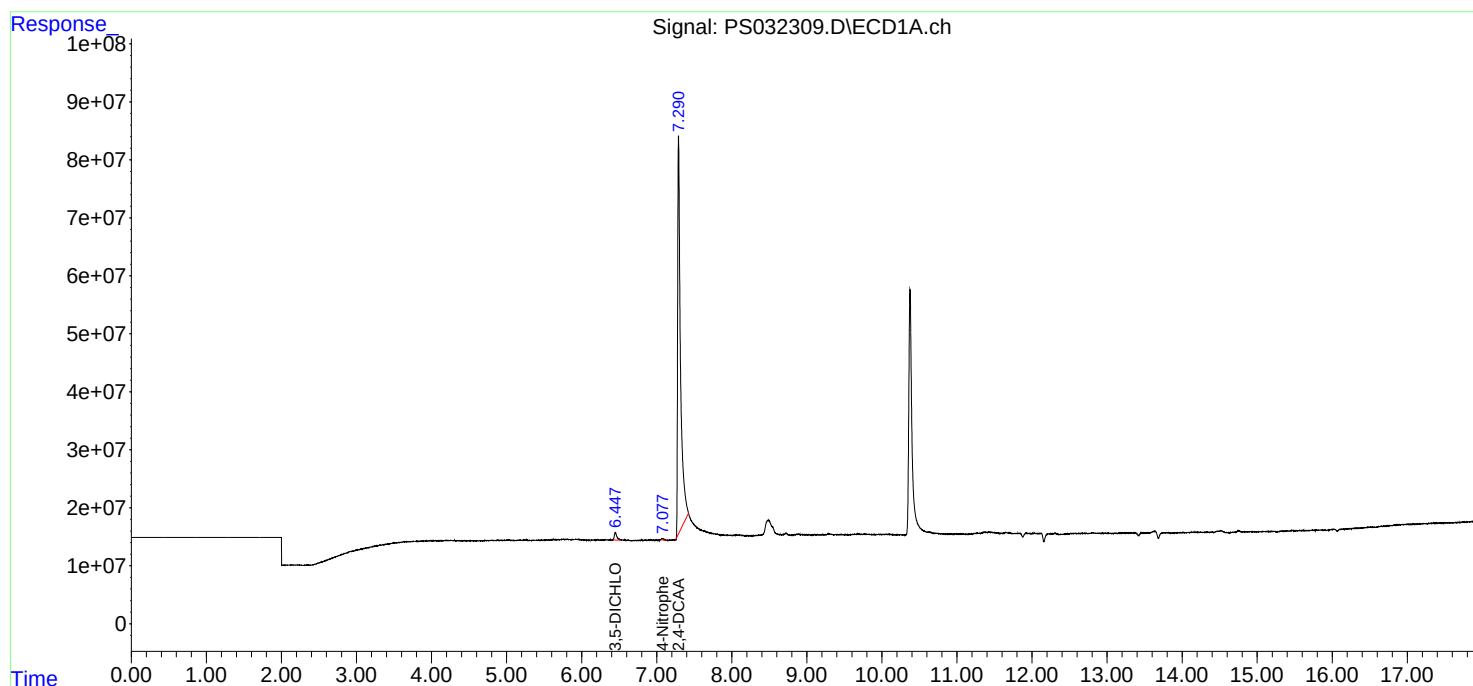


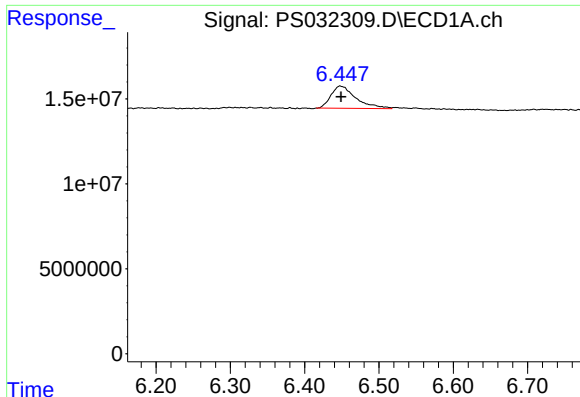

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.448 min
Delta R.T.: -0.002 min
Response: 30611242
Conc: 4.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

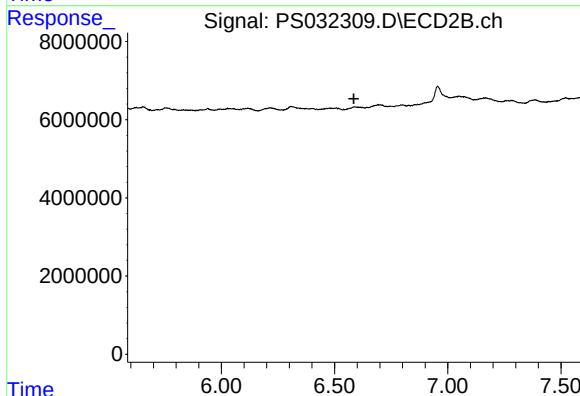


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

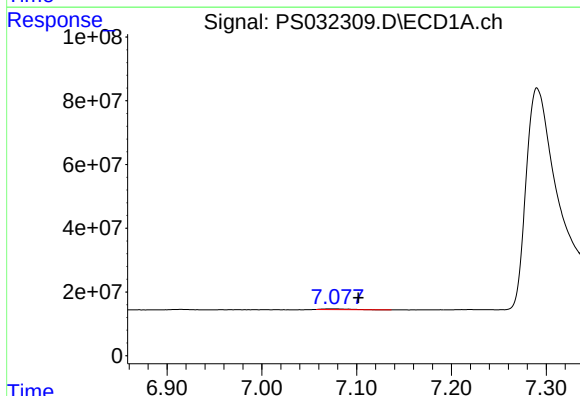


#3 4-Nitrophenol

R.T.: 7.077 min
Delta R.T.: -0.025 min
Response: 4222320
Conc: 3.15 ng/ml

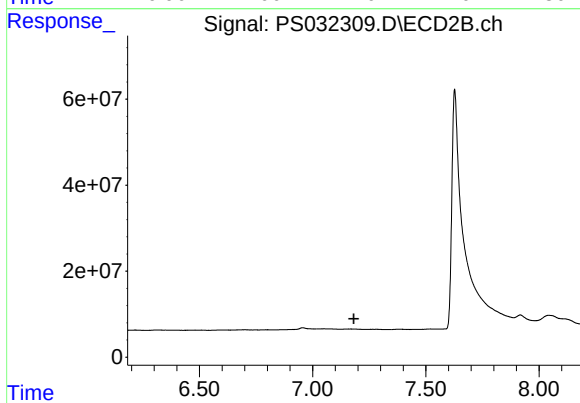

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

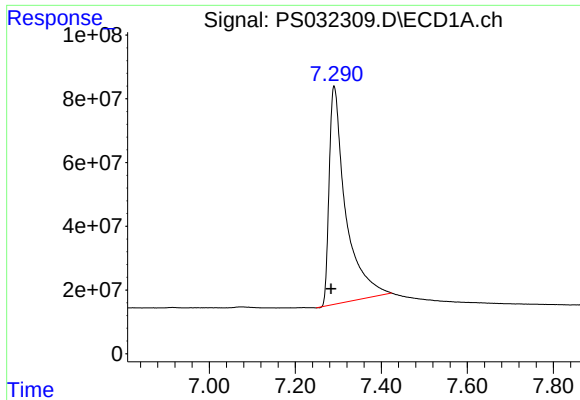

#4 2,4-DCAA


R.T.: 7.290 min
Delta R.T.: 0.007 min
Response: 1819702638
Conc: 401.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

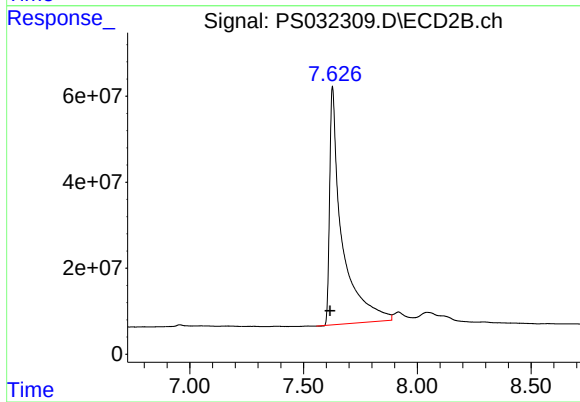


#4 2,4-DCAA

R.T.: 7.627 min
Delta R.T.: 0.010 min
Response: 2097986840
Conc: 575.50 ng/ml

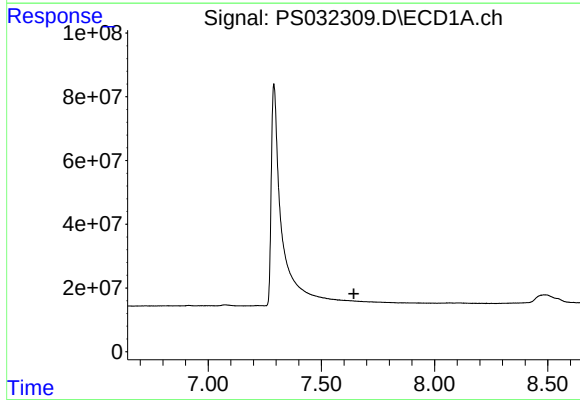

#6 MCPP

R.T.: 7.632 min
Delta R.T.: -0.012 min
Response: -318038
Conc: N.D.

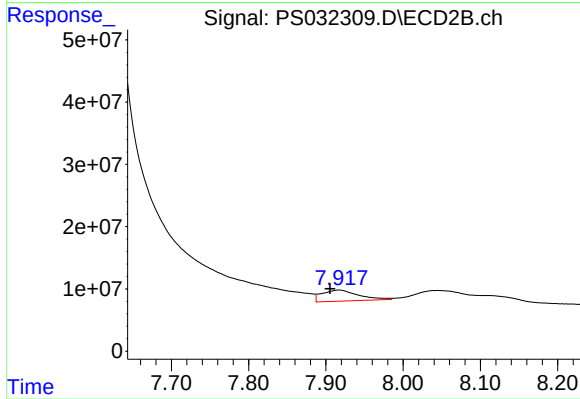

#6 MCPP

R.T.: 7.917 min
Delta R.T.: 0.011 min
Response: 58209499
Conc: 4.38 ug/ml