

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110822\
 Data File : PS021062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 09:00
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 12:25:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.359f	0.000	1950955	0	<MDL	N.D.	#
Target Compounds								
1) T	Dalapon	2.510	0.000	1200000	0	<MDL	N.D.	#
3) T	4-Nitroph...	6.245	0.000	2541619	0	1.690	N.D.	#
6) T	MCP	6.698	0.000	1304493	0	<MDL	N.D.	#
7) T	MCPA	6.801f	7.301	2878450	6012734	<MDL	<MDL	#
8) T	DICHLORPROP	7.090f	0.000	1099302	0	<MDL	N.D.	#
10) T	Pentachlo...	7.582	0.000	603039	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	8.122	0.000	1006104	0	<MDL	N.D.	#
12) T	2,4,5-T	8.361	0.000	4357334	0	<MDL	N.D.	#
13) T	2,4-DB	8.877	9.554f	1048431	2843313	<MDL	2.555	#
14) T	DINOSEB	9.883f	0.000	13884110	0	1.279	N.D.	#
15) T	Picloram	9.777	10.978f	120925	6315727	<MDL	<MDL	#
16) T	DCPA	10.208	0.000	334999	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110822\
Data File : PS021062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 09:00
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 12:25:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

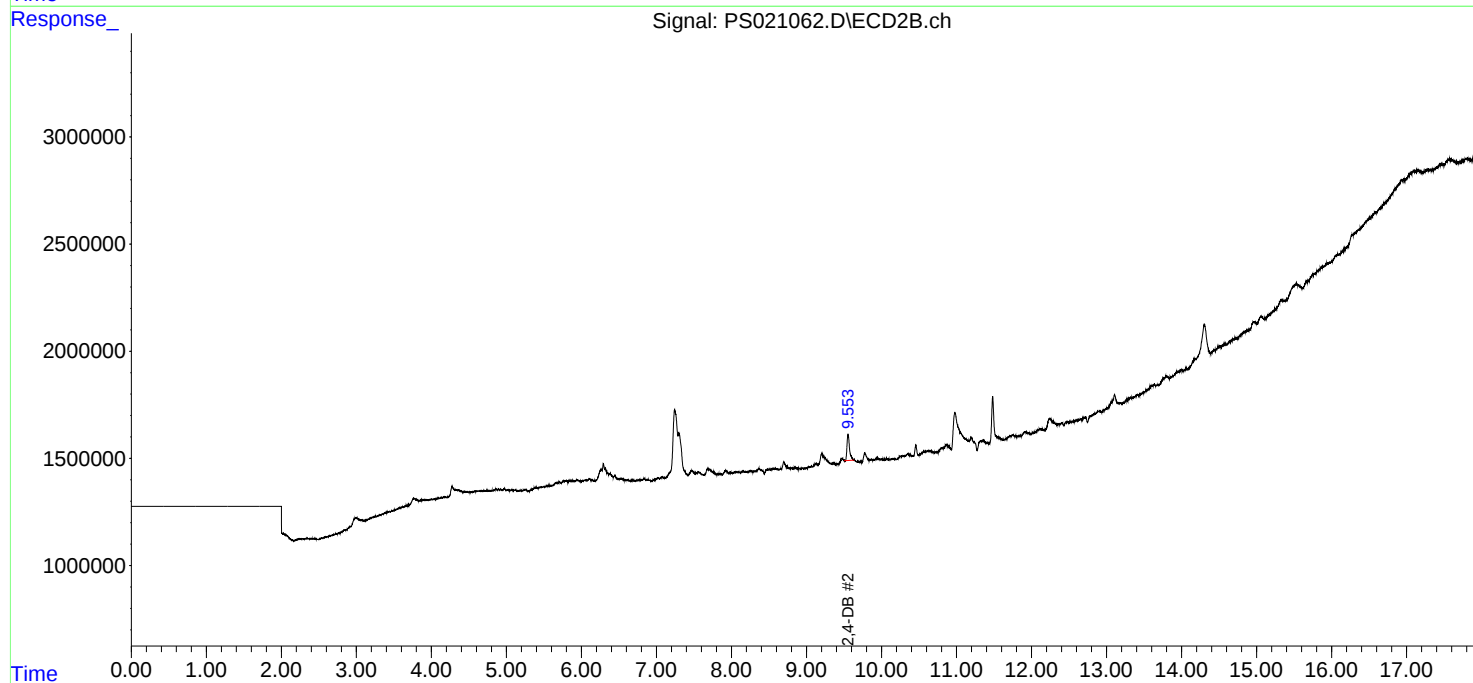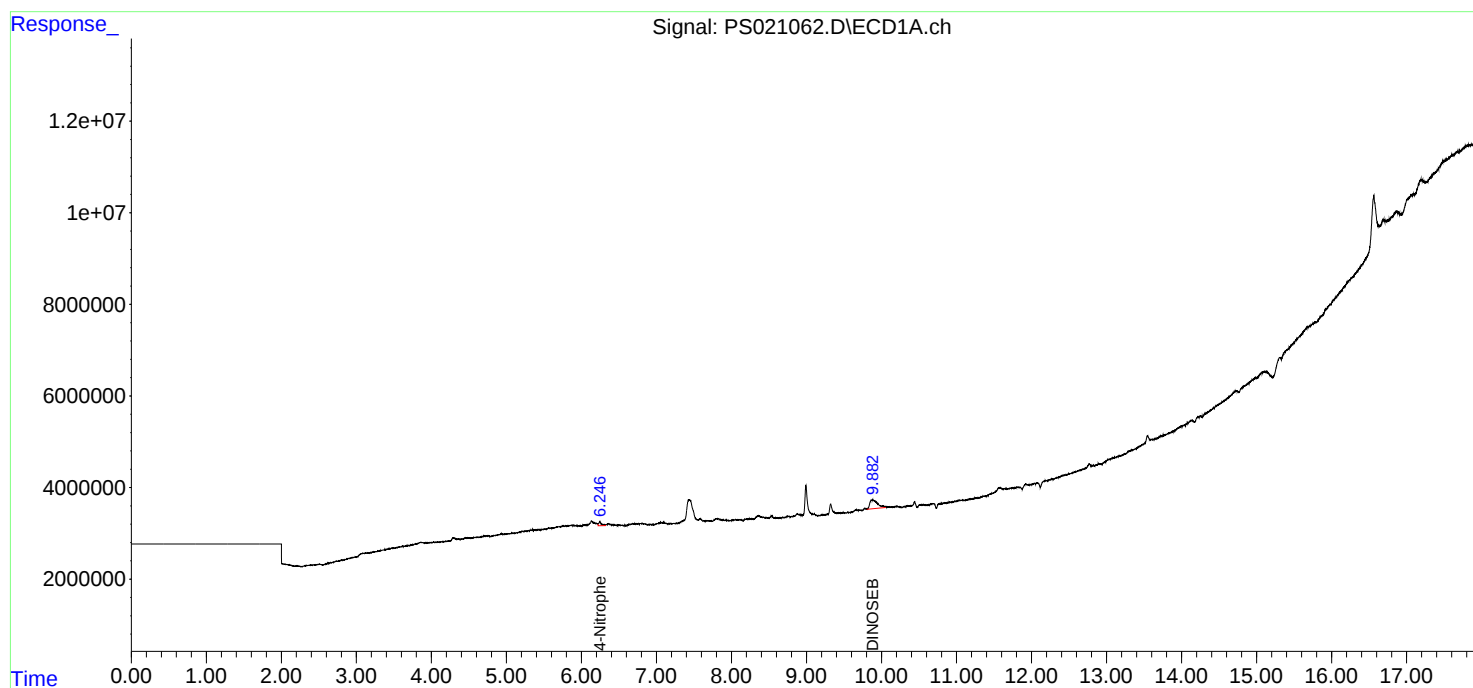


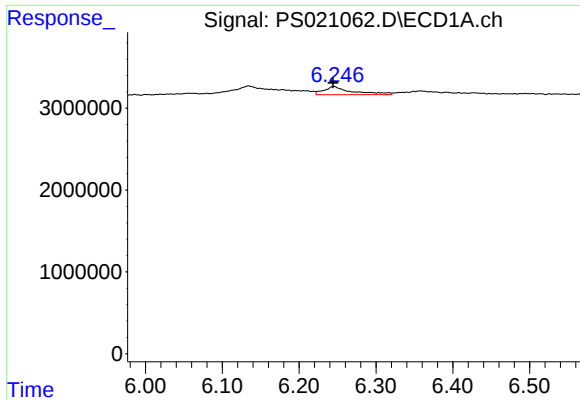

#3 4-Nitrophenol


R.T.: 6.245 min
Delta R.T.: 0.001 min
Response: 2541619
Conc: 1.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

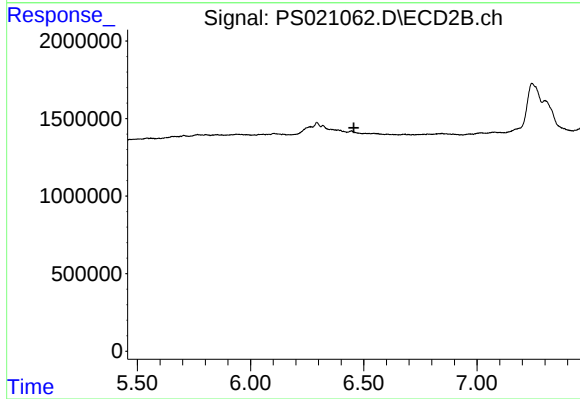


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

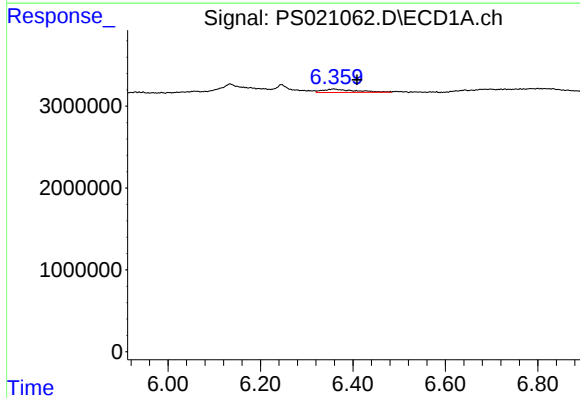


#4 2,4-DCAA

R.T.: 6.359 min
Delta R.T.: -0.051 min
Response: 1950955
Conc: N.D.

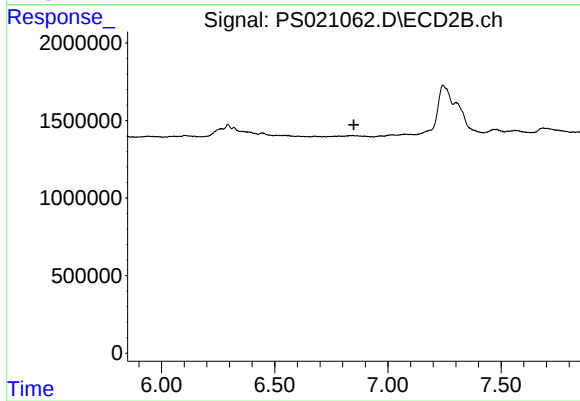

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.

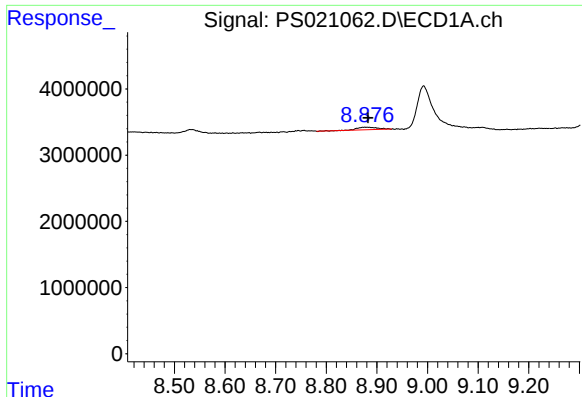

#13 2,4-DB


R.T.: 8.877 min
Delta R.T.: -0.005 min
Response: 1048431
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

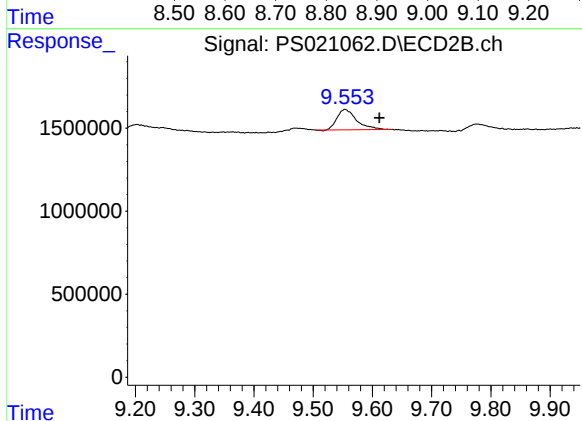


#13 2,4-DB

R.T.: 9.554 min
Delta R.T.: -0.058 min
Response: 2843313
Conc: 2.55 ng/ml

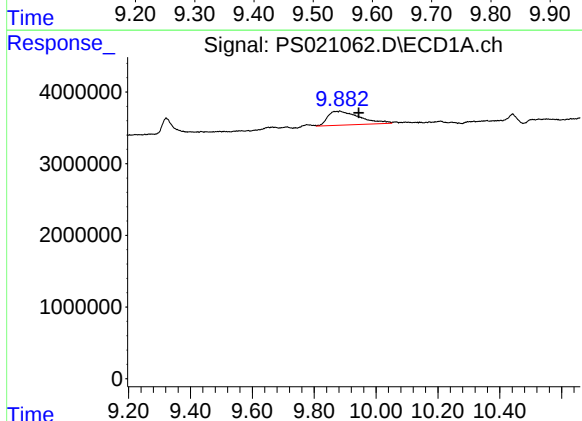

#14 DINOSEB

R.T.: 9.883 min
Delta R.T.: -0.061 min
Response: 13884110
Conc: 1.28 ng/ml

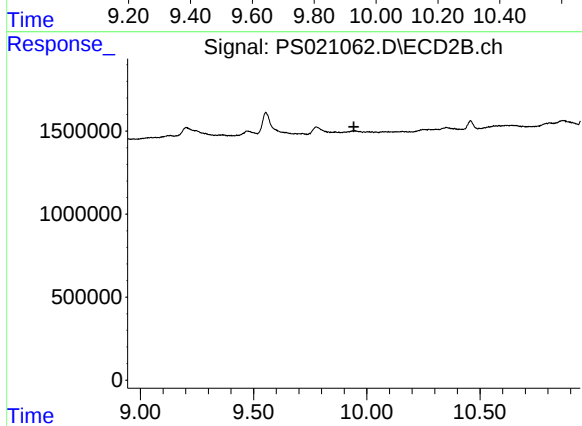

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.943 min
Response: 0
Conc: N.D.