

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110823\
 Data File : PS024784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2023 10:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 23:11:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.358	6.776	1125.7E6	370.9E6	551.411	549.810
Target Compounds						
1) T Dalapon	0.000	2.564	0	1143938	N.D.	1.086
3) T 4-Nitroph...	6.197	6.375	11335633	1407661	8.745	3.206 #
6) T MCPP	6.683	0.000	1741193	0	<MDL	N.D. #
7) T MCPA	0.000	7.257	0	2606175	N.D.	<MDL
8) T DICHLORPROP	0.000	7.565	0	2469382	N.D.	3.380
9) T 2,4-D	0.000	7.779f	0	988053	N.D.	1.104
11) T 2,4,5-TP ...	0.000	8.614	0	691807	N.D.	<MDL
12) T 2,4,5-T	0.000	9.029f	0	1376633	N.D.	<MDL
13) T 2,4-DB	0.000	9.480	0	1092886	N.D.	2.242
15) T Picloram	9.683	10.772	21386978	7713103	1.202	1.269
16) T DCPA	0.000	10.772	0	7713103	N.D.	1.535



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110823\
Data File : PS024784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 10:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 23:11:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

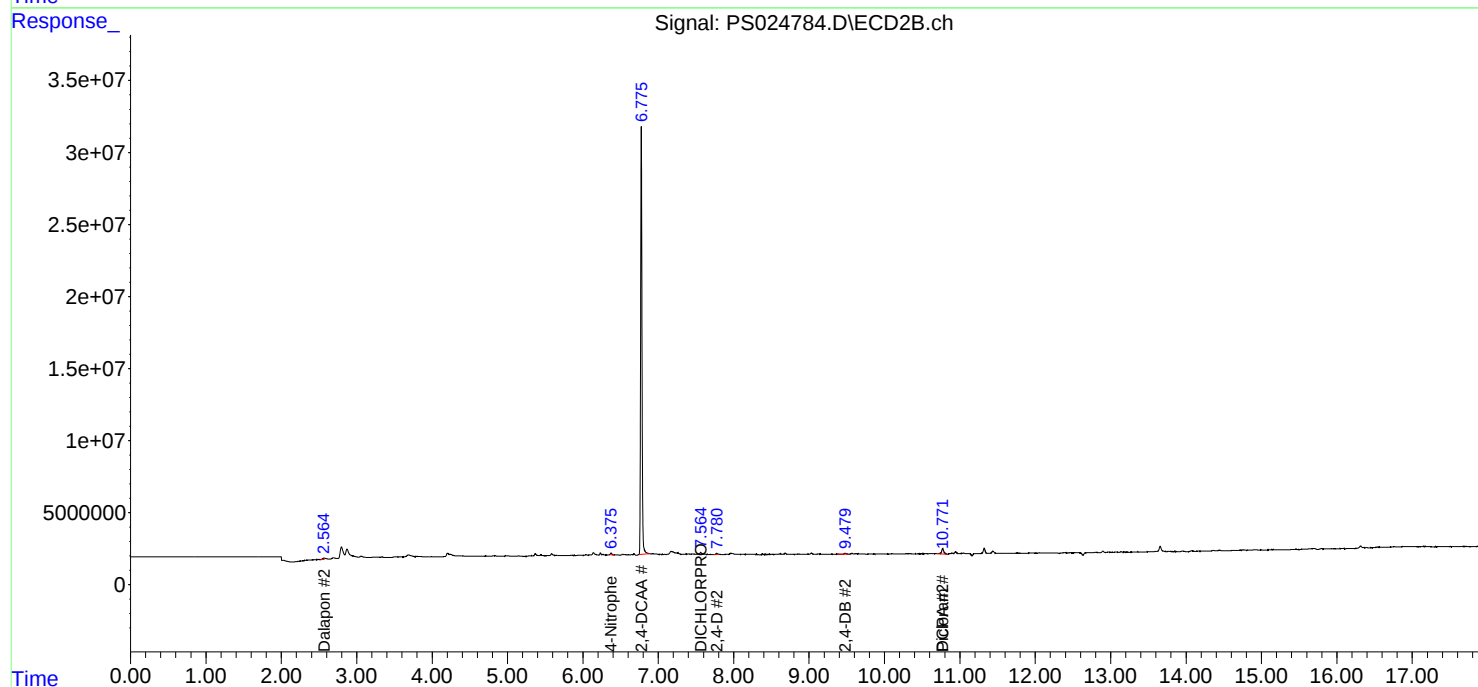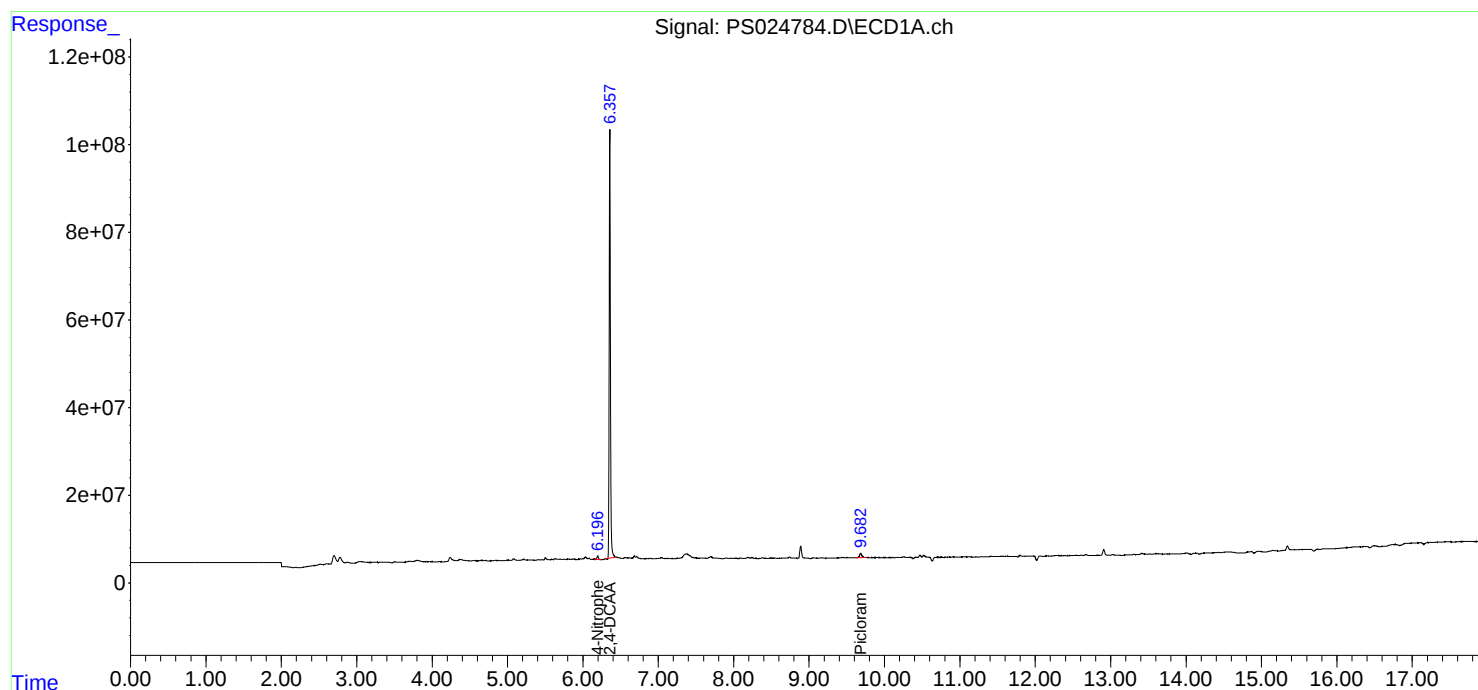


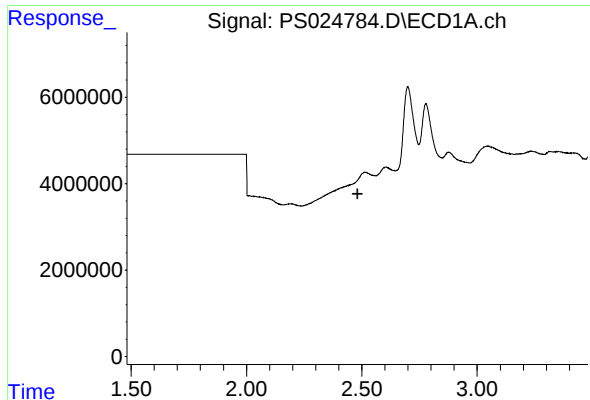

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

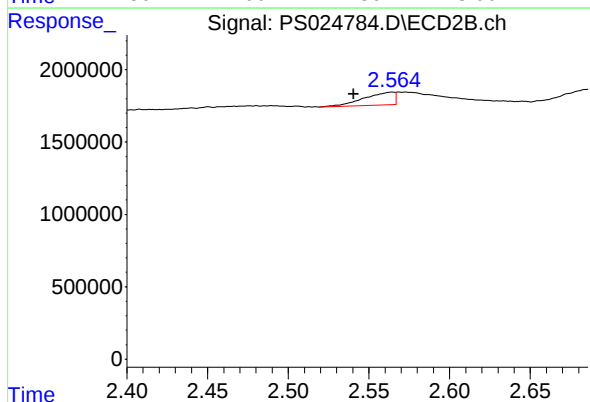


#1 Dalapon

R.T.: 2.564 min
Delta R.T.: 0.024 min
Response: 1143938
Conc: 1.09 ng/ml

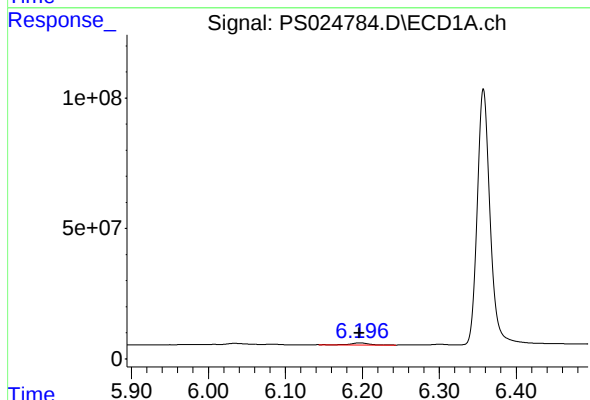


#3 4-Nitrophenol

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 11335633
Conc: 8.75 ng/ml

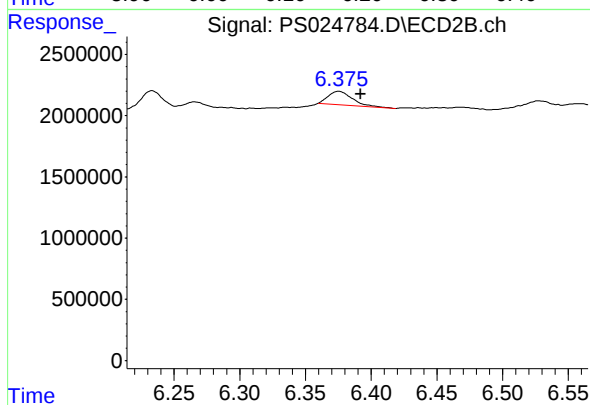

#3 4-Nitrophenol


R.T.: 6.375 min
Delta R.T.: -0.017 min
Response: 1407661
Conc: 3.21 ng/ml

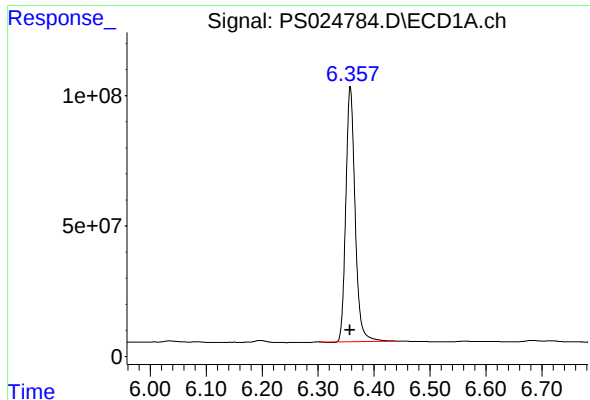

#4 2,4-DCAA


R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 1125706325
Conc: 551.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

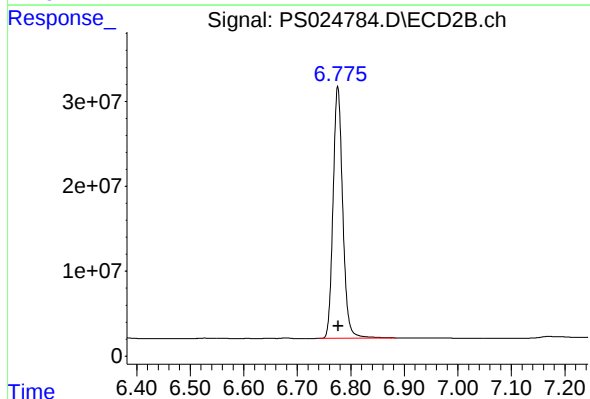


#4 2,4-DCAA

R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 370901478
Conc: 549.81 ng/ml

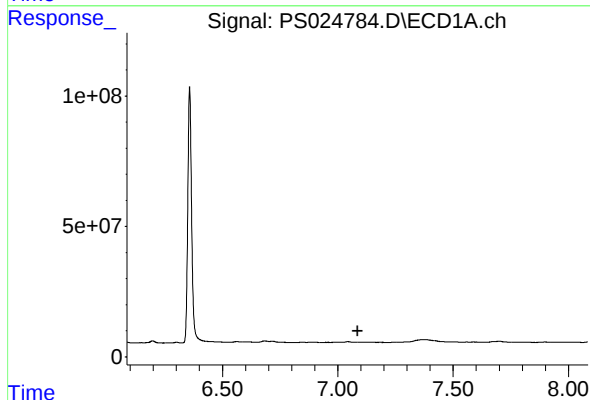


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

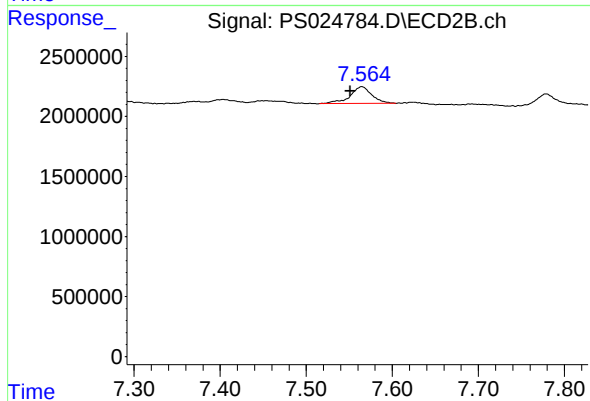

#8 DICHLORPROP


R.T.: 7.565 min
Delta R.T.: 0.013 min
Response: 2469382
Conc: 3.38 ng/ml

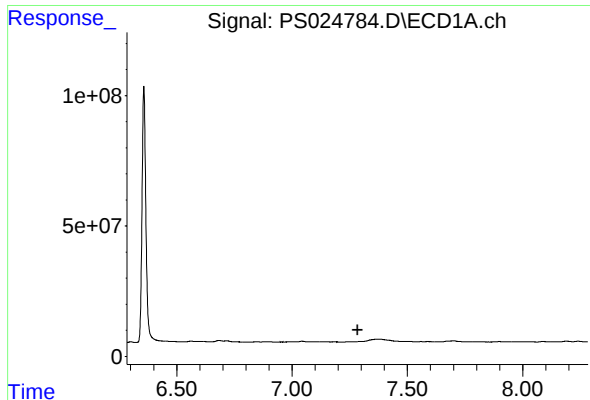

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

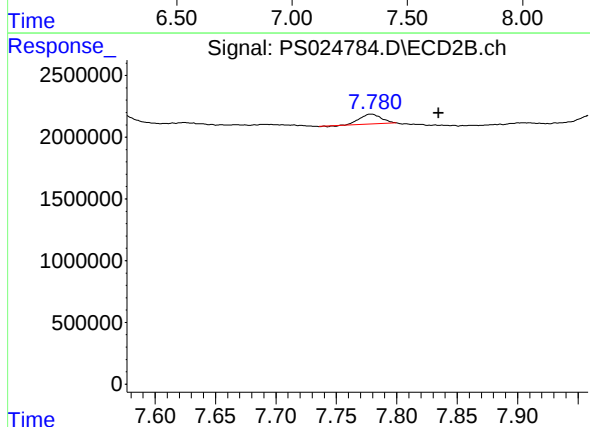


#9 2,4-D

R.T.: 7.779 min
Delta R.T.: -0.056 min
Response: 988053
Conc: 1.10 ng/ml

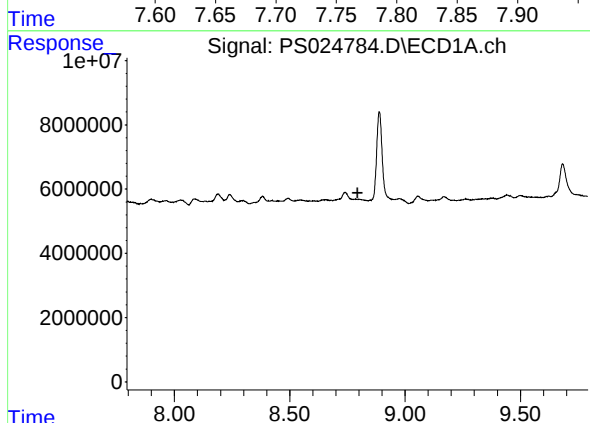


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

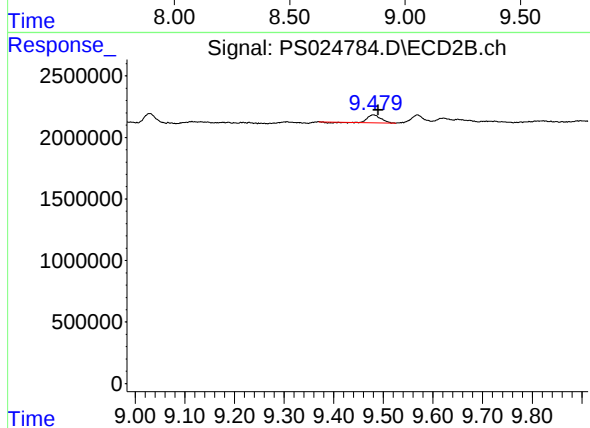

#13 2,4-DB


R.T.: 9.480 min
Delta R.T.: -0.010 min
Response: 1092886
Conc: 2.24 ng/ml

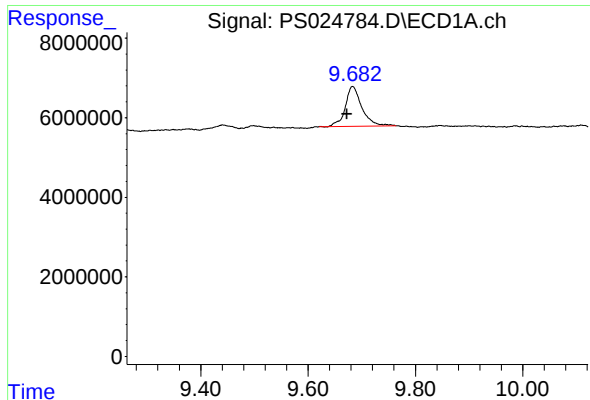

#15 Picloram


R.T.: 9.683 min
Delta R.T.: 0.011 min
Response: 21386978
Conc: 1.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

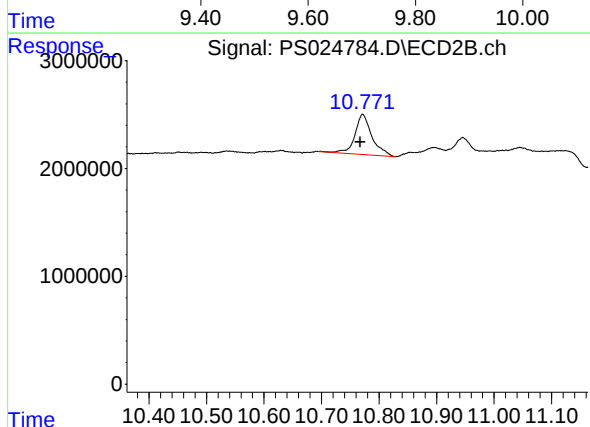


#15 Picloram

R.T.: 10.772 min
Delta R.T.: 0.004 min
Response: 7713103
Conc: 1.27 ng/ml

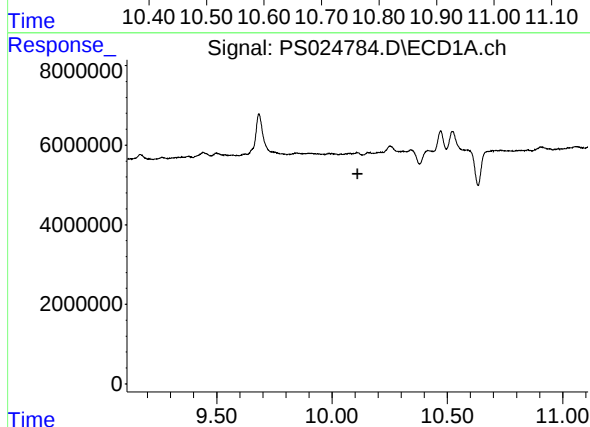

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.111 min
Response: 0
Conc: N.D.

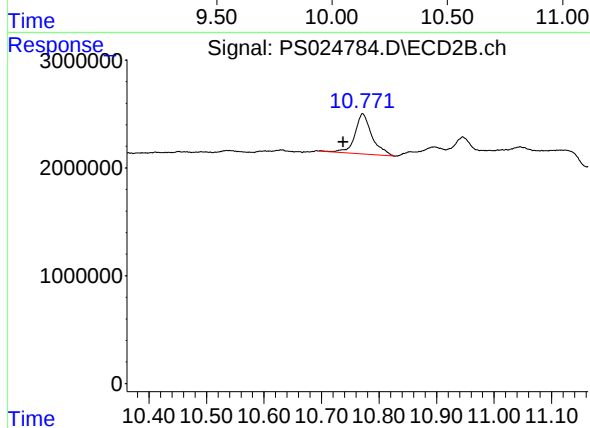

#16 DCPA

R.T.: 10.772 min
Delta R.T.: 0.034 min
Response: 7713103
Conc: 1.53 ng/ml