

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 11:13
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 15:57:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.944	0	243522	N.D.	0.666 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.090	0	38541	N.D.	0.085 #
3) T	4-Nitroph...	0.000	10.080	0	148325	N.D.	0.847 #
5) T	DICAMBA	0.000	11.216	0	51064	N.D.	0.038 #
6) T	MCP	0.000	11.450	0	464514	N.D.	0.512 #
7) T	MCPA	0.000	11.785	0	86009	N.D.	0.061 #
8) T	DICHLORPROP	0.000	12.376	0	122587	N.D.	0.370 #
9) T	2,4-D	0.000	12.754	0	85572	N.D.	0.214 #
10) T	Pentachlo...	0.000	13.350	0	74096	N.D.	0.015 #
12) T	2,4,5-T	0.000	14.506	0	1826983	N.D.	1.169 #
15) T	Picloram	16.911	16.815	8235102	6350426	3.878	2.387 #
16) T	DCPA	0.000	16.815	0	6350426	N.D.	2.648 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 11:13
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 15:57:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

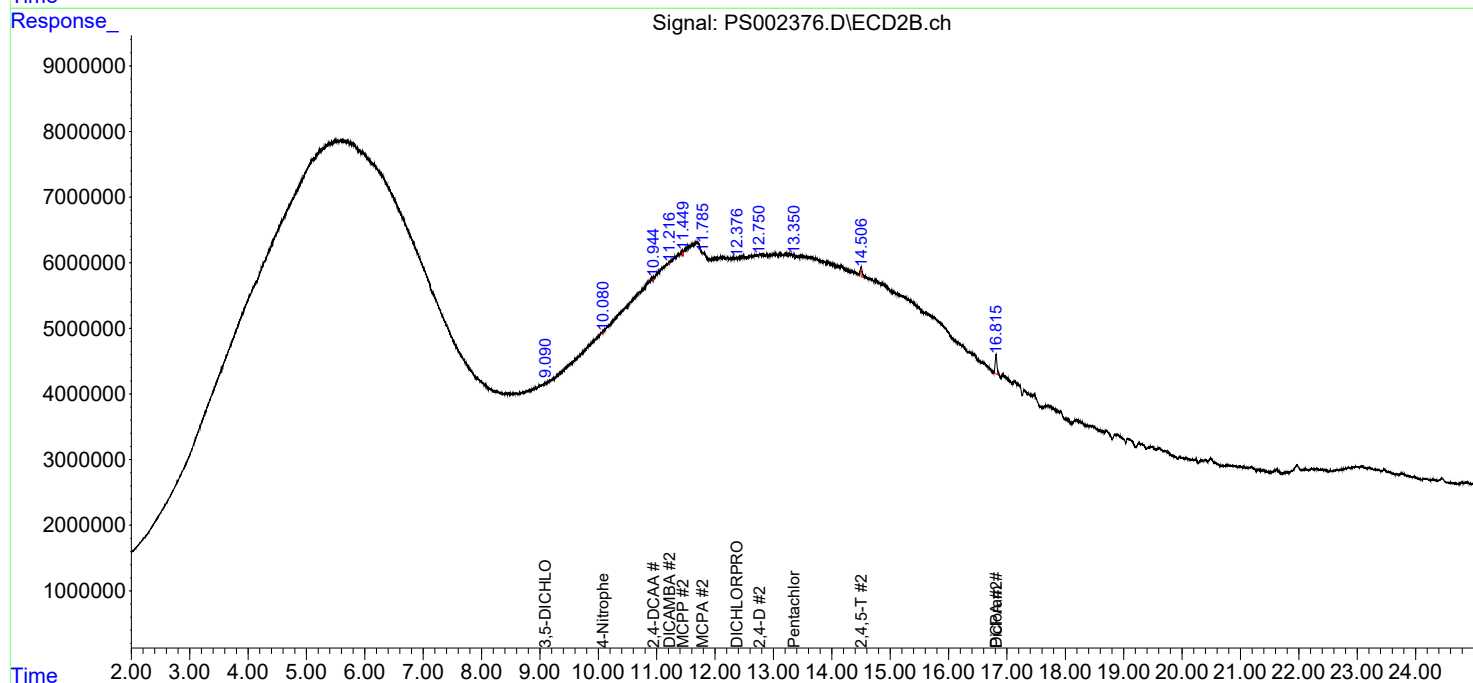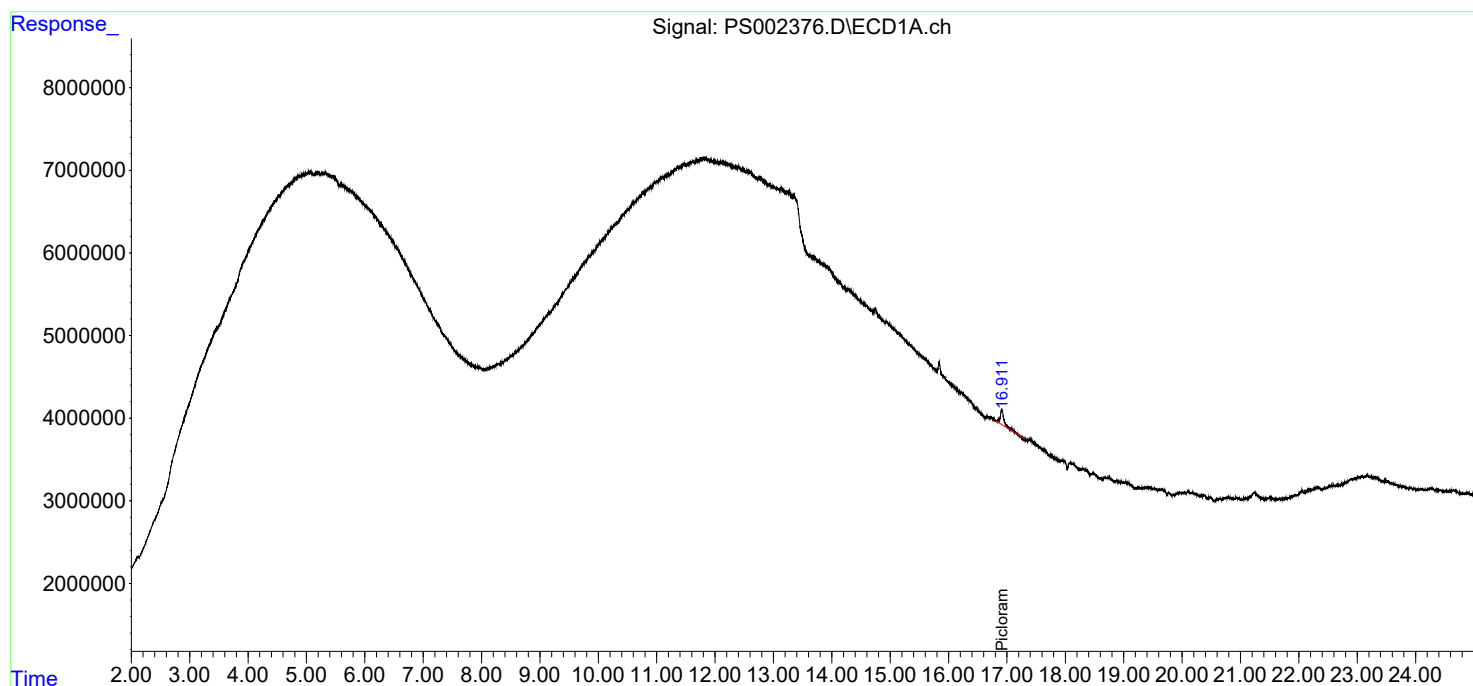


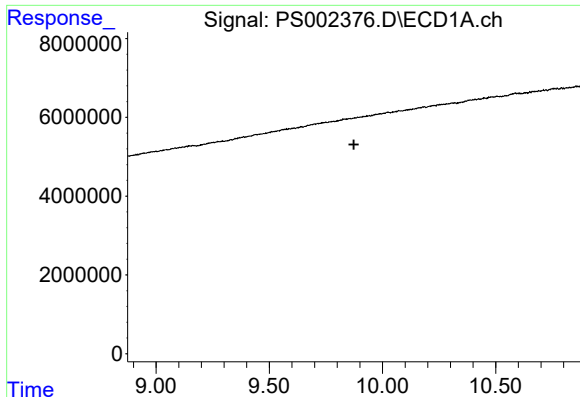

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

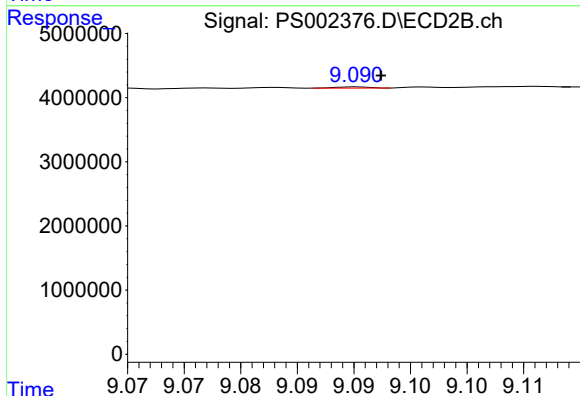


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.090 min
Delta R.T.: -0.002 min
Response: 38541
Conc: 0.09 ng/ml

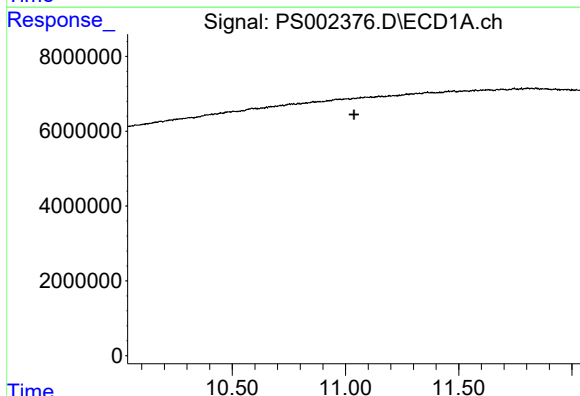


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

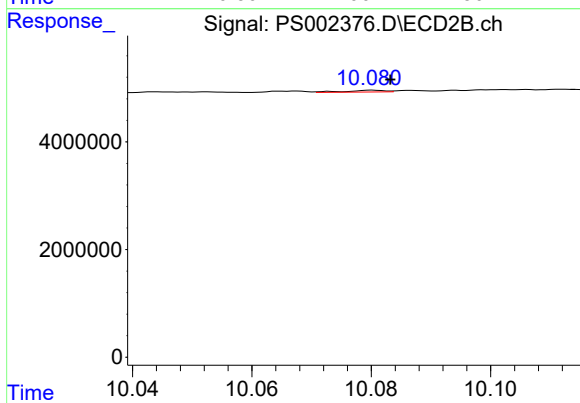

#3 4-Nitrophenol


R.T.: 10.080 min
Delta R.T.: -0.003 min
Response: 148325
Conc: 0.85 ng/ml

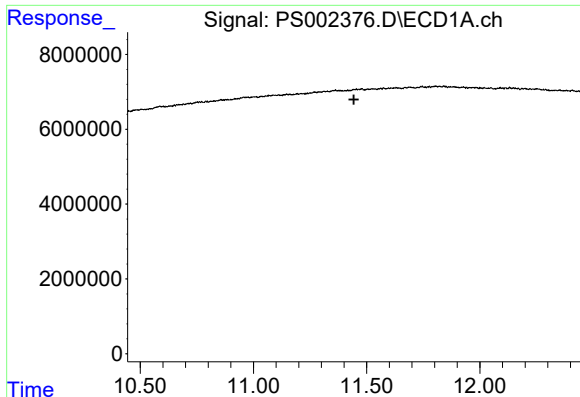

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.444 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

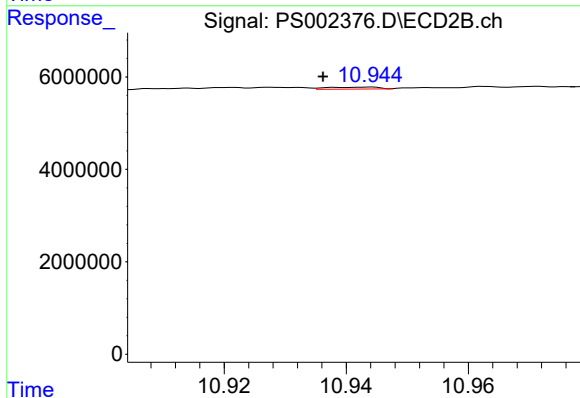


#4 2,4-DCAA

R.T.: 10.944 min
Delta R.T.: 0.008 min
Response: 243522
Conc: 0.67 ng/ml

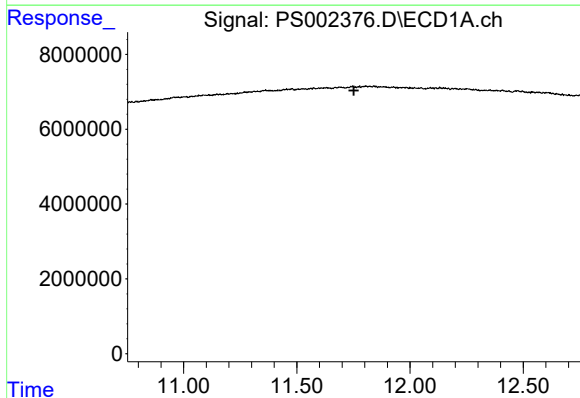


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 11.752 min
Response: 0
Conc: N.D.

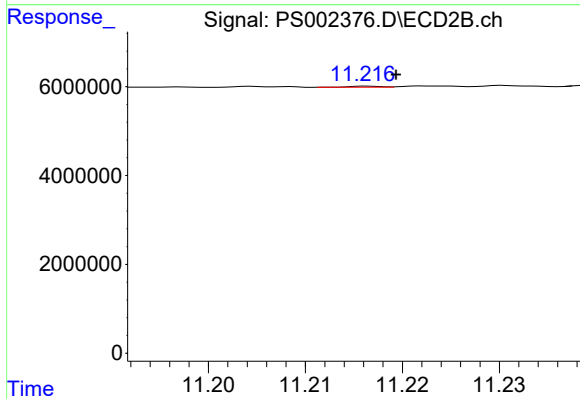

#5 DICAMBA


R.T.: 11.216 min
Delta R.T.: -0.003 min
Response: 51064
Conc: 0.04 ng/ml

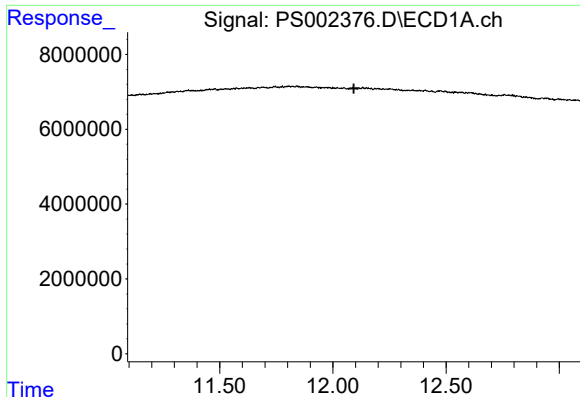

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 12.093 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

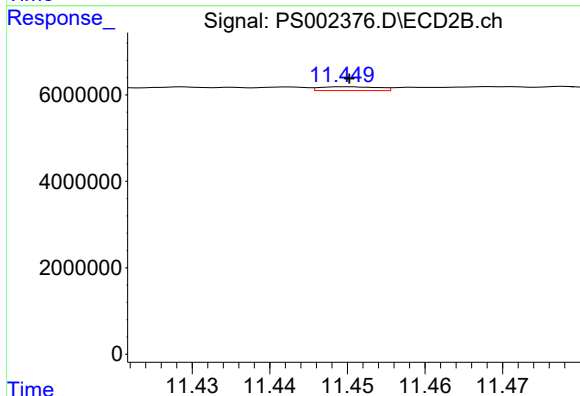


#6 MCPP

R.T.: 11.450 min
Delta R.T.: 0.000 min
Response: 464514
Conc: 0.51 ug/ml

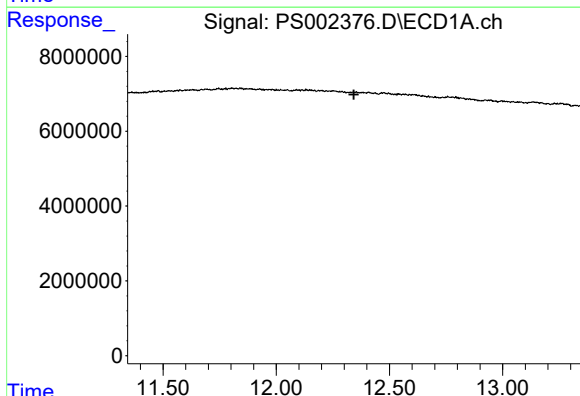


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.343 min
Response: 0
Conc: N.D.

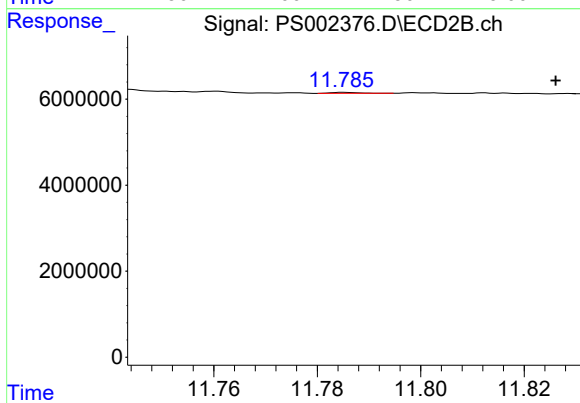

#7 MCPA


R.T.: 11.785 min
Delta R.T.: -0.041 min
Response: 86009
Conc: 0.06 ug/ml

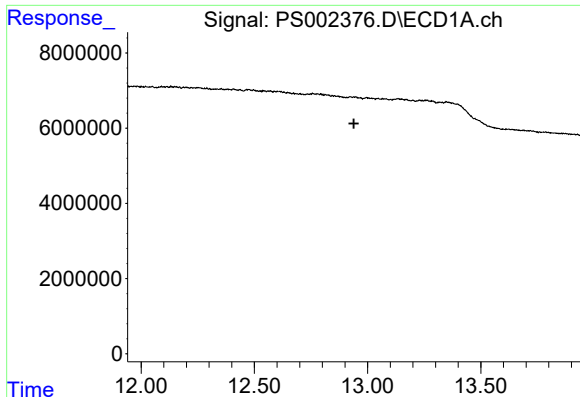

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.939 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

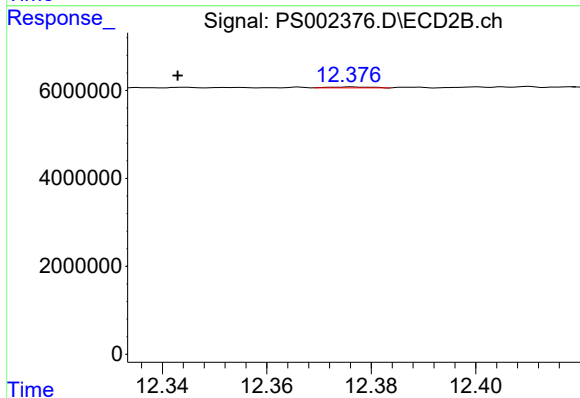


#8 DICHLORPROP

R.T.: 12.376 min
Delta R.T.: 0.033 min
Response: 122587
Conc: 0.37 ng/ml

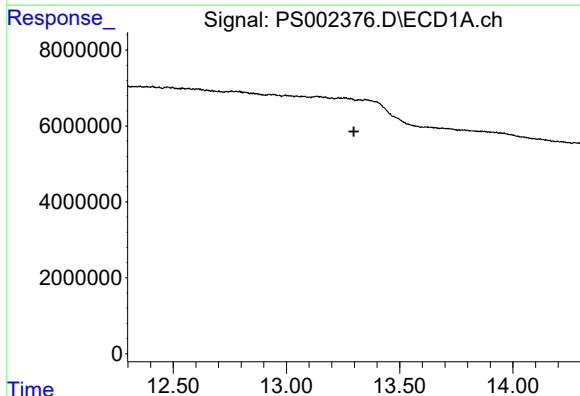


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.298 min
Response: 0
Conc: N.D.

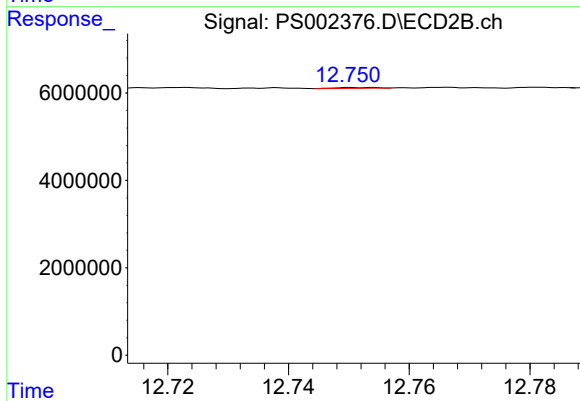

#9 2,4-D


R.T.: 12.754 min
Delta R.T.: -0.060 min
Response: 85572
Conc: 0.21 ng/ml

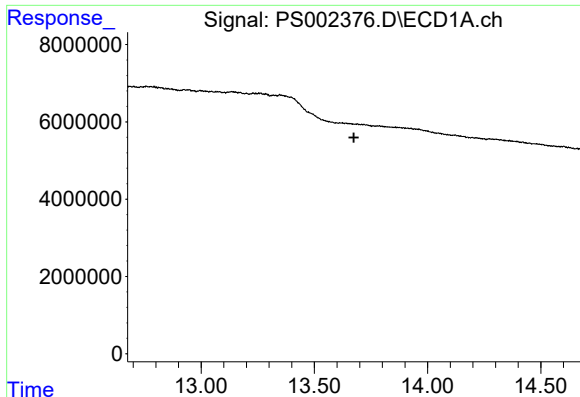

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

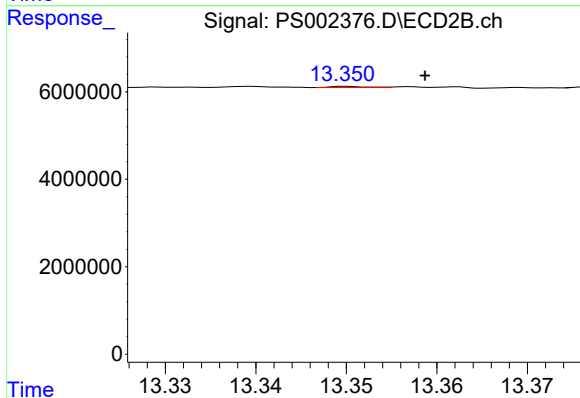


#10 Pentachlorophenol

R.T.: 13.350 min
Delta R.T.: -0.009 min
Response: 74096
Conc: 0.01 ng/ml

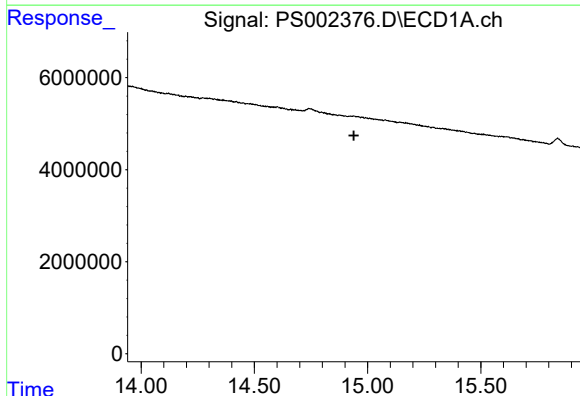


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.940 min
Response: 0
Conc: N.D.

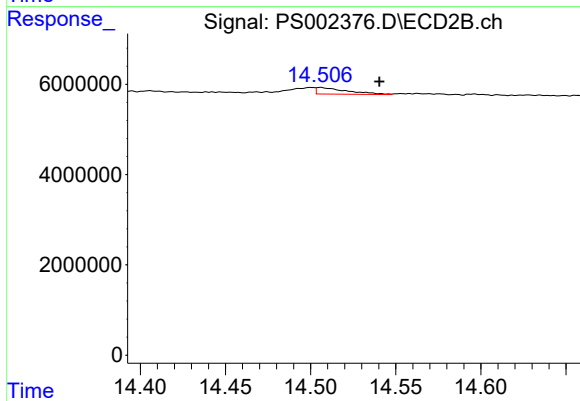

#12 2,4,5-T


R.T.: 14.506 min
Delta R.T.: -0.035 min
Response: 1826983
Conc: 1.17 ng/ml

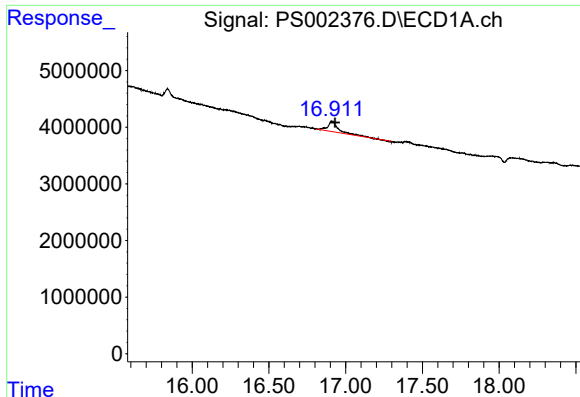

#15 Picloram


R.T.: 16.911 min
Delta R.T.: -0.020 min
Response: 8235102
Conc: 3.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

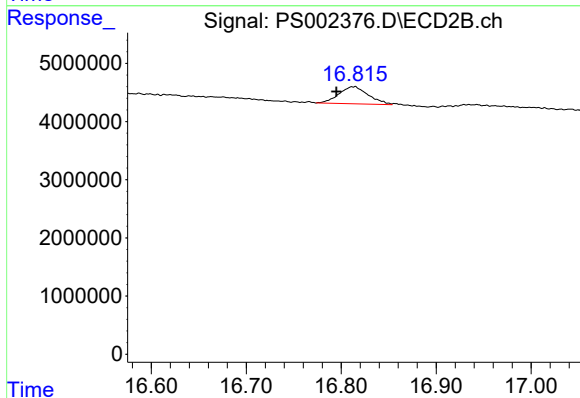


#15 Picloram

R.T.: 16.815 min
Delta R.T.: 0.020 min
Response: 6350426
Conc: 2.39 ng/ml

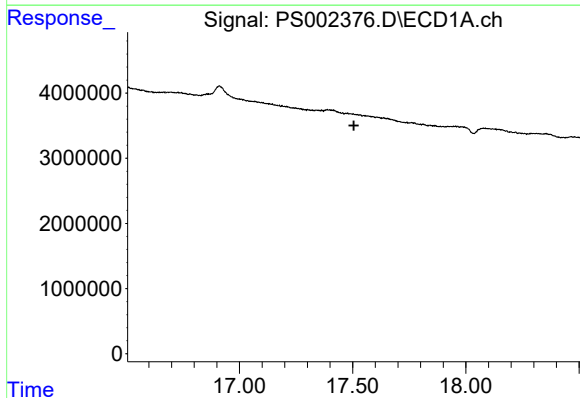

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

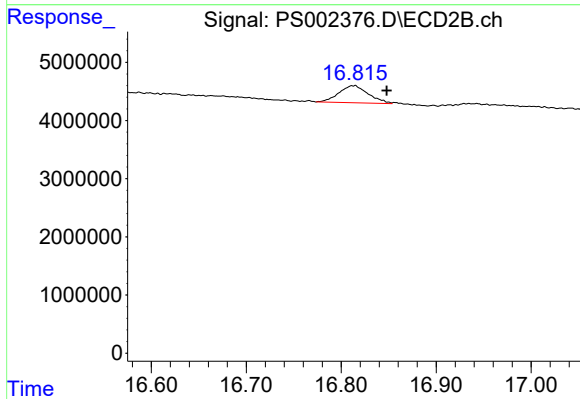

#16 DCPA

R.T.: 16.815 min
Delta R.T.: -0.033 min
Response: 6350426
Conc: 2.65 ng/ml