

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 11:44
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 15:57:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.429	10.919	141.8E6	142.4E6	465.494	389.193
Target Compounds							
1) T	Dalapon	0.000	2.358	0	131278	N.D.	0.305 #
7) T	MCPA	0.000	11.813	0	1235836	N.D.	0.878 #
10) T	Pentachlo...	0.000	13.342	0	55706	N.D.	0.011 #
12) T	2,4,5-T	0.000	14.550	0	461896	N.D.	0.295 #
15) T	Picloram	0.000	16.855	0	3241388	N.D.	1.218 #
16) T	DCPA	0.000	16.855	0	3241388	N.D.	1.352 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 11:44
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 15:57:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

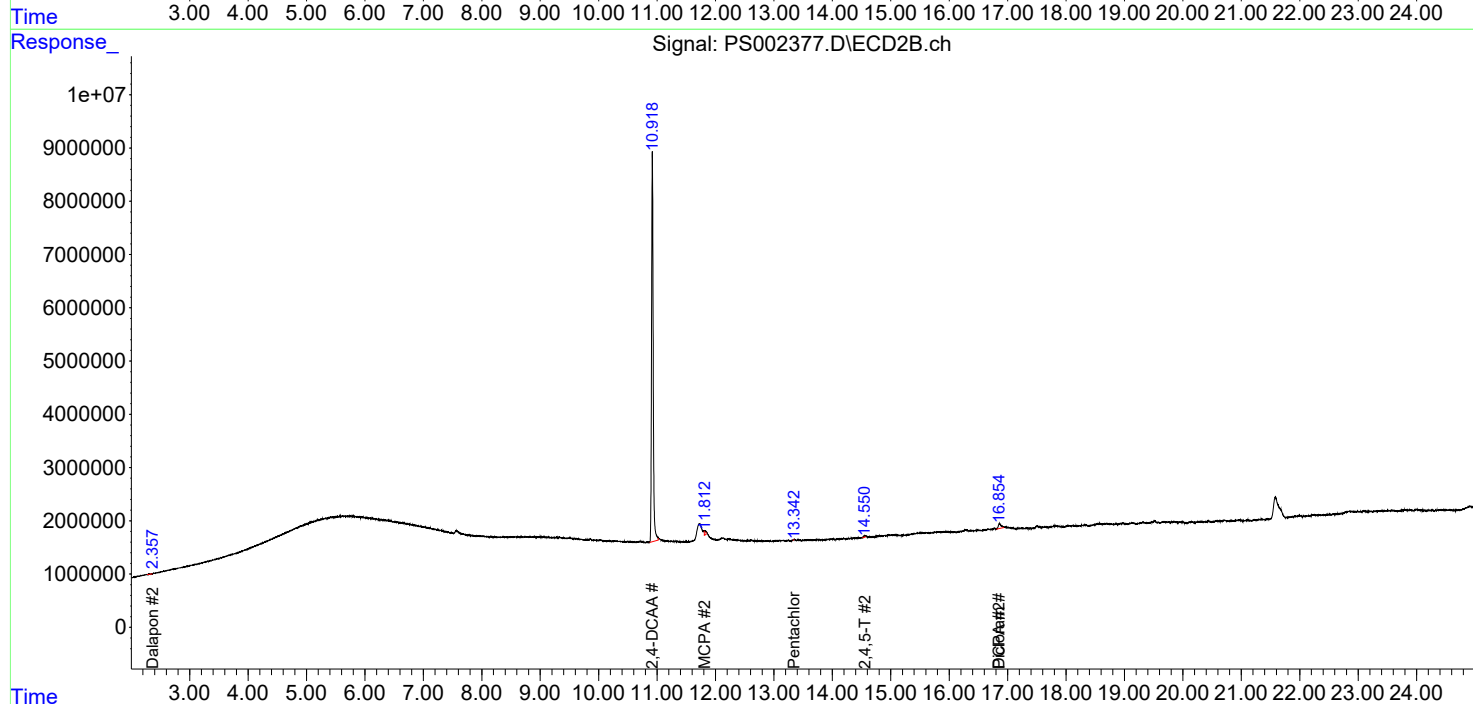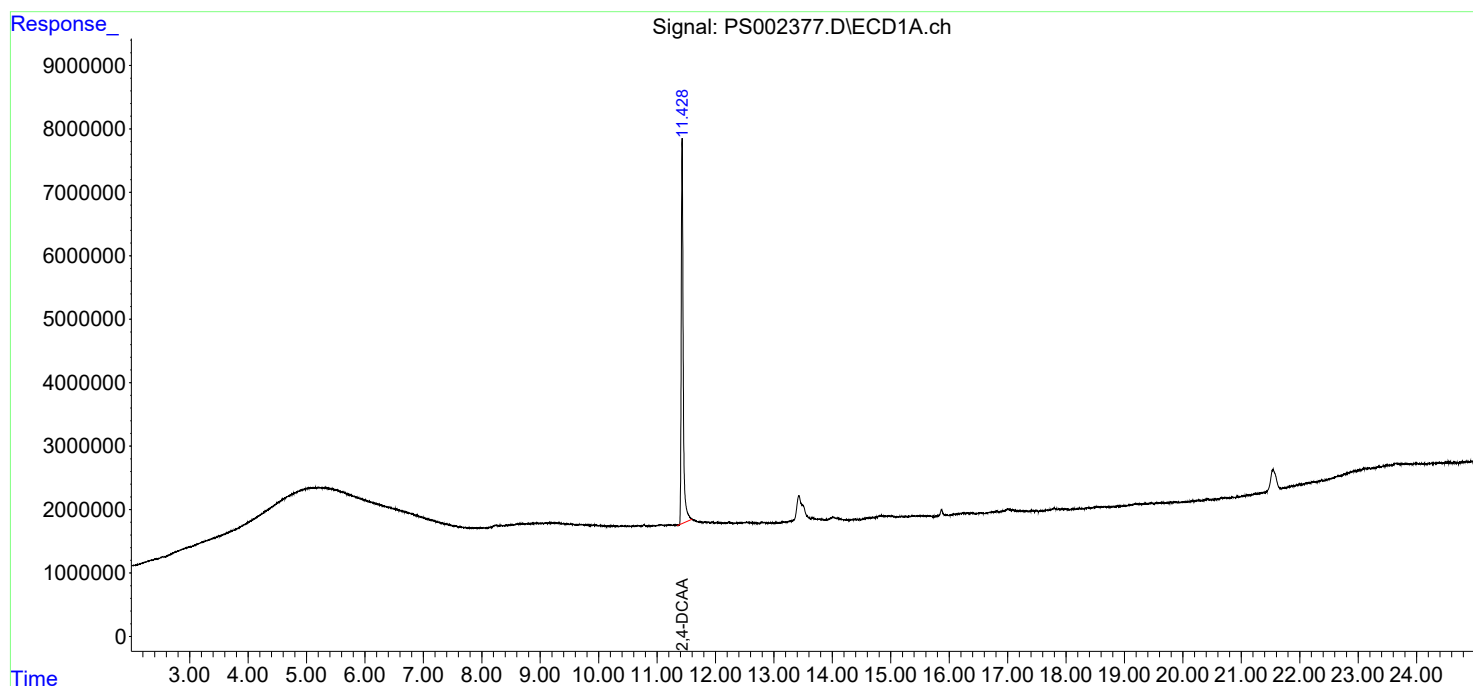


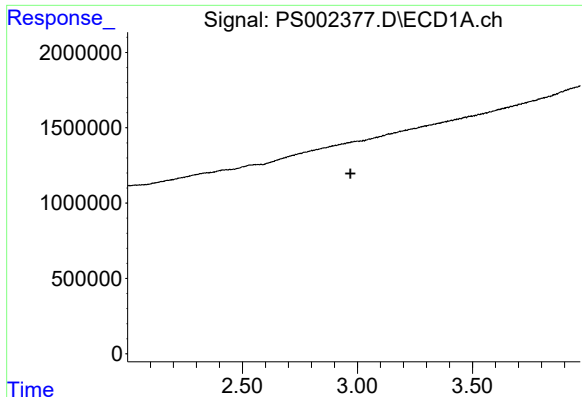

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

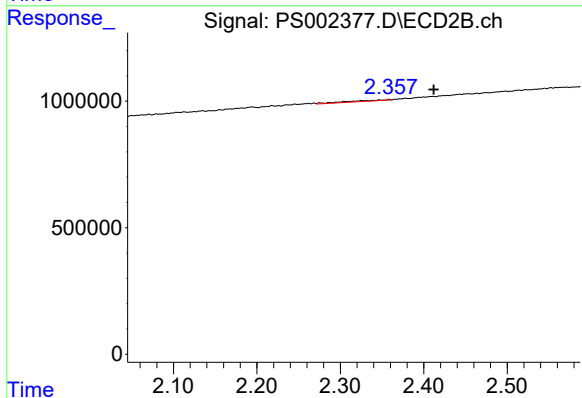


#1 Dalapon

R.T.: 2.358 min
Delta R.T.: -0.054 min
Response: 131278
Conc: 0.31 ng/ml

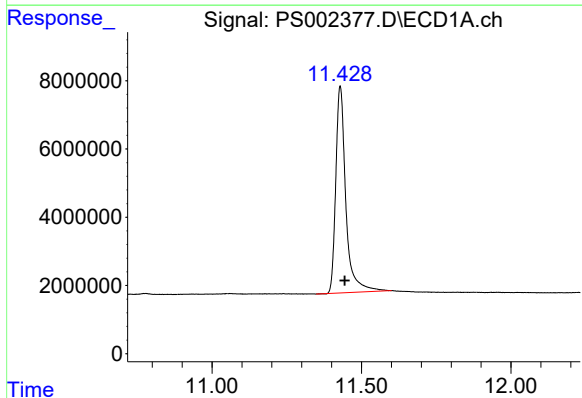


#4 2,4-DCAA

R.T.: 11.429 min
Delta R.T.: -0.015 min
Response: 141789390
Conc: 465.49 ng/ml

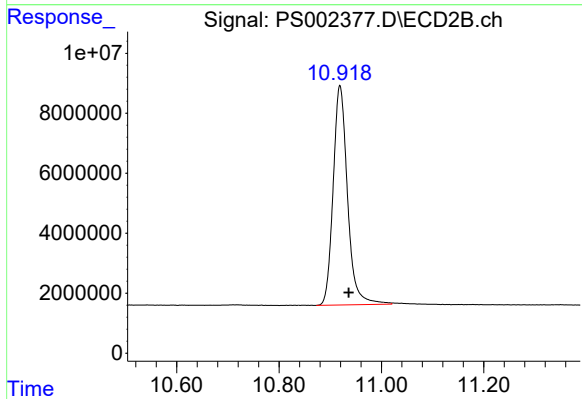

#4 2,4-DCAA


R.T.: 10.919 min
Delta R.T.: -0.017 min
Response: 142410598
Conc: 389.19 ng/ml

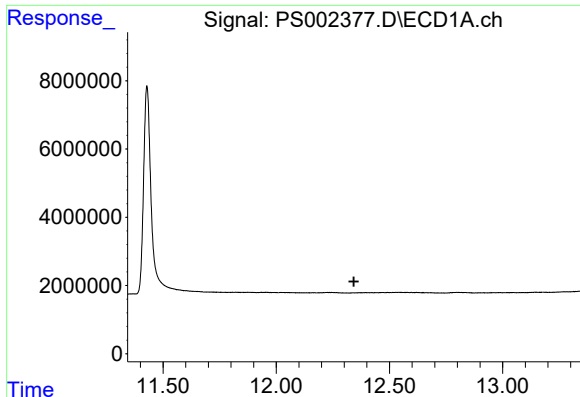

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

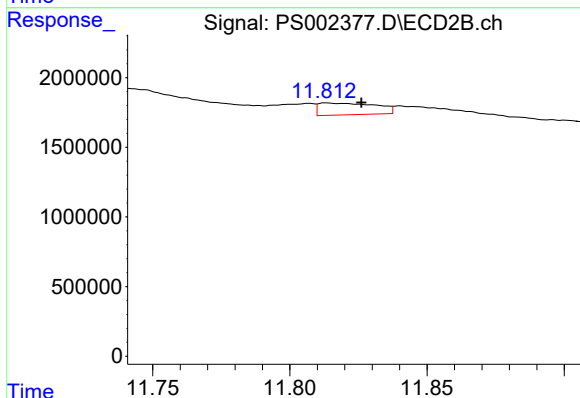


#7 MCPA

R.T.: 11.813 min
Delta R.T.: -0.013 min
Response: 1235836
Conc: 0.88 ug/ml

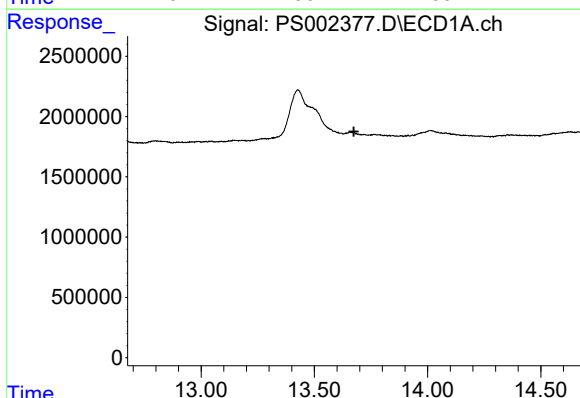


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.675 min
Response: 0
Conc: N.D.

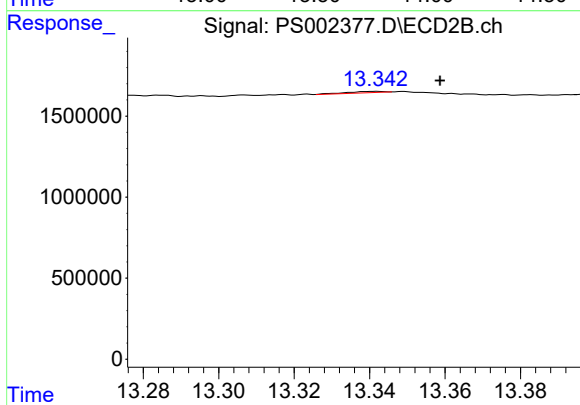

#10 Pentachlorophenol


R.T.: 13.342 min
Delta R.T.: -0.017 min
Response: 55706
Conc: 0.01 ng/ml

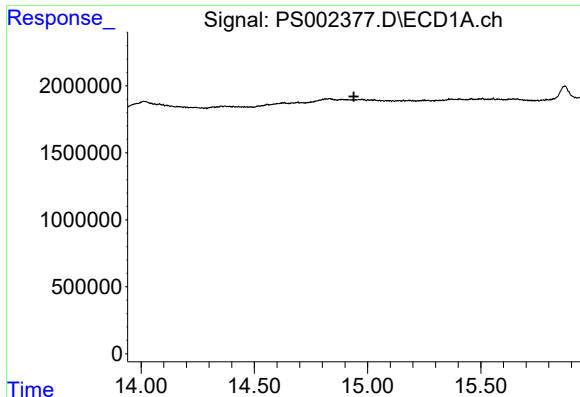

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

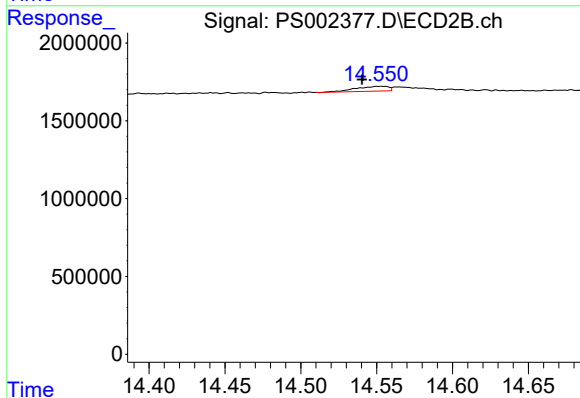


#12 2,4,5-T

R.T.: 14.550 min
Delta R.T.: 0.009 min
Response: 461896
Conc: 0.30 ng/ml

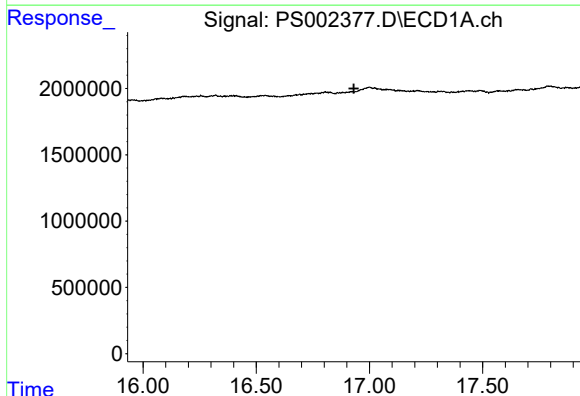


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.931 min
Response: 0
Conc: N.D.

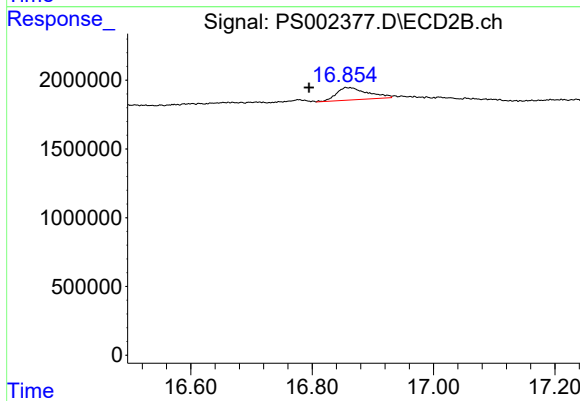

#15 Picloram


R.T.: 16.855 min
Delta R.T.: 0.060 min
Response: 3241388
Conc: 1.22 ng/ml

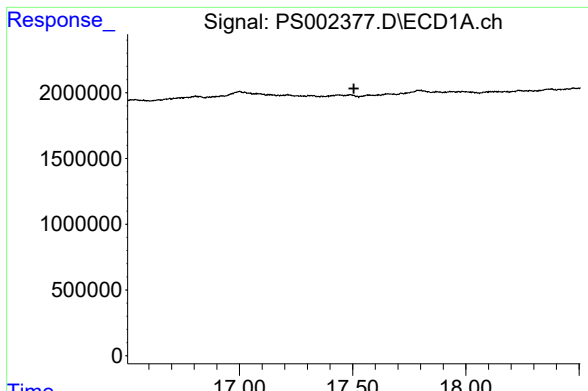

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

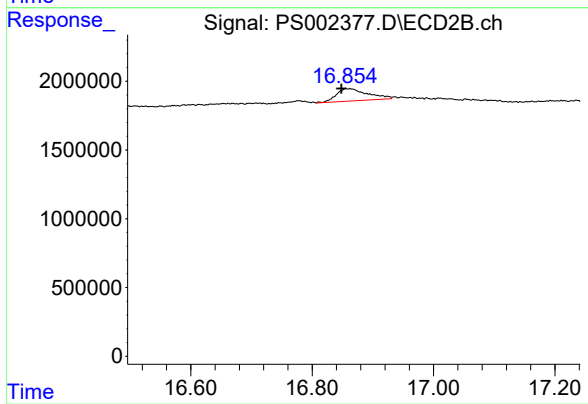

#16 DCPA

R.T.: 16.855 min
Delta R.T.: 0.007 min
Response: 3241388
Conc: 1.35 ng/ml