

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002389.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 18:22
 Operator : EI\SJ
 Sample : J5768-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 22:00:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.426	10.920	174.5E6	172.0E6	572.940	469.992
Target Compounds							
1) T	Dalapon	2.909	2.358	4701338	2975584	10.662	6.914 #
3) T	4-Nitroph...	0.000	10.078	0	3530794	N.D.	20.152 #
5) T	DICAMBA	0.000	11.268	0	38014	N.D.	0.028 #
6) T	MCP	12.108	0.000	53787140	0	57.310	N.D. #
7) T	MCPA	0.000	11.816	0	4289478	N.D.	3.048 #
9) T	2,4-D	0.000	12.755	0	83700	N.D.	0.210 #
10) T	Pentachlo...	13.667	0.000	3403615	0	0.704	N.D. #
12) T	2,4,5-T	0.000	14.543	0	127494	N.D.	0.082 #
14) T	DINOSEB	0.000	15.657	0	2537905	N.D.	1.696 #
15) T	Picloram	0.000	16.797	0	1185749	N.D.	0.446 #
16) T	DCPA	17.567	16.839	-1323926	11366199	N.D.	4.739



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002389.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 18:22
Operator : EI\SJ
Sample : J5768-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 22:00:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

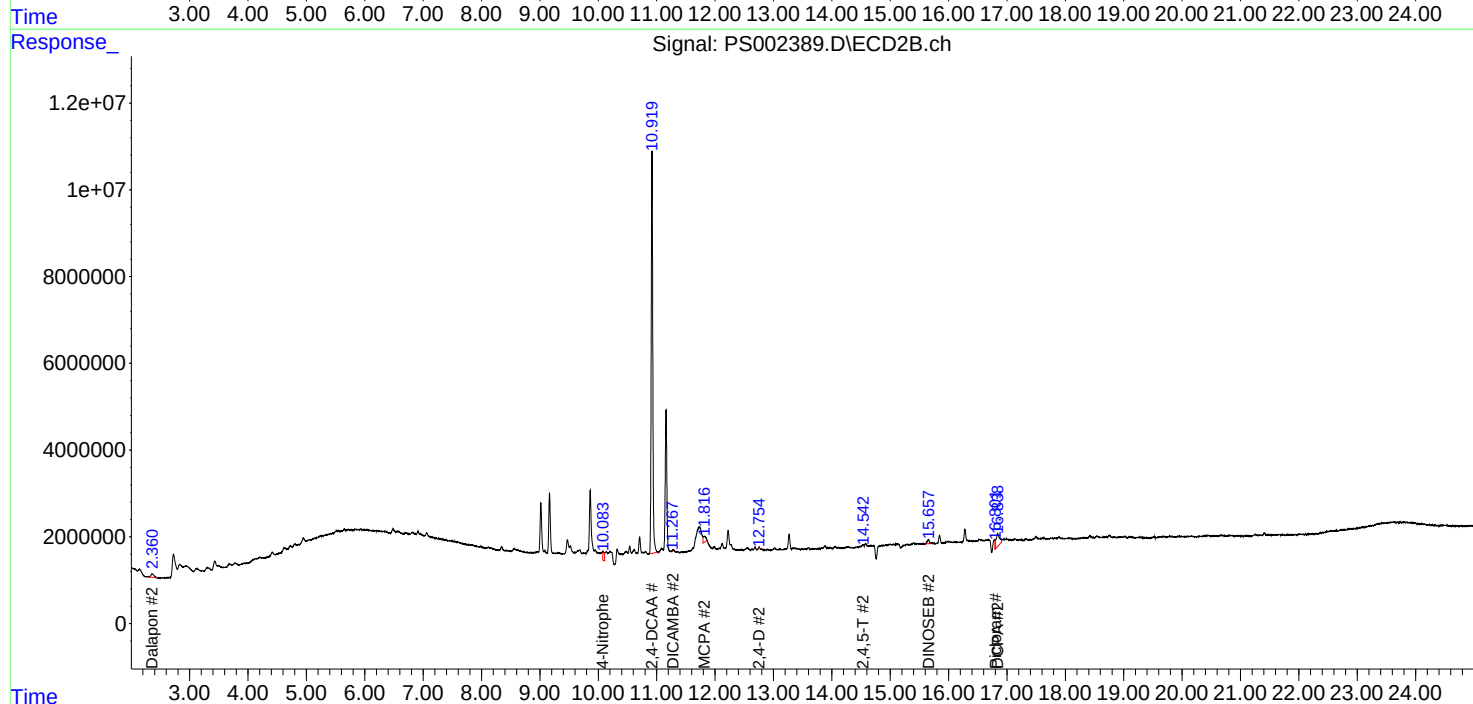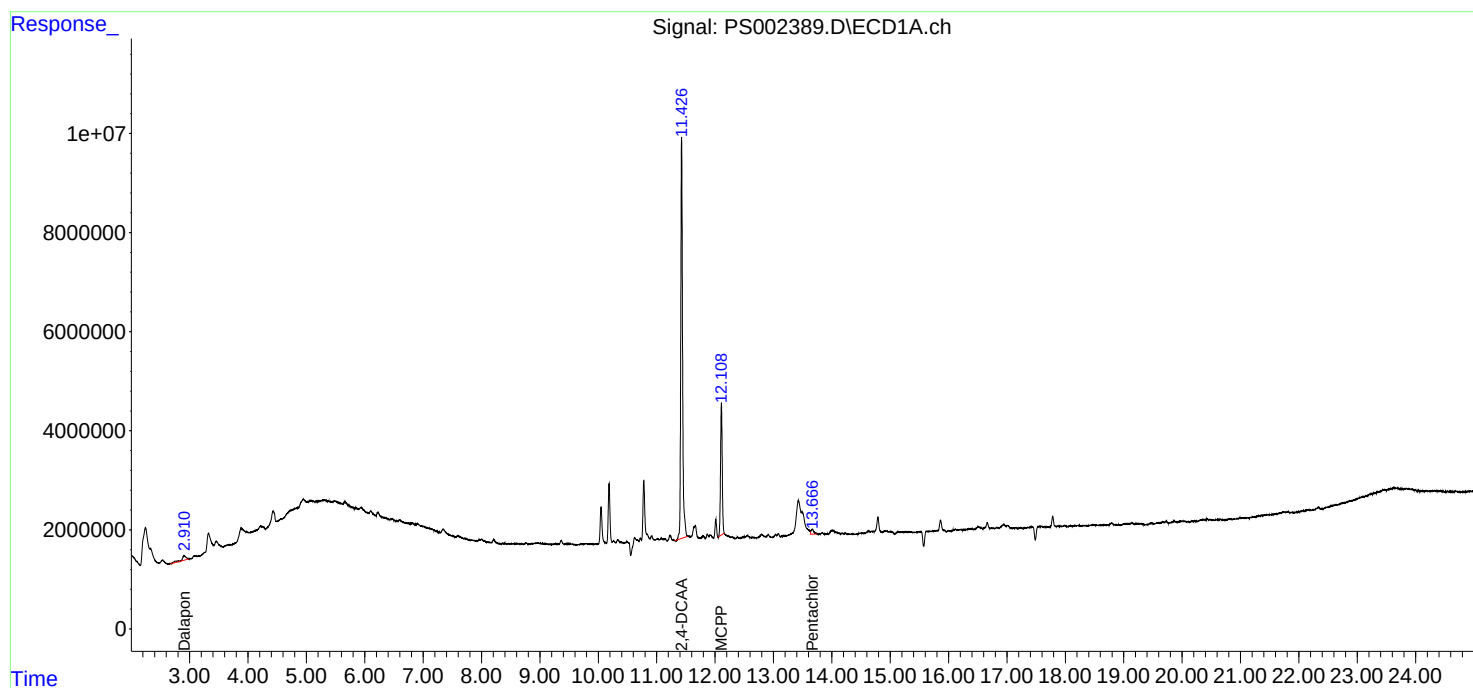


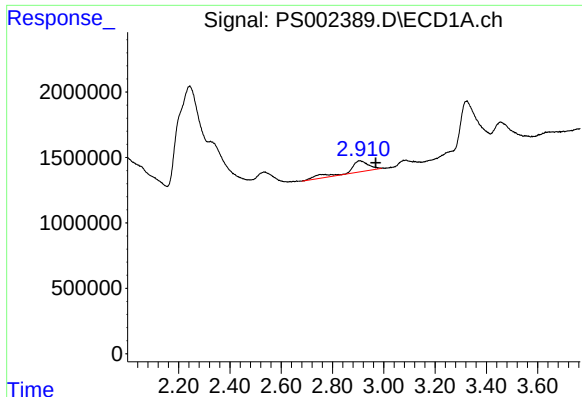

#1 Dalapon


R.T.: 2.909 min
Delta R.T.: -0.060 min
Response: 4701338
Conc: 10.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

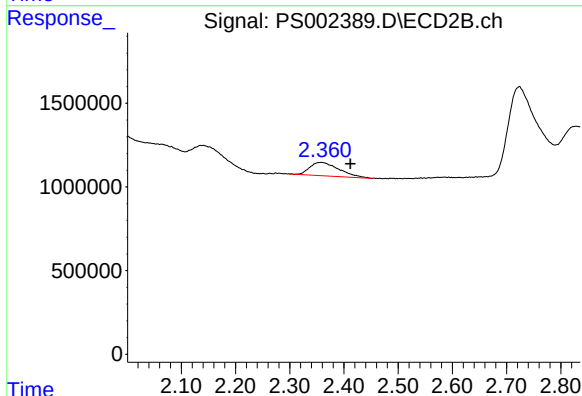


#1 Dalapon

R.T.: 2.358 min
Delta R.T.: -0.054 min
Response: 2975584
Conc: 6.91 ng/ml

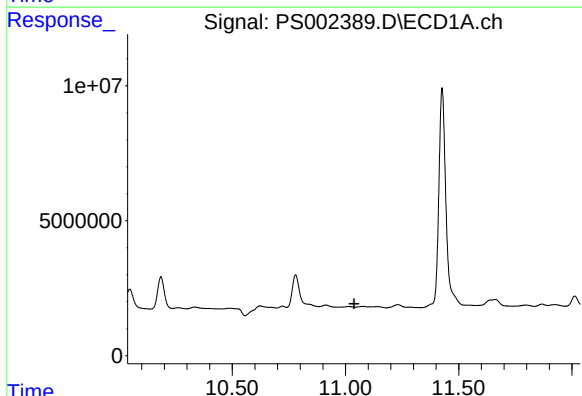


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

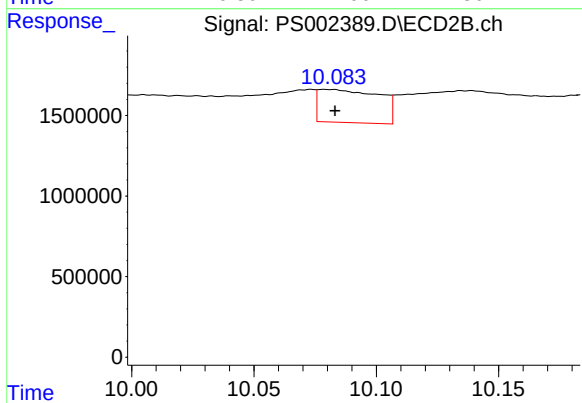

#3 4-Nitrophenol


R.T.: 10.078 min
Delta R.T.: -0.005 min
Response: 3530794
Conc: 20.15 ng/ml

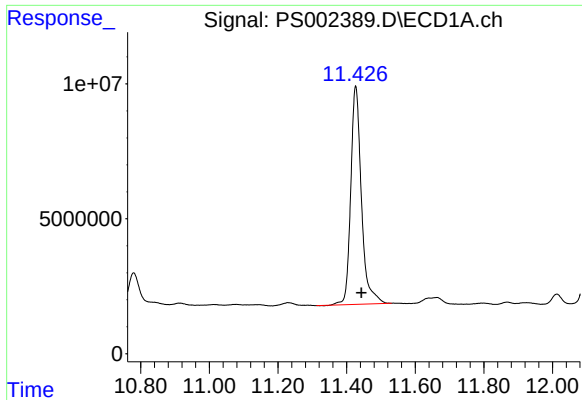

#4 2,4-DCAA


R.T.: 11.426 min
Delta R.T.: -0.017 min
Response: 174517427
Conc: 572.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

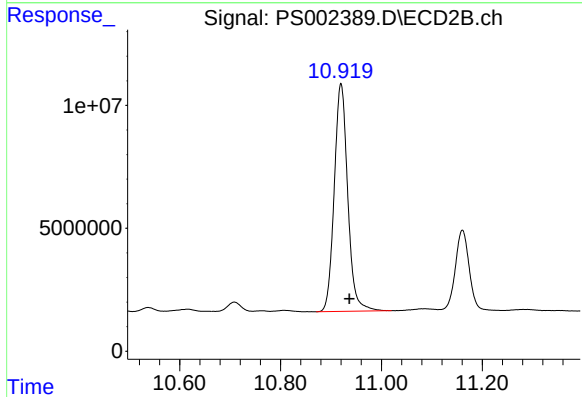


#4 2,4-DCAA

R.T.: 10.920 min
Delta R.T.: -0.016 min
Response: 171975826
Conc: 469.99 ng/ml

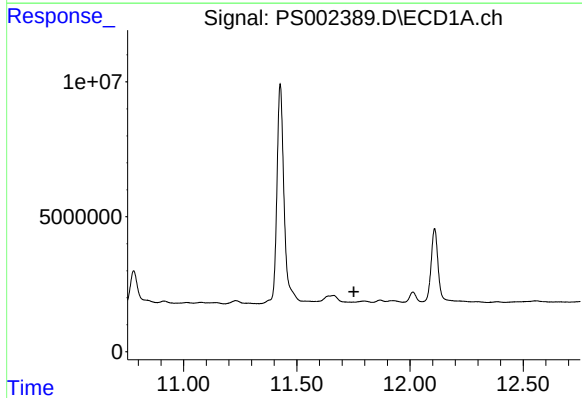


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.752 min
Response: 0
Conc: N.D.

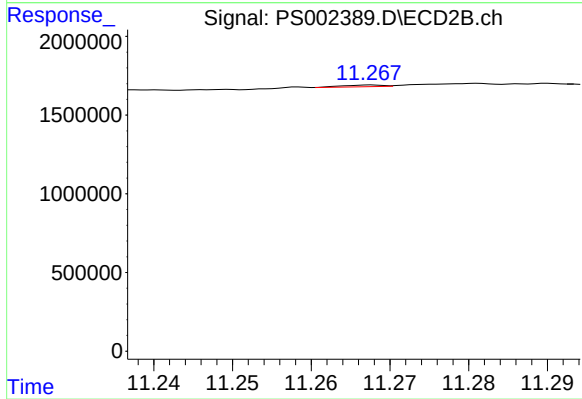

#5 DICAMBA


R.T.: 11.268 min
Delta R.T.: 0.048 min
Response: 38014
Conc: 0.03 ng/ml

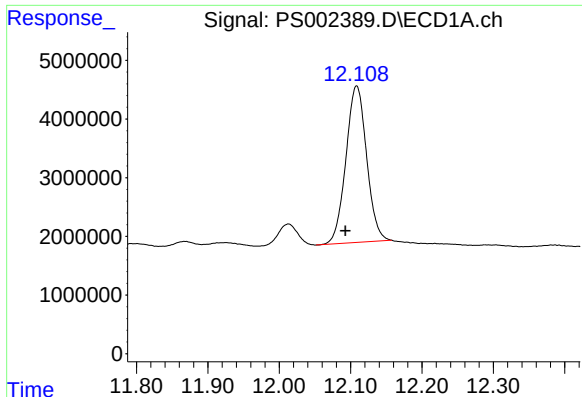

#6 MCPP


R.T.: 12.108 min
Delta R.T.: 0.016 min
Response: 53787140
Conc: 57.31 ug/ml

Instrument :
ECD_S
ClientSampleId :

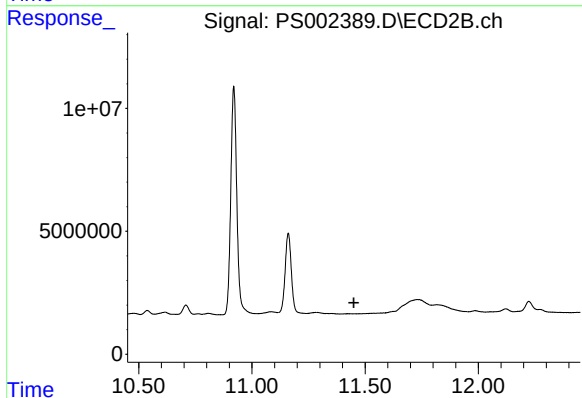


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.450 min
Response: 0
Conc: N.D.

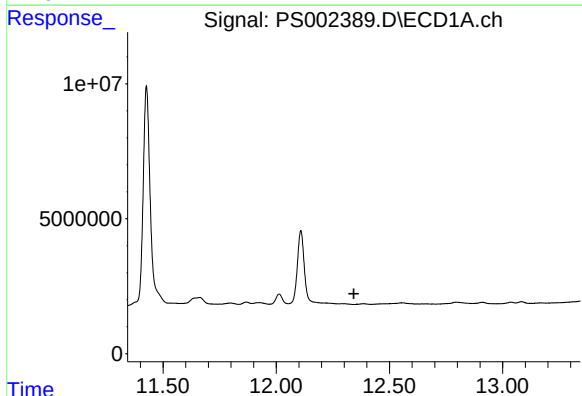


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

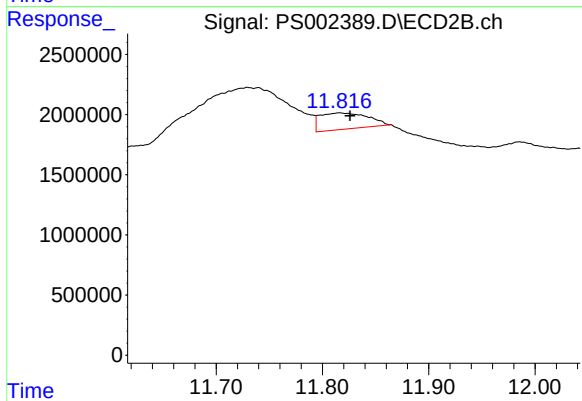

#7 MCPA


R.T.: 11.816 min
Delta R.T.: -0.010 min
Response: 4289478
Conc: 3.05 ug/ml

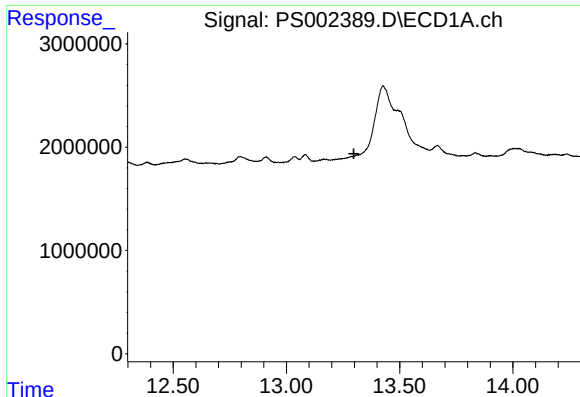

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

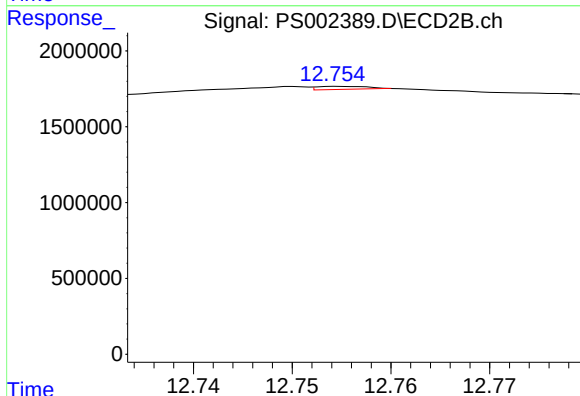


#9 2,4-D

R.T.: 12.755 min
Delta R.T.: -0.059 min
Response: 83700
Conc: 0.21 ng/ml

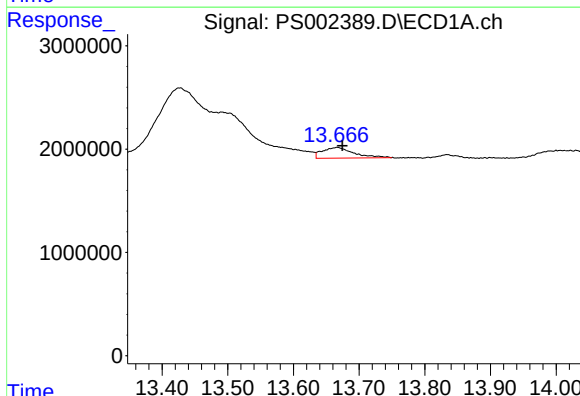


#10 Pentachlorophenol

R.T.: 13.667 min
Delta R.T.: -0.008 min
Response: 3403615
Conc: 0.70 ng/ml

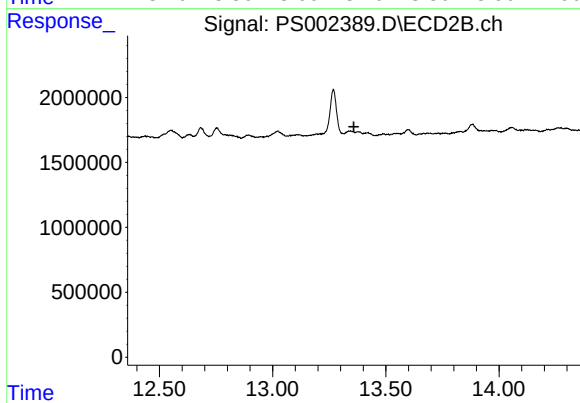

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.359 min
Response: 0
Conc: N.D.

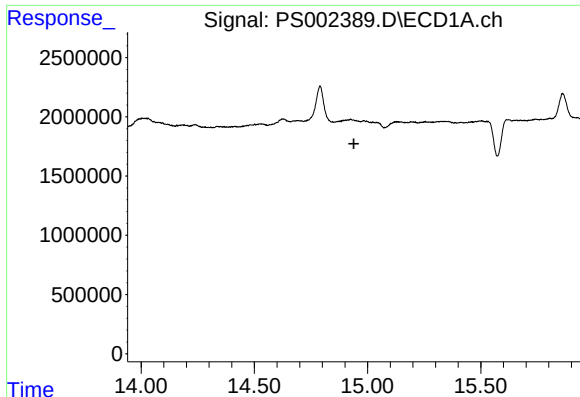

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

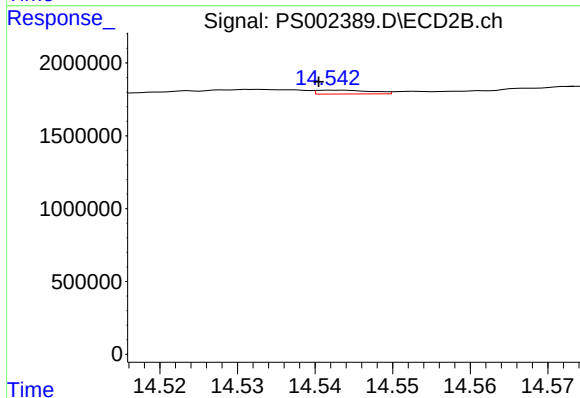


#12 2,4,5-T

R.T.: 14.543 min
Delta R.T.: 0.002 min
Response: 127494
Conc: 0.08 ng/ml

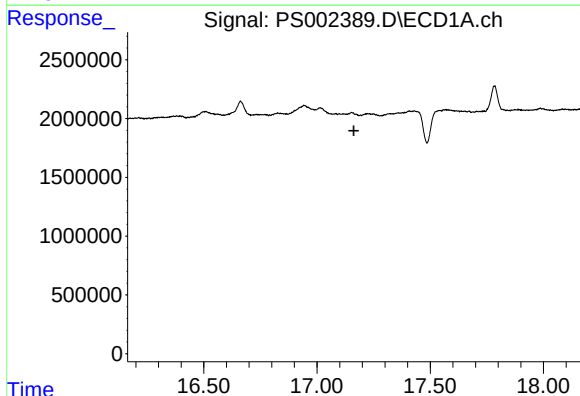


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.163 min
Response: 0
Conc: N.D.

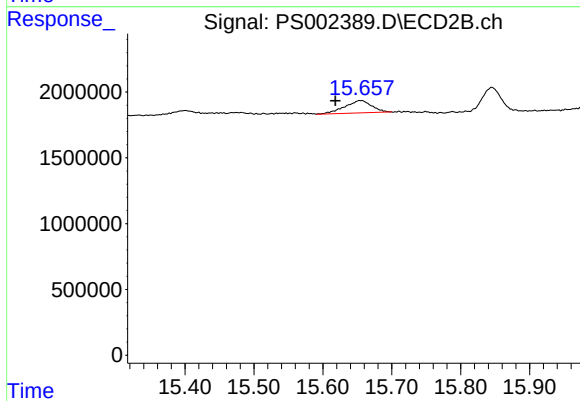

#14 DINOSEB


R.T.: 15.657 min
Delta R.T.: 0.039 min
Response: 2537905
Conc: 1.70 ng/ml

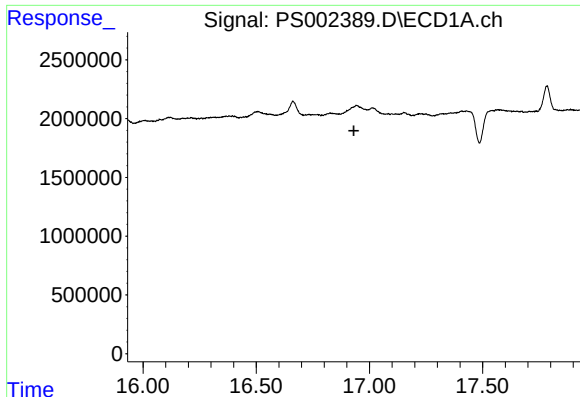

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

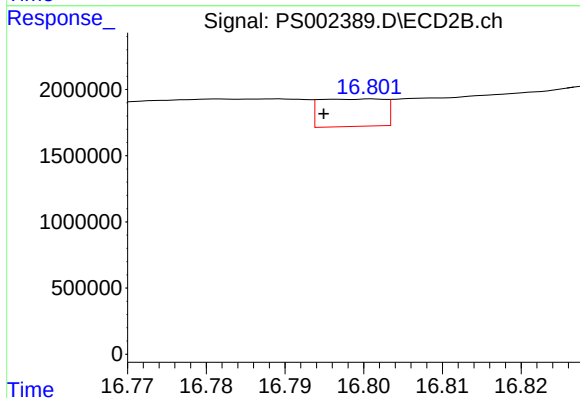


#15 Picloram

R.T.: 16.797 min
Delta R.T.: 0.002 min
Response: 1185749
Conc: 0.45 ng/ml

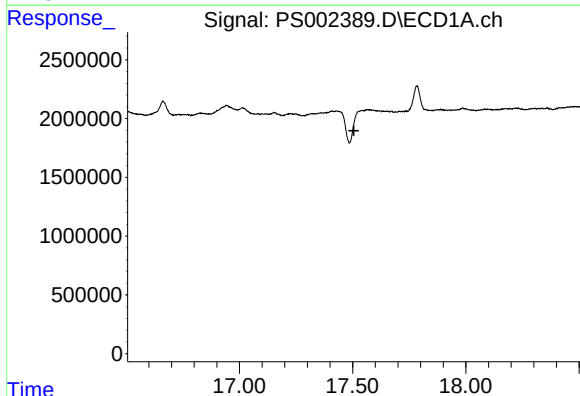

#16 DCPA

R.T.: 17.567 min
Delta R.T.: 0.062 min
Response: -1323926
Conc: N.D.

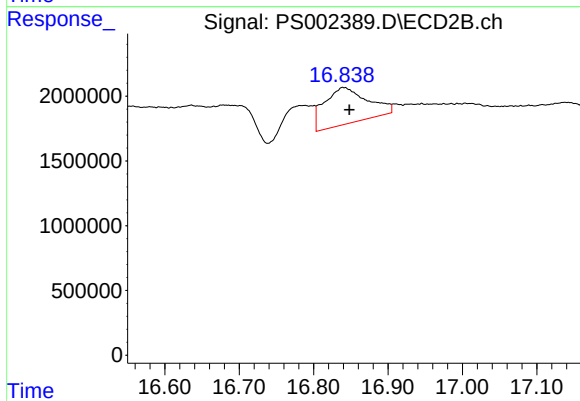

#16 DCPA

R.T.: 16.839 min
Delta R.T.: -0.009 min
Response: 11366199
Conc: 4.74 ng/ml