

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 19:56
 Operator : EI\SJ
 Sample : J5768-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 22:01:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.462	10.956	113.0E6	108.6E6	371.130	296.703
Target Compounds							
1) T	Dalapon	2.942	2.394	3271642	4116463	7.420	9.564 #
2) T	3,5-DICHL...	0.000	9.052	0	13217511	N.D.	29.155 #
3) T	4-Nitroph...	11.056	10.111	1743200	595737	10.744	3.400 #
5) T	DICAMBA	0.000	11.196	0	35631694	N.D.	26.339 #
7) T	MCPA	0.000	11.852	0	486657	N.D.	0.346 #
9) T	2,4-D	0.000	12.790	0	646506	N.D.	1.619 #
11) T	2,4,5-TP ...	0.000	13.924	0	14553305	N.D.	7.215 #
12) T	2,4,5-T	0.000	14.574	0	412840	N.D.	0.264 #
15) T	Picloram	0.000	16.818	0	2574043	N.D.	0.968 #
16) T	DCPA	0.000	16.818	0	2574043	N.D.	1.073 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 19:56
Operator : EI\SJ
Sample : J5768-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 22:01:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

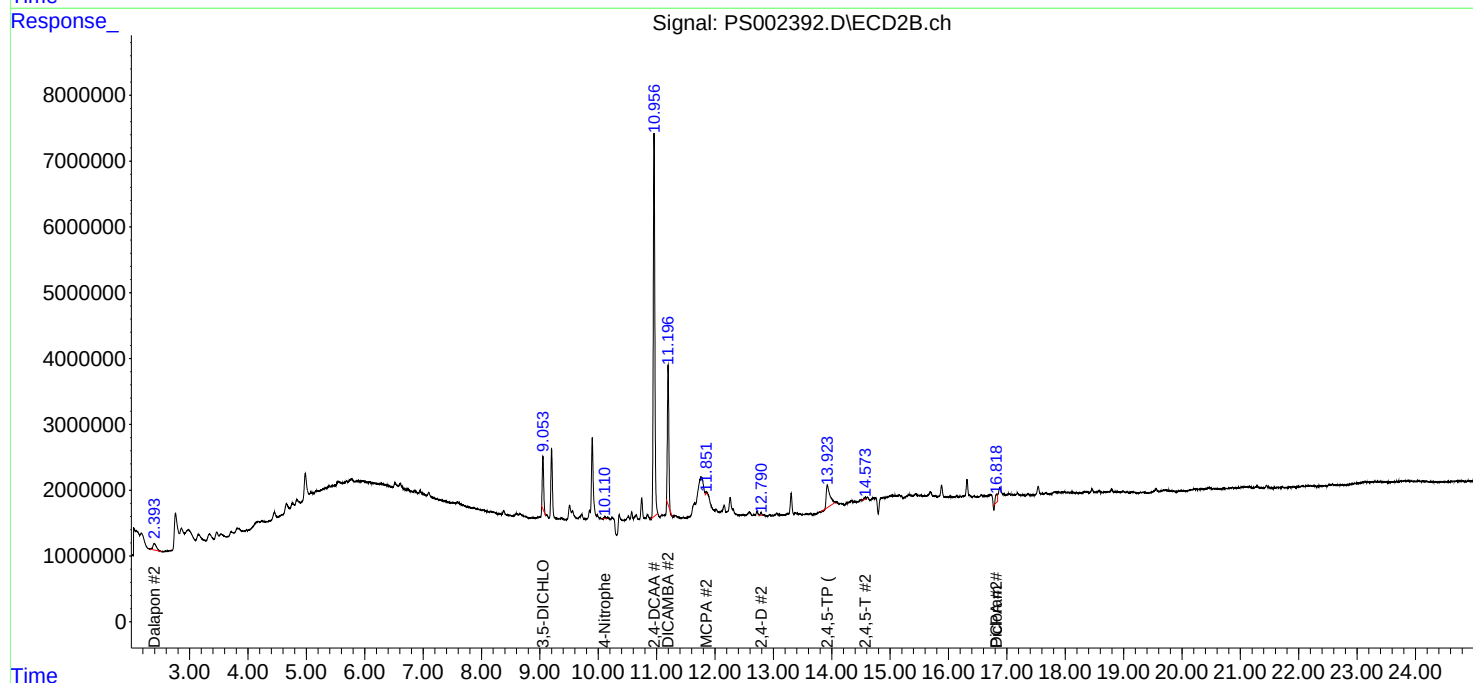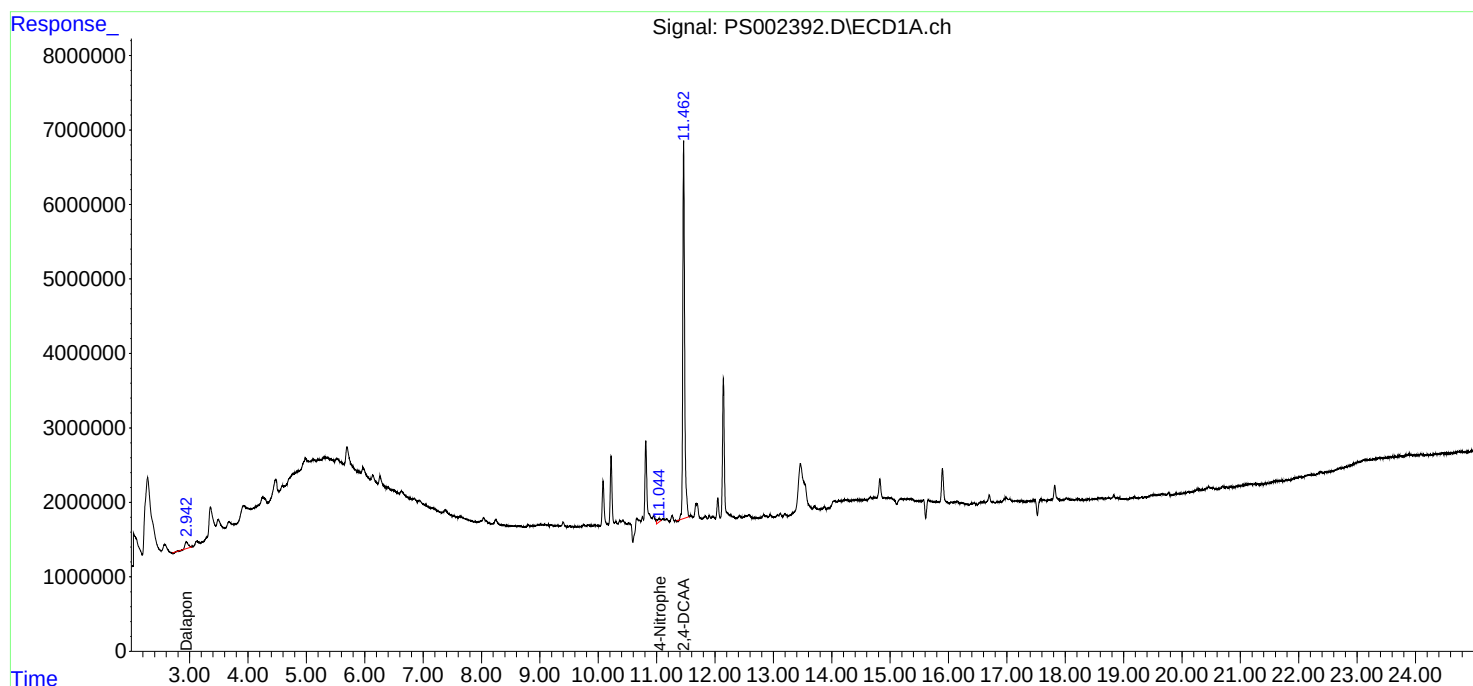


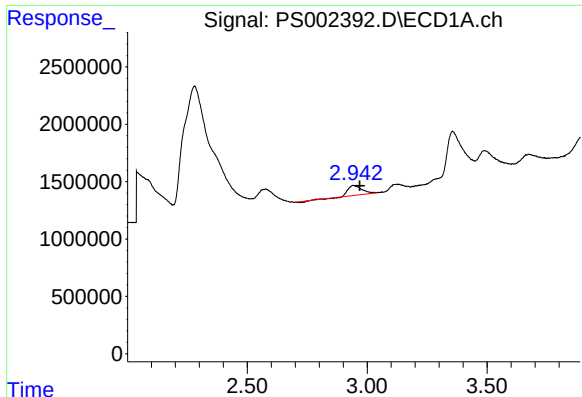

#1 Dalapon


R.T.: 2.942 min
Delta R.T.: -0.027 min
Response: 3271642
Conc: 7.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

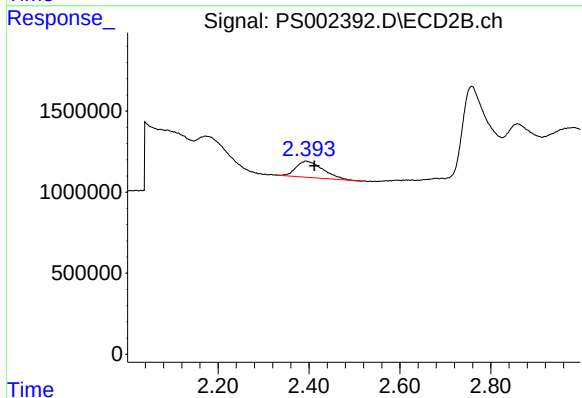


#1 Dalapon

R.T.: 2.394 min
Delta R.T.: -0.018 min
Response: 4116463
Conc: 9.56 ng/ml

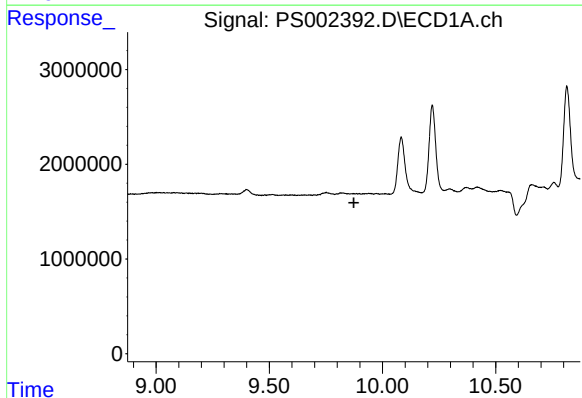


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.874 min
Response: 0
Conc: N.D.

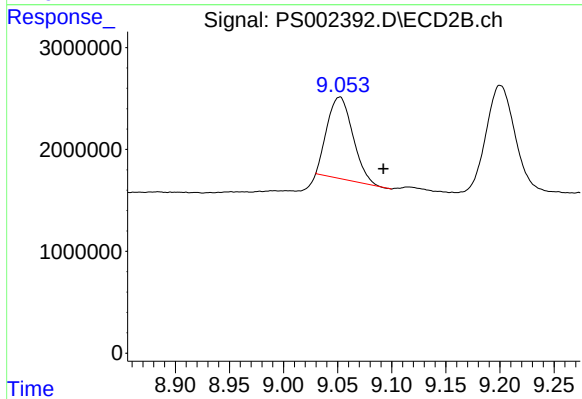

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.052 min
Delta R.T.: -0.040 min
Response: 13217511
Conc: 29.16 ng/ml

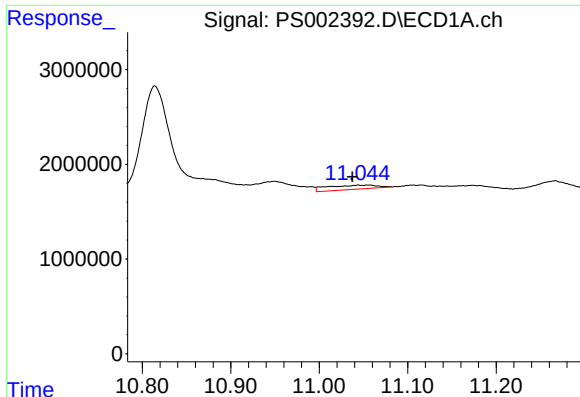

#3 4-Nitrophenol


R.T.: 11.056 min
Delta R.T.: 0.018 min
Response: 1743200
Conc: 10.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

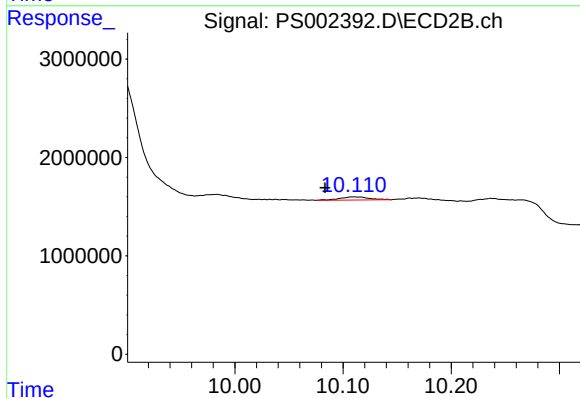


#3 4-Nitrophenol

R.T.: 10.111 min
Delta R.T.: 0.027 min
Response: 595737
Conc: 3.40 ng/ml

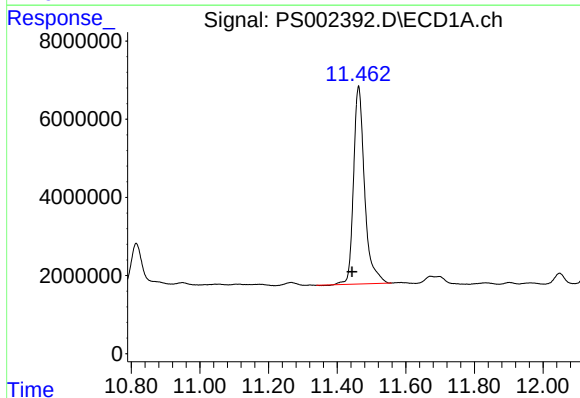


#4 2,4-DCAA

R.T.: 11.462 min
Delta R.T.: 0.019 min
Response: 113046159
Conc: 371.13 ng/ml

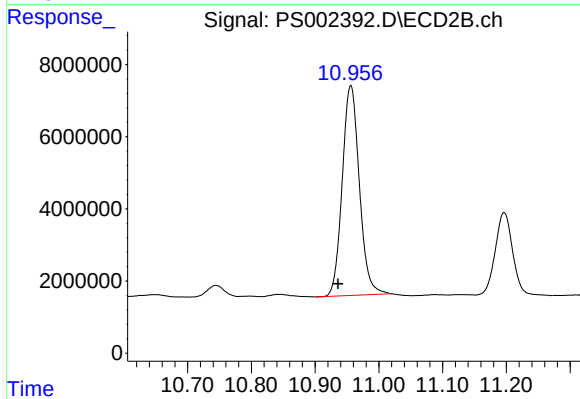

#4 2,4-DCAA


R.T.: 10.956 min
Delta R.T.: 0.020 min
Response: 108567295
Conc: 296.70 ng/ml

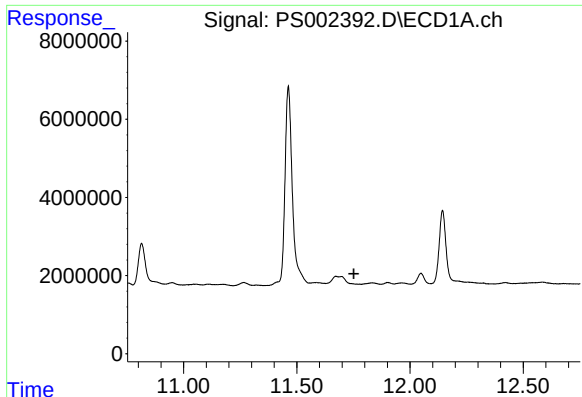

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

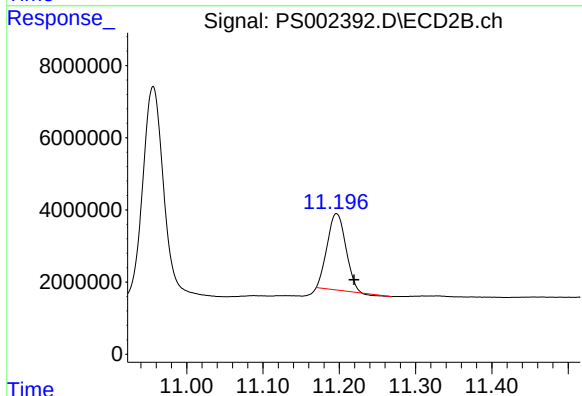


#5 DICAMBA

R.T.: 11.196 min
Delta R.T.: -0.023 min
Response: 35631694
Conc: 26.34 ng/ml

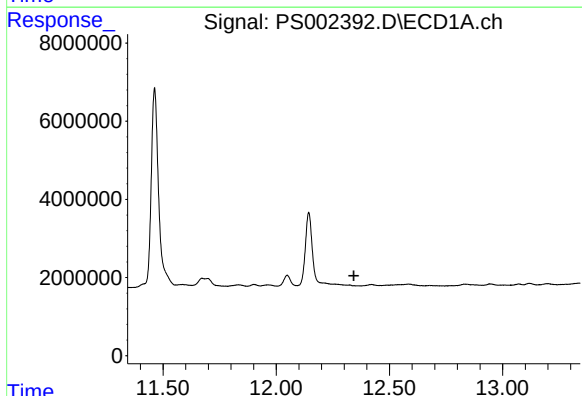


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.343 min
Response: 0
Conc: N.D.

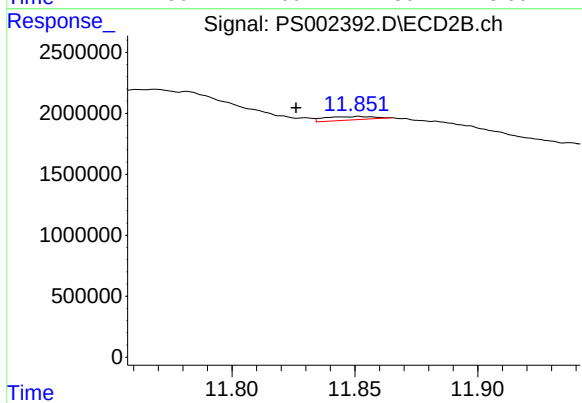

#7 MCPA


R.T.: 11.852 min
Delta R.T.: 0.026 min
Response: 486657
Conc: 0.35 ug/ml

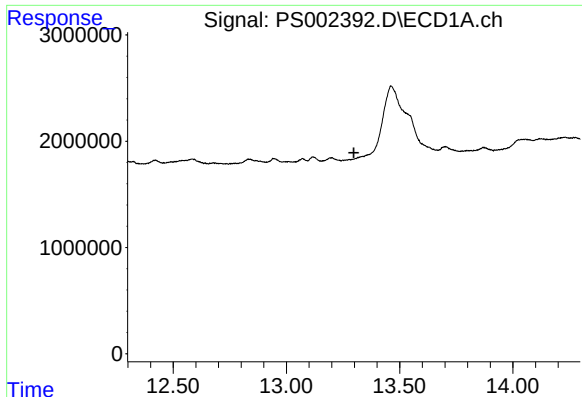

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

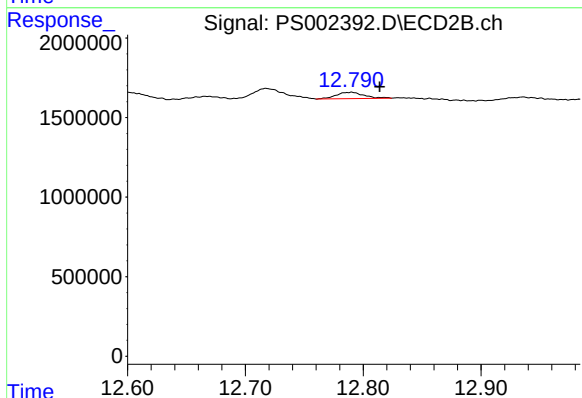


#9 2,4-D

R.T.: 12.790 min
Delta R.T.: -0.024 min
Response: 646506
Conc: 1.62 ng/ml

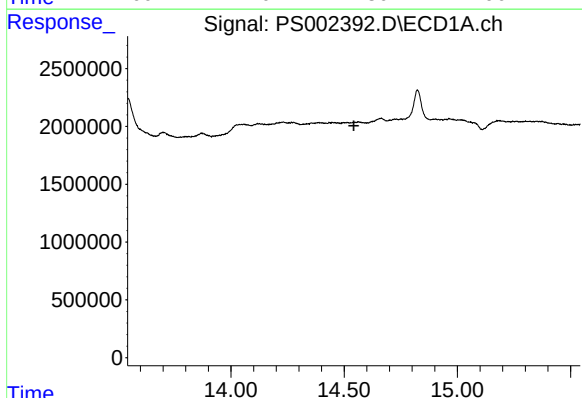


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.543 min
Response: 0
Conc: N.D.

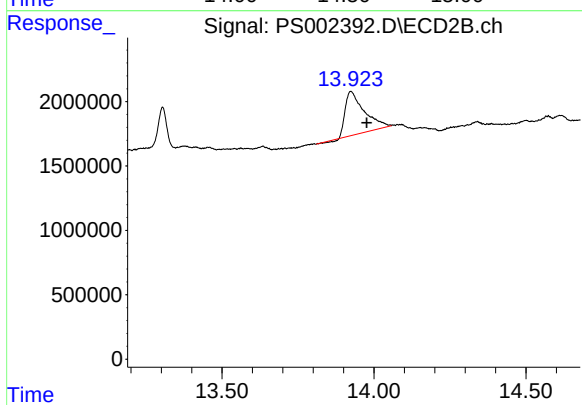

#11 2,4,5-TP (SILVEX)


R.T.: 13.924 min
Delta R.T.: -0.053 min
Response: 14553305
Conc: 7.21 ng/ml

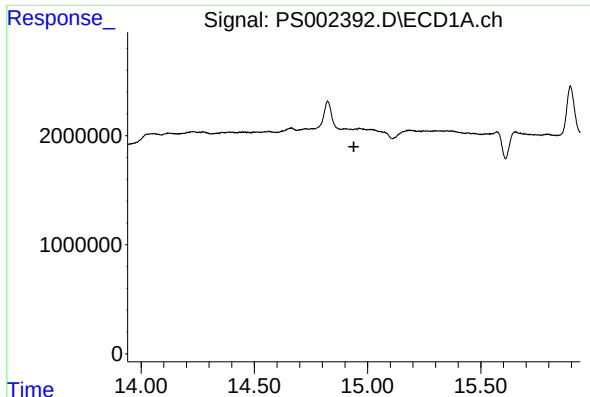

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

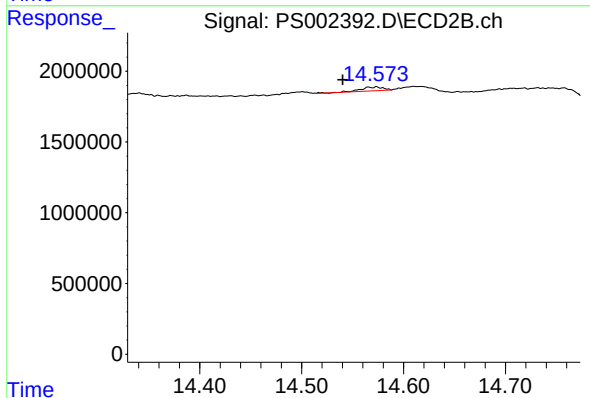


#12 2,4,5-T

R.T.: 14.574 min
Delta R.T.: 0.033 min
Response: 412840
Conc: 0.26 ng/ml

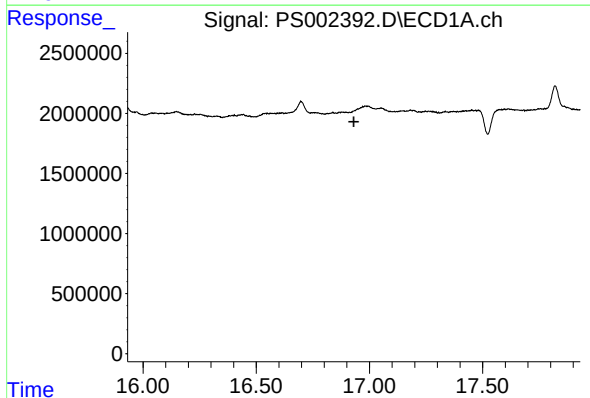


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.931 min
Response: 0
Conc: N.D.

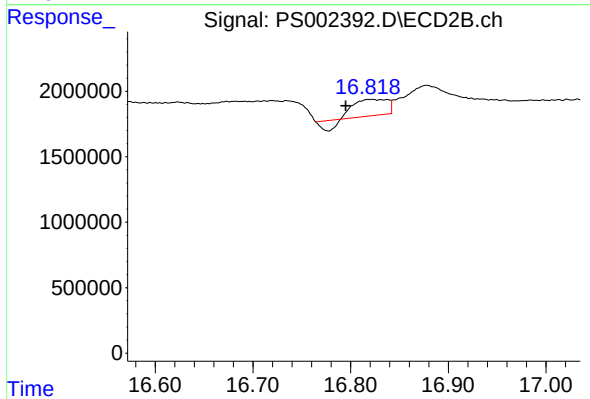

#15 Picloram


R.T.: 16.818 min
Delta R.T.: 0.023 min
Response: 2574043
Conc: 0.97 ng/ml

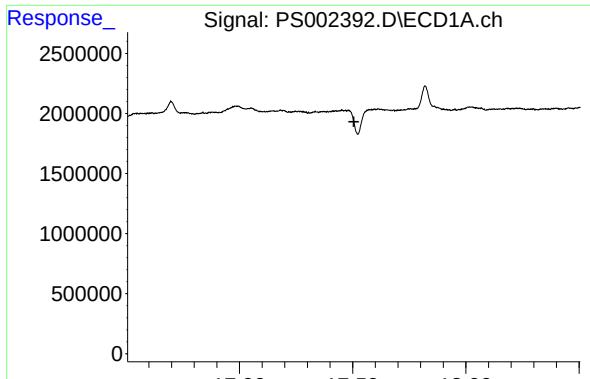

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

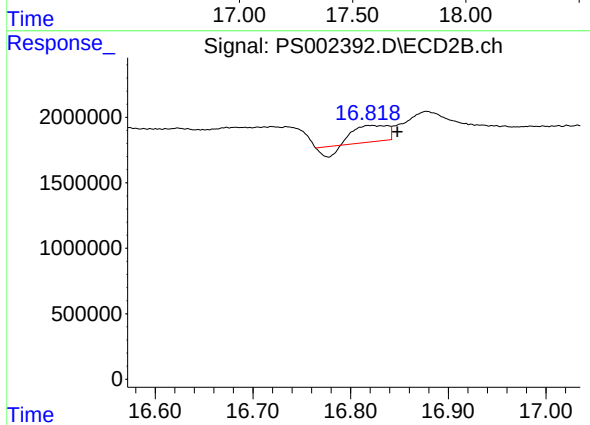

#16 DCPA

R.T.: 16.818 min
Delta R.T.: -0.030 min
Response: 2574043
Conc: 1.07 ng/ml