

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 21:29
 Operator : EI\SJ
 Sample : J5858-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 22:02:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.406	10.899	176.1E6	168.9E6	578.058	461.451
Target Compounds							
2) T	3,5-DICHL...	0.000	9.144	0	29258765	N.D.	64.539 #
3) T	4-Nitroph...	0.000	10.057	0	8905145	N.D.	50.825 #
5) T	DICAMBA	0.000	11.263	0	1164241	N.D.	0.861 #
6) T	MCP	12.087	0.000	59180163	0	63.056	N.D. #
7) T	MCPA	0.000	11.798	0	7095238	N.D.	5.042 #
10) T	Pentachlo...	13.646	0.000	3894002	0	0.805	N.D. #
11) T	2,4,5-TP ...	0.000	13.947	0	498516	N.D.	0.247 #
12) T	2,4,5-T	0.000	14.557	0	1764848	N.D.	1.129 #
14) T	DINOSEB	0.000	15.634	0	2999190	N.D.	2.004 #
15) T	Picloram	0.000	16.760	0	1732602	N.D.	0.651 #
16) T	DCPA	0.000	16.848	0	779326	N.D.	0.325 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 21:29
Operator : EI\SJ
Sample : J5858-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 22:02:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

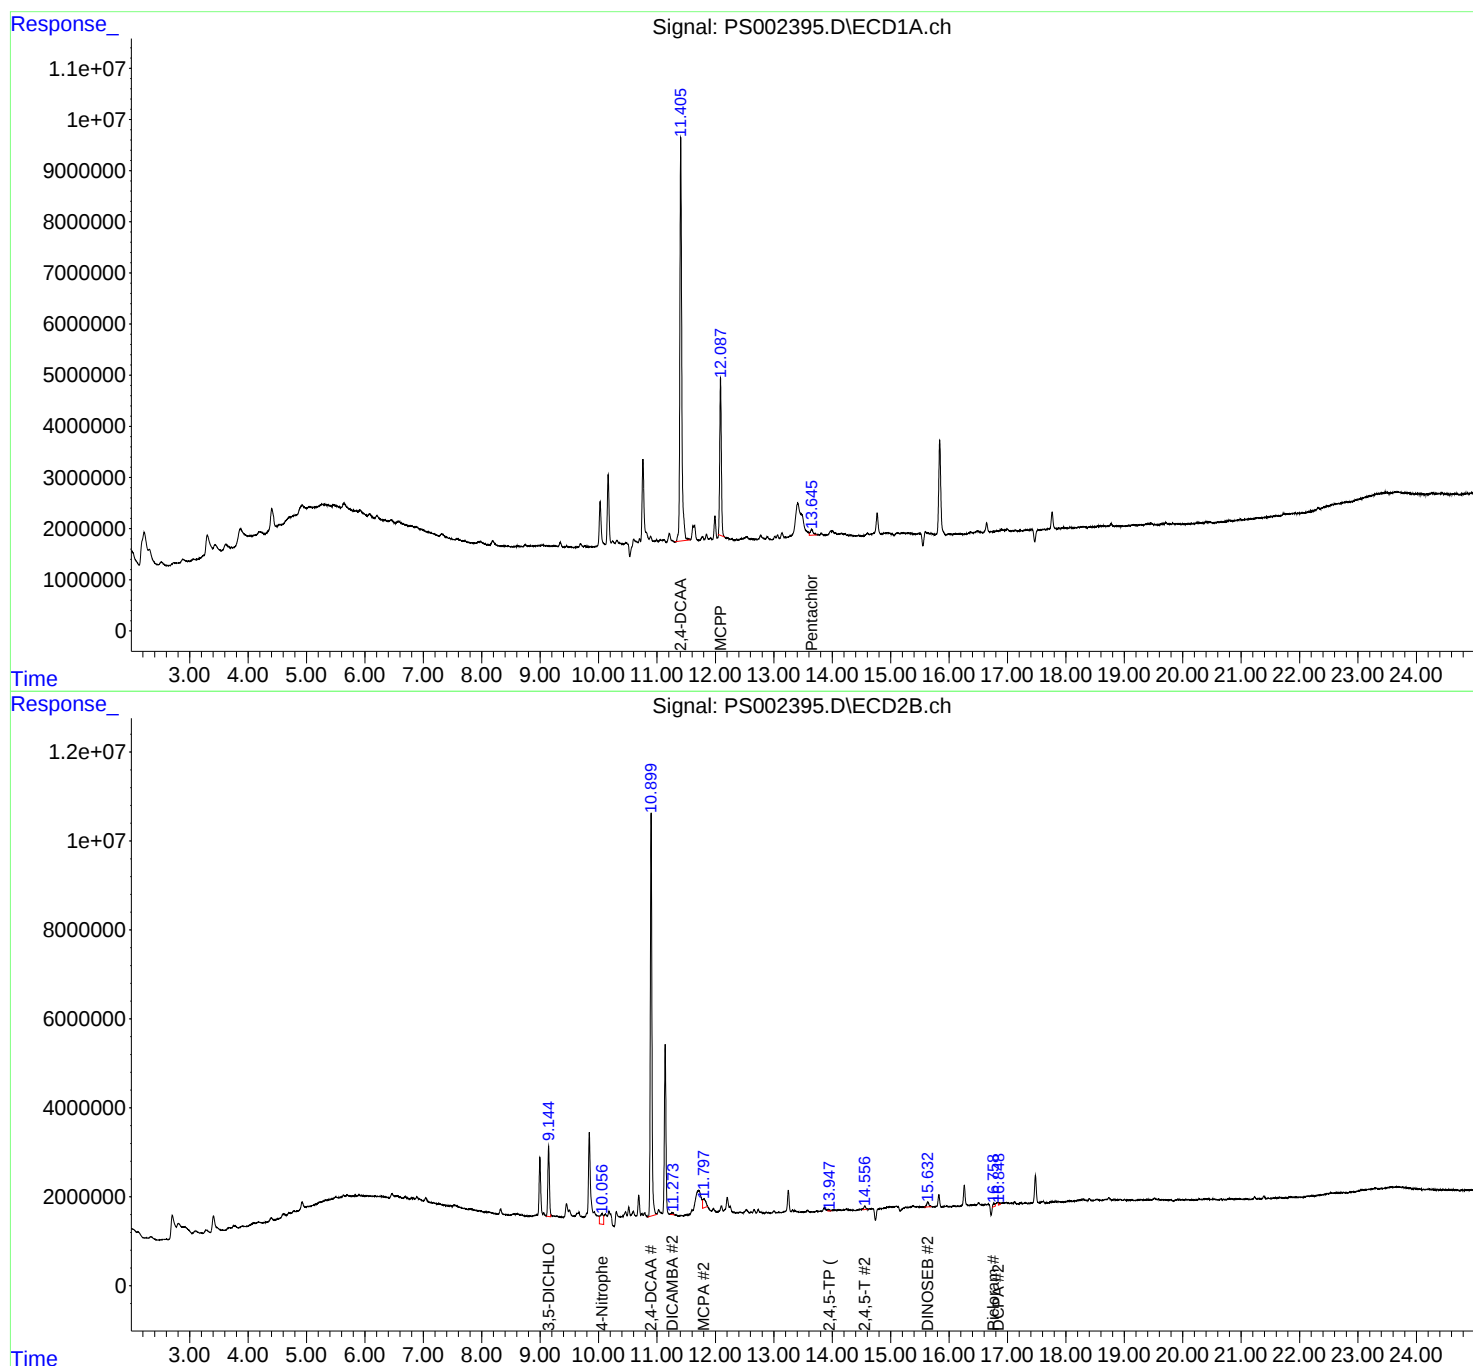


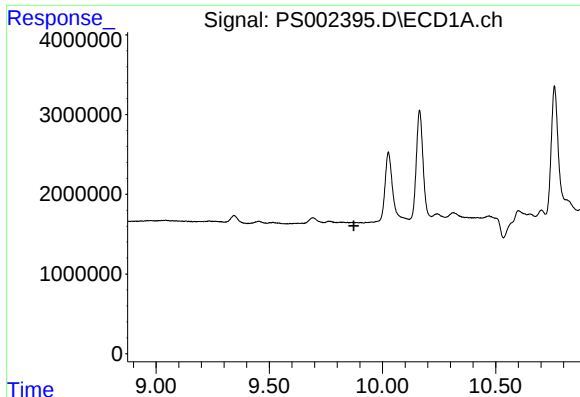

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

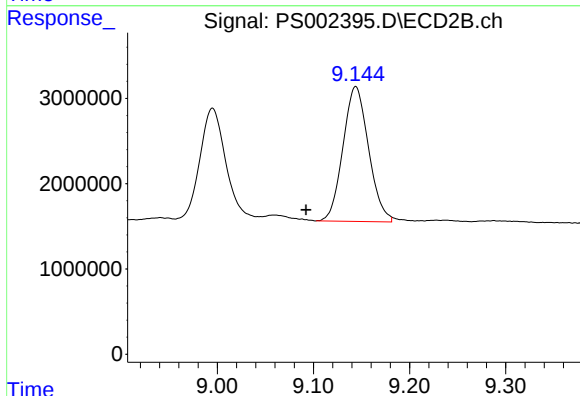


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.144 min
Delta R.T.: 0.052 min
Response: 29258765
Conc: 64.54 ng/ml

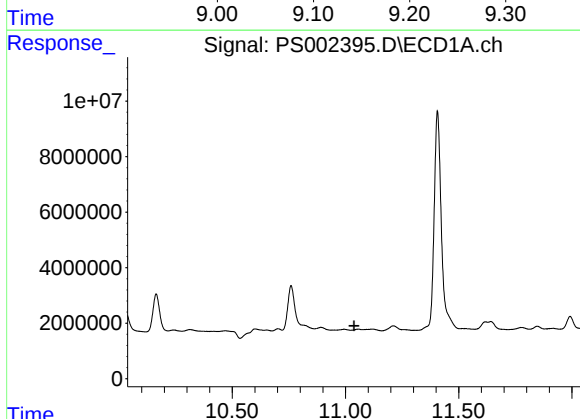


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

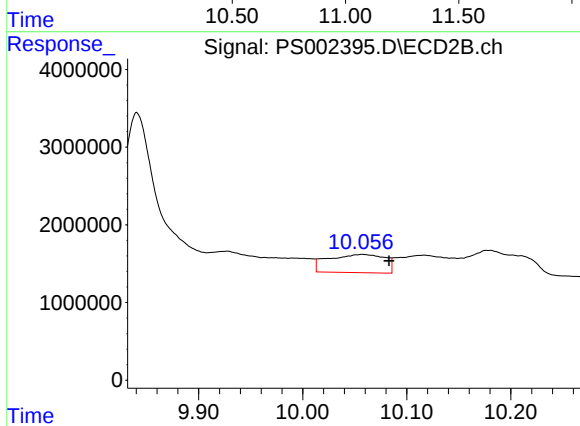

#3 4-Nitrophenol


R.T.: 10.057 min
Delta R.T.: -0.026 min
Response: 8905145
Conc: 50.82 ng/ml

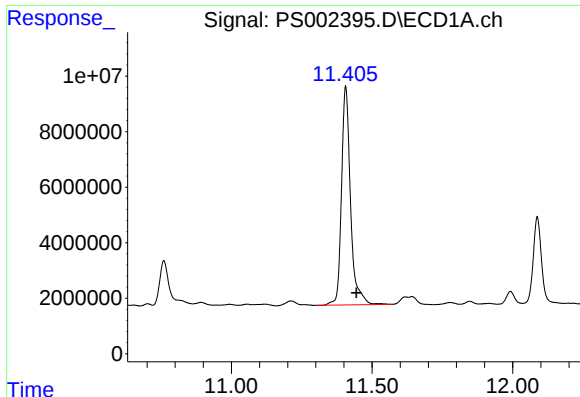

#4 2,4-DCAA


R.T.: 11.406 min
Delta R.T.: -0.038 min
Response: 176076245
Conc: 578.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

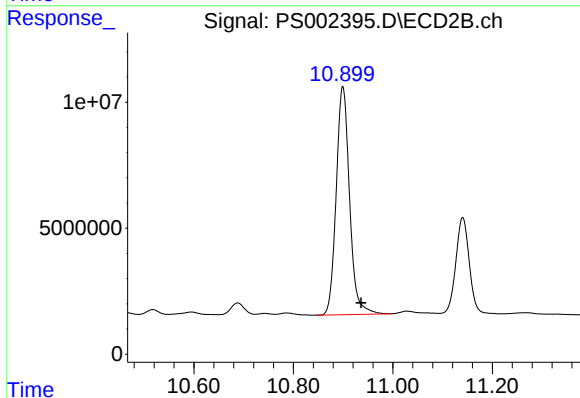


#4 2,4-DCAA

R.T.: 10.899 min
Delta R.T.: -0.037 min
Response: 168850574
Conc: 461.45 ng/ml

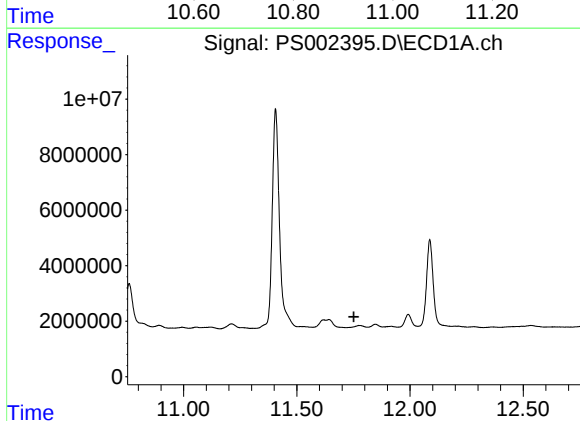


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.752 min
Response: 0
Conc: N.D.

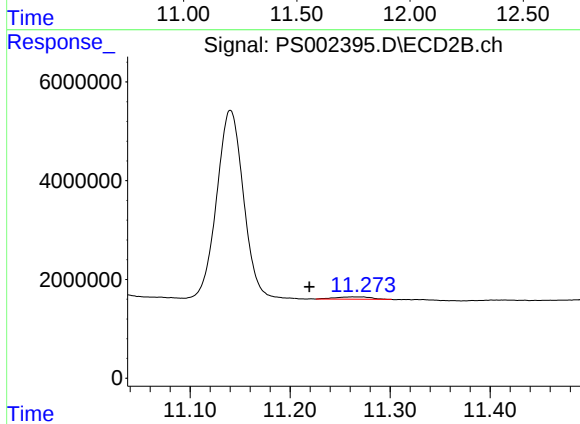

#5 DICAMBA


R.T.: 11.263 min
Delta R.T.: 0.043 min
Response: 1164241
Conc: 0.86 ng/ml

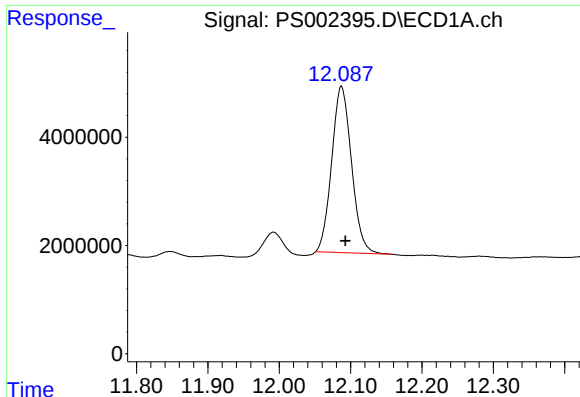

#6 MCPP


R.T.: 12.087 min
Delta R.T.: -0.006 min
Response: 59180163
Conc: 63.06 ug/ml

Instrument :
ECD_S
ClientSampleId :

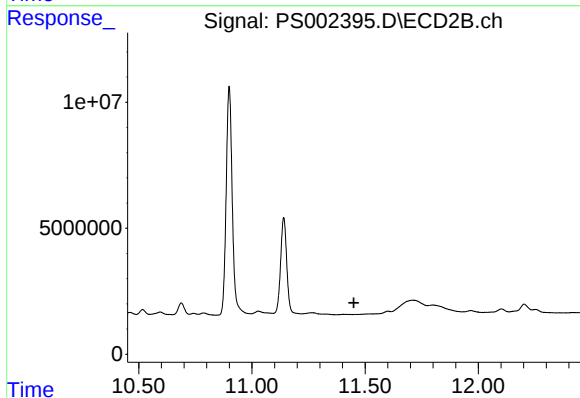


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.450 min
Response: 0
Conc: N.D.

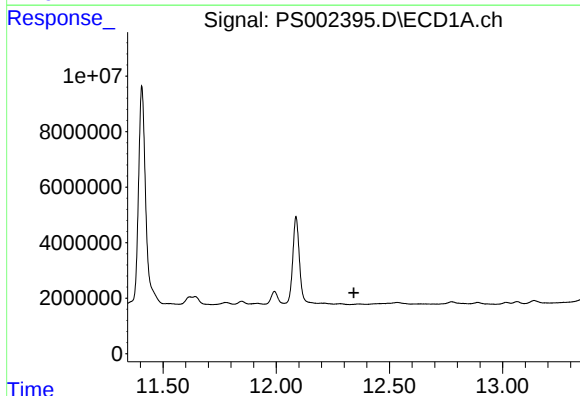


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

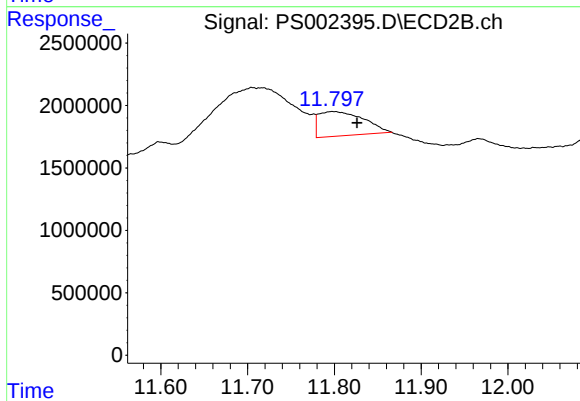

#7 MCPA


R.T.: 11.798 min
Delta R.T.: -0.028 min
Response: 7095238
Conc: 5.04 ug/ml

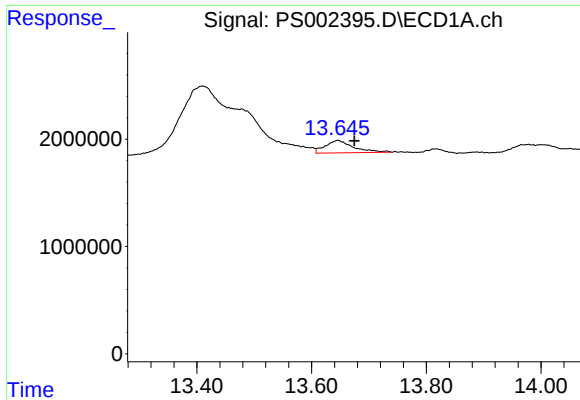

#10 Pentachlorophenol


R.T.: 13.646 min
Delta R.T.: -0.029 min
Response: 3894002
Conc: 0.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

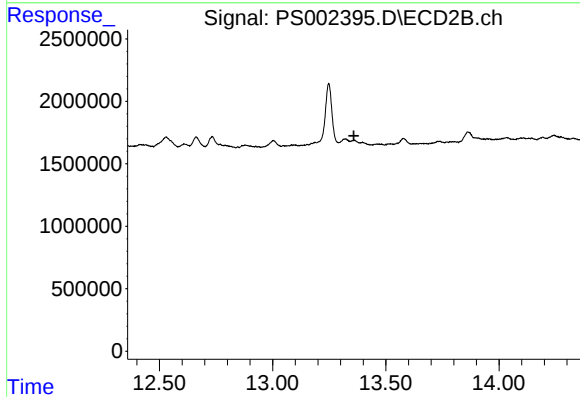


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.359 min
Response: 0
Conc: N.D.

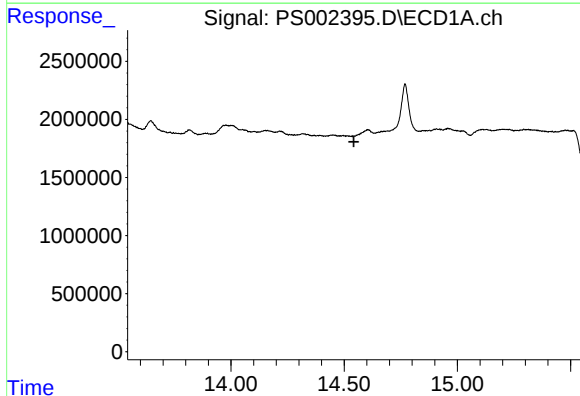


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.543 min
Response: 0
Conc: N.D.

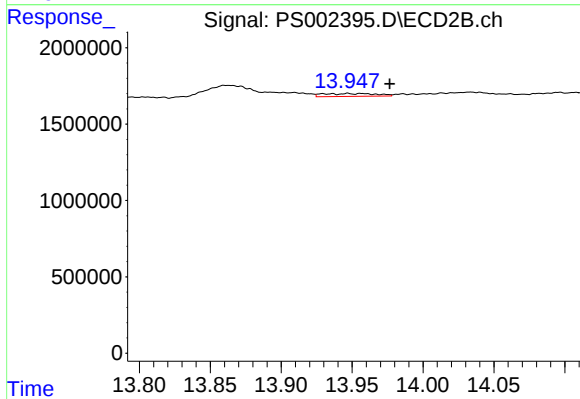

#11 2,4,5-TP (SILVEX)


R.T.: 13.947 min
Delta R.T.: -0.030 min
Response: 498516
Conc: 0.25 ng/ml

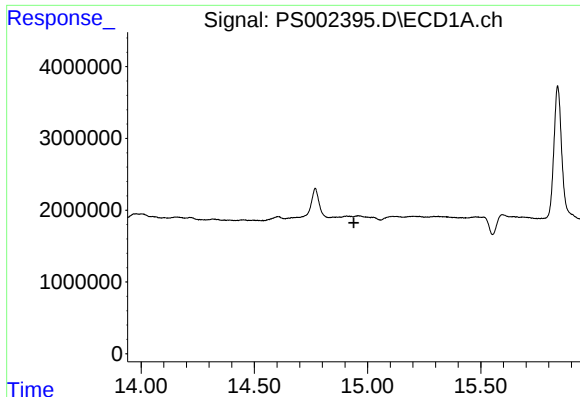

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

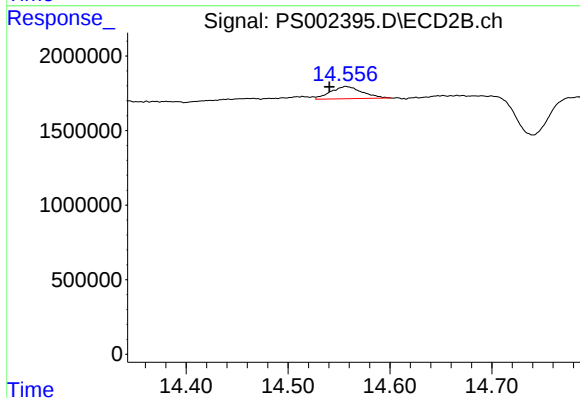


#12 2,4,5-T

R.T.: 14.557 min
Delta R.T.: 0.016 min
Response: 1764848
Conc: 1.13 ng/ml

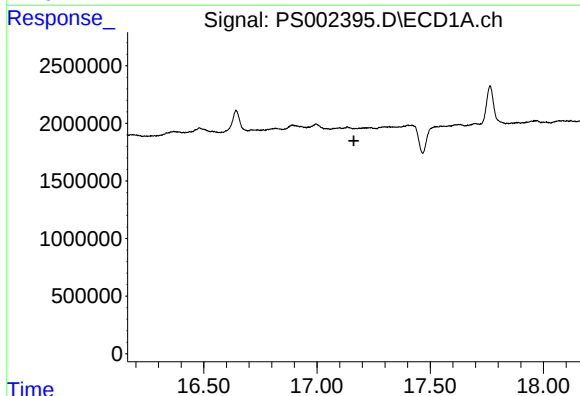


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.163 min
Response: 0
Conc: N.D.

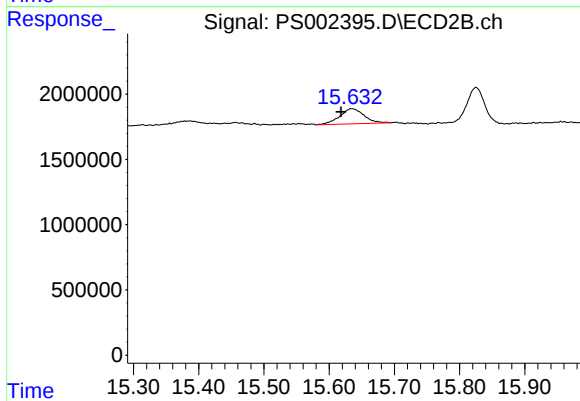

#14 DINOSEB


R.T.: 15.634 min
Delta R.T.: 0.016 min
Response: 2999190
Conc: 2.00 ng/ml

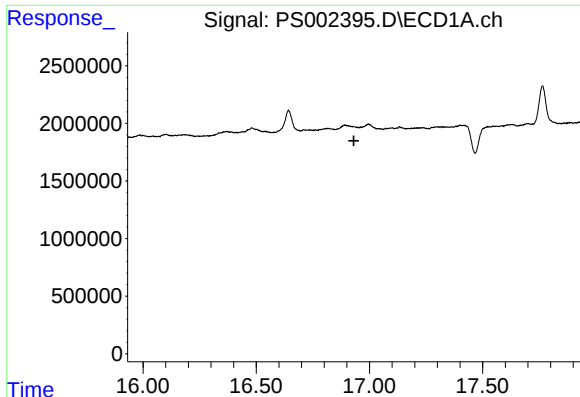

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

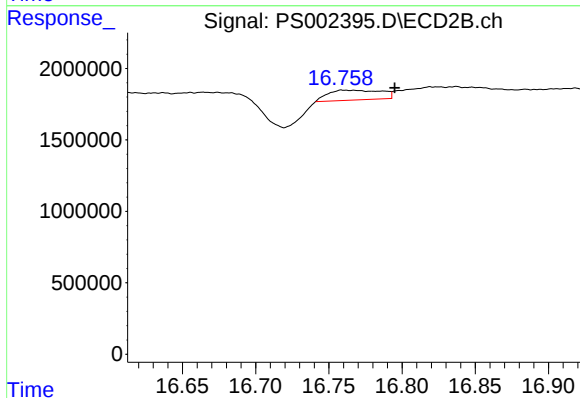


#15 Picloram

R.T.: 16.760 min
Delta R.T.: -0.035 min
Response: 1732602
Conc: 0.65 ng/ml

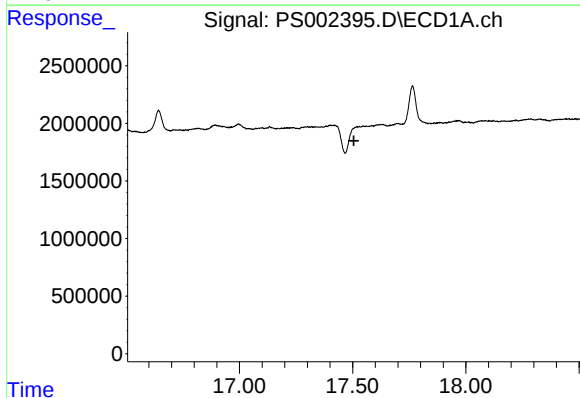

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

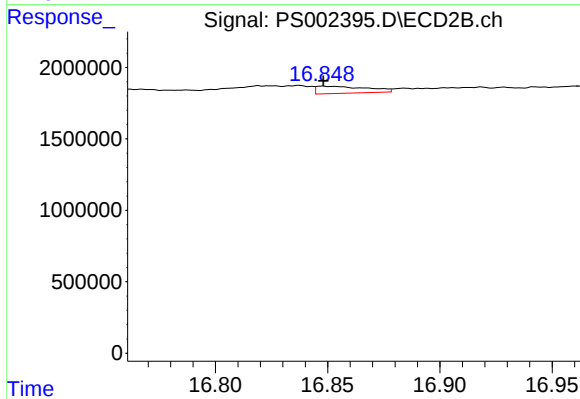

#16 DCPA

R.T.: 16.848 min
Delta R.T.: 0.000 min
Response: 779326
Conc: 0.32 ng/ml