

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 22:31
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 03:16:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.439	10.932	144.0E6	148.2E6	472.829	404.899
Target Compounds							
7) T	MCPA	0.000	11.826	0	2938217	N.D.	2.088 #
10) T	Pentachlo...	0.000	13.357	0	542762	N.D.	0.107 #
15) T	Picloram	0.000	16.791	0	102805	N.D.	0.039 #
16) T	DCPA	0.000	16.791	0	102805	N.D.	0.043 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 22:31
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 03:16:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

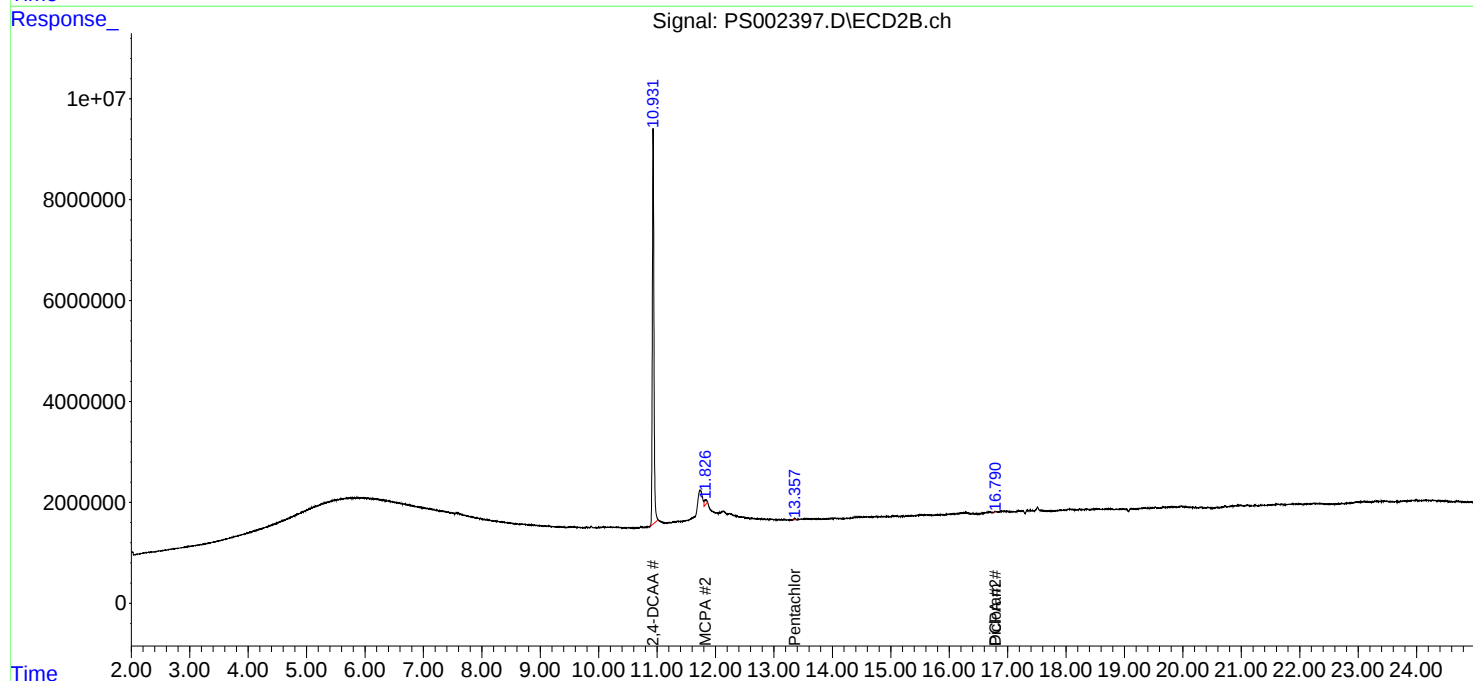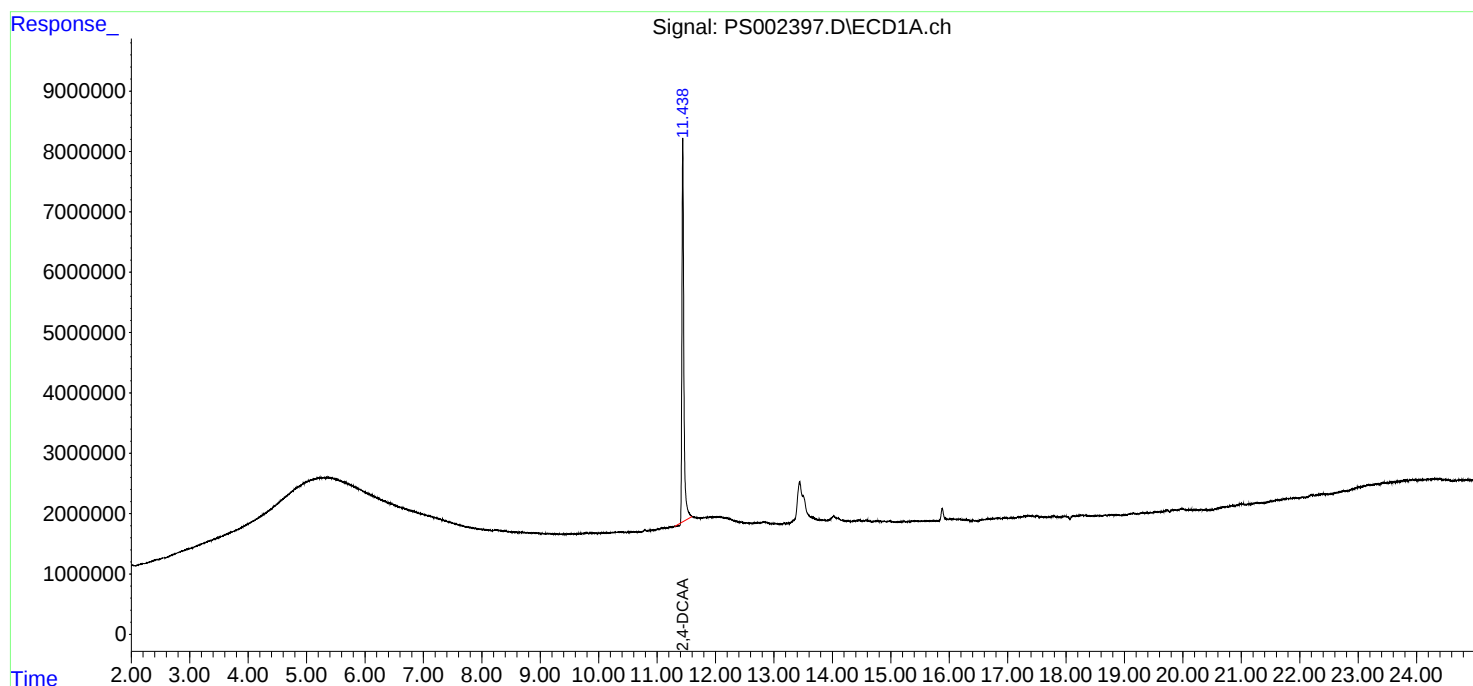


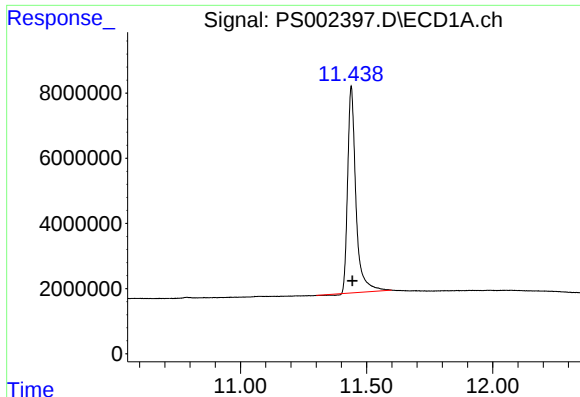

#4 2,4-DCAA


R.T.: 11.439 min
Delta R.T.: -0.005 min
Response: 144023662
Conc: 472.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

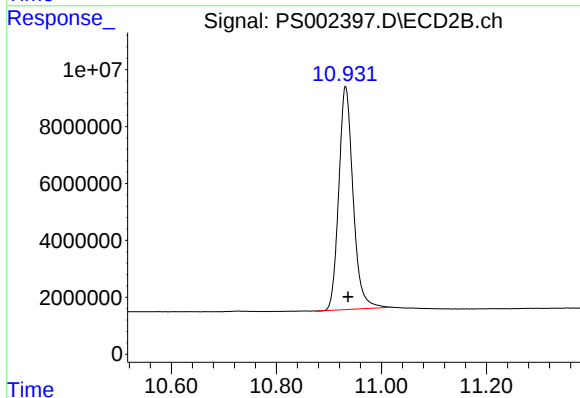


#4 2,4-DCAA

R.T.: 10.932 min
Delta R.T.: -0.005 min
Response: 148157428
Conc: 404.90 ng/ml

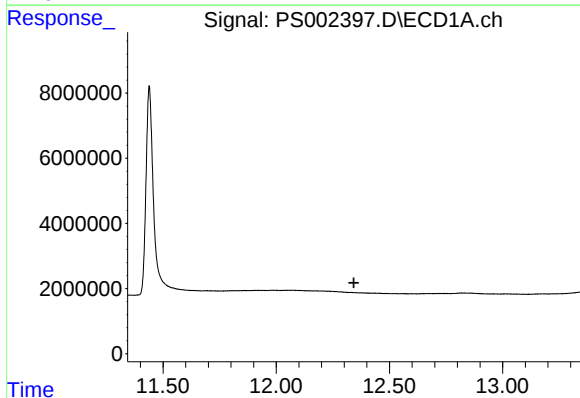


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

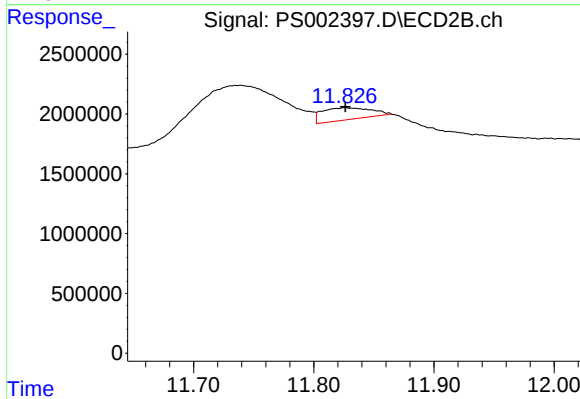

#7 MCPA


R.T.: 11.826 min
Delta R.T.: 0.000 min
Response: 2938217
Conc: 2.09 ug/ml

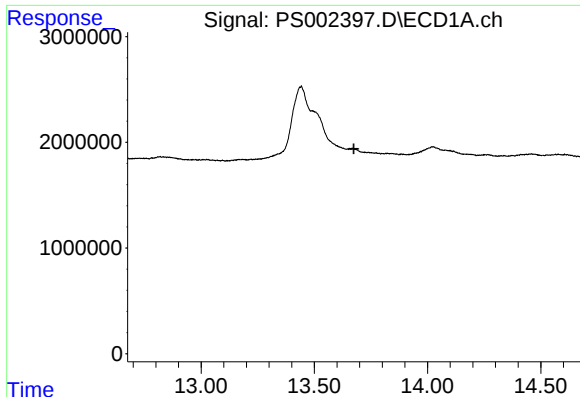

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

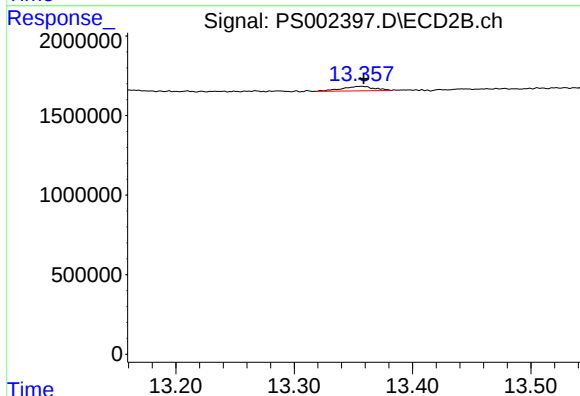


#10 Pentachlorophenol

R.T.: 13.357 min
Delta R.T.: -0.001 min
Response: 542762
Conc: 0.11 ng/ml

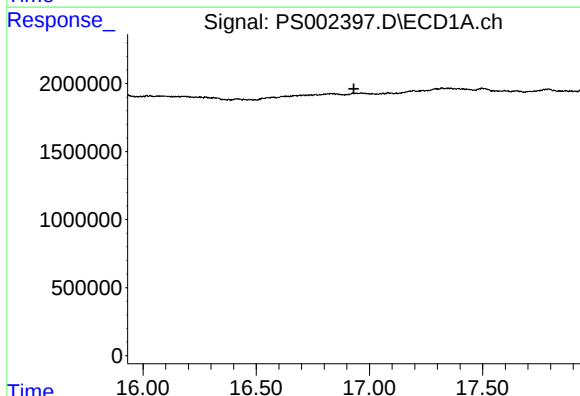


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.931 min
Response: 0
Conc: N.D.

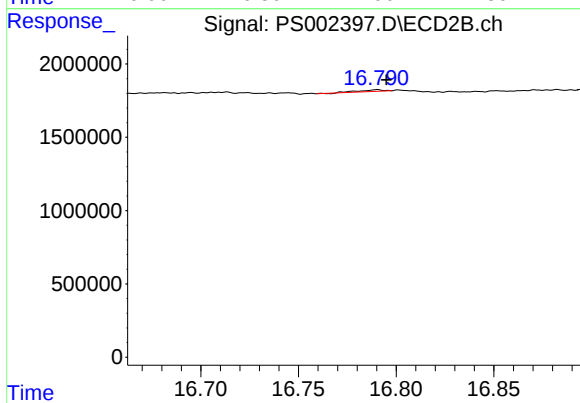

#15 Picloram


R.T.: 16.791 min
Delta R.T.: -0.004 min
Response: 102805
Conc: 0.04 ng/ml

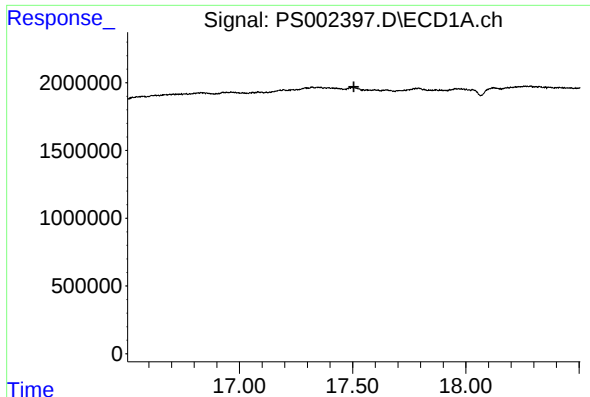

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

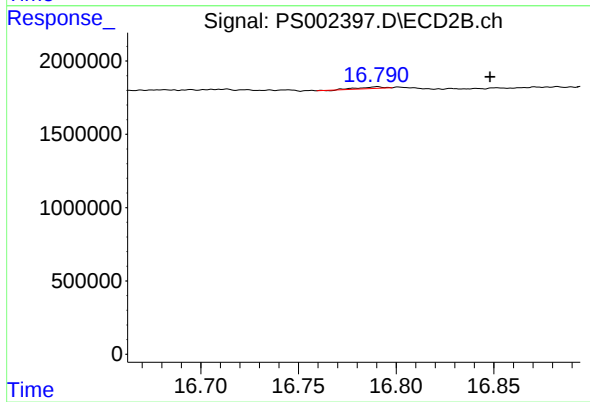

#16 DCPA

R.T.: 16.791 min
Delta R.T.: -0.057 min
Response: 102805
Conc: 0.04 ng/ml