

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 23:34
 Operator : EI\SJ
 Sample : J5858-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 03:17:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.405	10.898	171.2E6	165.0E6	561.982	451.033
Target Compounds							
2) T	3,5-DICHL...	0.000	9.142	0	26310129	N.D.	58.035 #
3) T	4-Nitroph...	0.000	10.051	0	2148788	N.D.	12.264 #
5) T	DICAMBA	0.000	11.261	0	1049326	N.D.	0.776 #
6) T	MCP	12.086	0.000	52156186	0	55.572	N.D. #
7) T	MCPA	0.000	11.785	0	8013490	N.D.	5.695 #
10) T	Pentachlo...	0.000	13.397	0	1031868	N.D.	0.203 #
11) T	2,4,5-TP ...	0.000	13.934	0	763816	N.D.	0.379 #
12) T	2,4,5-T	0.000	14.550	0	2191122	N.D.	1.402 #
13) T	2,4-DB	0.000	15.131	0	146810	N.D.	0.648 #
14) T	DINOSEB	0.000	15.636	0	3259448	N.D.	2.178 #
15) T	Picloram	16.912	16.816	19887967	29230629	9.365	10.988
16) T	DCPA	0.000	16.816	0	29230629	N.D.	12.188 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 23:34
Operator : EI\SJ
Sample : J5858-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 03:17:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

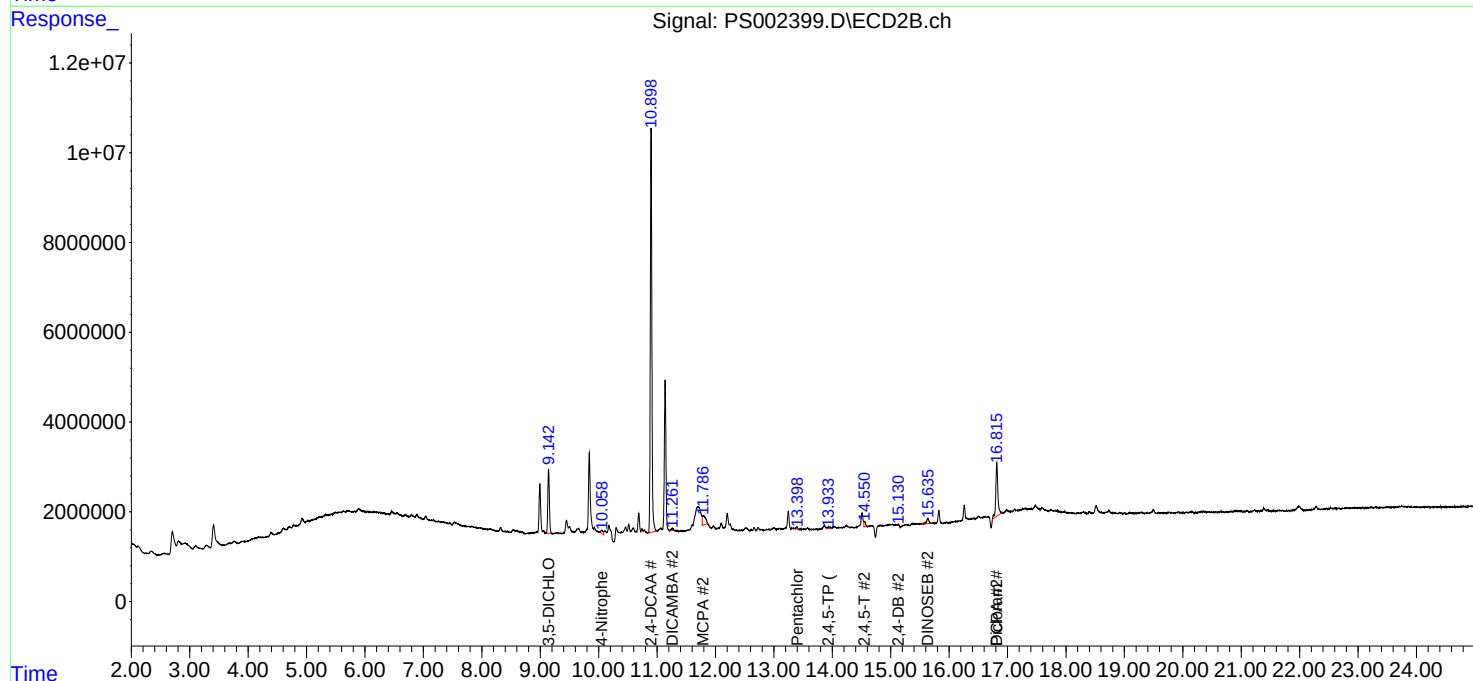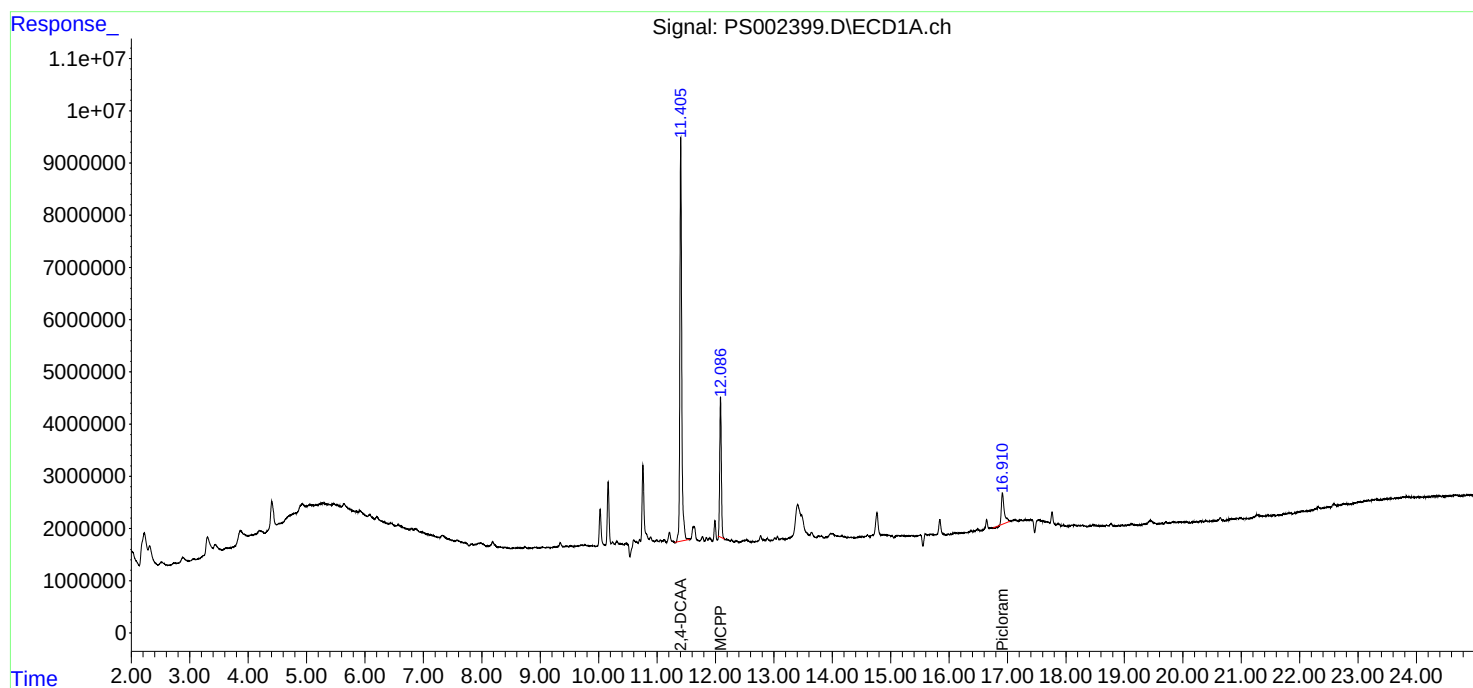


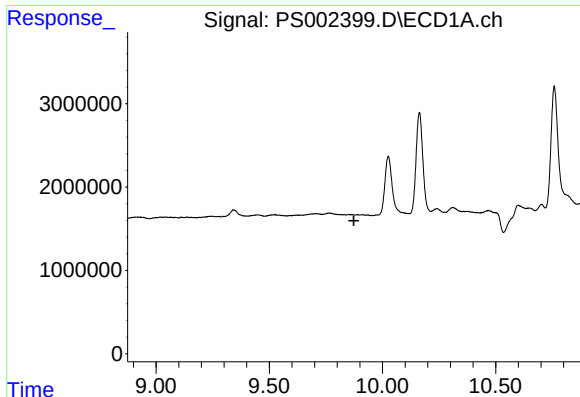

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

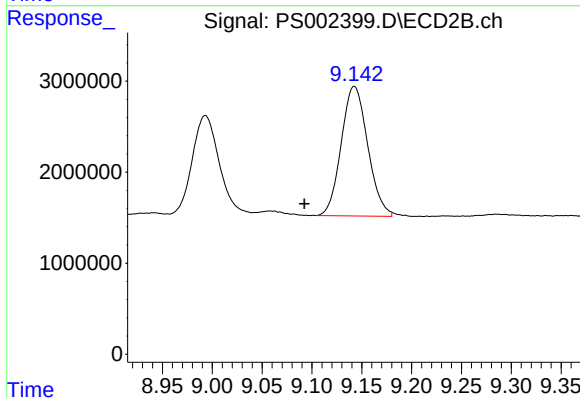


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.142 min
Delta R.T.: 0.050 min
Response: 26310129
Conc: 58.04 ng/ml

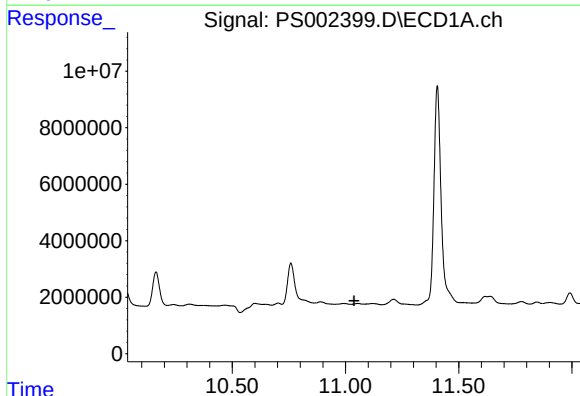


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

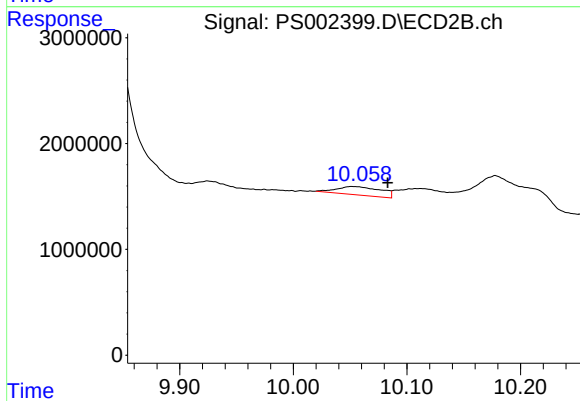

#3 4-Nitrophenol


R.T.: 10.051 min
Delta R.T.: -0.032 min
Response: 2148788
Conc: 12.26 ng/ml

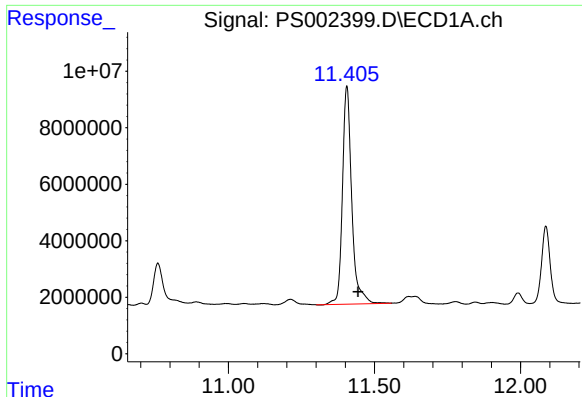

#4 2,4-DCAA


R.T.: 11.405 min
Delta R.T.: -0.038 min
Response: 171179580
Conc: 561.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

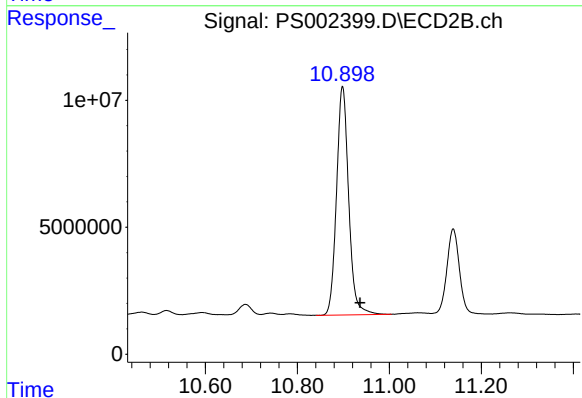


#4 2,4-DCAA

R.T.: 10.898 min
Delta R.T.: -0.038 min
Response: 165038398
Conc: 451.03 ng/ml

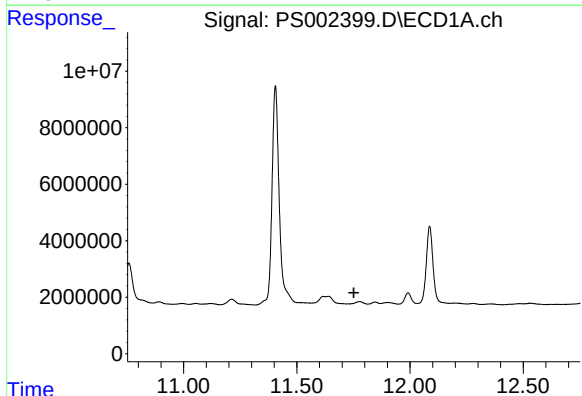


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.752 min
Response: 0
Conc: N.D.

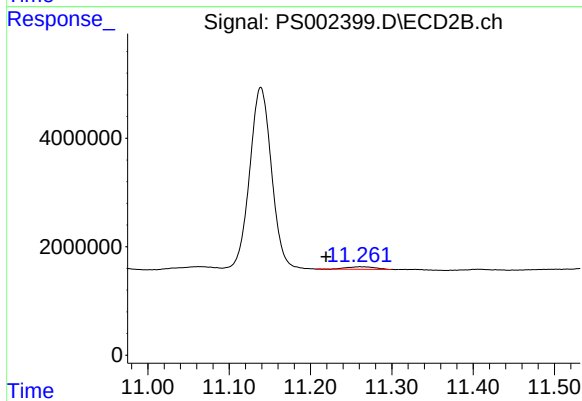

#5 DICAMBA


R.T.: 11.261 min
Delta R.T.: 0.042 min
Response: 1049326
Conc: 0.78 ng/ml

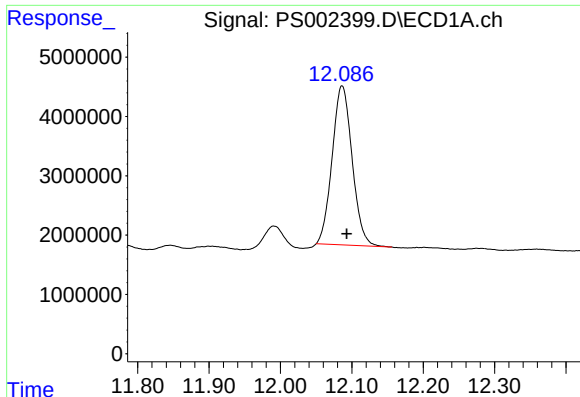

#6 MCP


R.T.: 12.086 min
Delta R.T.: -0.006 min
Response: 52156186
Conc: 55.57 ug/ml

Instrument :
ECD_S
ClientSampleId :

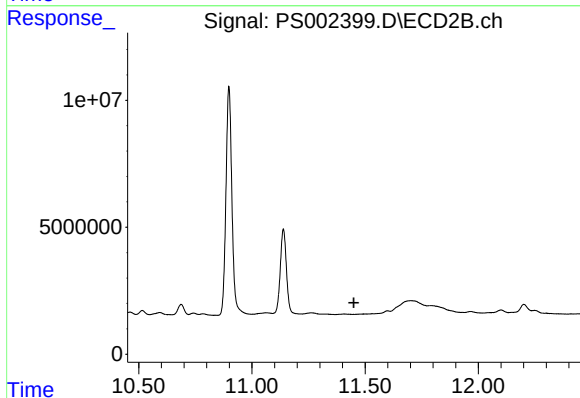


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.450 min
Response: 0
Conc: N.D.

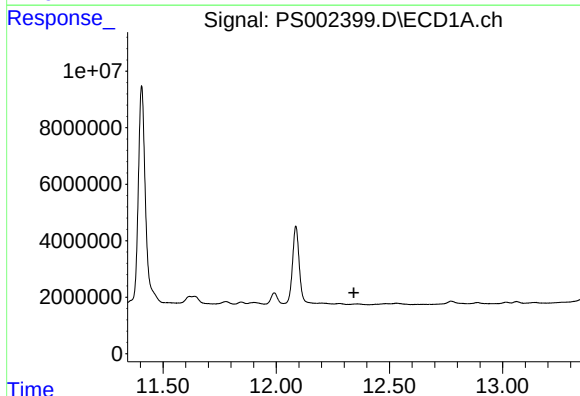


#7 MCP

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

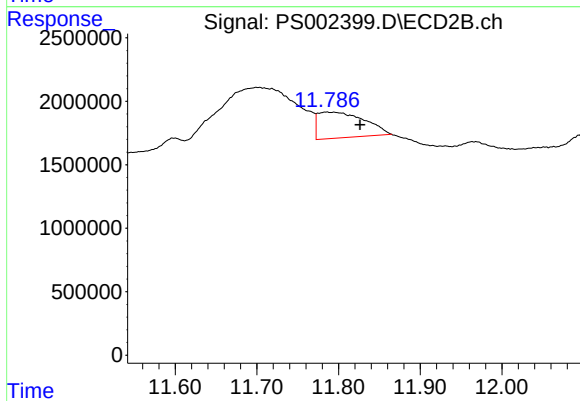

#7 MCP


R.T.: 11.785 min
Delta R.T.: -0.041 min
Response: 8013490
Conc: 5.69 ug/ml

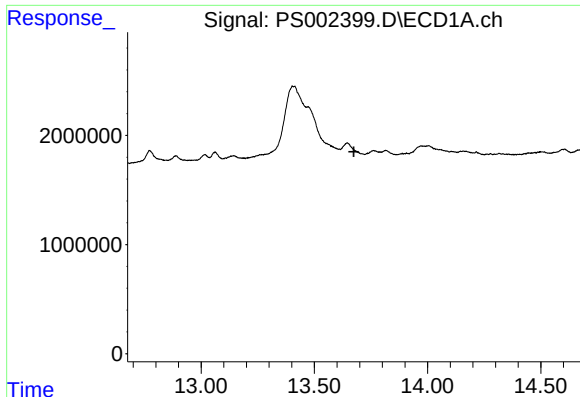

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

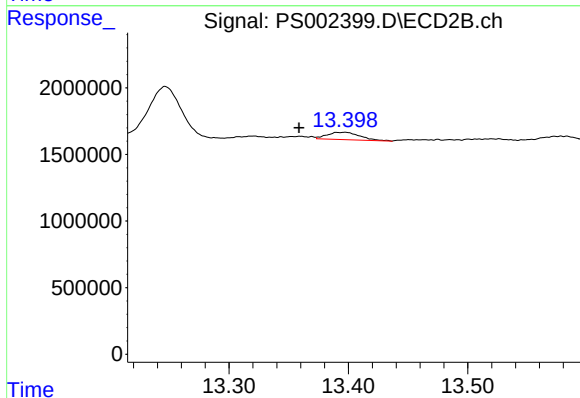


#10 Pentachlorophenol

R.T.: 13.397 min
Delta R.T.: 0.039 min
Response: 1031868
Conc: 0.20 ng/ml

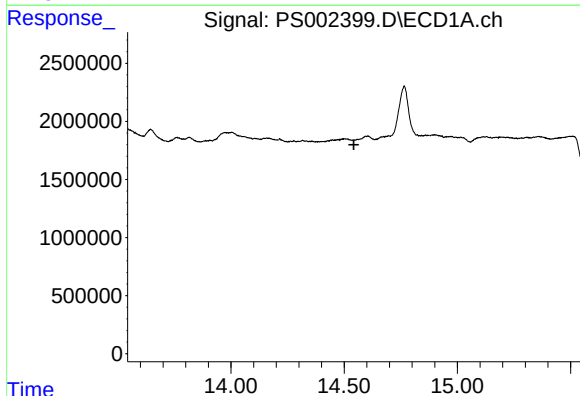


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.543 min
Response: 0
Conc: N.D.

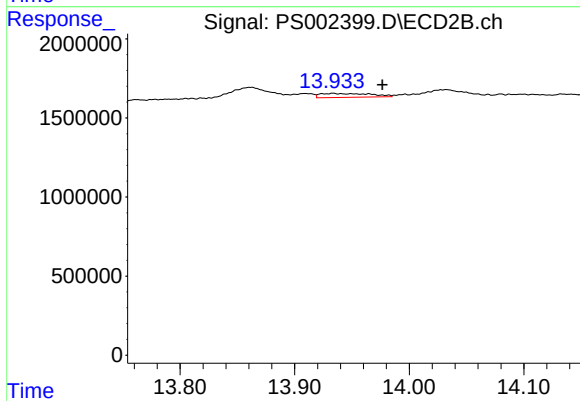

#11 2,4,5-TP (SILVEX)


R.T.: 13.934 min
Delta R.T.: -0.043 min
Response: 763816
Conc: 0.38 ng/ml

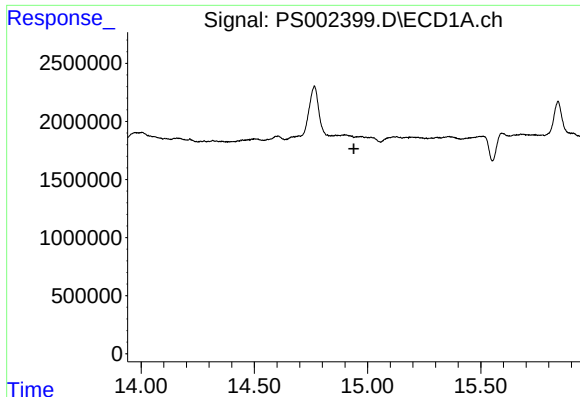

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

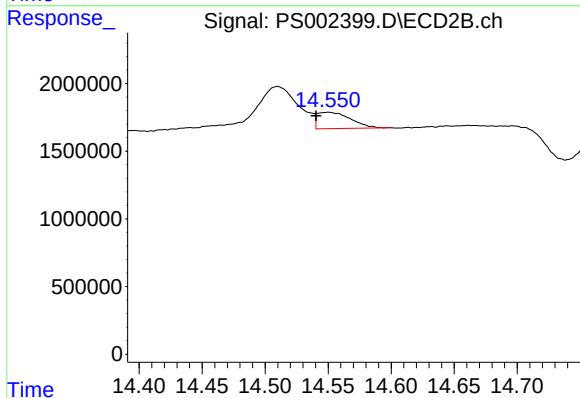


#12 2,4,5-T

R.T.: 14.550 min
Delta R.T.: 0.010 min
Response: 2191122
Conc: 1.40 ng/ml

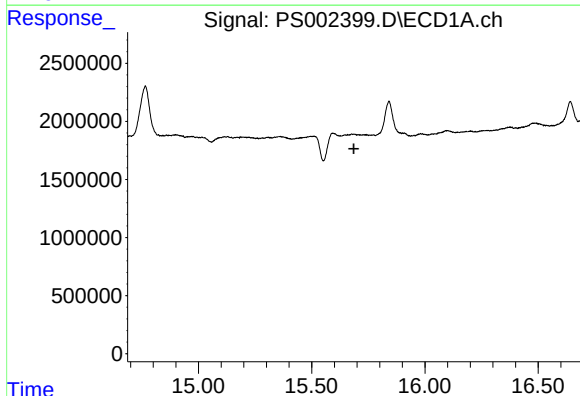


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.686 min
Response: 0
Conc: N.D.

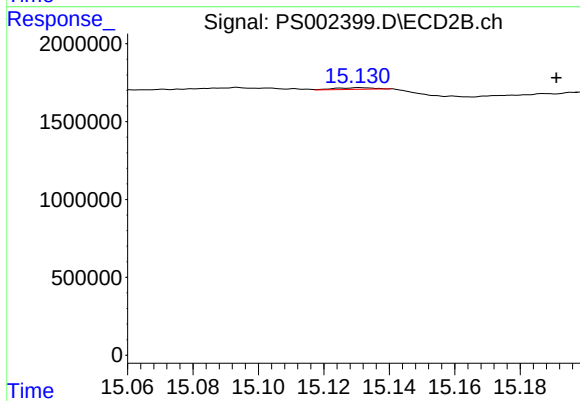

#13 2,4-DB


R.T.: 15.131 min
Delta R.T.: -0.060 min
Response: 146810
Conc: 0.65 ng/ml

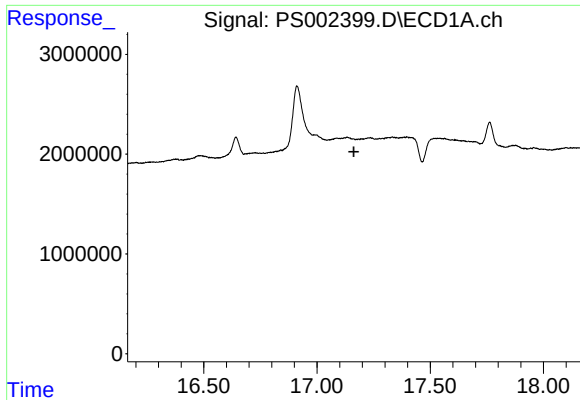

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

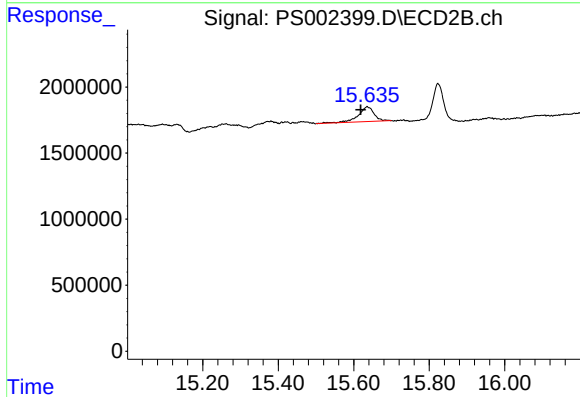


#14 DINOSEB

R.T.: 15.636 min
Delta R.T.: 0.018 min
Response: 3259448
Conc: 2.18 ng/ml

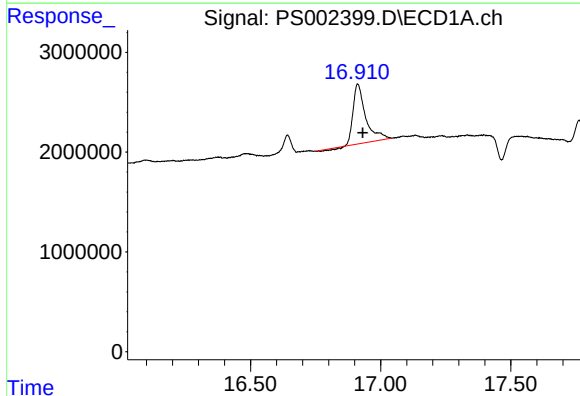


#15 Picloram

R.T.: 16.912 min
Delta R.T.: -0.020 min
Response: 19887967
Conc: 9.36 ng/ml

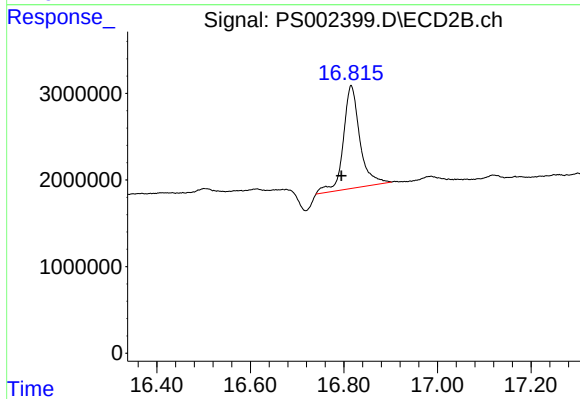

#15 Picloram


R.T.: 16.816 min
Delta R.T.: 0.021 min
Response: 29230629
Conc: 10.99 ng/ml

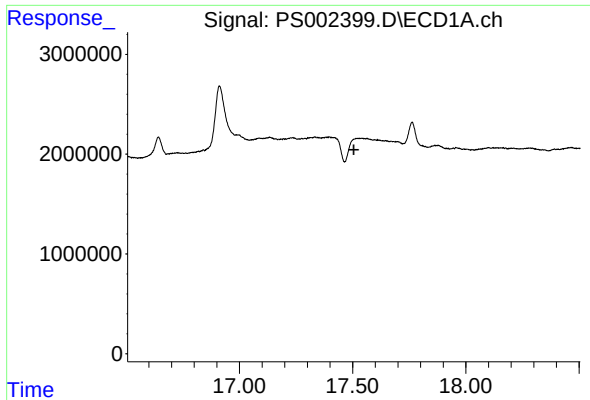

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

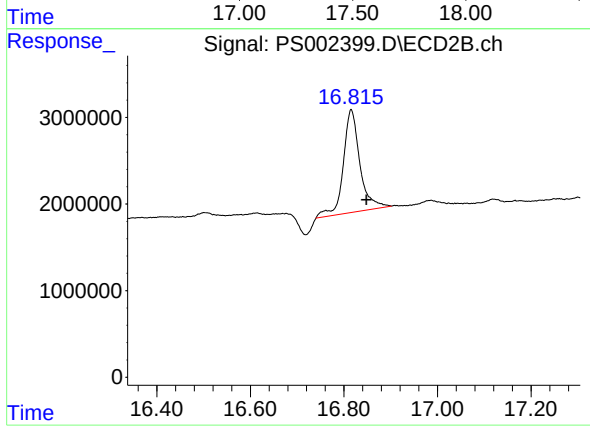

#16 DCPA

R.T.: 16.816 min
Delta R.T.: -0.032 min
Response: 29230629
Conc: 12.19 ng/ml