

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2018 00:36
 Operator : EI\SJ
 Sample : J5863-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 03:18:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.405	10.897	135.7E6	132.2E6	445.666	361.163
Target Compounds							
2) T	3,5-DICHL...	0.000	9.059	0	1363112	N.D.	3.007 #
3) T	4-Nitroph...	0.000	10.052	0	1984129	N.D.	11.324 #
5) T	DICAMBA	0.000	11.264	0	505475	N.D.	0.374 #
6) T	MCP	12.086	0.000	46629750	0	49.684	N.D. #
7) T	MCPA	0.000	11.800	0	7527041	N.D.	5.349 #
9) T	2,4-D	0.000	12.872	0	653335	N.D.	1.636 #
12) T	2,4,5-T	0.000	14.553	0	3885286	N.D.	2.485 #
14) T	DINOSEB	0.000	15.634	0	4608508	N.D.	3.079 #
15) T	Picloram	0.000	16.760	0	1021325	N.D.	0.384 #
16) T	DCPA	0.000	16.831	0	2763759	N.D.	1.152 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2018 00:36
Operator : EI\SJ
Sample : J5863-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 03:18:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

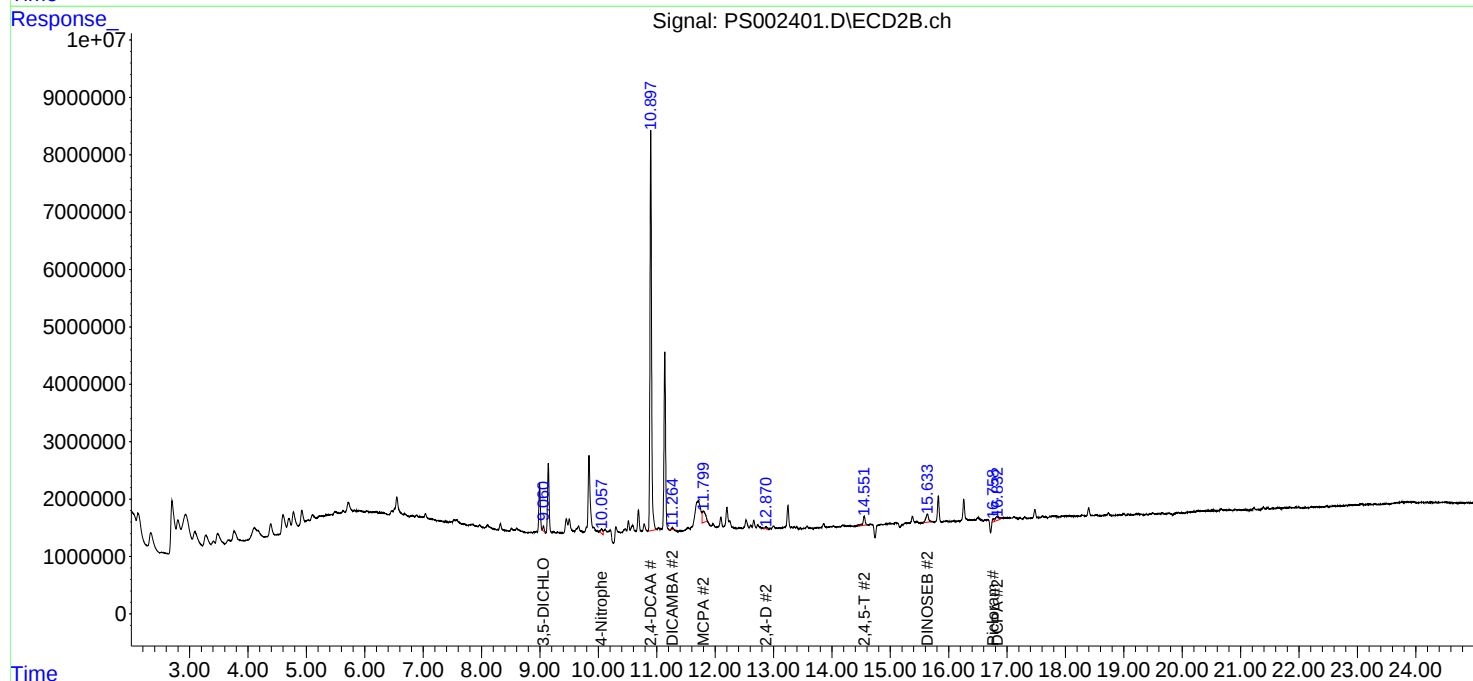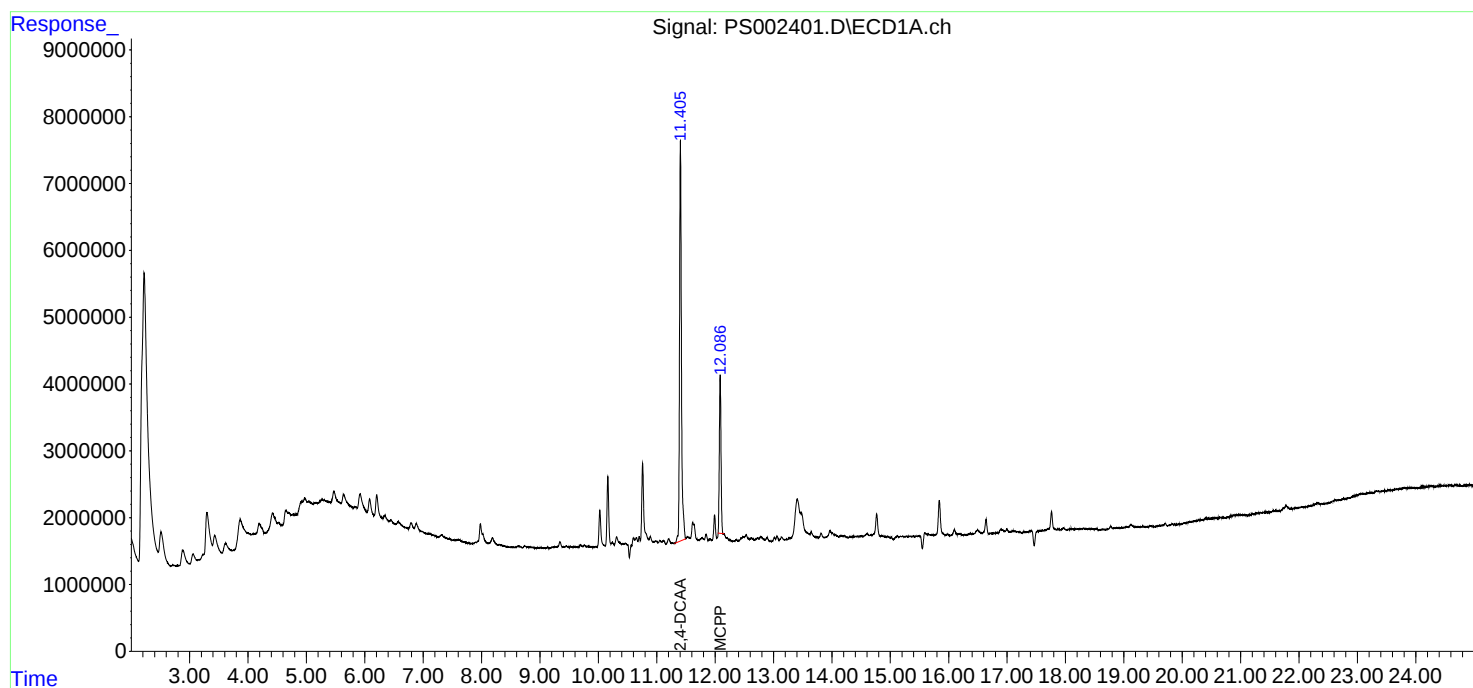


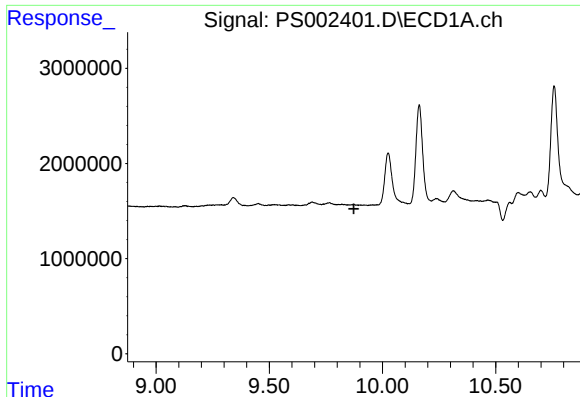

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

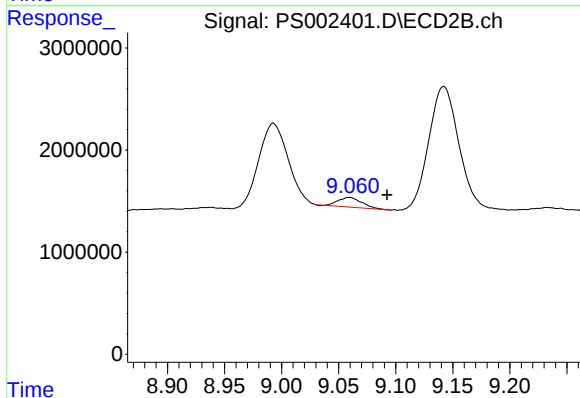


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.059 min
Delta R.T.: -0.033 min
Response: 1363112
Conc: 3.01 ng/ml

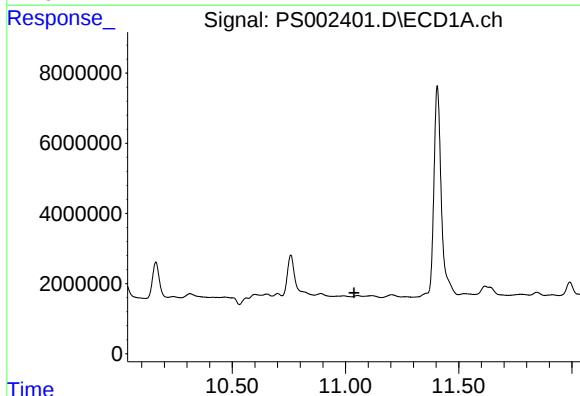


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

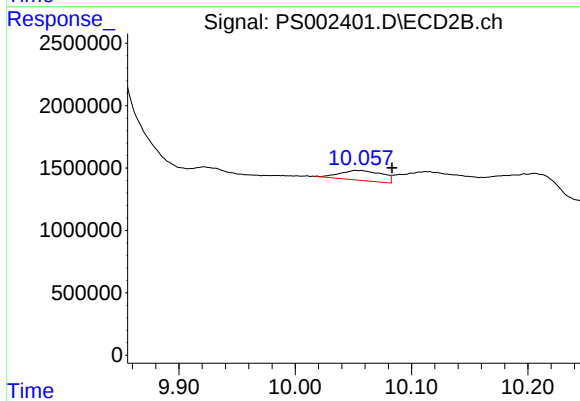

#3 4-Nitrophenol


R.T.: 10.052 min
Delta R.T.: -0.031 min
Response: 1984129
Conc: 11.32 ng/ml

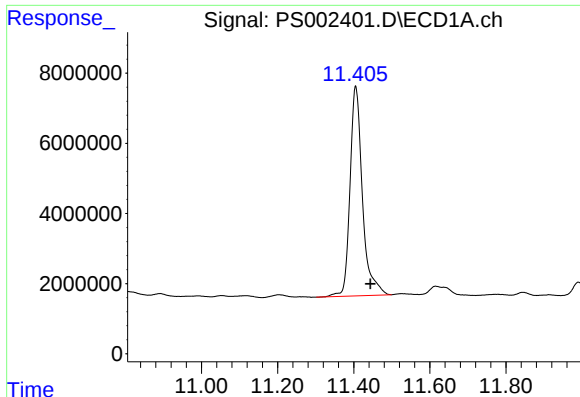

#4 2,4-DCAA


R.T.: 11.405 min
Delta R.T.: -0.039 min
Response: 135749593
Conc: 445.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

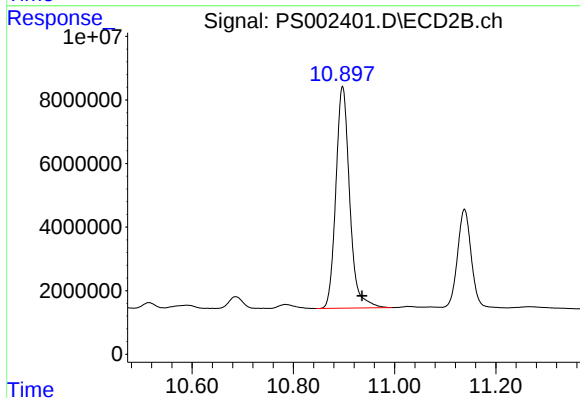


#4 2,4-DCAA

R.T.: 10.897 min
Delta R.T.: -0.039 min
Response: 132153892
Conc: 361.16 ng/ml

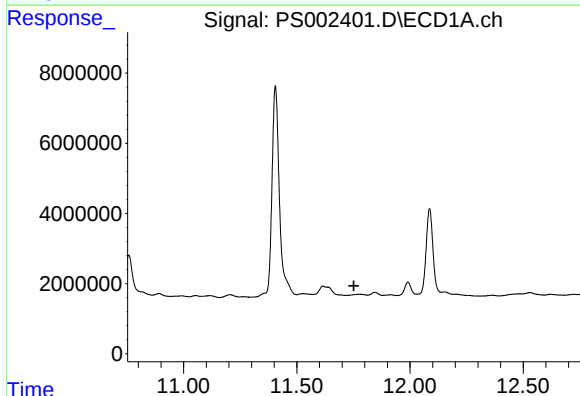


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.752 min
Response: 0
Conc: N.D.

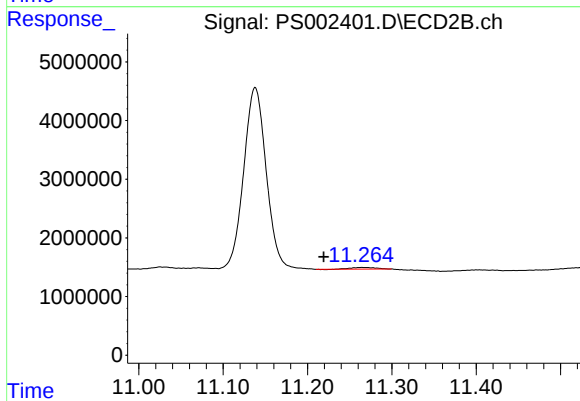

#5 DICAMBA


R.T.: 11.264 min
Delta R.T.: 0.045 min
Response: 505475
Conc: 0.37 ng/ml

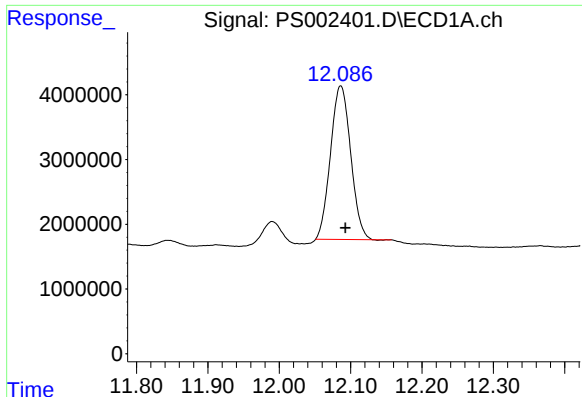

#6 MCPP


R.T.: 12.086 min
Delta R.T.: -0.007 min
Response: 46629750
Conc: 49.68 ug/ml

Instrument :
ECD_S
ClientSampleId :

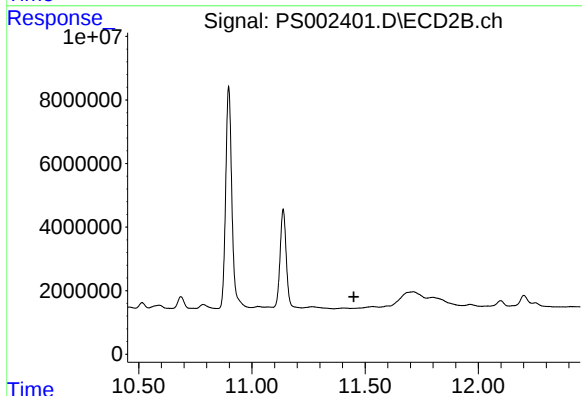


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.450 min
Response: 0
Conc: N.D.

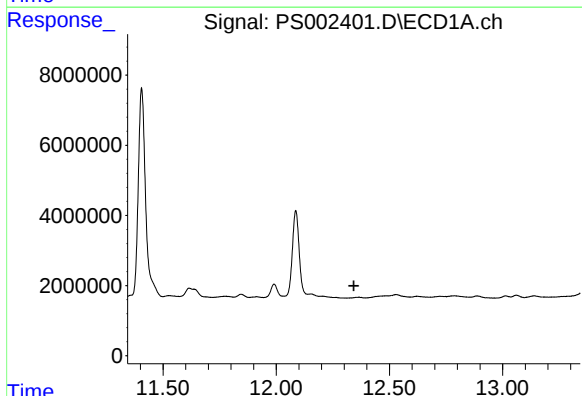


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

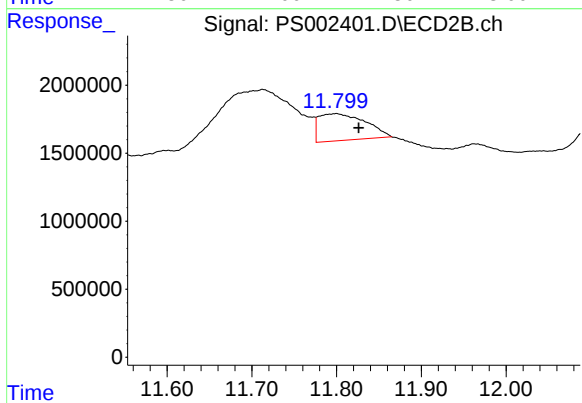

#7 MCPA


R.T.: 11.800 min
Delta R.T.: -0.026 min
Response: 7527041
Conc: 5.35 ug/ml

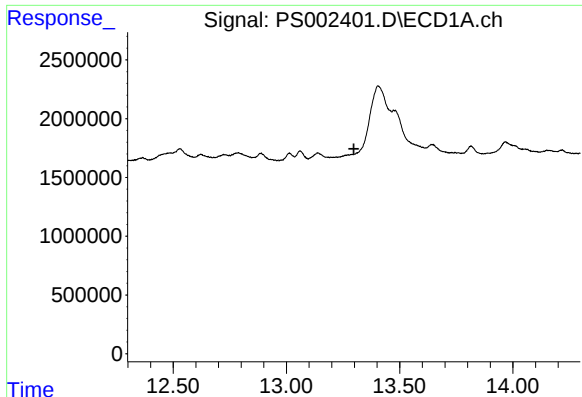

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

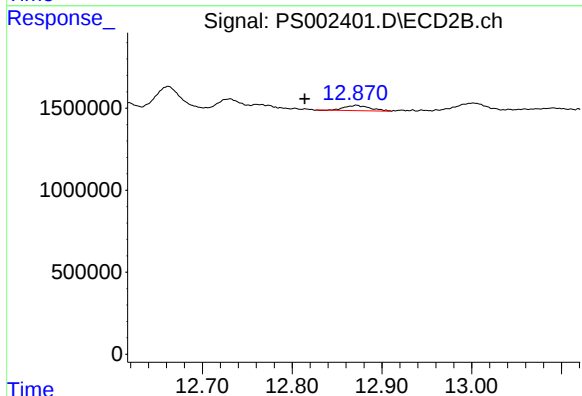


#9 2,4-D

R.T.: 12.872 min
Delta R.T.: 0.058 min
Response: 653335
Conc: 1.64 ng/ml

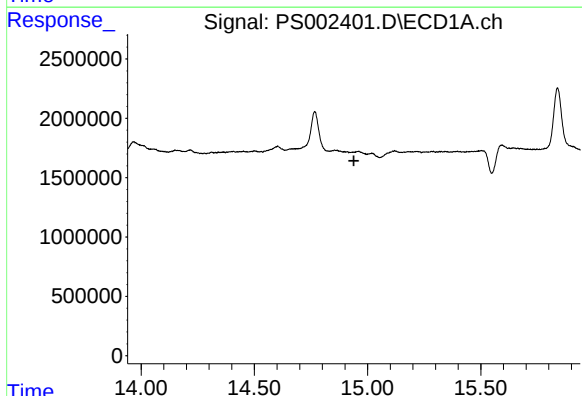


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.940 min
Response: 0
Conc: N.D.

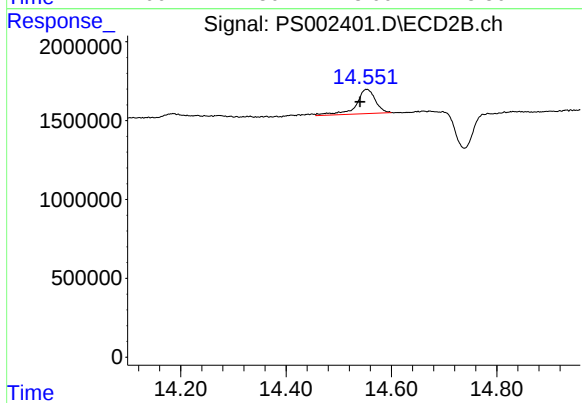

#12 2,4,5-T


R.T.: 14.553 min
Delta R.T.: 0.013 min
Response: 3885286
Conc: 2.49 ng/ml

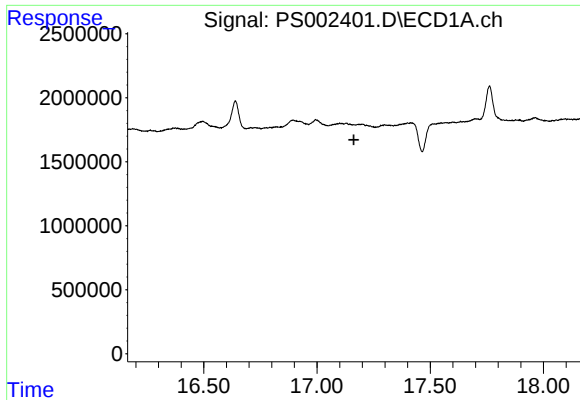

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

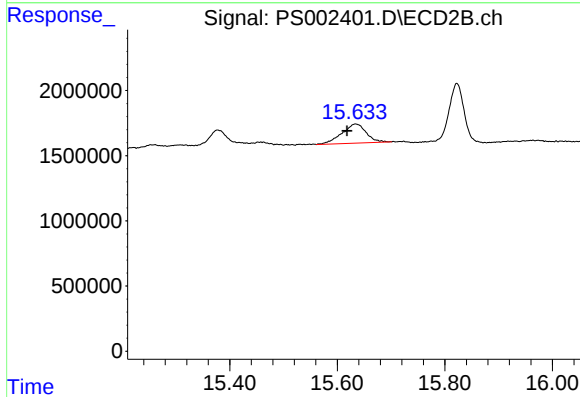


#14 DINOSEB

R.T.: 15.634 min
Delta R.T.: 0.016 min
Response: 4608508
Conc: 3.08 ng/ml

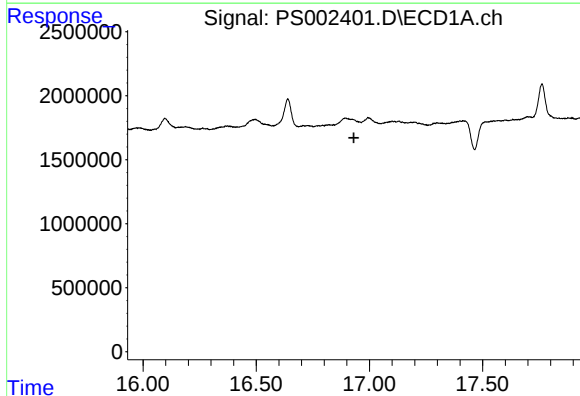


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.931 min
Response: 0
Conc: N.D.

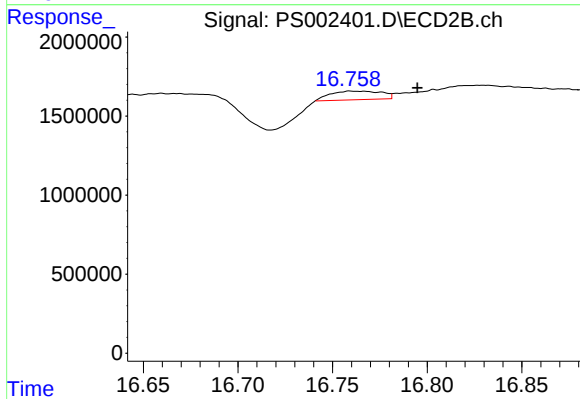

#15 Picloram


R.T.: 16.760 min
Delta R.T.: -0.035 min
Response: 1021325
Conc: 0.38 ng/ml

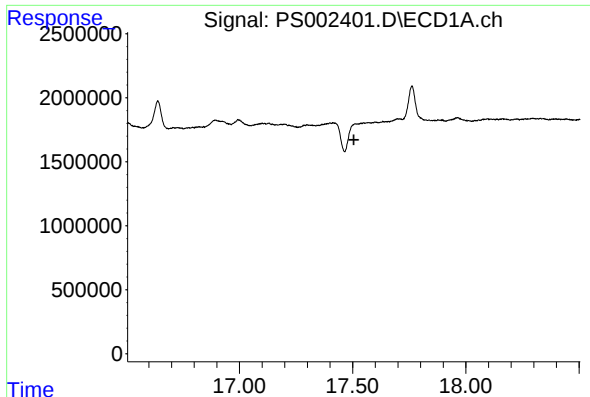

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

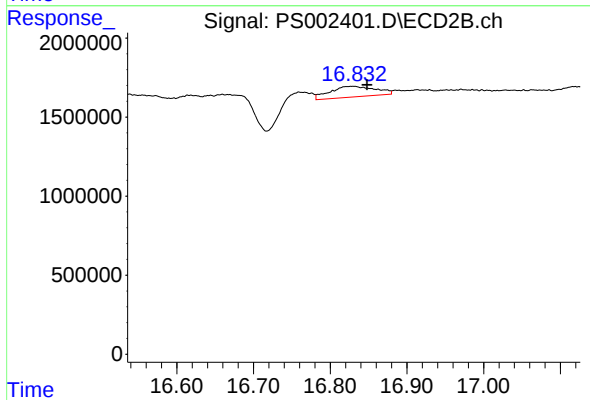

#16 DCPA

R.T.: 16.831 min
Delta R.T.: -0.017 min
Response: 2763759
Conc: 1.15 ng/ml