

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2018 01:07
 Operator : EI\SJ
 Sample : J5877-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 03:18:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.444	10.935	88401658	84783345	290.222	231.704
Target Compounds							
1) T	Dalapon	0.000	2.370	0	1956489	N.D.	4.546 #
2) T	3,5-DICHL...	0.000	9.094	0	260970	N.D.	0.576 #
3) T	4-Nitroph...	0.000	10.091	0	2533271	N.D.	14.458 #
6) T	MCP	12.123	0.000	30839525	0	32.859	N.D. #
7) T	MCPA	0.000	11.828	0	1274596	N.D.	0.906 #
8) T	DICHLORPROP	0.000	12.288	0	456063	N.D.	1.376 #
10) T	Pentachlo...	13.678	0.000	3164008	0	0.654	N.D. #
12) T	2,4,5-T	0.000	14.590	0	116249	N.D.	0.074 #
14) T	DINOSEB	0.000	15.670	0	1589413	N.D.	1.062 #
15) T	Picloram	0.000	16.799	0	759956	N.D.	0.286 #
16) T	DCPA	0.000	16.855	0	850828	N.D.	0.355 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2018 01:07
Operator : EI\SJ
Sample : J5877-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 03:18:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

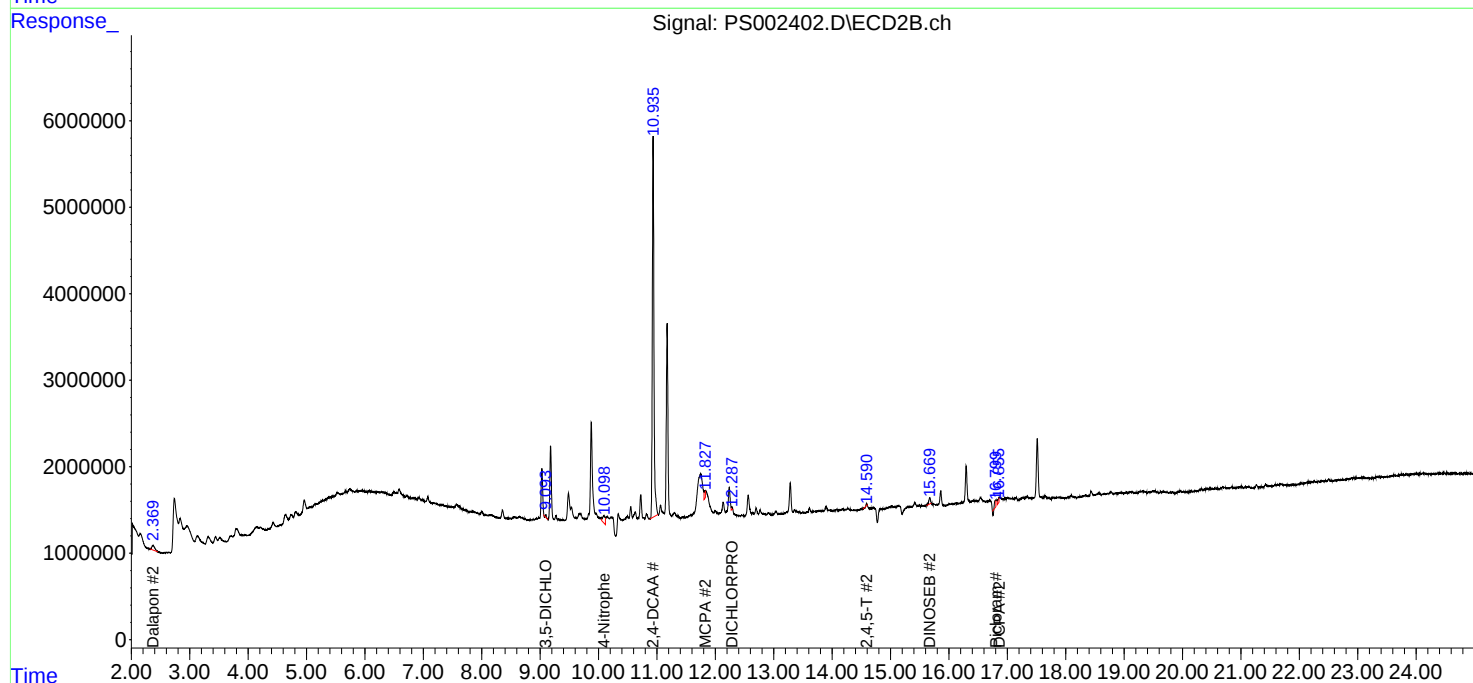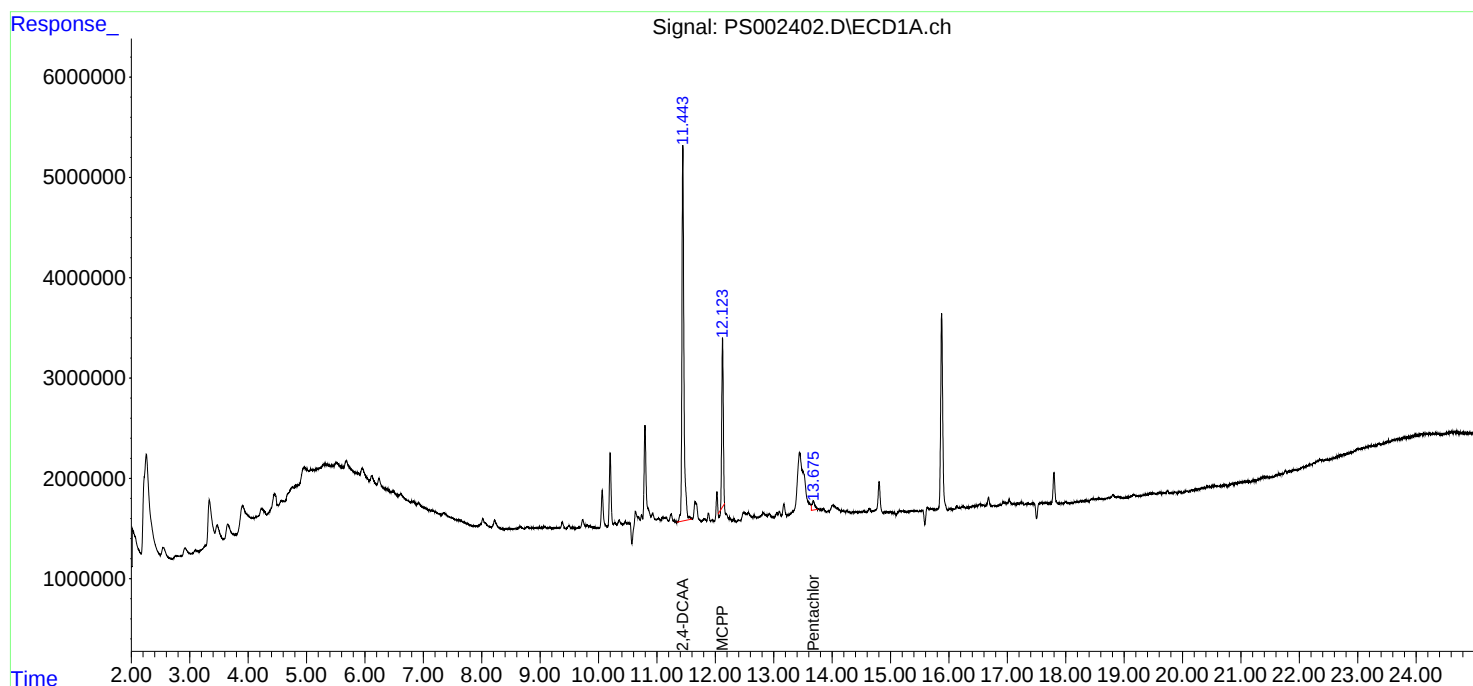


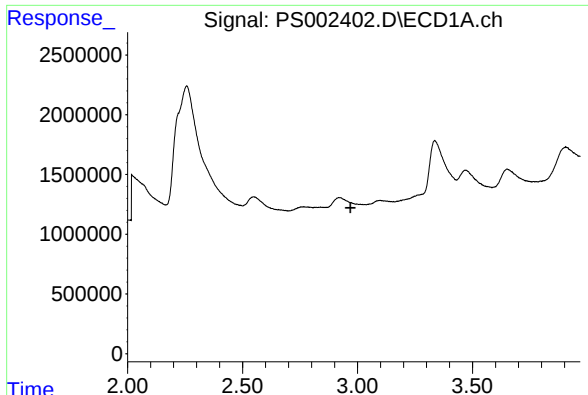

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

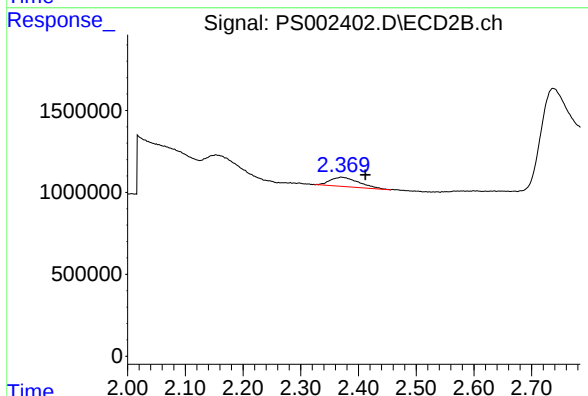


#1 Dalapon

R.T.: 2.370 min
Delta R.T.: -0.042 min
Response: 1956489
Conc: 4.55 ng/ml

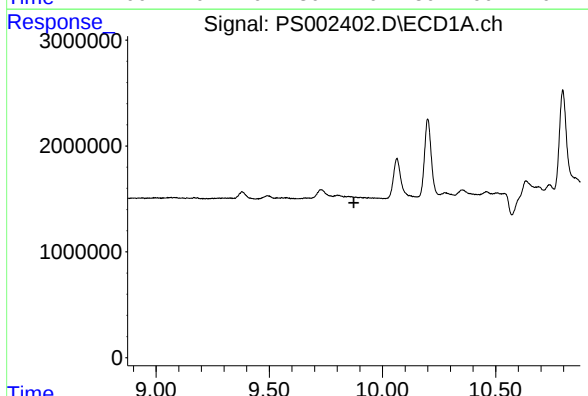


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.874 min
Response: 0
Conc: N.D.

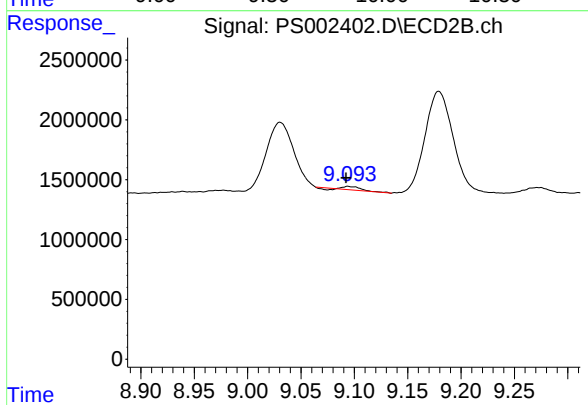

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.094 min
Delta R.T.: 0.001 min
Response: 260970
Conc: 0.58 ng/ml

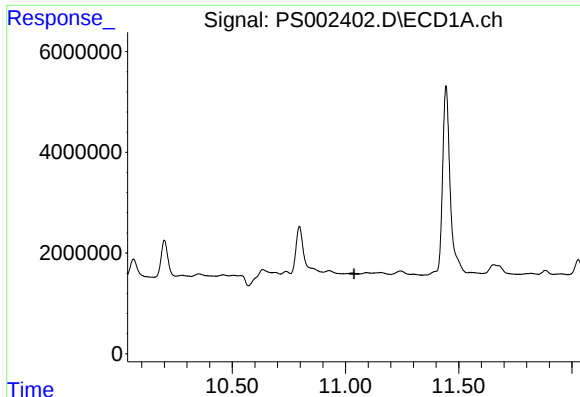

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

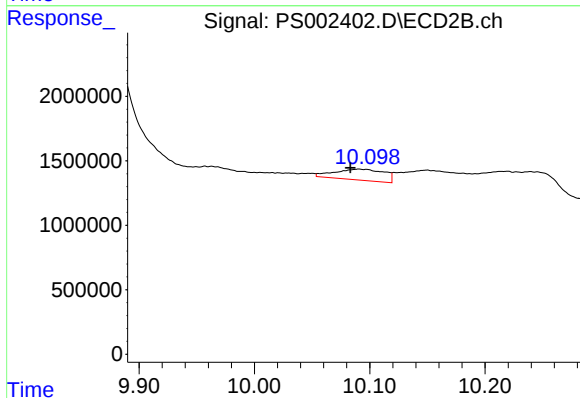


#3 4-Nitrophenol

R.T.: 10.091 min
Delta R.T.: 0.008 min
Response: 2533271
Conc: 14.46 ng/ml

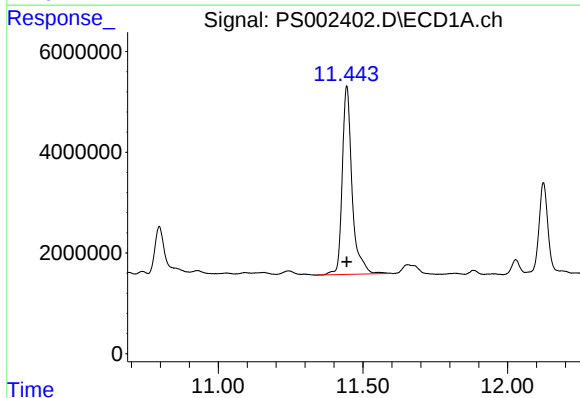


#4 2,4-DCAA

R.T.: 11.444 min
Delta R.T.: 0.000 min
Response: 88401658
Conc: 290.22 ng/ml

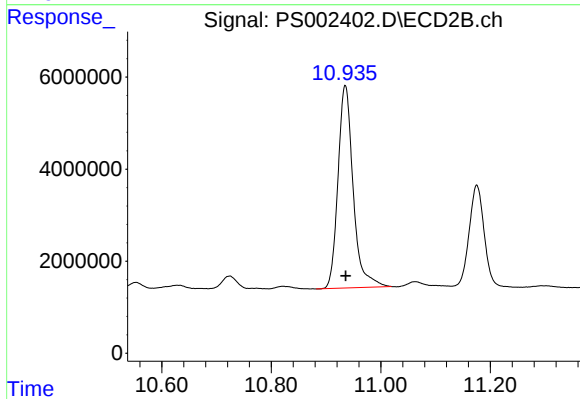

#4 2,4-DCAA


R.T.: 10.935 min
Delta R.T.: -0.001 min
Response: 84783345
Conc: 231.70 ng/ml

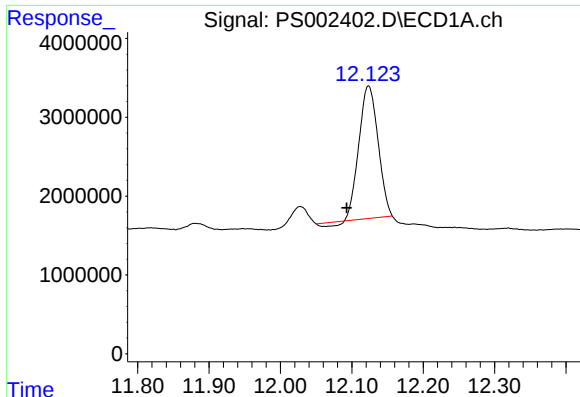

#6 MCPP


R.T.: 12.123 min
Delta R.T.: 0.031 min
Response: 30839525
Conc: 32.86 ug/ml

Instrument :
ECD_S
ClientSampleId :

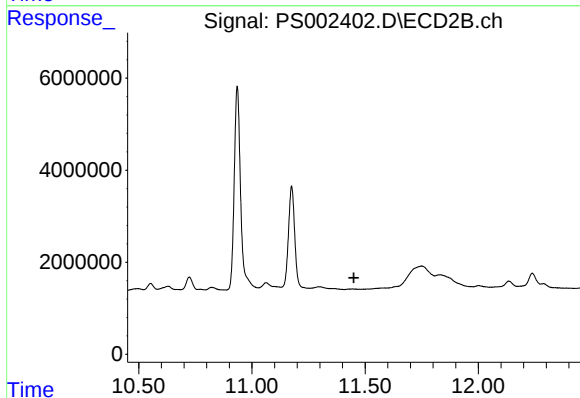


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.450 min
Response: 0
Conc: N.D.

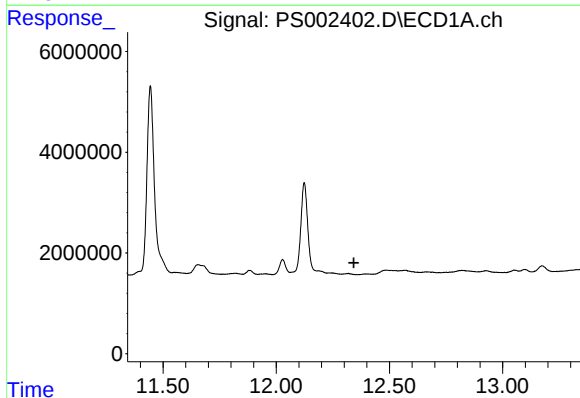


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

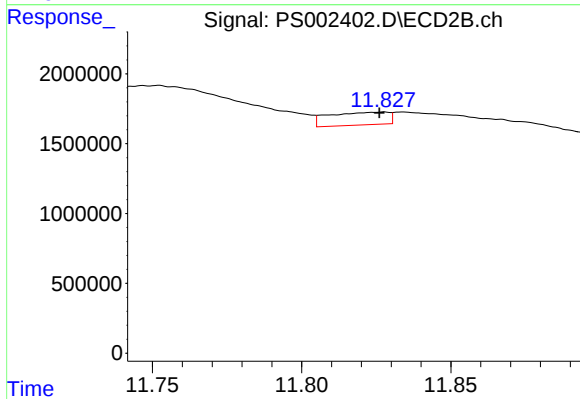

#7 MCPA


R.T.: 11.828 min
Delta R.T.: 0.002 min
Response: 1274596
Conc: 0.91 ug/ml

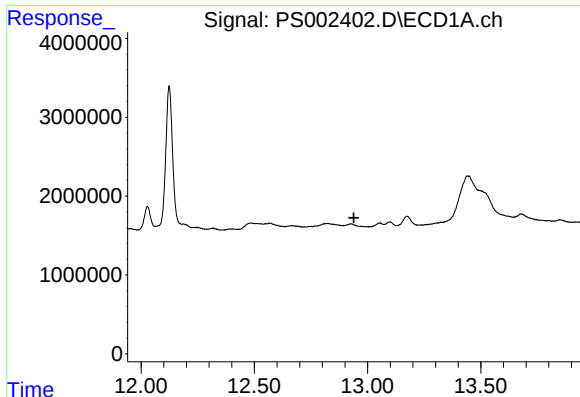

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.939 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

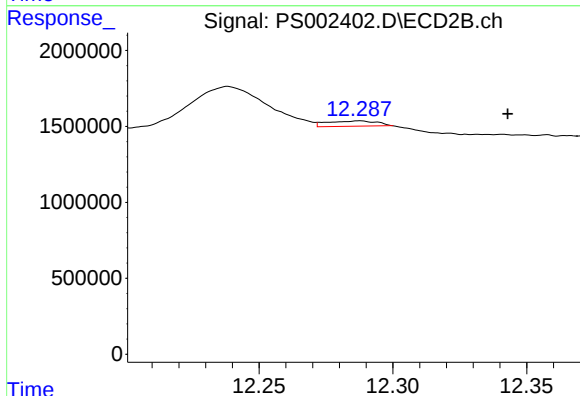


#8 DICHLORPROP

R.T.: 12.288 min
Delta R.T.: -0.055 min
Response: 456063
Conc: 1.38 ng/ml

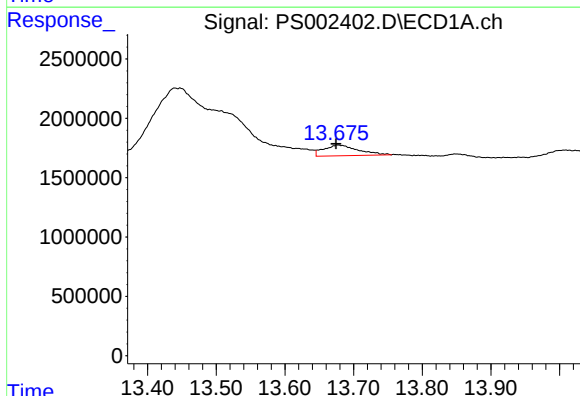


#10 Pentachlorophenol

R.T.: 13.678 min
Delta R.T.: 0.003 min
Response: 3164008
Conc: 0.65 ng/ml

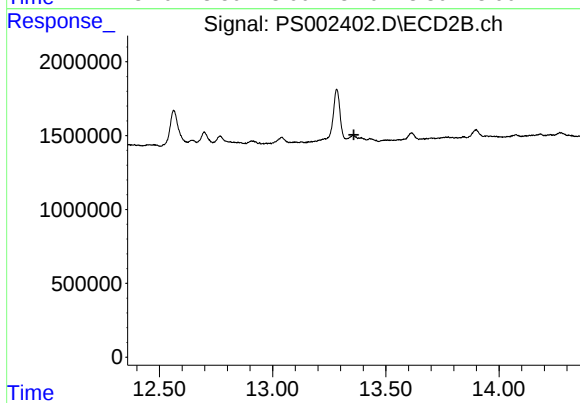

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.359 min
Response: 0
Conc: N.D.

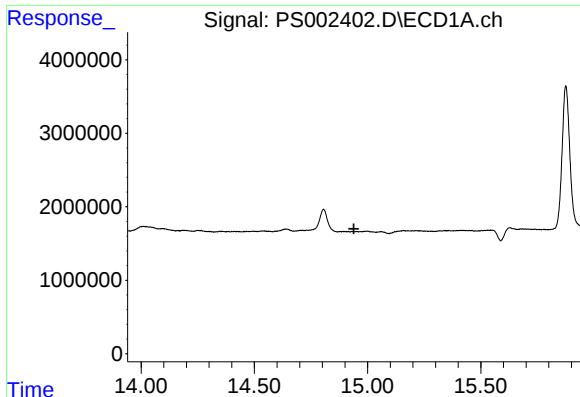

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

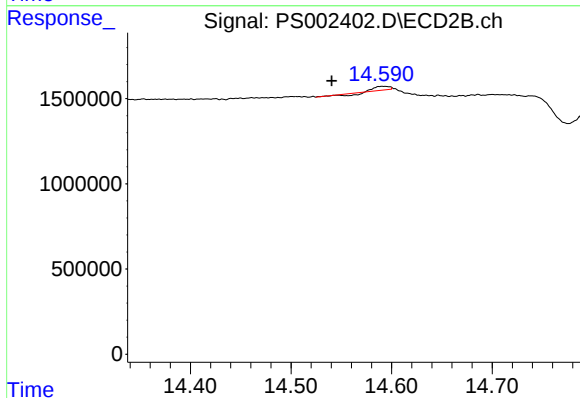


#12 2,4,5-T

R.T.: 14.590 min
Delta R.T.: 0.050 min
Response: 116249
Conc: 0.07 ng/ml

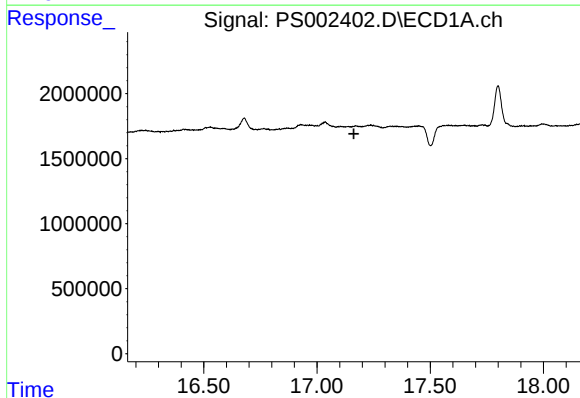


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.163 min
Response: 0
Conc: N.D.

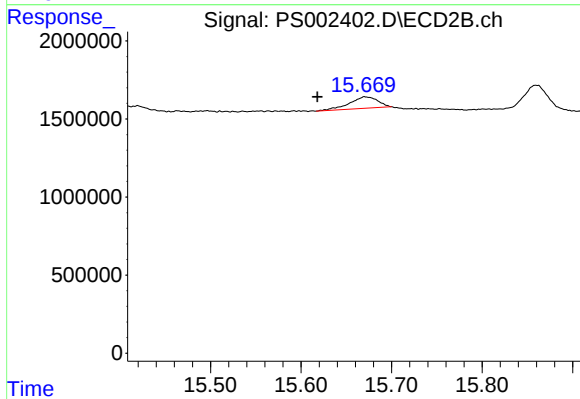

#14 DINOSEB


R.T.: 15.670 min
Delta R.T.: 0.052 min
Response: 1589413
Conc: 1.06 ng/ml

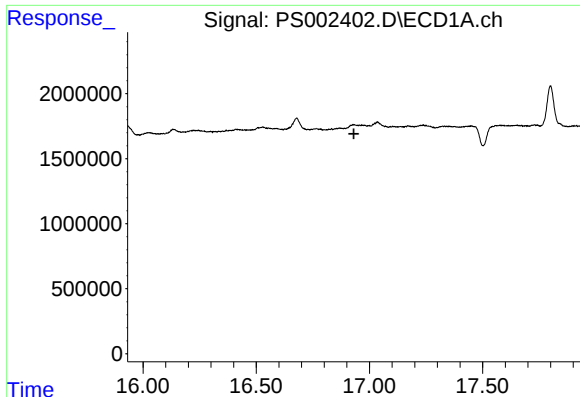

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

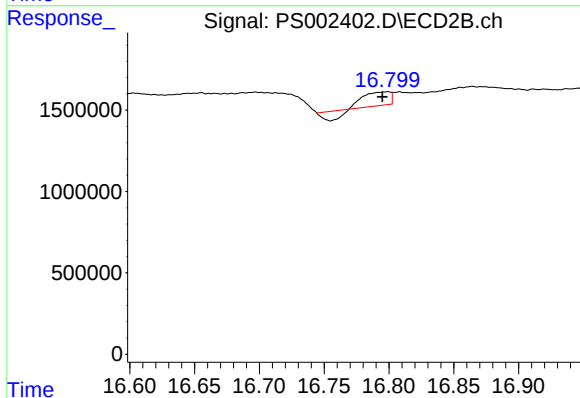


#15 Picloram

R.T.: 16.799 min
Delta R.T.: 0.004 min
Response: 759956
Conc: 0.29 ng/ml

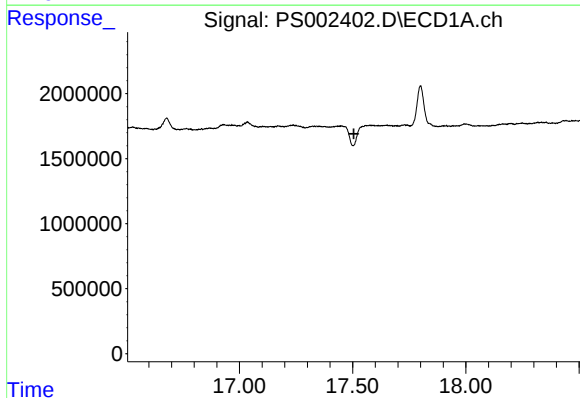

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

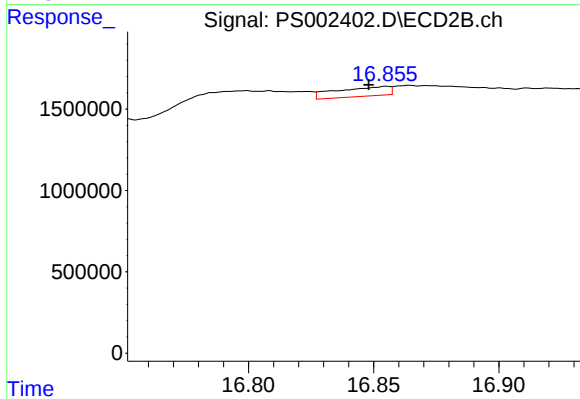

#16 DCPA

R.T.: 16.855 min
Delta R.T.: 0.007 min
Response: 850828
Conc: 0.35 ng/ml