

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2018 01:38
 Operator : EI\SJ
 Sample : J5884-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 03:18:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.427	10.924	115.7E6	112.6E6	379.682	307.856
Target Compounds							
1) T	Dalapon	2.902	2.359	4251825	3817608	9.642	8.870
3) T	4-Nitroph...	0.000	10.084	0	2169994	N.D.	12.385 #
6) T	MCP	12.106	0.000	44834735	0	47.771	N.D. #
7) T	MCPA	0.000	11.818	0	3054407	N.D.	2.171 #
8) T	DICHLORPROP	0.000	12.278	0	1222337	N.D.	3.688 #
9) T	2,4-D	0.000	12.755	0	160082	N.D.	0.401 #
12) T	2,4,5-T	0.000	14.585	0	764566	N.D.	0.489 #
13) T	2,4-DB	0.000	15.124	0	943866	N.D.	4.163 #
14) T	DINOSEB	0.000	15.663	0	2097781	N.D.	1.402 #
15) T	Picloram	0.000	16.793	0	4251327	N.D.	1.598 #
16) T	DCPA	0.000	16.854	0	3827651	N.D.	1.596 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2018 01:38
Operator : EI\SJ
Sample : J5884-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 03:18:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

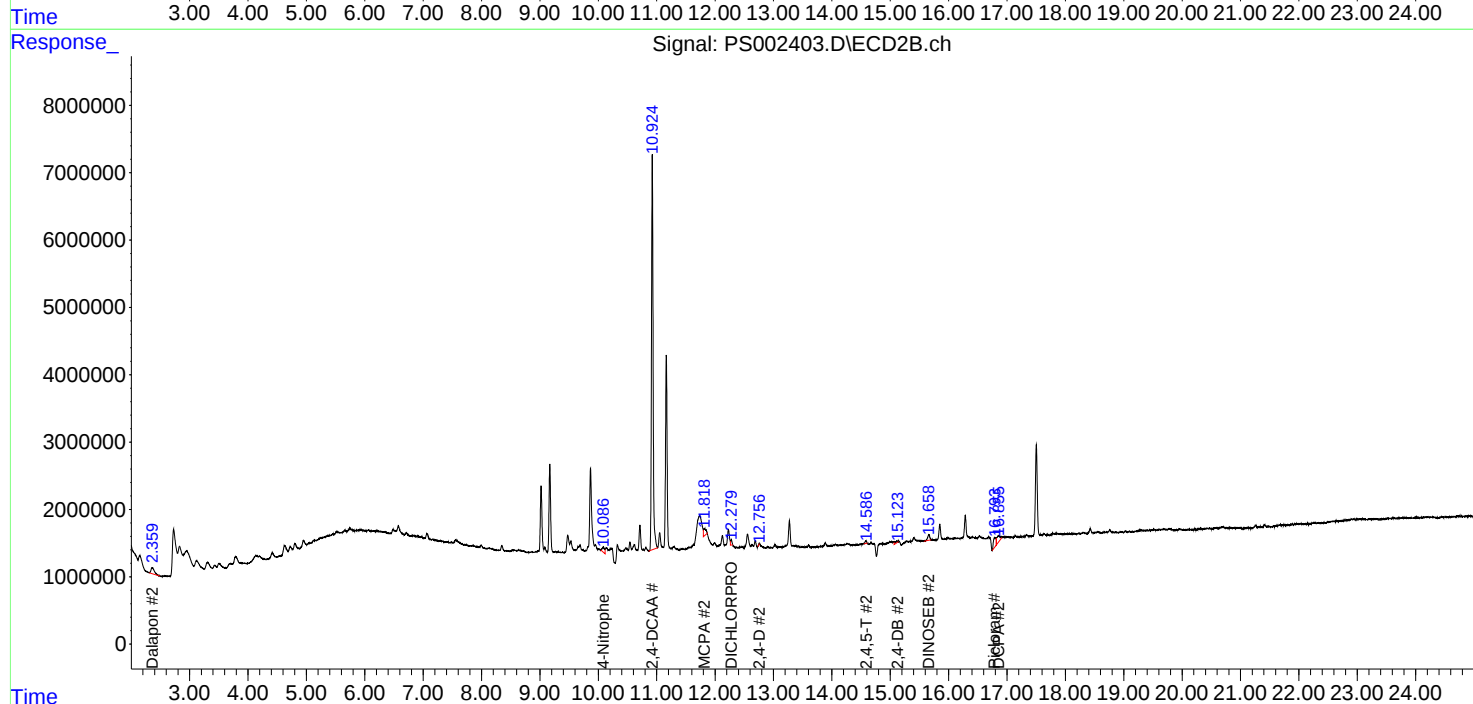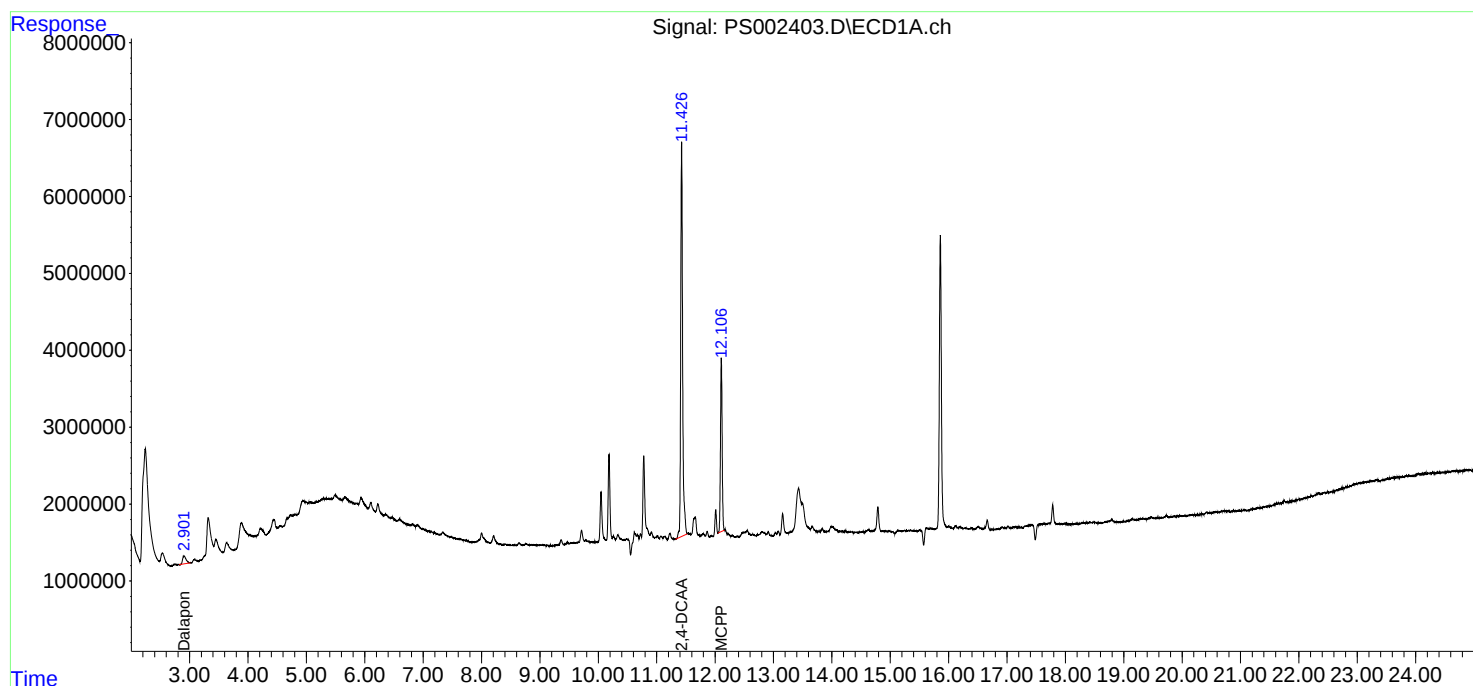


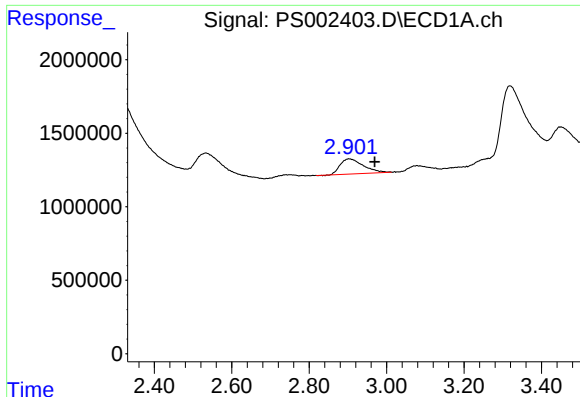

#1 Dalapon


R.T.: 2.902 min
Delta R.T.: -0.067 min
Response: 4251825
Conc: 9.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

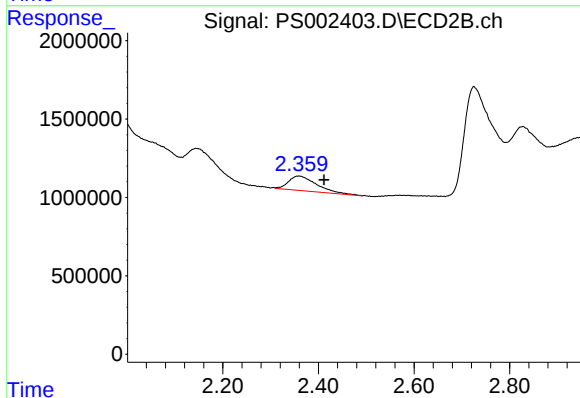


#1 Dalapon

R.T.: 2.359 min
Delta R.T.: -0.053 min
Response: 3817608
Conc: 8.87 ng/ml

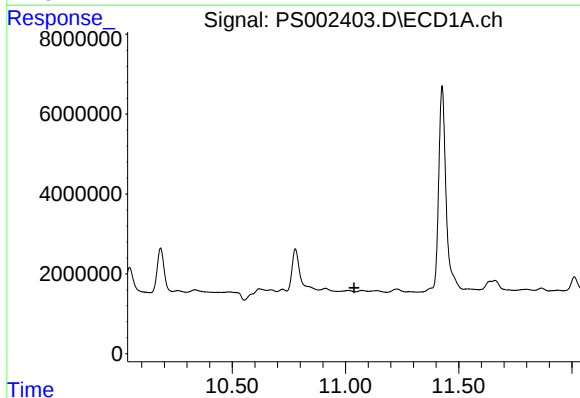


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

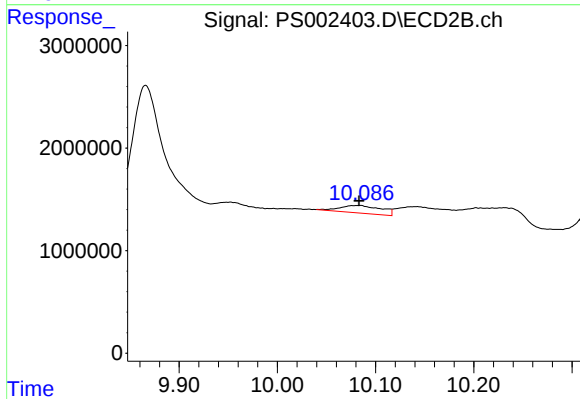

#3 4-Nitrophenol


R.T.: 10.084 min
Delta R.T.: 0.001 min
Response: 2169994
Conc: 12.38 ng/ml

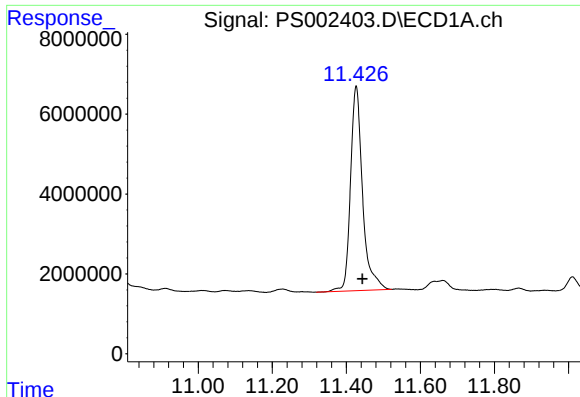

#4 2,4-DCAA


R.T.: 11.427 min
Delta R.T.: -0.017 min
Response: 115651062
Conc: 379.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

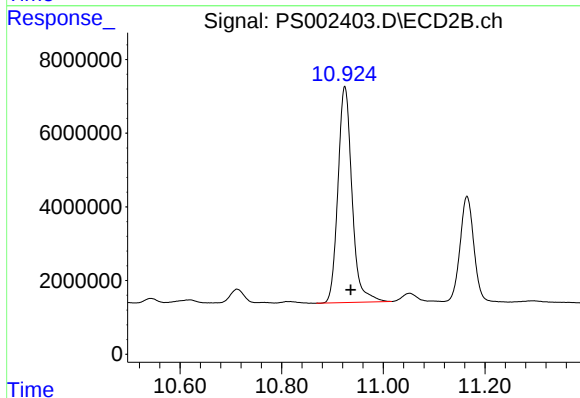


#4 2,4-DCAA

R.T.: 10.924 min
Delta R.T.: -0.012 min
Response: 112648458
Conc: 307.86 ng/ml

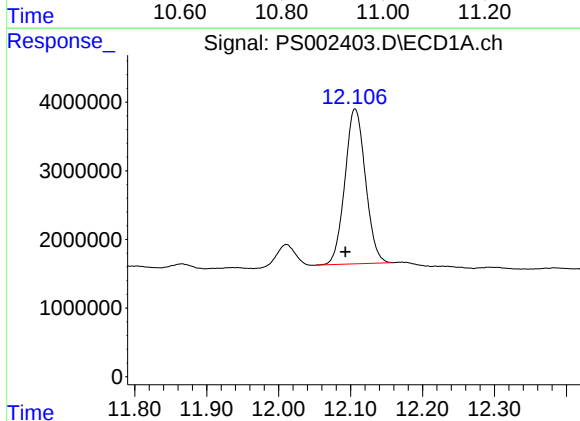


#6 MCP

R.T.: 12.106 min
Delta R.T.: 0.014 min
Response: 44834735
Conc: 47.77 ug/ml

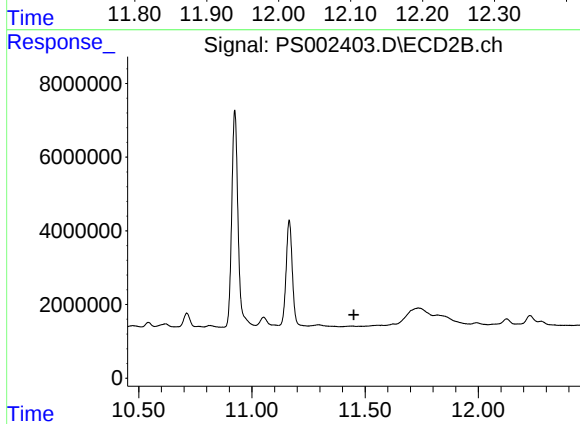

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.450 min
Response: 0
Conc: N.D.

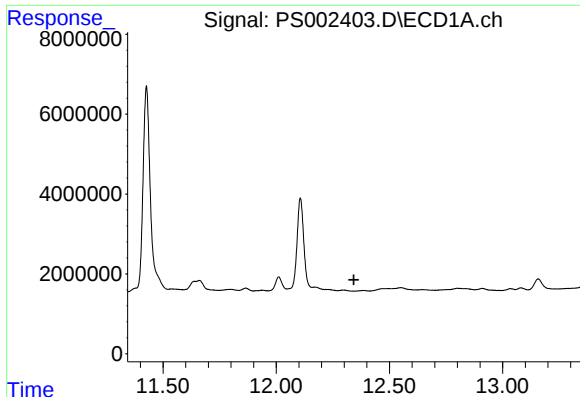

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

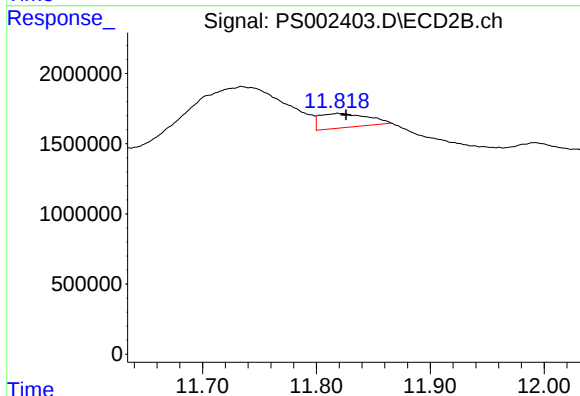


#7 MCPA

R.T.: 11.818 min
Delta R.T.: -0.008 min
Response: 3054407
Conc: 2.17 ug/ml

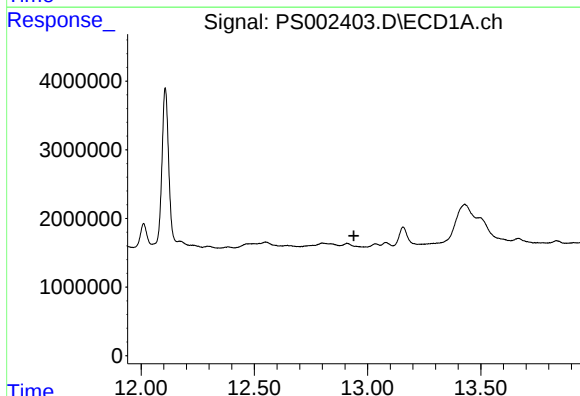


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.939 min
Response: 0
Conc: N.D.

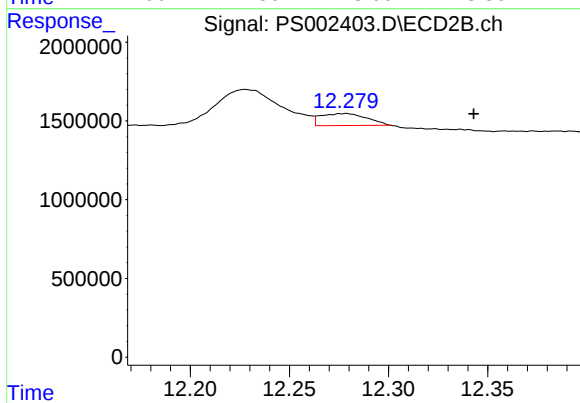

#8 DICHLORPROP


R.T.: 12.278 min
Delta R.T.: -0.065 min
Response: 1222337
Conc: 3.69 ng/ml

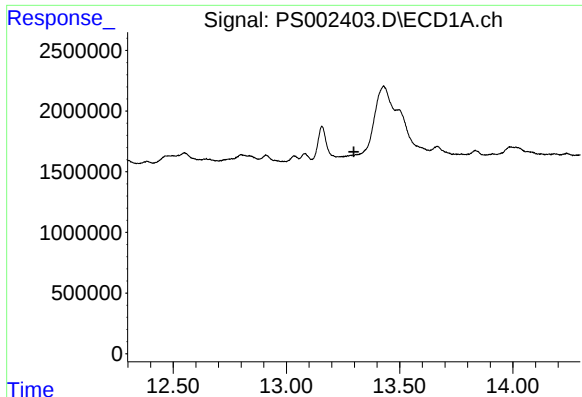

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

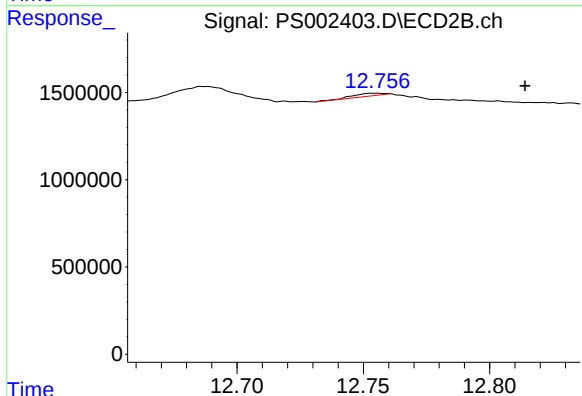


#9 2,4-D

R.T.: 12.755 min
Delta R.T.: -0.059 min
Response: 160082
Conc: 0.40 ng/ml

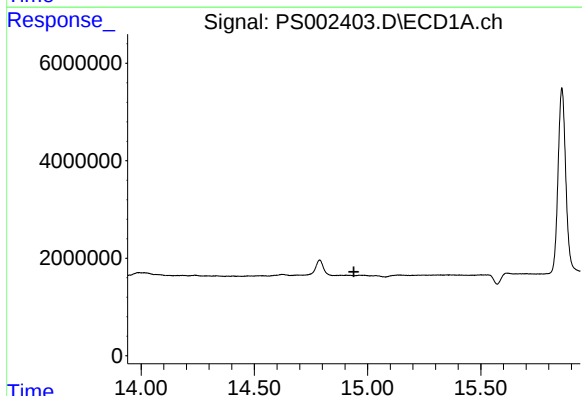


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.940 min
Response: 0
Conc: N.D.

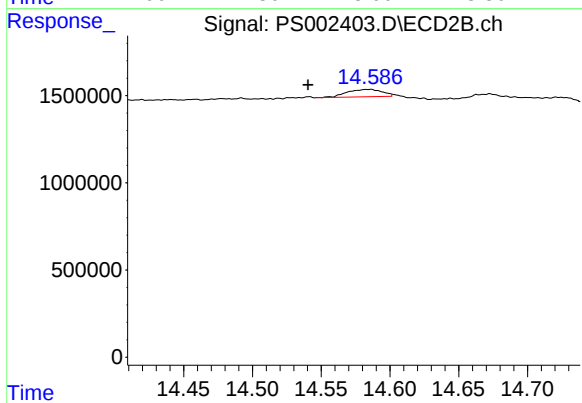

#12 2,4,5-T


R.T.: 14.585 min
Delta R.T.: 0.045 min
Response: 764566
Conc: 0.49 ng/ml

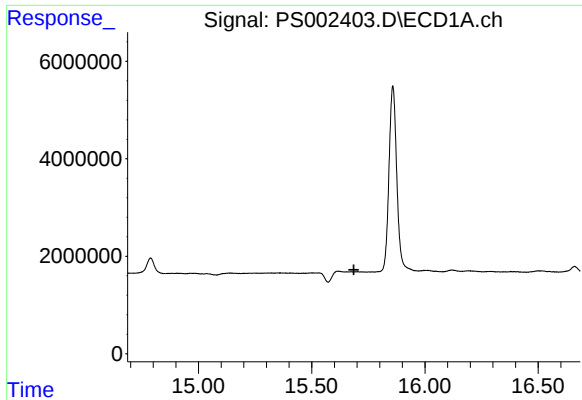

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

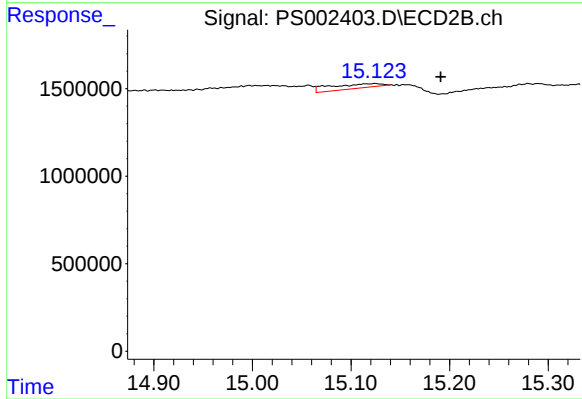


#13 2,4-DB

R.T.: 15.124 min
Delta R.T.: -0.067 min
Response: 943866
Conc: 4.16 ng/ml

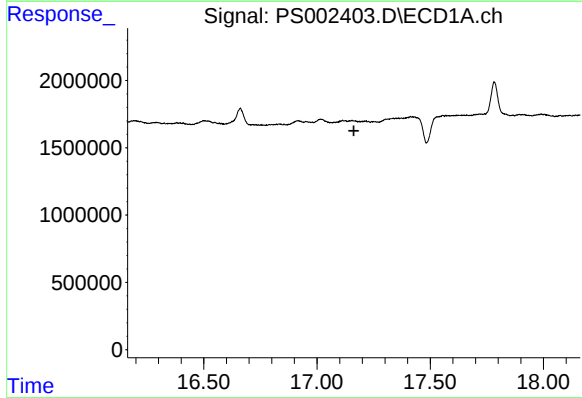


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.163 min
Response: 0
Conc: N.D.

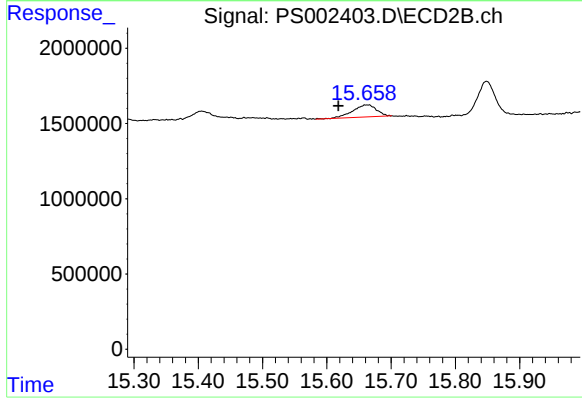

#14 DINOSEB


R.T.: 15.663 min
Delta R.T.: 0.045 min
Response: 2097781
Conc: 1.40 ng/ml

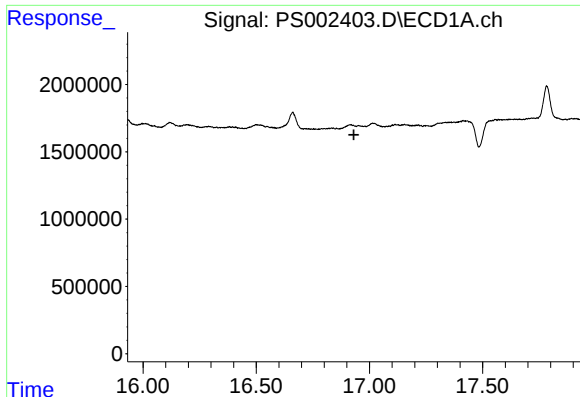

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

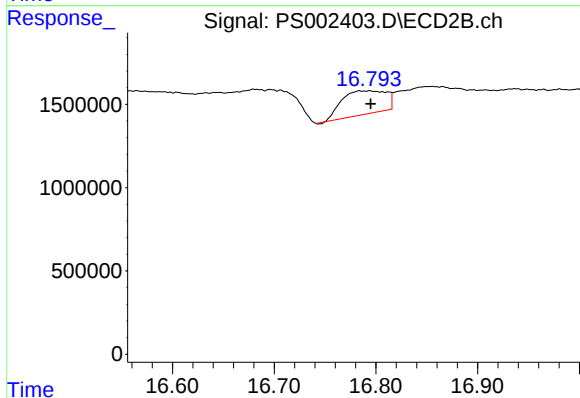


#15 Picloram

R.T.: 16.793 min
Delta R.T.: -0.002 min
Response: 4251327
Conc: 1.60 ng/ml

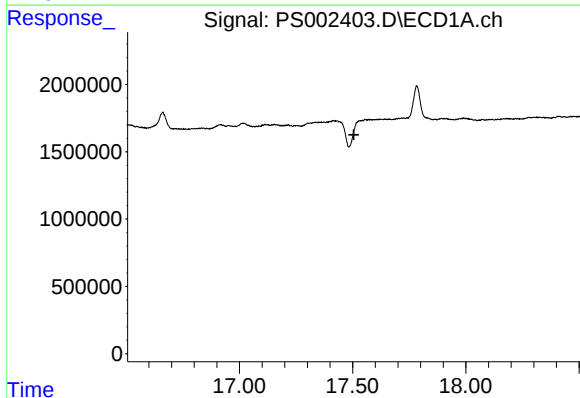

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

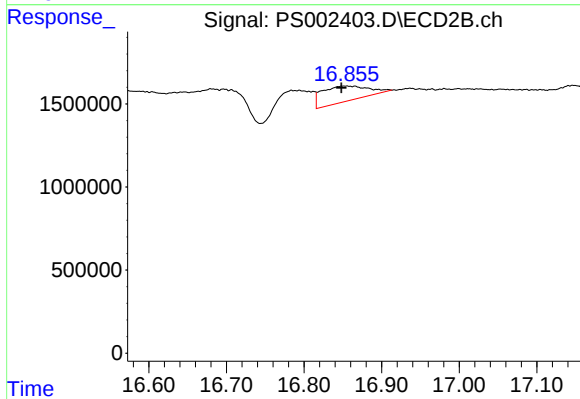

#16 DCPA

R.T.: 16.854 min
Delta R.T.: 0.006 min
Response: 3827651
Conc: 1.60 ng/ml