

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002404.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2018 02:09
 Operator : EI\SJ
 Sample : J5884-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 03:19:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.437	10.929	115.2E6	111.5E6	378.174	304.701
Target Compounds							
1) T	Dalapon	2.914	2.370	4477842	1841133	10.155	4.278 #
2) T	3,5-DICHL...	0.000	9.025	0	9180256	N.D.	20.250 #
3) T	4-Nitroph...	0.000	10.086	0	2234318	N.D.	12.752 #
6) T	MCP	12.118	0.000	43115633	0	45.939	N.D. #
7) T	MCPA	0.000	11.828	0	1628588	N.D.	1.157 #
8) T	DICHLORPROP	0.000	12.281	0	888632	N.D.	2.681 #
12) T	2,4,5-T	0.000	14.588	0	930868	N.D.	0.595 #
13) T	2,4-DB	15.630	15.244	6882177	63486	35.524	0.280 #
14) T	DINOSEB	0.000	15.665	0	2847400	N.D.	1.902 #
15) T	Picloram	0.000	16.792	0	2781244	N.D.	1.045 #
16) T	DCPA	0.000	16.853	0	2396256	N.D.	0.999 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002404.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2018 02:09
Operator : EI\SJ
Sample : J5884-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 03:19:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

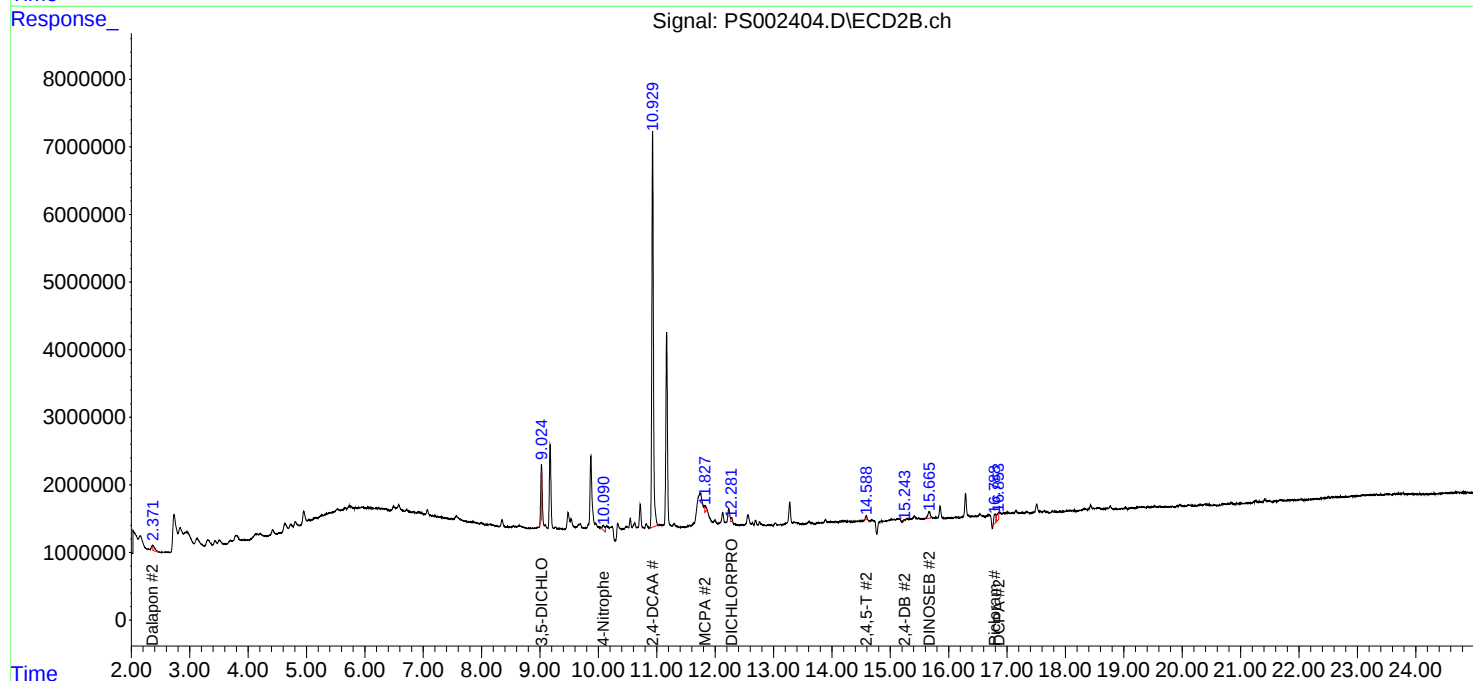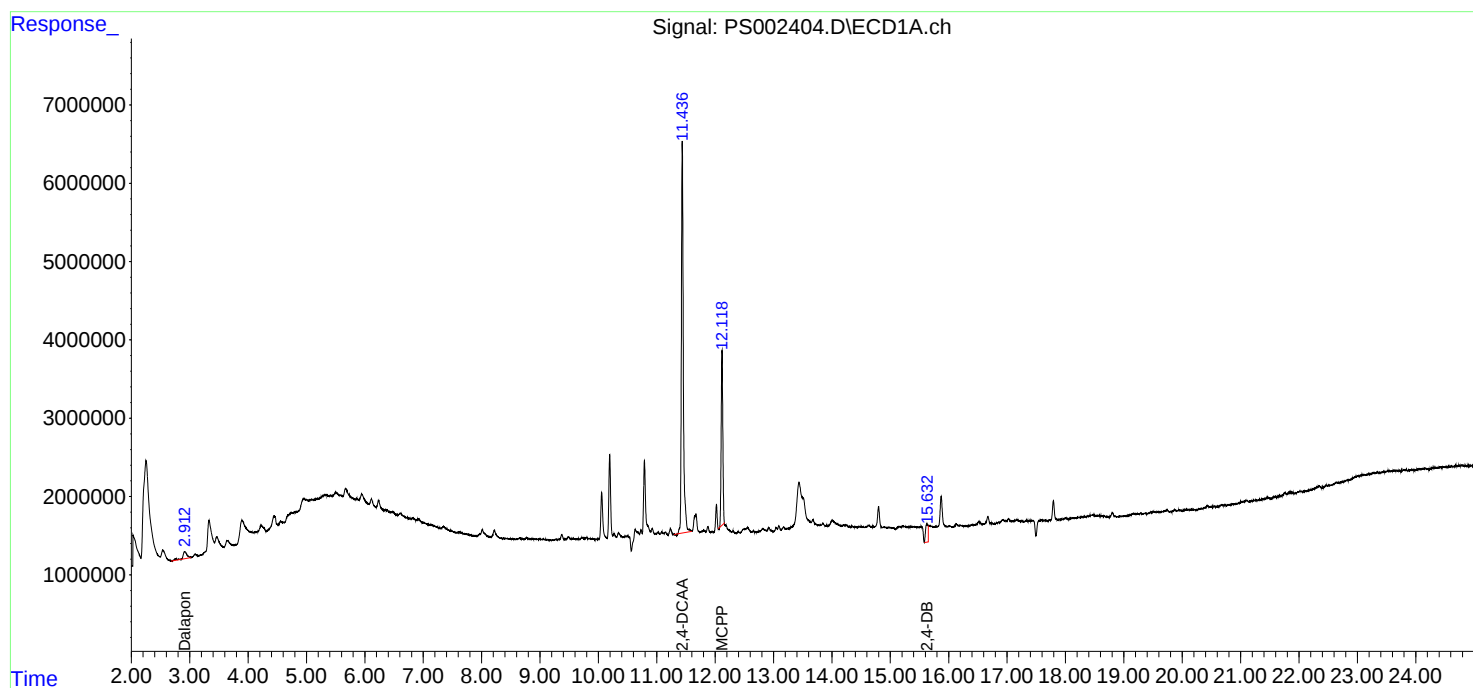


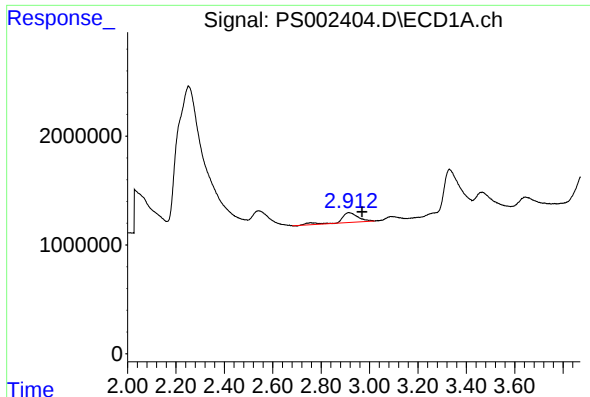

#1 Dalapon


R.T.: 2.914 min
Delta R.T.: -0.055 min
Response: 4477842
Conc: 10.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

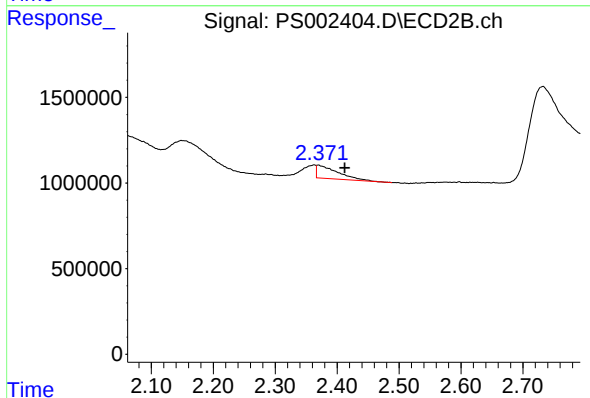


#1 Dalapon

R.T.: 2.370 min
Delta R.T.: -0.042 min
Response: 1841133
Conc: 4.28 ng/ml

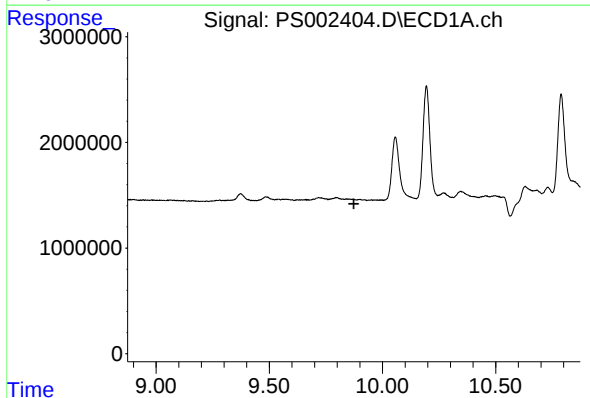


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.874 min
Response: 0
Conc: N.D.

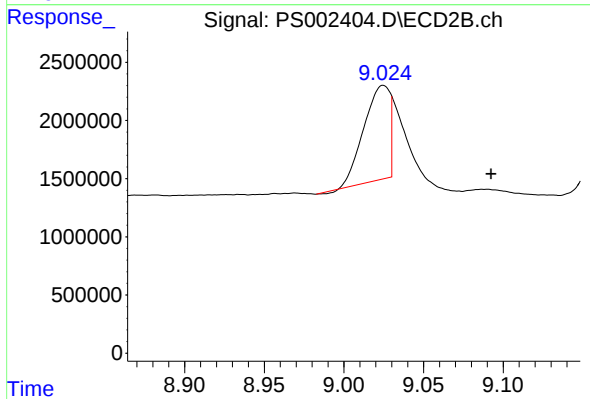

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.025 min
Delta R.T.: -0.068 min
Response: 9180256
Conc: 20.25 ng/ml

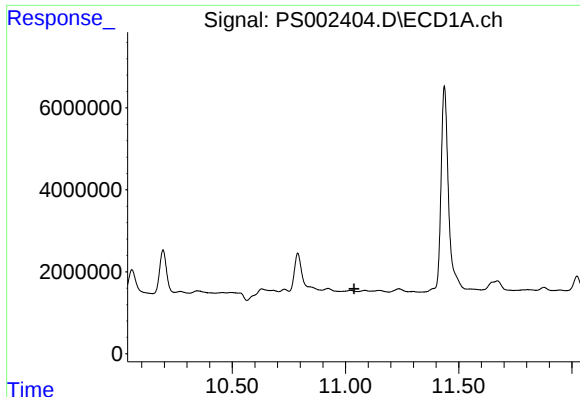

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

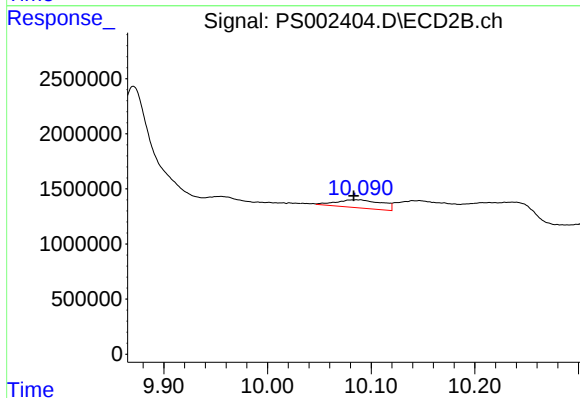


#3 4-Nitrophenol

R.T.: 10.086 min
Delta R.T.: 0.002 min
Response: 2234318
Conc: 12.75 ng/ml

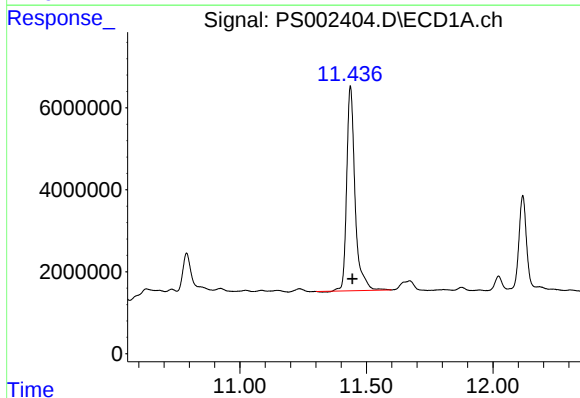


#4 2,4-DCAA

R.T.: 11.437 min
Delta R.T.: -0.007 min
Response: 115191777
Conc: 378.17 ng/ml

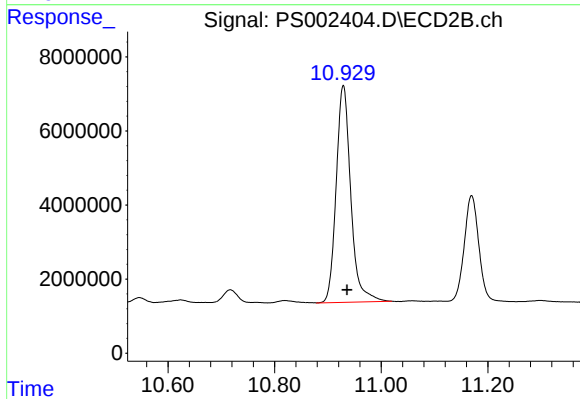

#4 2,4-DCAA


R.T.: 10.929 min
Delta R.T.: -0.007 min
Response: 111493808
Conc: 304.70 ng/ml

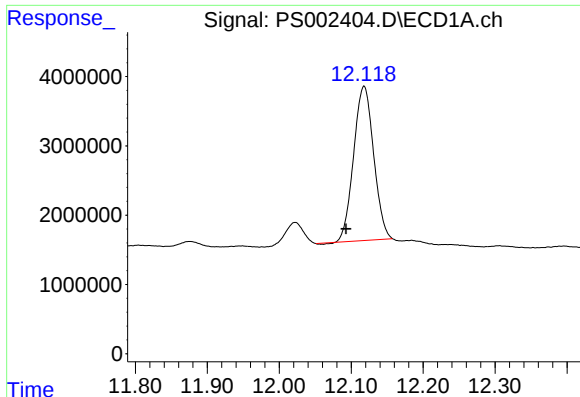

#6 MCP


R.T.: 12.118 min
Delta R.T.: 0.025 min
Response: 43115633
Conc: 45.94 ug/ml

Instrument :
ECD_S
ClientSampleId :

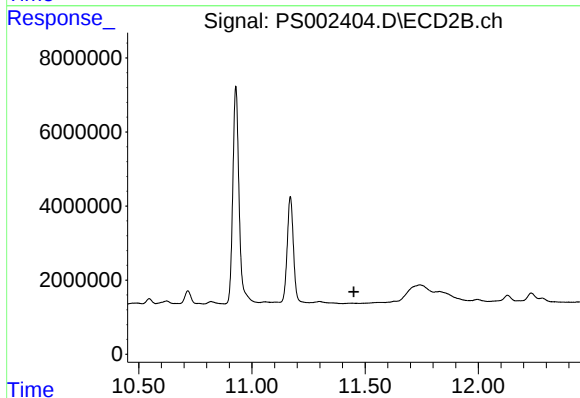


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.450 min
Response: 0
Conc: N.D.

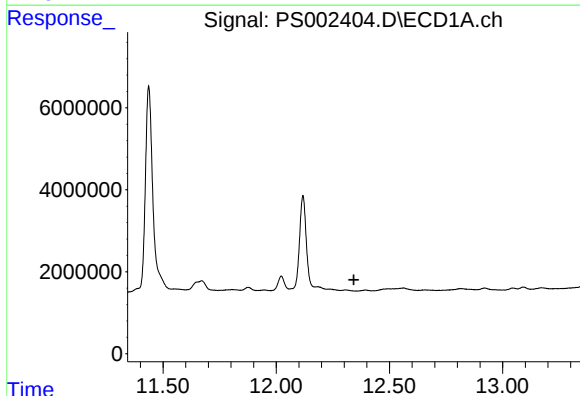


#7 MCP

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

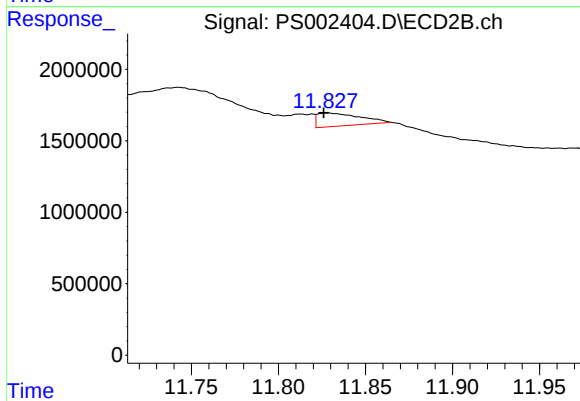

#7 MCP


R.T.: 11.828 min
Delta R.T.: 0.002 min
Response: 1628588
Conc: 1.16 ug/ml

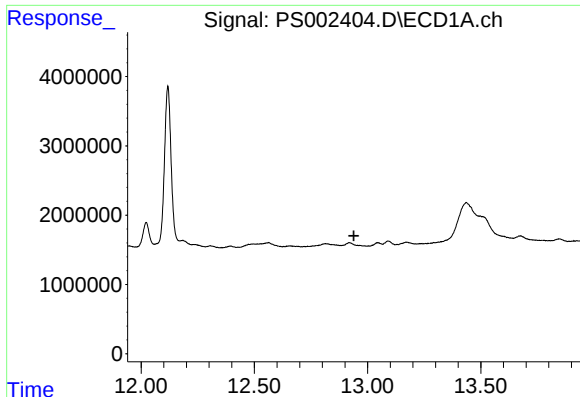

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.939 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

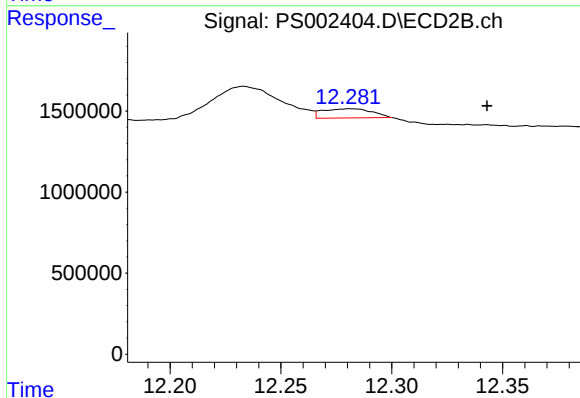


#8 DICHLORPROP

R.T.: 12.281 min
Delta R.T.: -0.062 min
Response: 888632
Conc: 2.68 ng/ml

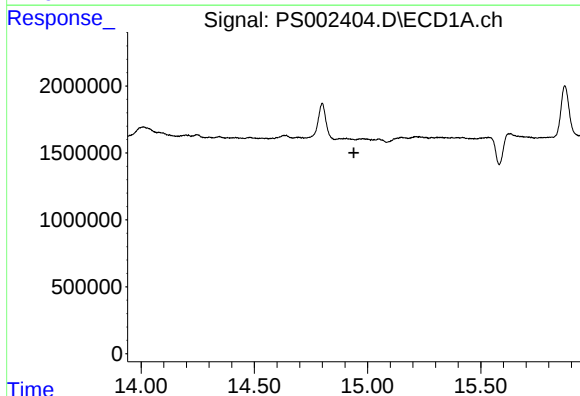


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.940 min
Response: 0
Conc: N.D.

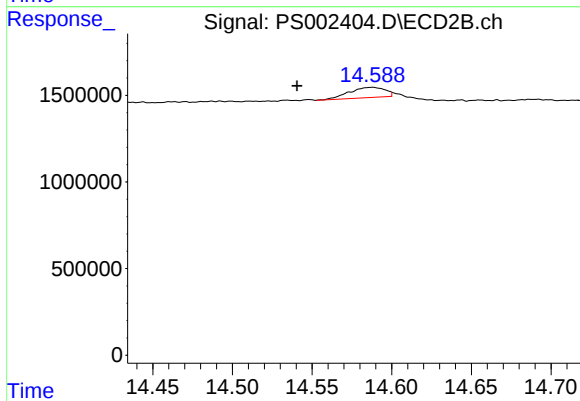

#12 2,4,5-T


R.T.: 14.588 min
Delta R.T.: 0.048 min
Response: 930868
Conc: 0.60 ng/ml

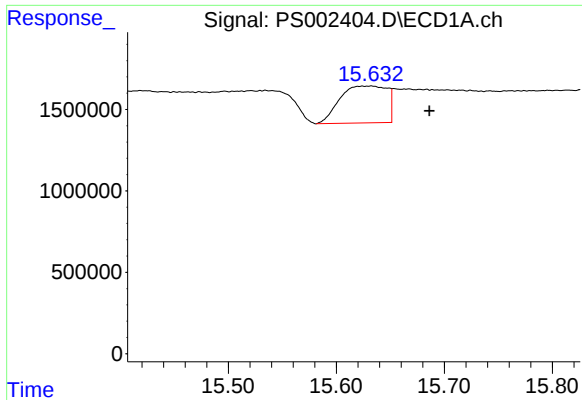

#13 2,4-DB


R.T.: 15.630 min
Delta R.T.: -0.056 min
Response: 6882177
Conc: 35.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

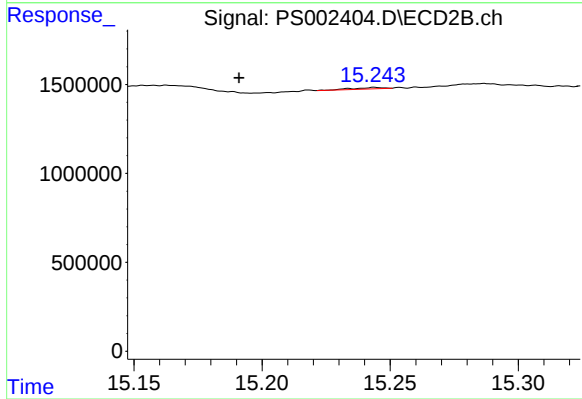


#13 2,4-DB

R.T.: 15.244 min
Delta R.T.: 0.053 min
Response: 63486
Conc: 0.28 ng/ml

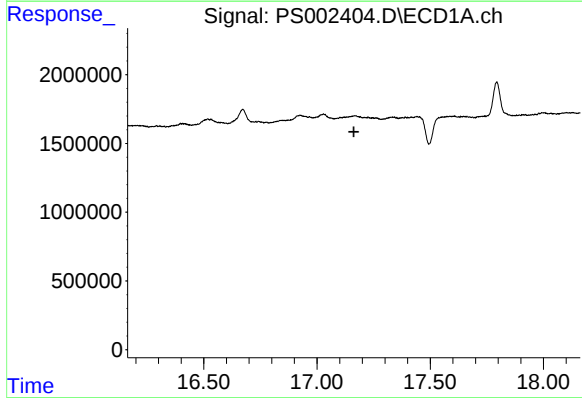


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.163 min
Response: 0
Conc: N.D.

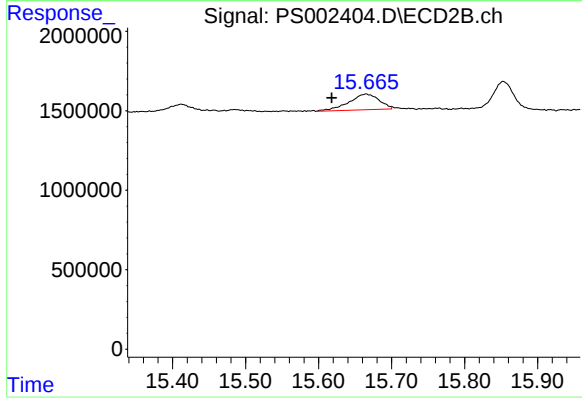

#14 DINOSEB


R.T.: 15.665 min
Delta R.T.: 0.047 min
Response: 2847400
Conc: 1.90 ng/ml

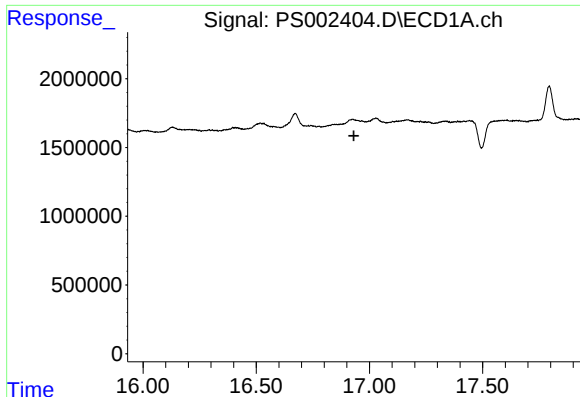

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

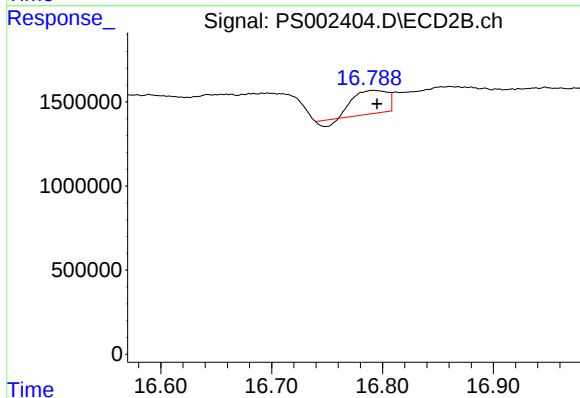


#15 Picloram

R.T.: 16.792 min
Delta R.T.: -0.003 min
Response: 2781244
Conc: 1.05 ng/ml

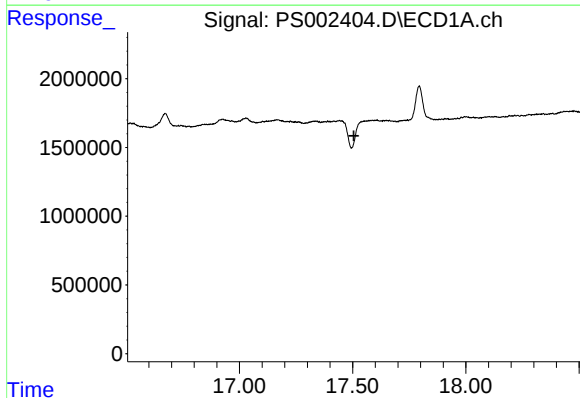

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

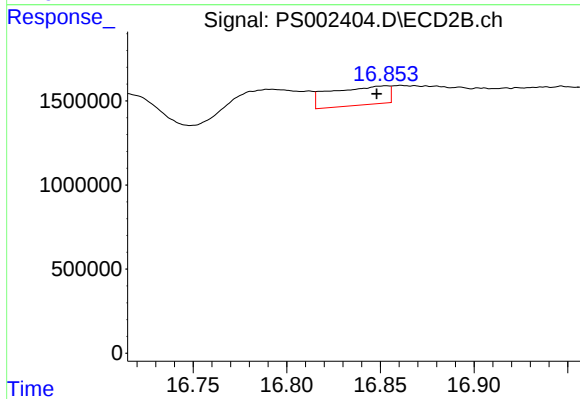

#16 DCPA

R.T.: 16.853 min
Delta R.T.: 0.005 min
Response: 2396256
Conc: 1.00 ng/ml