

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
 Data File : PS002405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2018 02:40
 Operator : EI\SJ
 Sample : J5884-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 10:08:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.433	10.925	101.9E6	97803722	334.557	267.287
Target Compounds							
1) T	Dalapon	0.000	2.358	0	1606046	N.D.	3.732 #
3) T	4-Nitroph...	0.000	10.080	0	486144	N.D.	2.775 #
6) T	MCP	12.113	0.000	31409842	0	33.467	N.D. #
7) T	MCPA	0.000	11.828	0	1356971	N.D.	0.964 #
8) T	DICHLORPROP	0.000	12.278	0	826366	N.D.	2.493 #
9) T	2,4-D	0.000	12.756	0	44742	N.D.	0.112 #
10) T	Pentachlo...	13.665	13.348	3888106	1677076	0.804	0.330 #
12) T	2,4,5-T	0.000	14.578	0	723071	N.D.	0.463 #
14) T	DINOSEB	0.000	15.661	0	2275833	N.D.	1.521 #
15) T	Picloram	0.000	16.797	0	748080	N.D.	0.281 #
16) T	DCPA	0.000	16.851	0	288274	N.D.	0.120 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2018 02:40
Operator : EI\SJ
Sample : J5884-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 10:08:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

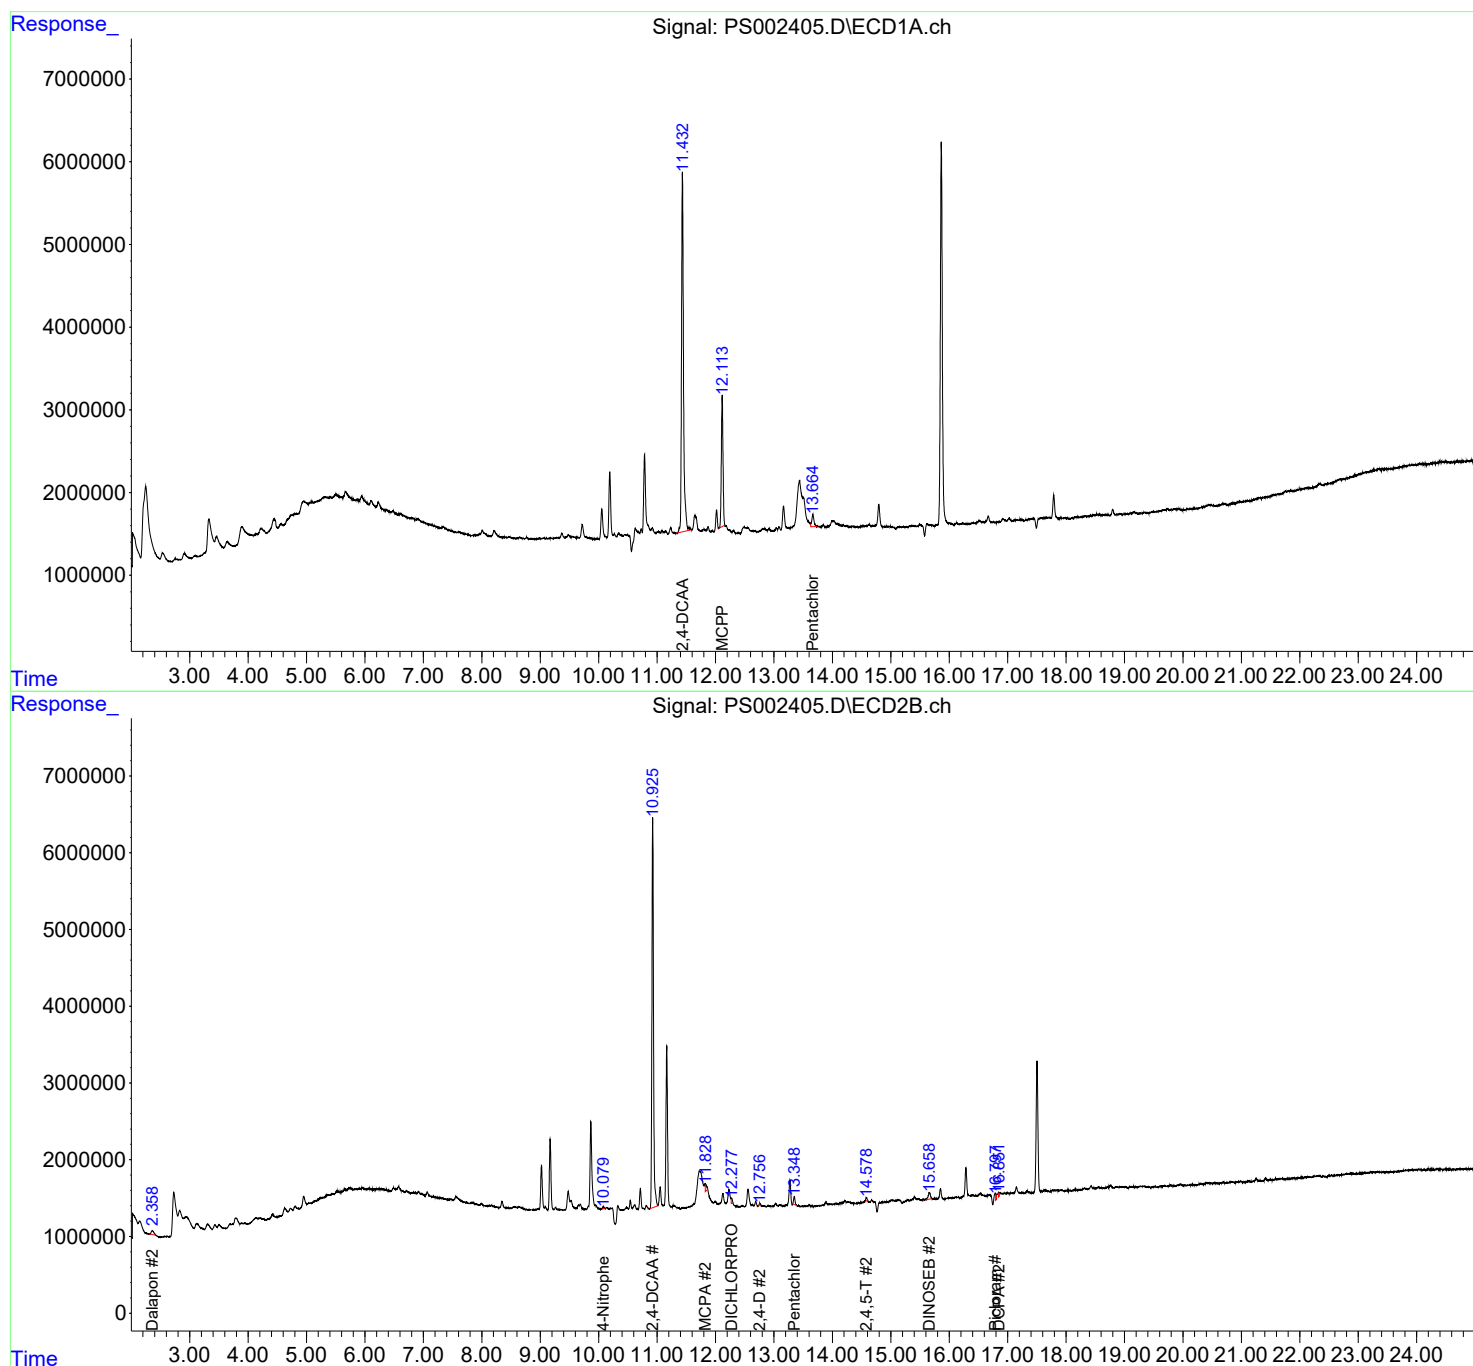


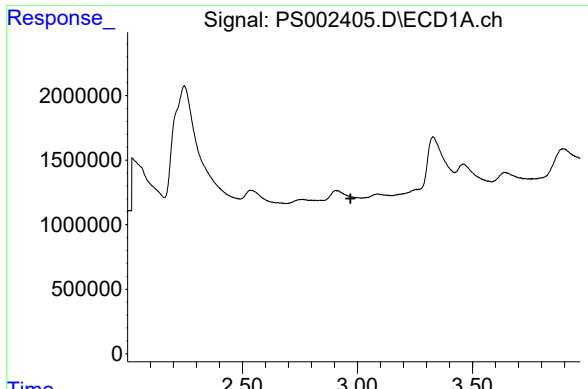

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

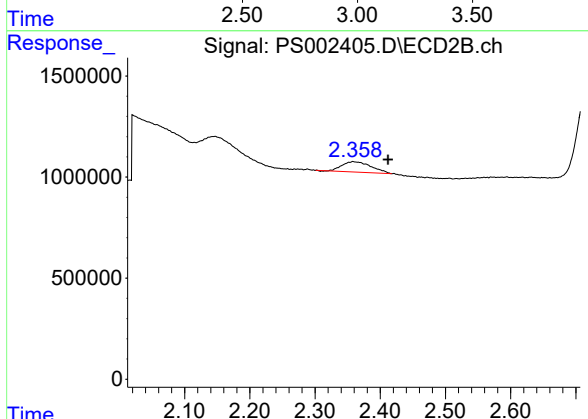


#1 Dalapon

R.T.: 2.358 min
Delta R.T.: -0.054 min
Response: 1606046
Conc: 3.73 ng/ml

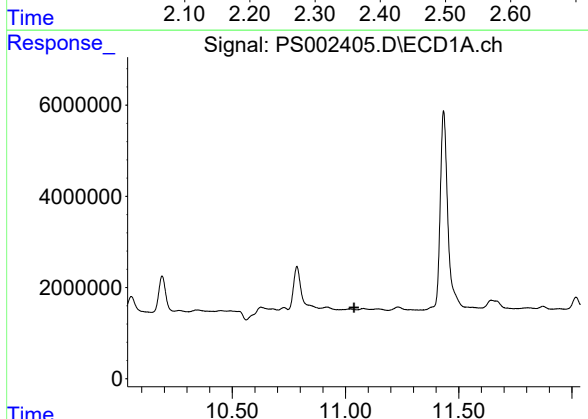


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

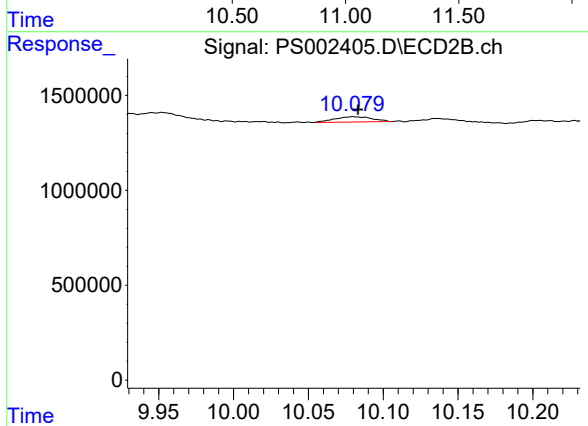

#3 4-Nitrophenol


R.T.: 10.080 min
Delta R.T.: -0.003 min
Response: 486144
Conc: 2.77 ng/ml

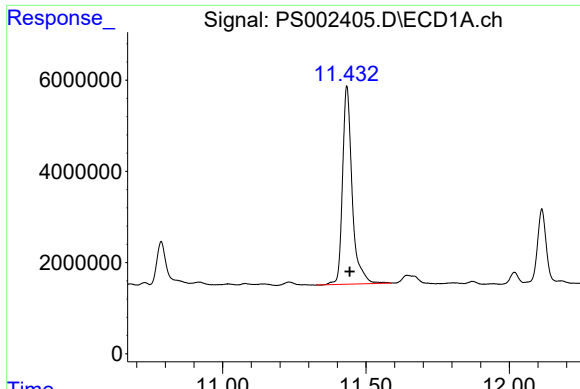

#4 2,4-DCAA


R.T.: 11.433 min
Delta R.T.: -0.011 min
Response: 101905893
Conc: 334.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

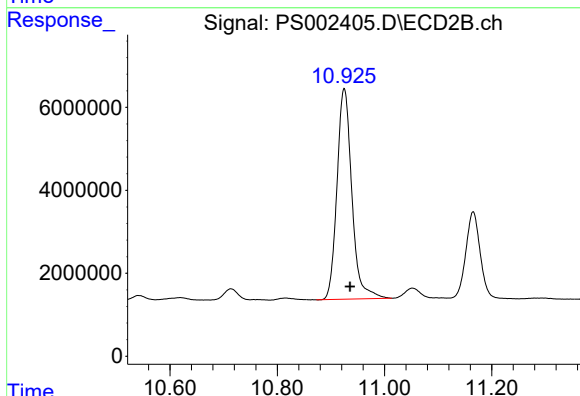


#4 2,4-DCAA

R.T.: 10.925 min
Delta R.T.: -0.011 min
Response: 97803722
Conc: 267.29 ng/ml

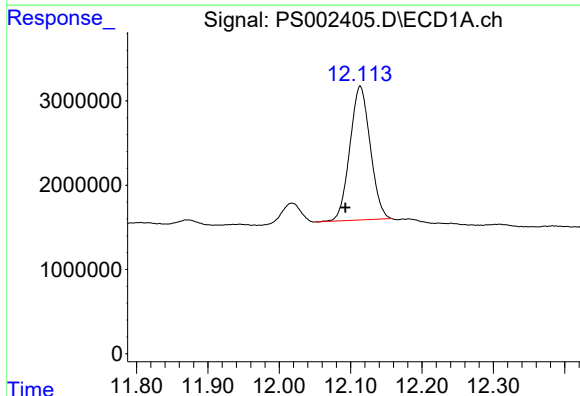


#6 MCP

R.T.: 12.113 min
Delta R.T.: 0.021 min
Response: 31409842
Conc: 33.47 ug/ml

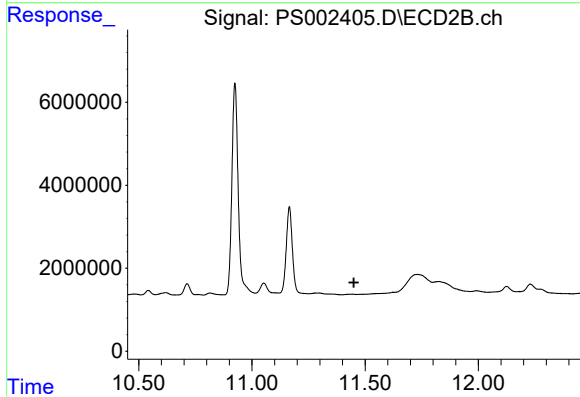

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.450 min
Response: 0
Conc: N.D.

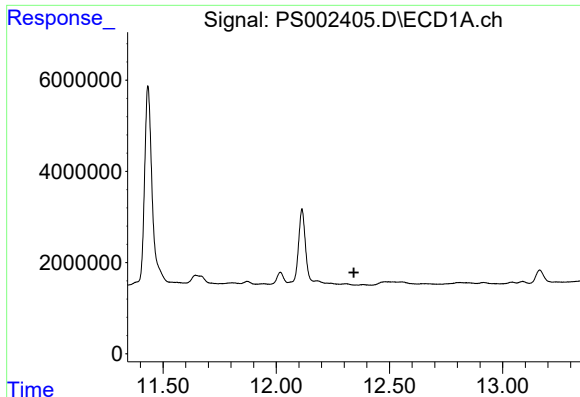

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

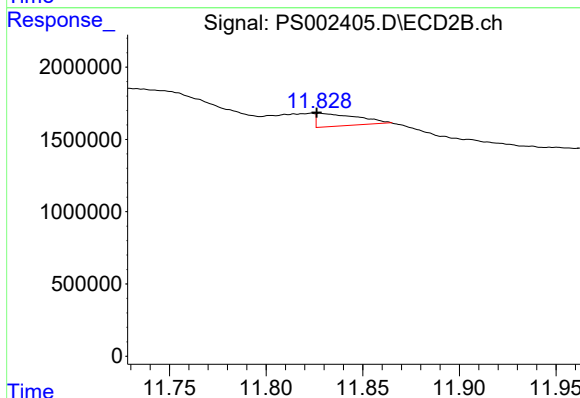


#7 MCPA

R.T.: 11.828 min
Delta R.T.: 0.002 min
Response: 1356971
Conc: 0.96 ug/ml

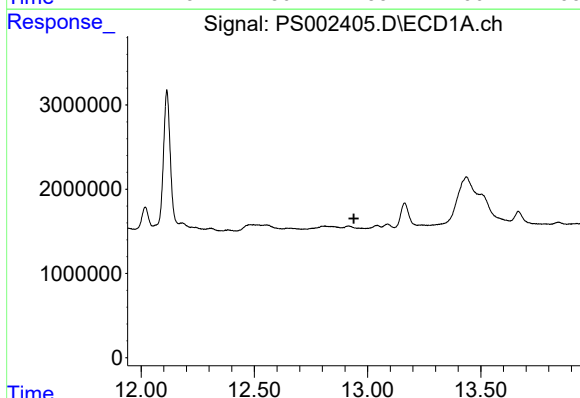


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.939 min
Response: 0
Conc: N.D.

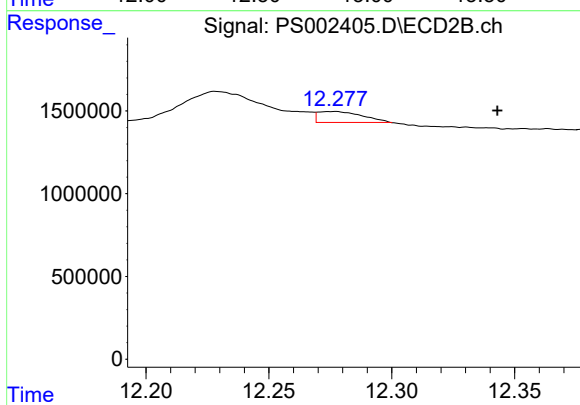

#8 DICHLORPROP


R.T.: 12.278 min
Delta R.T.: -0.065 min
Response: 826366
Conc: 2.49 ng/ml

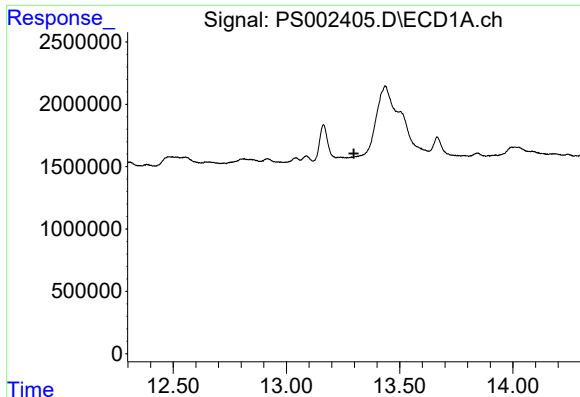

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

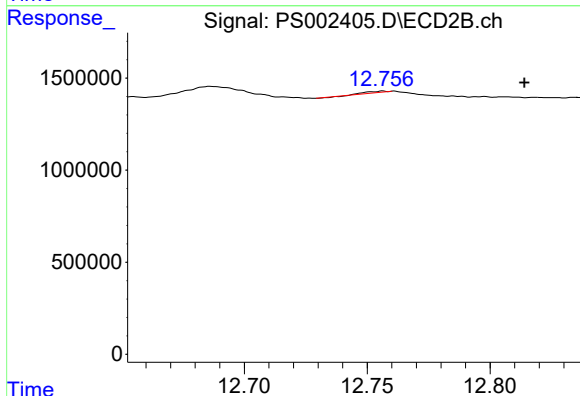


#9 2,4-D

R.T.: 12.756 min
Delta R.T.: -0.057 min
Response: 44742
Conc: 0.11 ng/ml

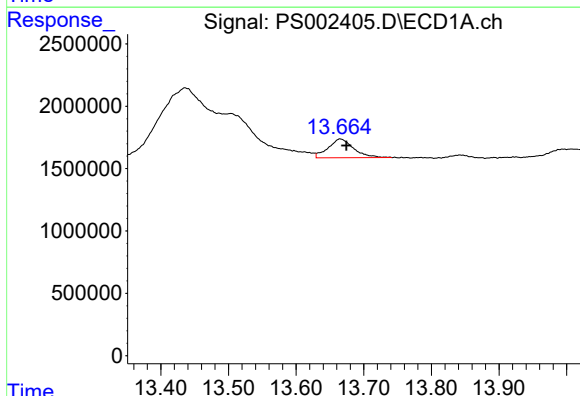


#10 Pentachlorophenol

R.T.: 13.665 min
Delta R.T.: -0.009 min
Response: 3888106
Conc: 0.80 ng/ml

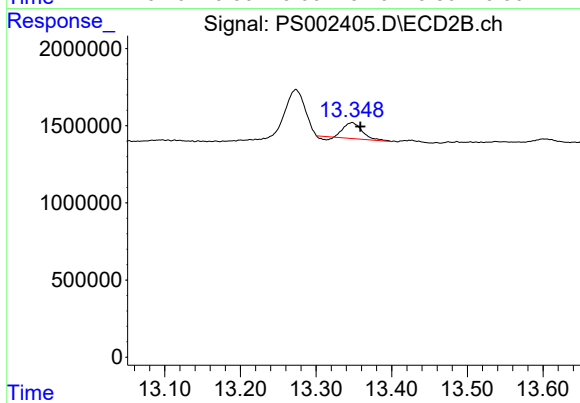

#10 Pentachlorophenol


R.T.: 13.348 min
Delta R.T.: -0.011 min
Response: 1677076
Conc: 0.33 ng/ml

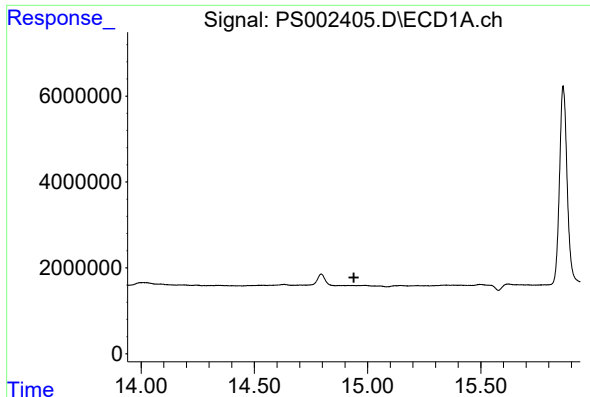

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

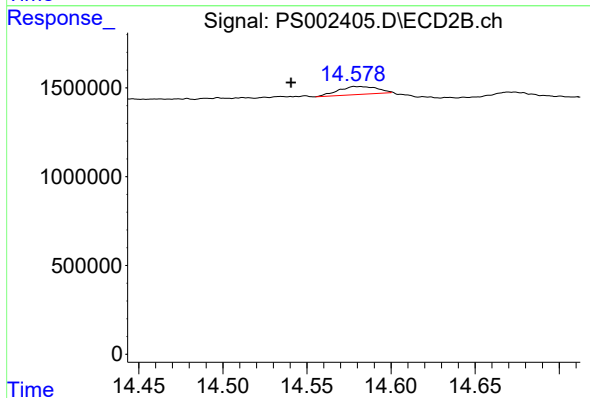


#12 2,4,5-T

R.T.: 14.578 min
Delta R.T.: 0.038 min
Response: 723071
Conc: 0.46 ng/ml

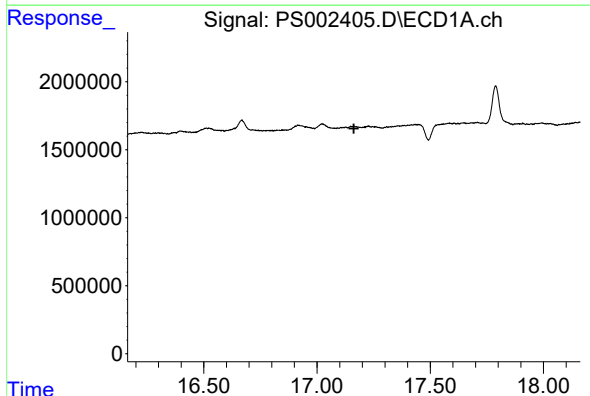


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.163 min
Response: 0
Conc: N.D.

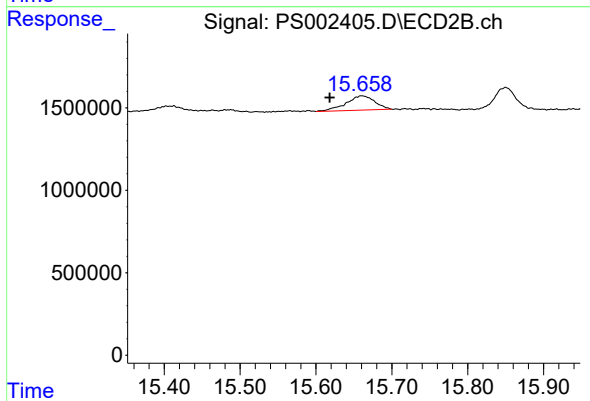

#14 DINOSEB


R.T.: 15.661 min
Delta R.T.: 0.043 min
Response: 2275833
Conc: 1.52 ng/ml

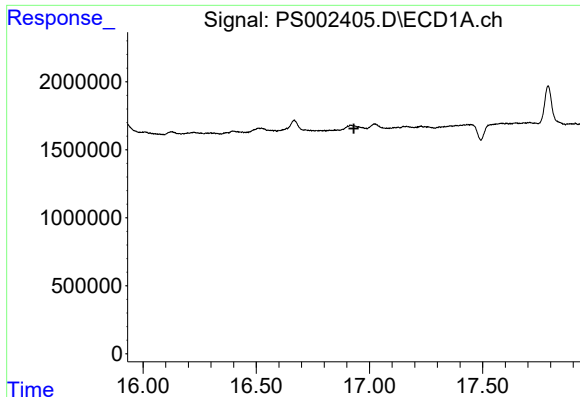

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

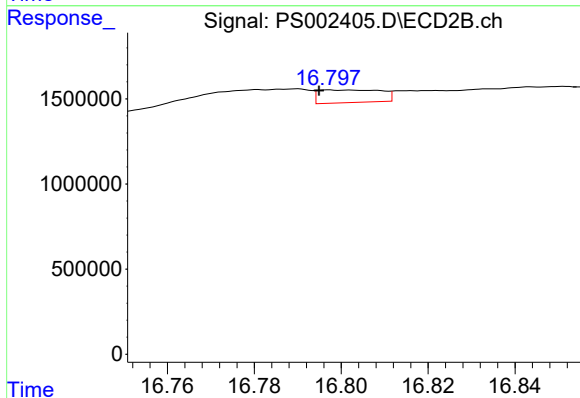


#15 Picloram

R.T.: 16.797 min
Delta R.T.: 0.002 min
Response: 748080
Conc: 0.28 ng/ml

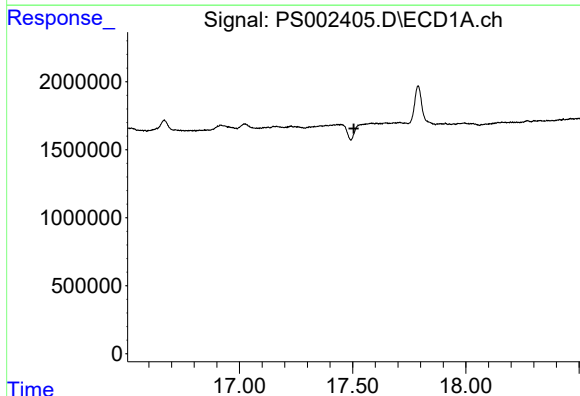

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

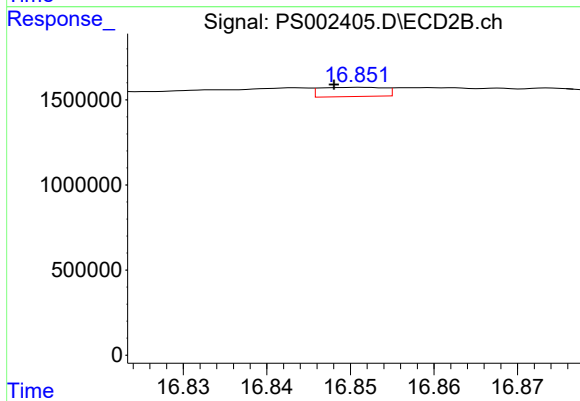

#16 DCPA

R.T.: 16.851 min
Delta R.T.: 0.003 min
Response: 288274
Conc: 0.12 ng/ml