

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110922\
 Data File : PS021083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2022 08:53
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 11:50:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.418	0.000	3386325	0	1.623	N.D.	#
Target Compounds								
1) T	Dalapon	2.514	0.000	390237	0	<MDL	N.D.	#
3) T	4-Nitroph...	6.244	0.000	7712941	0	5.128	N.D.	#
5) T	DICAMBA	6.557	0.000	2663021	0	<MDL	N.D.	#
6) T	MCP	6.745	0.000	4837866	0	<MDL	N.D.	#
7) T	MCPA	6.818	0.000	1775116	0	<MDL	N.D.	#
8) T	DICHLORPROP	0.000	7.659	0	1027187	N.D.	<MDL	
9) T	2,4-D	7.398f	0.000	3916115	0	1.401	N.D.	#
10) T	Pentachlo...	7.588	8.360	1452602	964440	<MDL	<MDL	#
11) T	2,4,5-TP ...	8.119	8.678f	2050142	1151419	<MDL	<MDL	#
12) T	2,4,5-T	8.383	9.154f	862842	4438047	<MDL	<MDL	#
13) T	2,4-DB	8.893	0.000	277840	0	<MDL	N.D.	#
14) T	DINOSEB	9.946	0.000	589406	0	<MDL	N.D.	#
15) T	Picloram	9.791	10.918	30916446	14120287	1.464	1.113	
16) T	DCPA	10.214	10.863	918591	2329316	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110922\
Data File : PS021083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2022 08:53
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 11:50:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

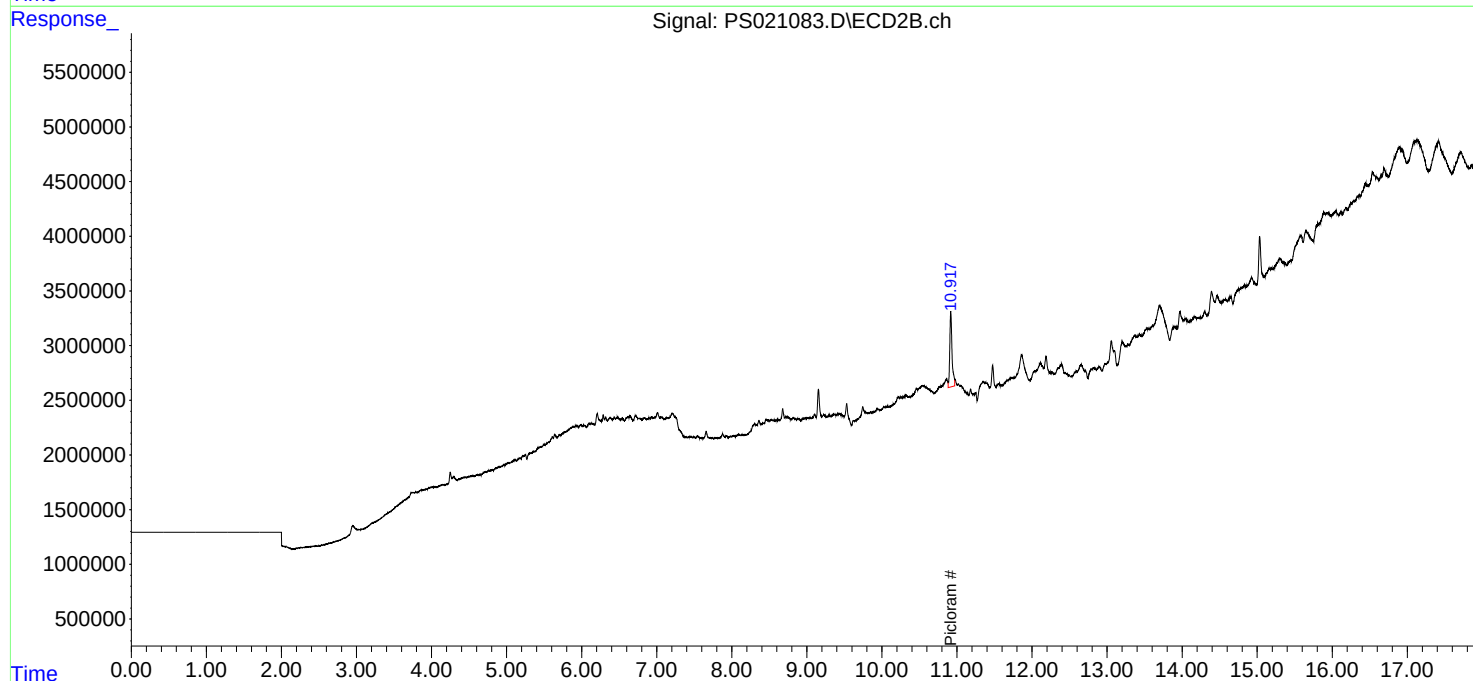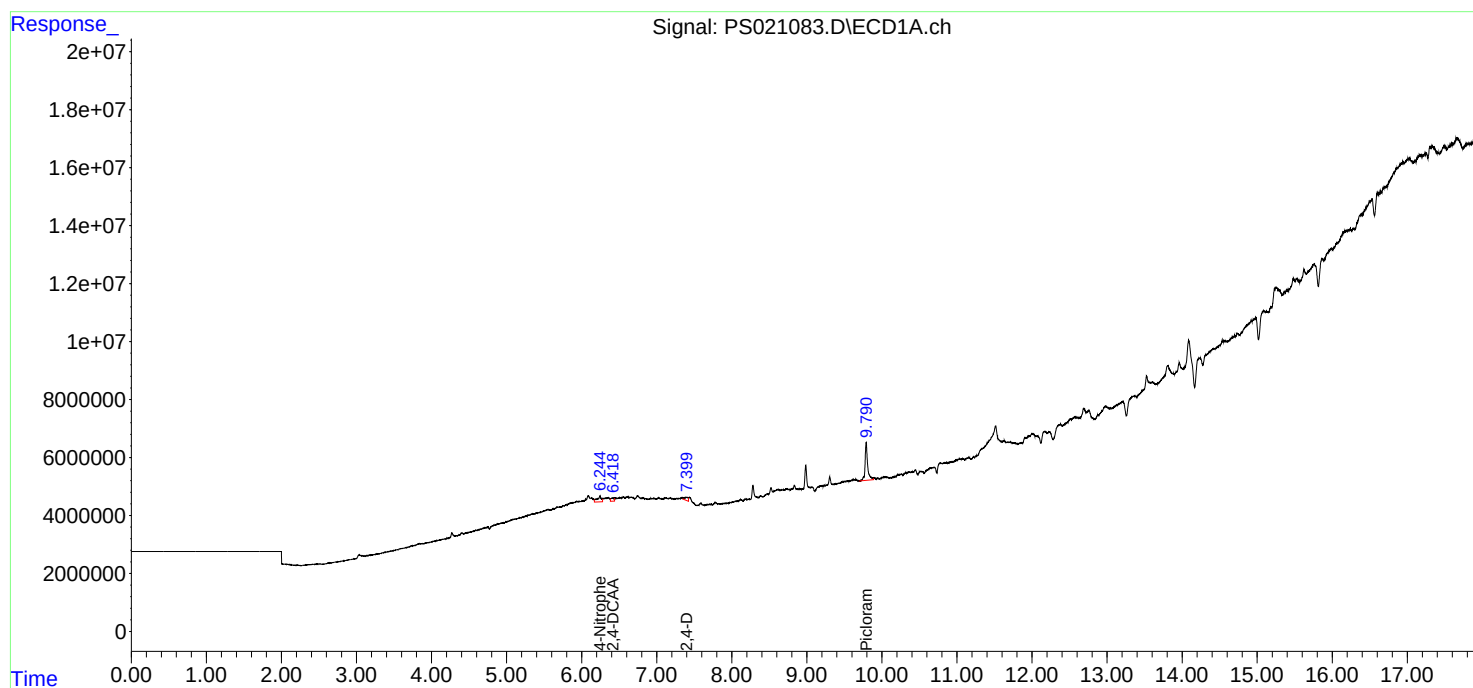


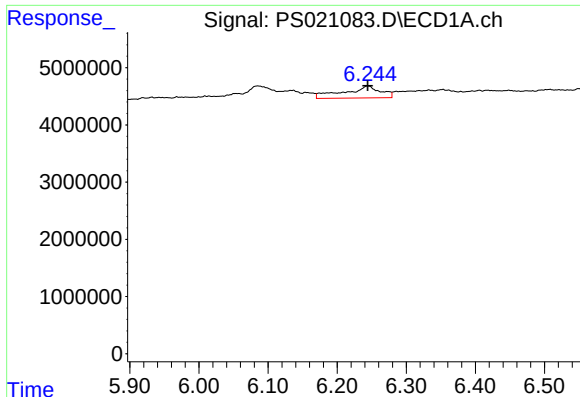

#3 4-Nitrophenol


R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 7712941
Conc: 5.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

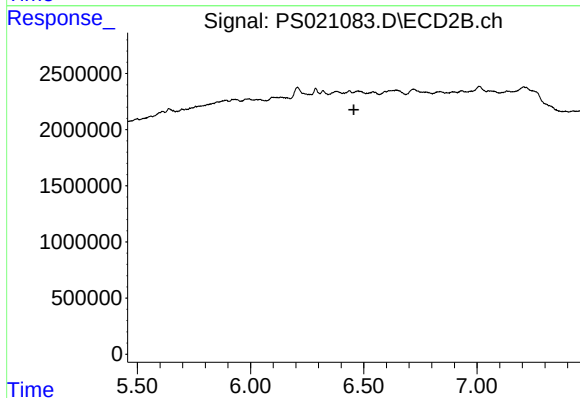


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

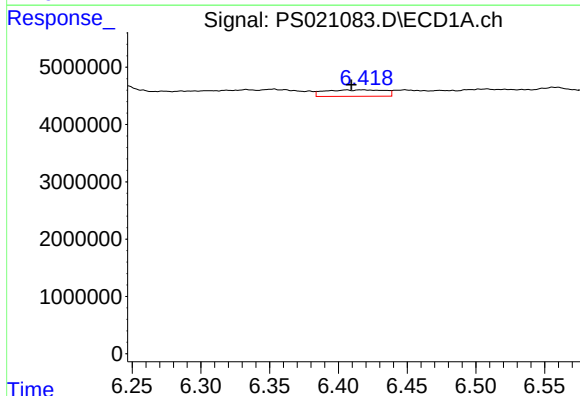


#4 2,4-DCAA

R.T.: 6.418 min
Delta R.T.: 0.009 min
Response: 3386325
Conc: 1.62 ng/ml

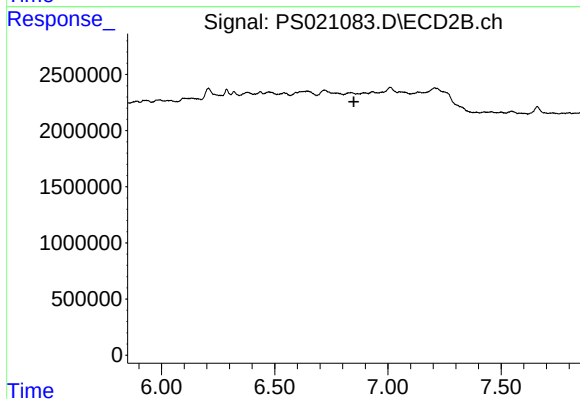

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.

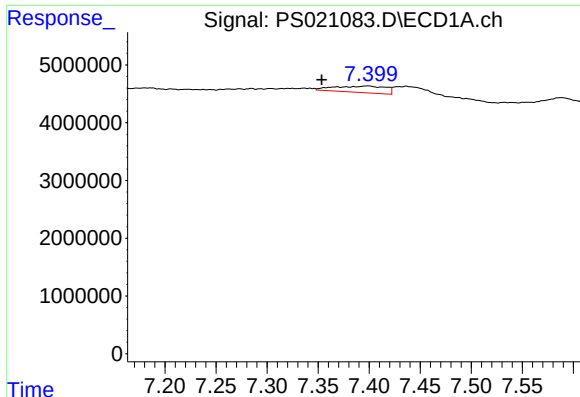

#9 2,4-D


R.T.: 7.398 min
Delta R.T.: 0.045 min
Response: 3916115
Conc: 1.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

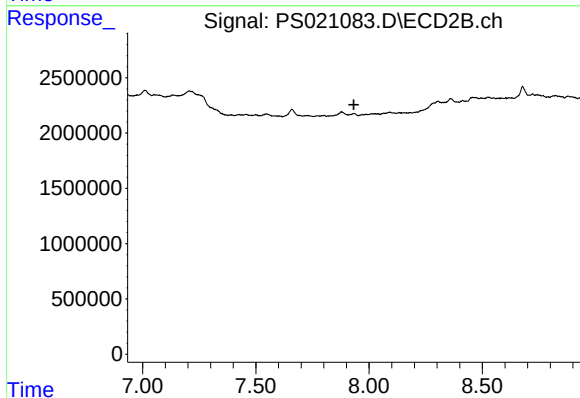


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.933 min
Response: 0
Conc: N.D.

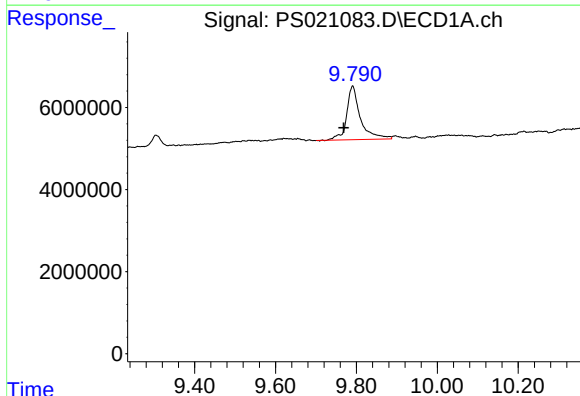

#15 Picloram

R.T.: 9.791 min
Delta R.T.: 0.022 min
Response: 30916446
Conc: 1.46 ng/ml

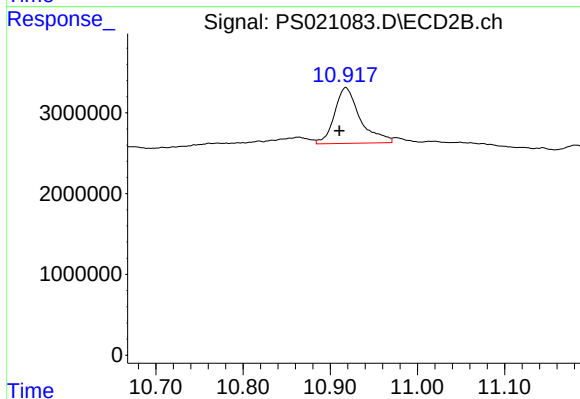

#15 Picloram

R.T.: 10.918 min
Delta R.T.: 0.007 min
Response: 14120287
Conc: 1.11 ng/ml