

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110922\
 Data File : PS021084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2022 09:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 11:51:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.410	6.846	1147.7E6	791.8E6	549.901	572.497
Target Compounds							
1) T	Dalapon	2.512	0.000	252753	0	<MDL	N.D. #
3) T	4-Nitroph...	6.251	0.000	4828078	0	3.210	N.D. #
6) T	MCP	6.784f	0.000	13175912	0	2.019	N.D. #
7) T	MCPA	6.784f	0.000	13175912	0	1.404	N.D. #
8) T	DICHLORPROP	7.223f	7.670	454126	1633445	<MDL	1.061 #
9) T	2,4-D	7.337	0.000	303273	0	<MDL	N.D. #
10) T	Pentachlo...	7.582	0.000	1159961	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.120	8.692	2909601	1189733	<MDL	<MDL #
12) T	2,4,5-T	8.328f	0.000	9280785	0	<MDL	N.D. #
13) T	2,4-DB	8.865	9.547f	2364516	4777325	<MDL	4.292 #
15) T	Picloram	9.766	10.966f	2166568	8701048	<MDL	<MDL #
16) T	DCPA	10.202	0.000	706799	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110922\
Data File : PS021084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2022 09:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 11:51:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

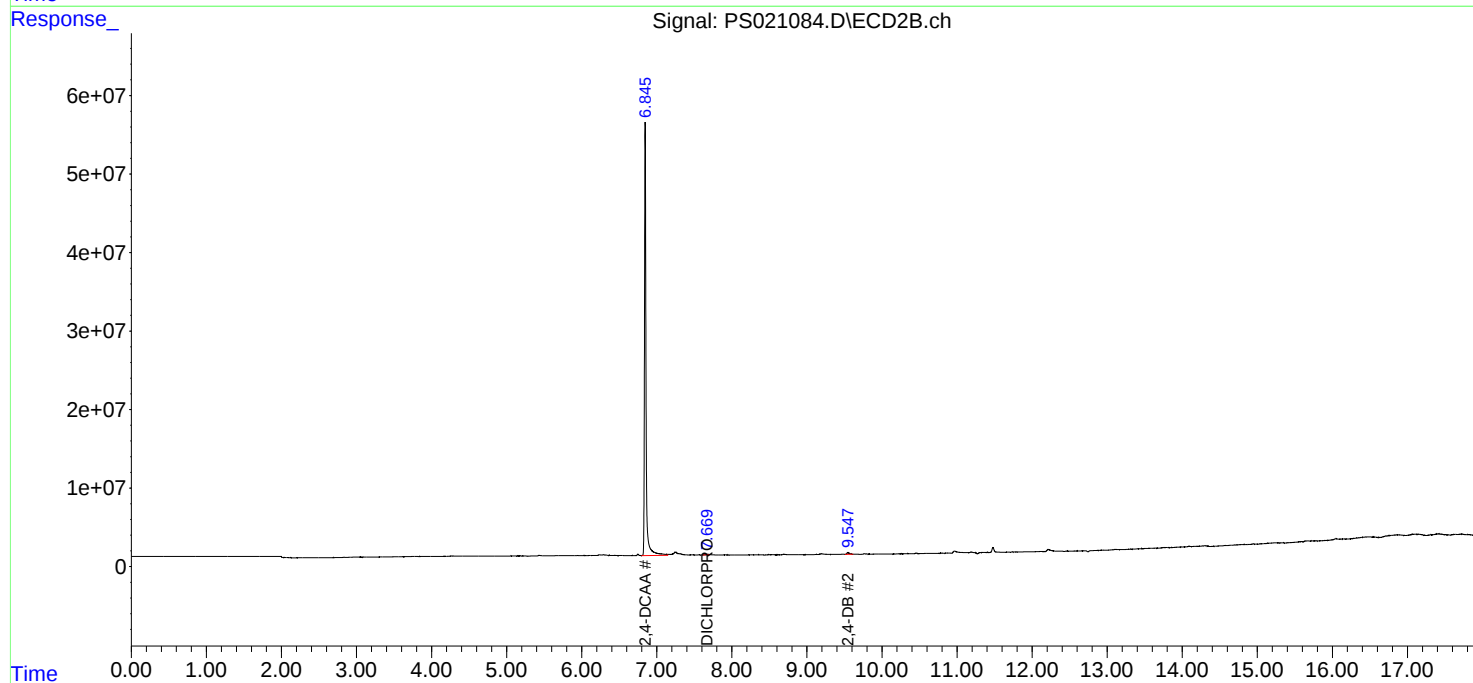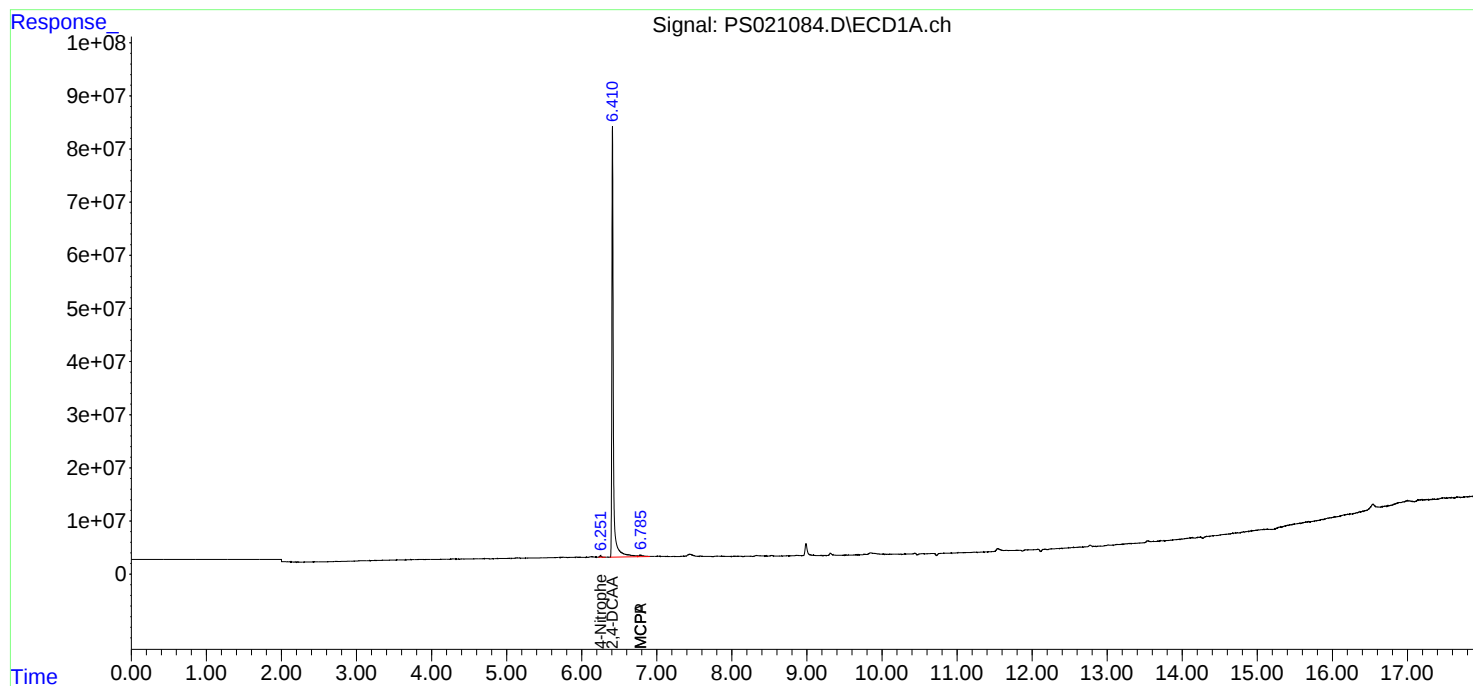


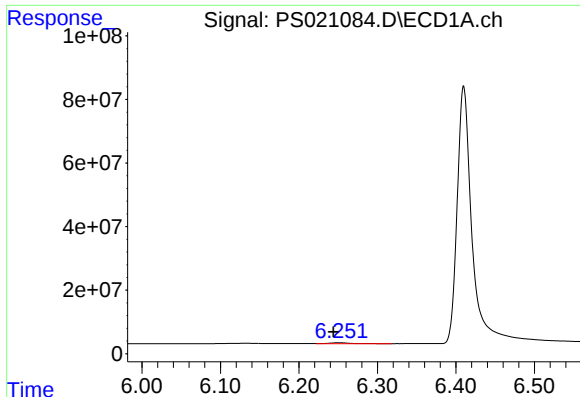

#3 4-Nitrophenol


R.T.: 6.251 min
Delta R.T.: 0.007 min
Response: 4828078
Conc: 3.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

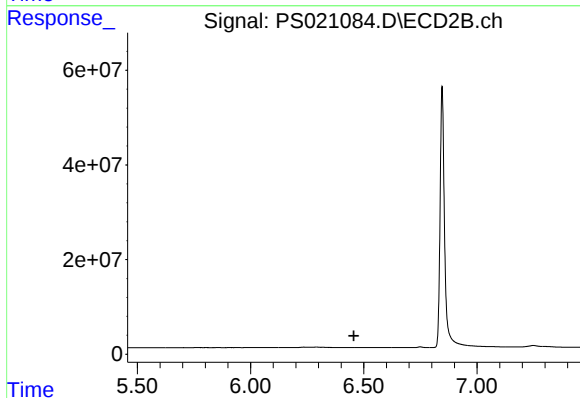


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

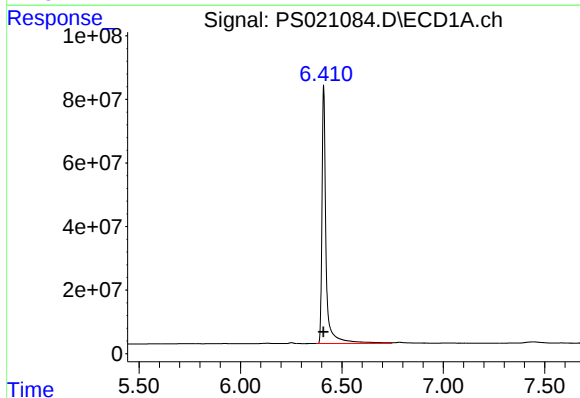


#4 2,4-DCAA

R.T.: 6.410 min
Delta R.T.: 0.000 min
Response: 1147685865
Conc: 549.90 ng/ml

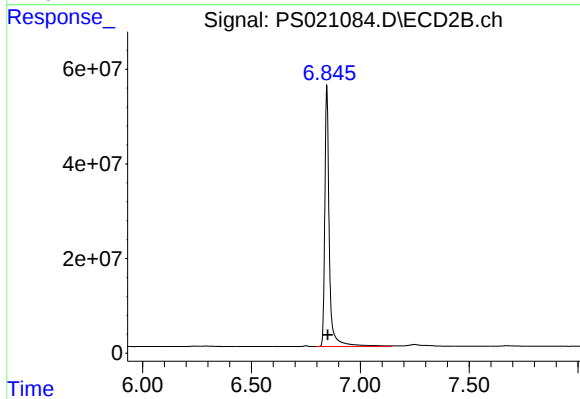

#4 2,4-DCAA


R.T.: 6.846 min
Delta R.T.: -0.004 min
Response: 791846064
Conc: 572.50 ng/ml

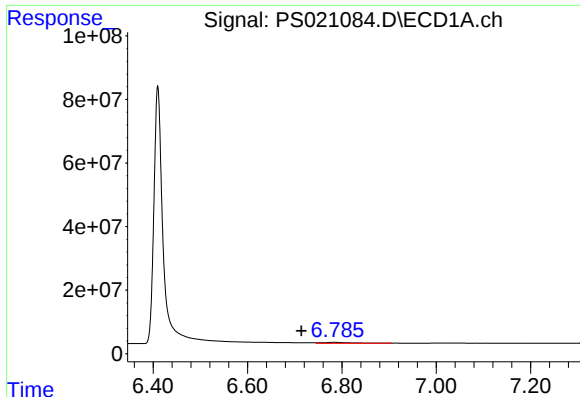

#6 MCPP


R.T.: 6.784 min
Delta R.T.: 0.069 min
Response: 13175912
Conc: 2.02 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

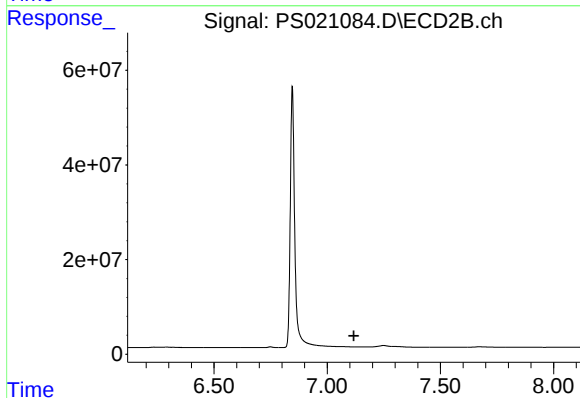


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.118 min
Response: 0
Conc: N.D.

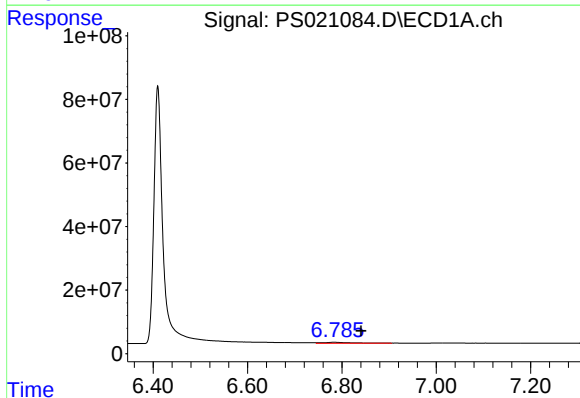


#7 MCPA

R.T.: 6.784 min
Delta R.T.: -0.057 min
Response: 13175912
Conc: 1.40 ug/ml

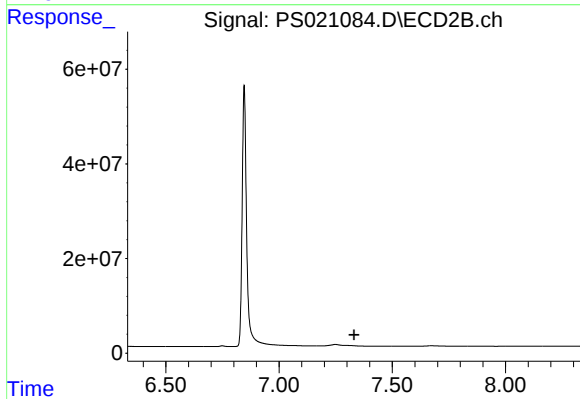

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.331 min
Response: 0
Conc: N.D.

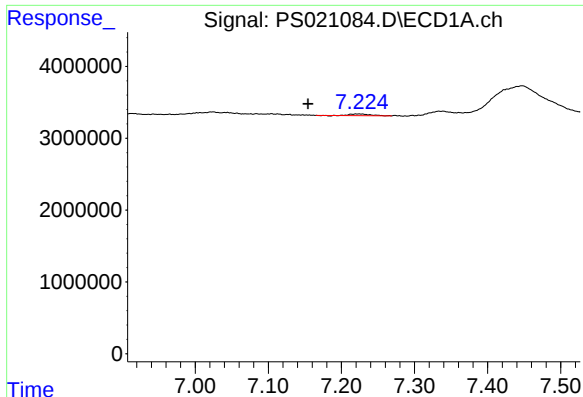

#8 DICHLORPROP


R.T.: 7.223 min
Delta R.T.: 0.069 min
Response: 454126
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

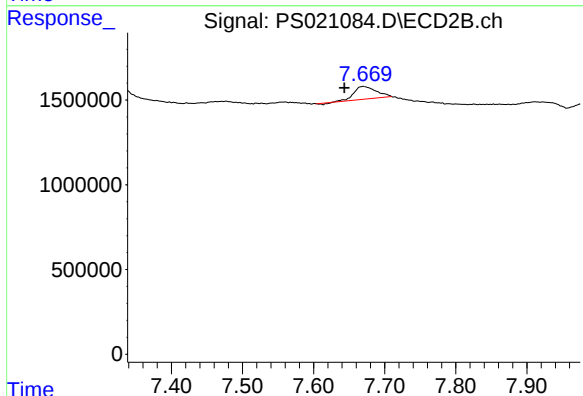


#8 DICHLORPROP

R.T.: 7.670 min
Delta R.T.: 0.027 min
Response: 1633445
Conc: 1.06 ng/ml

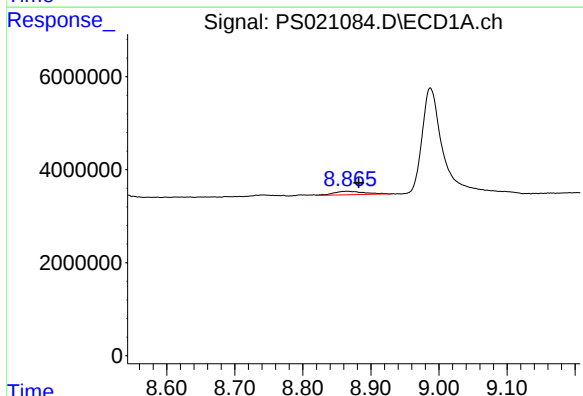

#13 2,4-DB

R.T.: 8.865 min
Delta R.T.: -0.017 min
Response: 2364516
Conc: N.D.

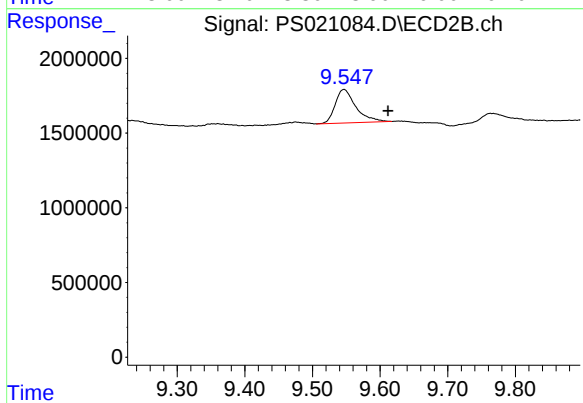

#13 2,4-DB

R.T.: 9.547 min
Delta R.T.: -0.065 min
Response: 4777325
Conc: 4.29 ng/ml