

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110922\
 Data File : PS021094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2022 14:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 20:51:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.409	6.846	1136.9E6	779.3E6	544.752	563.433
Target Compounds							
1) T	Dalapon	2.535	0.000	1152539	0	<MDL	N.D. #
3) T	4-Nitroph...	6.250	0.000	5547238	0	3.688	N.D. #
5) T	DICAMBA	0.000	7.054	0	1847120	N.D.	<MDL
6) T	MCP	6.677	7.054f	4804457	1847120	<MDL	<MDL #
7) T	MCPA	6.895f	0.000	389934	0	<MDL	N.D. #
8) T	DICHLORPROP	7.093f	7.674	231792	4149957	<MDL	2.695 #
9) T	2,4-D	7.335	0.000	99164	0	<MDL	N.D. #
10) T	Pentachlo...	7.583	8.360	795760	558185	<MDL	<MDL #
11) T	2,4,5-TP ...	8.127	8.691	2862090	5732008	<MDL	<MDL #
12) T	2,4,5-T	8.399	9.121	1145194	795749	<MDL	<MDL #
13) T	2,4-DB	8.901	9.634	358164	1019454	<MDL	<MDL #
14) T	DINOSEB	9.903f	0.000	6956436	0	<MDL	N.D. #
15) T	Picloram	9.764	10.888	3430034	5433365	<MDL	<MDL #
16) T	DCPA	10.209	10.888	1210185	5433365	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110922\
Data File : PS021094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2022 14:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 20:51:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

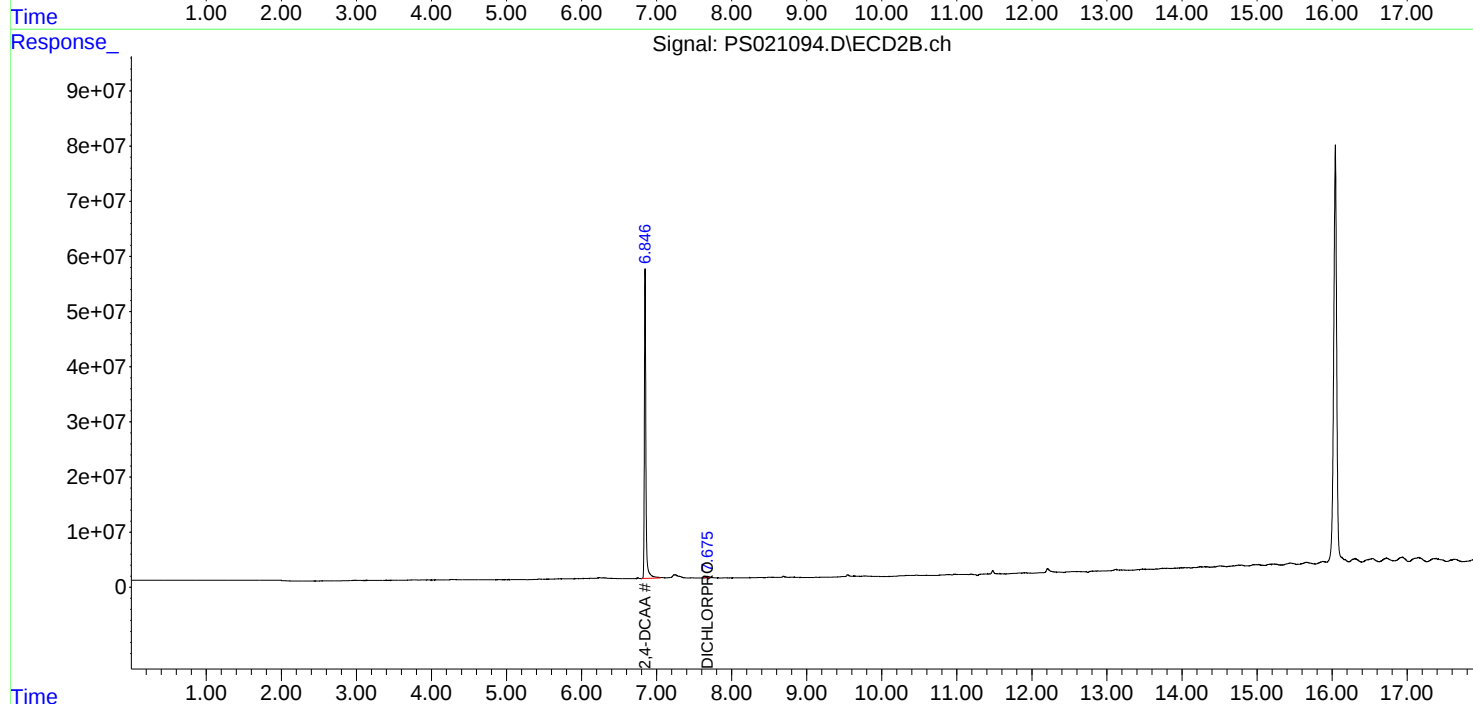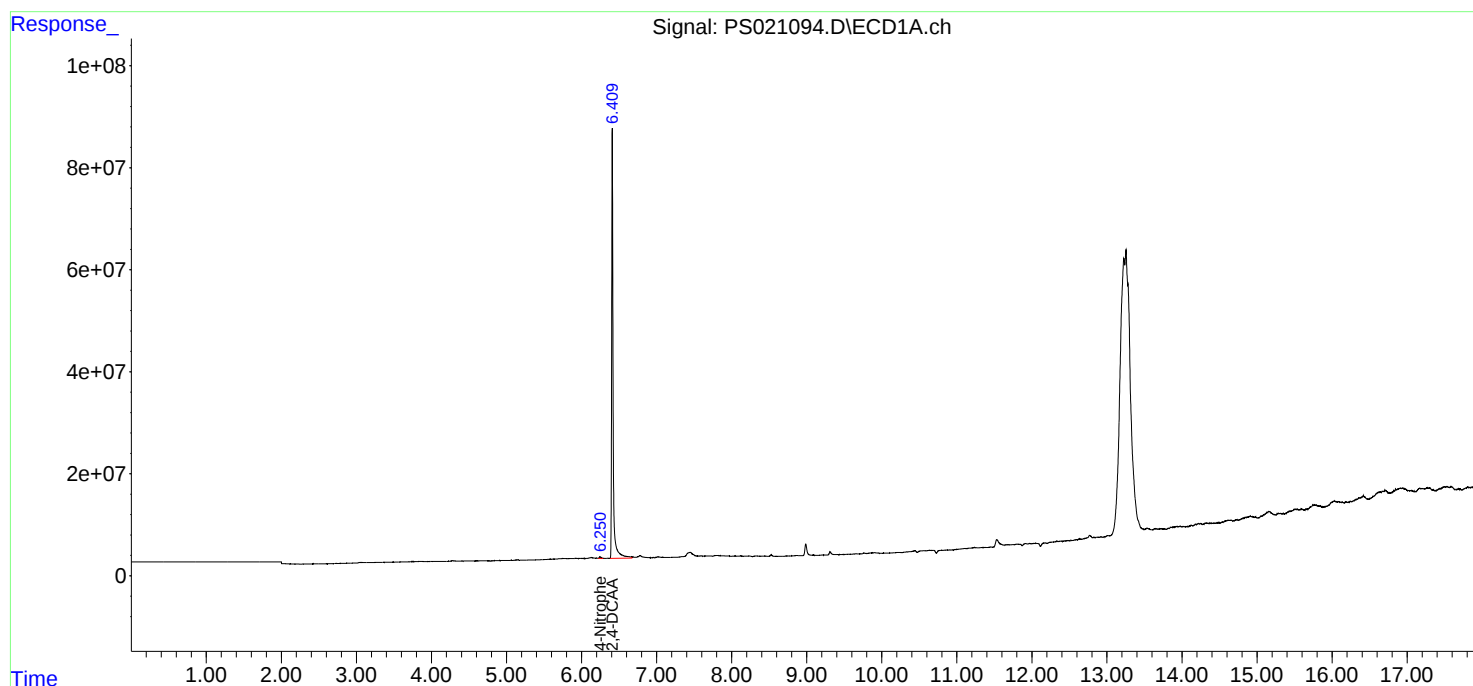


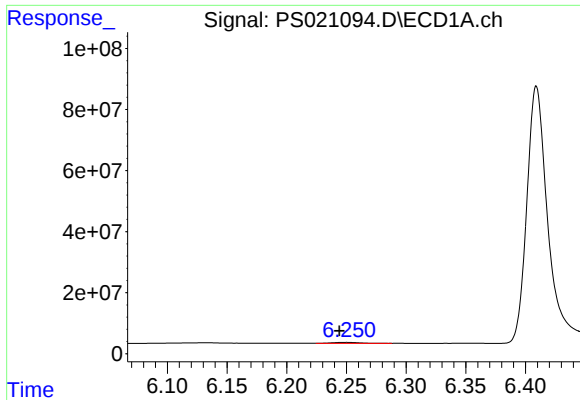

#3 4-Nitrophenol


R.T.: 6.250 min
Delta R.T.: 0.006 min
Response: 5547238
Conc: 3.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

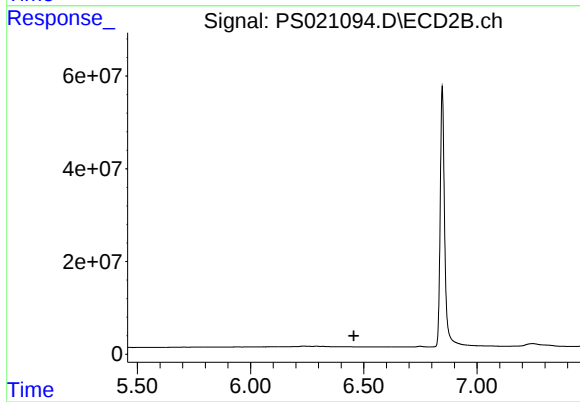


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

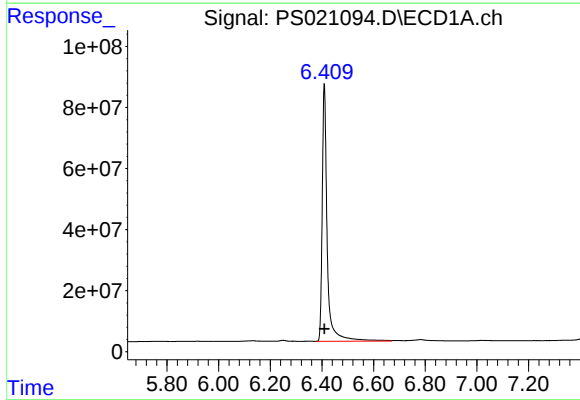


#4 2,4-DCAA

R.T.: 6.409 min
Delta R.T.: 0.000 min
Response: 1136938376
Conc: 544.75 ng/ml

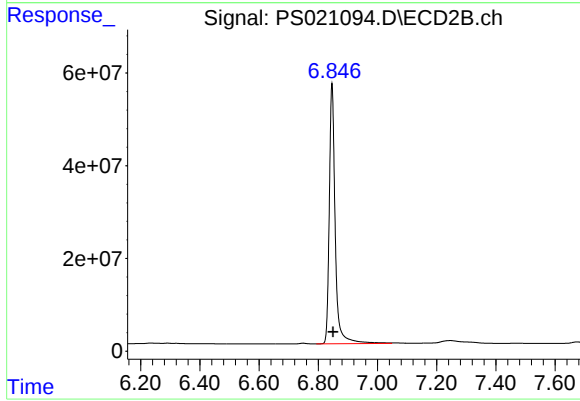

#4 2,4-DCAA


R.T.: 6.846 min
Delta R.T.: -0.003 min
Response: 779309389
Conc: 563.43 ng/ml

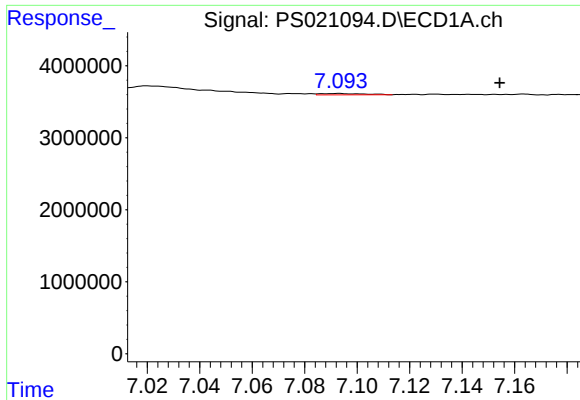

#8 DICHLORPROP

R.T.: 7.093 min
Delta R.T.: -0.062 min
Response: 231792
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

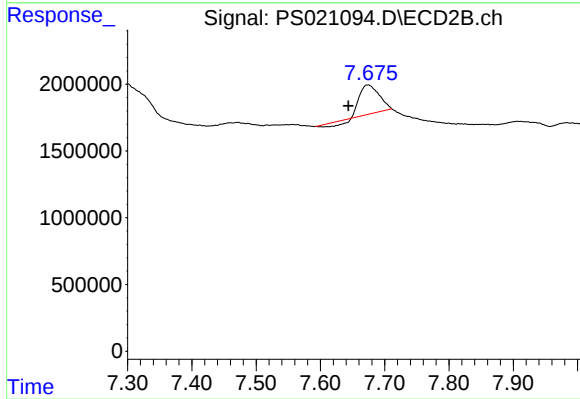

#8 DICHLORPROP

R.T.: 7.674 min
Delta R.T.: 0.031 min
Response: 4149957
Conc: 2.70 ng/ml