

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110924\
 Data File : PS028378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2024 00:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 01:12:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 08 17:46:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	7.753	1363.1E6	775.4E6	493.757	486.655
Target Compounds							
2) T	3,5-DICHL...	6.406	0.000	94066	0	<MDL	N.D. #
3) T	4-Nitroph...	7.039	0.000	7372685	0	3.976	N.D. #
6) T	MCP	7.674f	0.000	24535273	0	3.000	N.D. #
7) T	MCPA	0.000	8.272f	0	10141169	N.D.	1.266
8) T	DICHLORPROP	8.101f	8.723f	1080578	12971604	<MDL	7.282 #
10) T	Pentachlo...	8.719f	0.000	1086757	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.309f	9.941f	4983963	5463391	<MDL	<MDL #
12) T	2,4,5-T	9.557	0.000	1322032	0	<MDL	N.D. #
14) T	DINOSEB	11.362	0.000	1964554	0	<MDL	N.D. #
15) T	Picloram	11.147	12.376	10523078	9878474	<MDL	<MDL #
16) T	DCPA	0.000	12.376f	0	9878474	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110924\
Data File : PS028378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2024 00:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 01:12:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
Quant Title : 8080.M
QLast Update : Fri Nov 08 17:46:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

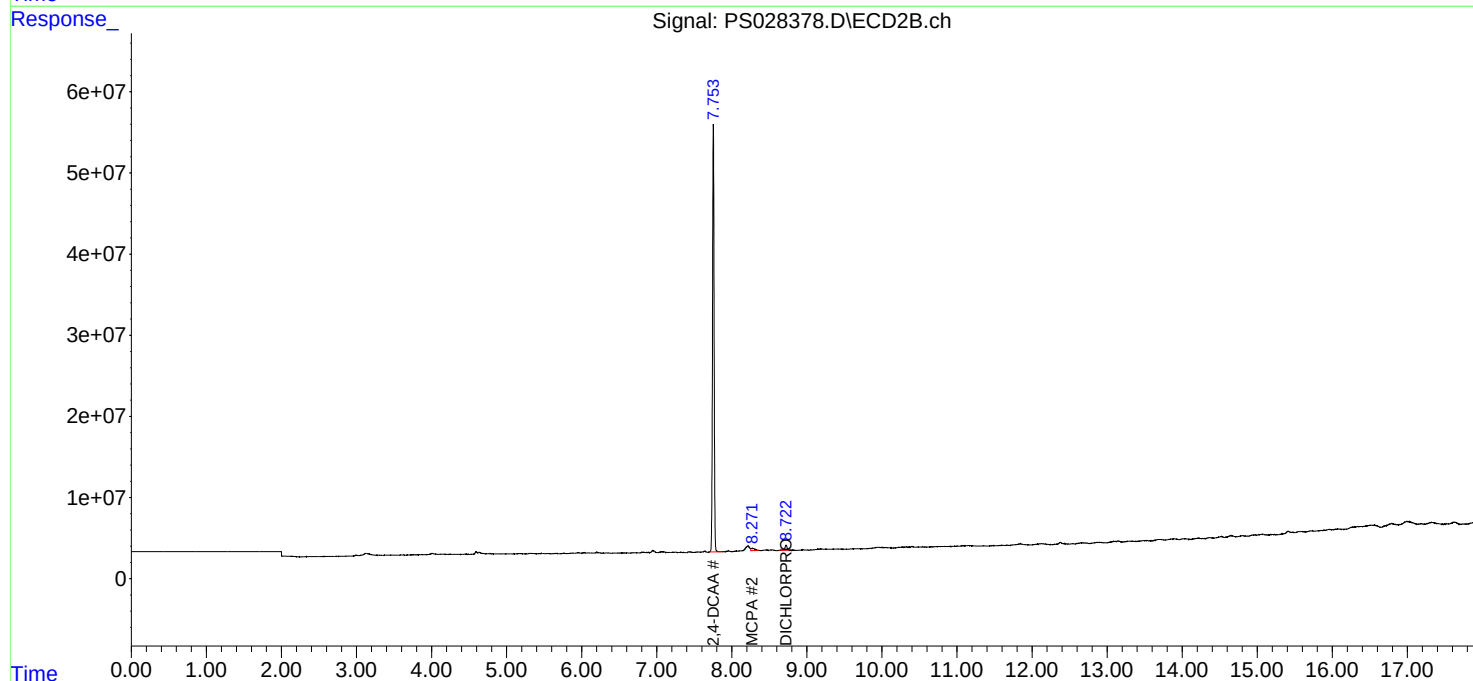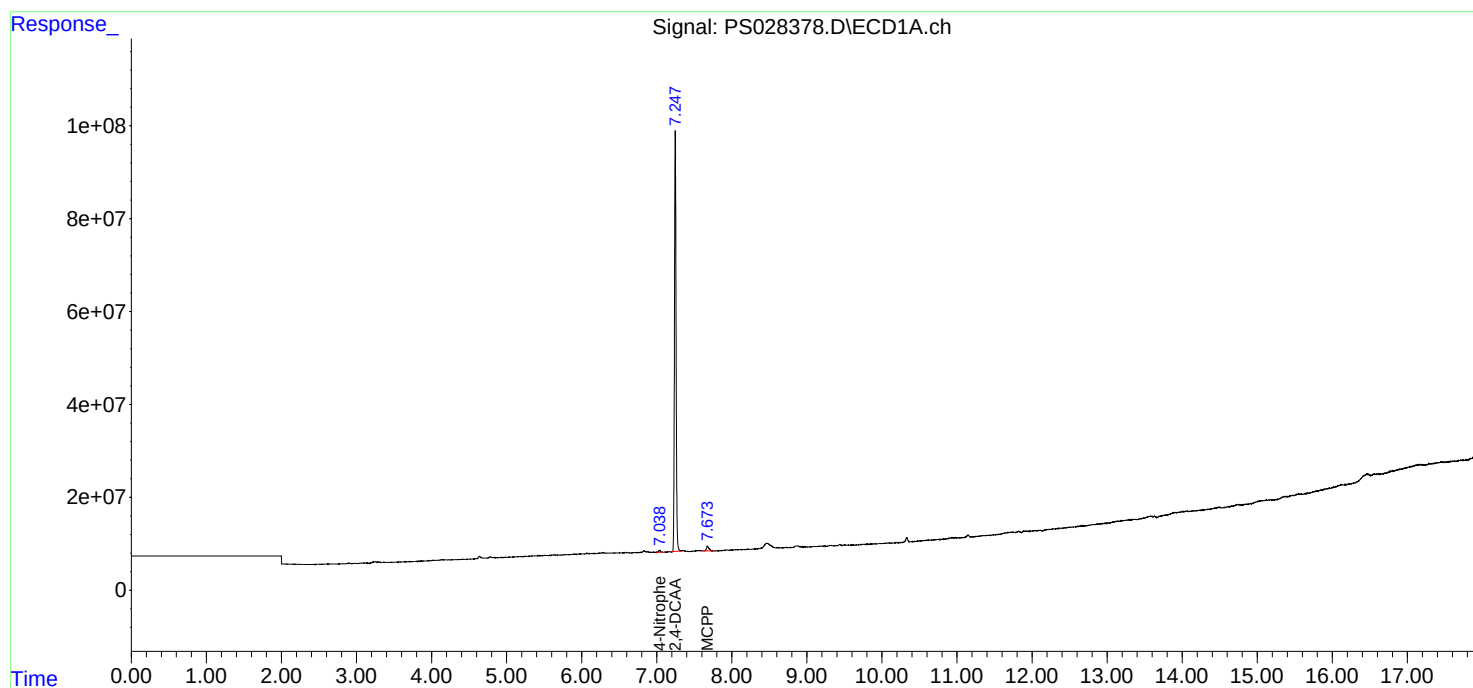


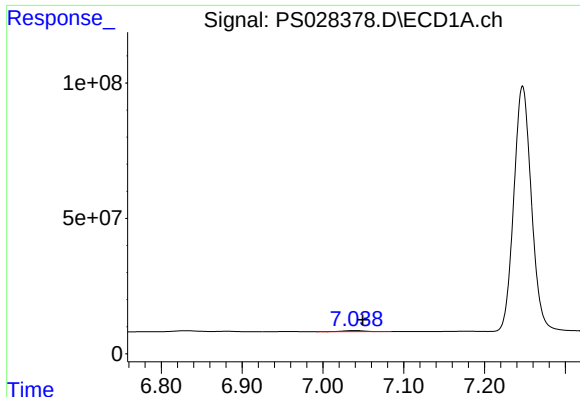

#3 4-Nitrophenol


R.T.: 7.039 min
Delta R.T.: -0.010 min
Response: 7372685
Conc: 3.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

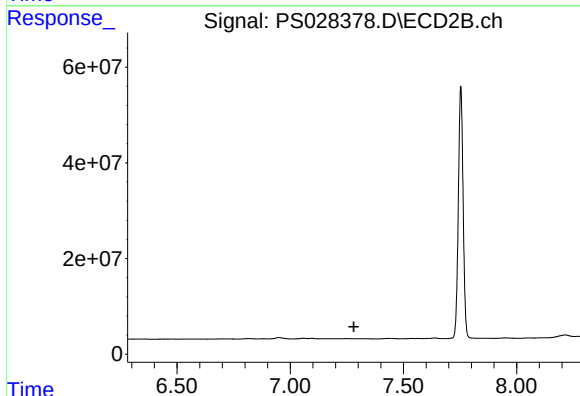


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.281 min
Response: 0
Conc: N.D.

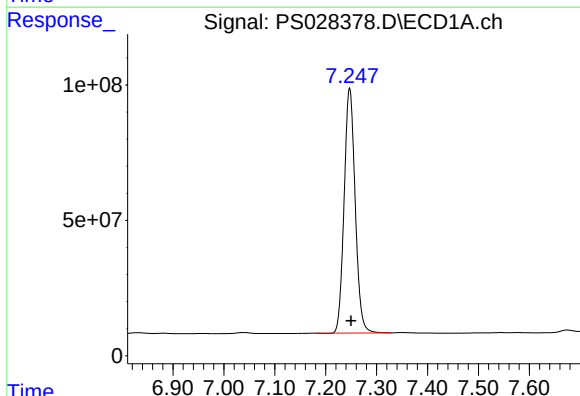


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: -0.003 min
Response: 1363140651
Conc: 493.76 ng/ml

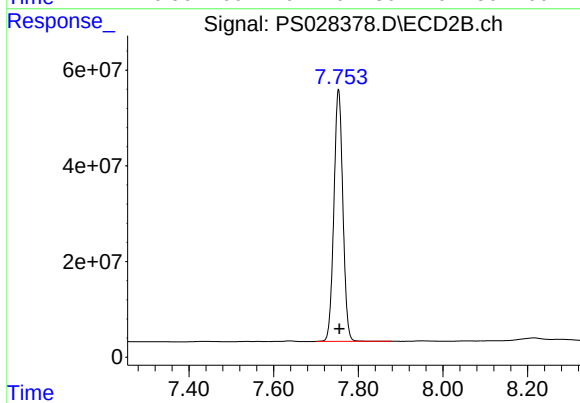

#4 2,4-DCAA


R.T.: 7.753 min
Delta R.T.: -0.002 min
Response: 775445925
Conc: 486.65 ng/ml

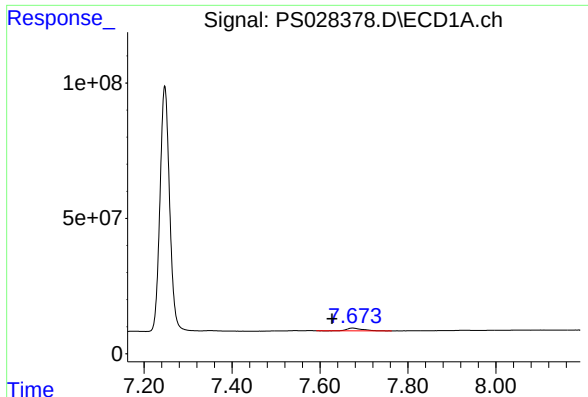

#6 MCPP


R.T.: 7.674 min
Delta R.T.: 0.047 min
Response: 24535273
Conc: 3.00 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

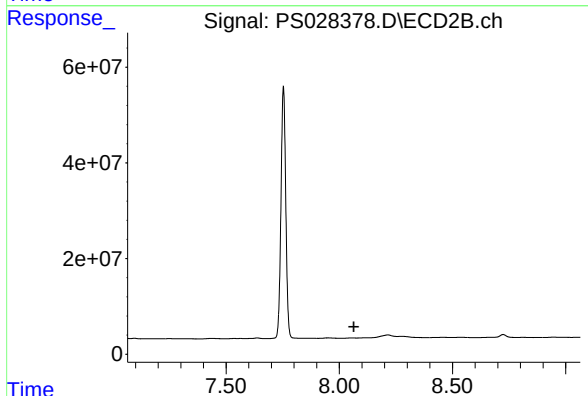


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.

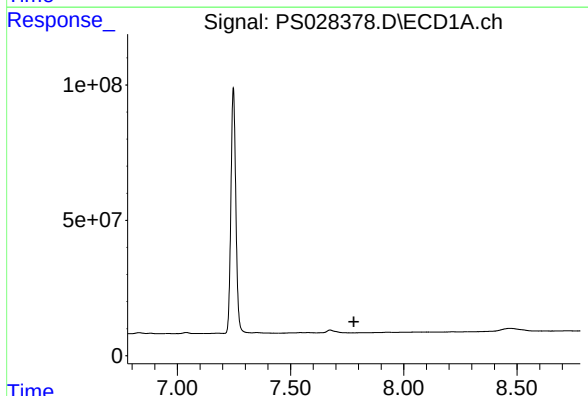


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.779 min
Response: 0
Conc: N.D.

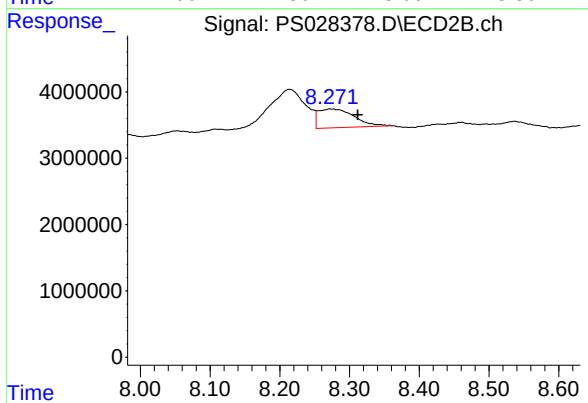

#7 MCPA


R.T.: 8.272 min
Delta R.T.: -0.040 min
Response: 10141169
Conc: 1.27 ug/ml

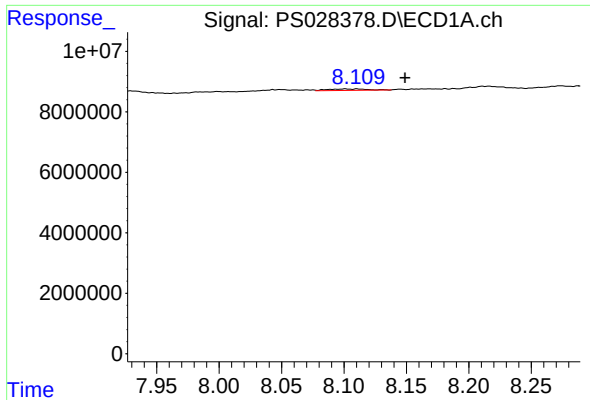

#8 DICHLORPROP

R.T.: 8.101 min
Delta R.T.: -0.048 min
Response: 1080578
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

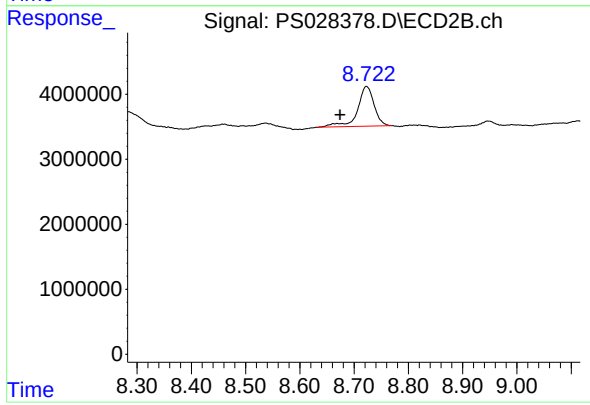

#8 DICHLORPROP

R.T.: 8.723 min
Delta R.T.: 0.049 min
Response: 12971604
Conc: 7.28 ng/ml