

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111021\
 Data File : PS017378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2021 17:38
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 00:29:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 19 01:21:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.148	6.738	1197.3E6	454.8E6	783.306	778.146
Target Compounds							
1) T	Dalapon	2.988	2.491	1673.8E6	494.2E6	770.844	763.832
2) T	3,5-DICHL...	6.373	5.936	1548.4E6	638.6E6	717.283	735.302
3) T	4-Nitroph...	6.979	6.363	577.8E6	225.2E6	662.441	698.717
5) T	DICAMBA	7.337	6.898	4424.1E6	1902.4E6	738.617	747.192
6) T	MCPD	7.507	6.995	332.4E6	153.5E6	74.349	76.208
7) T	MCPA	7.656	7.207	466.2E6	214.3E6	75.572	72.387
8) T	DICHLORPROP	8.027	7.515	1098.0E6	478.6E6	732.302	744.223
9) T	2,4-D	8.257	7.806	1310.9E6	559.8E6	740.105	743.896
10) T	Pentachlo...	8.561	8.229	15451.1E6	6157.7E6	744.701	754.194
11) T	2,4,5-TP ...	9.111	8.589	6079.7E6	2614.8E6	747.567	758.546
12) T	2,4,5-T	9.395	8.965	6157.7E6	2443.5E6	766.633	770.930
13) T	2,4-DB	9.944	9.470	1190.0E6	306.0E6	791.068	737.851
14) T	DINOSEB	11.095	9.795	4623.4E6	1839.6E6	816.164	833.694
15) T	Picloram	10.919	10.774	8531.8E6	3065.7E6	798.754	800.511
16) T	DCPA	11.363	10.724	7861.9E6	3255.8E6	771.973	762.971



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111021\
Data File : PS017378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2021 17:38
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 00:29:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
Quant Title : 8080.M
QLast Update : Tue Oct 19 01:21:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

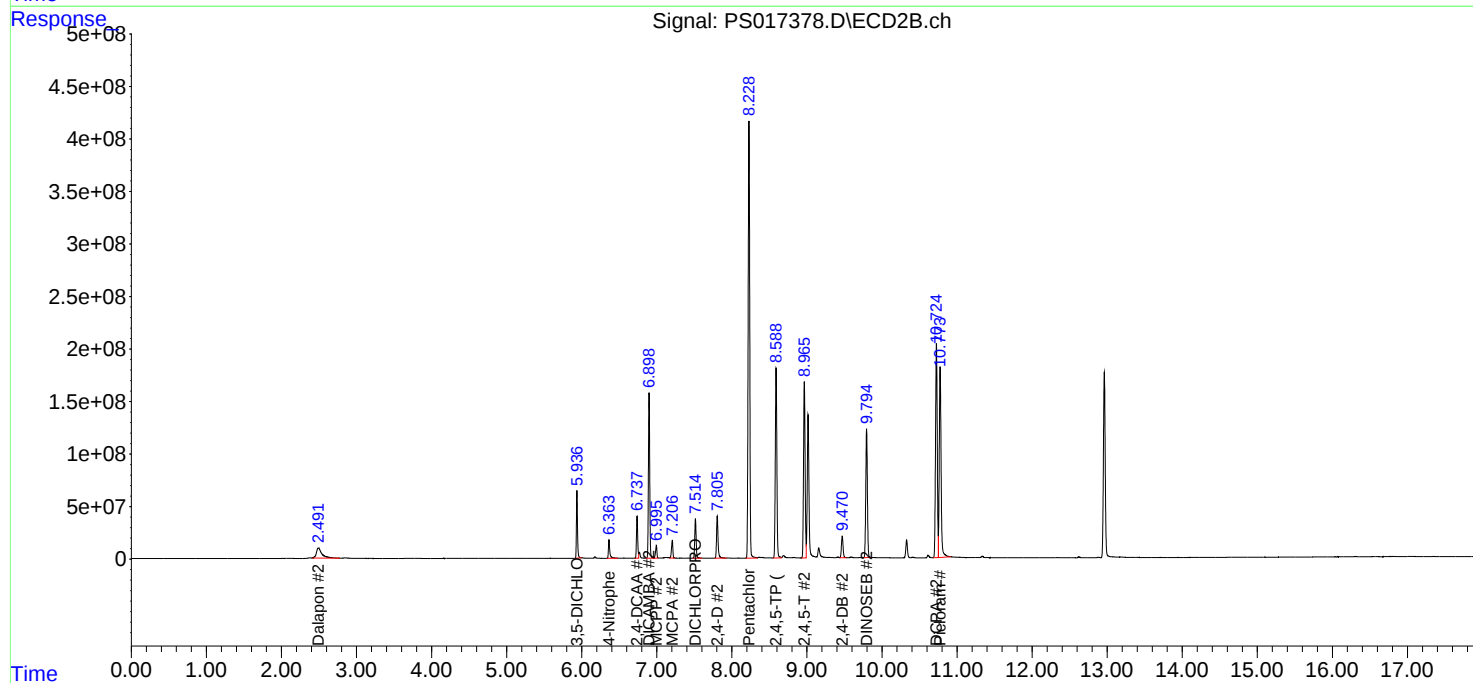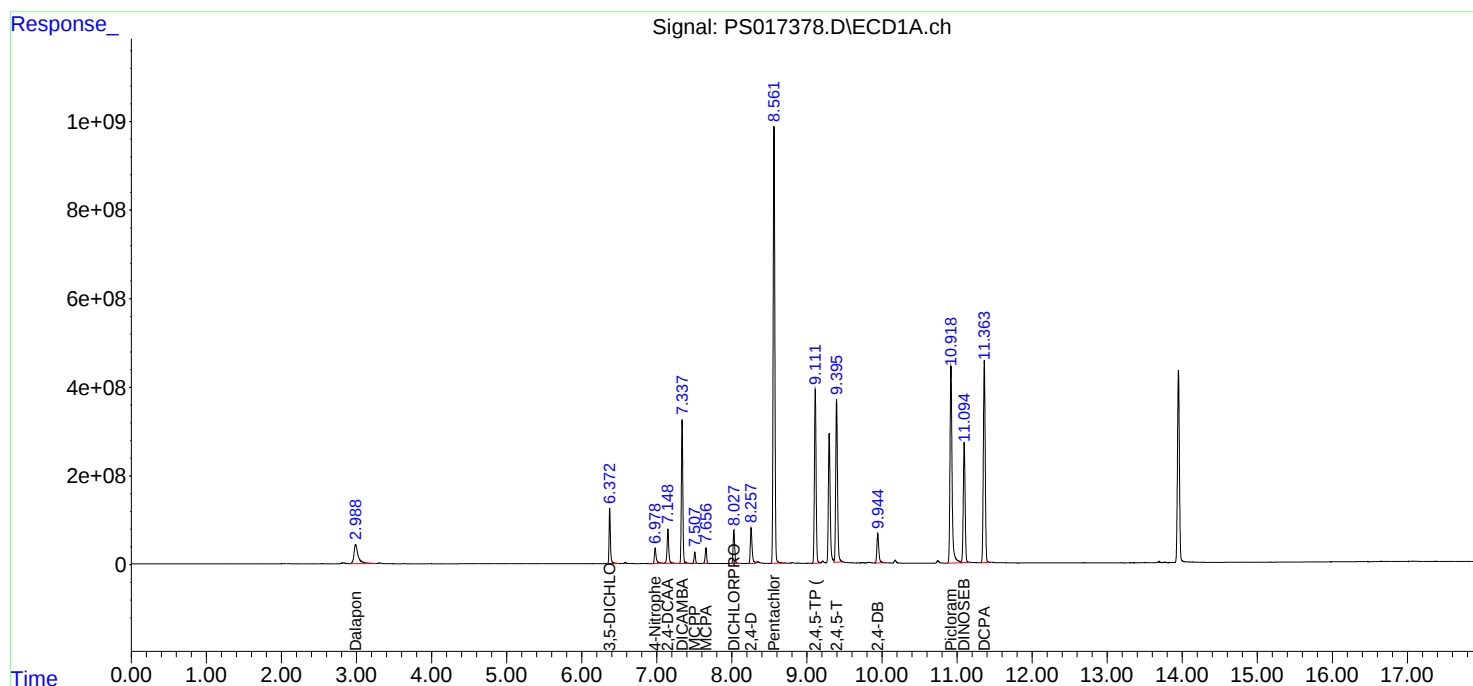


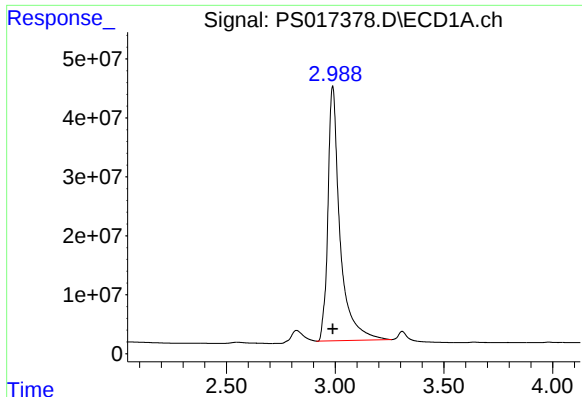

#1 Dalapon


R.T.: 2.988 min
Delta R.T.: 0.000 min
Response: 1673817518
Conc: 770.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

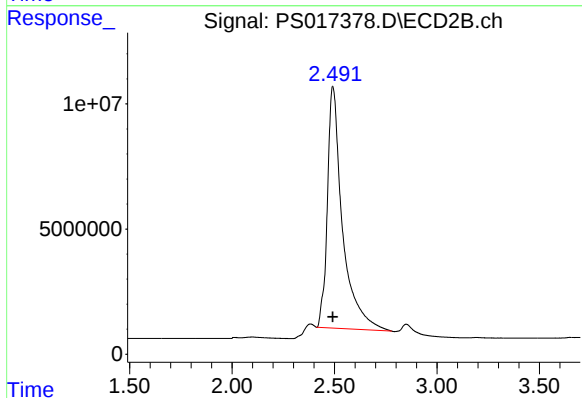


#1 Dalapon

R.T.: 2.491 min
Delta R.T.: 0.000 min
Response: 494232938
Conc: 763.83 ng/ml

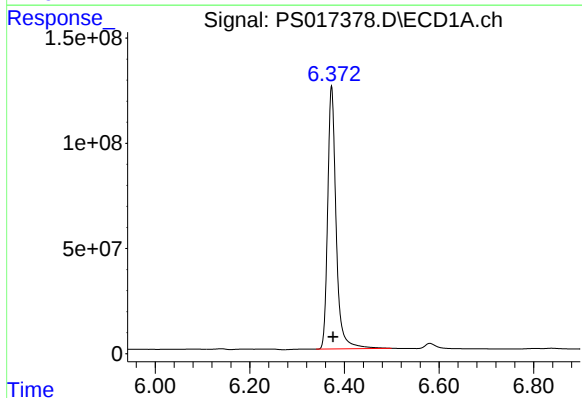


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.373 min
Delta R.T.: -0.003 min
Response: 1548398778
Conc: 717.28 ng/ml

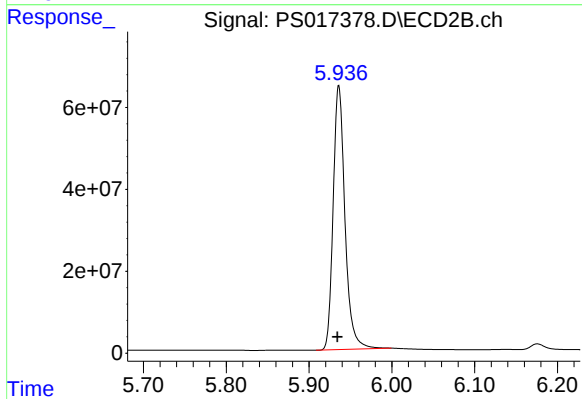

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.936 min
Delta R.T.: 0.002 min
Response: 638633490
Conc: 735.30 ng/ml

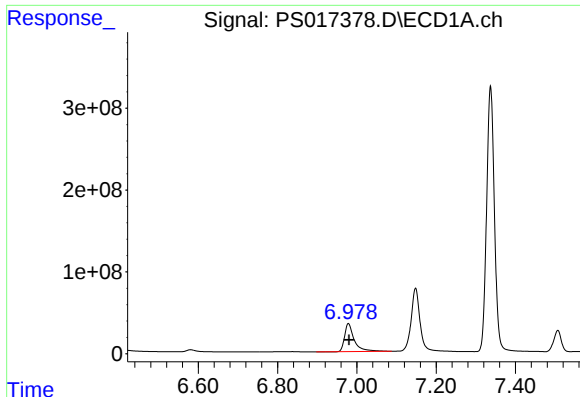

#3 4-Nitrophenol


R.T.: 6.979 min
Delta R.T.: -0.002 min
Response: 577752199
Conc: 662.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

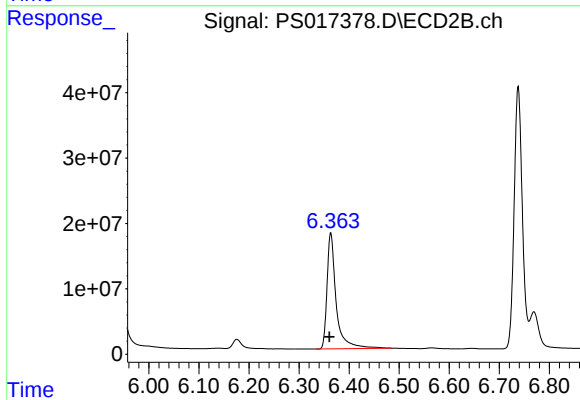


#3 4-Nitrophenol

R.T.: 6.363 min
Delta R.T.: 0.002 min
Response: 225227986
Conc: 698.72 ng/ml

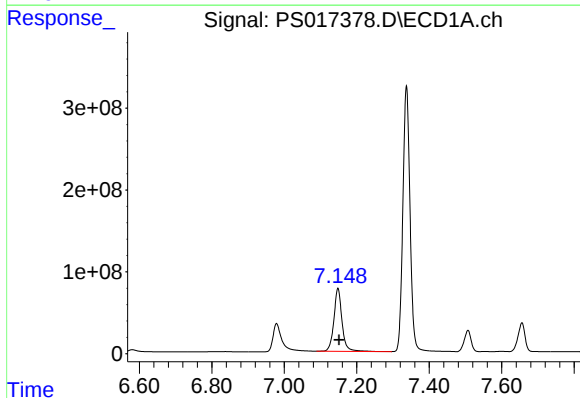


#4 2,4-DCAA

R.T.: 7.148 min
Delta R.T.: -0.003 min
Response: 1197251247
Conc: 783.31 ng/ml

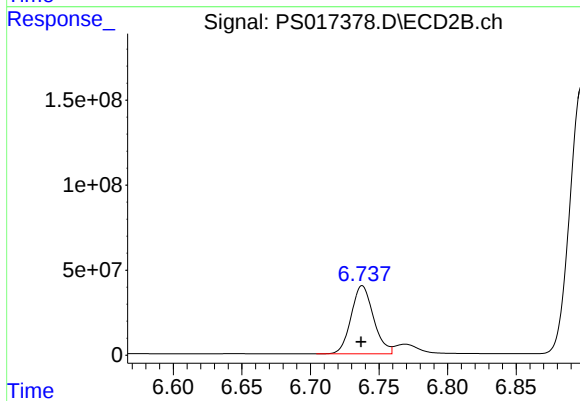

#4 2,4-DCAA


R.T.: 6.738 min
Delta R.T.: 0.000 min
Response: 454780900
Conc: 778.15 ng/ml

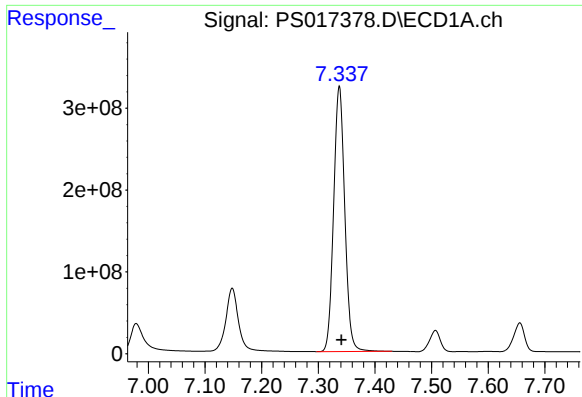

#5 DICAMBA


R.T.: 7.337 min
Delta R.T.: -0.004 min
Response: 4424112367
Conc: 738.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

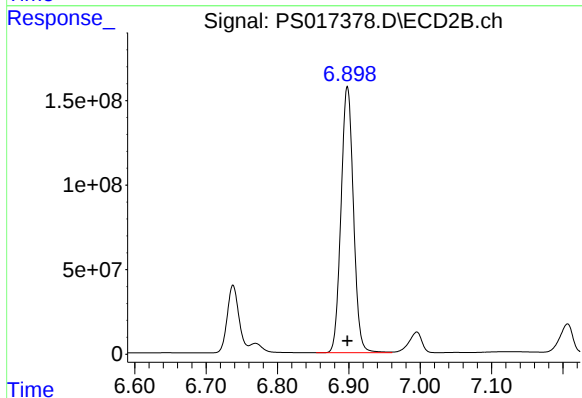


#5 DICAMBA

R.T.: 6.898 min
Delta R.T.: 0.000 min
Response: 1902400113
Conc: 747.19 ng/ml

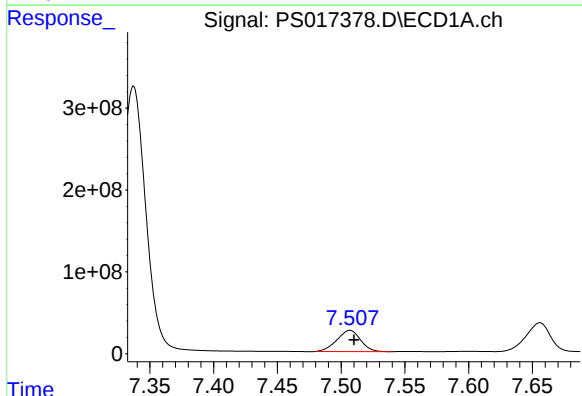


#6 MCP

R.T.: 7.507 min
Delta R.T.: -0.003 min
Response: 332373742
Conc: 74.35 ug/ml

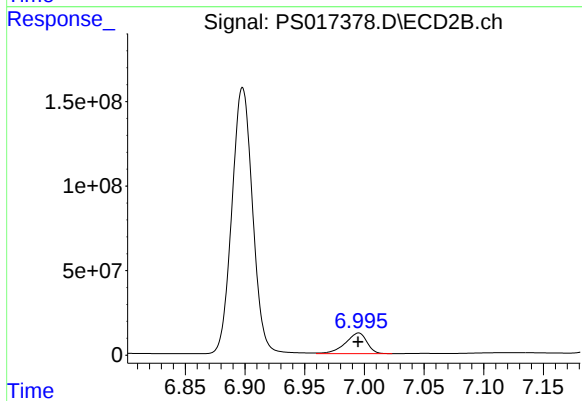

#6 MCP


R.T.: 6.995 min
Delta R.T.: 0.000 min
Response: 153473553
Conc: 76.21 ug/ml

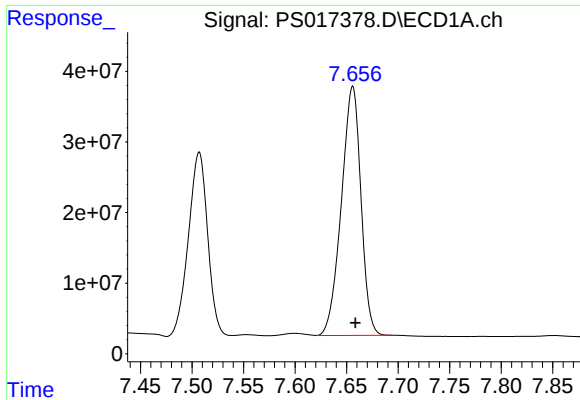

#7 MCPA


R.T.: 7.656 min
Delta R.T.: -0.003 min
Response: 466240686
Conc: 75.57 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

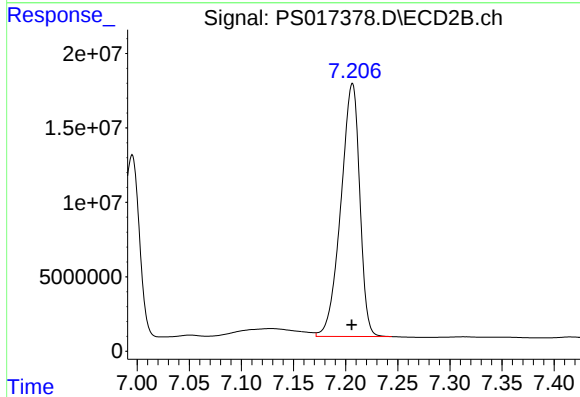


#7 MCPA

R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 214293946
Conc: 72.39 ug/ml

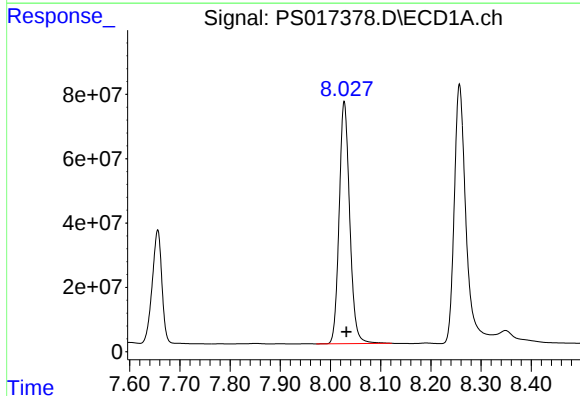


#8 DICHLORPROP

R.T.: 8.027 min
Delta R.T.: -0.004 min
Response: 1098007557
Conc: 732.30 ng/ml

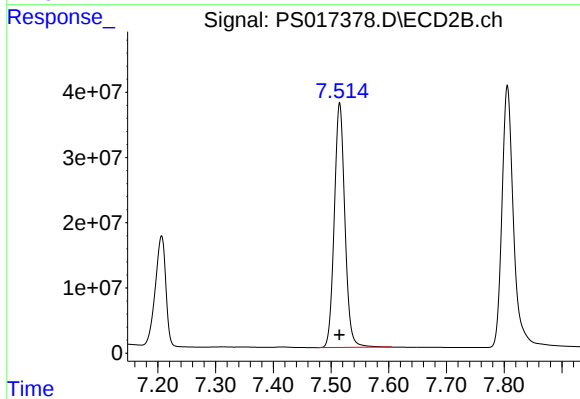

#8 DICHLORPROP


R.T.: 7.515 min
Delta R.T.: 0.000 min
Response: 478605449
Conc: 744.22 ng/ml

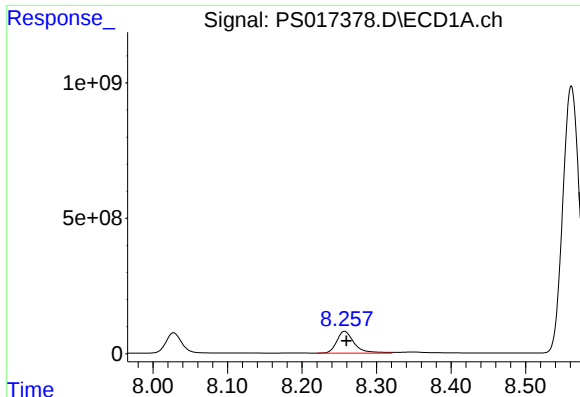

#9 2,4-D


R.T.: 8.257 min
Delta R.T.: -0.003 min
Response: 1310875505
Conc: 740.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

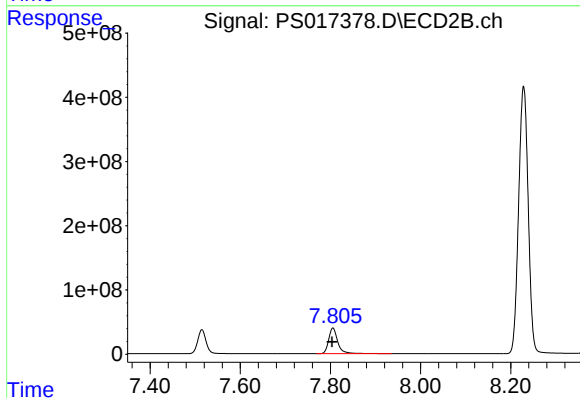


#9 2,4-D

R.T.: 7.806 min
Delta R.T.: 0.002 min
Response: 559841334
Conc: 743.90 ng/ml

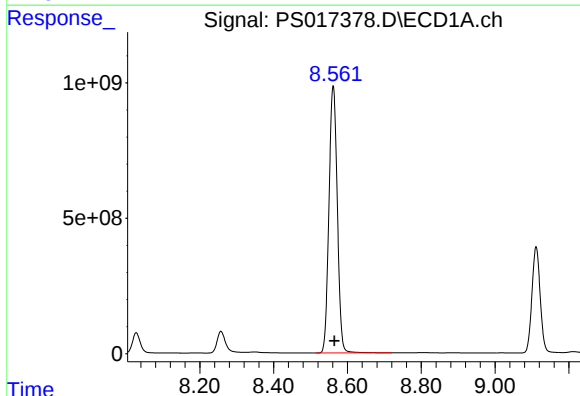


#10 Pentachlorophenol

R.T.: 8.561 min
Delta R.T.: -0.003 min
Response: 15451101813
Conc: 744.70 ng/ml

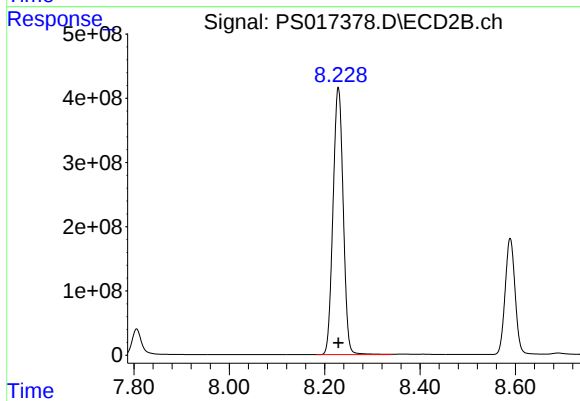

#10 Pentachlorophenol


R.T.: 8.229 min
Delta R.T.: 0.000 min
Response: 6157745403
Conc: 754.19 ng/ml

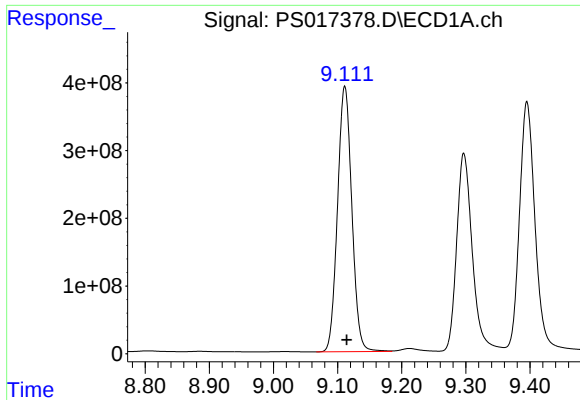

#11 2,4,5-TP (SILVEX)


R.T.: 9.111 min
Delta R.T.: -0.003 min
Response: 6079743663
Conc: 747.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

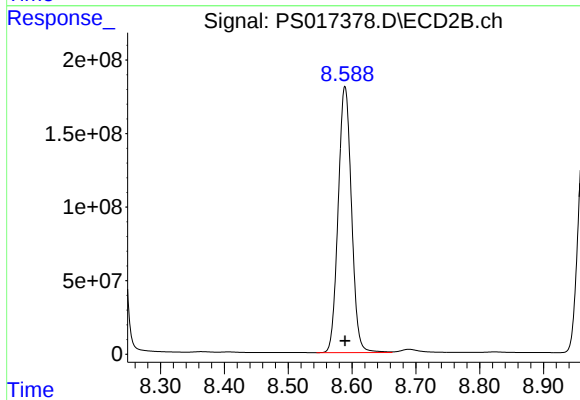


#11 2,4,5-TP (SILVEX)

R.T.: 8.589 min
Delta R.T.: 0.000 min
Response: 2614821325
Conc: 758.55 ng/ml

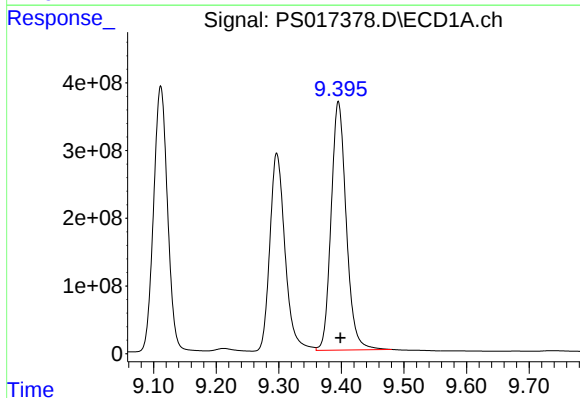


#12 2,4,5-T

R.T.: 9.395 min
Delta R.T.: -0.003 min
Response: 6157701509
Conc: 766.63 ng/ml

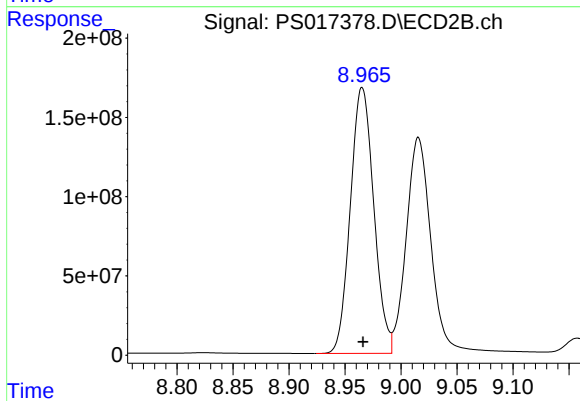

#12 2,4,5-T


R.T.: 8.965 min
Delta R.T.: 0.000 min
Response: 2443456511
Conc: 770.93 ng/ml

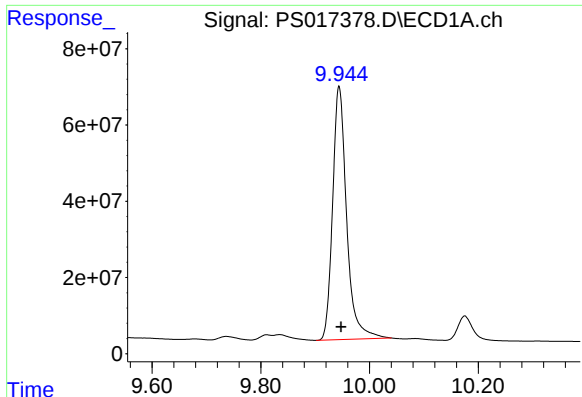

#13 2,4-DB


R.T.: 9.944 min
Delta R.T.: -0.004 min
Response: 1190040599
Conc: 791.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

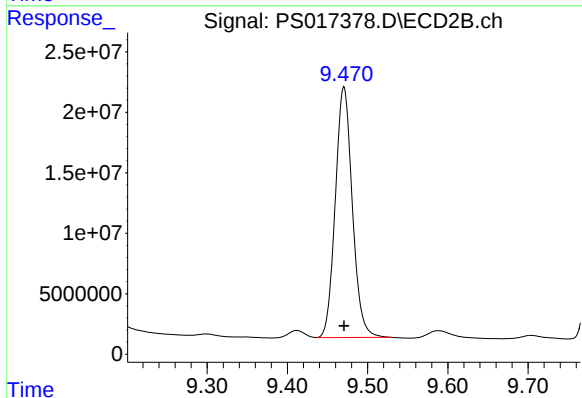


#13 2,4-DB

R.T.: 9.470 min
Delta R.T.: 0.000 min
Response: 306042754
Conc: 737.85 ng/ml

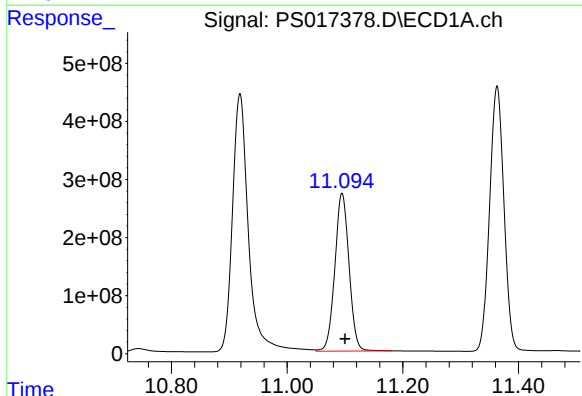


#14 DINOSEB

R.T.: 11.095 min
Delta R.T.: -0.005 min
Response: 4623420779
Conc: 816.16 ng/ml

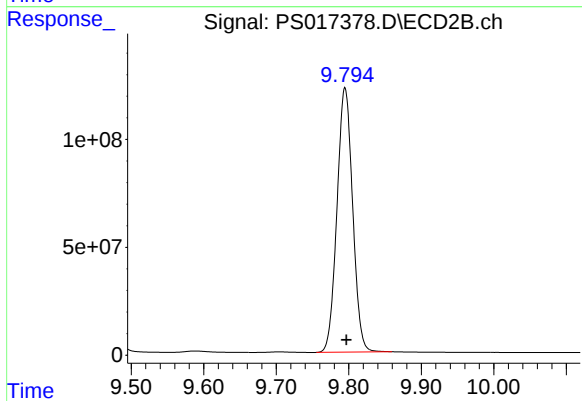

#14 DINOSEB


R.T.: 9.795 min
Delta R.T.: -0.002 min
Response: 1839611244
Conc: 833.69 ng/ml

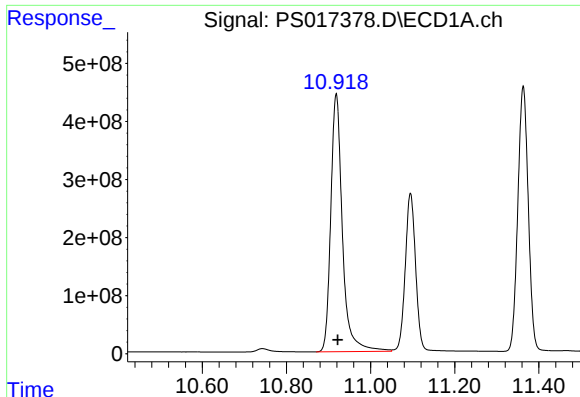

#15 Picloram


R.T.: 10.919 min
Delta R.T.: -0.004 min
Response: 8531837642
Conc: 798.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

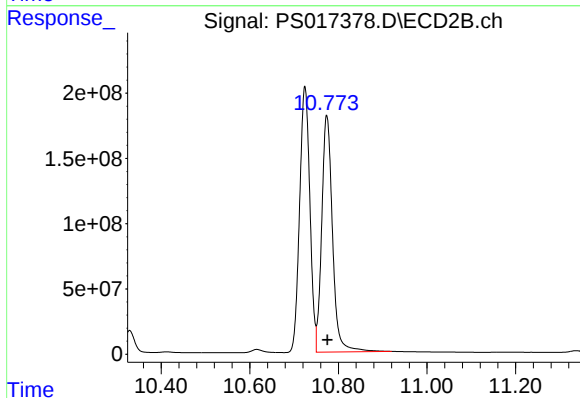


#15 Picloram

R.T.: 10.774 min
Delta R.T.: -0.001 min
Response: 3065736065
Conc: 800.51 ng/ml

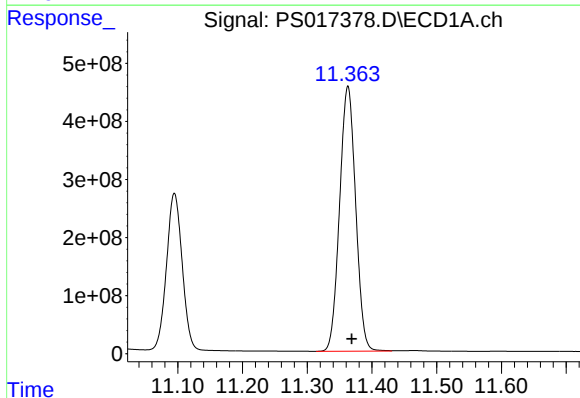

#16 DCPA

R.T.: 11.363 min
Delta R.T.: -0.006 min
Response: 7861930261
Conc: 771.97 ng/ml

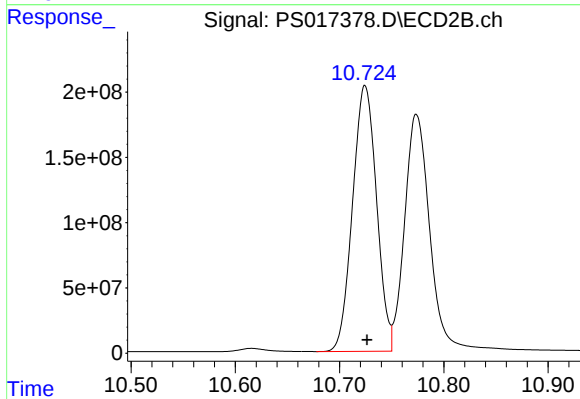

#16 DCPA

R.T.: 10.724 min
Delta R.T.: -0.002 min
Response: 3255791012
Conc: 762.97 ng/ml