

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111022\
 Data File : PS021097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2022 08:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 13:31:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.410	6.846	1188.0E6	809.9E6	569.222	585.529
Target Compounds							
3) T	4-Nitroph...	6.250	0.000	6095754	0	4.053	N.D. #
6) T	MCP	0.000	7.164f	0	444057	N.D.	<MDL
7) T	MCPA	6.787f	0.000	15768305	0	1.681	N.D. #
8) T	DICHLORPROP	0.000	7.682	0	563599	N.D.	<MDL
10) T	Pentachlo...	7.581	0.000	698460	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.120	0.000	1937300	0	<MDL	N.D. #
12) T	2,4,5-T	8.366	0.000	3849048	0	<MDL	N.D. #
13) T	2,4-DB	8.885	9.554f	1835759	3090231	<MDL	2.776 #
14) T	DINOSEB	9.912	0.000	9541610	0	<MDL	N.D. #
15) T	Picloram	9.774	0.000	2906724	0	<MDL	N.D. #
16) T	DCPA	10.246	0.000	509027	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111022\
Data File : PS021097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2022 08:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 13:31:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

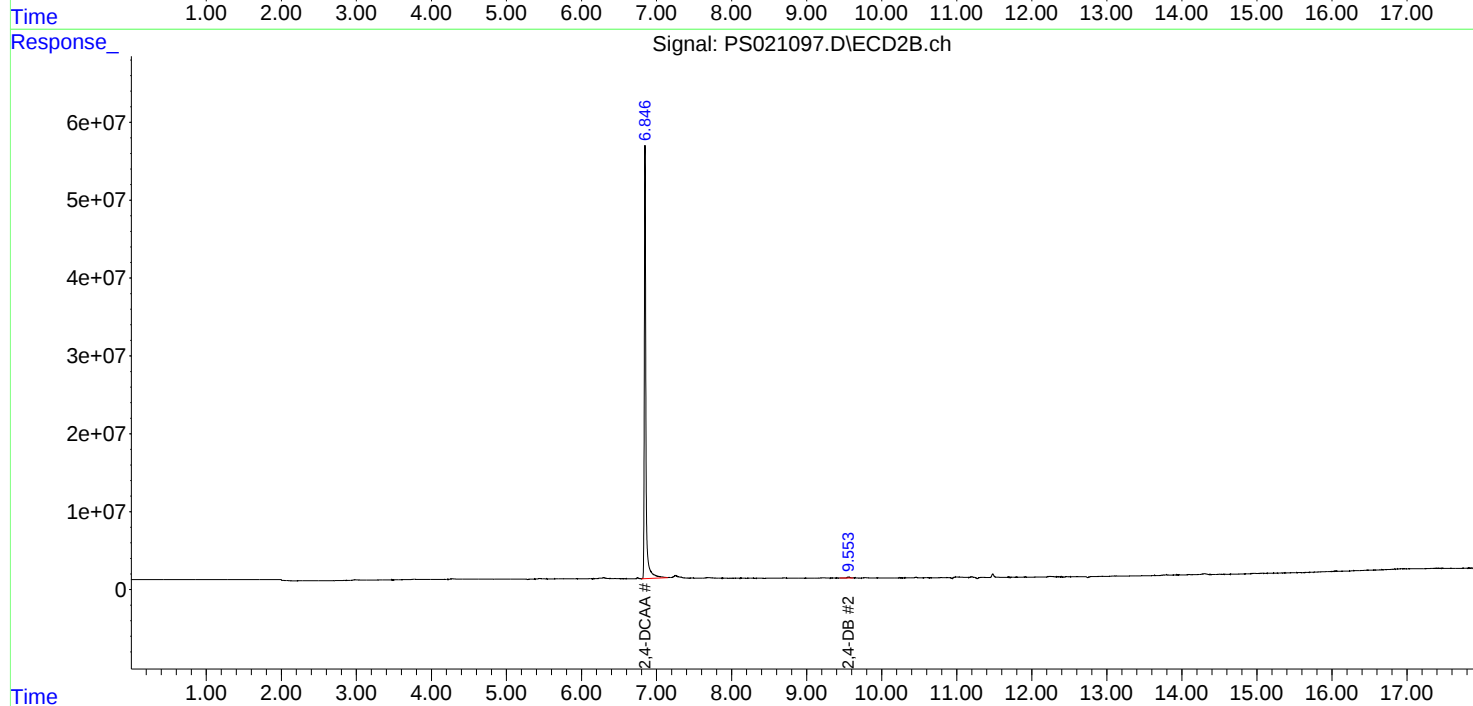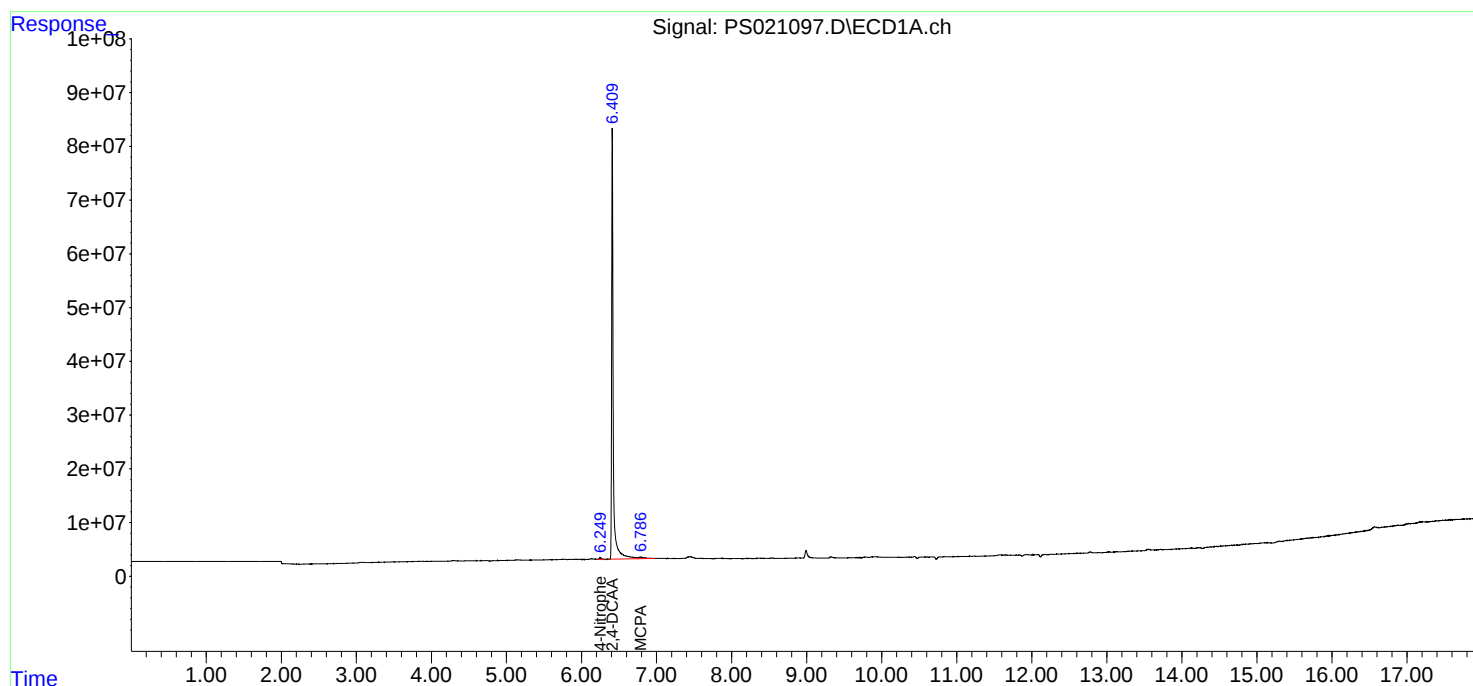


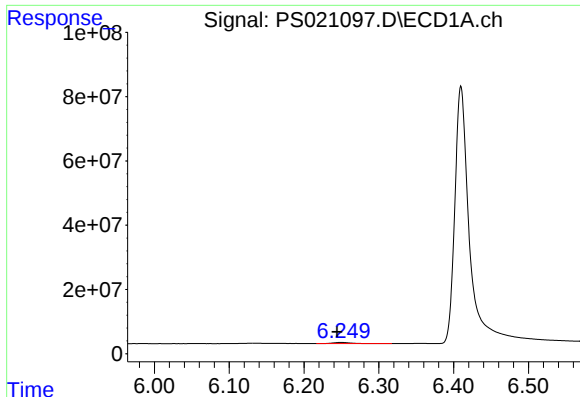

#3 4-Nitrophenol


R.T.: 6.250 min
Delta R.T.: 0.006 min
Response: 6095754
Conc: 4.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

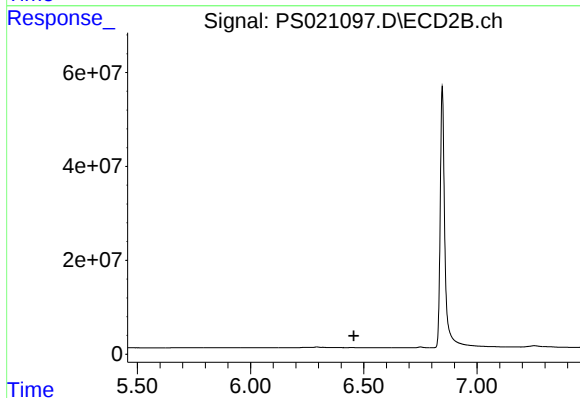


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

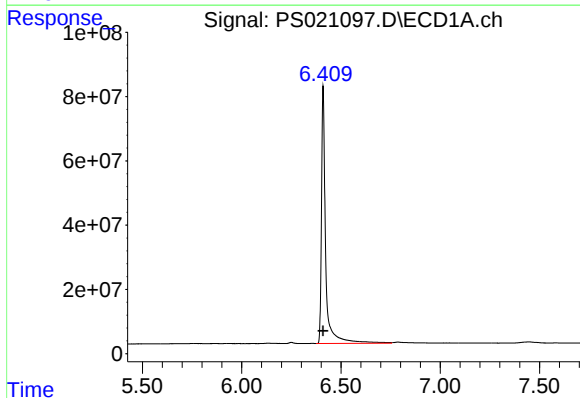


#4 2,4-DCAA

R.T.: 6.410 min
Delta R.T.: 0.000 min
Response: 1188009875
Conc: 569.22 ng/ml

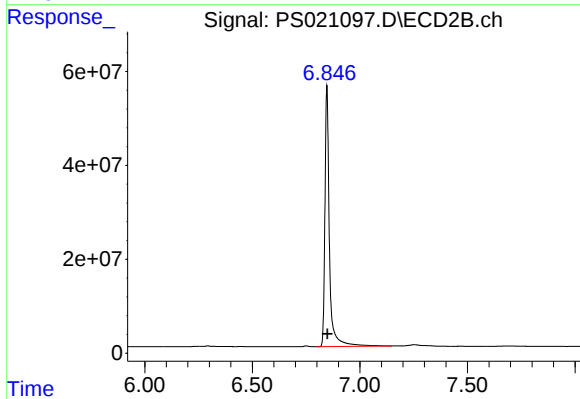

#4 2,4-DCAA


R.T.: 6.846 min
Delta R.T.: -0.003 min
Response: 809871431
Conc: 585.53 ng/ml

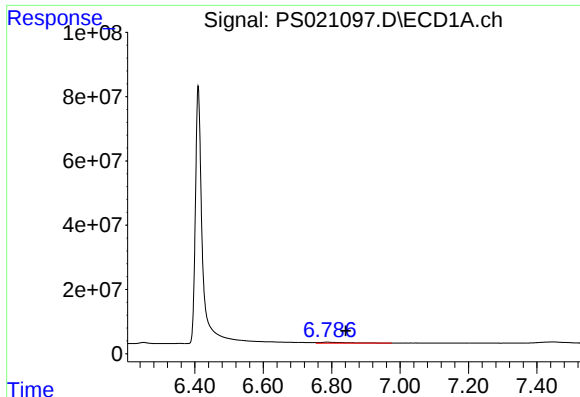

#7 MCPA


R.T.: 6.787 min
Delta R.T.: -0.054 min
Response: 15768305
Conc: 1.68 ug/ml

Instrument :
ECD_S
ClientSampleId :

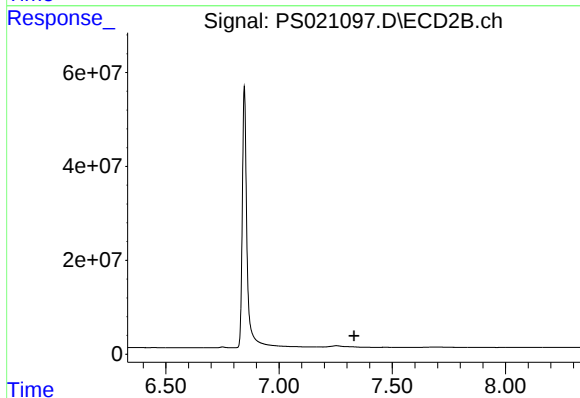


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.331 min
Response: 0
Conc: N.D.

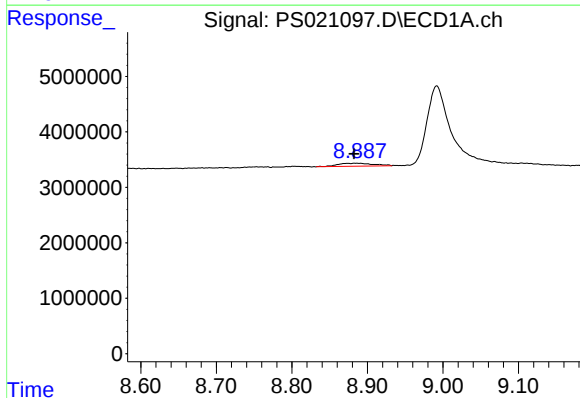

#13 2,4-DB

R.T.: 8.885 min
Delta R.T.: 0.003 min
Response: 1835759
Conc: N.D.

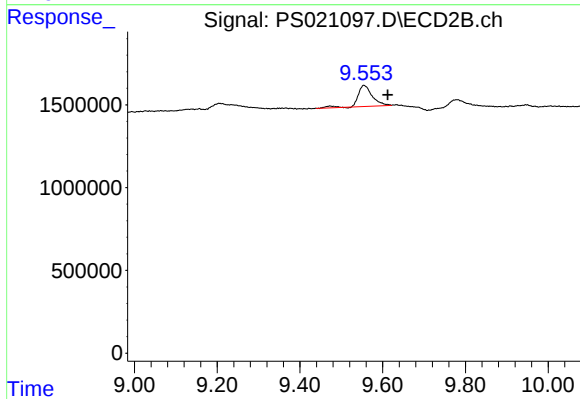

#13 2,4-DB

R.T.: 9.554 min
Delta R.T.: -0.058 min
Response: 3090231
Conc: 2.78 ng/ml