

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111022\
 Data File : PS021109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2022 15:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 16:15:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.407	6.844	1188.1E6	820.2E6	569.264	593.003
Target Compounds							
1) T	Dalapon	2.525	0.000	866559	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.790	0.000	926750	0	<MDL	N.D. #
3) T	4-Nitroph...	6.245	0.000	11360609	0	7.553	N.D. #
5) T	DICAMBA	0.000	7.000	0	2205727	N.D.	<MDL
6) T	MCPD	6.738	0.000	15198179	0	2.329	N.D. #
7) T	MCPA	6.772f	0.000	8602116	0	<MDL	N.D. #
8) T	DICHLORPROP	7.111f	7.657	523399	5777106	<MDL	3.752 #
9) T	2,4-D	0.000	7.921	0	988537	N.D.	<MDL
10) T	Pentachlo...	7.572	8.416f	1534341	4320179	<MDL	<MDL #
11) T	2,4,5-TP ...	8.117	8.757	15279751	8484735	1.150	<MDL #
12) T	2,4,5-T	8.387	9.098	3942311	13075088	<MDL	1.516 #
13) T	2,4-DB	8.824f	0.000	4451058	0	1.613	N.D. #
14) T	DINOSEB	9.881f	9.946	4525928	32404834	<MDL	5.062 #
15) T	Picloram	9.780	10.908	4716780	7693944	<MDL	<MDL #
16) T	DCPA	10.194	10.867	1356754	14005500	<MDL	1.312 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111022\
Data File : PS021109.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2022 15:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 16:15:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

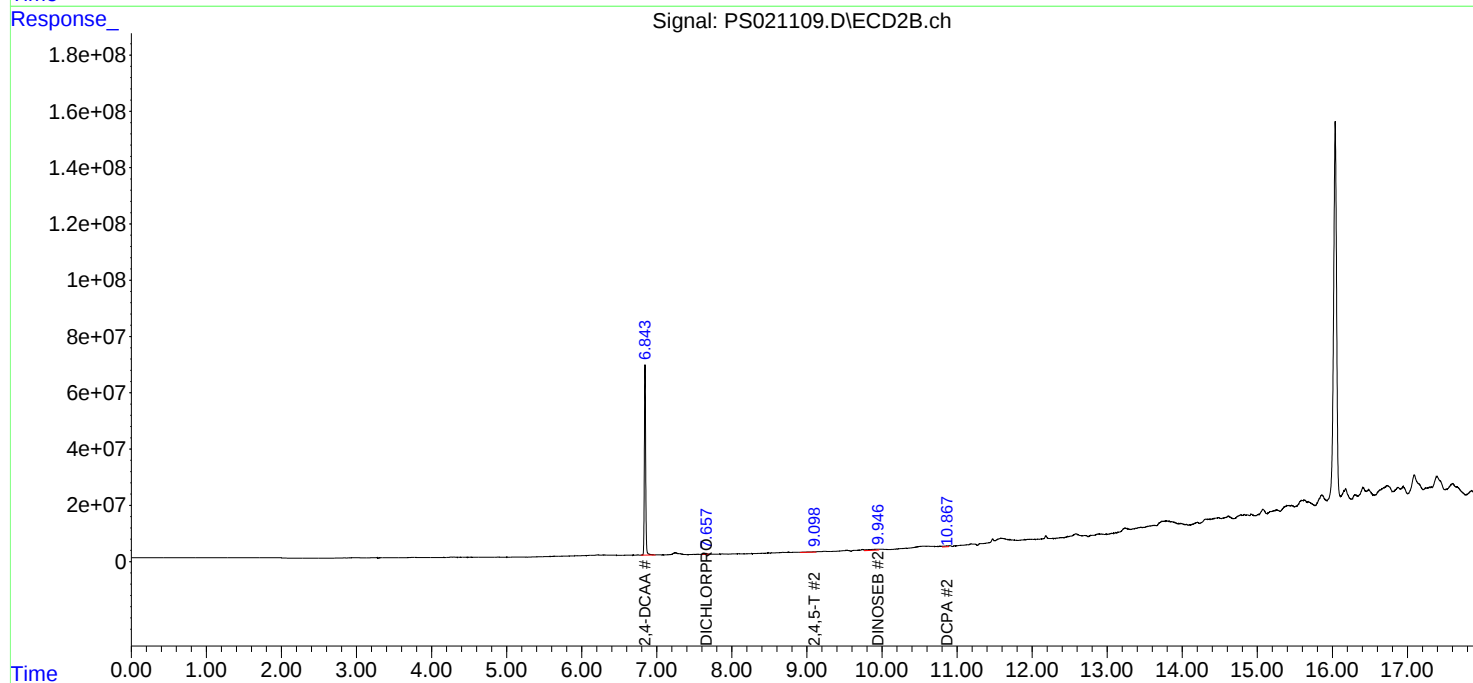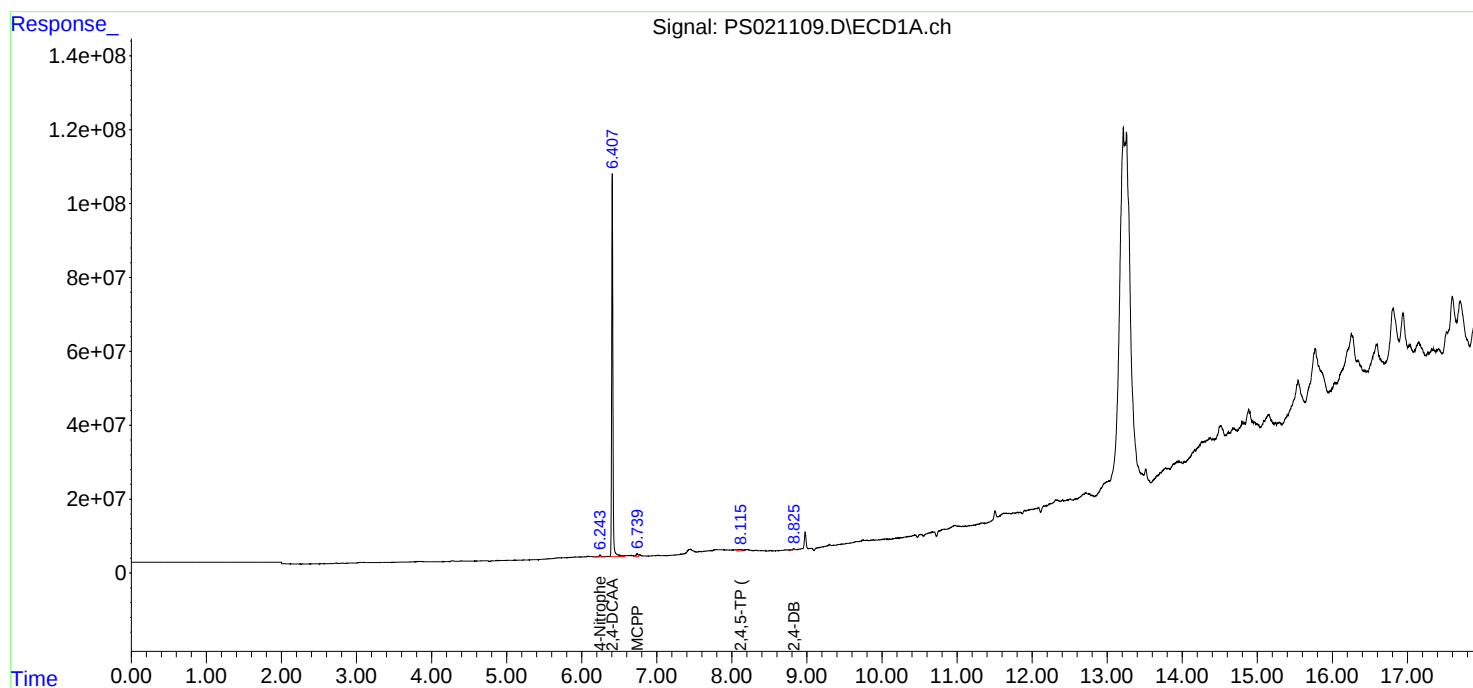


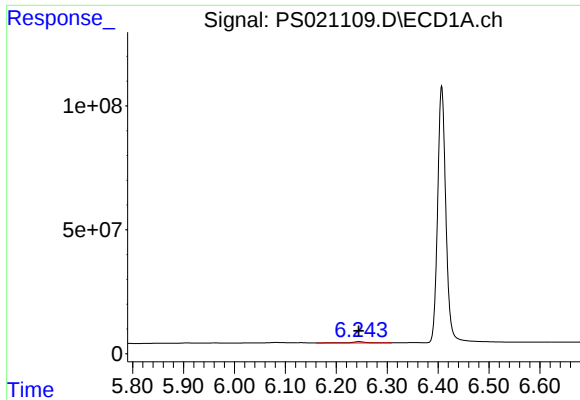

#3 4-Nitrophenol


R.T.: 6.245 min
Delta R.T.: 0.000 min
Response: 11360609
Conc: 7.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

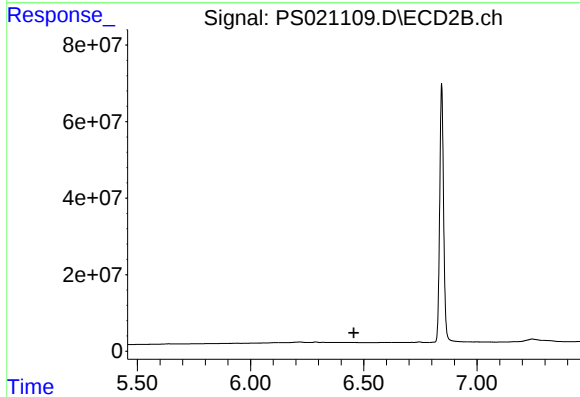


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

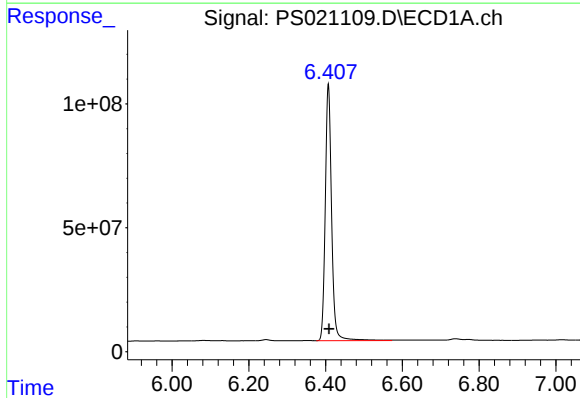


#4 2,4-DCAA

R.T.: 6.407 min
Delta R.T.: -0.002 min
Response: 1188098430
Conc: 569.26 ng/ml

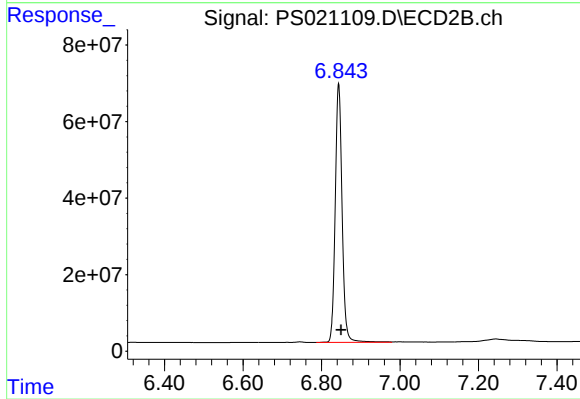

#4 2,4-DCAA


R.T.: 6.844 min
Delta R.T.: -0.006 min
Response: 820209936
Conc: 593.00 ng/ml

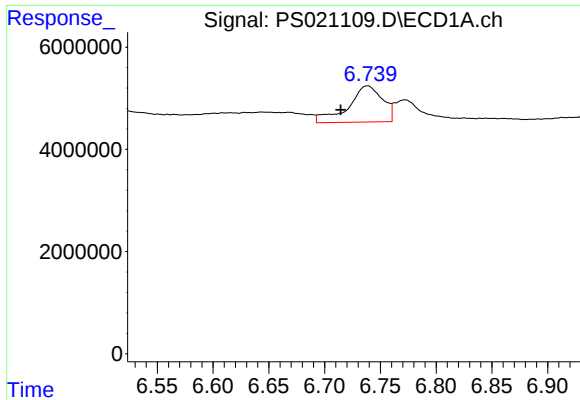

#6 MCP


R.T.: 6.738 min
Delta R.T.: 0.024 min
Response: 15198179
Conc: 2.33 ug/ml

Instrument :
ECD_S
ClientSampleId :

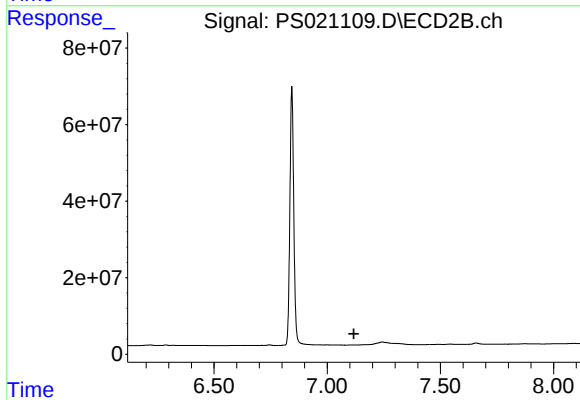


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.118 min
Response: 0
Conc: N.D.

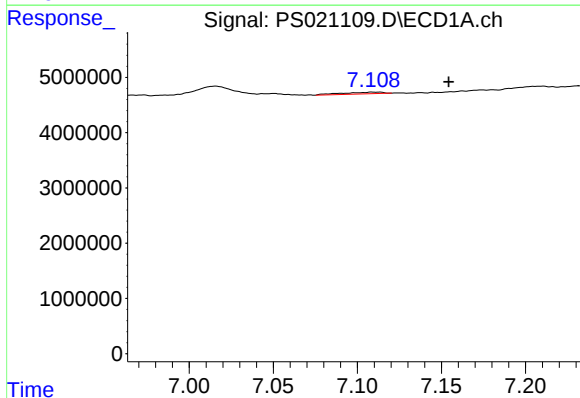


#8 DICHLORPROP

R.T.: 7.111 min
Delta R.T.: -0.044 min
Response: 523399
Conc: N.D.

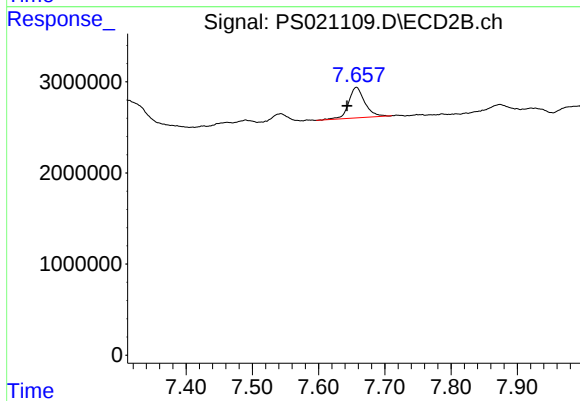

#8 DICHLORPROP


R.T.: 7.657 min
Delta R.T.: 0.014 min
Response: 5777106
Conc: 3.75 ng/ml

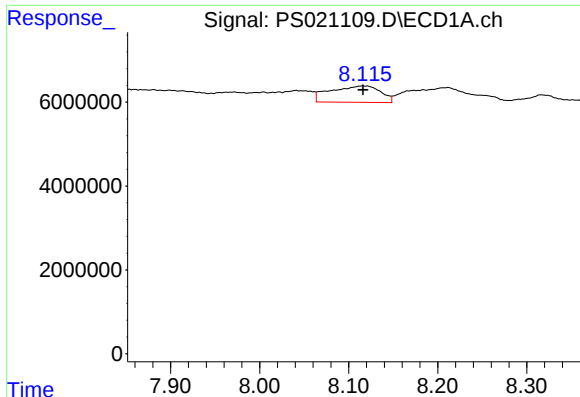

#11 2,4,5-TP (SILVEX)


R.T.: 8.117 min
Delta R.T.: 0.000 min
Response: 15279751
Conc: 1.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

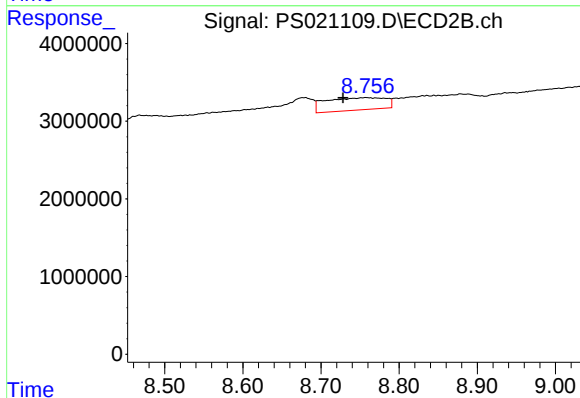


#11 2,4,5-TP (SILVEX)

R.T.: 8.757 min
Delta R.T.: 0.029 min
Response: 8484735
Conc: N.D.

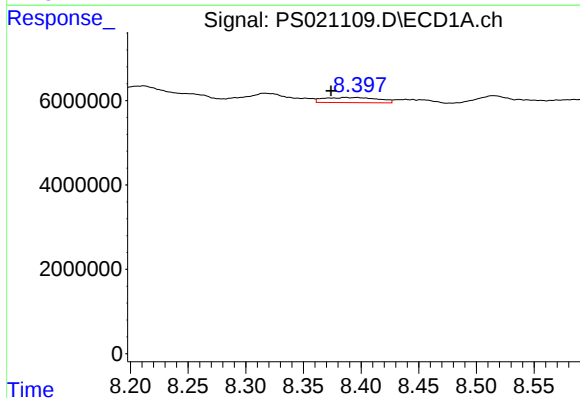


#12 2,4,5-T

R.T.: 8.387 min
Delta R.T.: 0.013 min
Response: 3942311
Conc: N.D.

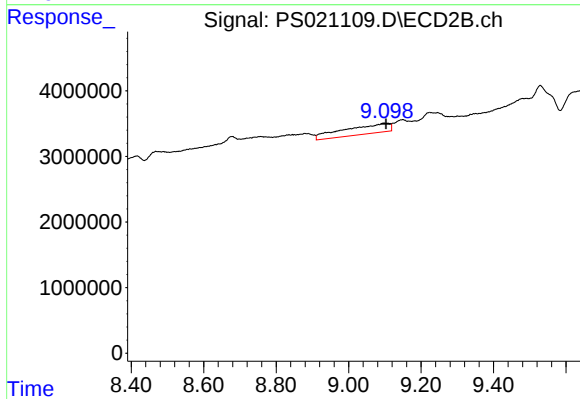

#12 2,4,5-T


R.T.: 9.098 min
Delta R.T.: -0.005 min
Response: 13075088
Conc: 1.52 ng/ml

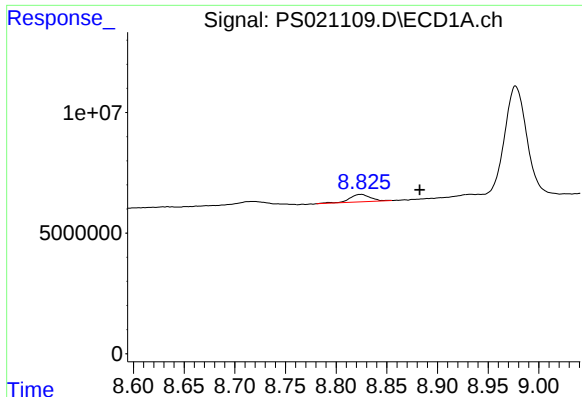

#13 2,4-DB


R.T.: 8.824 min
Delta R.T.: -0.058 min
Response: 4451058
Conc: 1.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

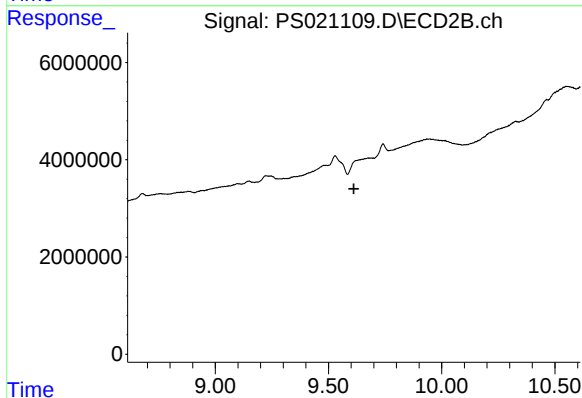


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.612 min
Response: 0
Conc: N.D.

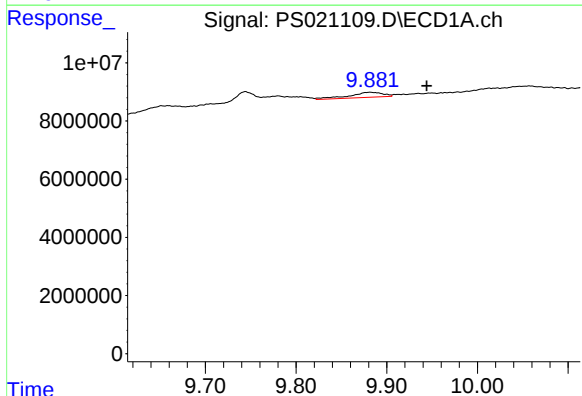


#14 DINOSEB

R.T.: 9.881 min
Delta R.T.: -0.063 min
Response: 4525928
Conc: N.D.

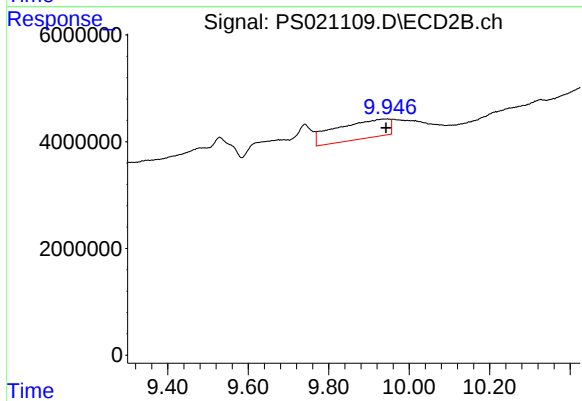

#14 DINOSEB


R.T.: 9.946 min
Delta R.T.: 0.003 min
Response: 32404834
Conc: 5.06 ng/ml

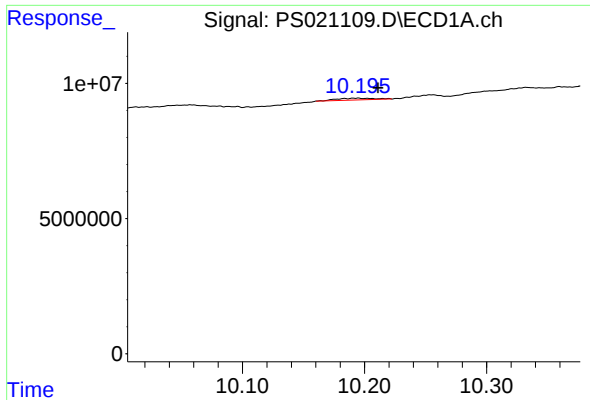

#16 DCPA

R.T.: 10.194 min
Delta R.T.: -0.017 min
Response: 1356754
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

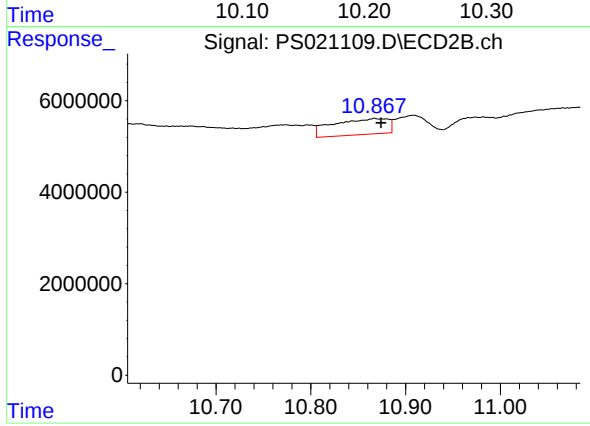

#16 DCPA

R.T.: 10.867 min
Delta R.T.: -0.007 min
Response: 14005500
Conc: 1.31 ng/ml