

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111022\
 Data File : PS021119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2022 20:28
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 03:42:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.407	6.844	1214.5E6	850.8E6	581.891	615.094
Target Compounds							
1) T	Dalapon	2.487	0.000	1314091	0	<MDL	N.D. #
3) T	4-Nitroph...	6.245	0.000	9156281	0	6.088	N.D. #
5) T	DICAMBA	6.619f	7.000	6564136	1516812	<MDL	<MDL #
6) T	MCP	6.740	0.000	8766538	0	1.343	N.D. #
7) T	MCPA	6.774f	0.000	7659622	0	<MDL	N.D. #
8) T	DICHLORPROP	7.204f	7.658	31746	3583350	<MDL	2.327 #
9) T	2,4-D	0.000	7.872f	0	1679362	N.D.	<MDL
10) T	Pentachlo...	7.571	8.359	1550628	182504	<MDL	<MDL #
11) T	2,4,5-TP ...	8.121	8.755	5102452	729731	<MDL	<MDL #
12) T	2,4,5-T	8.396	9.100	3996252	351824	<MDL	<MDL #
13) T	2,4-DB	8.826f	0.000	6153020	0	2.230	N.D. #
14) T	DINOSEB	9.883f	9.936	2485326	14325223	<MDL	2.238 #
15) T	Picloram	9.783	10.908	4930611	14908390	<MDL	1.175 #
16) T	DCPA	10.209	10.908	995113	14908390	<MDL	1.396 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111022\
Data File : PS021119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2022 20:28
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 03:42:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

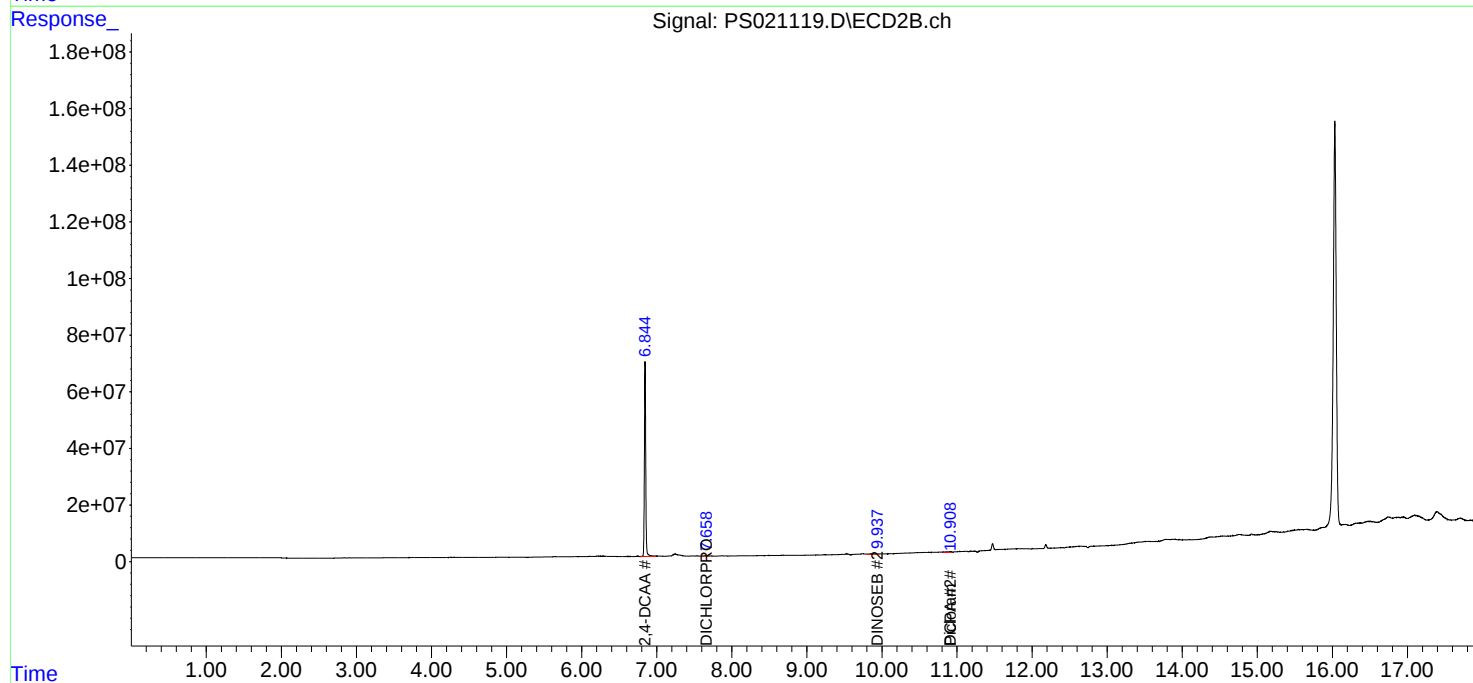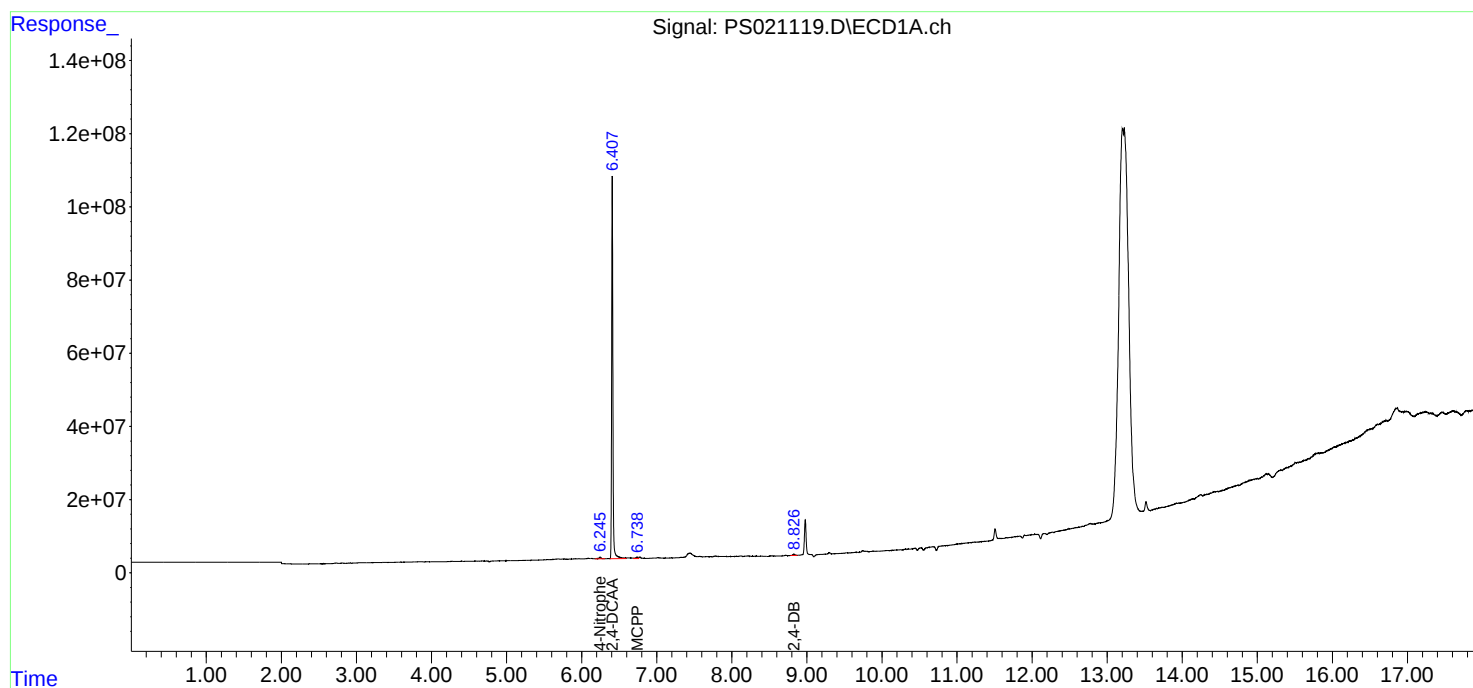


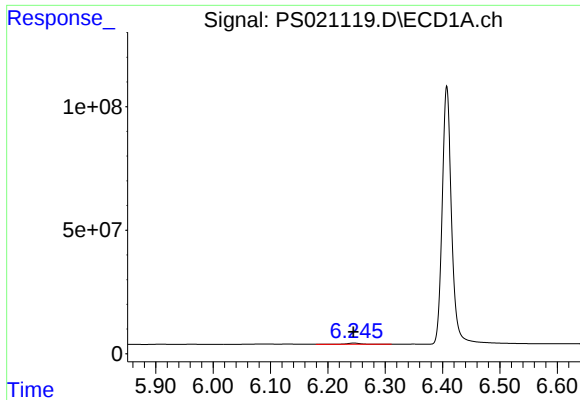

#3 4-Nitrophenol


R.T.: 6.245 min
Delta R.T.: 0.001 min
Response: 9156281
Conc: 6.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

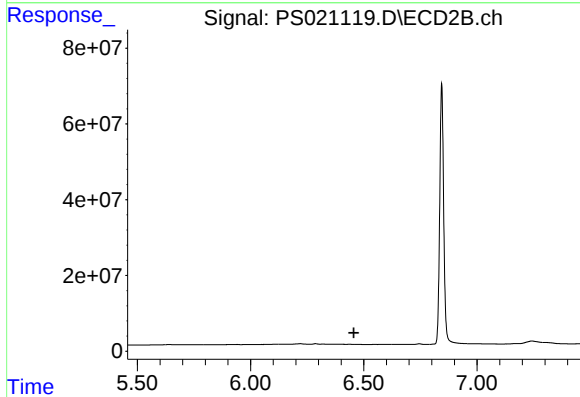


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

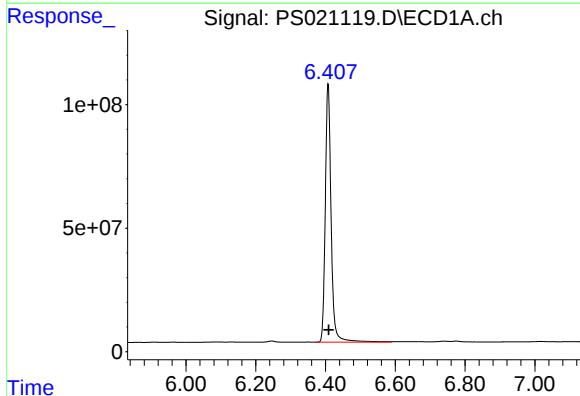


#4 2,4-DCAA

R.T.: 6.407 min
Delta R.T.: -0.002 min
Response: 1214450694
Conc: 581.89 ng/ml

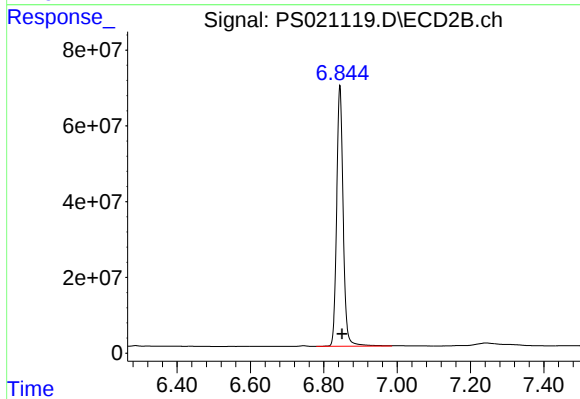

#4 2,4-DCAA


R.T.: 6.844 min
Delta R.T.: -0.006 min
Response: 850764806
Conc: 615.09 ng/ml

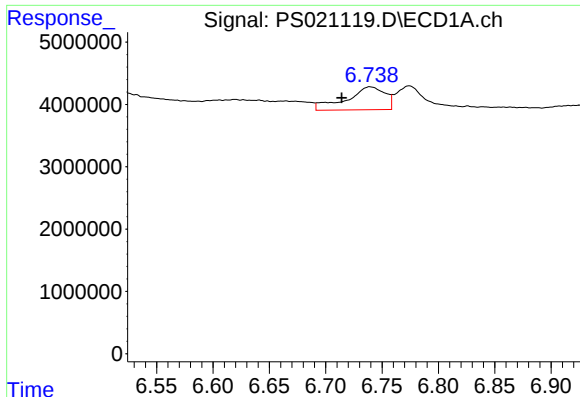

#6 MCP


R.T.: 6.740 min
Delta R.T.: 0.025 min
Response: 8766538
Conc: 1.34 ug/ml

Instrument :
ECD_S
ClientSampleId :

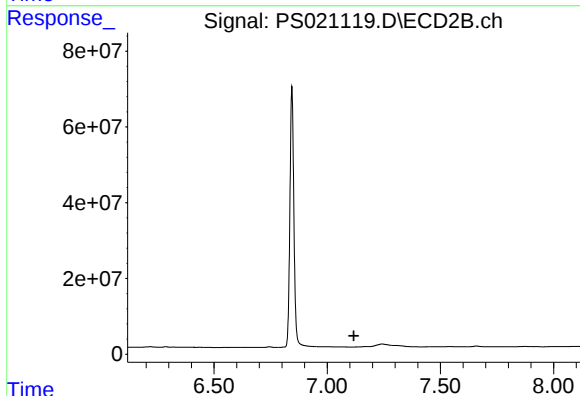


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.118 min
Response: 0
Conc: N.D.

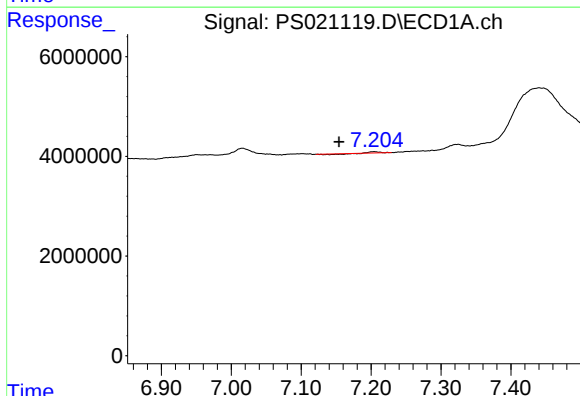


#8 DICHLORPROP

R.T.: 7.204 min
Delta R.T.: 0.050 min
Response: 31746
Conc: N.D.

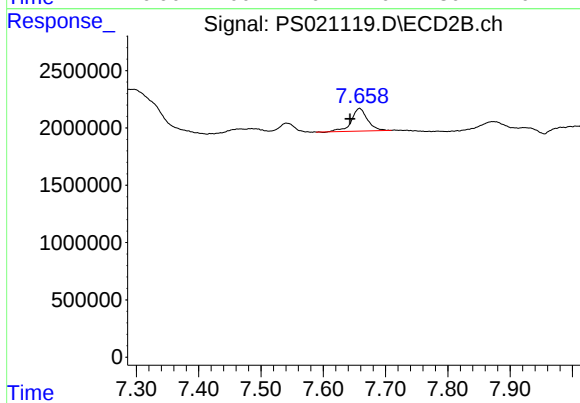

#8 DICHLORPROP


R.T.: 7.658 min
Delta R.T.: 0.015 min
Response: 3583350
Conc: 2.33 ng/ml

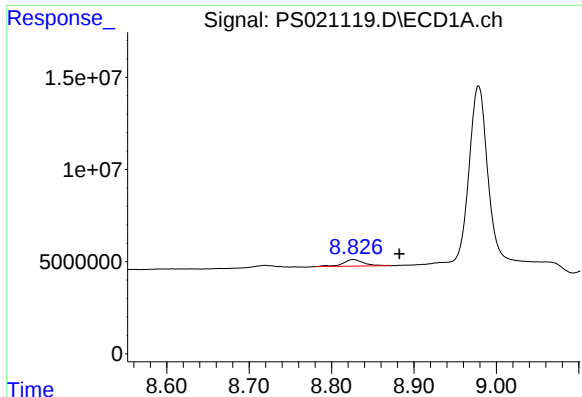

#13 2,4-DB


R.T.: 8.826 min
Delta R.T.: -0.056 min
Response: 6153020
Conc: 2.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

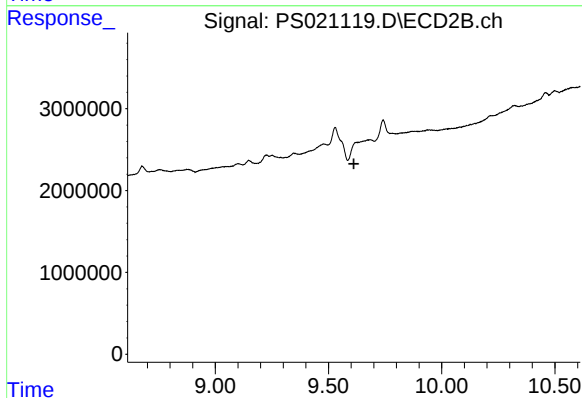


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.612 min
Response: 0
Conc: N.D.

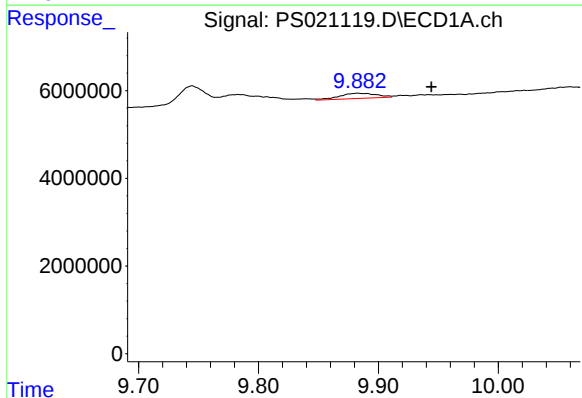


#14 DINOSEB

R.T.: 9.883 min
Delta R.T.: -0.061 min
Response: 2485326
Conc: N.D.

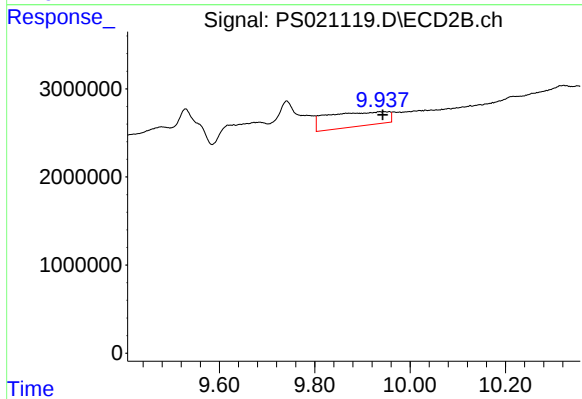

#14 DINOSEB


R.T.: 9.936 min
Delta R.T.: -0.006 min
Response: 14325223
Conc: 2.24 ng/ml

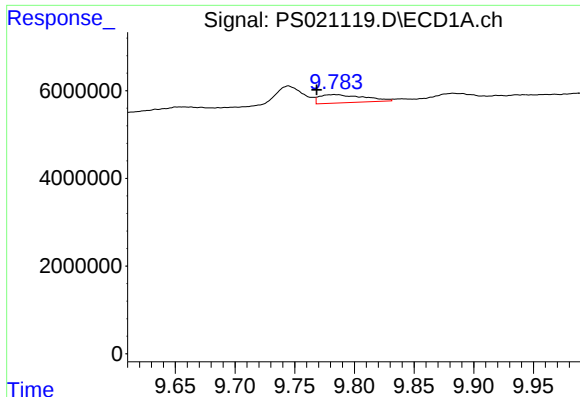

#15 Picloram


R.T.: 9.783 min
Delta R.T.: 0.015 min
Response: 4930611
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

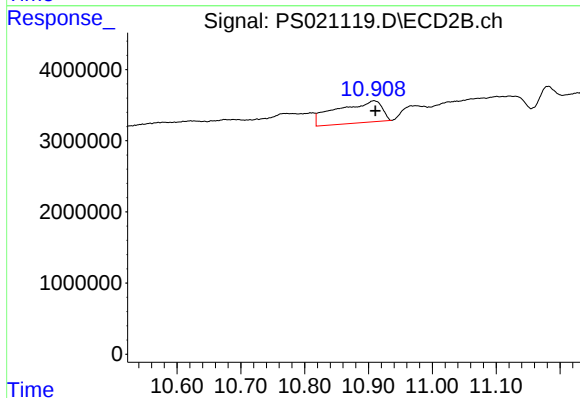


#15 Picloram

R.T.: 10.908 min
Delta R.T.: -0.002 min
Response: 14908390
Conc: 1.18 ng/ml

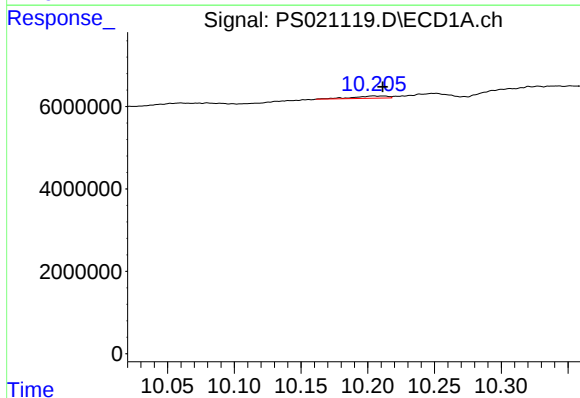

#16 DCPA

R.T.: 10.209 min
Delta R.T.: -0.002 min
Response: 995113
Conc: N.D.

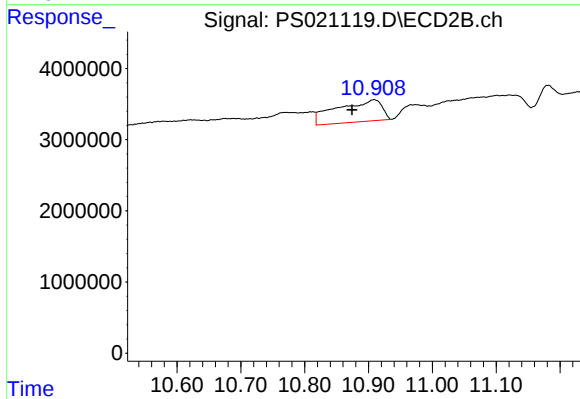

#16 DCPA

R.T.: 10.908 min
Delta R.T.: 0.034 min
Response: 14908390
Conc: 1.40 ng/ml