

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111022\
 Data File : PS021126.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2022 00:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 03:48:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.407	6.844	1212.6E6	853.5E6	581.008	617.057
Target Compounds							
1) T	Dalapon	2.505	0.000	425985	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.746	0.000	517104	0	<MDL	N.D. #
3) T	4-Nitroph...	6.245	0.000	11469026	0	7.625	N.D. #
5) T	DICAMBA	6.605f	7.005	7529631	2604700	<MDL	<MDL #
6) T	MCP	6.742	7.064f	8819327	1491472	1.351	<MDL #
7) T	MCPA	6.773f	0.000	8019548	0	<MDL	N.D. #
8) T	DICHLORPROP	7.115	7.659	59288	4656253	<MDL	3.024 #
9) T	2,4-D	0.000	7.877f	0	3565911	N.D.	1.904
10) T	Pentachlo...	7.573	8.361	2052633	4701878	<MDL	<MDL #
11) T	2,4,5-TP ...	8.119	8.759	10928600	5561257	<MDL	<MDL #
12) T	2,4,5-T	8.379	9.102	3273151	4687070	<MDL	<MDL #
13) T	2,4-DB	8.887	0.000	51455	0	<MDL	N.D. #
14) T	DINOSEB	9.942	9.939	1617345	33859951	<MDL	5.290 #
15) T	Picloram	9.786	10.908	10560799	29731917	<MDL	2.343 #
16) T	DCPA	10.197	10.908	1391521	29731917	<MDL	2.784 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111022\
Data File : PS021126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2022 00:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 03:48:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

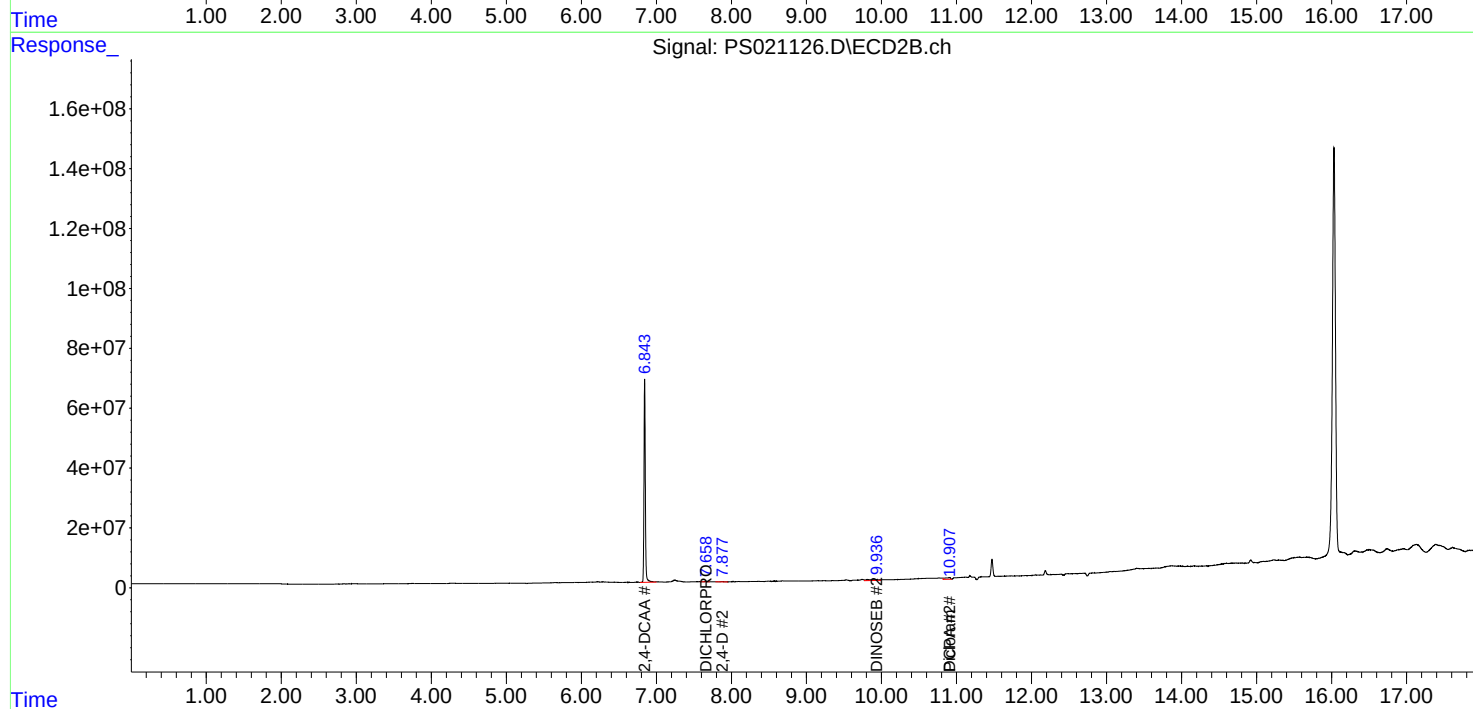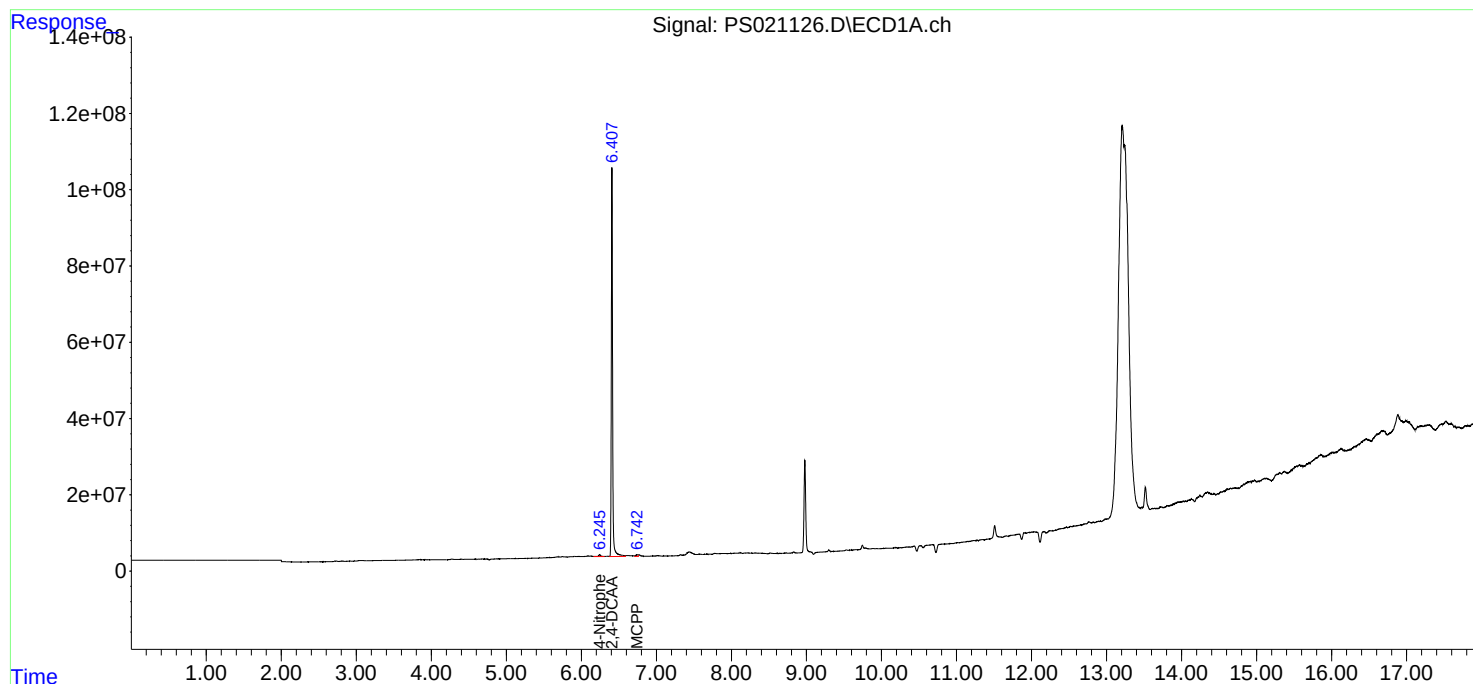


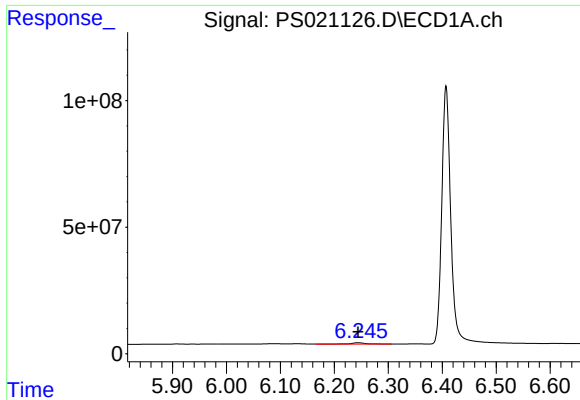

#3 4-Nitrophenol


R.T.: 6.245 min
Delta R.T.: 0.000 min
Response: 11469026
Conc: 7.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

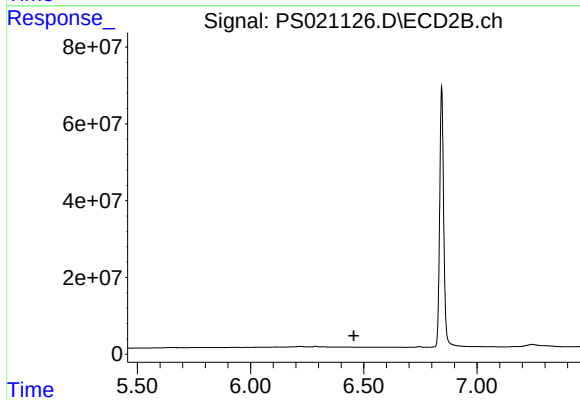


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

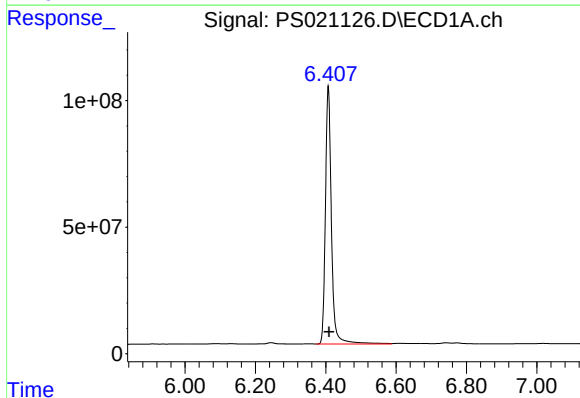


#4 2,4-DCAA

R.T.: 6.407 min
Delta R.T.: -0.002 min
Response: 1212607418
Conc: 581.01 ng/ml

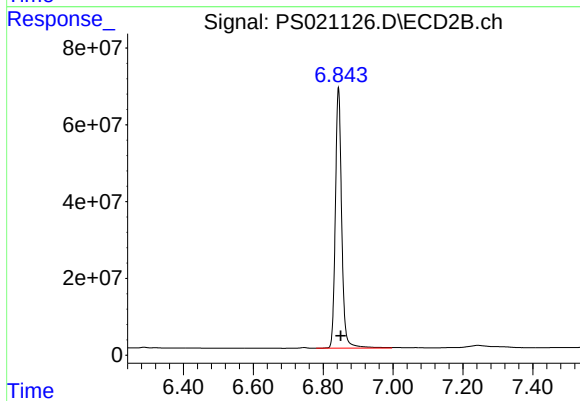

#4 2,4-DCAA


R.T.: 6.844 min
Delta R.T.: -0.006 min
Response: 853479313
Conc: 617.06 ng/ml

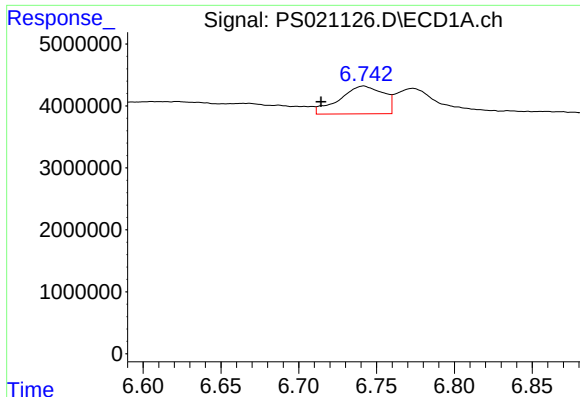

#6 MCP


R.T.: 6.742 min
Delta R.T.: 0.027 min
Response: 8819327
Conc: 1.35 ug/ml

Instrument :
ECD_S
ClientSampleId :

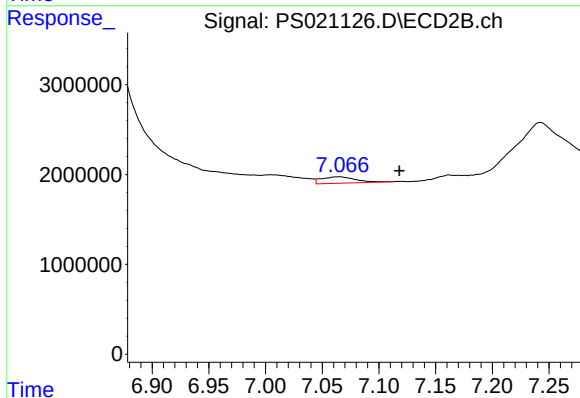


#6 MCP

R.T.: 7.064 min
Delta R.T.: -0.054 min
Response: 1491472
Conc: N.D.

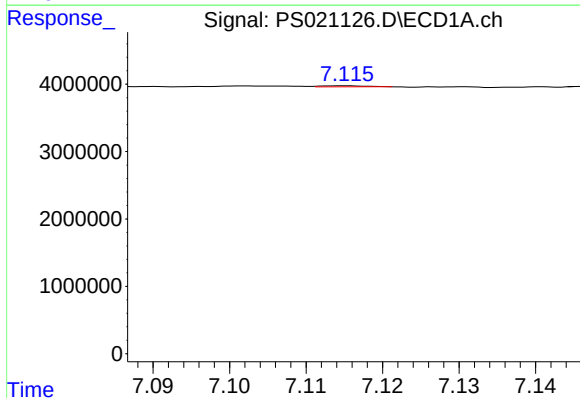


#8 DICHLORPROP

R.T.: 7.115 min
Delta R.T.: -0.039 min
Response: 59288
Conc: N.D.

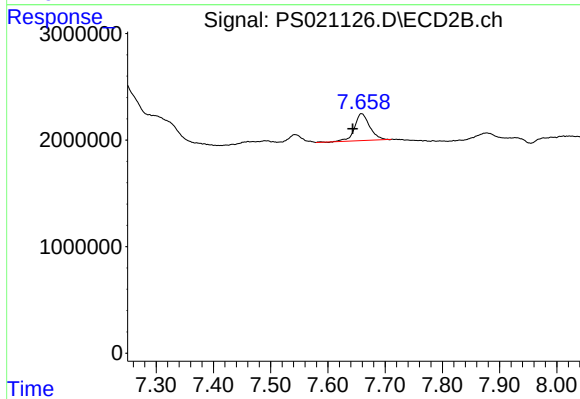

#8 DICHLORPROP


R.T.: 7.659 min
Delta R.T.: 0.016 min
Response: 4656253
Conc: 3.02 ng/ml

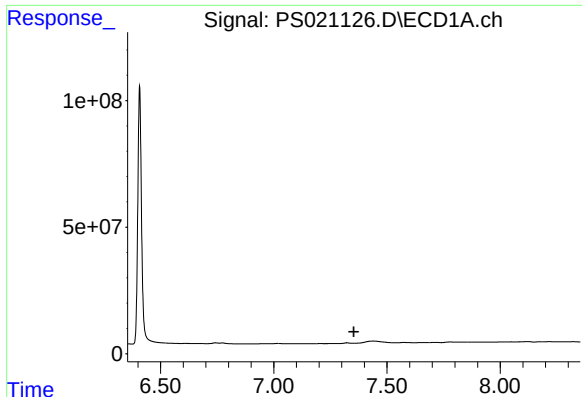

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.353 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

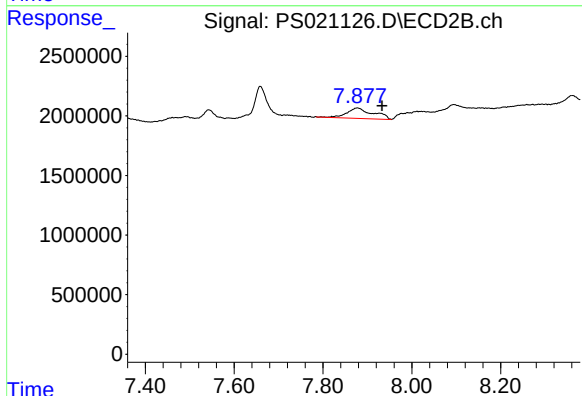


#9 2,4-D

R.T.: 7.877 min
Delta R.T.: -0.056 min
Response: 3565911
Conc: 1.90 ng/ml

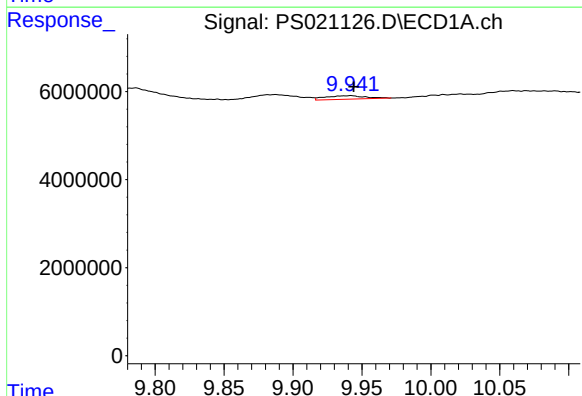


#14 DINOSEB

R.T.: 9.942 min
Delta R.T.: -0.003 min
Response: 1617345
Conc: N.D.

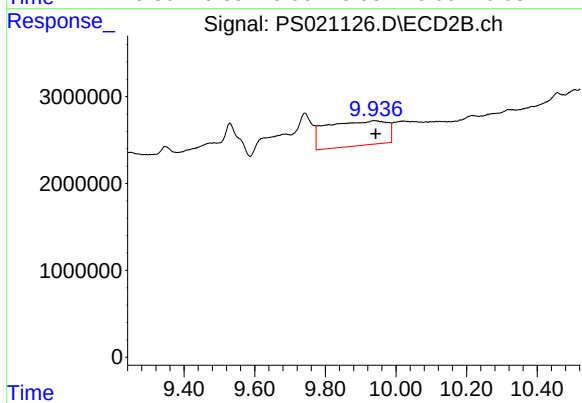

#14 DINOSEB


R.T.: 9.939 min
Delta R.T.: -0.003 min
Response: 33859951
Conc: 5.29 ng/ml

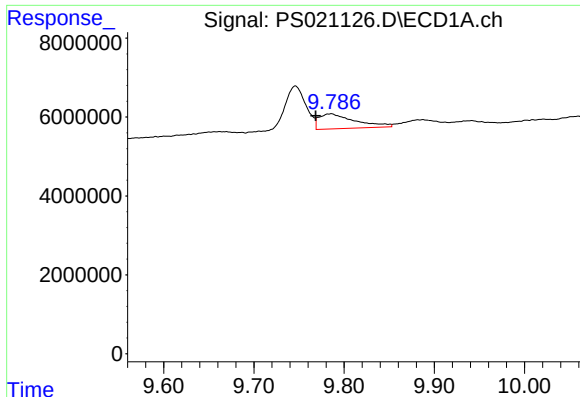

#15 Picloram


R.T.: 9.786 min
Delta R.T.: 0.017 min
Response: 10560799
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

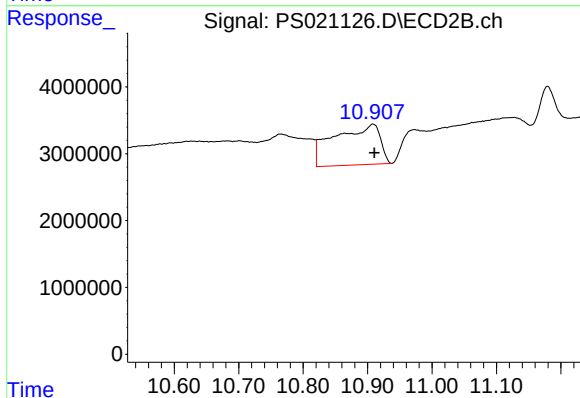


#15 Picloram

R.T.: 10.908 min
Delta R.T.: -0.002 min
Response: 29731917
Conc: 2.34 ng/ml

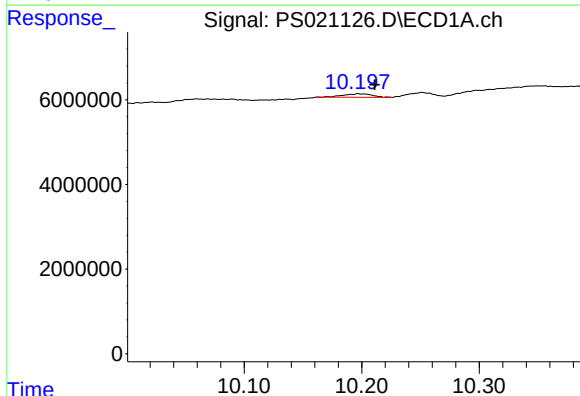

#16 DCPA

R.T.: 10.197 min
Delta R.T.: -0.014 min
Response: 1391521
Conc: N.D.

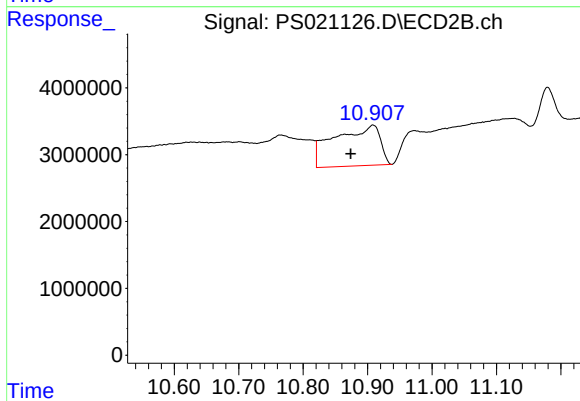

#16 DCPA

R.T.: 10.908 min
Delta R.T.: 0.034 min
Response: 29731917
Conc: 2.78 ng/ml