

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111023\
 Data File : PS024800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2023 07:54
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 13:02:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.357	6.775	1186.2E6	390.3E6	581.027	578.604
Target Compounds							
1) T	Dalapon	0.000	2.571	0	3518054	N.D.	3.339
3) T	4-Nitroph...	6.196	6.376	16992934	1511647	13.110	3.443 #
6) T	MCP	6.682	0.000	2980794	0	<MDL	N.D. #
7) T	MCPA	0.000	7.232	0	866749	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.565	0	4113832	N.D.	5.632
9) T	2,4-D	0.000	7.779f	0	2051710	N.D.	2.292
11) T	2,4,5-TP ...	0.000	8.614	0	743642	N.D.	<MDL
12) T	2,4,5-T	0.000	8.988	0	398197	N.D.	<MDL
13) T	2,4-DB	0.000	9.482	0	867172	N.D.	1.779
15) T	Picloram	9.684	10.771	57285723	18790814	3.221	3.093
16) T	DCPA	0.000	10.771	0	18790814	N.D.	3.739



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111023\
Data File : PS024800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2023 07:54
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 13:02:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

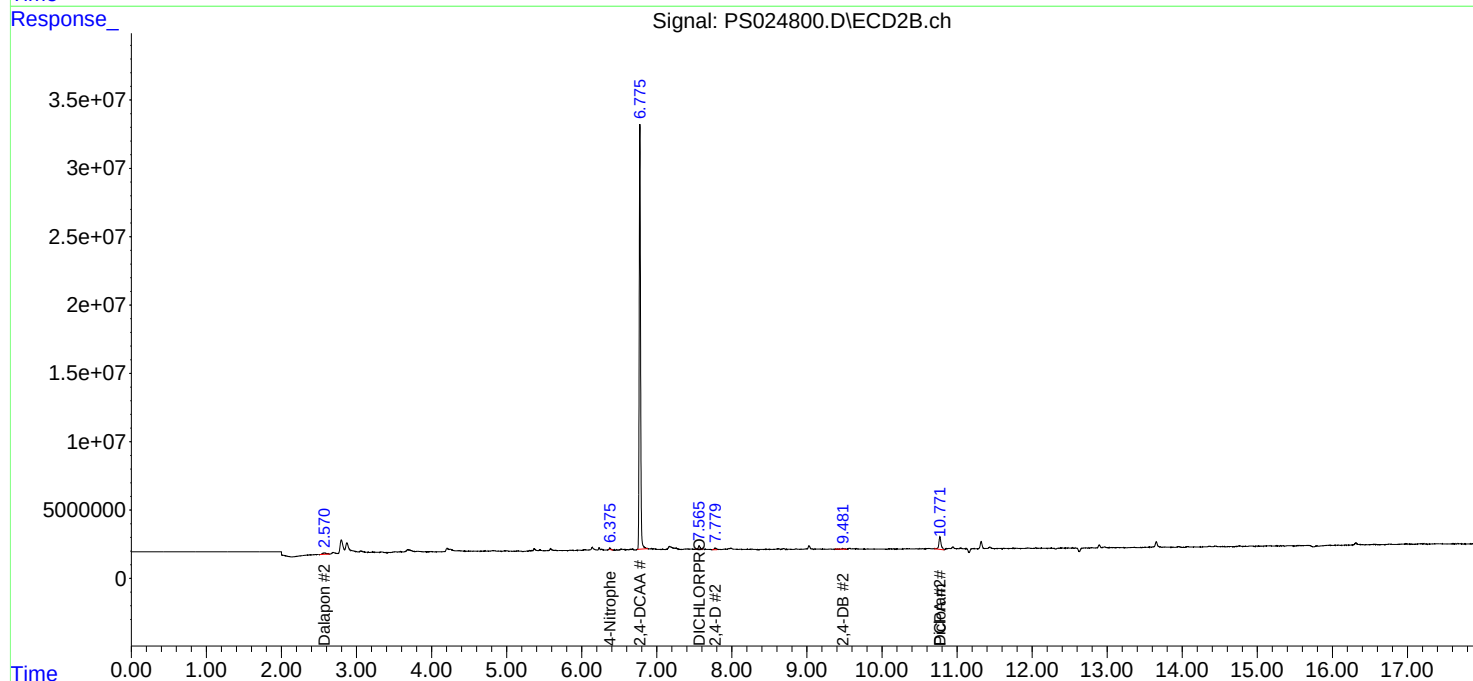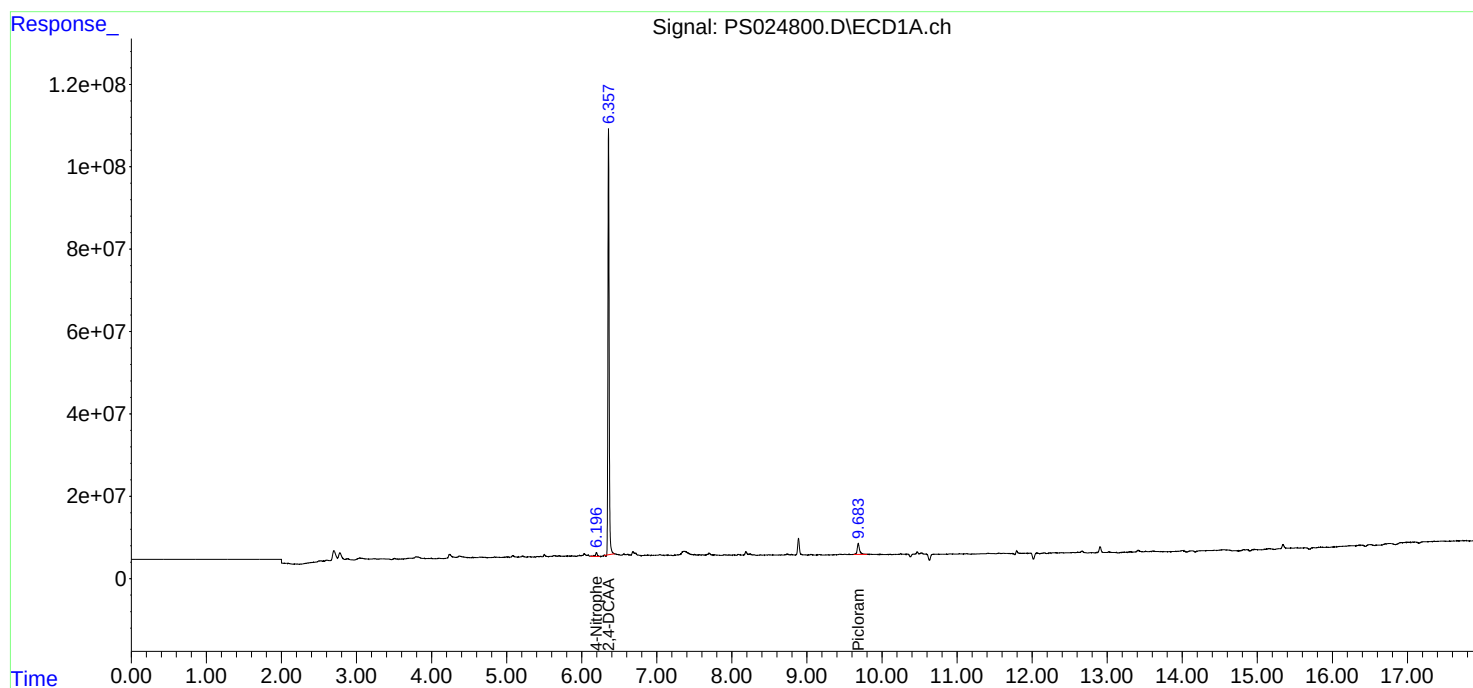


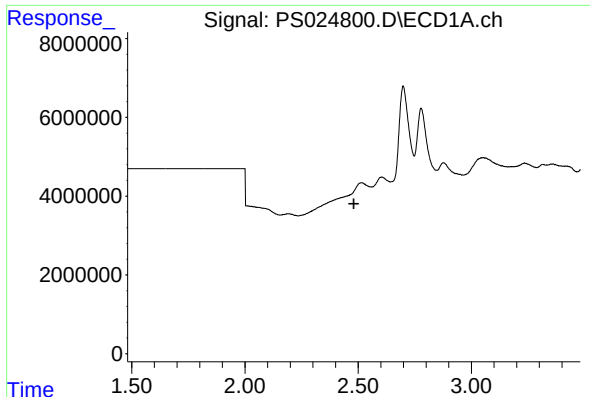

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

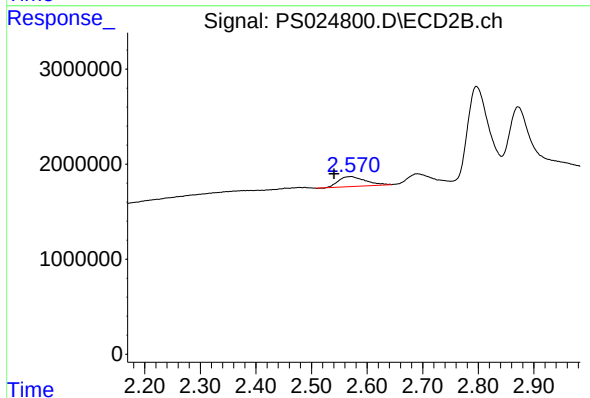


#1 Dalapon

R.T.: 2.571 min
Delta R.T.: 0.031 min
Response: 3518054
Conc: 3.34 ng/ml

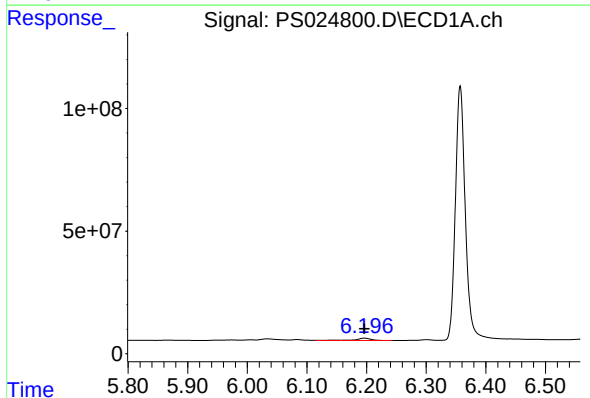


#3 4-Nitrophenol

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 16992934
Conc: 13.11 ng/ml

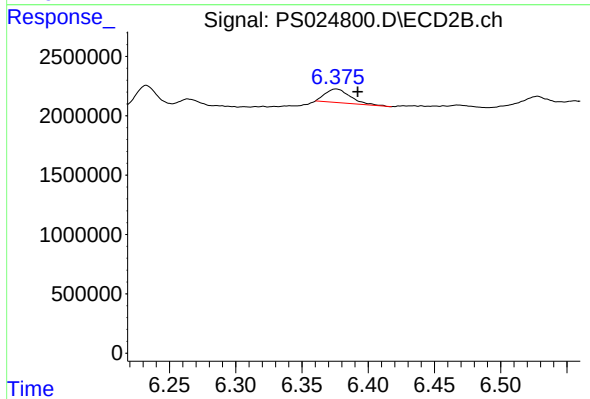

#3 4-Nitrophenol


R.T.: 6.376 min
Delta R.T.: -0.016 min
Response: 1511647
Conc: 3.44 ng/ml

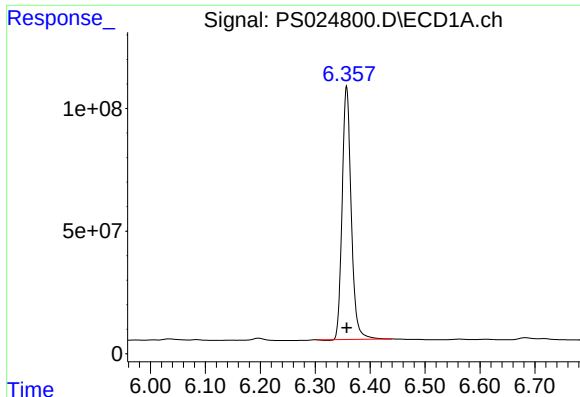

#4 2,4-DCAA


R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 1186168589
Conc: 581.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

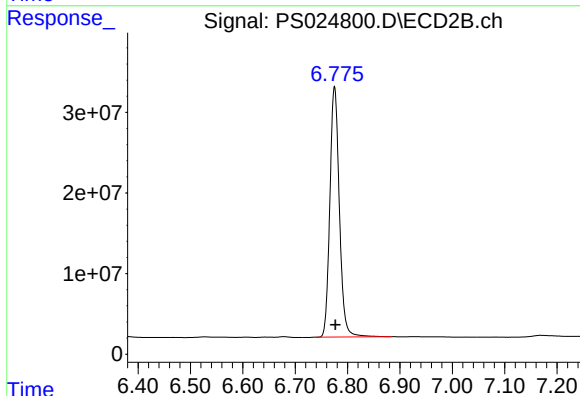


#4 2,4-DCAA

R.T.: 6.775 min
Delta R.T.: -0.002 min
Response: 390325527
Conc: 578.60 ng/ml

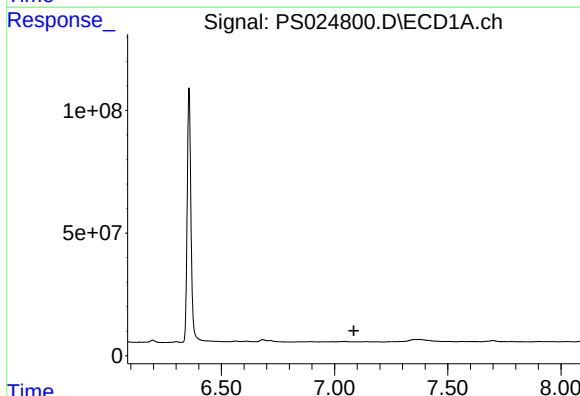


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.085 min
Response: 0
Conc: N.D.

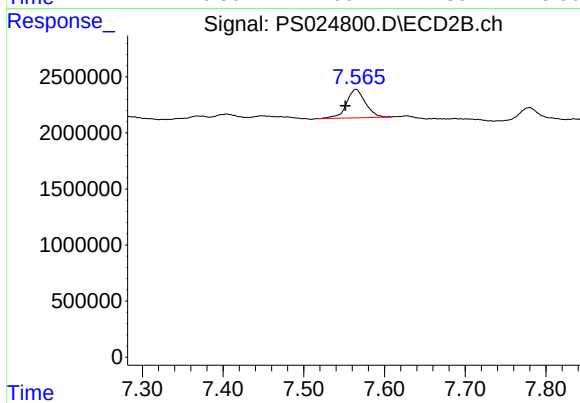

#8 DICHLORPROP


R.T.: 7.565 min
Delta R.T.: 0.013 min
Response: 4113832
Conc: 5.63 ng/ml

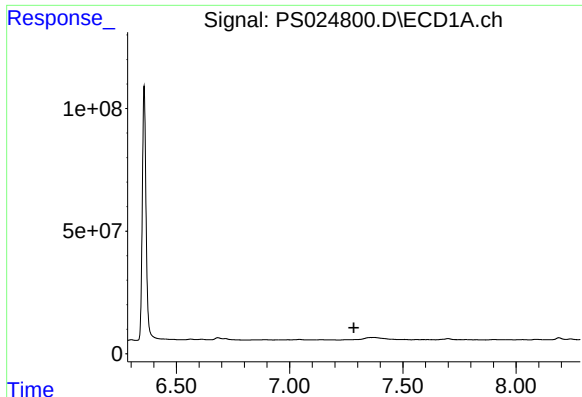

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

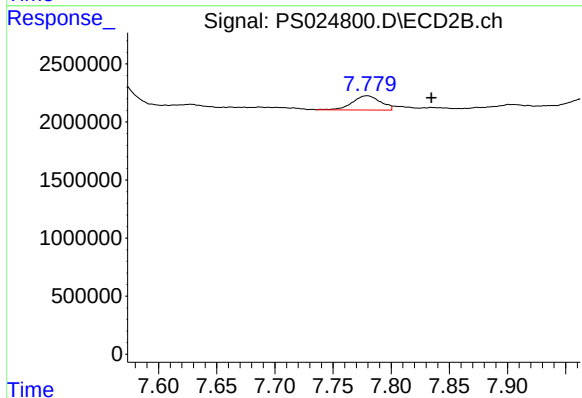


#9 2,4-D

R.T.: 7.779 min
Delta R.T.: -0.055 min
Response: 2051710
Conc: 2.29 ng/ml

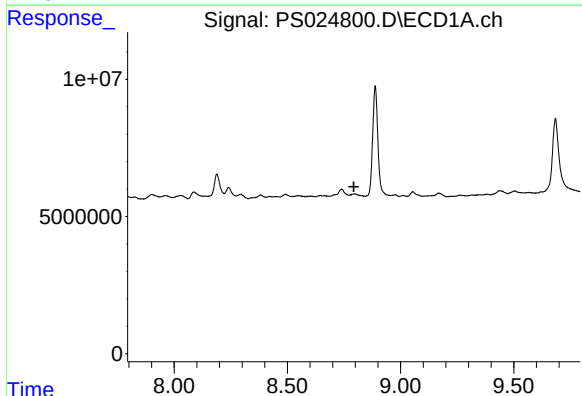


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

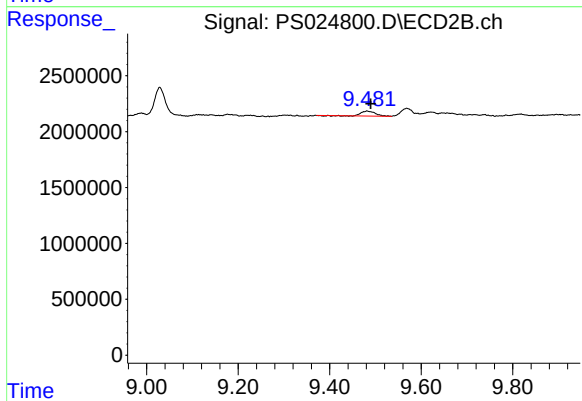

#13 2,4-DB


R.T.: 9.482 min
Delta R.T.: -0.008 min
Response: 867172
Conc: 1.78 ng/ml

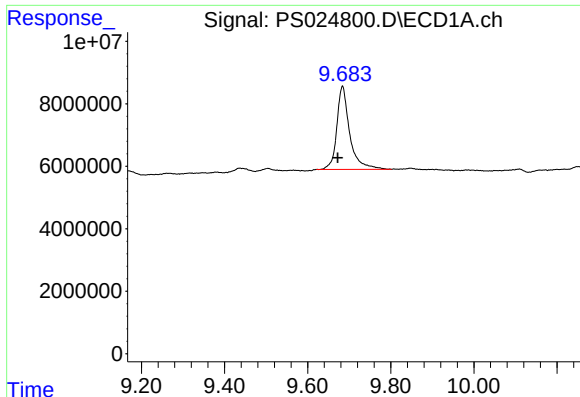

#15 Picloram


R.T.: 9.684 min
Delta R.T.: 0.011 min
Response: 57285723
Conc: 3.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

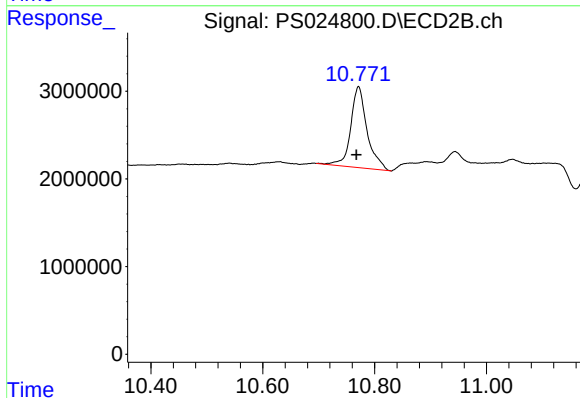


#15 Picloram

R.T.: 10.771 min
Delta R.T.: 0.003 min
Response: 18790814
Conc: 3.09 ng/ml

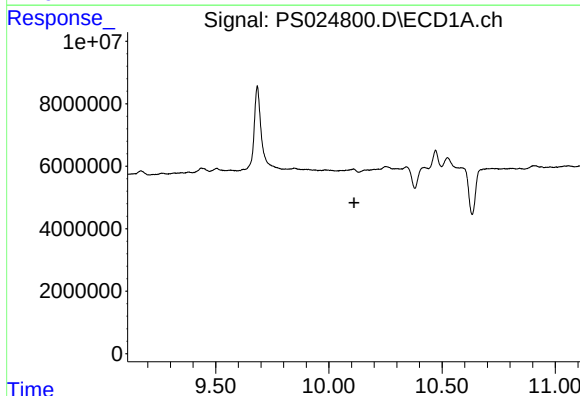

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.111 min
Response: 0
Conc: N.D.

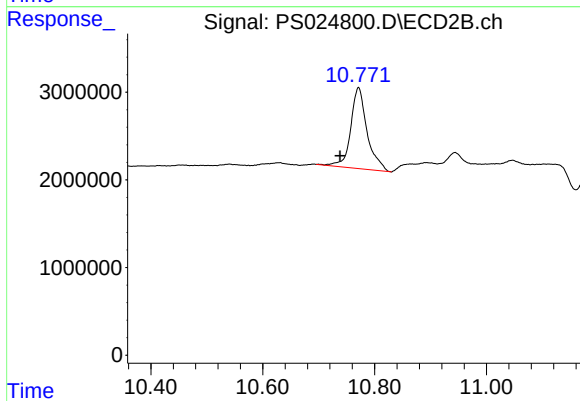

#16 DCPA

R.T.: 10.771 min
Delta R.T.: 0.033 min
Response: 18790814
Conc: 3.74 ng/ml