

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111023\
 Data File : PS024818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2023 17:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 02:15:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.356	6.775	1210.3E6	401.3E6	592.845	594.934
Target Compounds							
1) T	Dalapon	0.000	2.570	0	3316289	N.D.	3.148
3) T	4-Nitroph...	6.196	6.374	11327289	1421921	8.739	3.238 #
5) T	DICAMBA	0.000	6.976	0	1262306	N.D.	<MDL
6) T	MCP	6.680	6.976f	7435633	1262306	1.194	<MDL #
7) T	MCPA	0.000	7.232	0	6781014	N.D.	2.200
8) T	DICHLORPROP	0.000	7.563	0	6469937	N.D.	8.857
9) T	2,4-D	0.000	7.777f	0	1711932	N.D.	1.913
10) T	Pentachlo...	0.000	8.255	0	1751266	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.614	0	688454	N.D.	<MDL
12) T	2,4,5-T	0.000	8.987	0	616464	N.D.	<MDL
13) T	2,4-DB	0.000	9.478	0	1198362	N.D.	2.458
15) T	Picloram	9.680	10.771	10684703	8296056	<MDL	1.365 #
16) T	DCPA	0.000	10.771	0	8296056	N.D.	1.651



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111023\
Data File : PS024818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2023 17:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 02:15:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

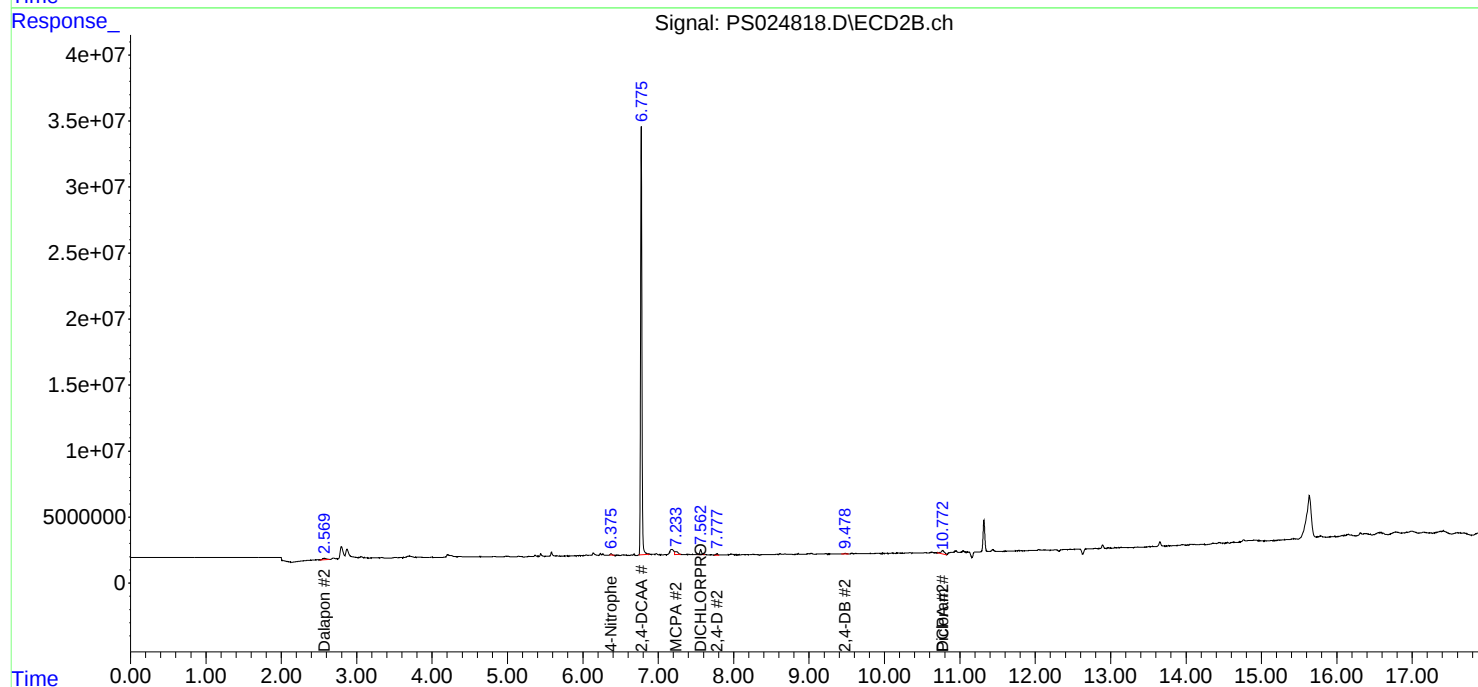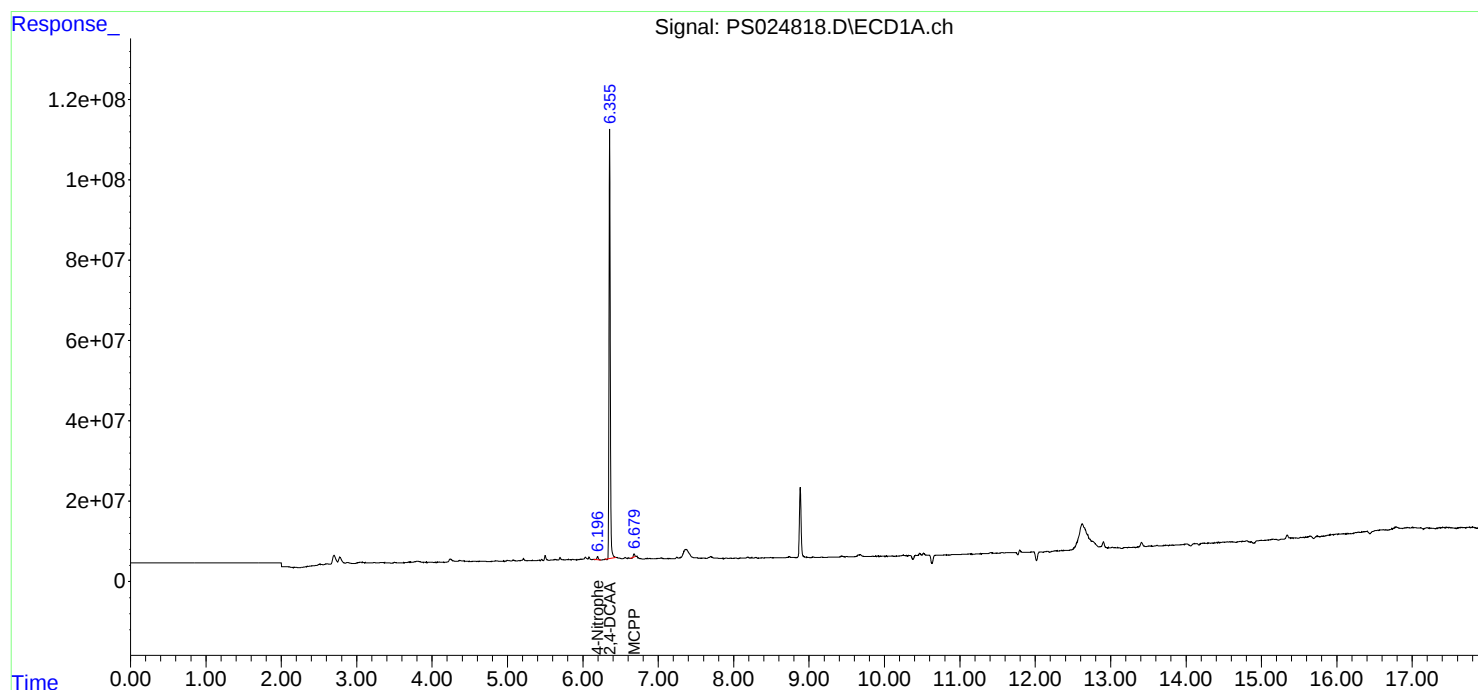


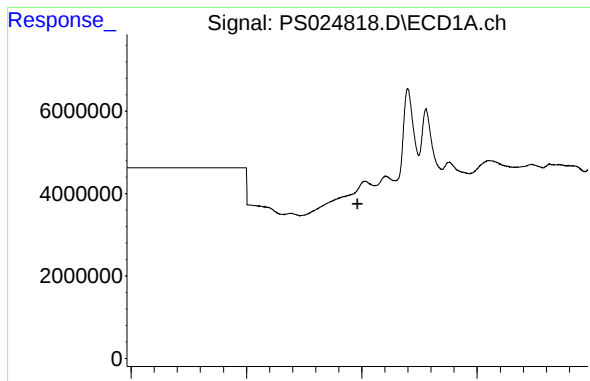

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

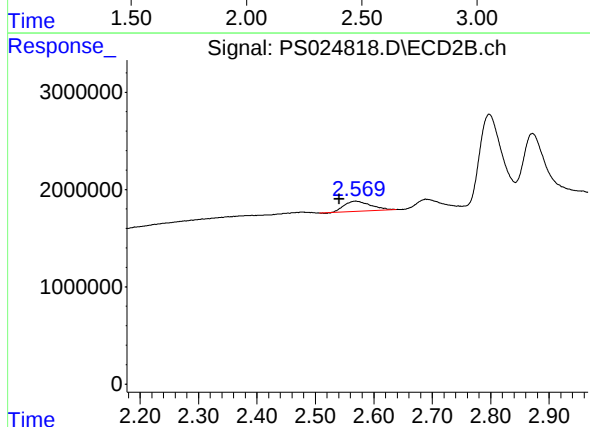


#1 Dalapon

R.T.: 2.570 min
Delta R.T.: 0.029 min
Response: 3316289
Conc: 3.15 ng/ml

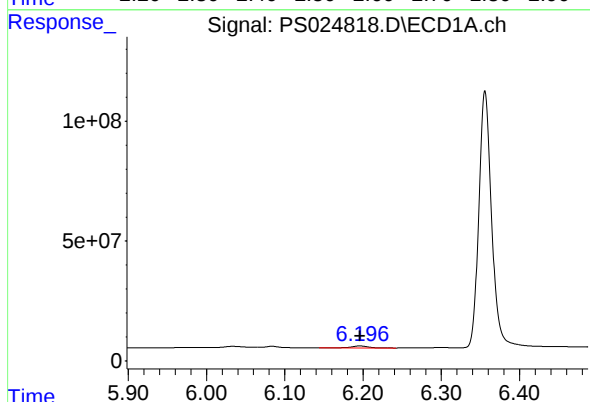


#3 4-Nitrophenol

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 11327289
Conc: 8.74 ng/ml

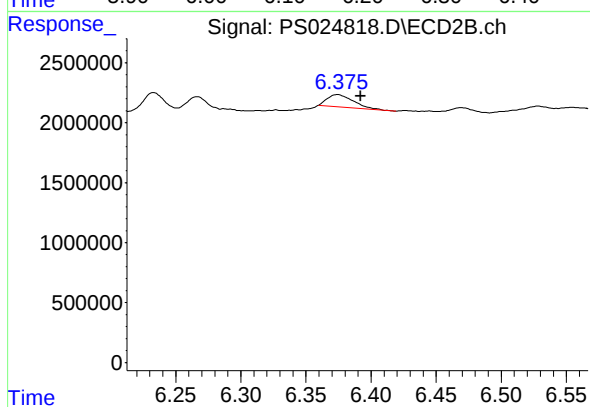

#3 4-Nitrophenol


R.T.: 6.374 min
Delta R.T.: -0.018 min
Response: 1421921
Conc: 3.24 ng/ml

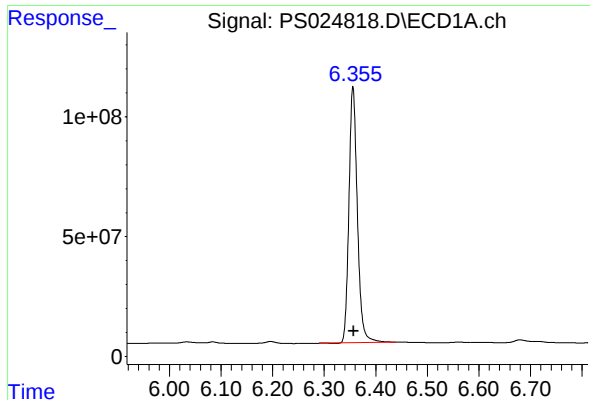

#4 2,4-DCAA


R.T.: 6.356 min
Delta R.T.: -0.001 min
Response: 1210294130
Conc: 592.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

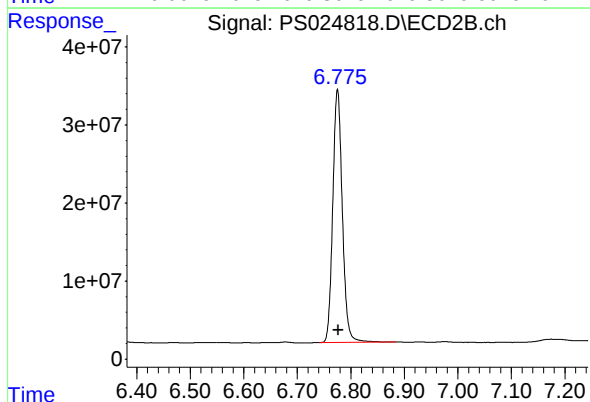


#4 2,4-DCAA

R.T.: 6.775 min
Delta R.T.: -0.001 min
Response: 401341671
Conc: 594.93 ng/ml

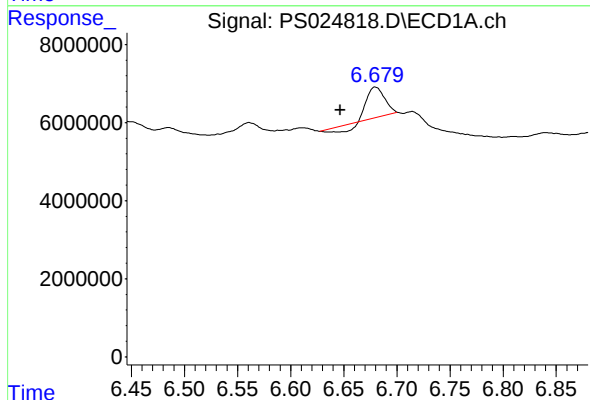


#6 MCPP

R.T.: 6.680 min
Delta R.T.: 0.033 min
Response: 7435633
Conc: 1.19 ug/ml

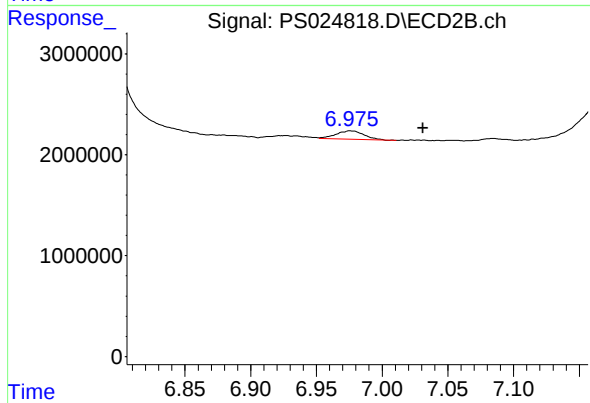

#6 MCPP


R.T.: 6.976 min
Delta R.T.: -0.055 min
Response: 1262306
Conc: N.D.

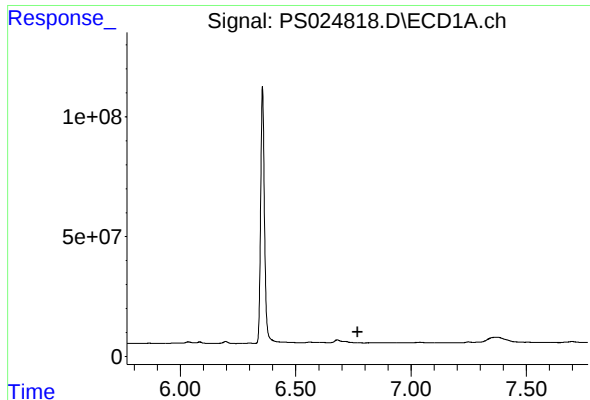

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.768 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

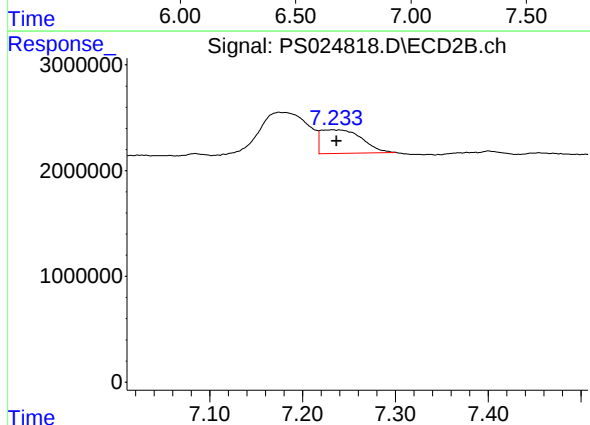


#7 MCPA

R.T.: 7.232 min
Delta R.T.: -0.004 min
Response: 6781014
Conc: 2.20 ug/ml

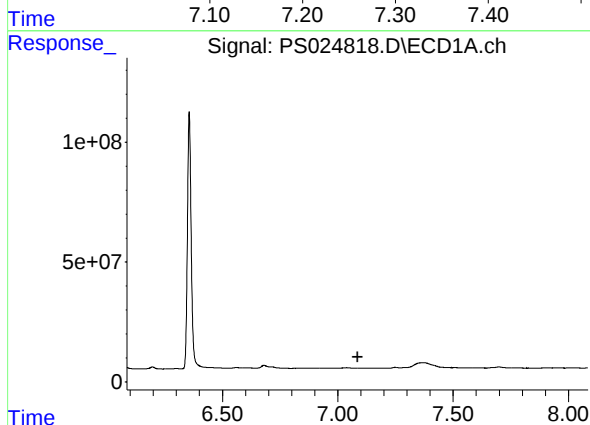


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

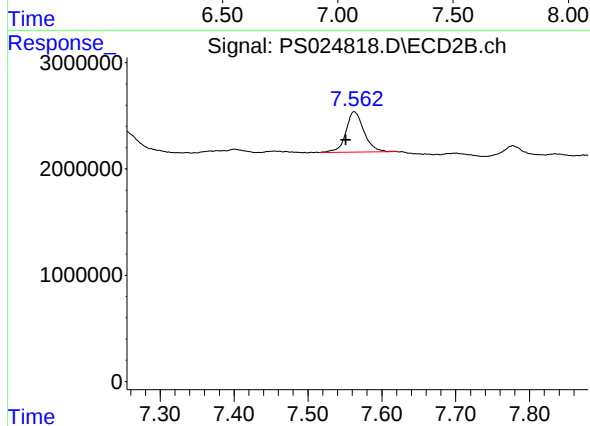

#8 DICHLORPROP


R.T.: 7.563 min
Delta R.T.: 0.011 min
Response: 6469937
Conc: 8.86 ng/ml

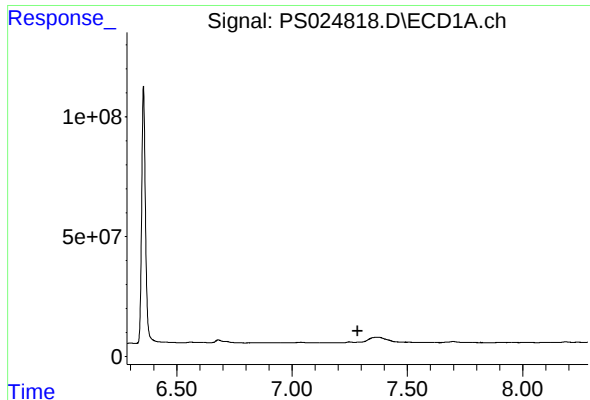

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

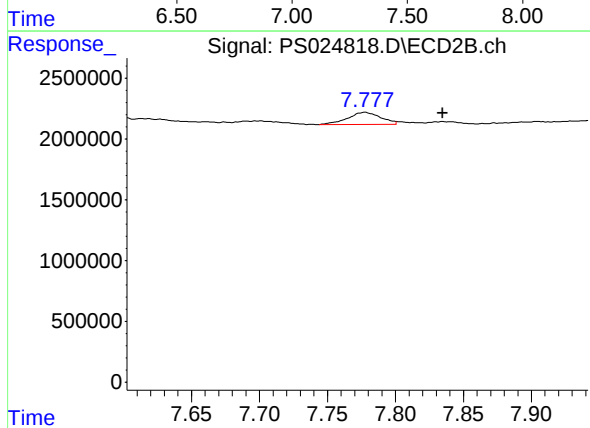


#9 2,4-D

R.T.: 7.777 min
Delta R.T.: -0.057 min
Response: 1711932
Conc: 1.91 ng/ml

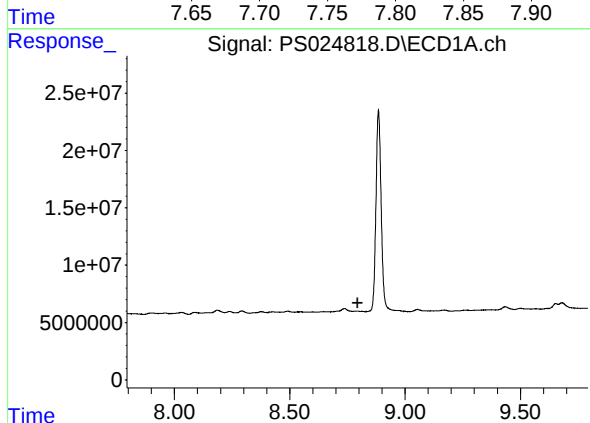


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

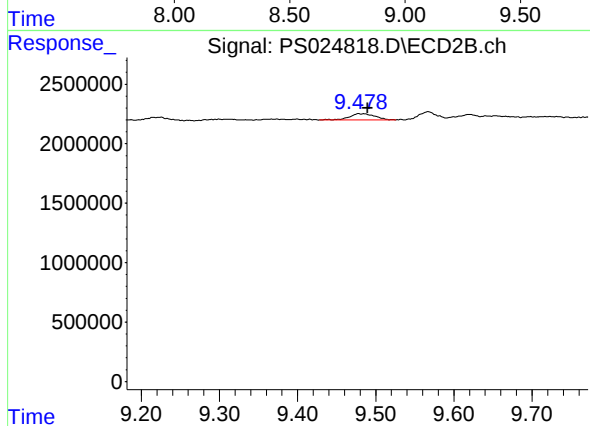

#13 2,4-DB


R.T.: 9.478 min
Delta R.T.: -0.012 min
Response: 1198362
Conc: 2.46 ng/ml

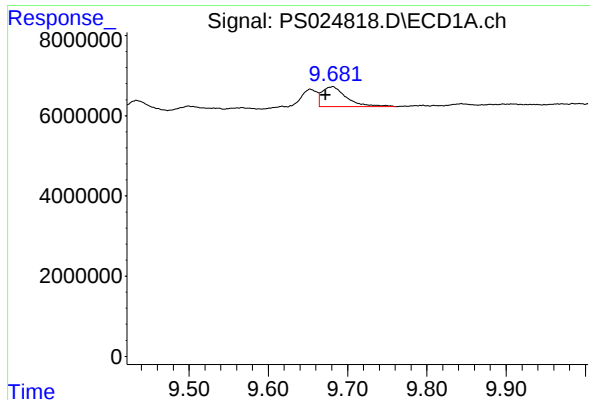

#15 Picloram


R.T.: 9.680 min
Delta R.T.: 0.008 min
Response: 10684703
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

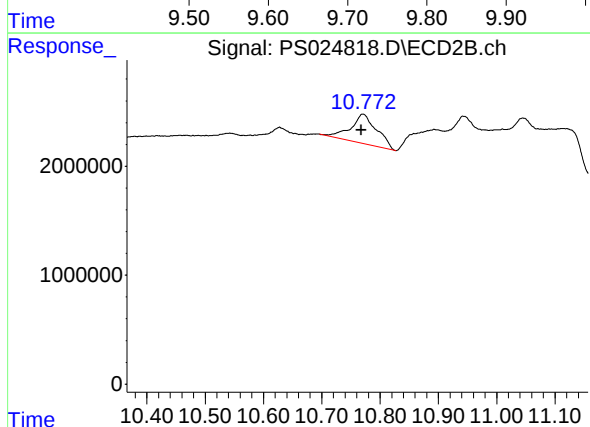


#15 Picloram

R.T.: 10.771 min
Delta R.T.: 0.003 min
Response: 8296056
Conc: 1.37 ng/ml

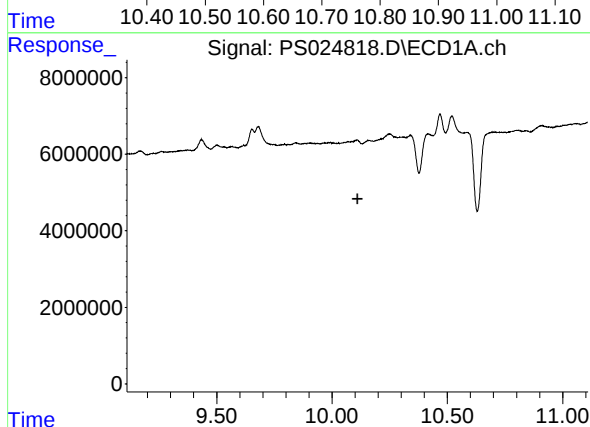

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.111 min
Response: 0
Conc: N.D.

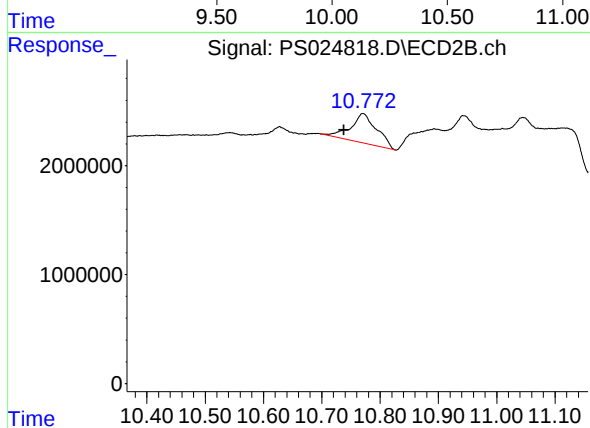

#16 DCPA

R.T.: 10.771 min
Delta R.T.: 0.033 min
Response: 8296056
Conc: 1.65 ng/ml