

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111025\
 Data File : PS032329.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2025 15:05
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 01:49:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.290	7.620	1956.6E6	2229.8E6	431.805	611.664 #
Target Compounds							
1) T	Dalapon	0.000	2.557f	0	42679010	N.D.	6.137
2) T	3,5-DICHL...	6.447	6.615f	22338591	3711677	3.455	<MDL #
3) T	4-Nitroph...	7.070f	0.000	5321232	0	3.964	N.D. #
6) T	MCP	0.000	7.904	0	128.6E6	N.D.	9.670
7) T	MCPA	7.782	0.000	286117	0	<MDL	N.D. #
9) T	2,4-D	8.393	0.000	2183908	0	<MDL	N.D. #
10) T	Pentachlo...	8.714	9.363	10186286	4400694	<MDL	<MDL #
11) T	2,4,5-TP ...	9.298	9.774f	7983592	7876973	<MDL	<MDL #
12) T	2,4,5-T	9.604f	10.188	9807486	1565163	<MDL	<MDL #
13) T	2,4-DB	10.164	0.000	1076590	0	<MDL	N.D. #
14) T	DINOSEB	11.353	11.116	67668460	3333871	3.252	<MDL #
15) T	Picloram	11.140f	12.182f	194107	46736555	<MDL	1.257 #
16) T	DCPA	11.655	12.182f	8264282	46736555	<MDL	1.467 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111025\
Data File : PS032329.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2025 15:05
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 01:49:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

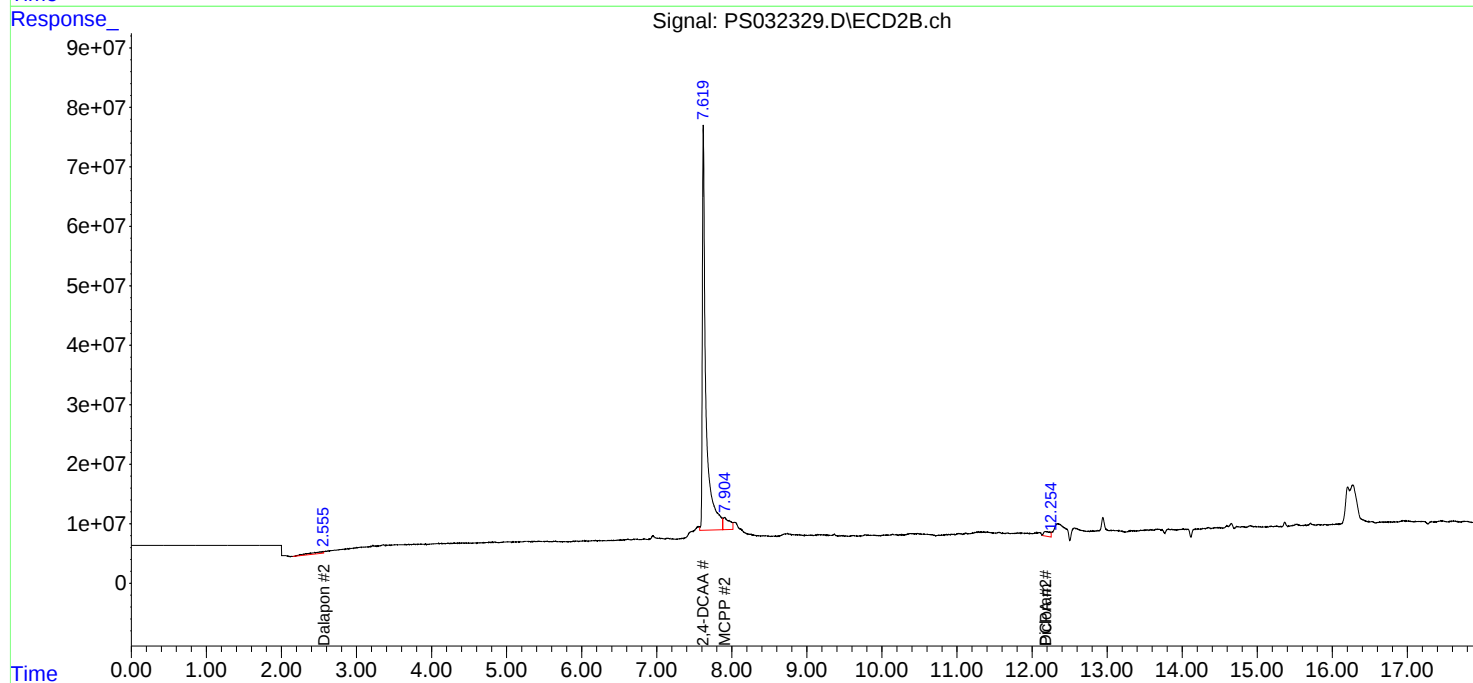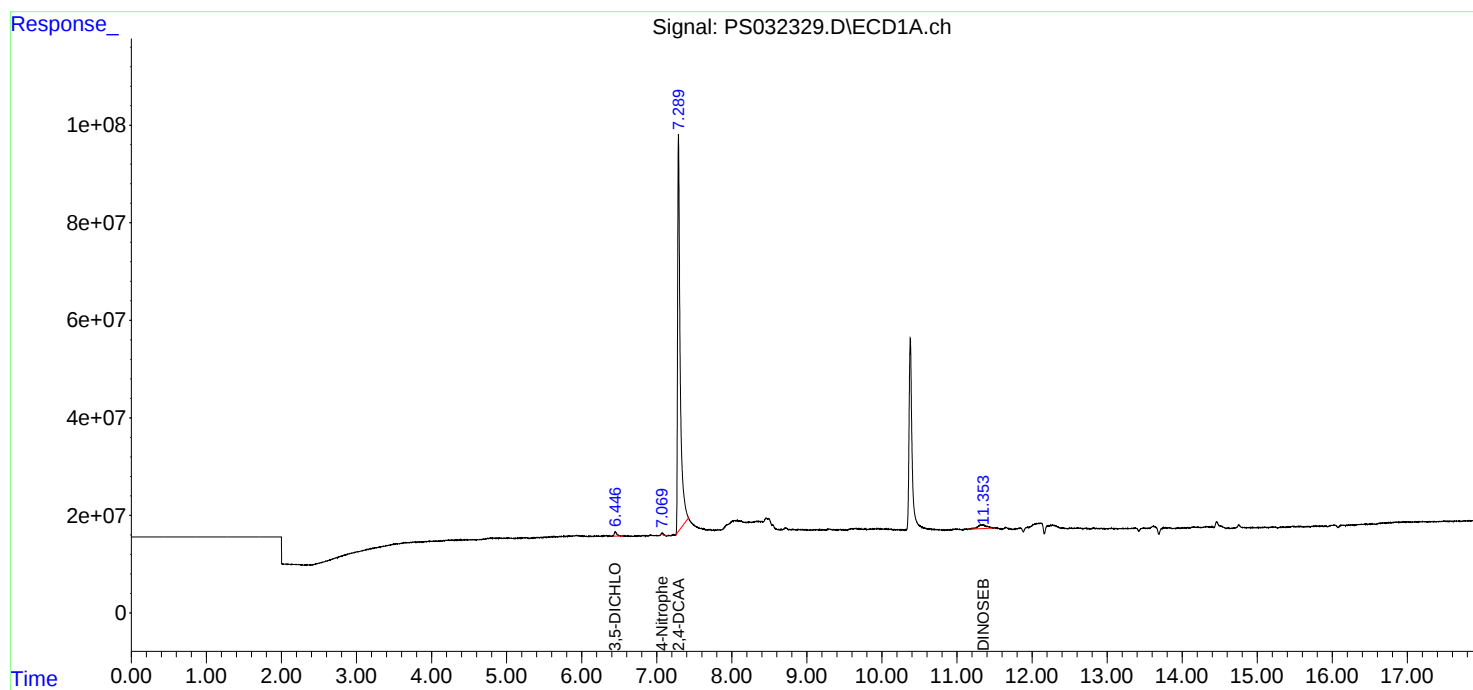


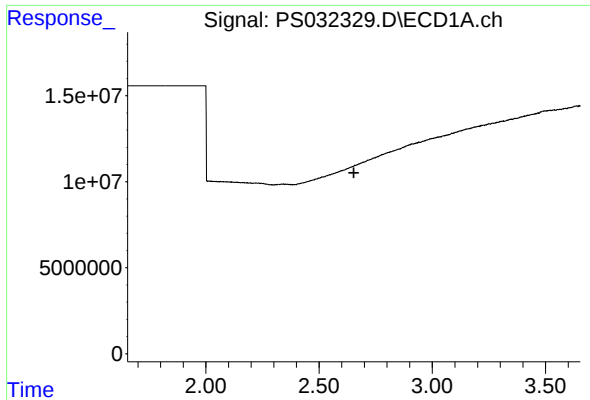

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.654 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

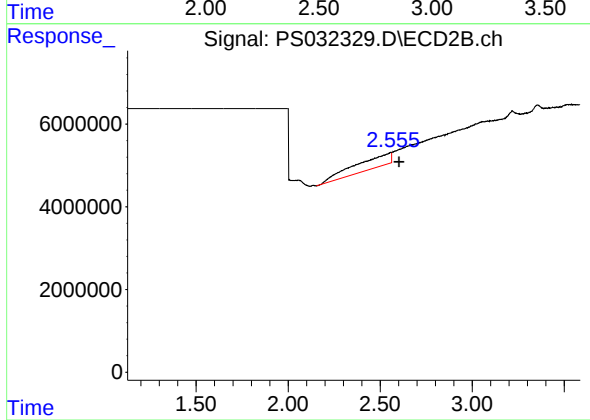


#1 Dalapon

R.T.: 2.557 min
Delta R.T.: -0.046 min
Response: 42679010
Conc: 6.14 ng/ml

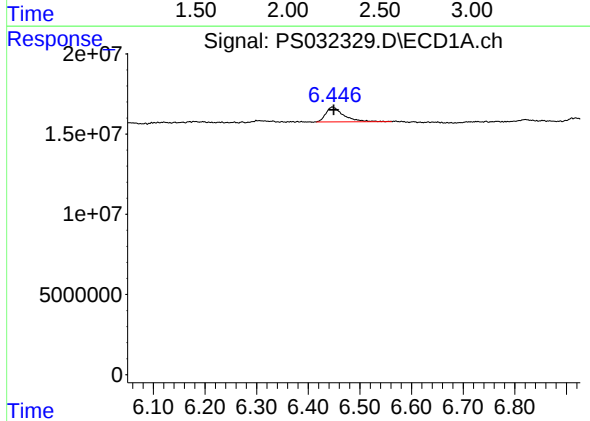


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.447 min
Delta R.T.: -0.002 min
Response: 22338591
Conc: 3.45 ng/ml

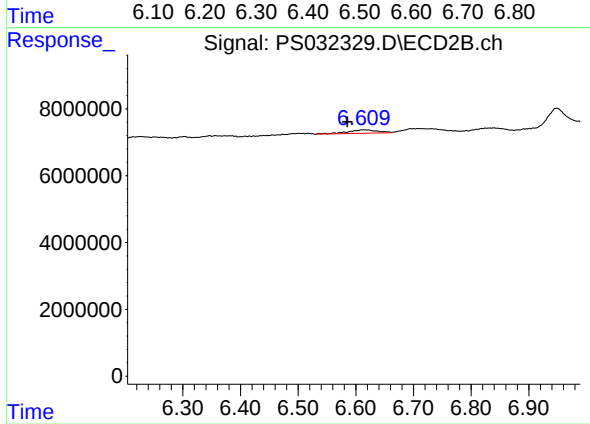

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.615 min
Delta R.T.: 0.030 min
Response: 3711677
Conc: N.D.

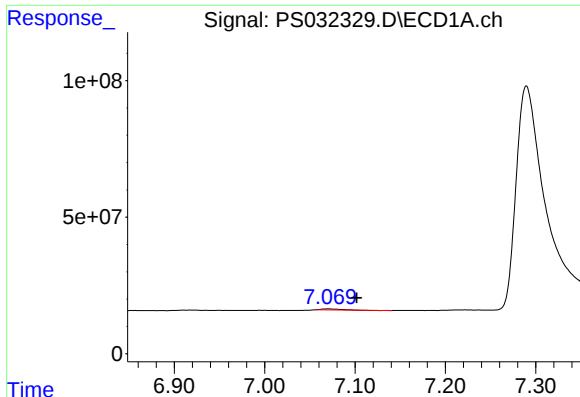

#3 4-Nitrophenol


R.T.: 7.070 min
Delta R.T.: -0.031 min
Response: 5321232
Conc: 3.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

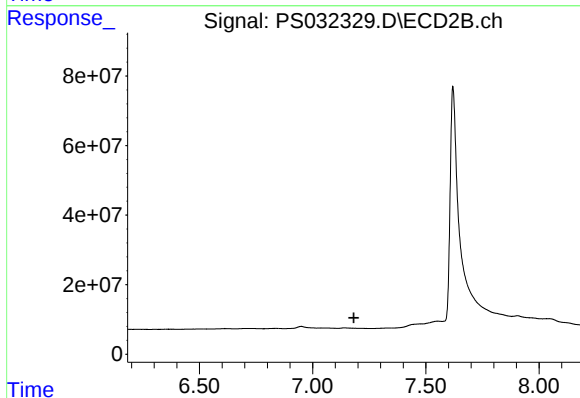


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.182 min
Response: 0
Conc: N.D.

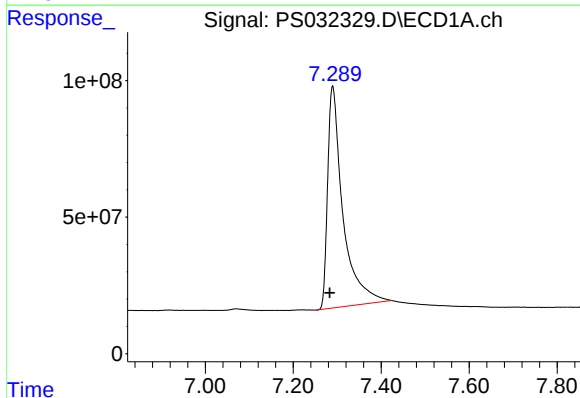


#4 2,4-DCAA

R.T.: 7.290 min
Delta R.T.: 0.006 min
Response: 1956628248
Conc: 431.81 ng/ml

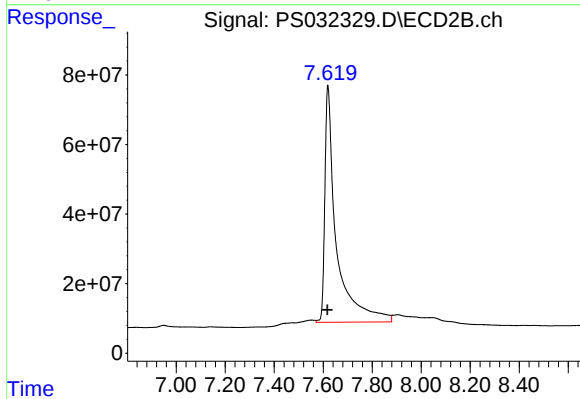

#4 2,4-DCAA


R.T.: 7.620 min
Delta R.T.: 0.002 min
Response: 2229818334
Conc: 611.66 ng/ml

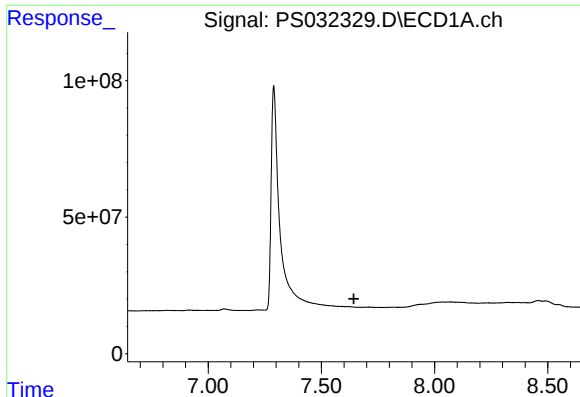

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.644 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

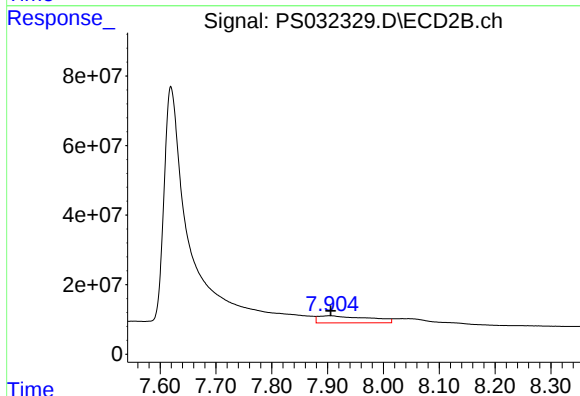


#6 MCP

R.T.: 7.904 min
Delta R.T.: -0.001 min
Response: 128620220
Conc: 9.67 ug/ml

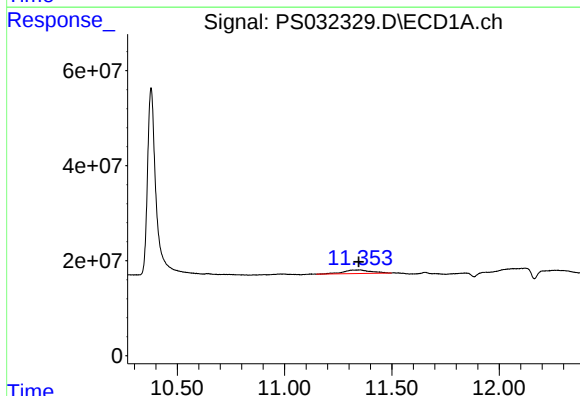


#14 DINOSEB

R.T.: 11.353 min
Delta R.T.: 0.008 min
Response: 67668460
Conc: 3.25 ng/ml

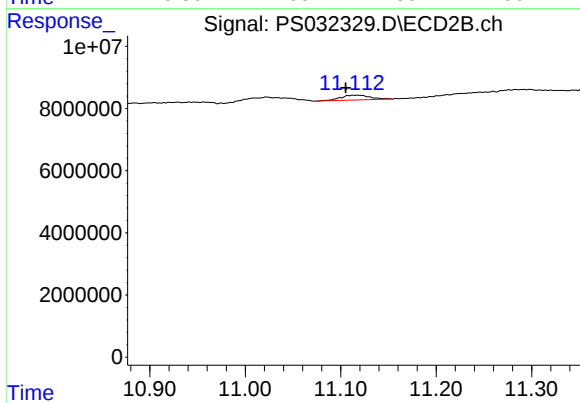

#14 DINOSEB


R.T.: 11.116 min
Delta R.T.: 0.011 min
Response: 3333871
Conc: N.D.

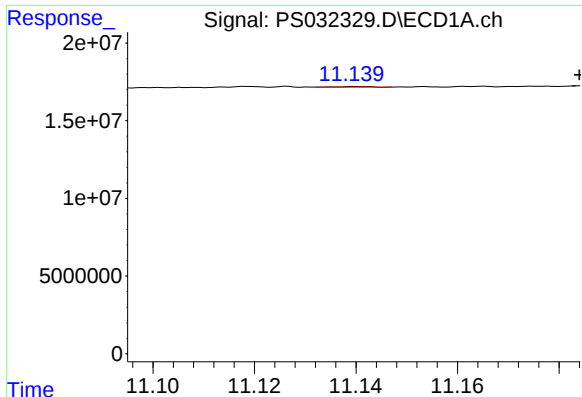

#15 Picloram


R.T.: 11.140 min
Delta R.T.: -0.044 min
Response: 194107
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

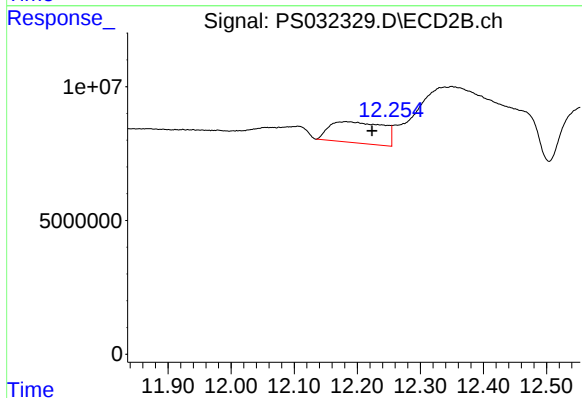


#15 Picloram

R.T.: 12.182 min
Delta R.T.: -0.041 min
Response: 46736555
Conc: 1.26 ng/ml

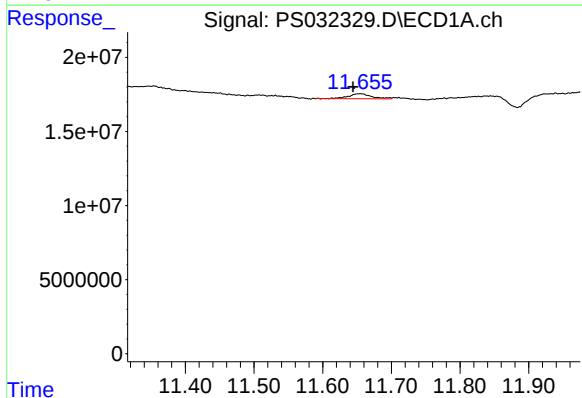

#16 DCPA

R.T.: 11.655 min
Delta R.T.: 0.010 min
Response: 8264282
Conc: N.D.

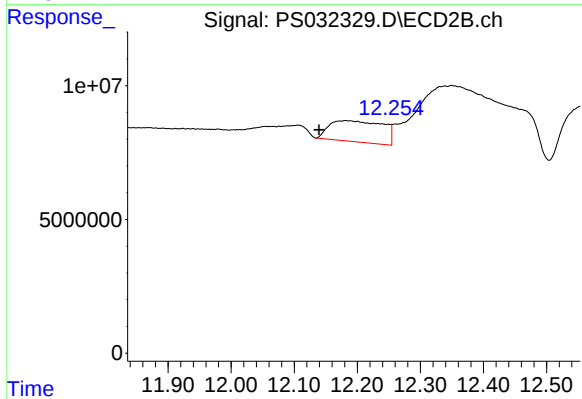

#16 DCPA

R.T.: 12.182 min
Delta R.T.: 0.042 min
Response: 46736555
Conc: 1.47 ng/ml