

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111119\
 Data File : PS007646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2019 12:47
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 16:23:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.433	5.155	576.8E6	309.1E6	418.805	439.941
Target Compounds							
7) T	MCPA	0.000	5.477	0 43744173		N.D.	14.554
15) T	Picloram	8.971	8.905	128.7E6	94127586	11.588	16.066 #
16) T	DCPA	0.000	8.905	0 94127586		N.D.	18.014



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111119\
Data File : PS007646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2019 12:47
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 16:23:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

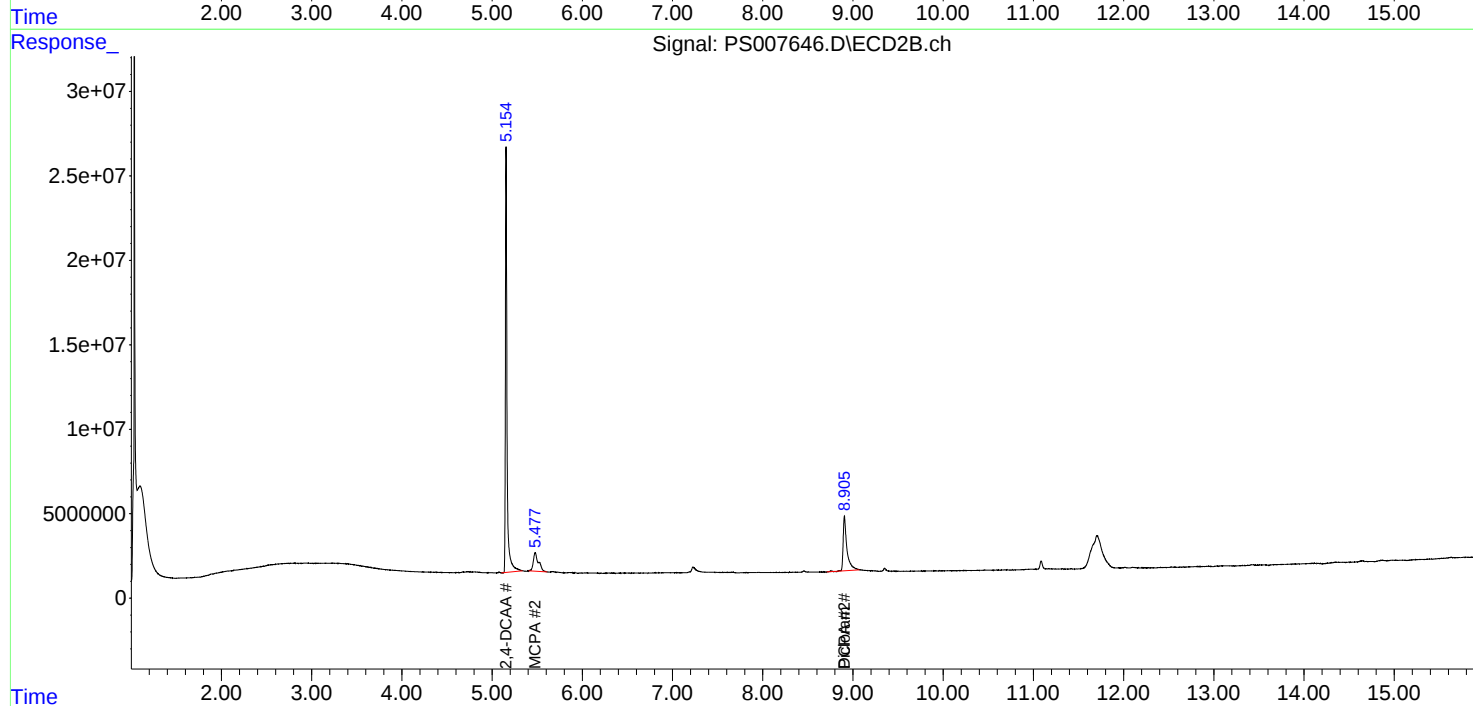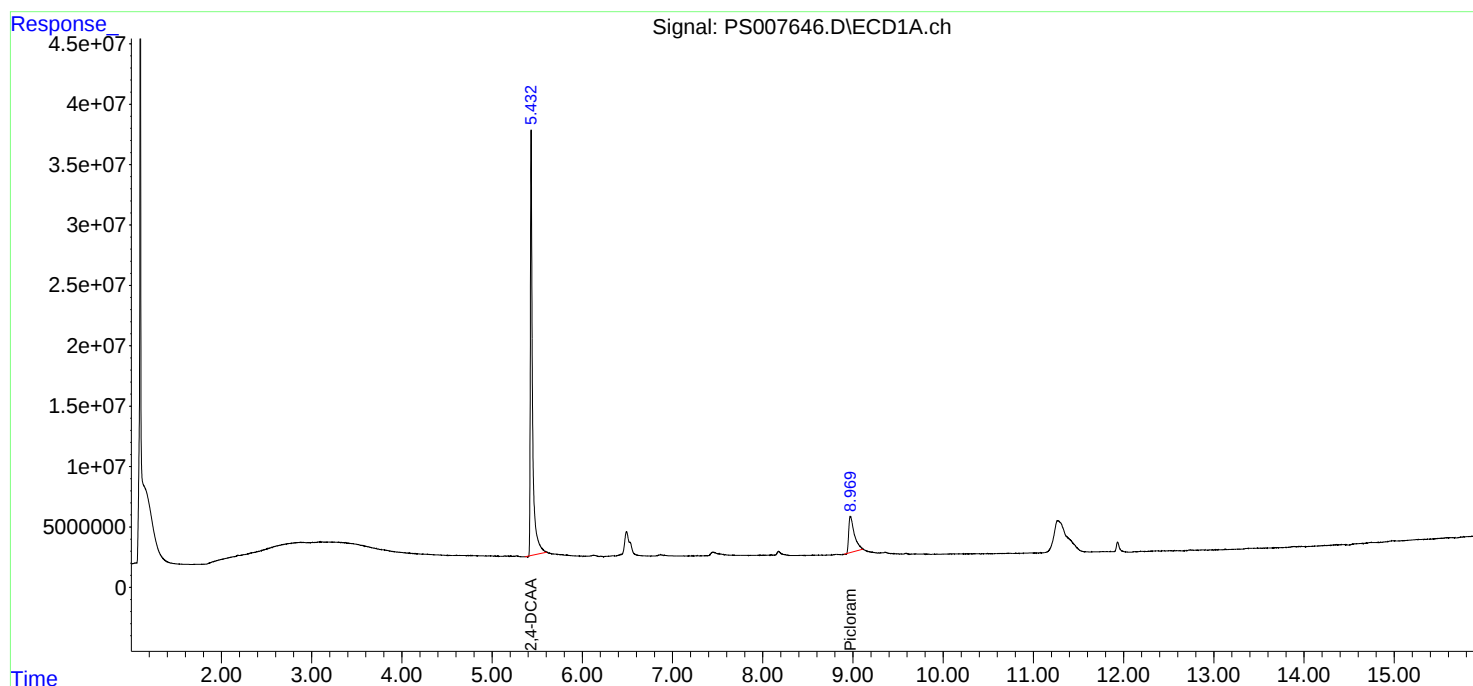


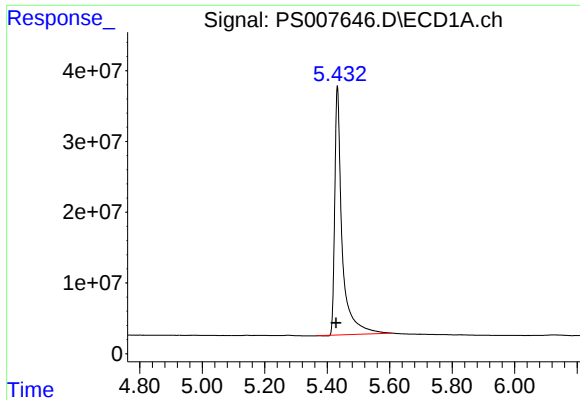

#4 2,4-DCAA


R.T.: 5.433 min
Delta R.T.: 0.004 min
Response: 576771462
Conc: 418.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

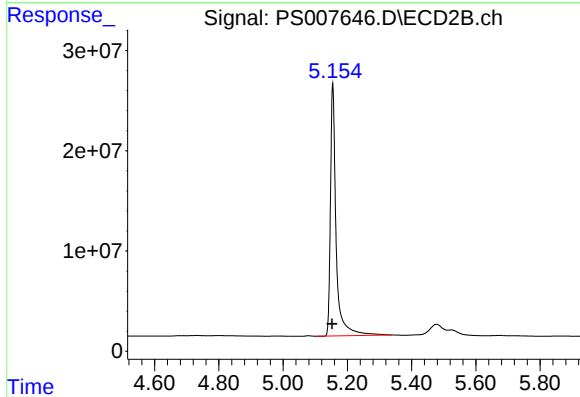


#4 2,4-DCAA

R.T.: 5.155 min
Delta R.T.: 0.002 min
Response: 309086661
Conc: 439.94 ng/ml

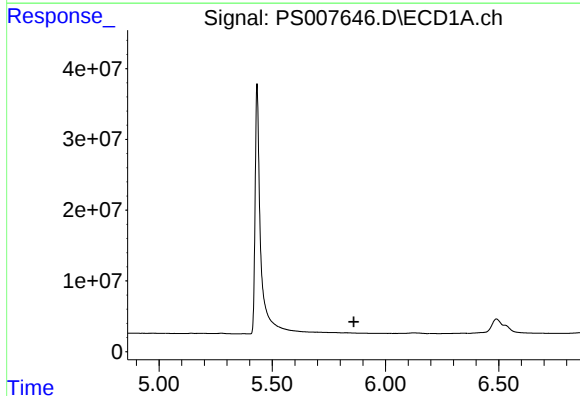


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.860 min
Response: 0
Conc: N.D.

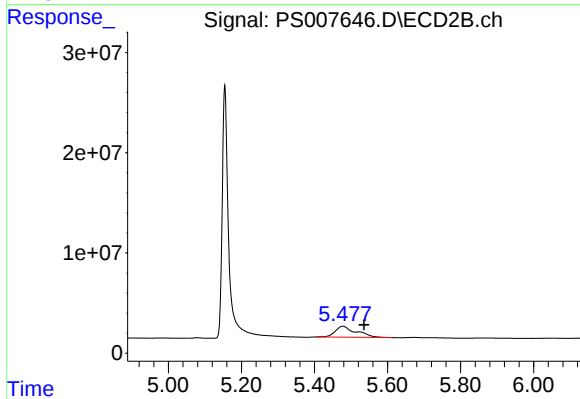

#7 MCPA


R.T.: 5.477 min
Delta R.T.: -0.059 min
Response: 43744173
Conc: 14.55 ug/ml

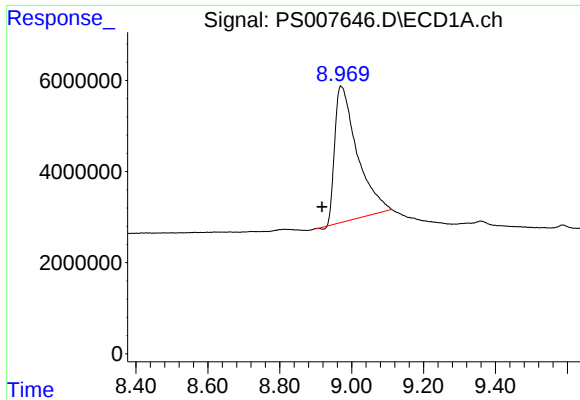

#15 Picloram


R.T.: 8.971 min
Delta R.T.: 0.053 min
Response: 128666279
Conc: 11.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

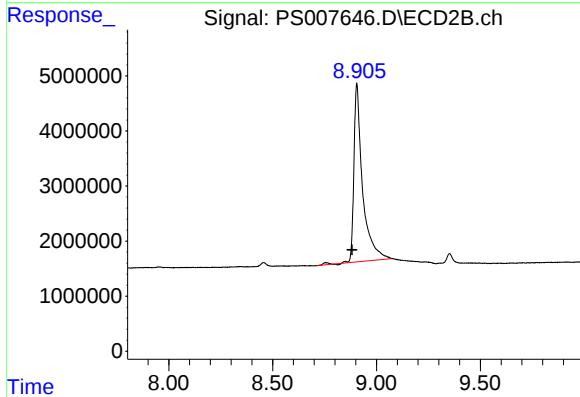


#15 Picloram

R.T.: 8.905 min
Delta R.T.: 0.023 min
Response: 94127586
Conc: 16.07 ng/ml

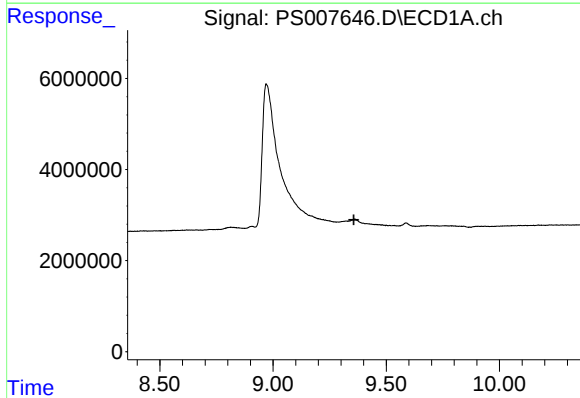

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.357 min
Response: 0
Conc: N.D.

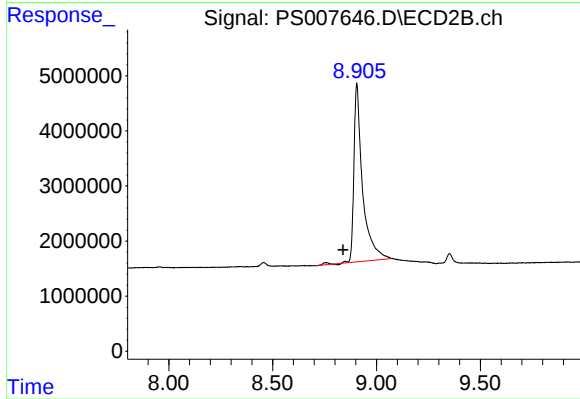

#16 DCPA

R.T.: 8.905 min
Delta R.T.: 0.065 min
Response: 94127586
Conc: 18.01 ng/ml