

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111122\
 Data File : PS021129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2022 08:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 14:16:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.408	6.844	1236.1E6	869.0E6	592.269	628.275
Target Compounds							
1) T	Dalapon	2.507	0.000	450073	0	<MDL	N.D. #
3) T	4-Nitroph...	6.244	0.000	9155444	0	6.087	N.D. #
5) T	DICAMBA	0.000	7.066f	0	3337650	N.D.	<MDL
6) T	MCP	6.749	7.066f	7229280	3337650	1.108	<MDL #
7) T	MCPA	6.776f	0.000	11173239	0	1.191	N.D. #
8) T	DICHLORPROP	7.207f	7.664	420593	4464988	<MDL	2.900 #
10) T	Pentachlo...	7.572	0.000	2012819	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.117	8.681f	6539813	538251	<MDL	<MDL #
12) T	2,4,5-T	8.386	9.102	3753771	1598881	<MDL	<MDL #
13) T	2,4-DB	8.836f	0.000	6039914	0	2.189	N.D. #
15) T	Picloram	9.749	10.912	27082242	7566938	1.282	<MDL #
16) T	DCPA	10.197	10.861	1479419	5073545	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111122\
Data File : PS021129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2022 08:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 14:16:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

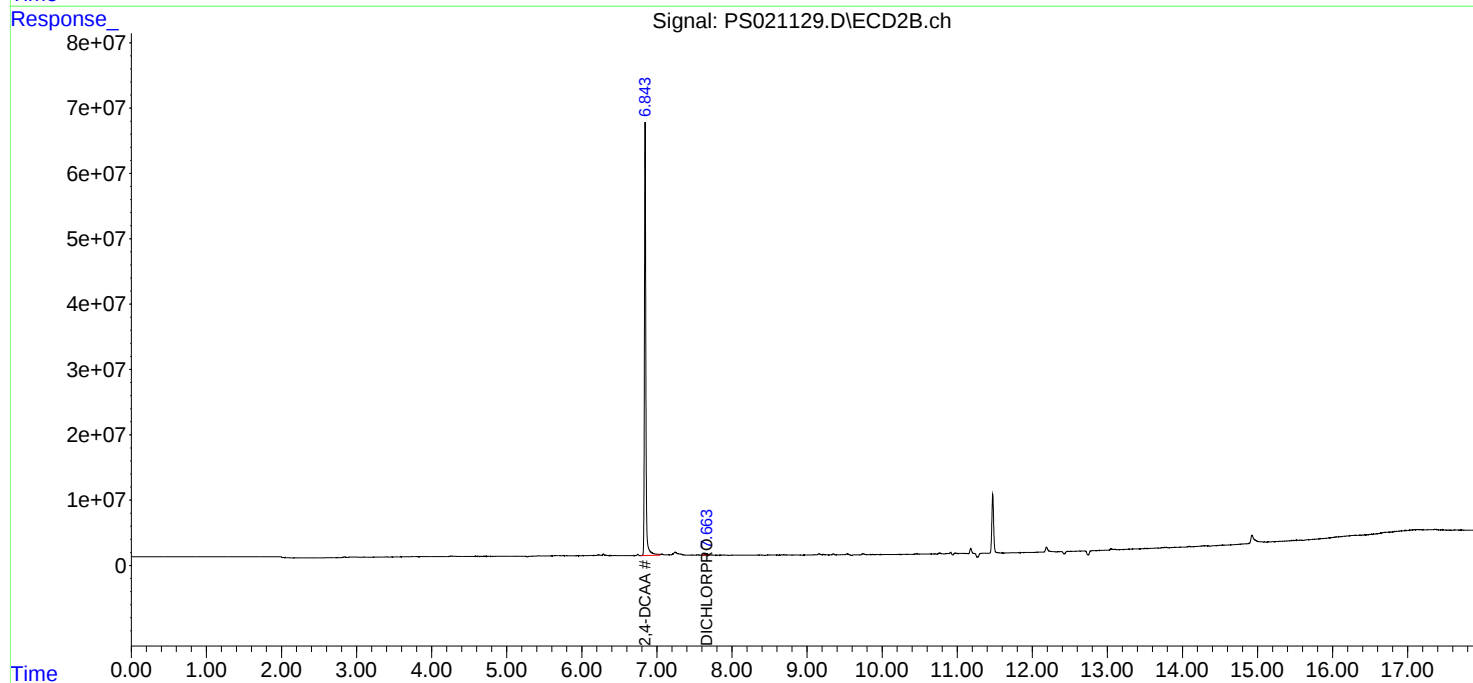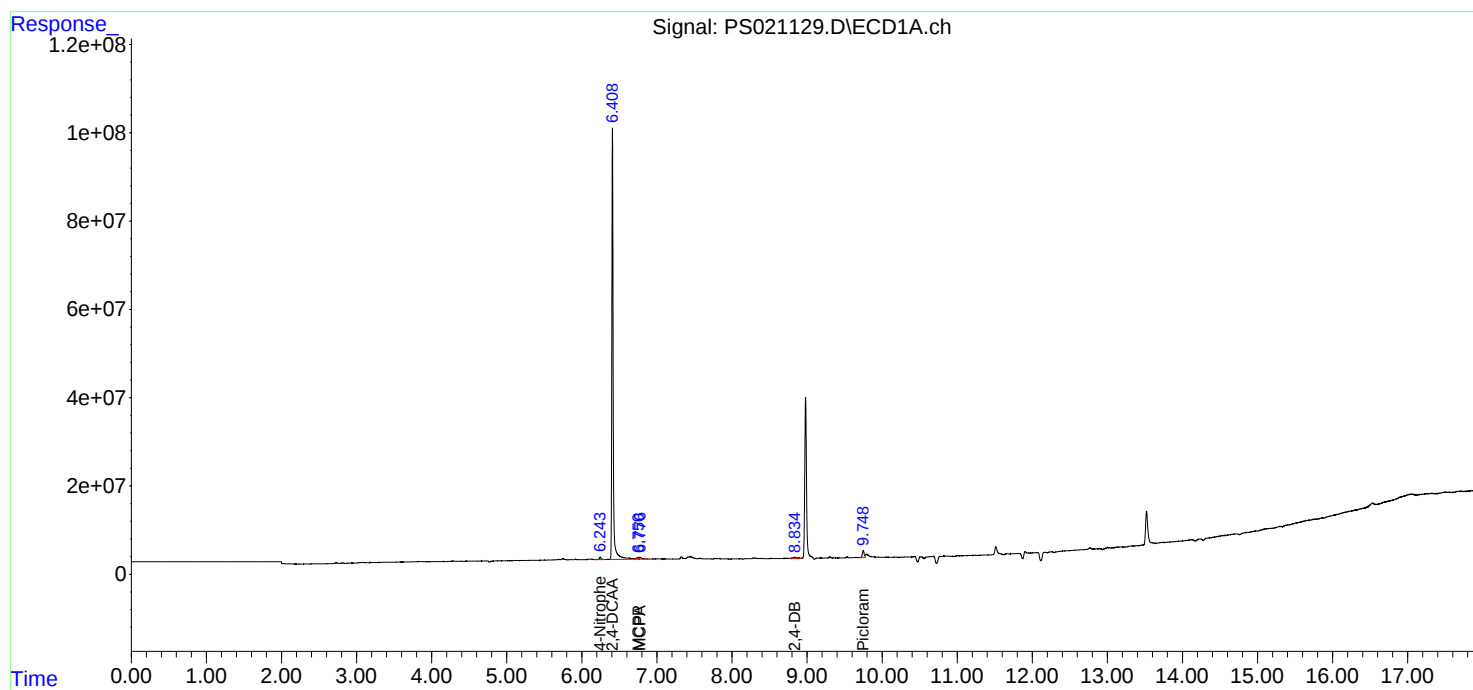


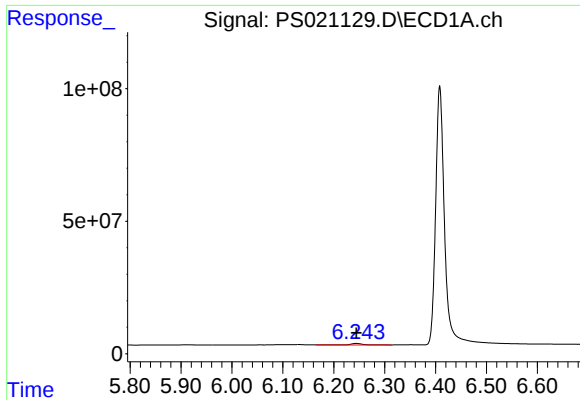

#3 4-Nitrophenol


R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 9155444
Conc: 6.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

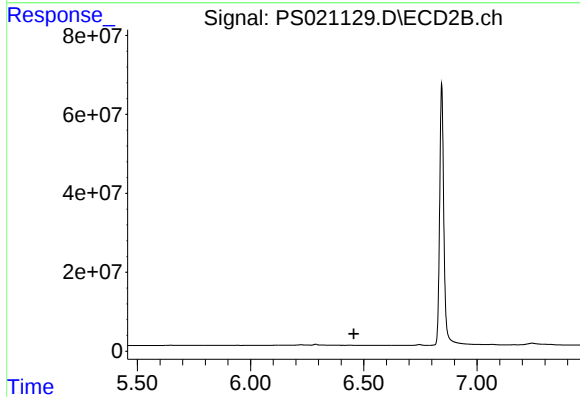


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

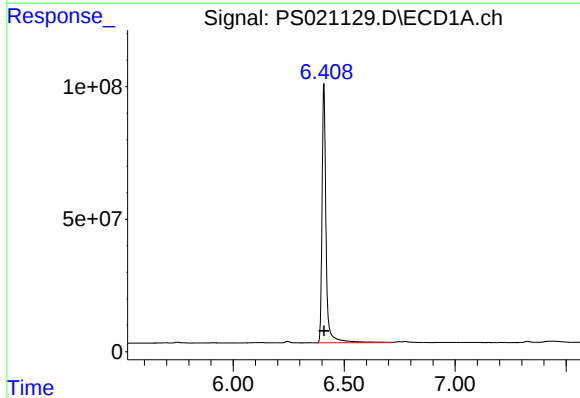


#4 2,4-DCAA

R.T.: 6.408 min
Delta R.T.: 0.000 min
Response: 123611542
Conc: 592.27 ng/ml

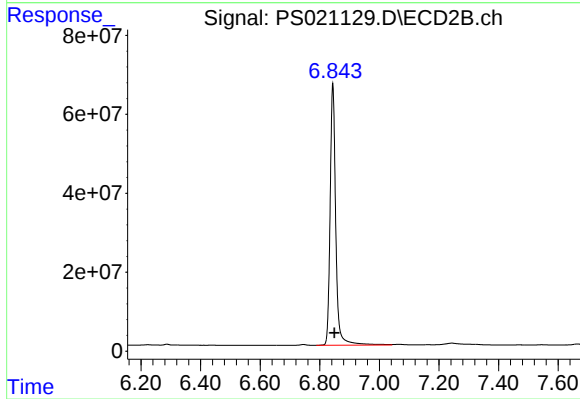

#4 2,4-DCAA


R.T.: 6.844 min
Delta R.T.: -0.006 min
Response: 868995639
Conc: 628.27 ng/ml

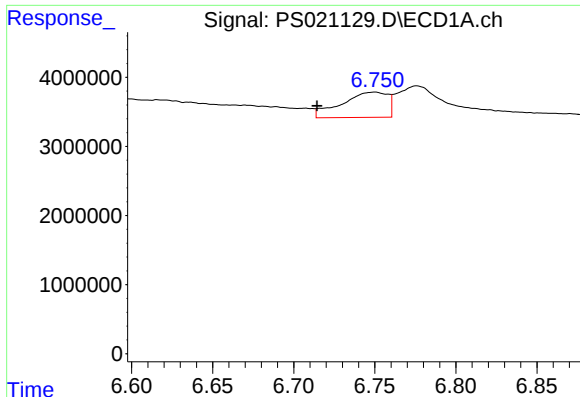

#6 MCPP


R.T.: 6.749 min
Delta R.T.: 0.035 min
Response: 7229280
Conc: 1.11 ug/ml

Instrument :
ECD_S
ClientSampleId :

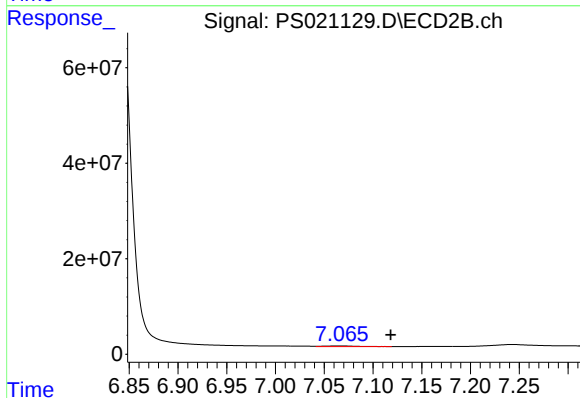


#6 MCPP

R.T.: 7.066 min
Delta R.T.: -0.052 min
Response: 3337650
Conc: N.D.

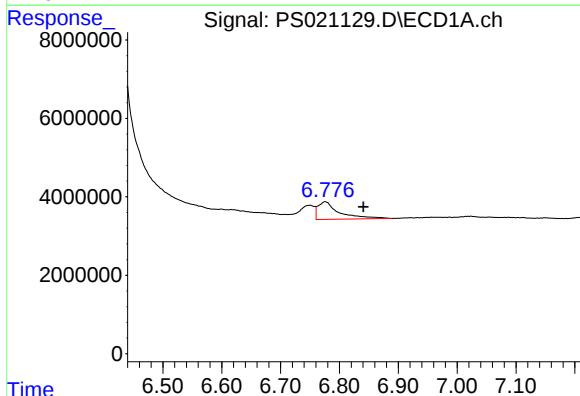


#7 MCPA

R.T.: 6.776 min
Delta R.T.: -0.065 min
Response: 11173239
Conc: 1.19 ug/ml

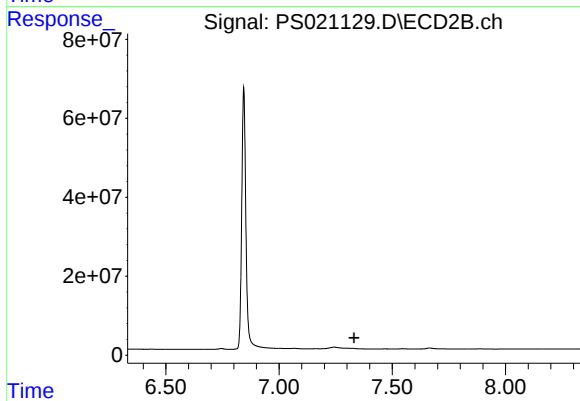

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.331 min
Response: 0
Conc: N.D.

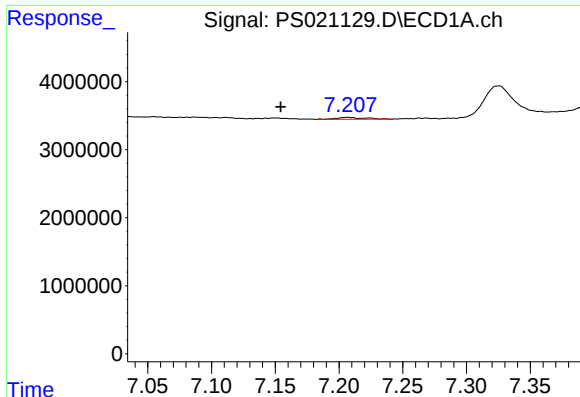

#8 DICHLORPROP


R.T.: 7.207 min
Delta R.T.: 0.053 min
Response: 420593
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

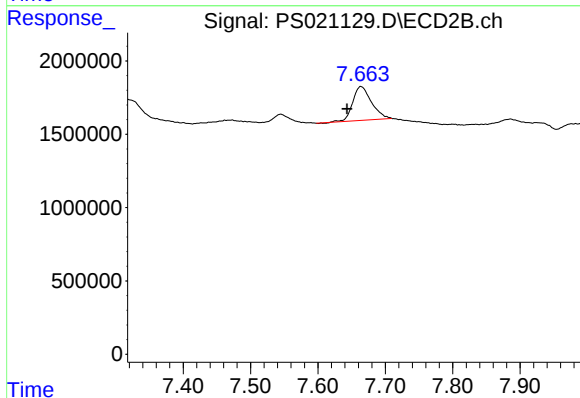


#8 DICHLORPROP

R.T.: 7.664 min
Delta R.T.: 0.020 min
Response: 4464988
Conc: 2.90 ng/ml

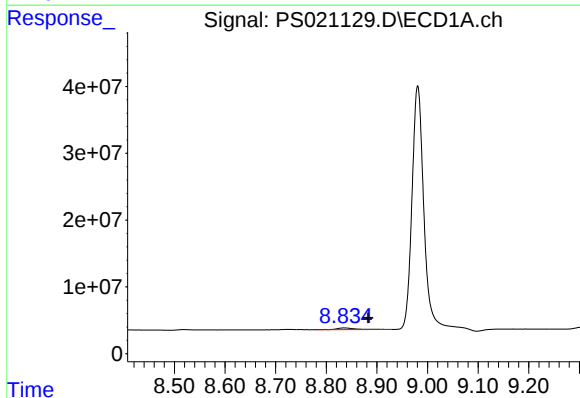


#13 2,4-DB

R.T.: 8.836 min
Delta R.T.: -0.047 min
Response: 6039914
Conc: 2.19 ng/ml

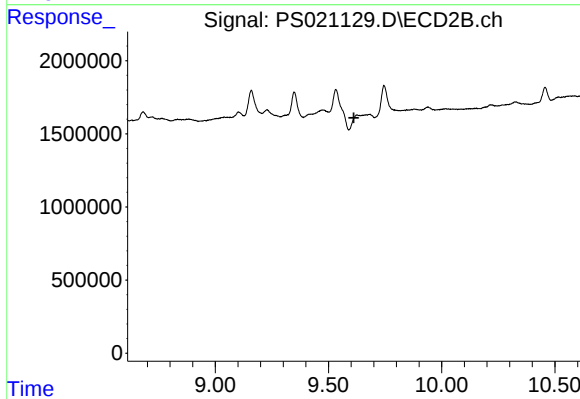

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.612 min
Response: 0
Conc: N.D.

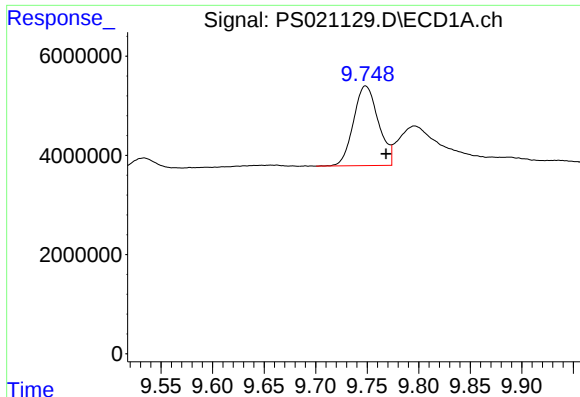

#15 Picloram

R.T.: 9.749 min
Delta R.T.: -0.020 min
Response: 27082242
Conc: 1.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

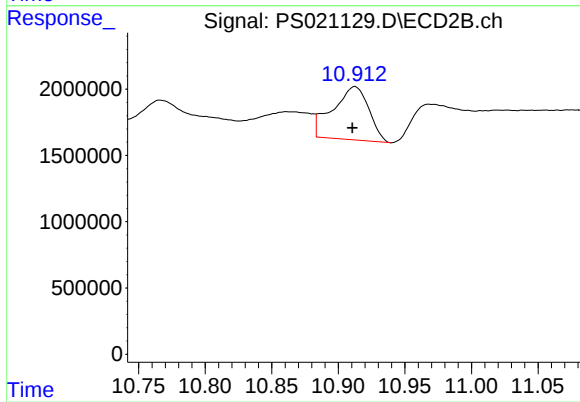

#15 Picloram

R.T.: 10.912 min
Delta R.T.: 0.002 min
Response: 7566938
Conc: N.D.