

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111122\
 Data File : PS021140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2022 15:26
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 20:14:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.408	6.844	1271.3E6	907.2E6	609.134	655.886
Target Compounds							
1) T	Dalapon	2.474	0.000	893003	0	<MDL	N.D. #
3) T	4-Nitroph...	6.244	0.000	10581288	0	7.035	N.D. #
5) T	DICAMBA	6.621f	7.067f	7665624	7644864	<MDL	1.231 #
6) T	MCP	6.747	7.067f	10809709	7644864	1.656	1.609
7) T	MCPA	6.775f	7.292	12601235	20092615	1.343	2.961 #
8) T	DICHLORPROP	7.212f	7.663	628824	6476110	<MDL	4.206 #
9) T	2,4-D	0.000	7.883f	0	979252	N.D.	<MDL
10) T	Pentachlo...	7.572	8.364	1359039	4031508	<MDL	<MDL #
11) T	2,4,5-TP ...	8.129	8.766	3786835	1109370	<MDL	<MDL #
12) T	2,4,5-T	8.410	9.107	5542814	919861	<MDL	<MDL #
13) T	2,4-DB	8.904	9.622	187978	1983132	<MDL	1.782 #
14) T	DINOSEB	9.933	9.879f	1098121	780713	<MDL	<MDL #
15) T	Picloram	9.748	10.903	41790595	11774227	1.978	<MDL #
16) T	DCPA	10.190	10.870	1384517	23531427	<MDL	2.204 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111122\
Data File : PS021140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2022 15:26
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 20:14:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

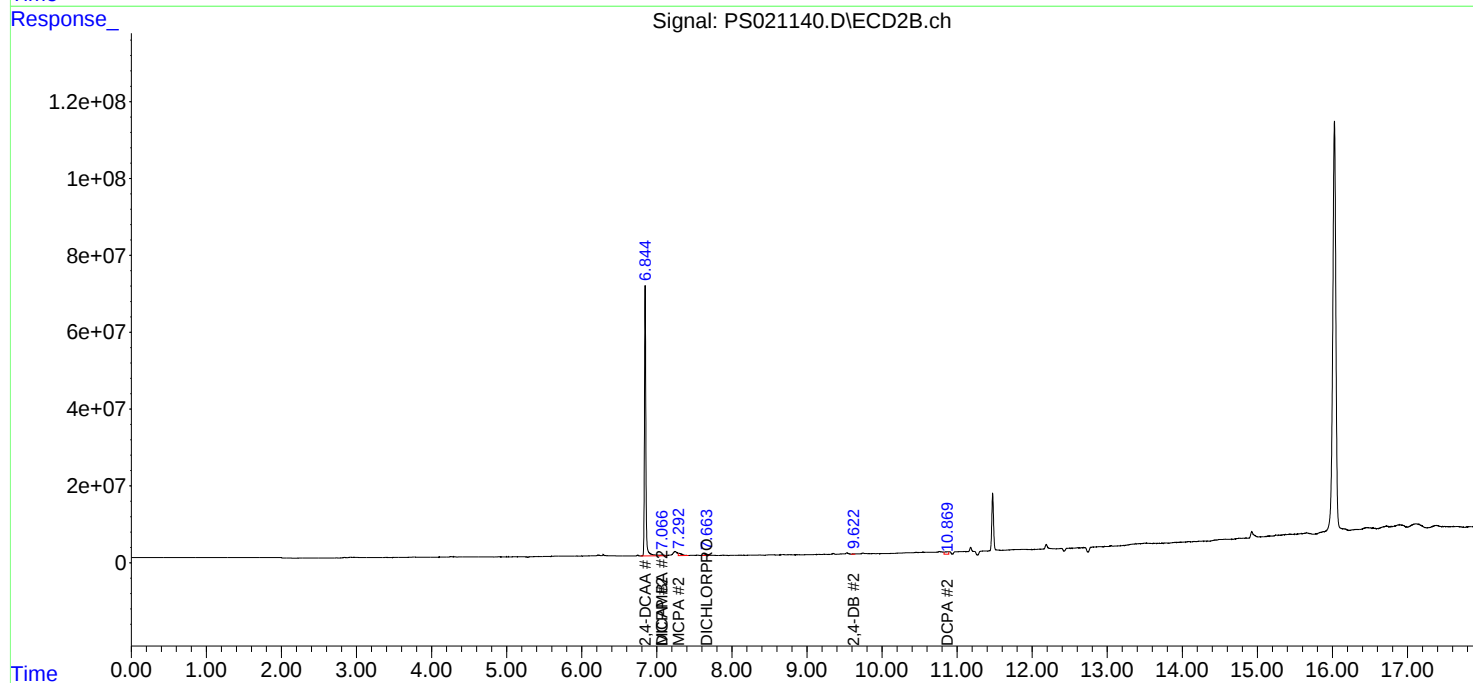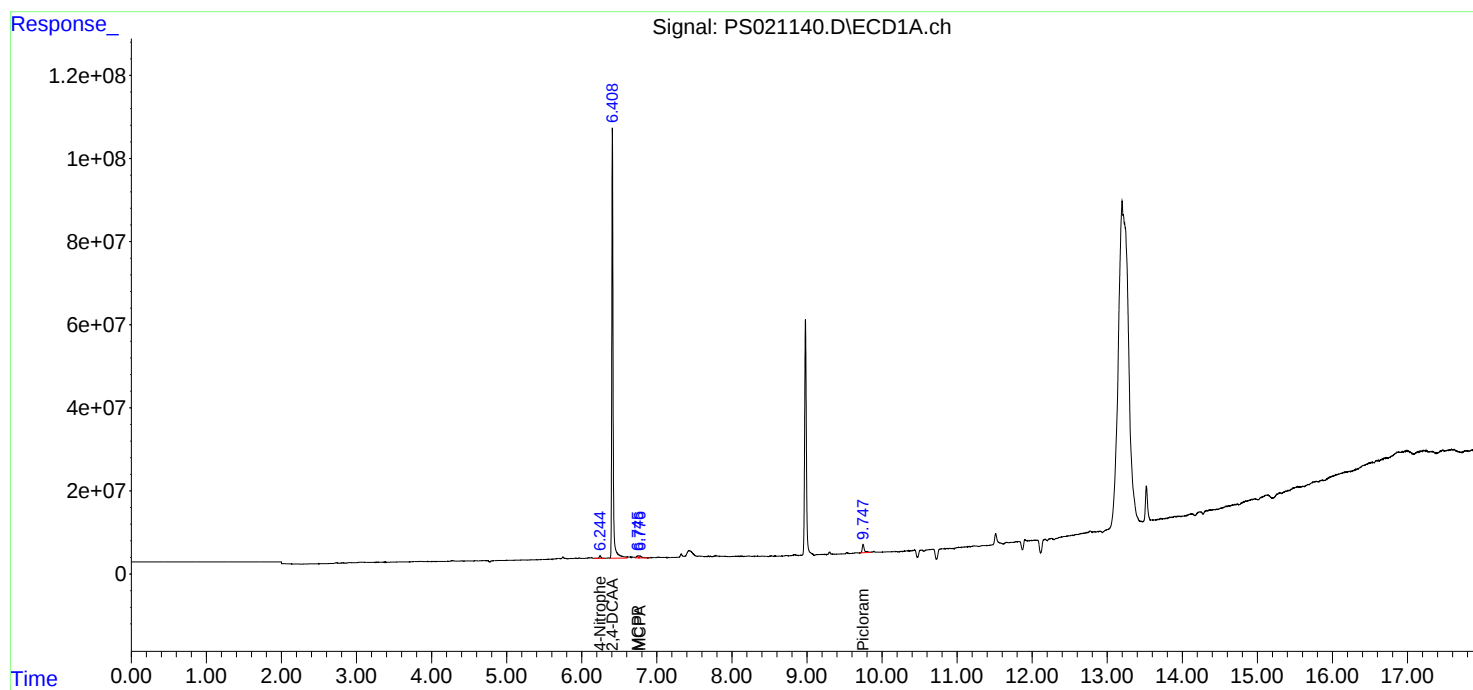


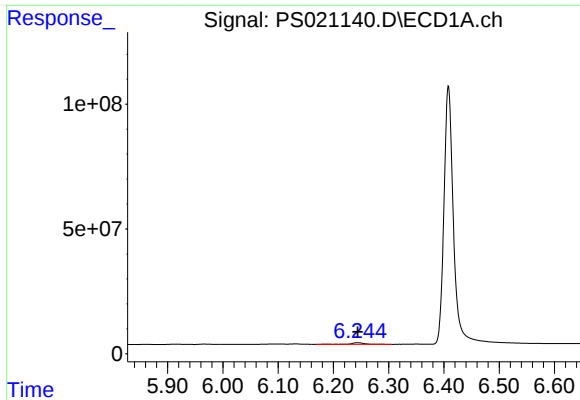

#3 4-Nitrophenol


R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 10581288
Conc: 7.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

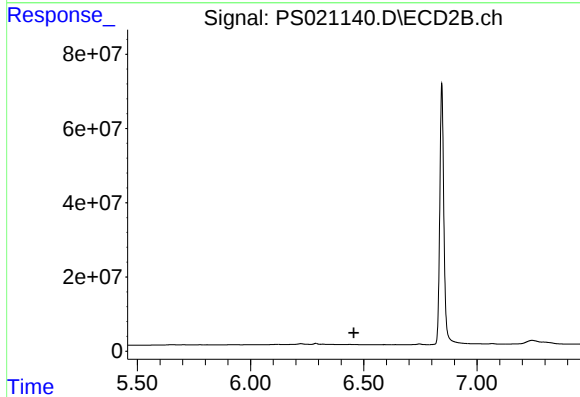


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

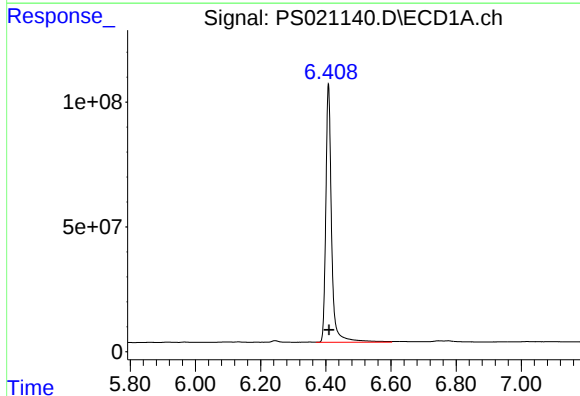


#4 2,4-DCAA

R.T.: 6.408 min
Delta R.T.: -0.001 min
Response: 1271309416
Conc: 609.13 ng/ml

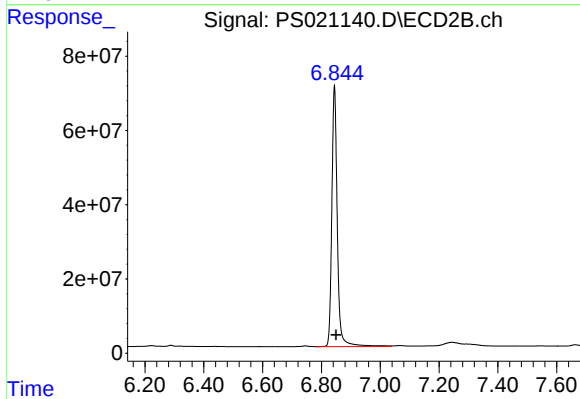

#4 2,4-DCAA


R.T.: 6.844 min
Delta R.T.: -0.005 min
Response: 907186115
Conc: 655.89 ng/ml

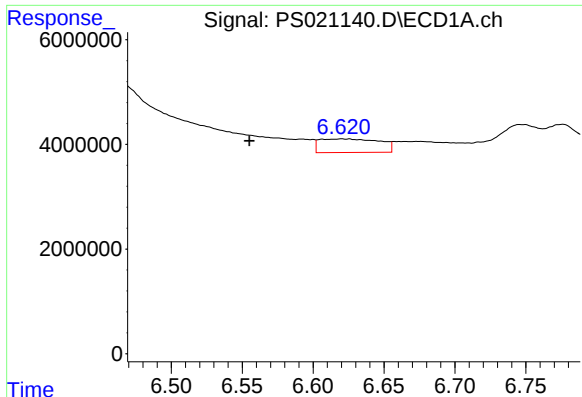

#5 DICAMBA


R.T.: 6.621 min
Delta R.T.: 0.066 min
Response: 7665624
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

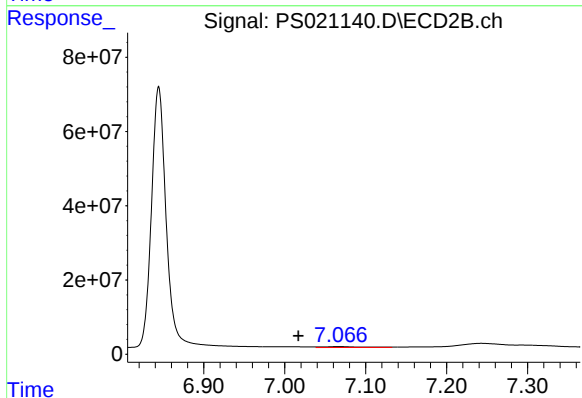


#5 DICAMBA

R.T.: 7.067 min
Delta R.T.: 0.050 min
Response: 7644864
Conc: 1.23 ng/ml

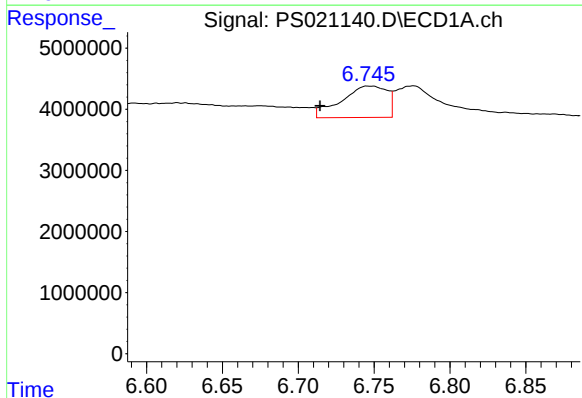


#6 MCP

R.T.: 6.747 min
Delta R.T.: 0.033 min
Response: 10809709
Conc: 1.66 ug/ml

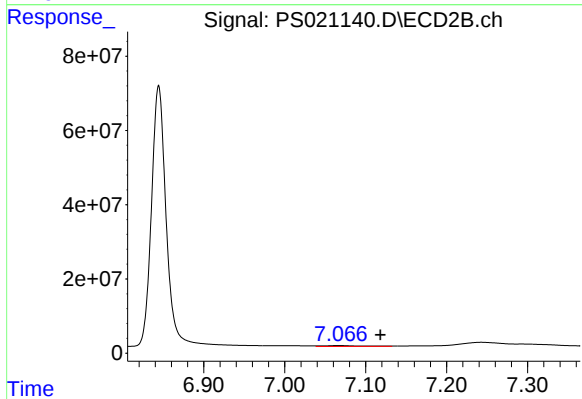

#6 MCP


R.T.: 7.067 min
Delta R.T.: -0.051 min
Response: 7644864
Conc: 1.61 ug/ml

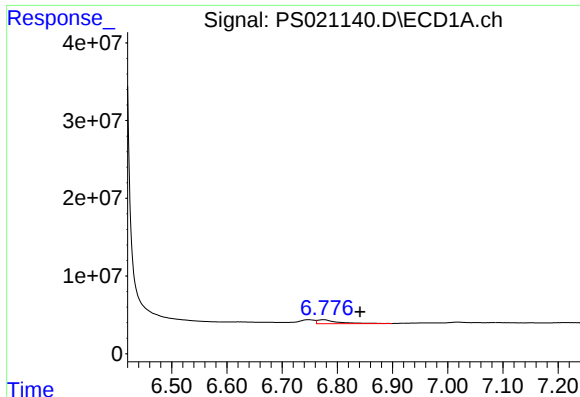

#7 MCPA


R.T.: 6.775 min
Delta R.T.: -0.066 min
Response: 12601235
Conc: 1.34 ug/ml

Instrument :
ECD_S
ClientSampleId :

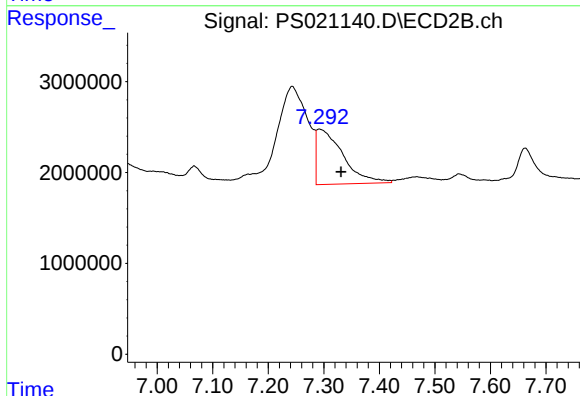


#7 MCPA

R.T.: 7.292 min
Delta R.T.: -0.039 min
Response: 20092615
Conc: 2.96 ug/ml

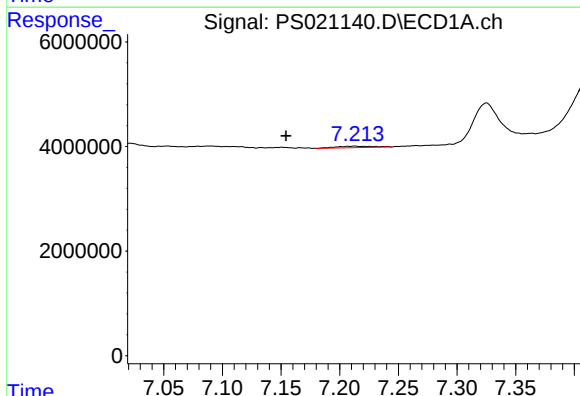


#8 DICHLORPROP

R.T.: 7.212 min
Delta R.T.: 0.058 min
Response: 628824
Conc: N.D.

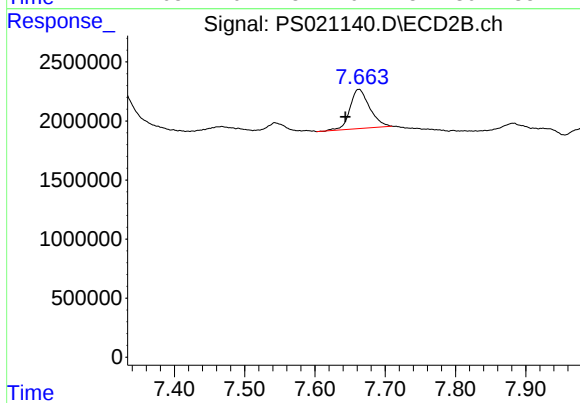

#8 DICHLORPROP


R.T.: 7.663 min
Delta R.T.: 0.019 min
Response: 6476110
Conc: 4.21 ng/ml

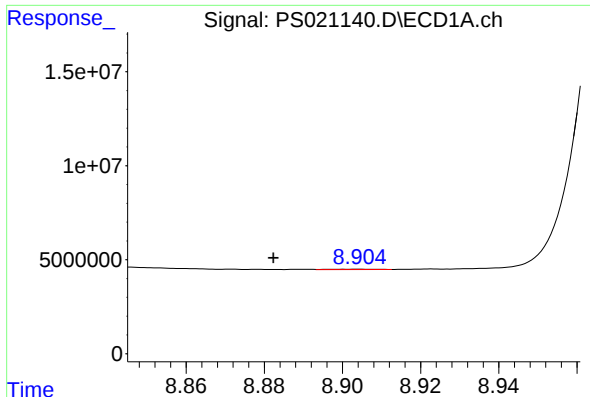

#13 2,4-DB


R.T.: 8.904 min
Delta R.T.: 0.022 min
Response: 187978
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

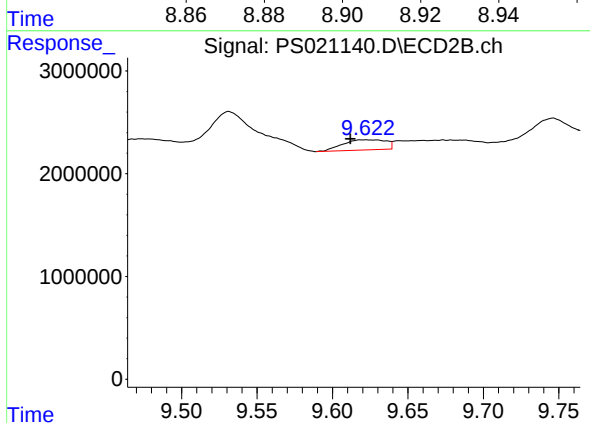


#13 2,4-DB

R.T.: 9.622 min
Delta R.T.: 0.010 min
Response: 1983132
Conc: 1.78 ng/ml

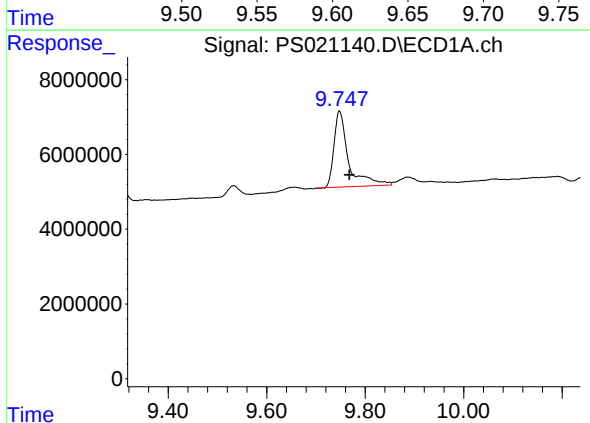


#15 Picloram

R.T.: 9.748 min
Delta R.T.: -0.020 min
Response: 41790595
Conc: 1.98 ng/ml

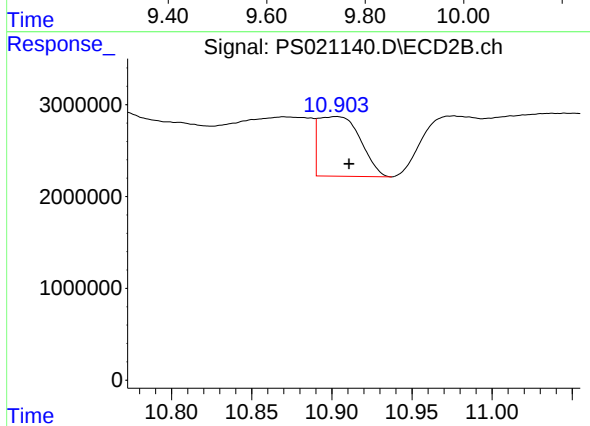

#15 Picloram


R.T.: 10.903 min
Delta R.T.: -0.008 min
Response: 11774227
Conc: N.D.

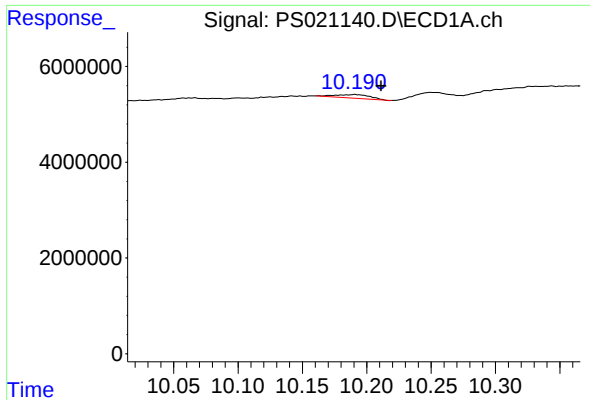

#16 DCPA

R.T.: 10.190 min
Delta R.T.: -0.021 min
Response: 1384517
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

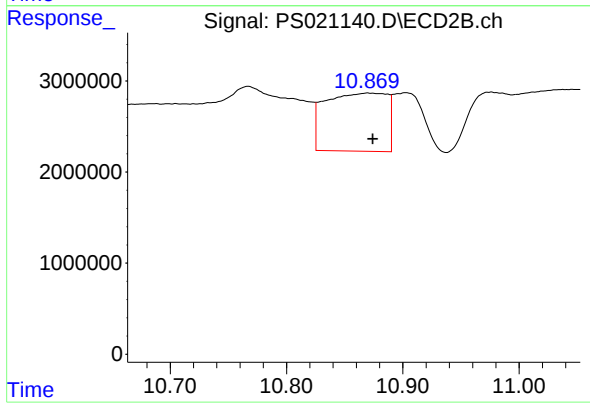

#16 DCPA

R.T.: 10.870 min
Delta R.T.: -0.004 min
Response: 23531427
Conc: 2.20 ng/ml