

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111125\
 Data File : PS032352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2025 21:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:37:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.285	7.623	1738.7E6	1868.0E6	383.703	512.425 #
Target Compounds							
2) T	3,5-DICHL...	6.444	0.000	27184255	0	4.204	N.D. #
6) T	MCP	0.000	7.909	0	24588045	N.D.	1.849
7) T	MCPA	7.811	0.000	12642356	0	<MDL	N.D. #
8) T	DICHLORPROP	8.170	0.000	679821	0	<MDL	N.D. #
10) T	Pentachlo...	8.711	9.365	4222927	4122430	<MDL	<MDL #
11) T	2,4,5-TP ...	9.290	9.771f	4198504	1581521	<MDL	<MDL #
12) T	2,4,5-T	9.580	10.138f	4918001	10110362	<MDL	<MDL #
13) T	2,4-DB	10.159	0.000	1253716	0	<MDL	N.D. #
14) T	DINOSEB	11.345	11.127	8128004	1513900	<MDL	<MDL #
15) T	Picloram	11.191	0.000	9146466	0	<MDL	N.D. #
16) T	DCPA	11.647	12.104f	5660296	16104633	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111125\
Data File : PS032352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2025 21:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:37:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

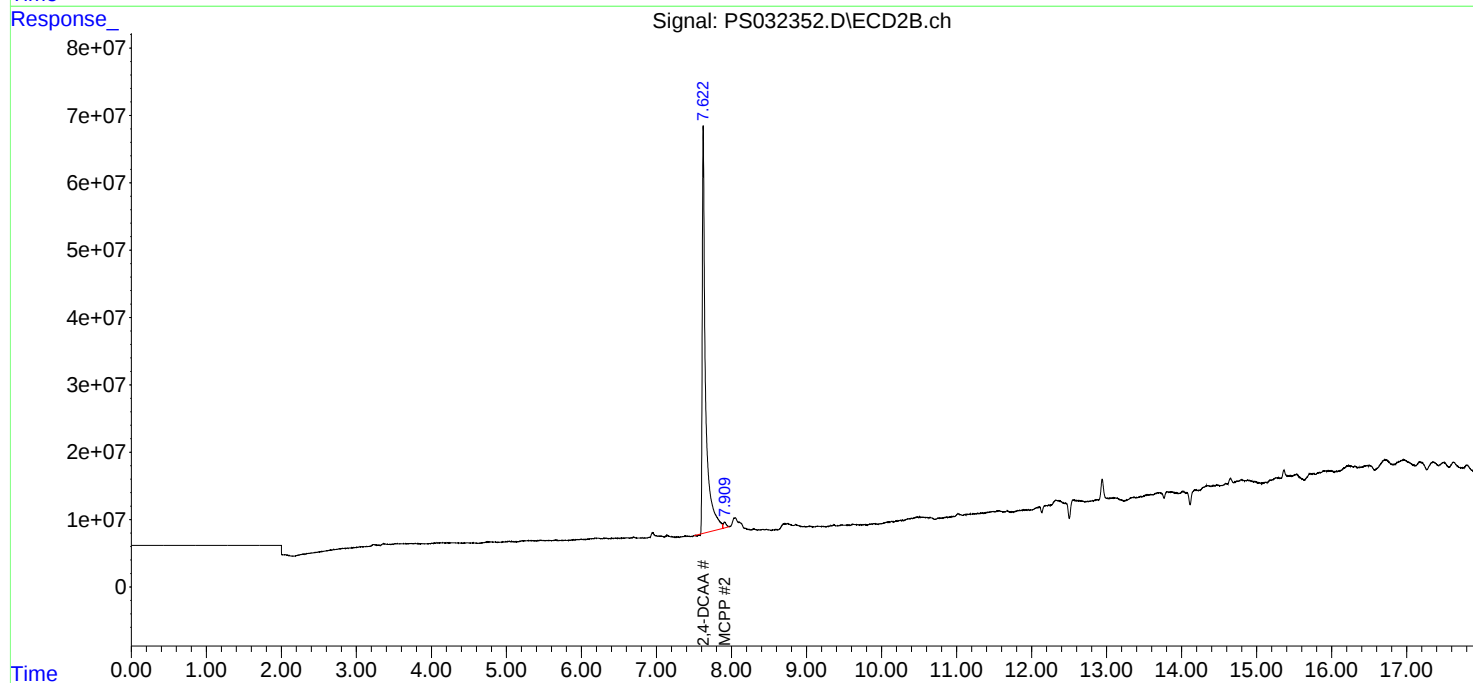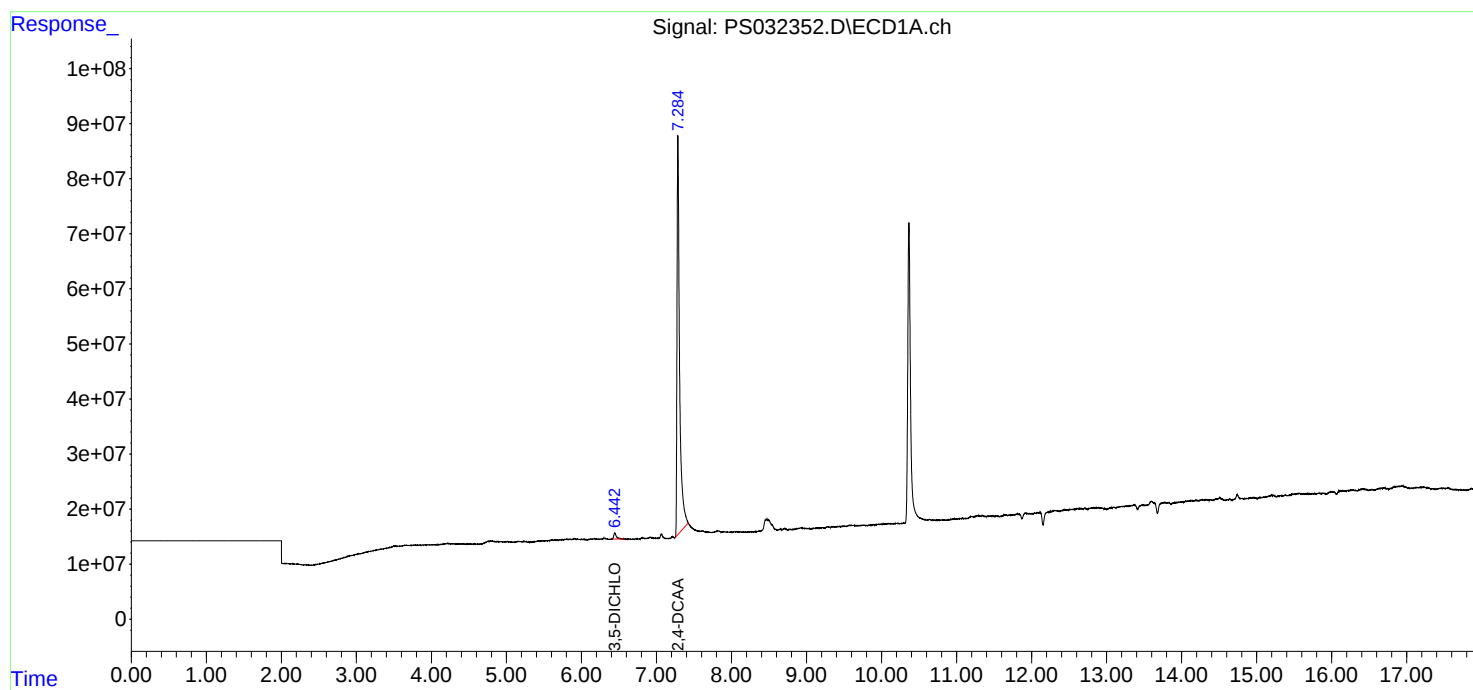


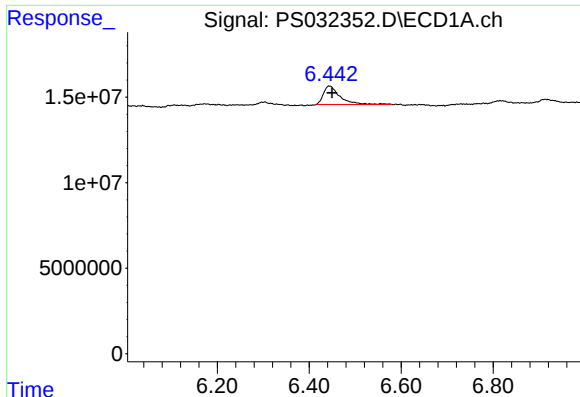

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.444 min
Delta R.T.: -0.005 min
Response: 27184255
Conc: 4.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

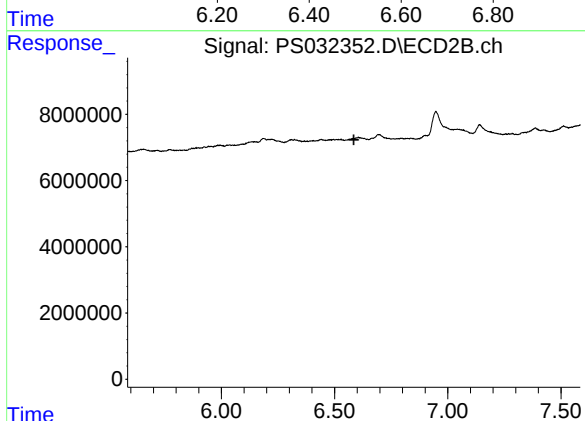


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

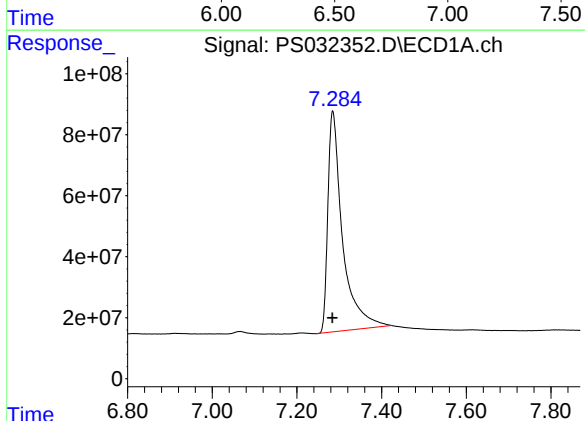


#4 2,4-DCAA

R.T.: 7.285 min
Delta R.T.: 0.002 min
Response: 1738664843
Conc: 383.70 ng/ml

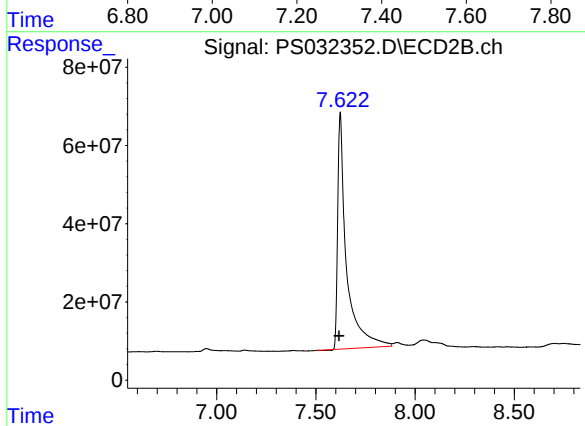

#4 2,4-DCAA


R.T.: 7.623 min
Delta R.T.: 0.005 min
Response: 1868042605
Conc: 512.42 ng/ml

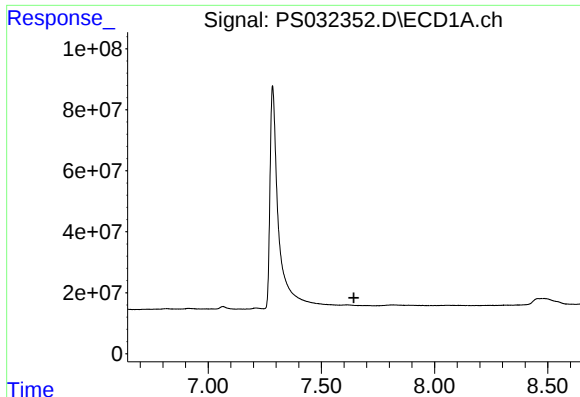

#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.644 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

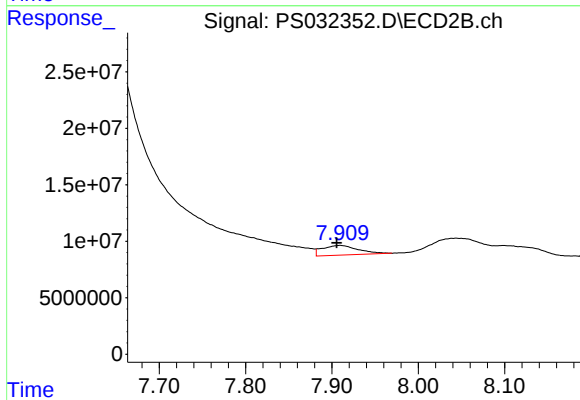

#6 MCPP

R.T.: 7.909 min
Delta R.T.: 0.004 min
Response: 24588045
Conc: 1.85 ug/ml