

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111125\
 Data File : PS032364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2025 03:21
 Operator : AR\AJ
 Sample : Q3601-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 04:36:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.267	7.627	10546628	39780435	2.328	10.912 #
Target Compounds							
1) T	Dalapon	2.632	2.606	2284.1E6	3589.0E6	318.169	516.111 #
2) T	3,5-DICHL...	6.492f	0.000	7300780	0	1.129	N.D. #
3) T	4-Nitroph...	7.083	7.189	6746216	-1269572	5.025	N.D. #
5) T	DICAMBA	7.437f	0.000	3300270	0	<MDL	N.D. #
6) T	MCP	7.667	7.878f	6907519	26072301	<MDL	1.960 #
7) T	MCPA	7.806	0.000	34240937	0	2.550	N.D. #
8) T	DICHLORPROP	8.163	8.519	1008044	5365055	<MDL	1.125 #
9) T	2,4-D	8.390	0.000	41622368	0	9.225	N.D. #
10) T	Pentachlo...	8.698	9.360	3151705	16947453	<MDL	<MDL #
11) T	2,4,5-TP ...	9.324f	9.734	35708609	34725997	1.373	1.293
13) T	2,4-DB	10.178	10.737	49218866	22850207	18.678	6.059 #
14) T	DINOSEB	11.336	11.117	1515317	6258960	<MDL	<MDL #
15) T	Picloram	11.194	12.245	1813866	14077279	<MDL	<MDL #
16) T	DCPA	11.637	0.000	6354297	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111125\
Data File : PS032364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2025 03:21
Operator : AR\AJ
Sample : Q3601-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 04:36:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

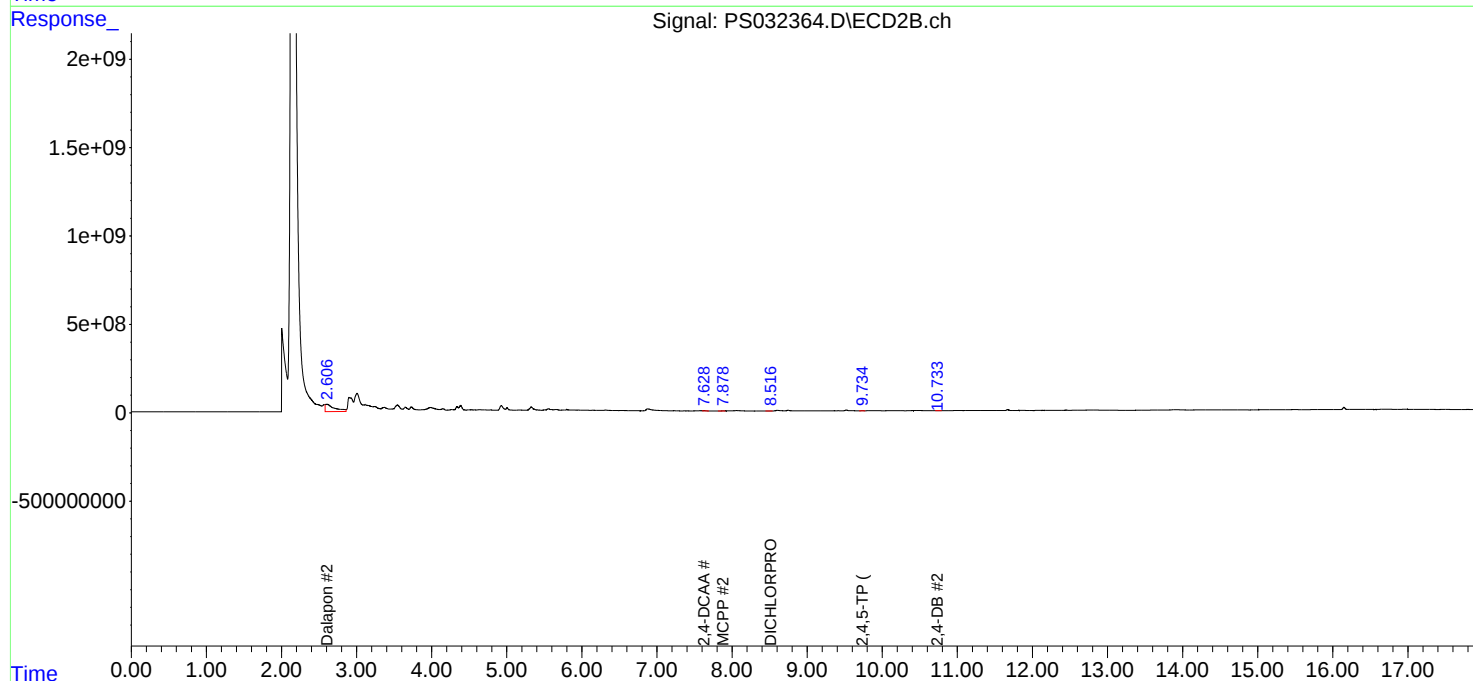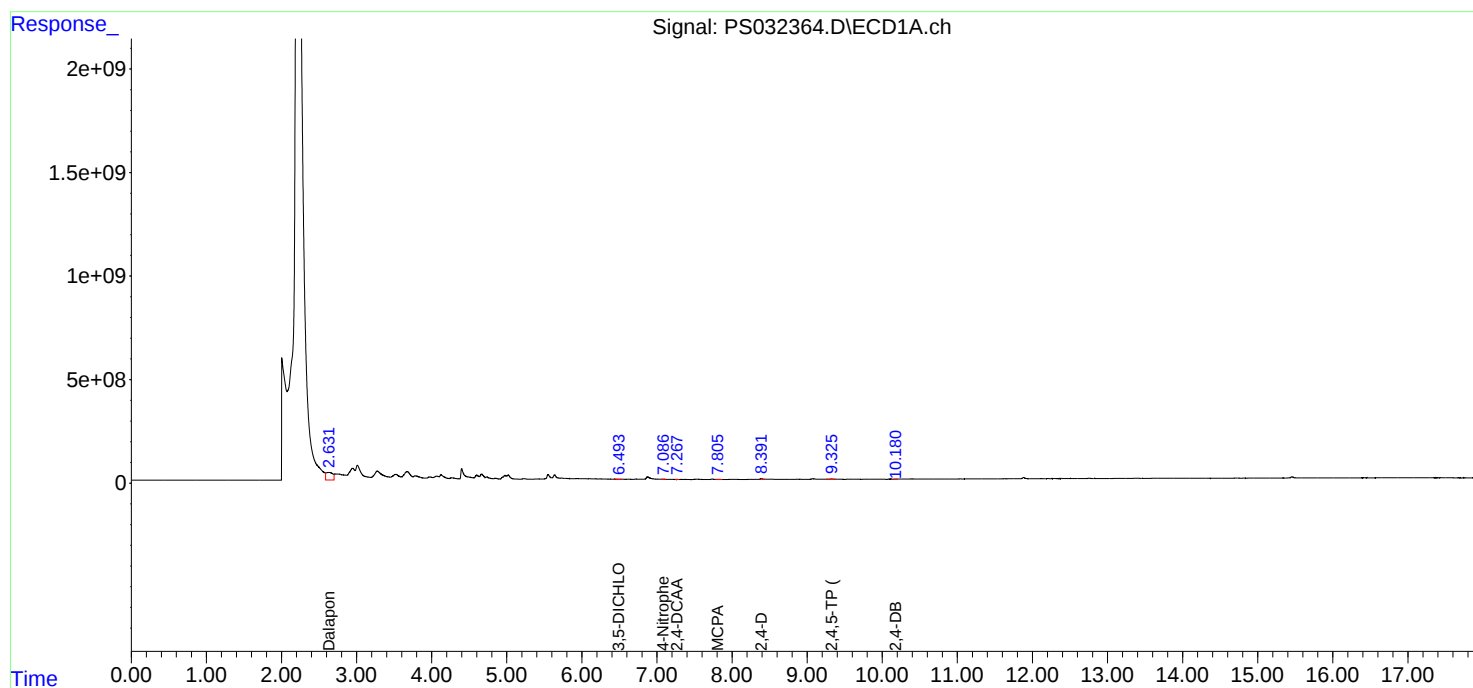


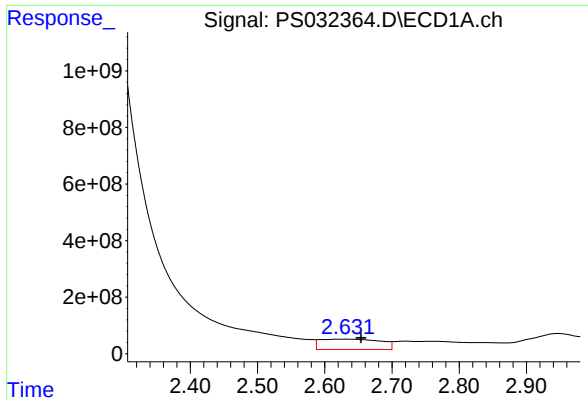

#1 Dalapon


R.T.: 2.632 min
Delta R.T.: -0.022 min
Response: 2284063987
Conc: 318.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-4

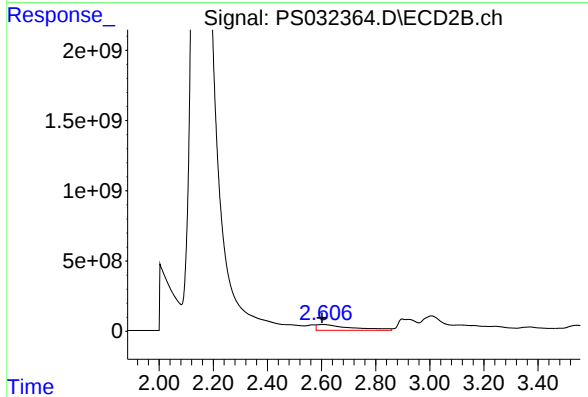


#1 Dalapon

R.T.: 2.606 min
Delta R.T.: 0.003 min
Response: 3589037913
Conc: 516.11 ng/ml

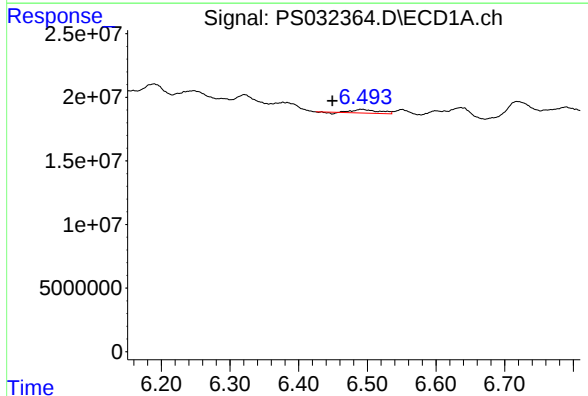


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.492 min
Delta R.T.: 0.042 min
Response: 7300780
Conc: 1.13 ng/ml

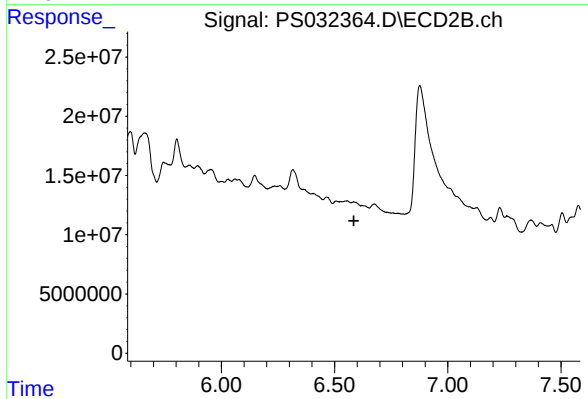

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

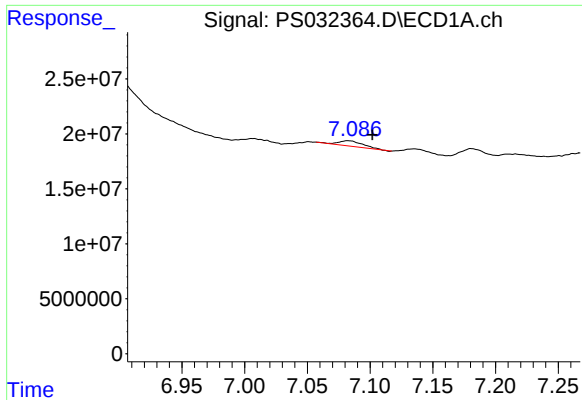

#3 4-Nitrophenol


R.T.: 7.083 min
Delta R.T.: -0.019 min
Response: 6746216
Conc: 5.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-4

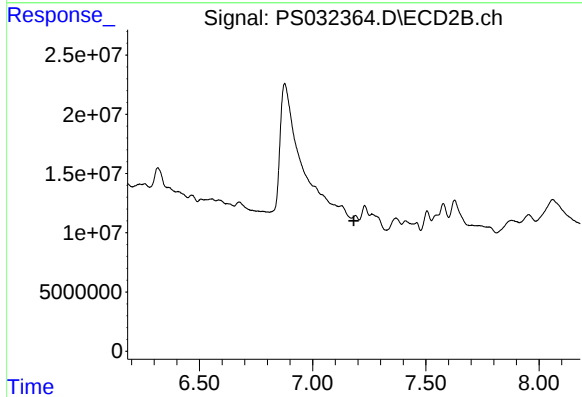


#3 4-Nitrophenol

R.T.: 7.189 min
Delta R.T.: 0.006 min
Response: -1269572
Conc: N.D.

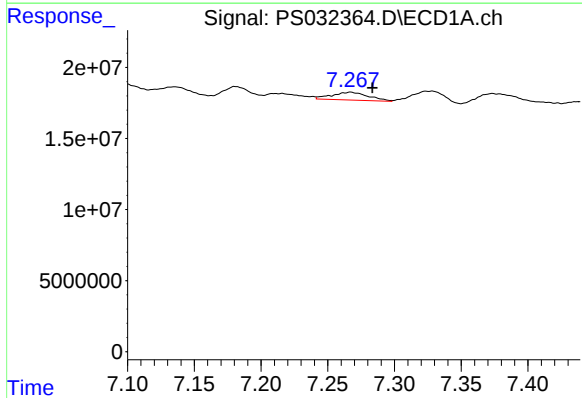


#4 2,4-DCAA

R.T.: 7.267 min
Delta R.T.: -0.017 min
Response: 10546628
Conc: 2.33 ng/ml

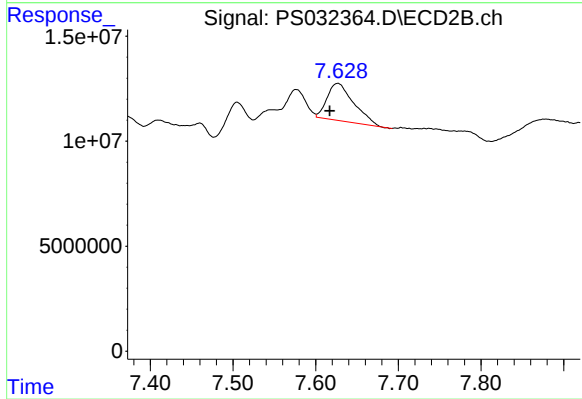

#4 2,4-DCAA


R.T.: 7.627 min
Delta R.T.: 0.009 min
Response: 39780435
Conc: 10.91 ng/ml

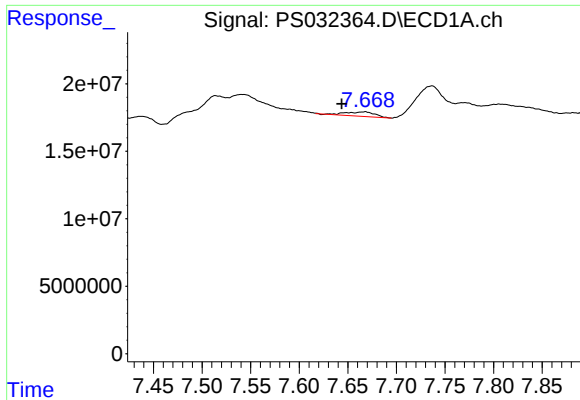

#6 MCPP


R.T.: 7.667 min
Delta R.T.: 0.023 min
Response: 6907519
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-4

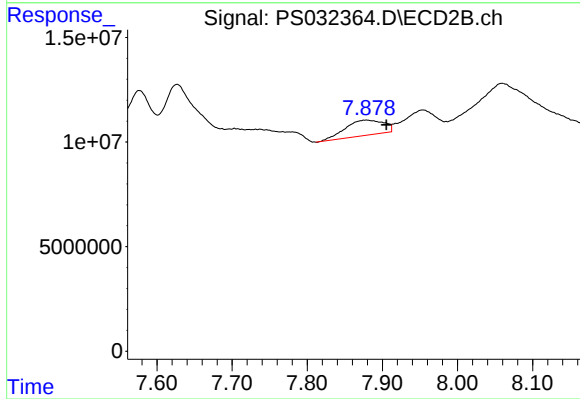


#6 MCPP

R.T.: 7.878 min
Delta R.T.: -0.027 min
Response: 26072301
Conc: 1.96 ug/ml

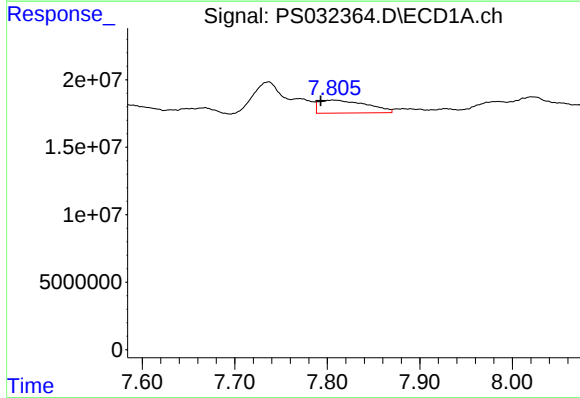


#7 MCPA

R.T.: 7.806 min
Delta R.T.: 0.014 min
Response: 34240937
Conc: 2.55 ug/ml

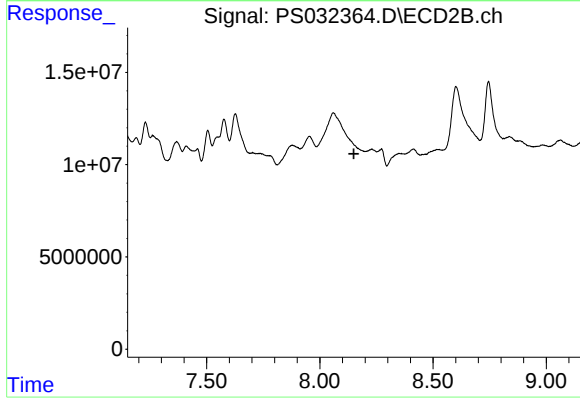

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 8.151 min
Response: 0
Conc: N.D.

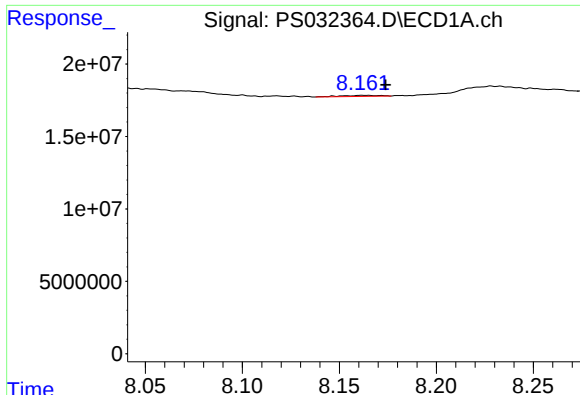

#8 DICHLORPROP


R.T.: 8.163 min
Delta R.T.: -0.011 min
Response: 1008044
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-4

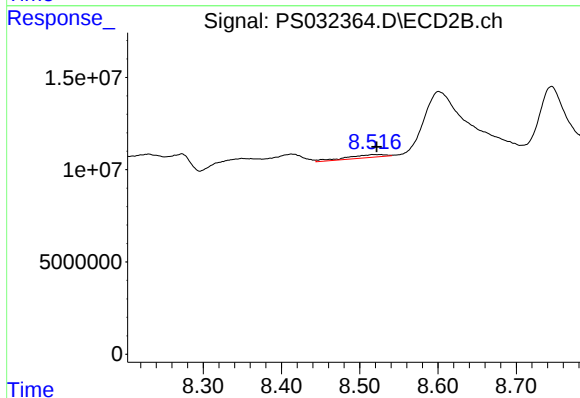


#8 DICHLORPROP

R.T.: 8.519 min
Delta R.T.: -0.003 min
Response: 5365055
Conc: 1.12 ng/ml

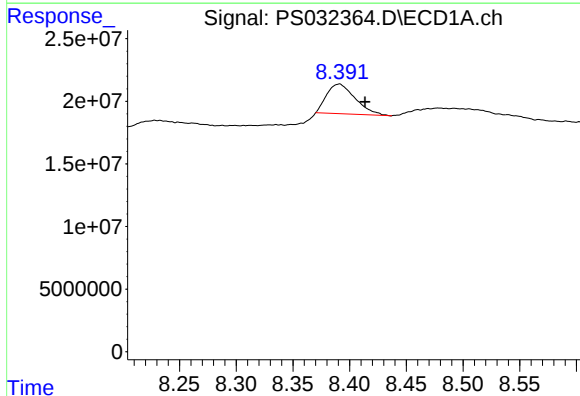


#9 2,4-D

R.T.: 8.390 min
Delta R.T.: -0.023 min
Response: 41622368
Conc: 9.23 ng/ml

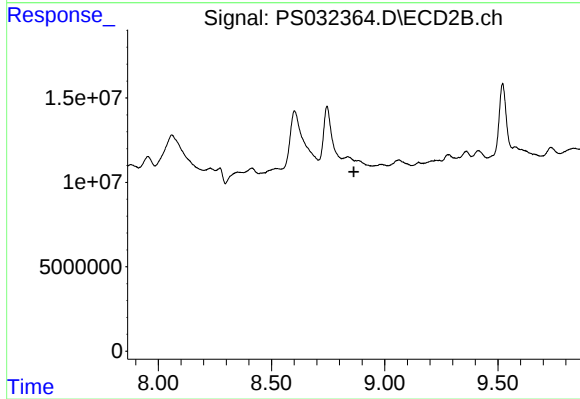

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.864 min
Response: 0
Conc: N.D.

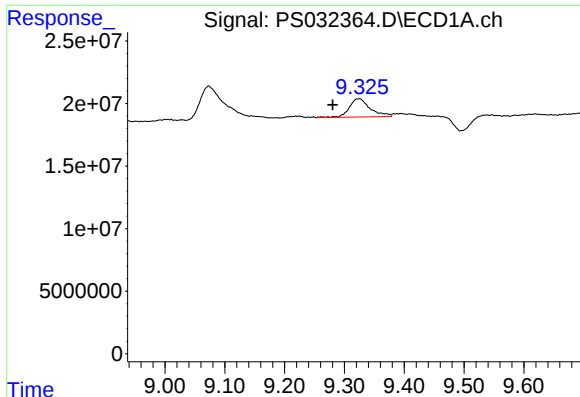

#11 2,4,5-TP (SILVEX)


R.T.: 9.324 min
Delta R.T.: 0.044 min
Response: 35708609
Conc: 1.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-4

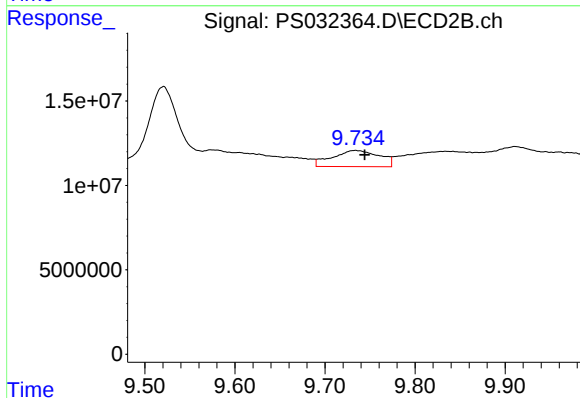


#11 2,4,5-TP (SILVEX)

R.T.: 9.734 min
Delta R.T.: -0.010 min
Response: 34725997
Conc: 1.29 ng/ml

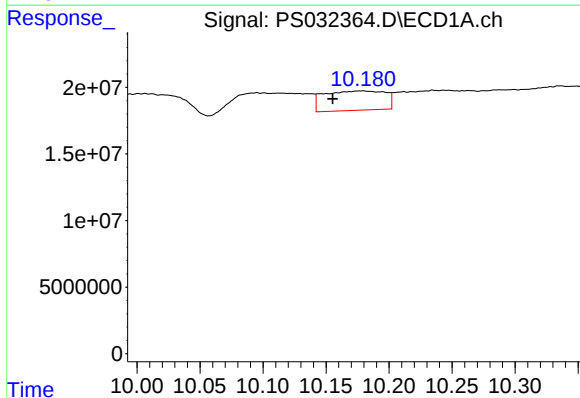

#13 2,4-DB

R.T.: 10.178 min
Delta R.T.: 0.023 min
Response: 49218866
Conc: 18.68 ng/ml

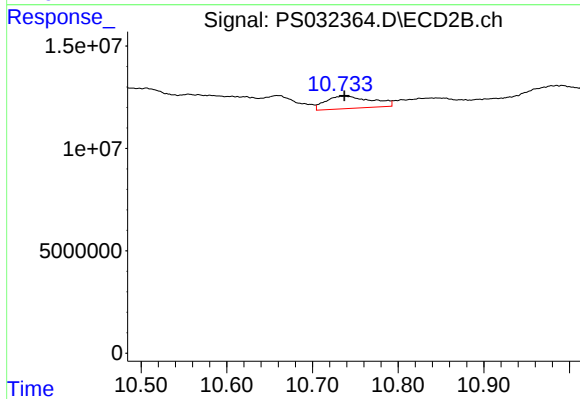

#13 2,4-DB

R.T.: 10.737 min
Delta R.T.: 0.000 min
Response: 22850207
Conc: 6.06 ng/ml