

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111125\
 Data File : PS032365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2025 03:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 04:36:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.284	7.622	1742.7E6	1895.9E6	384.601	520.054 #
Target Compounds							
1) T	Dalapon	0.000	2.650f	0	66013230	N.D.	9.493
2) T	3,5-DICHL...	6.444	0.000	30377825	0	4.698	N.D. #
3) T	4-Nitroph...	7.117	0.000	122049	0	<MDL	N.D. #
6) T	MCP	7.678f	7.910	225609	29669193	<MDL	2.231 #
7) T	MCPA	7.800	8.105f	1988340	3094967	<MDL	<MDL #
8) T	DICHLORPROP	8.180	0.000	213313	0	<MDL	N.D. #
9) T	2,4-D	8.388f	0.000	416282	0	<MDL	N.D. #
10) T	Pentachlo...	8.708	9.365	6217221	6601575	<MDL	<MDL #
11) T	2,4,5-TP ...	9.282	9.724	3215756	430671	<MDL	<MDL #
12) T	2,4,5-T	9.572	10.141f	875675	5392340	<MDL	<MDL #
13) T	2,4-DB	10.147	0.000	549545	0	<MDL	N.D. #
14) T	DINOSEB	11.333	11.118	6914103	2496453	<MDL	<MDL #
15) T	Picloram	11.194	12.250f	12022545	77668275	<MDL	2.089 #
16) T	DCPA	11.639	0.000	4553930	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111125\
Data File : PS032365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2025 03:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 04:36:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

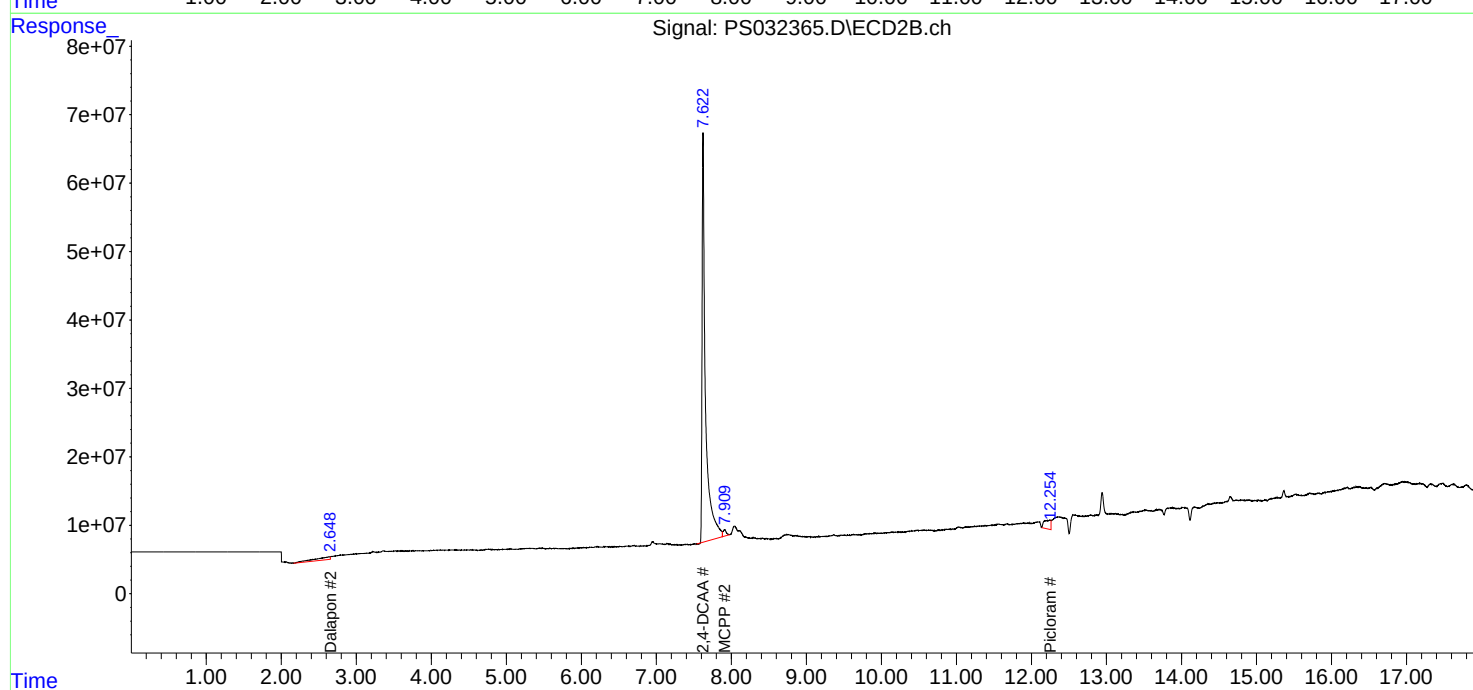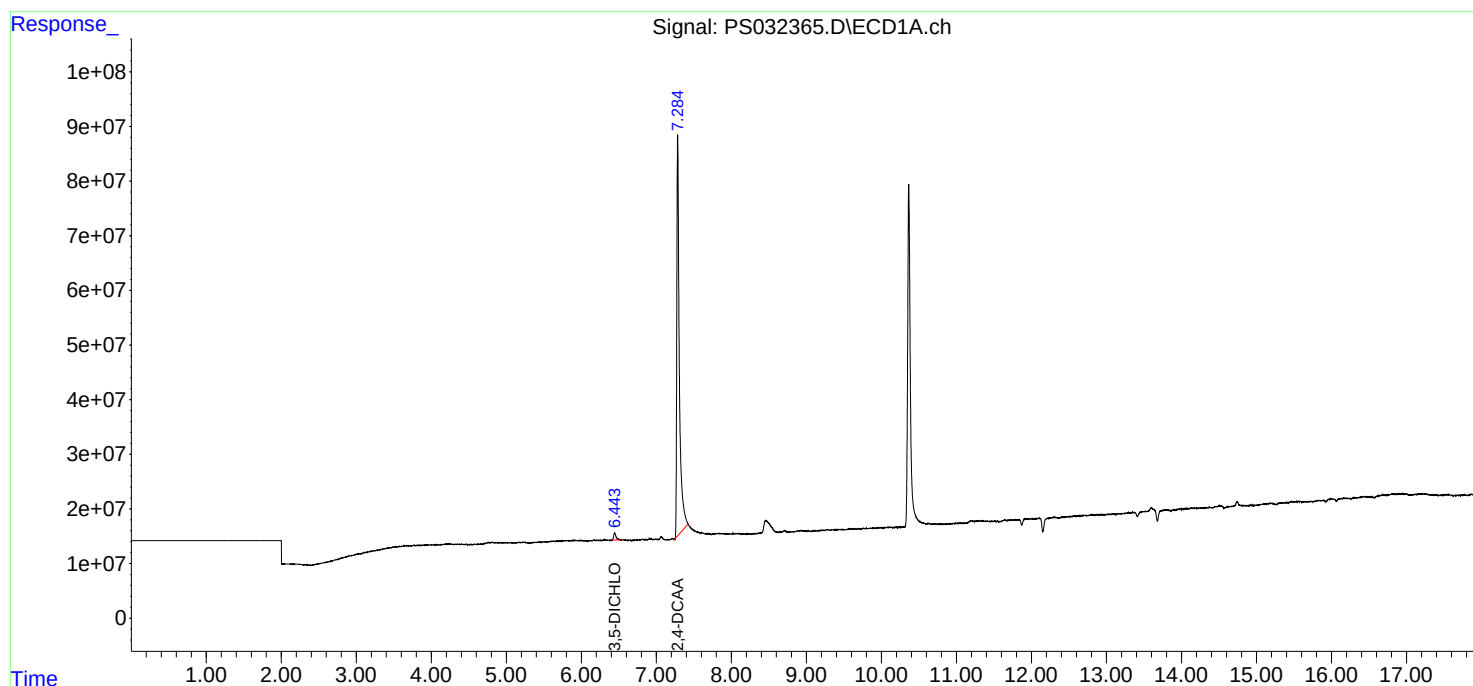


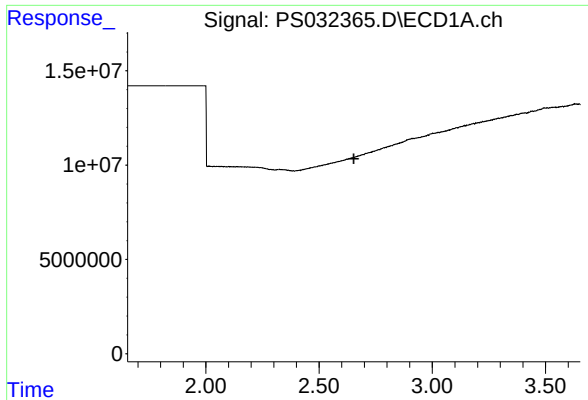

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.654 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

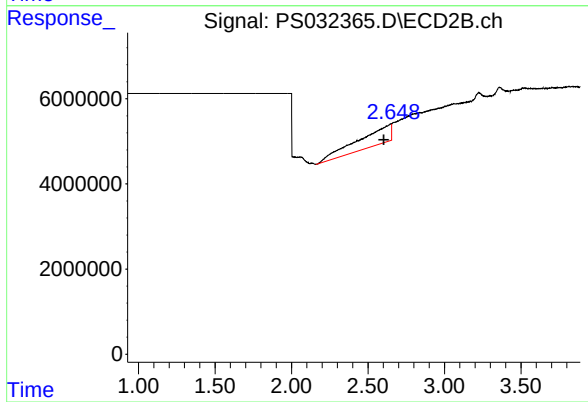


#1 Dalapon

R.T.: 2.650 min
Delta R.T.: 0.047 min
Response: 66013230
Conc: 9.49 ng/ml

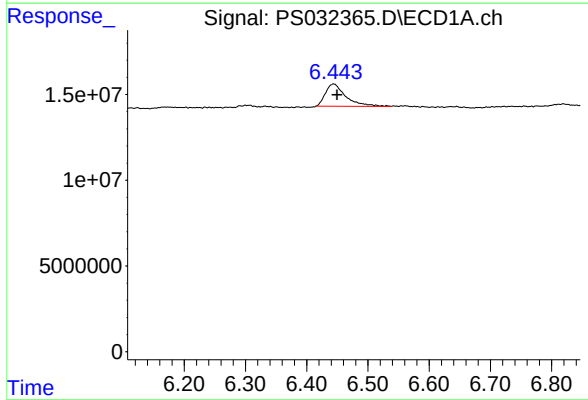


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.444 min
Delta R.T.: -0.005 min
Response: 30377825
Conc: 4.70 ng/ml

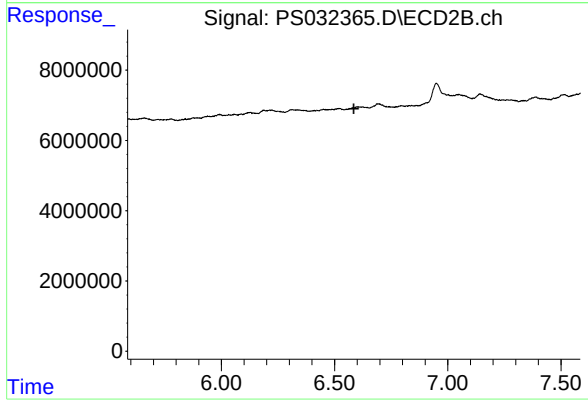

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.585 min
Response: 0
Conc: N.D.

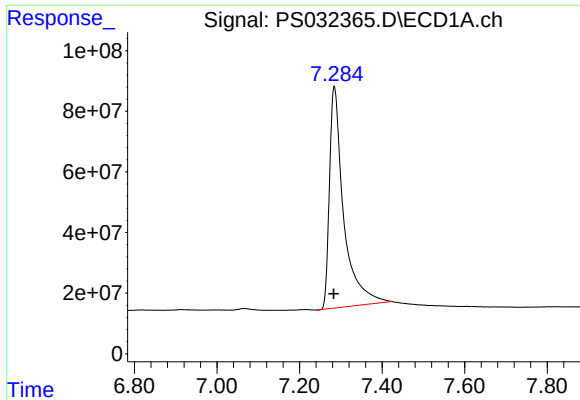

#4 2,4-DCAA


R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 1742733336
Conc: 384.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

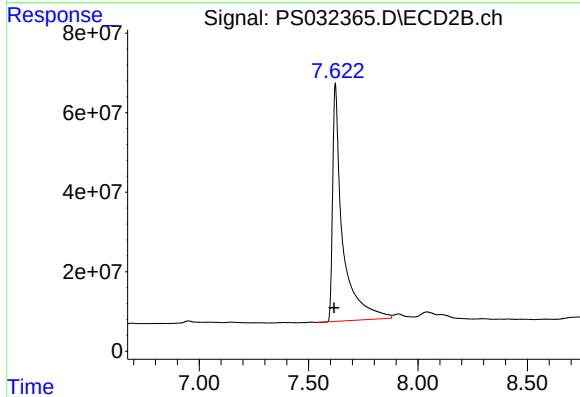


#4 2,4-DCAA

R.T.: 7.622 min
Delta R.T.: 0.005 min
Response: 1895856502
Conc: 520.05 ng/ml

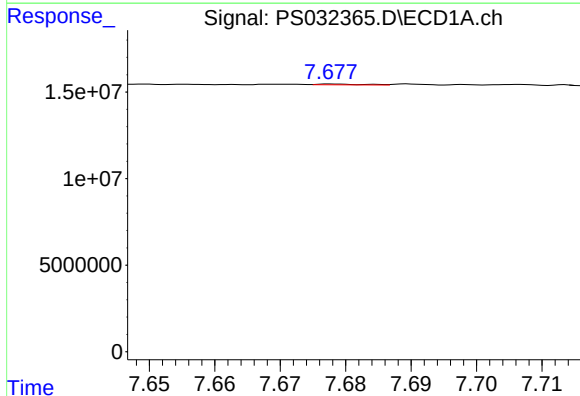


#6 MCP

R.T.: 7.678 min
Delta R.T.: 0.034 min
Response: 225609
Conc: N.D.

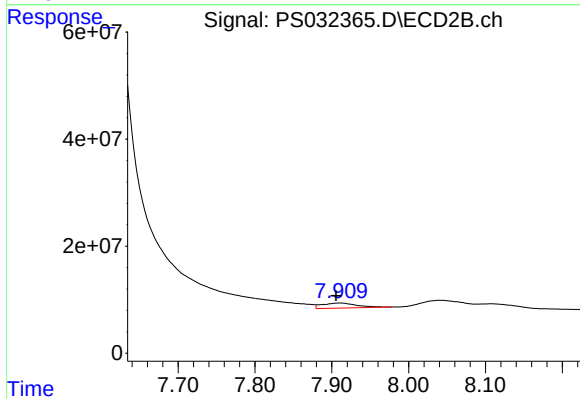

#6 MCP


R.T.: 7.910 min
Delta R.T.: 0.005 min
Response: 29669193
Conc: 2.23 ug/ml

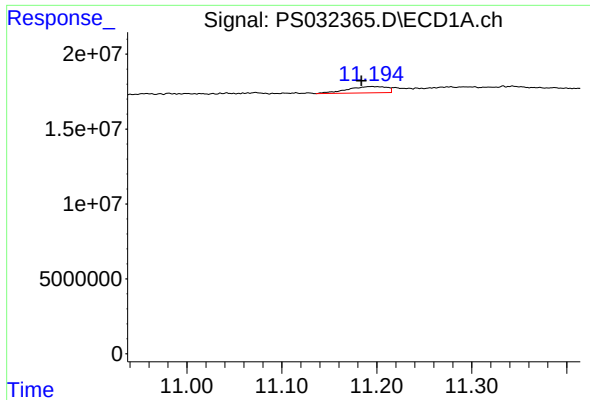

#15 Picloram

R.T.: 11.194 min
Delta R.T.: 0.010 min
Response: 12022545
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

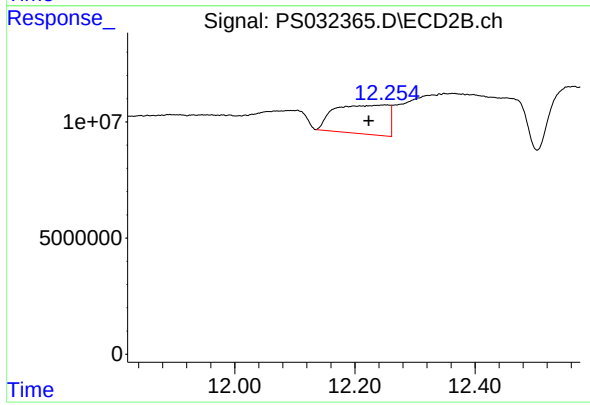

#15 Picloram

R.T.: 12.250 min
Delta R.T.: 0.027 min
Response: 77668275
Conc: 2.09 ng/ml