

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111125\
 Data File : PS032357.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2025 00:33
 Operator : AR\AJ
 Sample : Q3597-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/12/2025
 Supervised By :Yogesh Patel 11/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 01:25:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	7.281	7.617	1218.6E6	1210.6E6	268.931	332.084m
------	----------	-------	-------	----------	----------	---------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111125\
Data File : PS032357.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2025 00:33
Operator : AR\AJ
Sample : Q3597-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/12/2025
Supervised By :Yogesh Patel 11/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 01:25:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

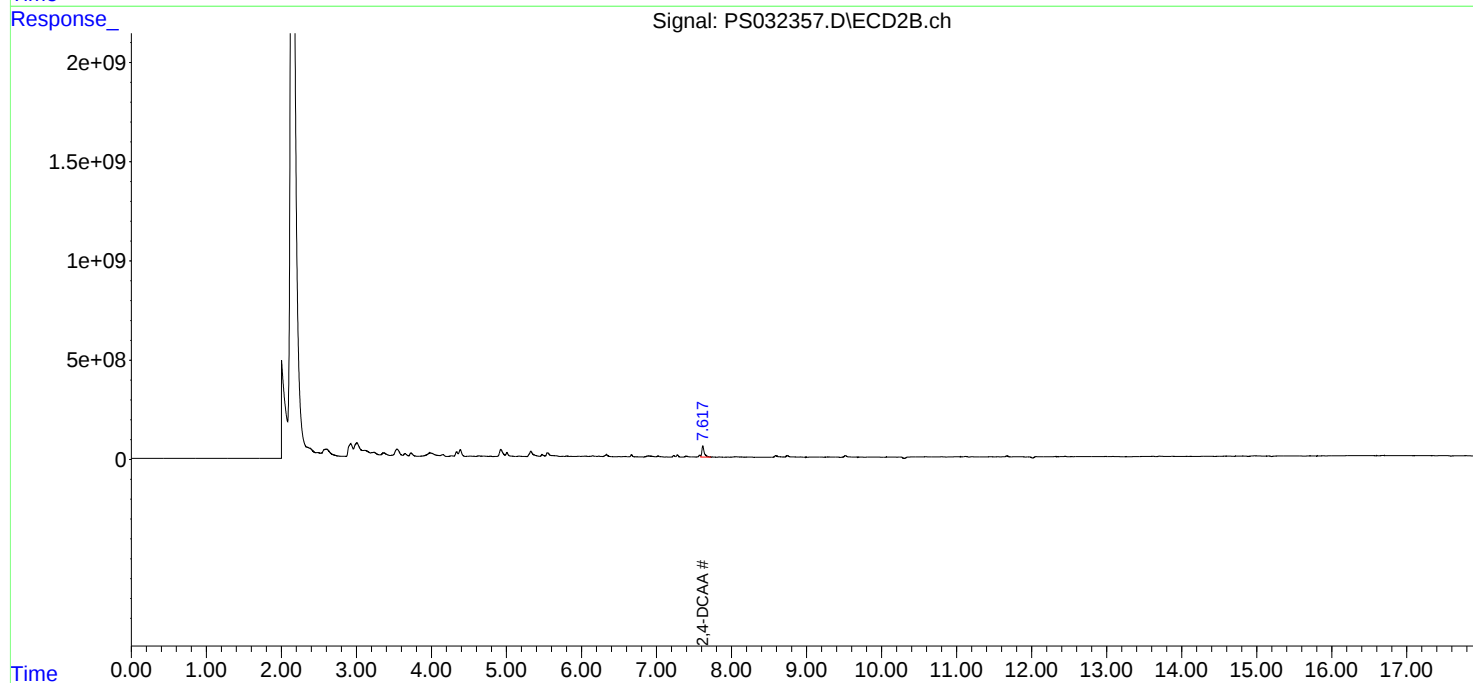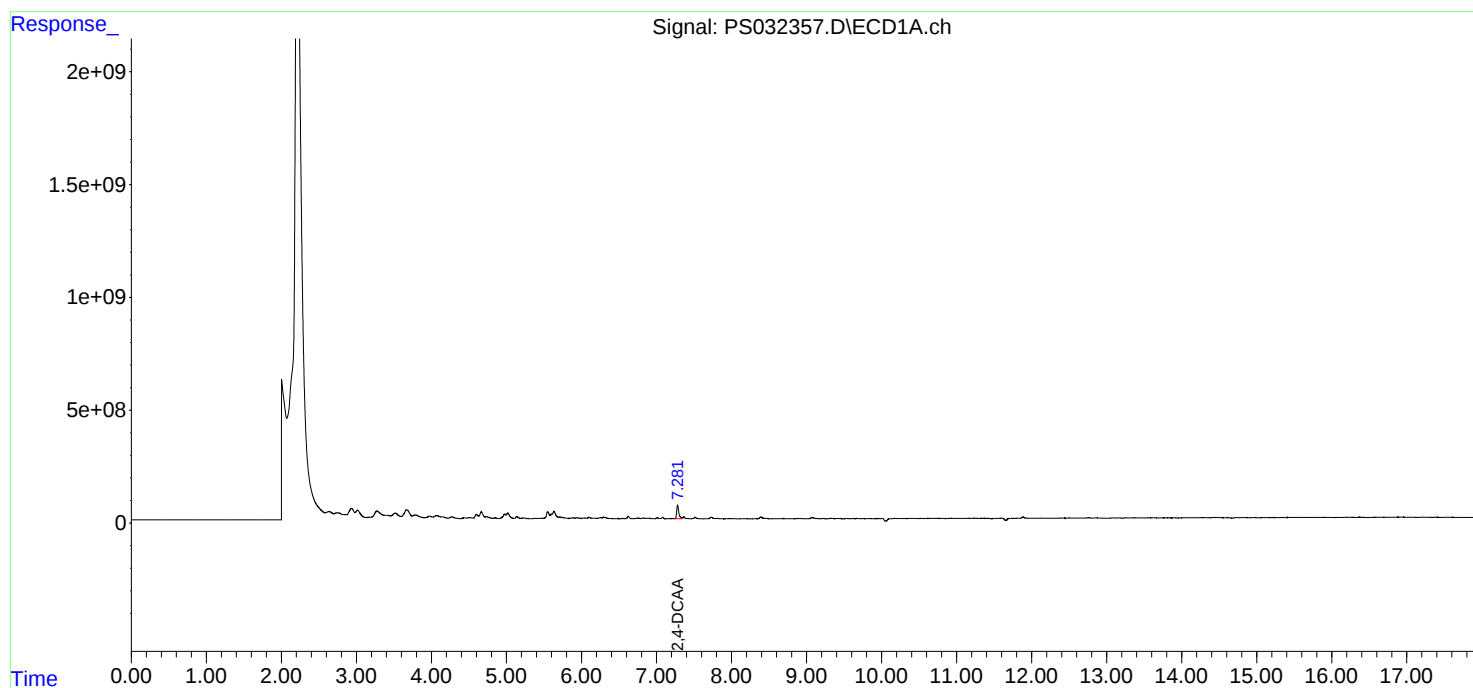

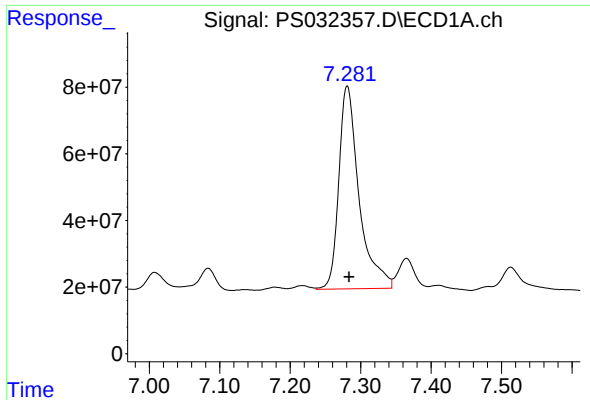


#4 2,4-DCAA

R.T.: 7.281 min
Delta R.T.: -0.002 min
Response: 1218598180
Conc: 268.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/12/2025
Supervised By :Yogesh Patel 11/12/2025

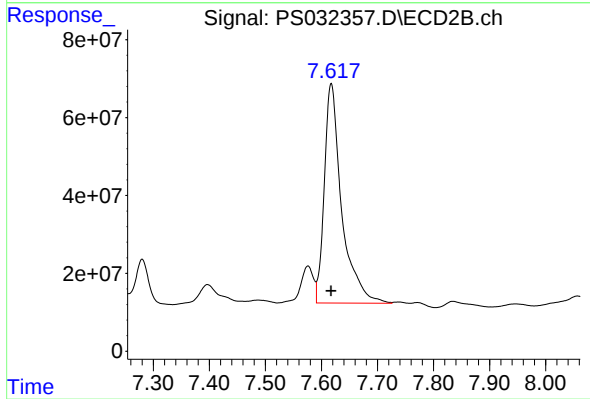

#4 2,4-DCAA

R.T.: 7.617 min
Delta R.T.: 0.000 min
Response: 1210609860
Conc: 332.08 ng/ml m