

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111218\
 Data File : PS002410.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2018 11:15
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 06:38:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.424	10.915	141.0E6	141.0E6	462.896	385.365
Target Compounds							
7) T	MCPA	0.000	11.822	0	1413863	N.D.	1.005 #
10) T	Pentachlo...	0.000	13.338	0	418618	N.D.	0.082 #
12) T	2,4,5-T	0.000	14.565	0	202565	N.D.	0.130 #
16) T	D CPA	0.000	16.868	0	131124	N.D.	0.055 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111218\
Data File : PS002410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2018 11:15
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 06:38:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

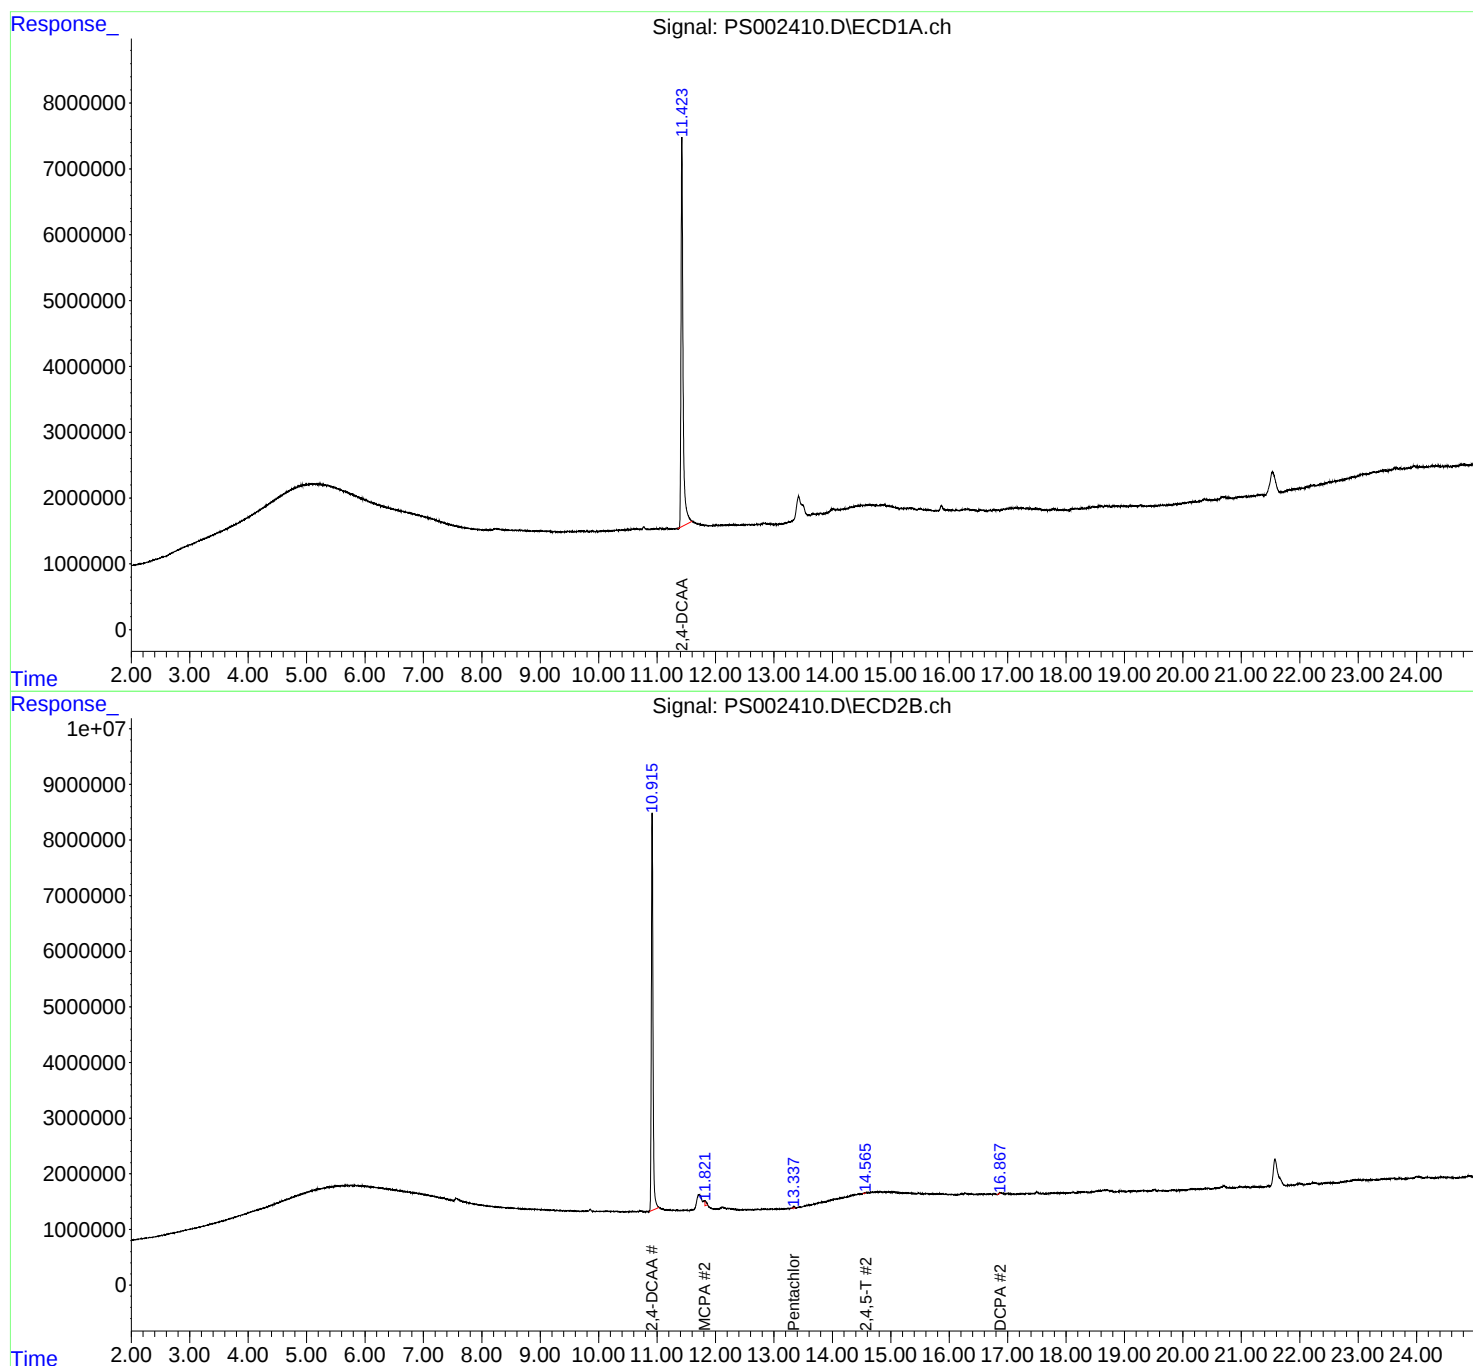


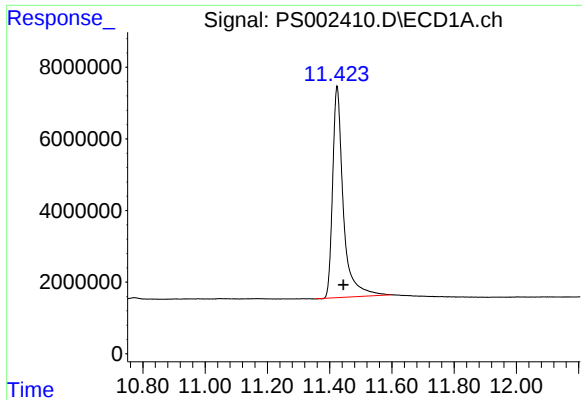

#4 2,4-DCAA


R.T.: 11.424 min
Delta R.T.: -0.020 min
Response: 140998093
Conc: 462.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

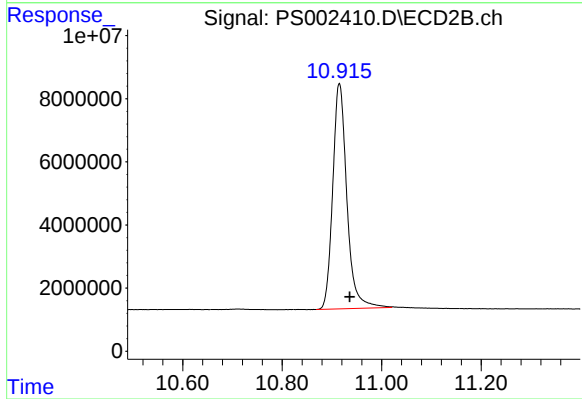


#4 2,4-DCAA

R.T.: 10.915 min
Delta R.T.: -0.021 min
Response: 141009854
Conc: 385.37 ng/ml

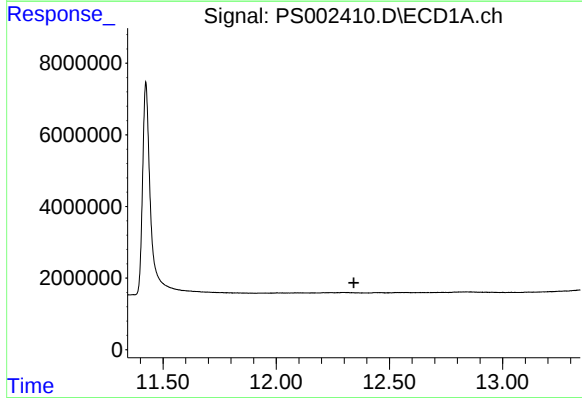


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

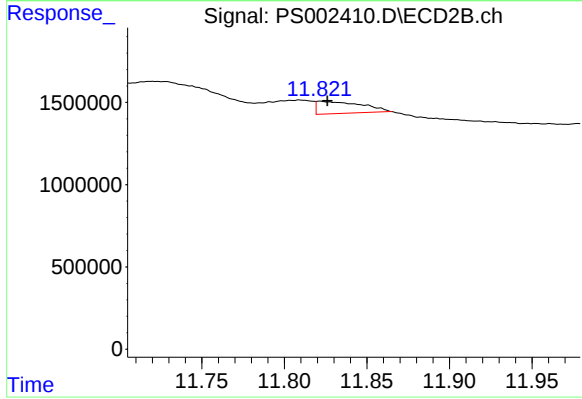

#7 MCPA


R.T.: 11.822 min
Delta R.T.: -0.005 min
Response: 1413863
Conc: 1.00 ug/ml

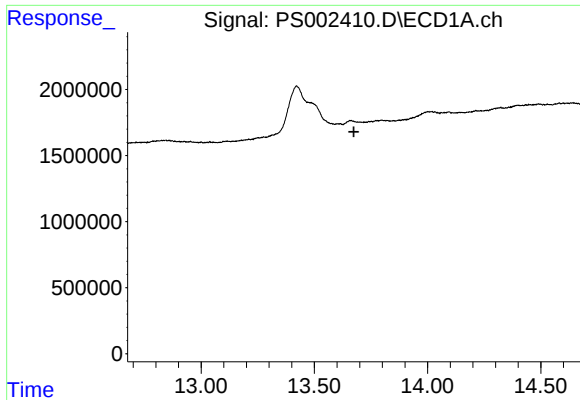

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

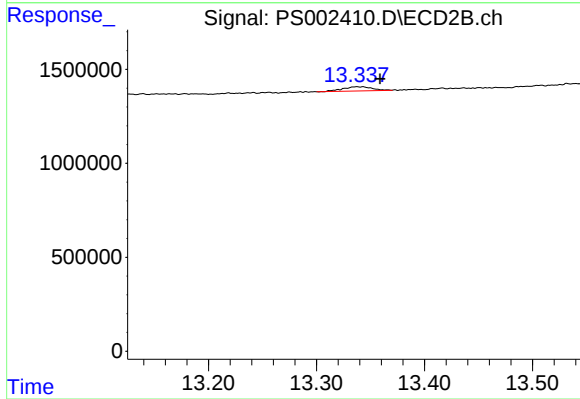


#10 Pentachlorophenol

R.T.: 13.338 min
Delta R.T.: -0.021 min
Response: 418618
Conc: 0.08 ng/ml

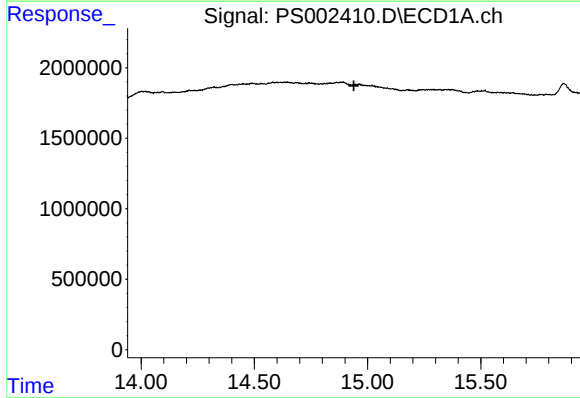


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.940 min
Response: 0
Conc: N.D.

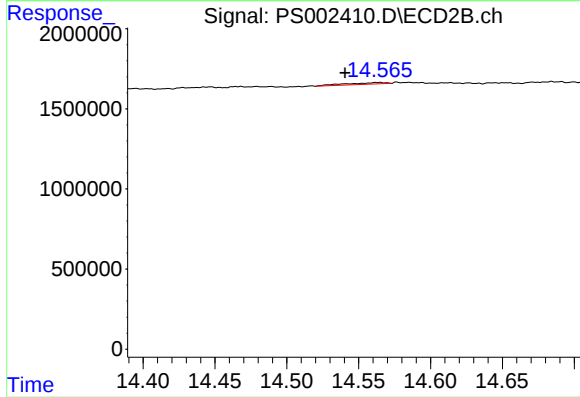

#12 2,4,5-T


R.T.: 14.565 min
Delta R.T.: 0.025 min
Response: 202565
Conc: 0.13 ng/ml

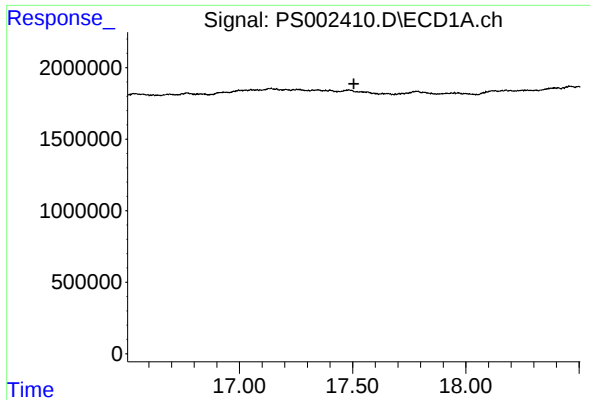

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

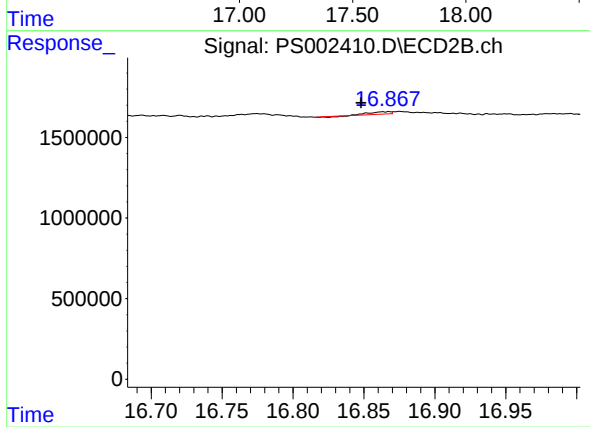

#16 DCPA

R.T.: 16.868 min
Delta R.T.: 0.020 min
Response: 131124
Conc: 0.05 ng/ml