

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111218\
 Data File : PS002412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2018 19:30
 Operator : EI\SJ
 Sample : J5269-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 06:38:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.408	10.900	160.8E6	155.4E6	528.018	424.580
Target Compounds							
1) T	Dalapon	0.000	2.446	0	8937110	N.D.	20.765 #
2) T	3,5-DICHL...	0.000	9.144	0	23580568	N.D.	52.014 #
3) T	4-Nitroph...	0.000	10.065	0	386661	N.D.	2.207 #
5) T	DICAMBA	0.000	11.266	0	574212	N.D.	0.424 #
6) T	MCP	12.089	0.000	47395061	0	50.499	N.D. #
7) T	MCPA	0.000	11.798	0	6042203	N.D.	4.294 #
12) T	2,4,5-T	0.000	14.556	0	2053598	N.D.	1.314 #
13) T	2,4-DB	0.000	15.256	0	42198	N.D.	0.186 #
14) T	DINOSEB	0.000	15.637	0	2498137	N.D.	1.669 #
15) T	Picloram	16.925	16.822	23042507	31312704	10.850	11.770
16) T	DCPA	0.000	16.822	0	31312704	N.D.	13.057 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111218\
Data File : PS002412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2018 19:30
Operator : EI\SJ
Sample : J5269-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 06:38:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

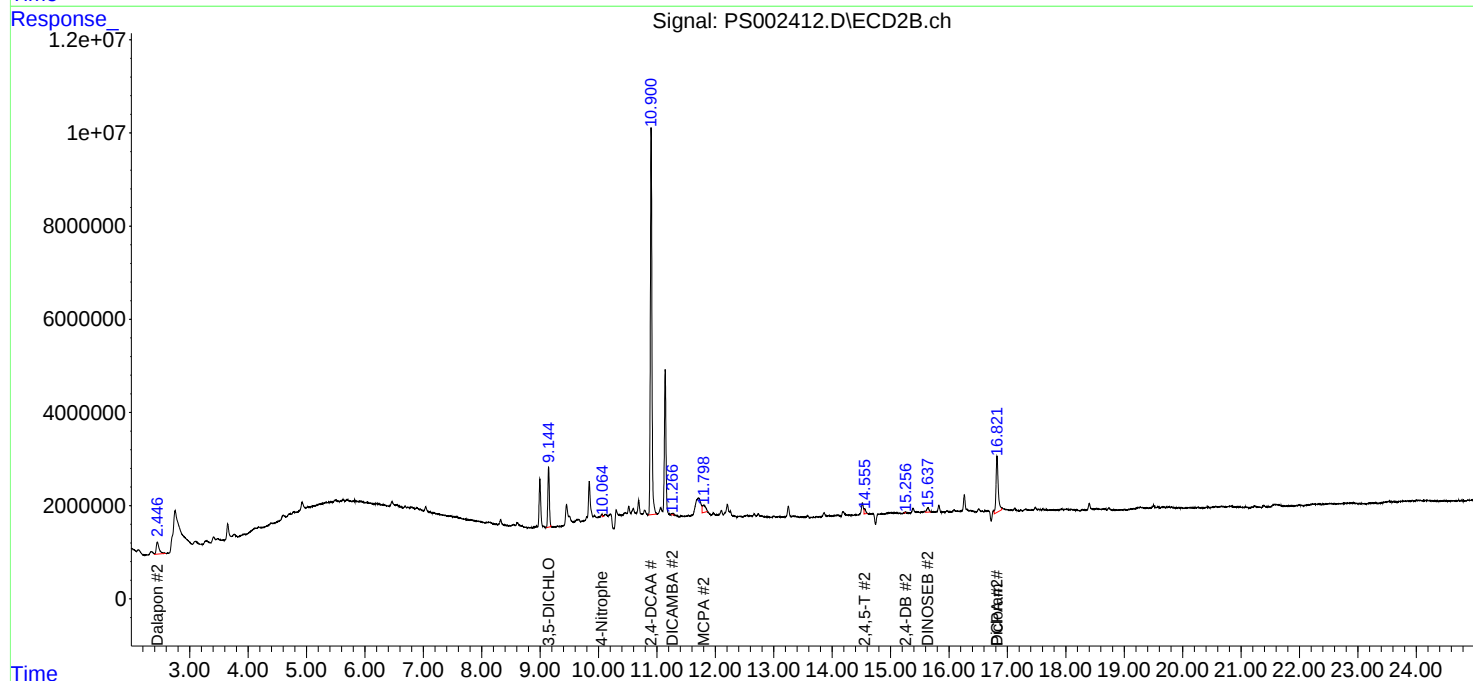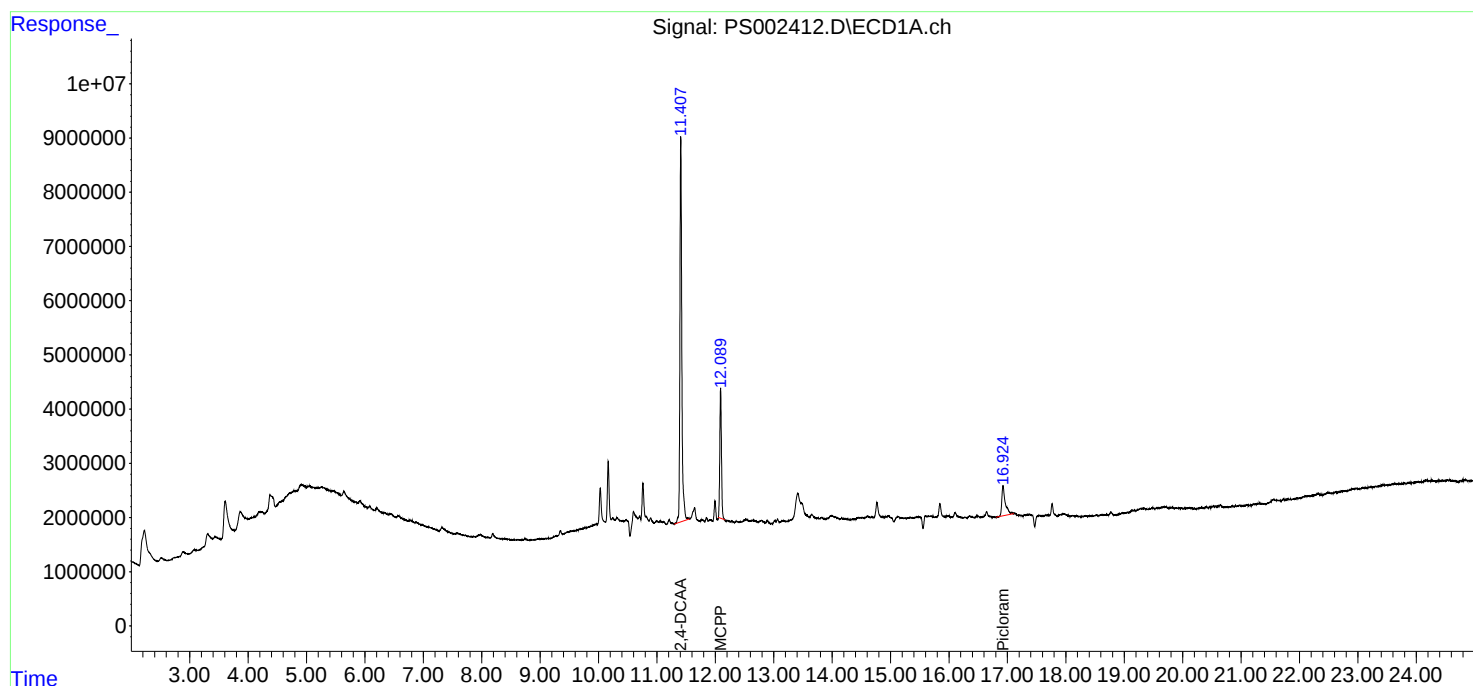


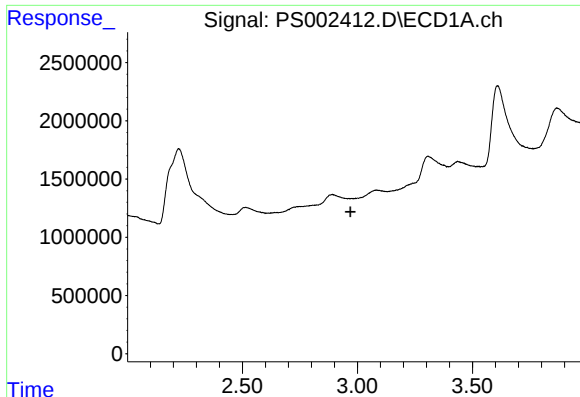

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

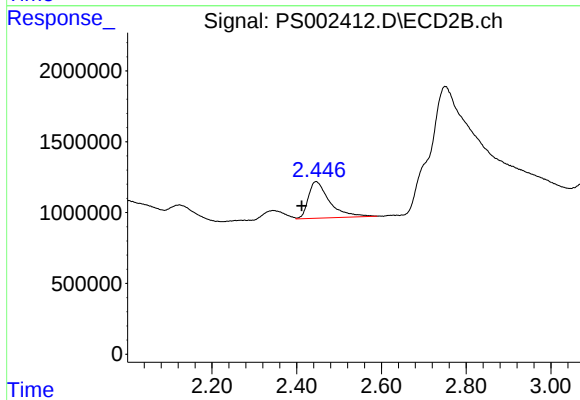


#1 Dalapon

R.T.: 2.446 min
Delta R.T.: 0.034 min
Response: 8937110
Conc: 20.76 ng/ml

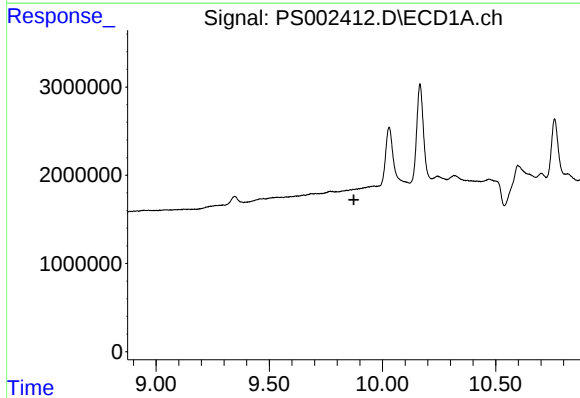


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.874 min
Response: 0
Conc: N.D.

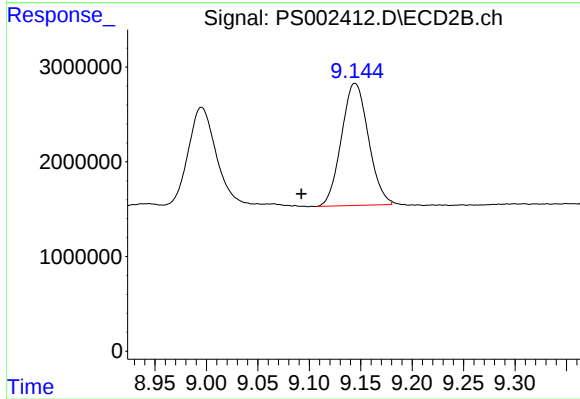

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.144 min
Delta R.T.: 0.052 min
Response: 23580568
Conc: 52.01 ng/ml

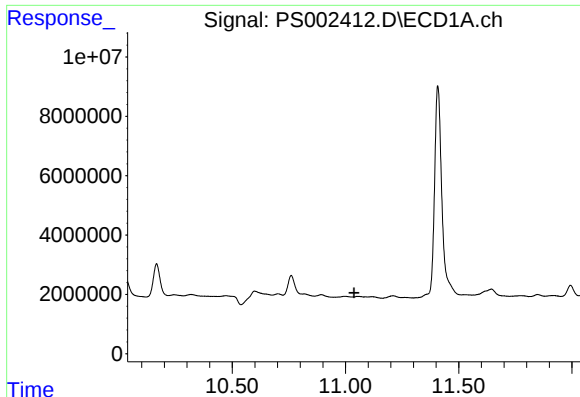

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

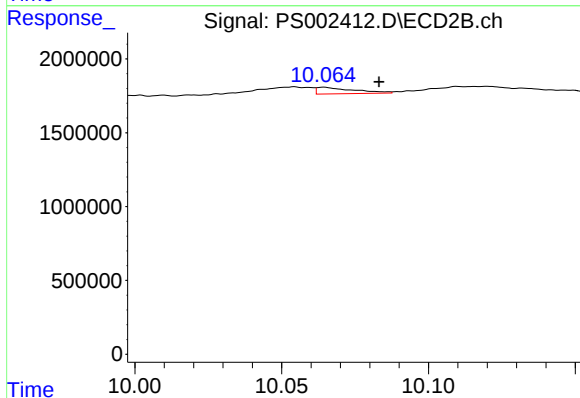


#3 4-Nitrophenol

R.T.: 10.065 min
Delta R.T.: -0.019 min
Response: 386661
Conc: 2.21 ng/ml

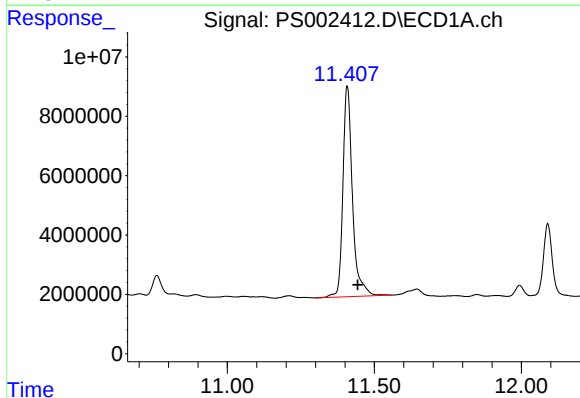


#4 2,4-DCAA

R.T.: 11.408 min
Delta R.T.: -0.036 min
Response: 160833977
Conc: 528.02 ng/ml

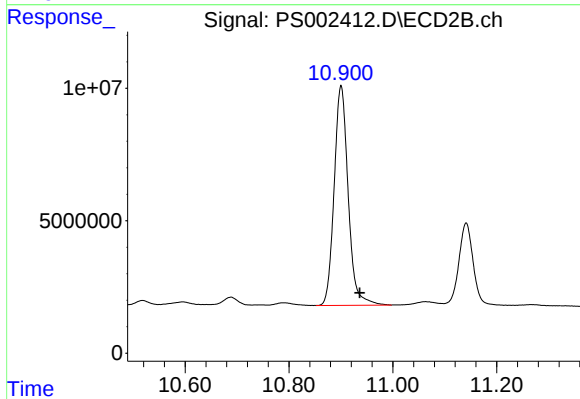

#4 2,4-DCAA


R.T.: 10.900 min
Delta R.T.: -0.036 min
Response: 155358852
Conc: 424.58 ng/ml

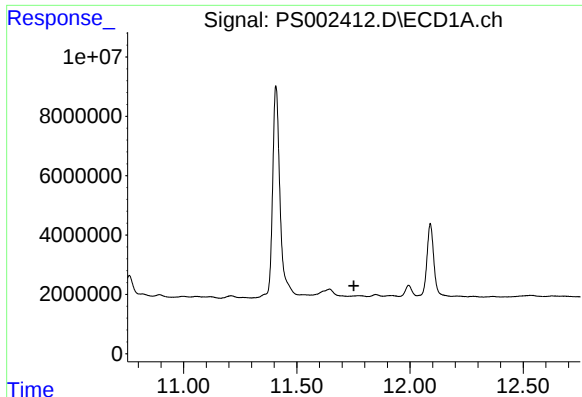

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

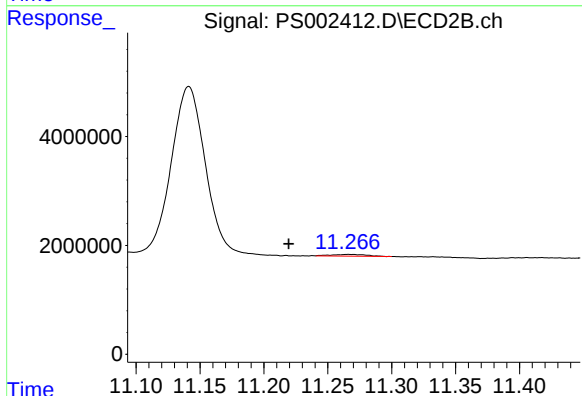


#5 DICAMBA

R.T.: 11.266 min
Delta R.T.: 0.047 min
Response: 574212
Conc: 0.42 ng/ml

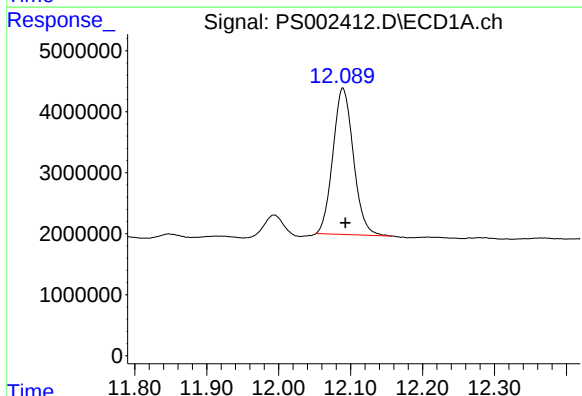


#6 MCP

R.T.: 12.089 min
Delta R.T.: -0.003 min
Response: 47395061
Conc: 50.50 ug/ml

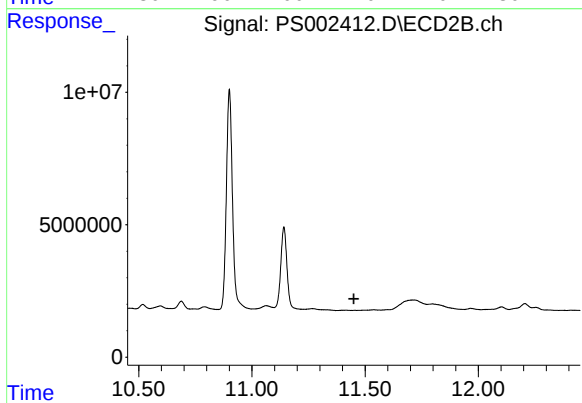

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.450 min
Response: 0
Conc: N.D.

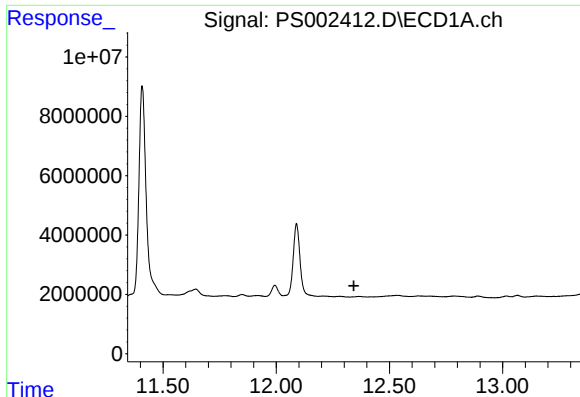

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

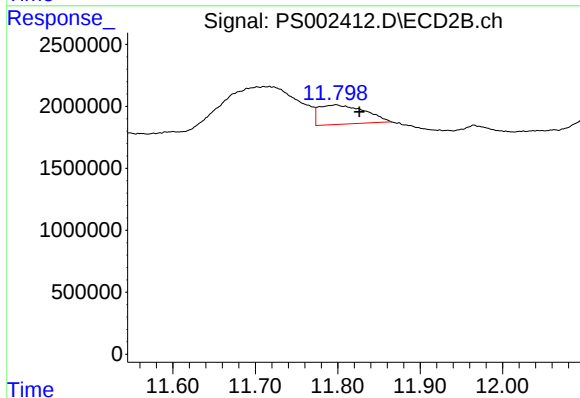


#7 MCPA

R.T.: 11.798 min
Delta R.T.: -0.028 min
Response: 6042203
Conc: 4.29 ug/ml

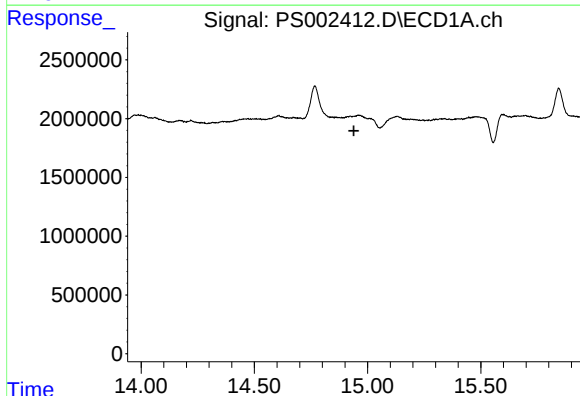


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.940 min
Response: 0
Conc: N.D.

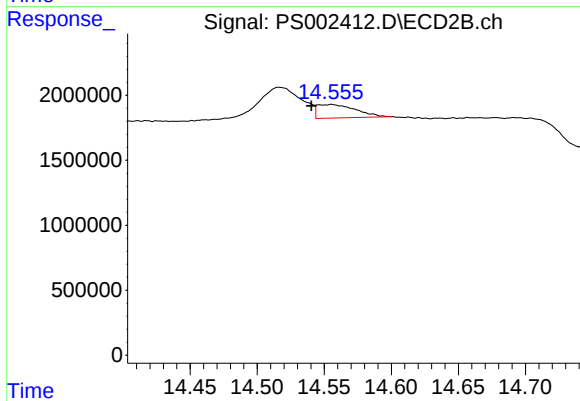

#12 2,4,5-T


R.T.: 14.556 min
Delta R.T.: 0.015 min
Response: 2053598
Conc: 1.31 ng/ml

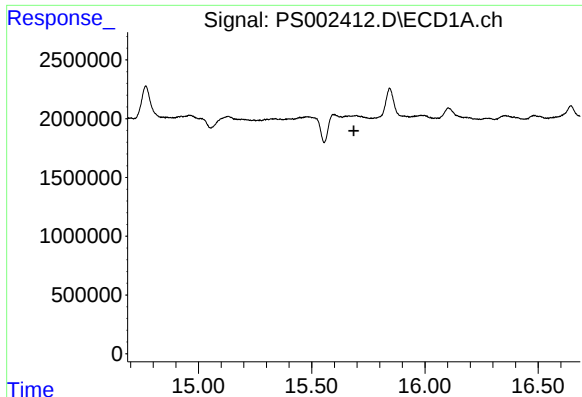

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

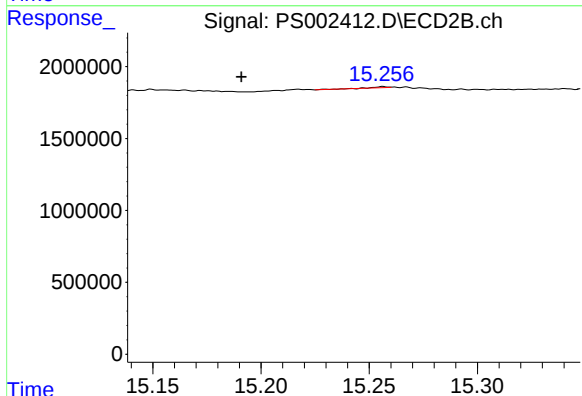


#13 2,4-DB

R.T.: 15.256 min
Delta R.T.: 0.065 min
Response: 42198
Conc: 0.19 ng/ml

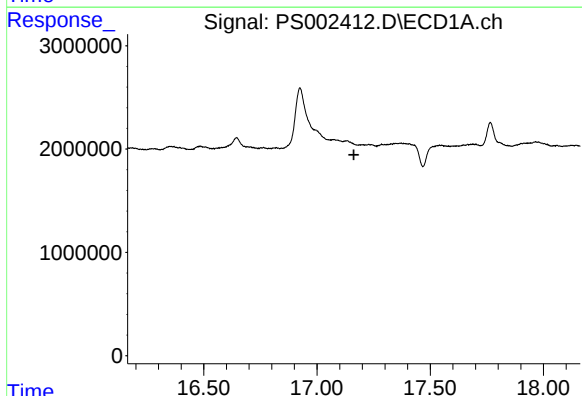


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.163 min
Response: 0
Conc: N.D.

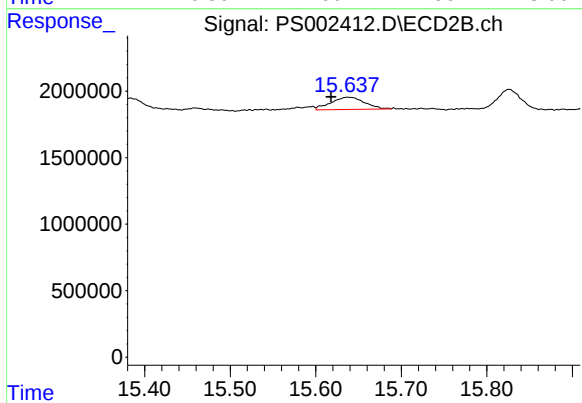

#14 DINOSEB


R.T.: 15.637 min
Delta R.T.: 0.019 min
Response: 2498137
Conc: 1.67 ng/ml

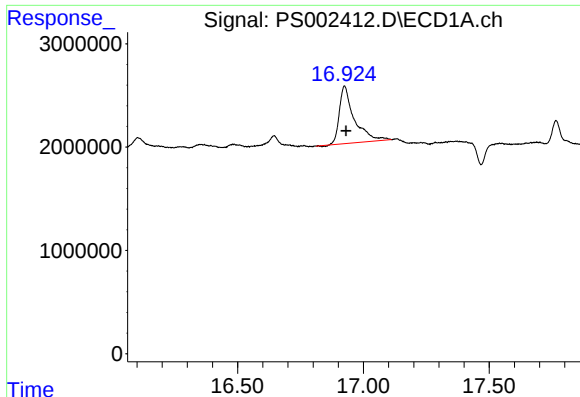

#15 Picloram


R.T.: 16.925 min
Delta R.T.: -0.007 min
Response: 23042507
Conc: 10.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

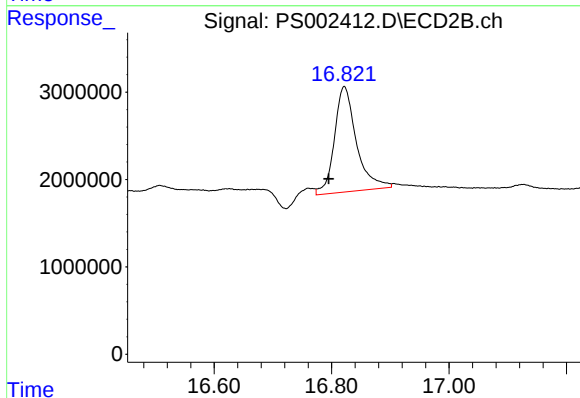


#15 Picloram

R.T.: 16.822 min
Delta R.T.: 0.027 min
Response: 31312704
Conc: 11.77 ng/ml

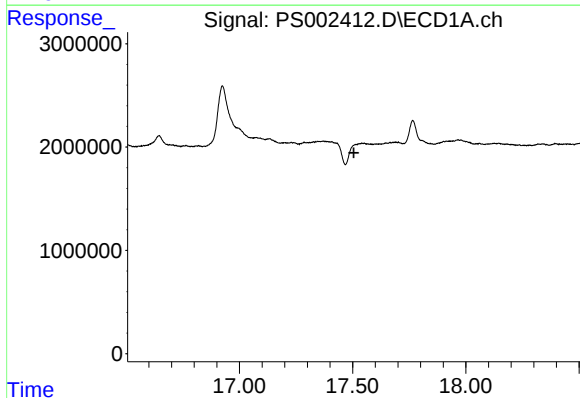

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

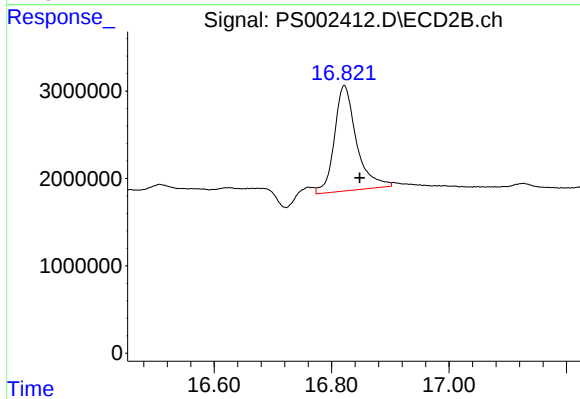

#16 DCPA

R.T.: 16.822 min
Delta R.T.: -0.027 min
Response: 31312704
Conc: 13.06 ng/ml