

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111218\
 Data File : PS002416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2018 21:34
 Operator : EI\SJ
 Sample : J5269-18
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 06:40:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.405	10.897	152.0E6	148.7E6	498.910	406.347
Target Compounds							
2) T	3,5-DICHL...	0.000	9.058	0	1139837	N.D.	2.514 #
3) T	4-Nitroph...	0.000	10.055	0	6819240	N.D.	38.920 #
5) T	DICAMBA	0.000	11.270	0	1188622	N.D.	0.879 #
6) T	MCP	12.085	11.495	58645146	66819	62.486	0.074 #
7) T	MCPA	0.000	11.798	0	7914362	N.D.	5.624 #
10) T	Pentachlo...	13.639	13.320	6826743	2312664	1.411	0.454 #
12) T	2,4,5-T	0.000	14.558	0	1402908	N.D.	0.897 #
14) T	DINOSEB	0.000	15.632	0	2426806	N.D.	1.621 #
15) T	Picloram	0.000	16.830	0	4320092	N.D.	1.624 #
16) T	DCPA	17.539	16.830	3396187	4320092	1.466	1.801



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111218\
Data File : PS002416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2018 21:34
Operator : EI\SJ
Sample : J5269-18
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 06:40:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

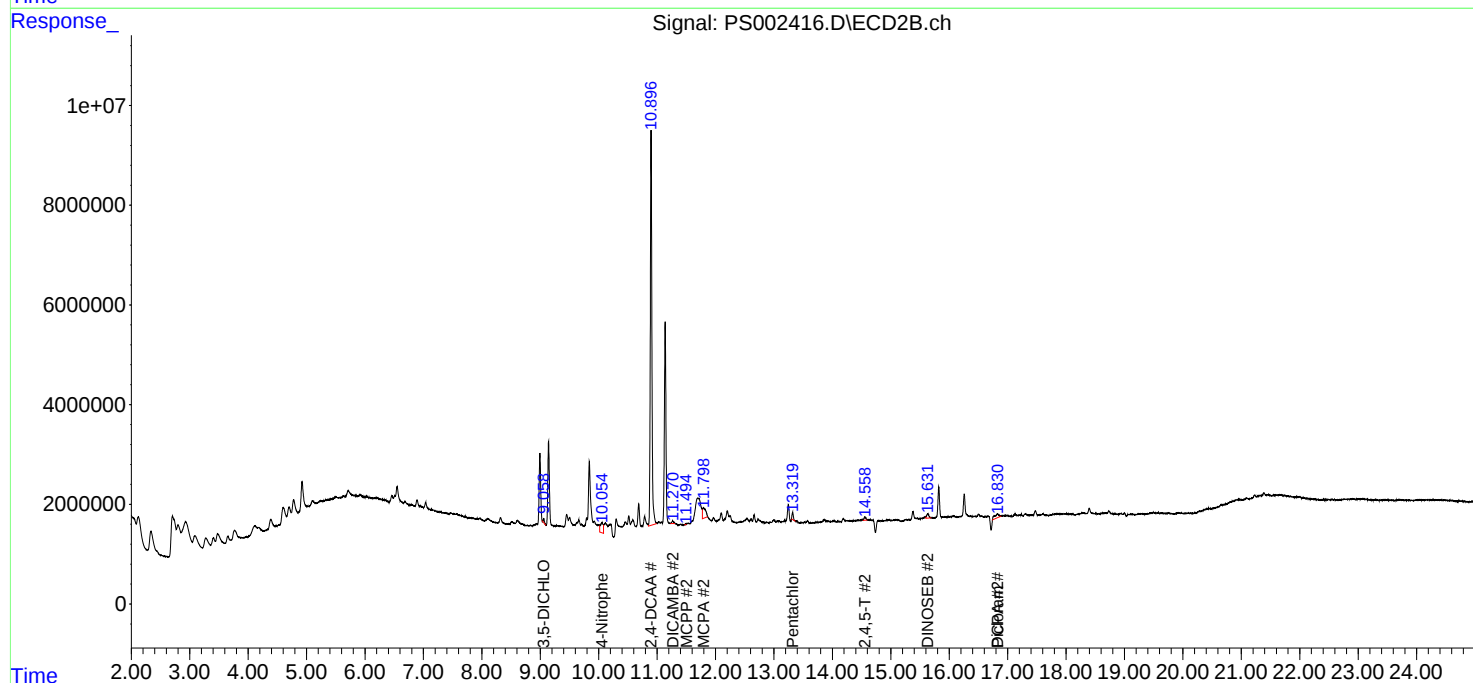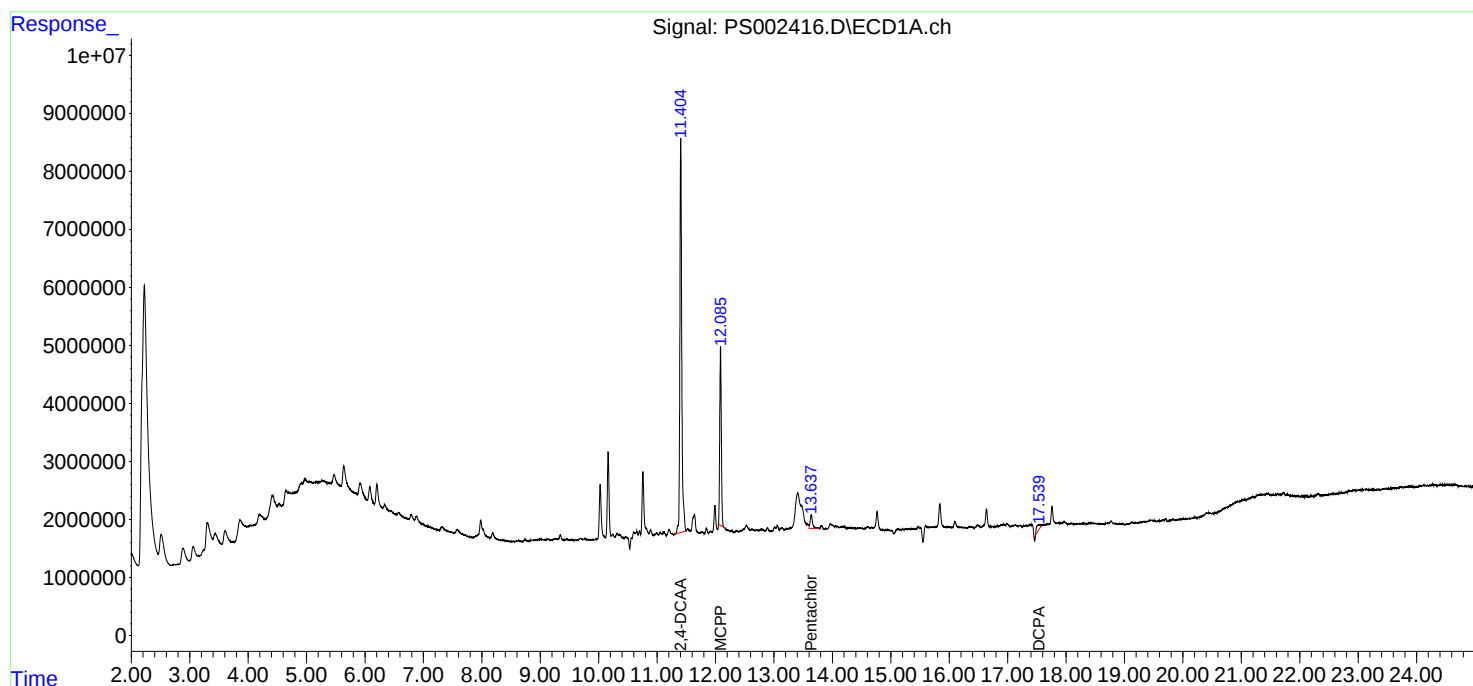


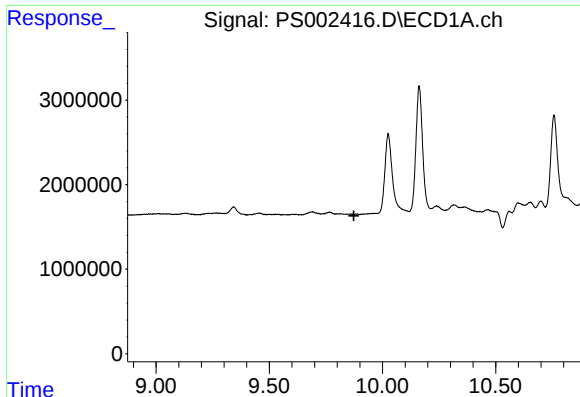

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

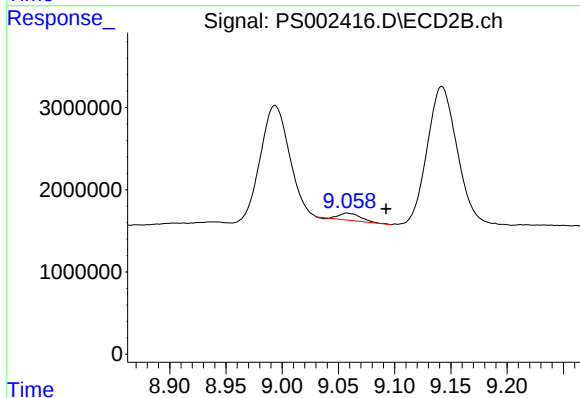


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.058 min
Delta R.T.: -0.035 min
Response: 1139837
Conc: 2.51 ng/ml

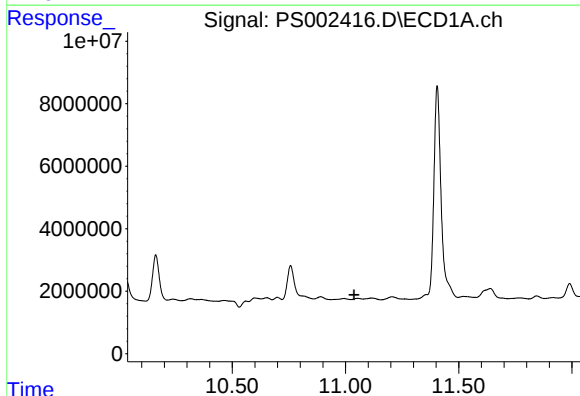


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

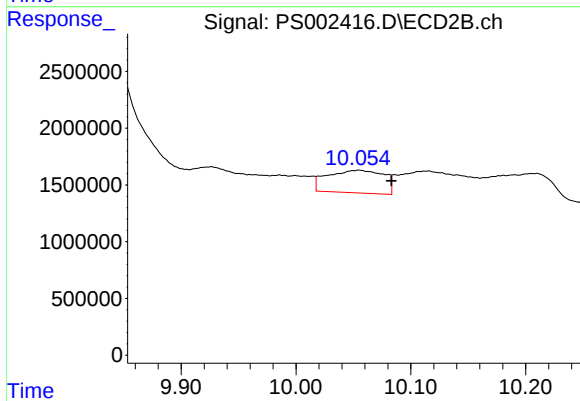

#3 4-Nitrophenol


R.T.: 10.055 min
Delta R.T.: -0.028 min
Response: 6819240
Conc: 38.92 ng/ml

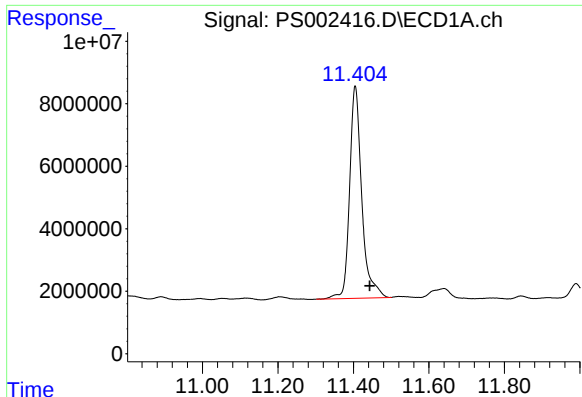

#4 2,4-DCAA


R.T.: 11.405 min
Delta R.T.: -0.039 min
Response: 151967811
Conc: 498.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

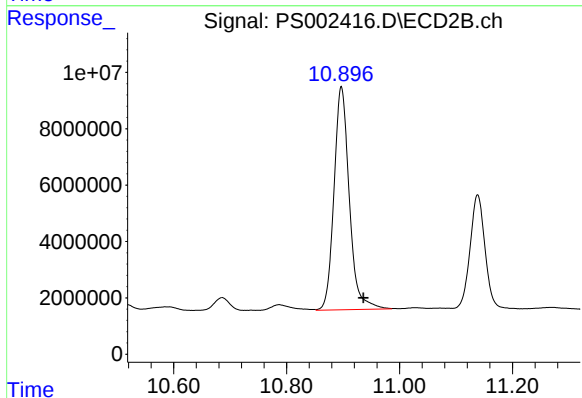


#4 2,4-DCAA

R.T.: 10.897 min
Delta R.T.: -0.039 min
Response: 148687444
Conc: 406.35 ng/ml

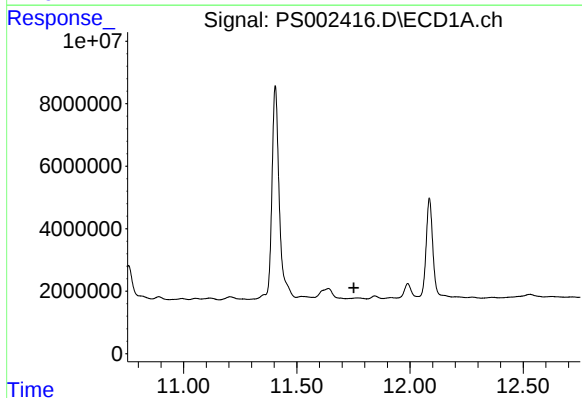


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.752 min
Response: 0
Conc: N.D.

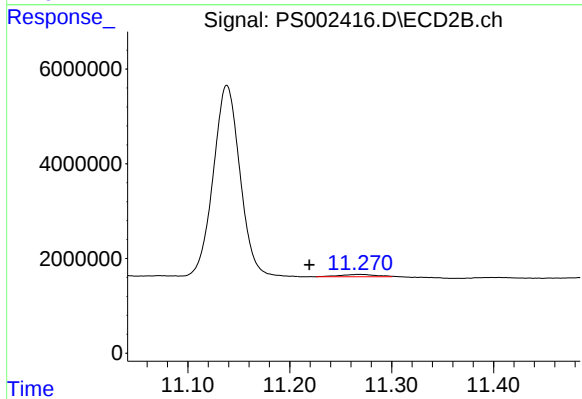

#5 DICAMBA


R.T.: 11.270 min
Delta R.T.: 0.050 min
Response: 1188622
Conc: 0.88 ng/ml

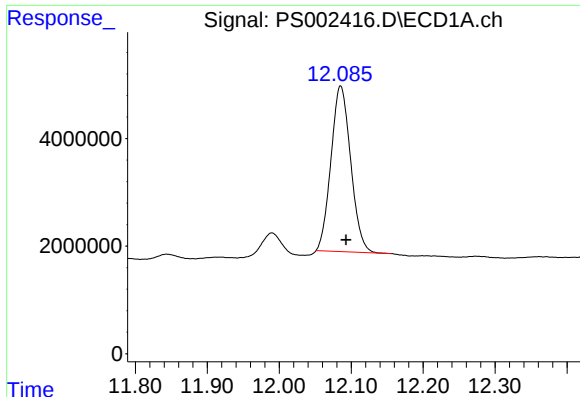

#6 MCPP


R.T.: 12.085 min
Delta R.T.: -0.007 min
Response: 58645146
Conc: 62.49 ug/ml

Instrument :
ECD_S
ClientSampleId :

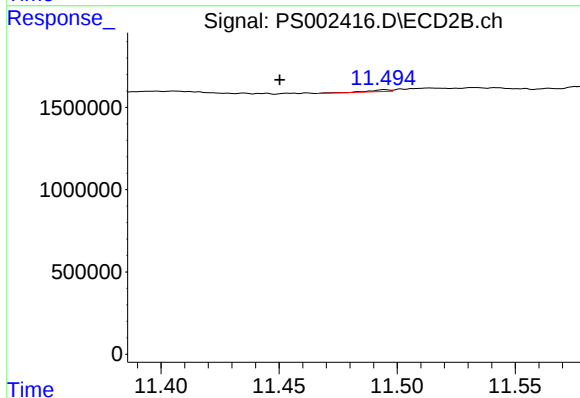


#6 MCPP

R.T.: 11.495 min
Delta R.T.: 0.045 min
Response: 66819
Conc: 0.07 ug/ml

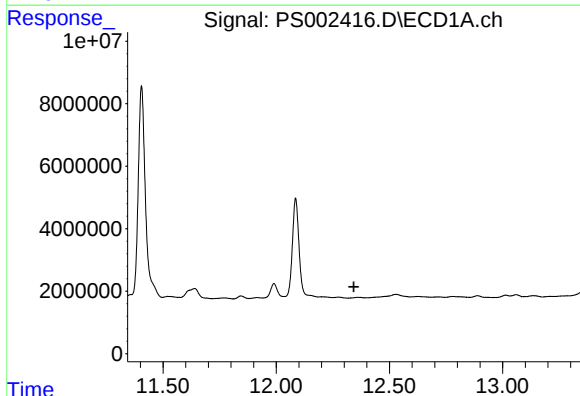


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

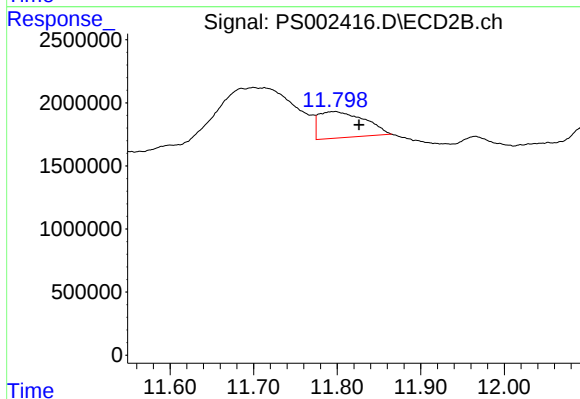

#7 MCPA


R.T.: 11.798 min
Delta R.T.: -0.028 min
Response: 7914362
Conc: 5.62 ug/ml

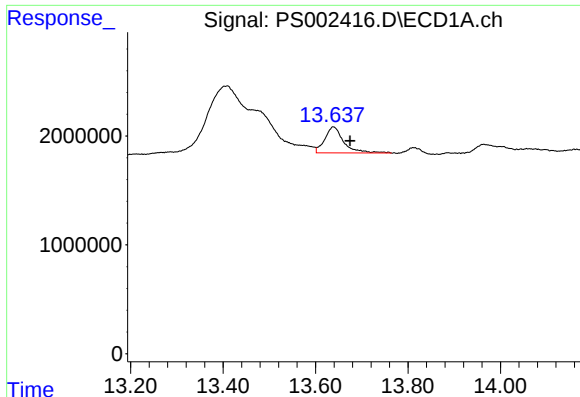

#10 Pentachlorophenol


R.T.: 13.639 min
Delta R.T.: -0.036 min
Response: 6826743
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

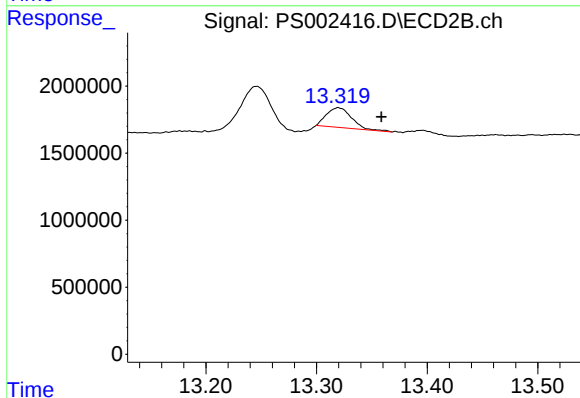


#10 Pentachlorophenol

R.T.: 13.320 min
Delta R.T.: -0.039 min
Response: 2312664
Conc: 0.45 ng/ml

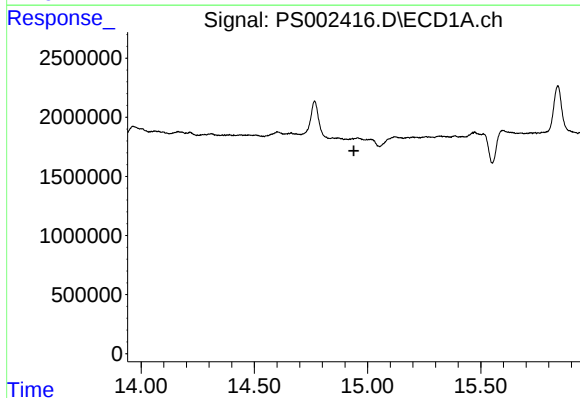


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.940 min
Response: 0
Conc: N.D.

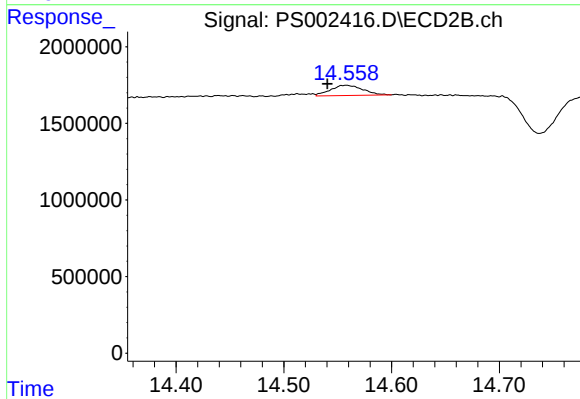

#12 2,4,5-T


R.T.: 14.558 min
Delta R.T.: 0.018 min
Response: 1402908
Conc: 0.90 ng/ml

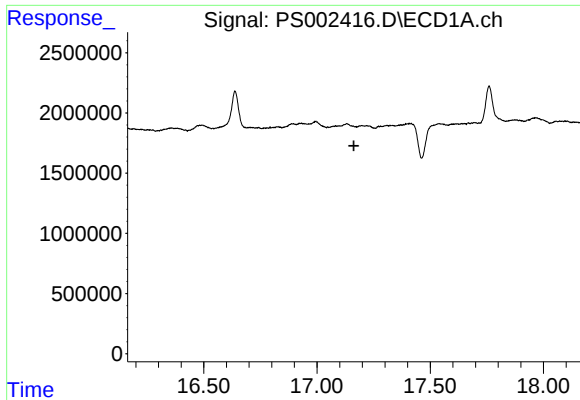

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

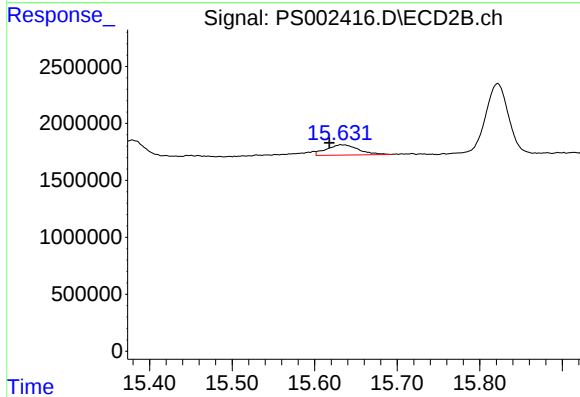


#14 DINOSEB

R.T.: 15.632 min
Delta R.T.: 0.013 min
Response: 2426806
Conc: 1.62 ng/ml

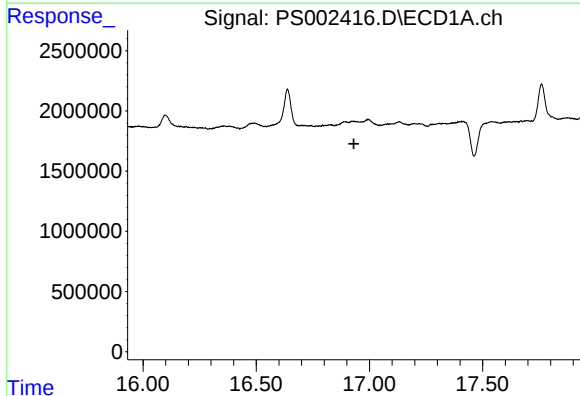


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.931 min
Response: 0
Conc: N.D.

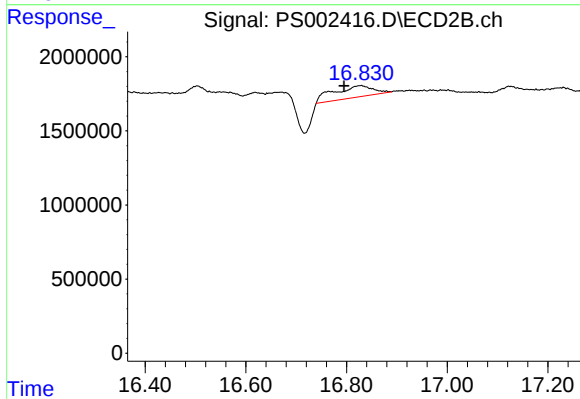

#15 Picloram


R.T.: 16.830 min
Delta R.T.: 0.035 min
Response: 4320092
Conc: 1.62 ng/ml

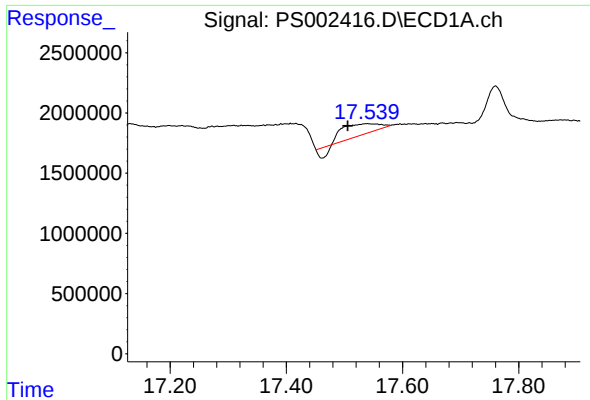

#16 DCPA

R.T.: 17.539 min
Delta R.T.: 0.033 min
Response: 3396187
Conc: 1.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

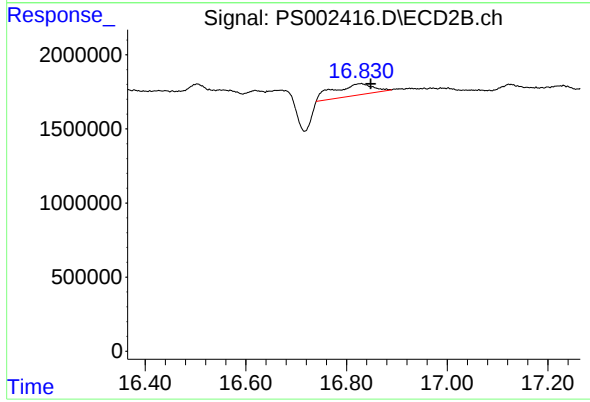

#16 DCPA

R.T.: 16.830 min
Delta R.T.: -0.018 min
Response: 4320092
Conc: 1.80 ng/ml