

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111218\
 Data File : PS002417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2018 22:05
 Operator : EI\SJ
 Sample : J5269-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 06:40:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.452	10.946	145.7E6	141.2E6	478.393	385.905
Target Compounds							
1) T	Dalapon	2.932	2.384	10767016	17928704	24.418	41.657 #
2) T	3,5-DICHL...	0.000	9.106	0	1044103	N.D.	2.303 #
3) T	4-Nitroph...	0.000	10.103	0	3128862	N.D.	17.858 #
5) T	DICAMBA	11.688	11.187	8002050	23022514	5.775	17.019 #
6) T	MCPD	12.133	0.000	30339107	0	32.326	N.D. #
7) T	MCPA	0.000	11.832	0	699806	N.D.	0.497 #
9) T	2,4-D	0.000	12.781	0	509819	N.D.	1.276 #
10) T	Pentachlo...	0.000	13.294	0	1873297	N.D.	0.368 #
14) T	DINOSEB	0.000	15.678	0	1402070	N.D.	0.937 #
16) T	DCPA	0.000	16.874	0	510484	N.D.	0.213 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111218\
Data File : PS002417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2018 22:05
Operator : EI\SJ
Sample : J5269-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 06:40:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

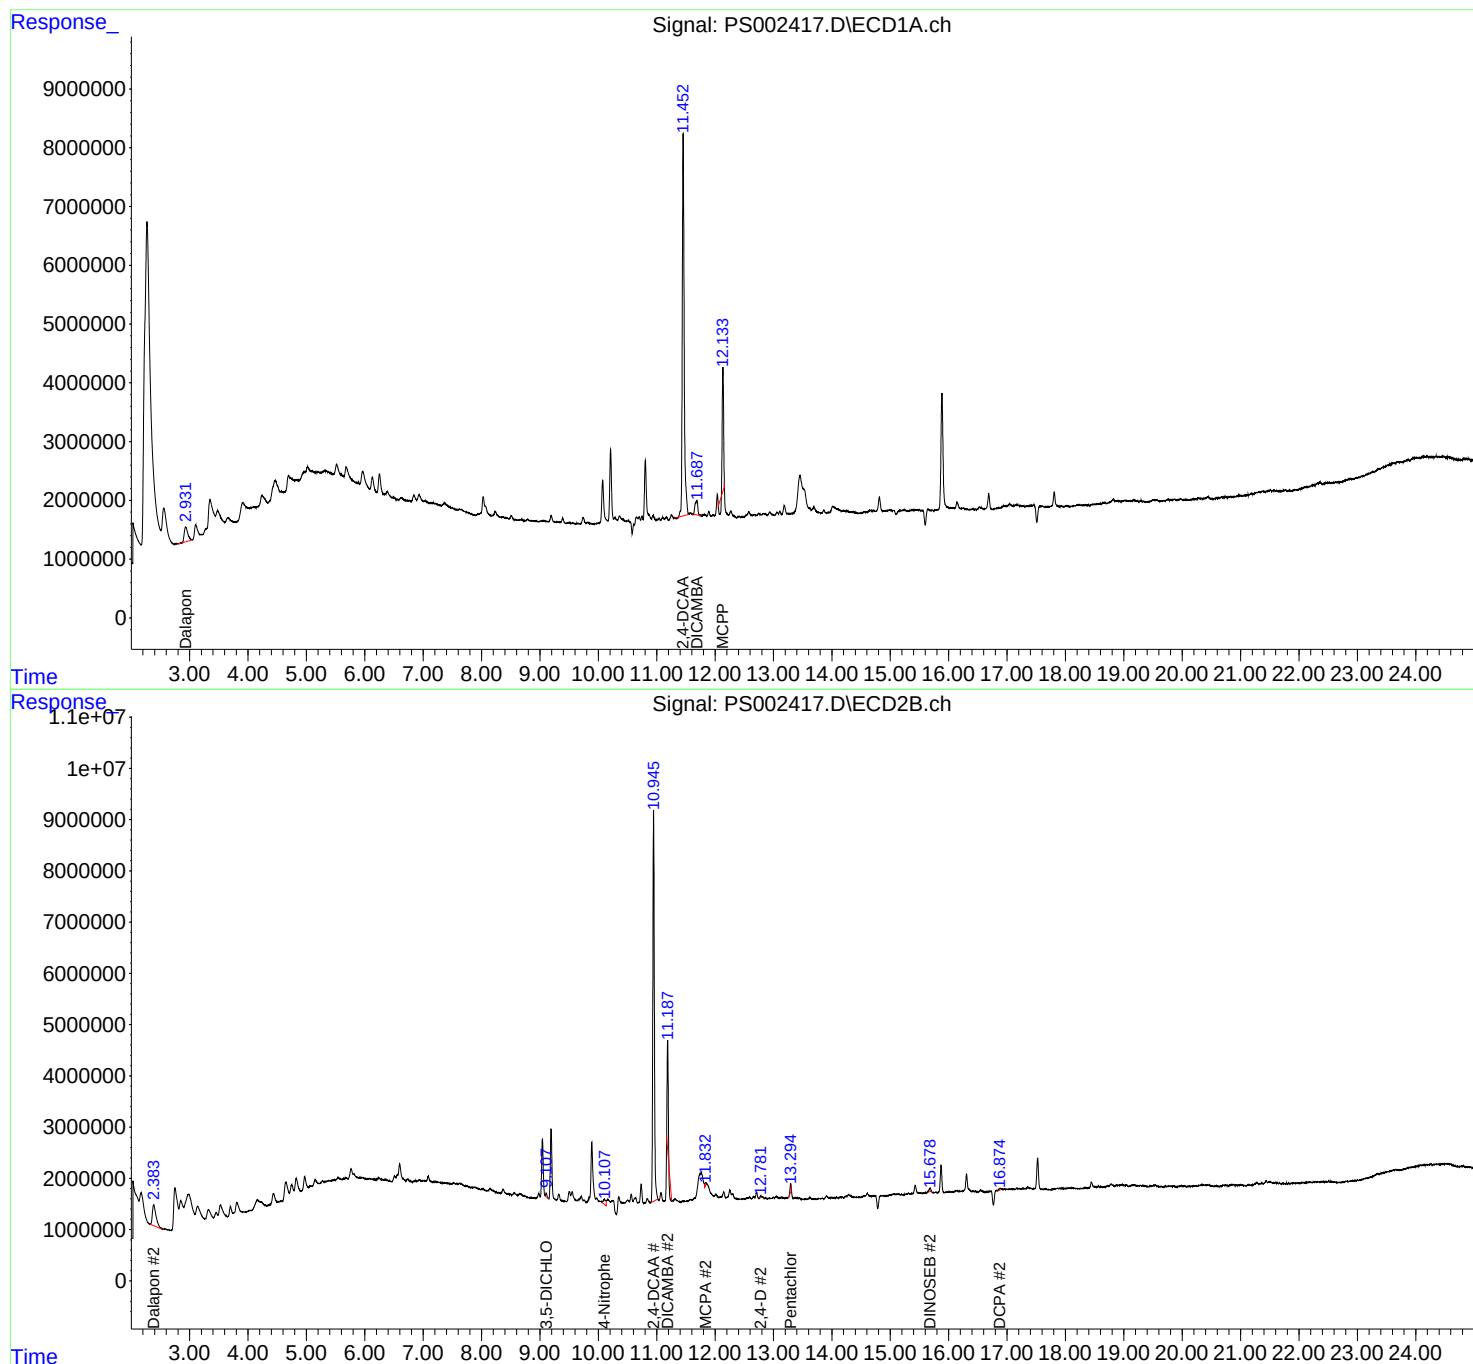


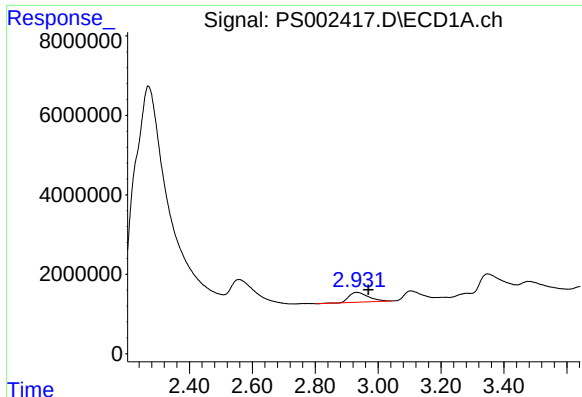

#1 Dalapon


R.T.: 2.932 min
Delta R.T.: -0.037 min
Response: 10767016
Conc: 24.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

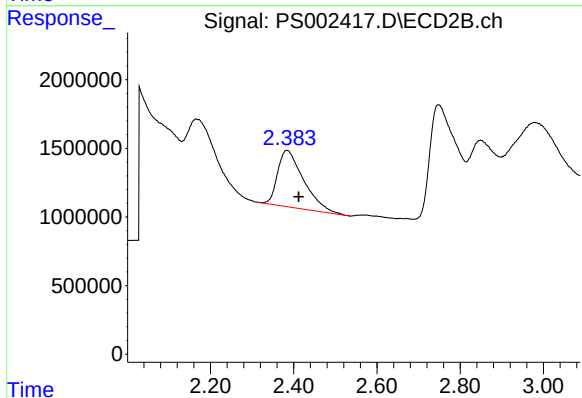


#1 Dalapon

R.T.: 2.384 min
Delta R.T.: -0.028 min
Response: 17928704
Conc: 41.66 ng/ml

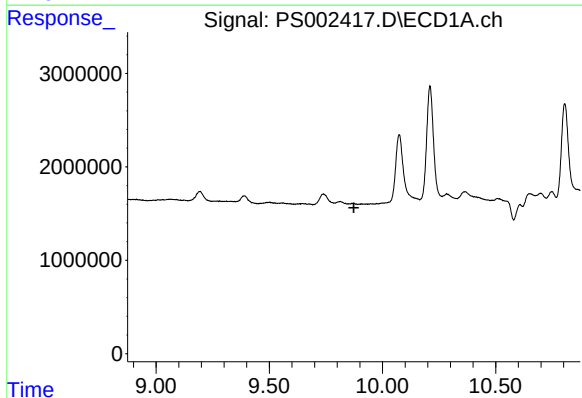


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.874 min
Response: 0
Conc: N.D.

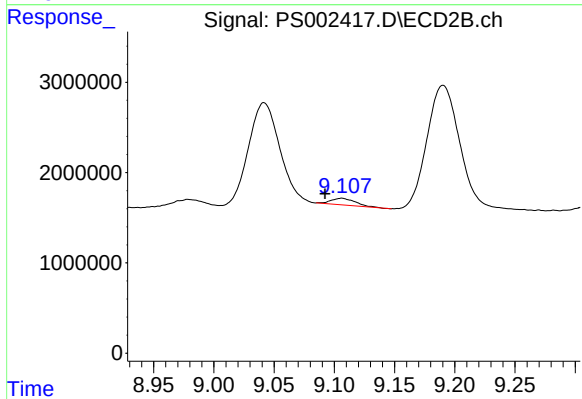

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.106 min
Delta R.T.: 0.014 min
Response: 1044103
Conc: 2.30 ng/ml

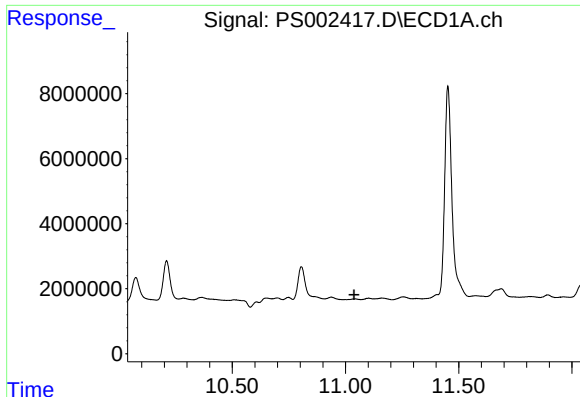

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

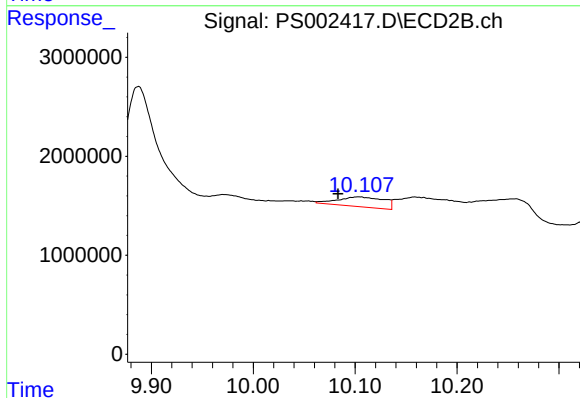


#3 4-Nitrophenol

R.T.: 10.103 min
Delta R.T.: 0.020 min
Response: 3128862
Conc: 17.86 ng/ml

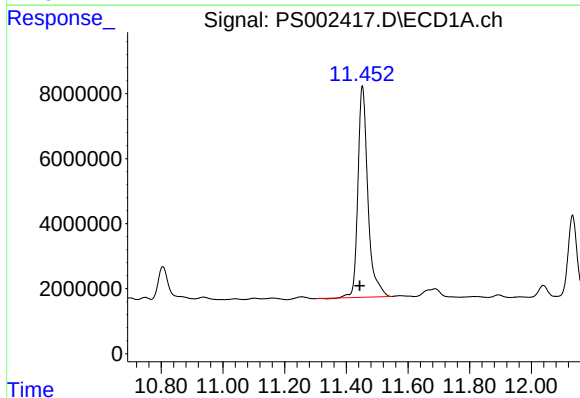


#4 2,4-DCAA

R.T.: 11.452 min
Delta R.T.: 0.008 min
Response: 145718393
Conc: 478.39 ng/ml

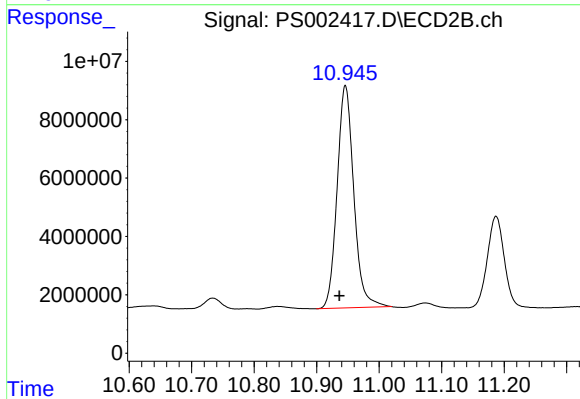

#4 2,4-DCAA


R.T.: 10.946 min
Delta R.T.: 0.010 min
Response: 141207431
Conc: 385.91 ng/ml

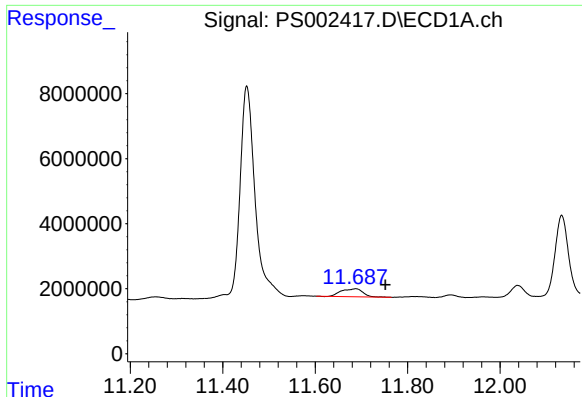

#5 DICAMBA


R.T.: 11.688 min
Delta R.T.: -0.065 min
Response: 8002050
Conc: 5.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

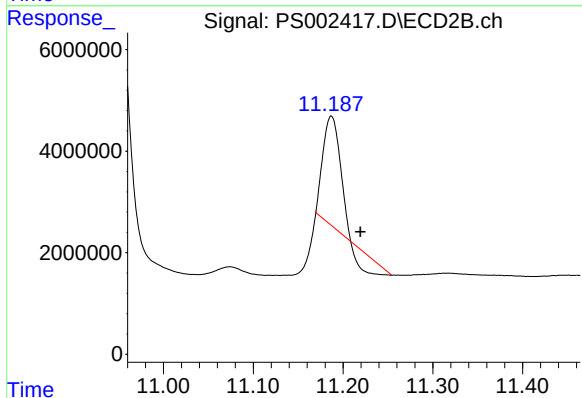


#5 DICAMBA

R.T.: 11.187 min
Delta R.T.: -0.032 min
Response: 23022514
Conc: 17.02 ng/ml

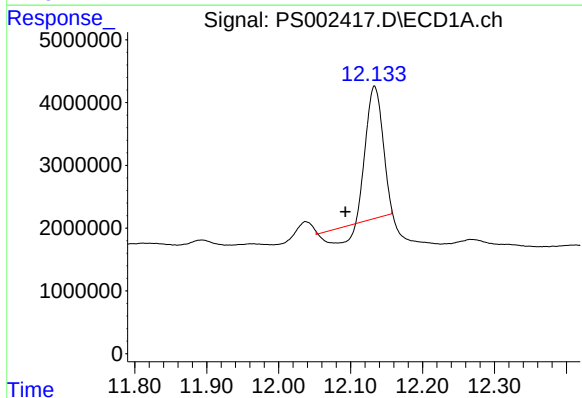


#6 MCP

R.T.: 12.133 min
Delta R.T.: 0.041 min
Response: 30339107
Conc: 32.33 ug/ml

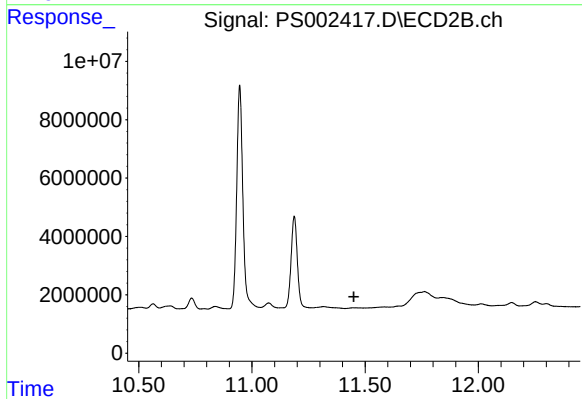

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.450 min
Response: 0
Conc: N.D.

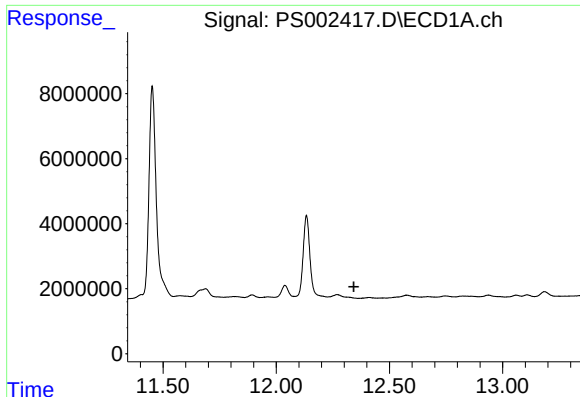

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

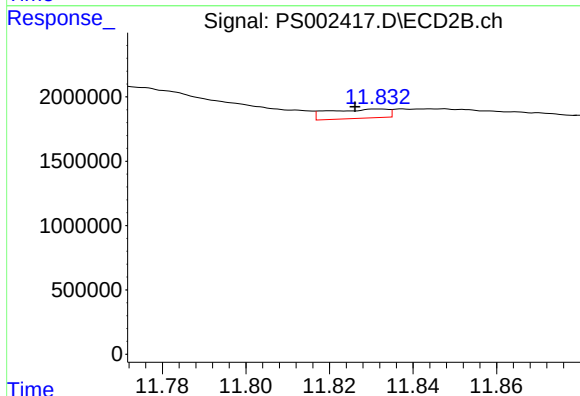


#7 MCPA

R.T.: 11.832 min
Delta R.T.: 0.006 min
Response: 699806
Conc: 0.50 ug/ml

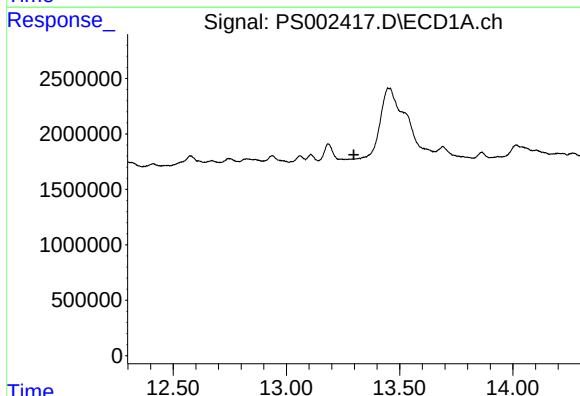


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.298 min
Response: 0
Conc: N.D.

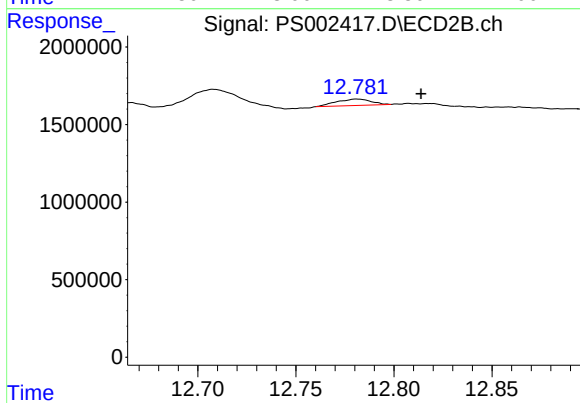

#9 2,4-D


R.T.: 12.781 min
Delta R.T.: -0.033 min
Response: 509819
Conc: 1.28 ng/ml

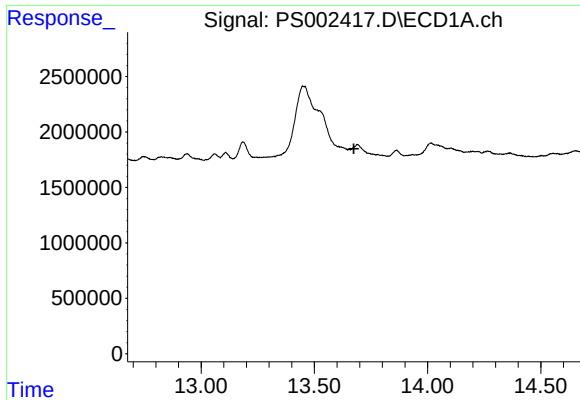

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

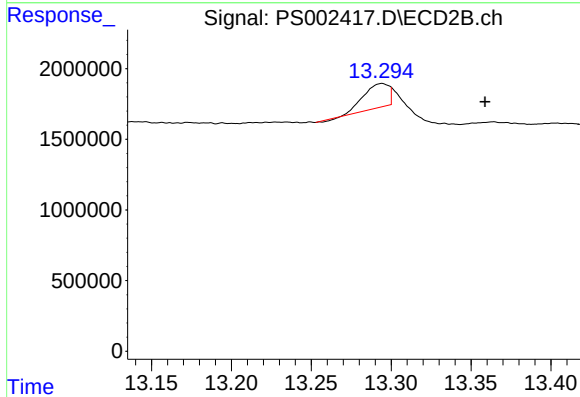


#10 Pentachlorophenol

R.T.: 13.294 min
Delta R.T.: -0.064 min
Response: 1873297
Conc: 0.37 ng/ml

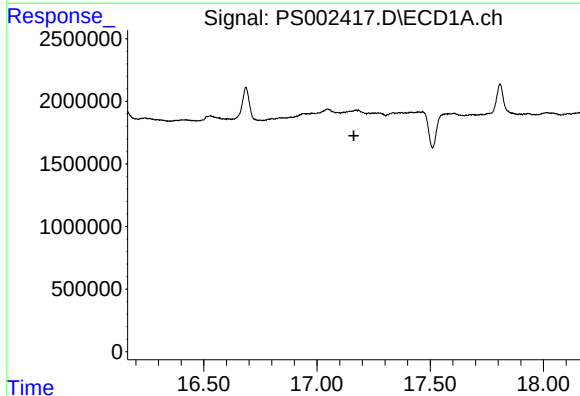


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.163 min
Response: 0
Conc: N.D.

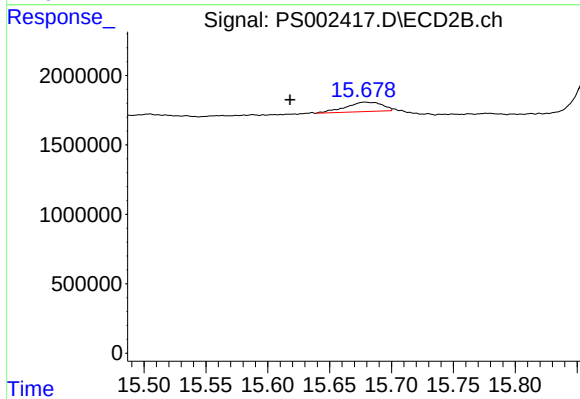

#14 DINOSEB


R.T.: 15.678 min
Delta R.T.: 0.060 min
Response: 1402070
Conc: 0.94 ng/ml

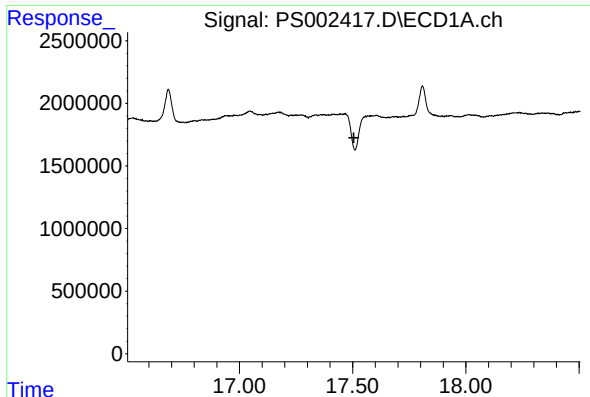

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

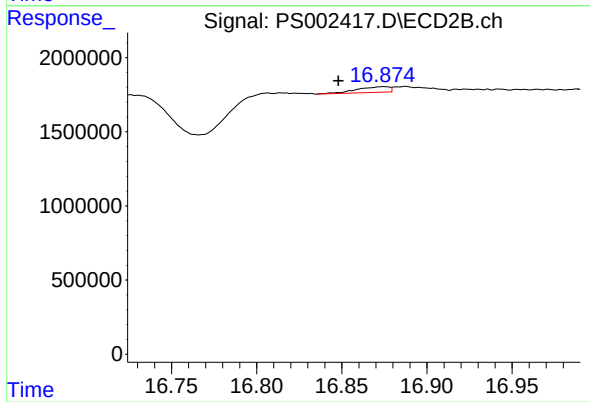

#16 DCPA

R.T.: 16.874 min
Delta R.T.: 0.026 min
Response: 510484
Conc: 0.21 ng/ml