

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111219\
 Data File : PS007661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2019 12:24
 Operator : SM\AJ
 Sample : K5760-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 3425

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 12:55:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.443	5.168	306.2E6	149.4E6	222.306	212.650
Target Compounds							
1) T	Dalapon	2.007	1.713	103.6E6	420.0E6	57.246	353.728 #
2) T	3,5-DICHL...	0.000	4.448	0	7282643	N.D.	8.061
7) T	MCPA	5.844	5.536	31701572	25280947	5.759	8.411 #
8) T	DICHLORPROP	0.000	5.754	0	10487161	N.D.	15.991
9) T	2,4-D	0.000	6.007	0	16123524	N.D.	19.994
10) T	Pentachlo...	0.000	6.454	0	11667887	N.D.	1.192
11) T	2,4,5-TP ...	0.000	6.765	0	19934778	N.D.	5.091
14) T	DINOSEB	0.000	8.000	0	28730021	N.D.	9.883
15) T	Picloram	0.000	8.919	0	45347270	N.D.	7.740



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111219\
Data File : PS007661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2019 12:24
Operator : SM\AJ
Sample : K5760-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
3425

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 12:55:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

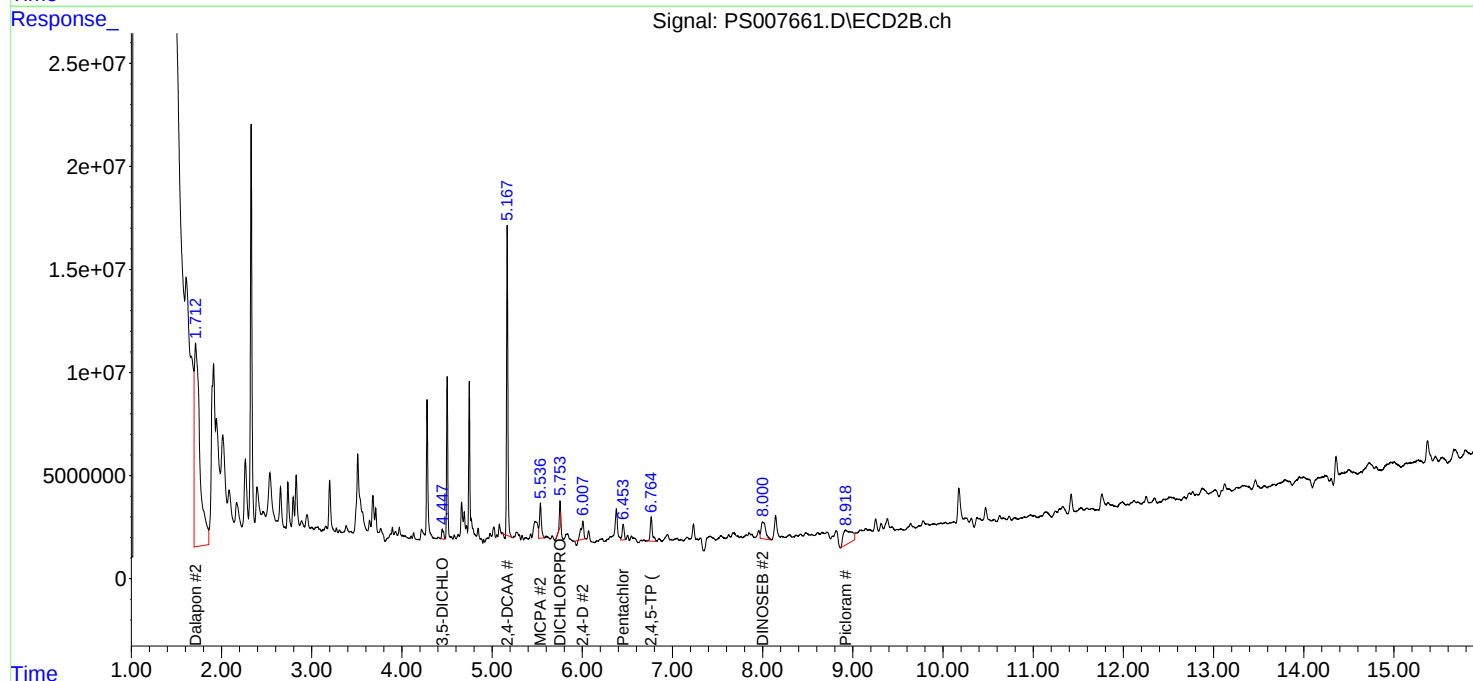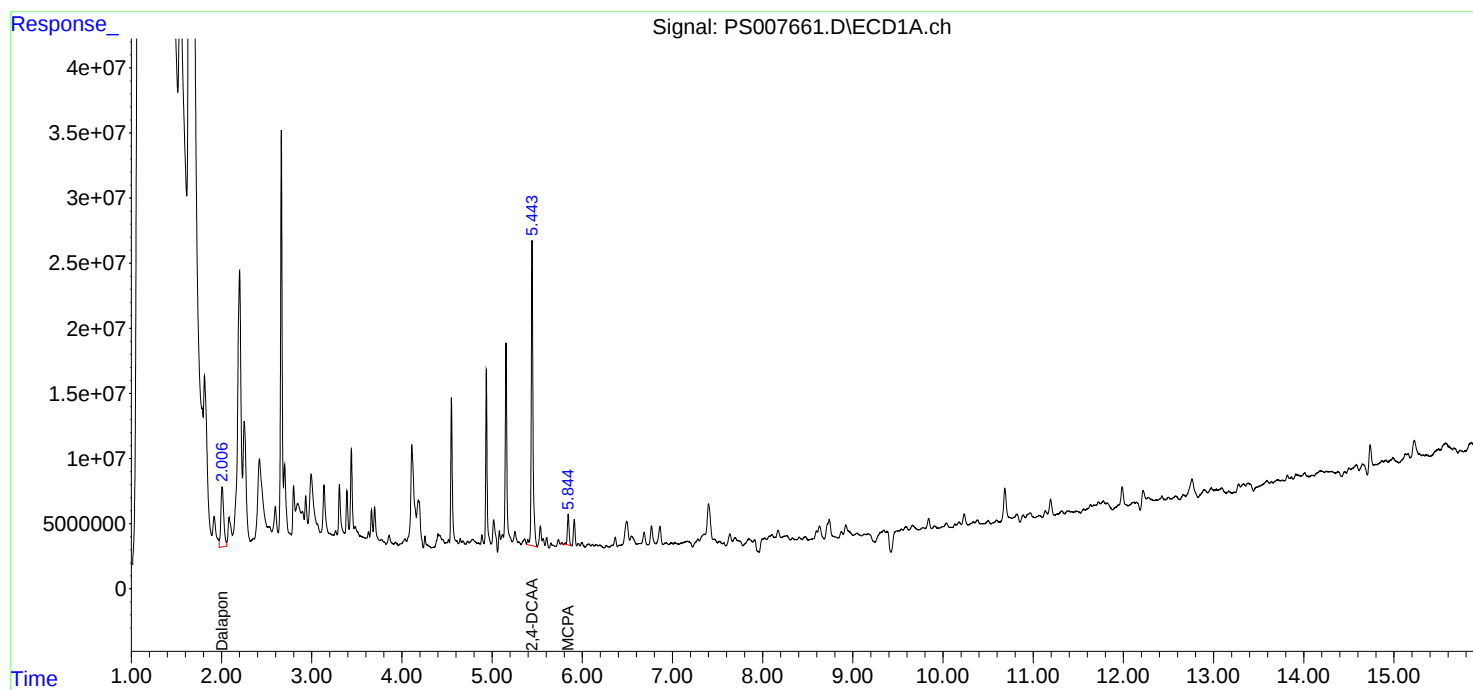


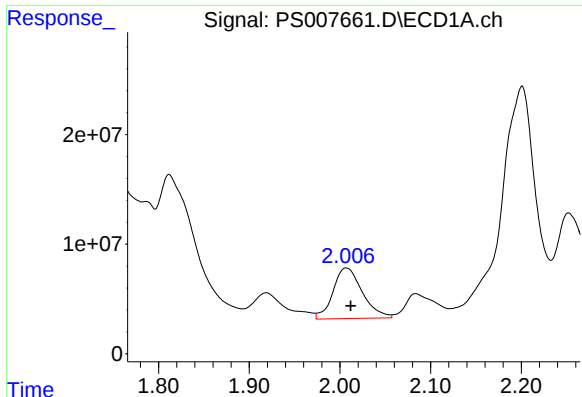

#1 Dalapon


R.T.: 2.007 min
Delta R.T.: -0.005 min
Response: 103568968
Conc: 57.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
3425

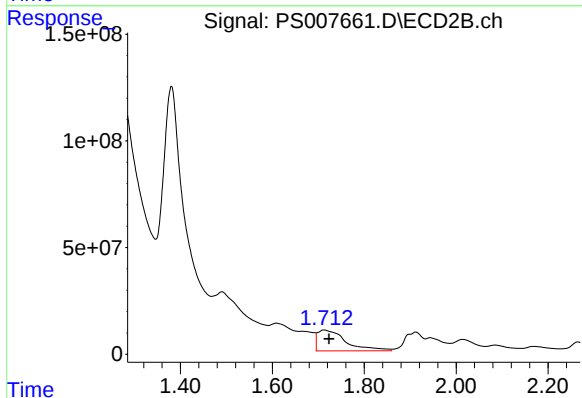


#1 Dalapon

R.T.: 1.713 min
Delta R.T.: -0.011 min
Response: 420017811
Conc: 353.73 ng/ml

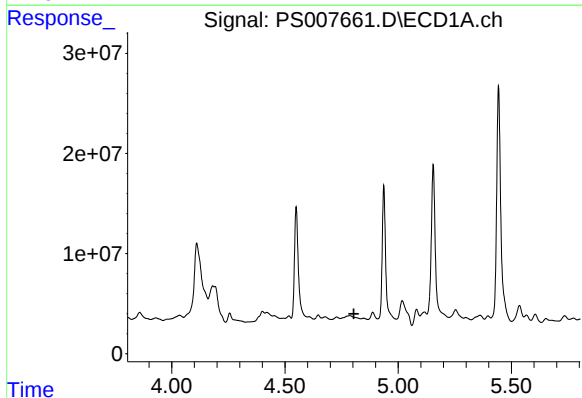


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

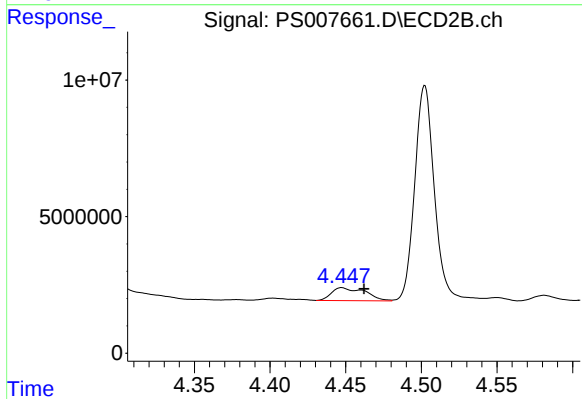

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.448 min
Delta R.T.: -0.014 min
Response: 7282643
Conc: 8.06 ng/ml

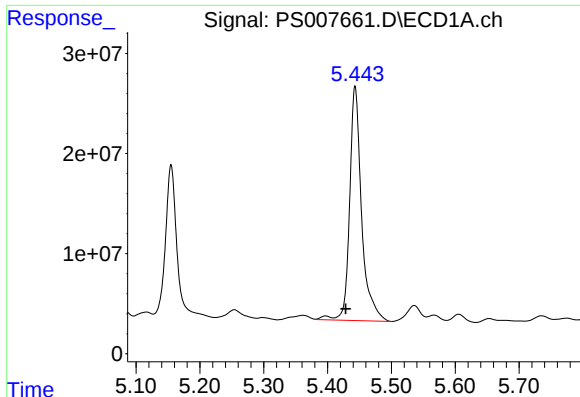

#4 2,4-DCAA


R.T.: 5.443 min
Delta R.T.: 0.015 min
Response: 306156048
Conc: 222.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
3425

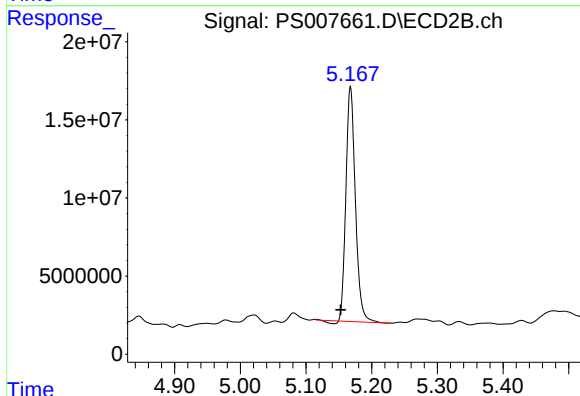


#4 2,4-DCAA

R.T.: 5.168 min
Delta R.T.: 0.015 min
Response: 149400168
Conc: 212.65 ng/ml

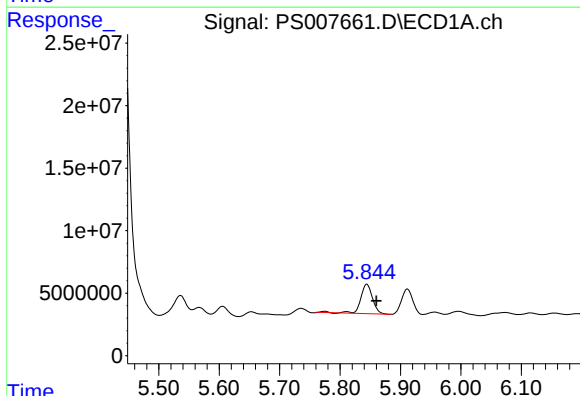


#7 MCPA

R.T.: 5.844 min
Delta R.T.: -0.016 min
Response: 31701572
Conc: 5.76 ug/ml

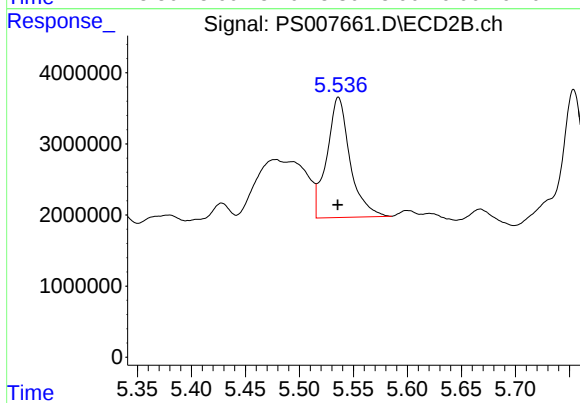

#7 MCPA


R.T.: 5.536 min
Delta R.T.: 0.000 min
Response: 25280947
Conc: 8.41 ug/ml

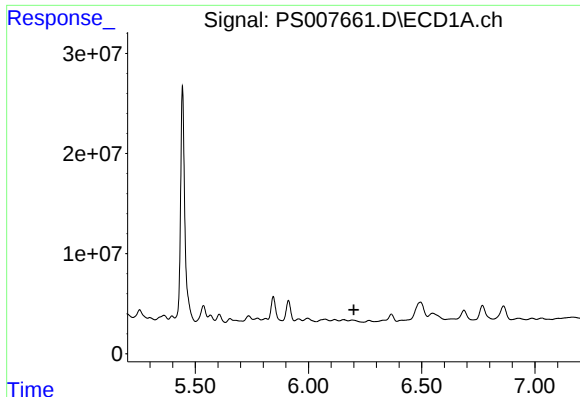

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
3425

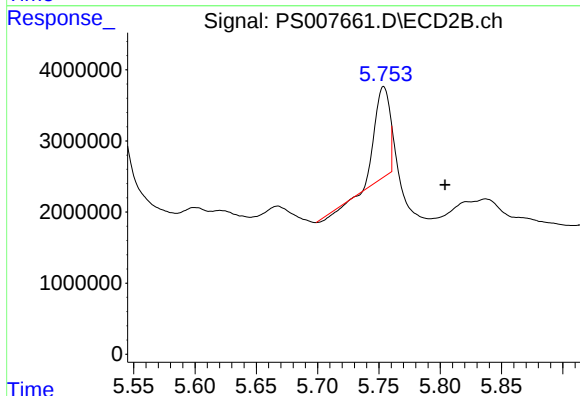


#8 DICHLORPROP

R.T.: 5.754 min
Delta R.T.: -0.050 min
Response: 10487161
Conc: 15.99 ng/ml

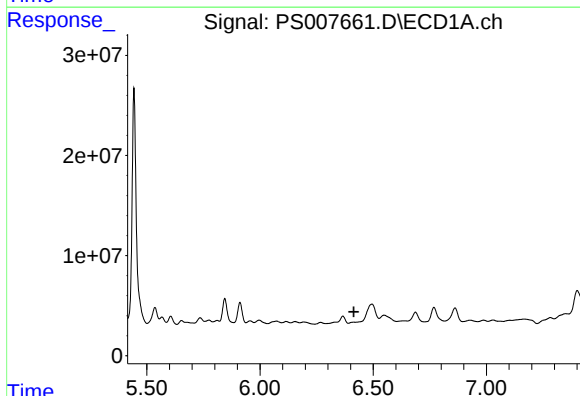


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.414 min
Response: 0
Conc: N.D.

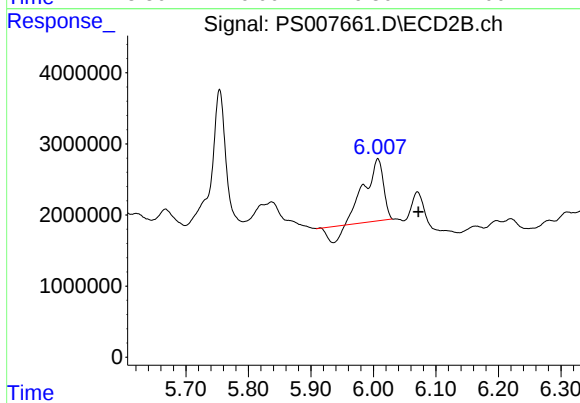

#9 2,4-D


R.T.: 6.007 min
Delta R.T.: -0.065 min
Response: 16123524
Conc: 19.99 ng/ml

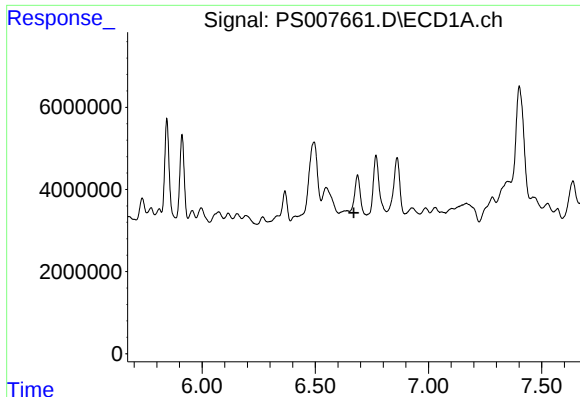

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
3425

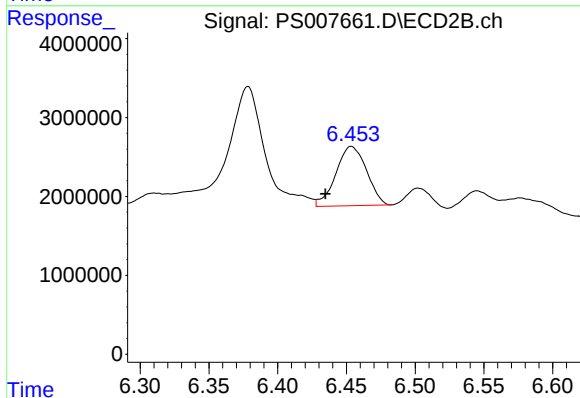


#10 Pentachlorophenol

R.T.: 6.454 min
Delta R.T.: 0.019 min
Response: 11667887
Conc: 1.19 ng/ml

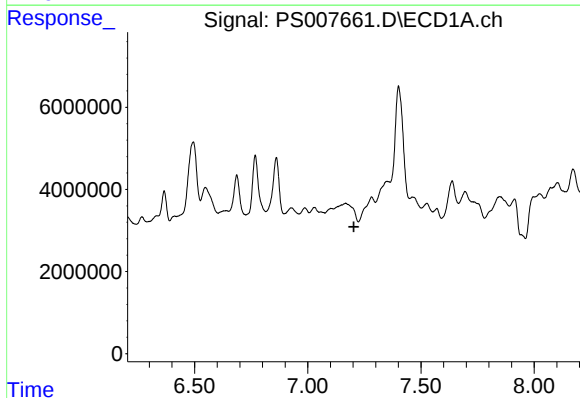


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

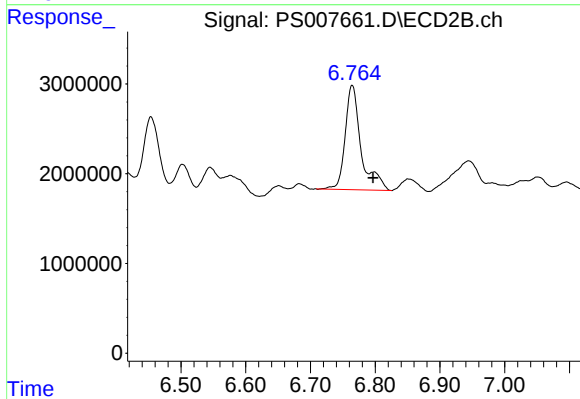

#11 2,4,5-TP (SILVEX)


R.T.: 6.765 min
Delta R.T.: -0.032 min
Response: 19934778
Conc: 5.09 ng/ml

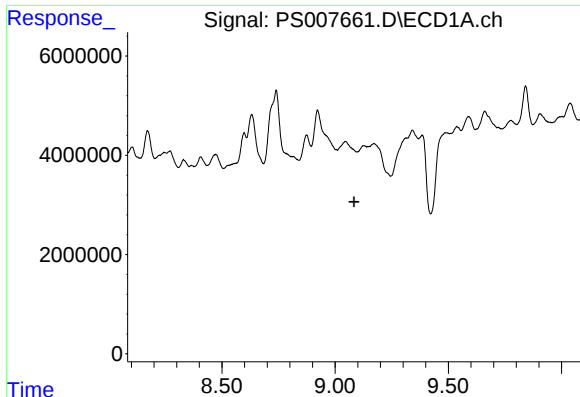

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
3425

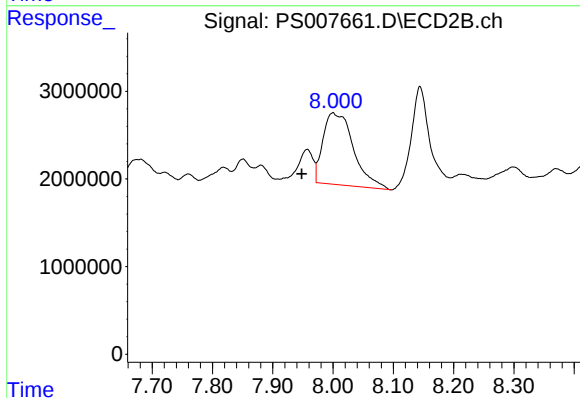


#14 DINOSEB

R.T.: 8.000 min
Delta R.T.: 0.051 min
Response: 28730021
Conc: 9.88 ng/ml

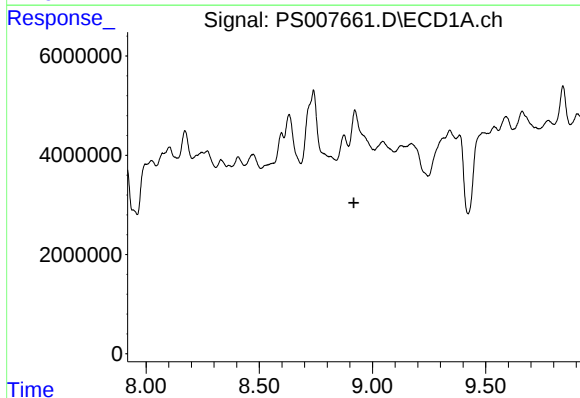

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

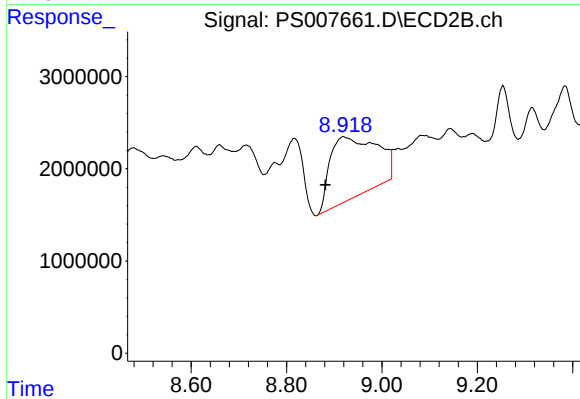

#15 Picloram

R.T.: 8.919 min
Delta R.T.: 0.037 min
Response: 45347270
Conc: 7.74 ng/ml