

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111219\
 Data File : PS007669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2019 16:26
 Operator : SM\AJ
 Sample : PB124723TB
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB124723TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 17:24:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.430	5.154	618.3E6	320.8E6	448.956	456.616
Target Compounds							
1) T	Dalapon	1.993	1.699	117.4E6	127.8E6	64.919	107.605 #
2) T	3,5-DICHL...	0.000	4.489	0	81730713	N.D.	90.467
5) T	DICAMBA	5.521	0.000	34163683	0	6.715	N.D. #
7) T	MCPA	5.897	5.522	26292065	34354969	4.777	11.430 #
9) T	2,4-D	6.480	6.056	108.0E6	5843074	76.996	7.246 #
10) T	Pentachlo...	0.000	6.442	0	10068367	N.D.	1.028
11) T	2,4,5-TP ...	0.000	6.751	0	53689722	N.D.	13.711
14) T	DINOSEB	0.000	7.945	0	10872187	N.D.	3.740
15) T	Picloram	0.000	8.914	0	19772806	N.D.	3.375



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111219\
Data File : PS007669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2019 16:26
Operator : SM\AJ
Sample : PB124723TB
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB124723TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 17:24:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

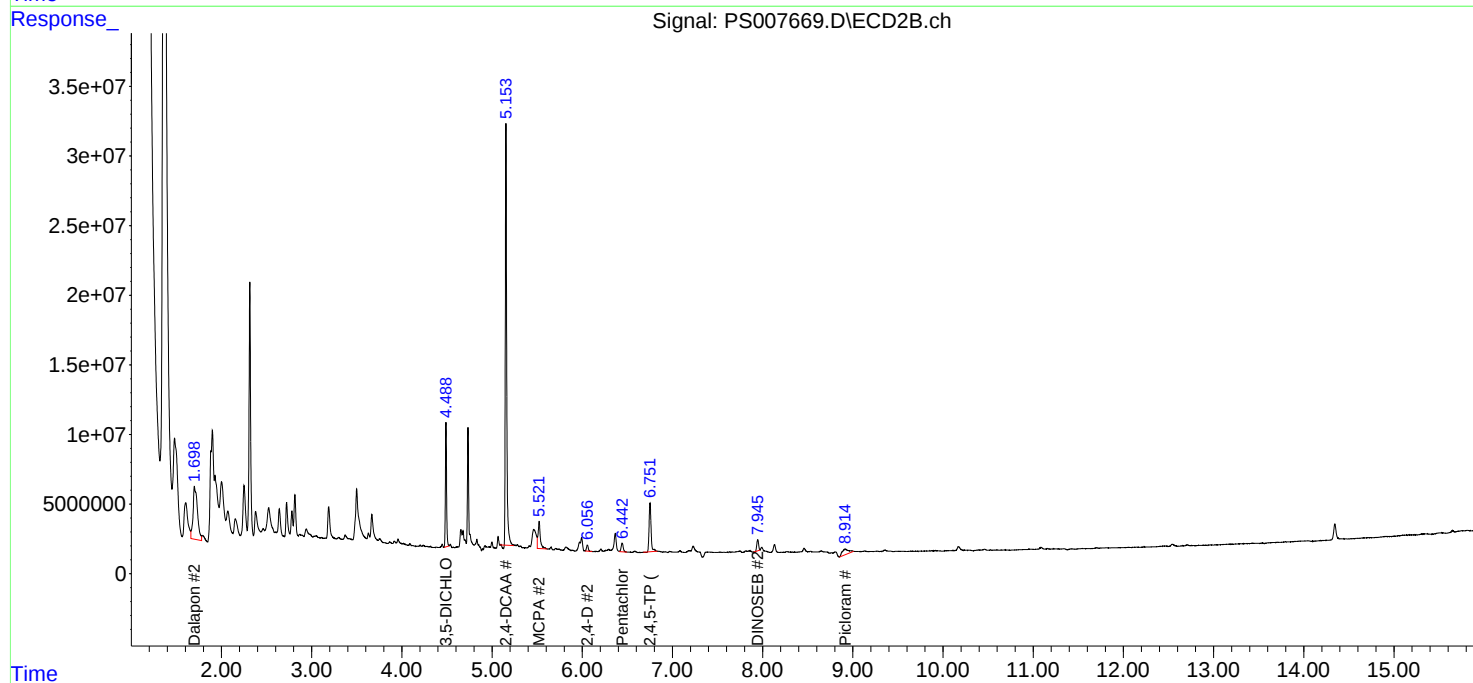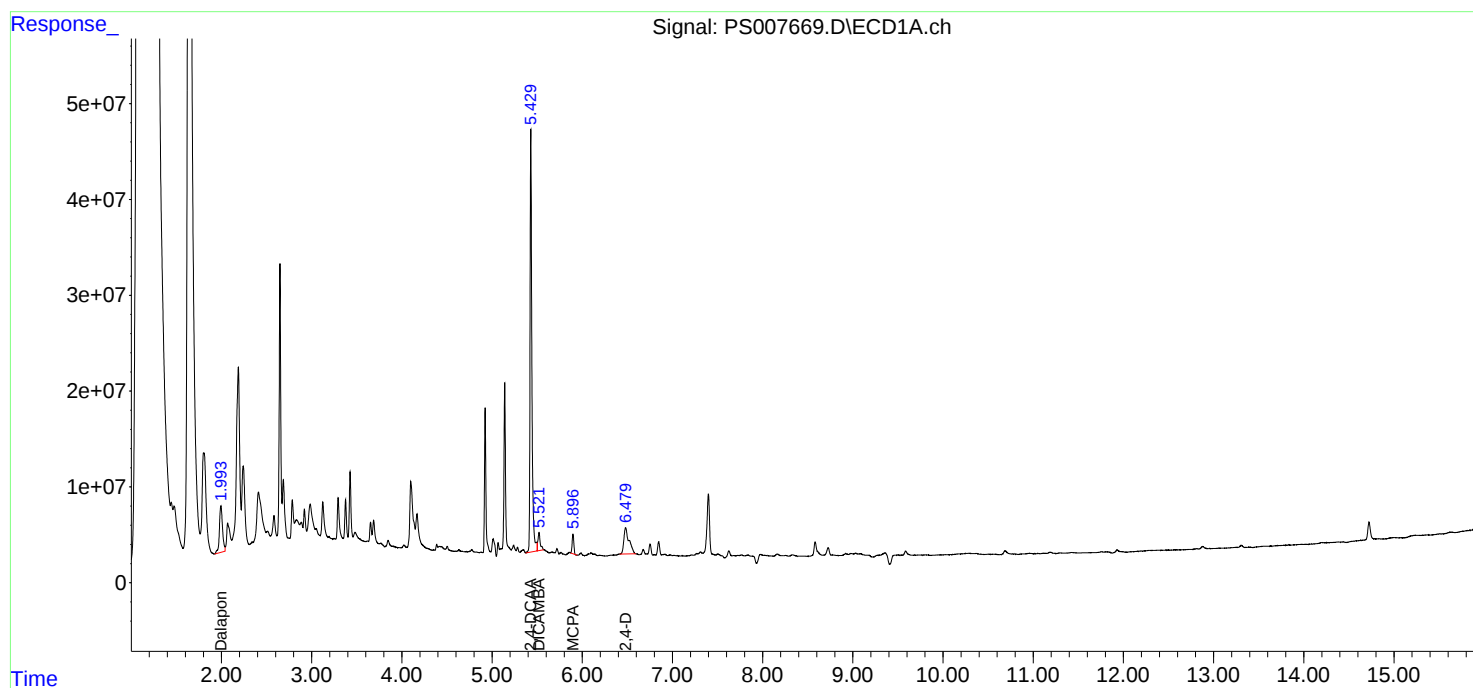


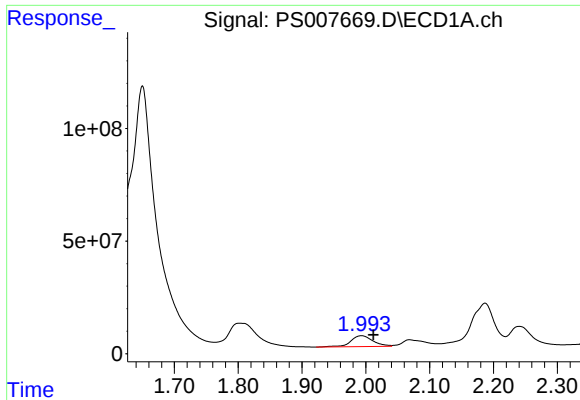

#1 Dalapon


R.T.: 1.993 min
Delta R.T.: -0.019 min
Response: 117449470
Conc: 64.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124723TB

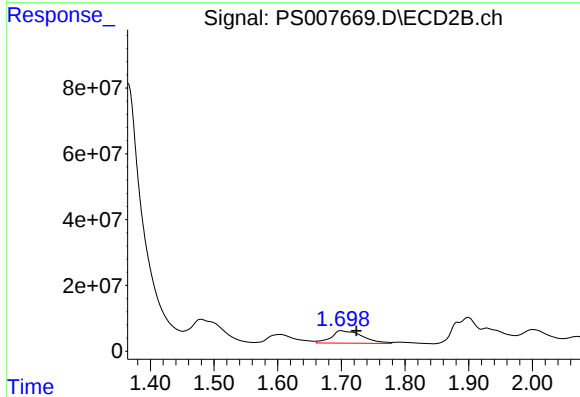


#1 Dalapon

R.T.: 1.699 min
Delta R.T.: -0.024 min
Response: 127770142
Conc: 107.60 ng/ml

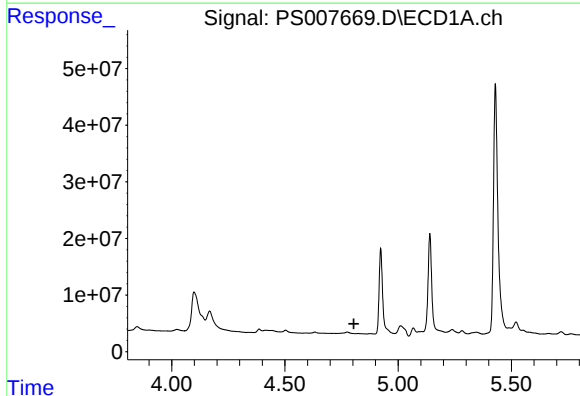


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

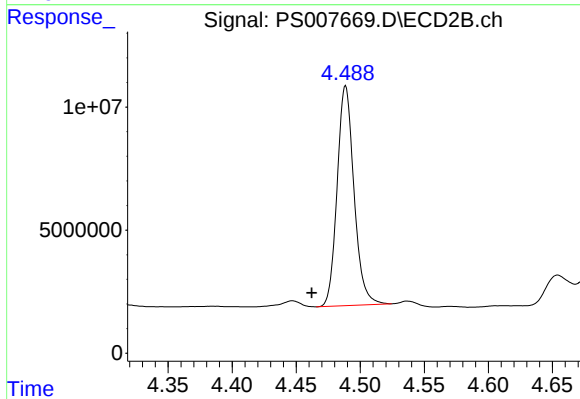

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.489 min
Delta R.T.: 0.026 min
Response: 81730713
Conc: 90.47 ng/ml

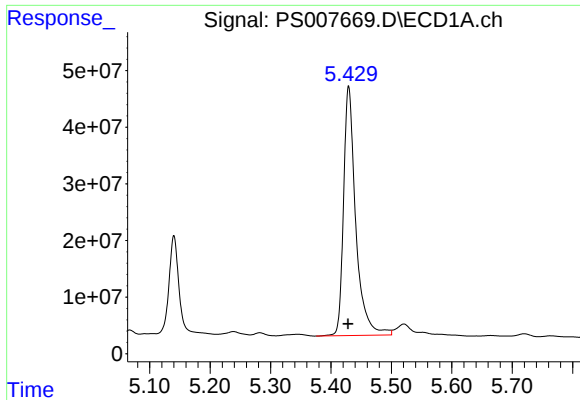

#4 2,4-DCAA


R.T.: 5.430 min
Delta R.T.: 0.001 min
Response: 618295407
Conc: 448.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124723TB

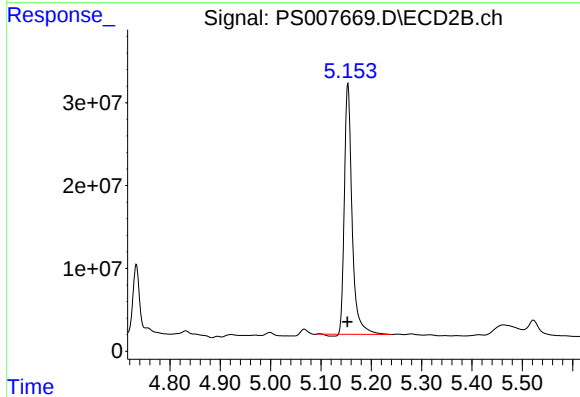


#4 2,4-DCAA

R.T.: 5.154 min
Delta R.T.: 0.000 min
Response: 320802079
Conc: 456.62 ng/ml

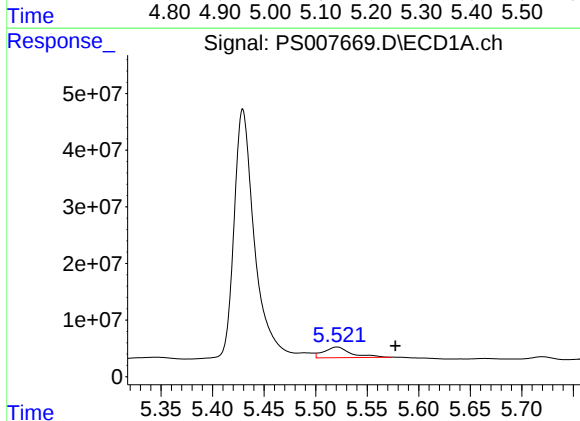


#5 DICAMBA

R.T.: 5.521 min
Delta R.T.: -0.057 min
Response: 34163683
Conc: 6.72 ng/ml

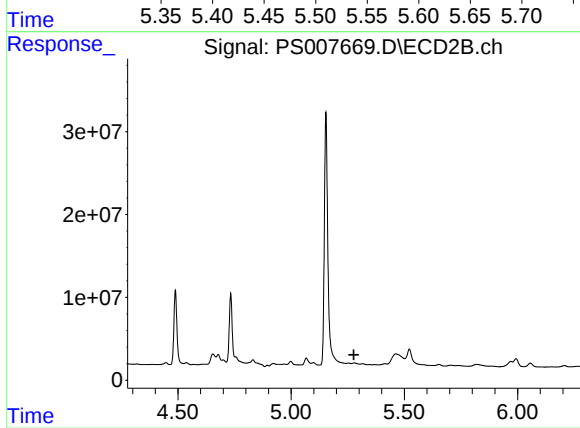

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

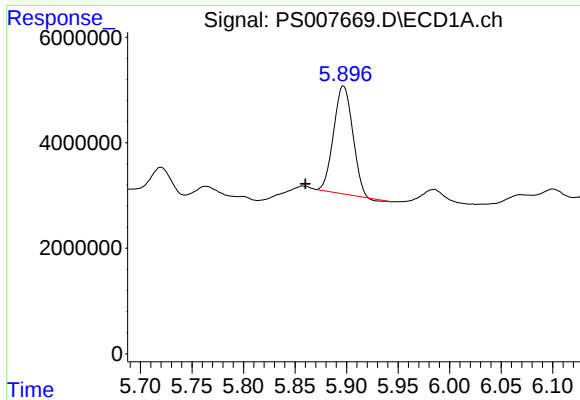

#7 MCPA


R.T.: 5.897 min
Delta R.T.: 0.037 min
Response: 26292065
Conc: 4.78 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB124723TB

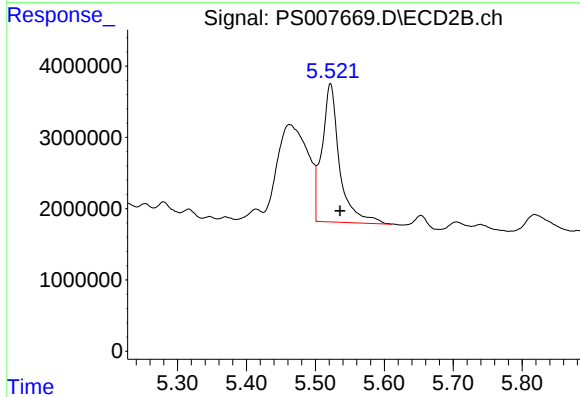


#7 MCPA

R.T.: 5.522 min
Delta R.T.: -0.014 min
Response: 34354969
Conc: 11.43 ug/ml

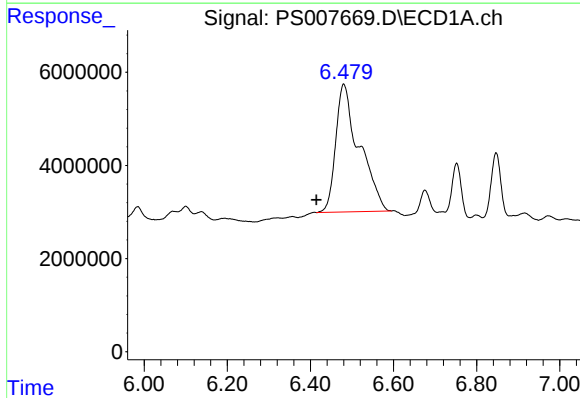


#9 2,4-D

R.T.: 6.480 min
Delta R.T.: 0.066 min
Response: 107990760
Conc: 77.00 ng/ml

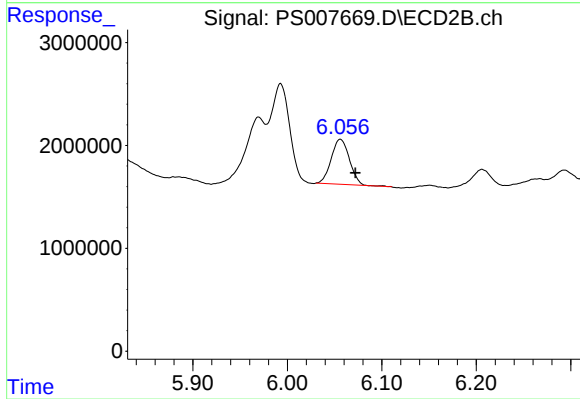

#9 2,4-D


R.T.: 6.056 min
Delta R.T.: -0.016 min
Response: 5843074
Conc: 7.25 ng/ml

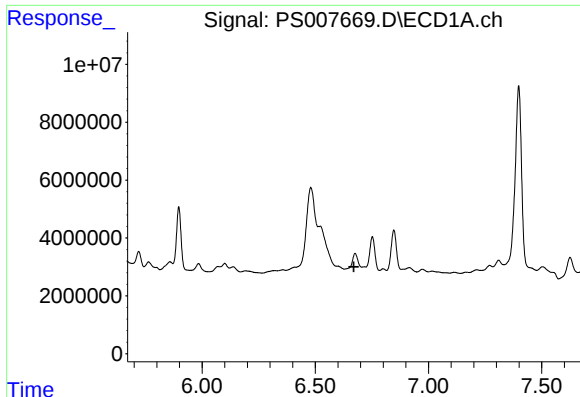

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124723TB

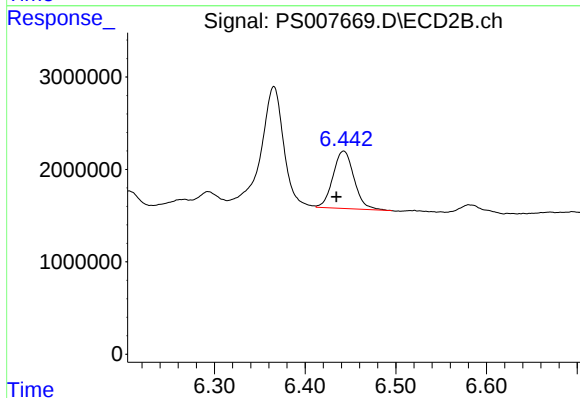


#10 Pentachlorophenol

R.T.: 6.442 min
Delta R.T.: 0.008 min
Response: 10068367
Conc: 1.03 ng/ml

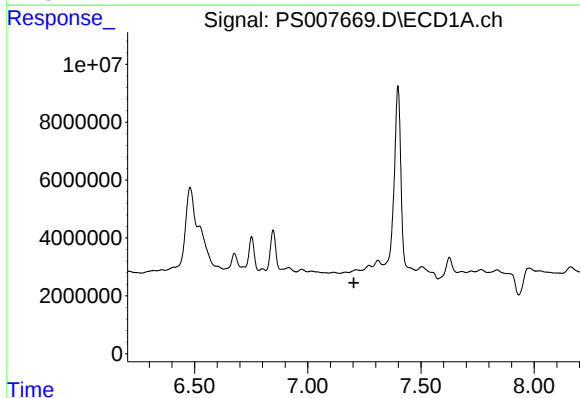


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

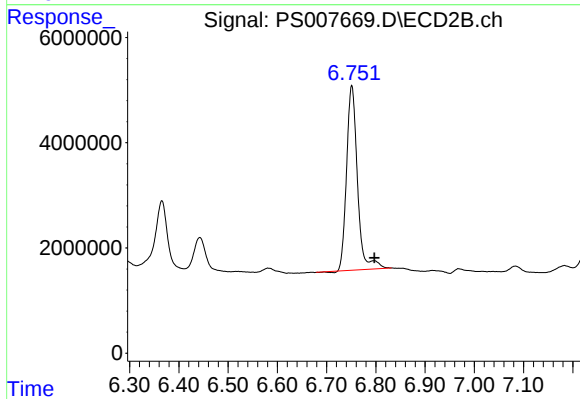

#11 2,4,5-TP (SILVEX)


R.T.: 6.751 min
Delta R.T.: -0.046 min
Response: 53689722
Conc: 13.71 ng/ml

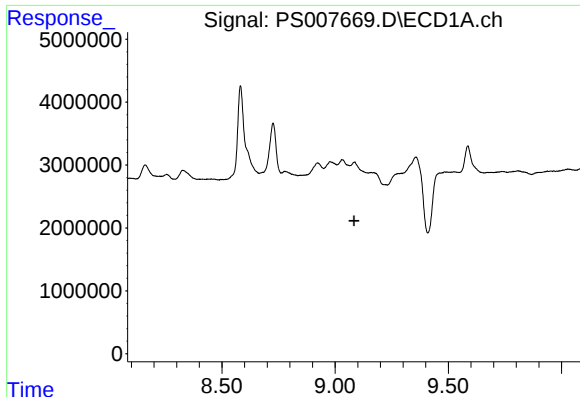

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124723TB

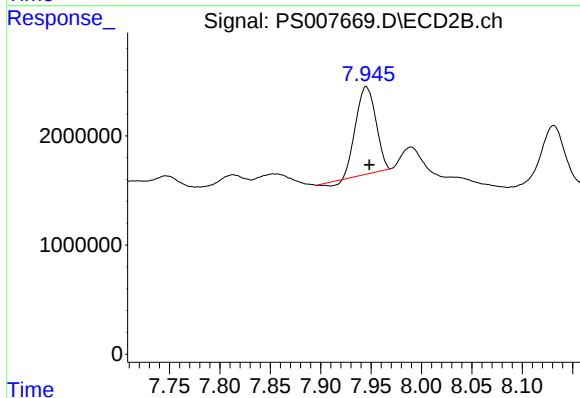


#14 DINOSEB

R.T.: 7.945 min
Delta R.T.: -0.003 min
Response: 10872187
Conc: 3.74 ng/ml

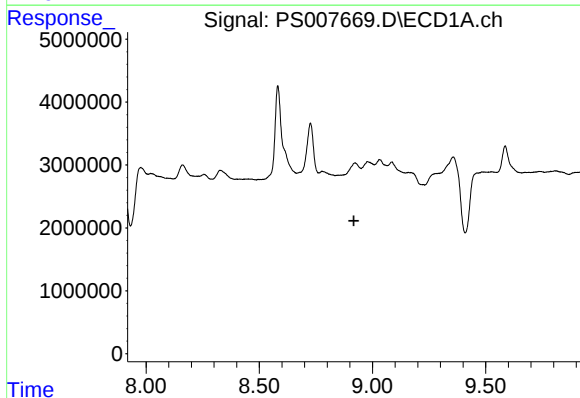

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

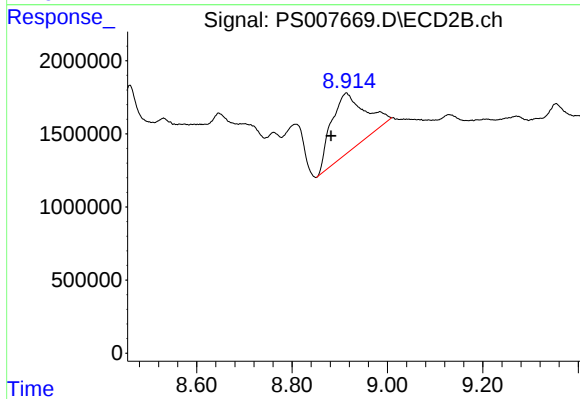

#15 Picloram

R.T.: 8.914 min
Delta R.T.: 0.032 min
Response: 19772806
Conc: 3.37 ng/ml