

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111219\
 Data File : PS007679.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2019 20:06
 Operator : SM\AJ
 Sample : K5760-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RBR-30

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 01:10:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.431	5.155	387.7E6	205.0E6	281.550	291.799
Target Compounds							
1) T	Dalapon	1.992	1.700	80262602	108.3E6	44.364	91.234 #
2) T	3,5-DICHL...	0.000	4.447	0	6734789	N.D.	7.455
3) T	4-Nitroph...	0.000	4.832	0	17885472	N.D.	43.465
5) T	DICAMBA	0.000	5.209	0	7957423	N.D.	3.007
9) T	2,4-D	6.482	0.000	107.5E6	0	76.651	N.D. #
10) T	Pentachlo...	0.000	6.440	0	14873068	N.D.	1.519
11) T	2,4,5-TP ...	0.000	6.801	0	4892444	N.D.	1.249
12) T	2,4,5-T	0.000	7.211	0	25681926	N.D.	6.954
15) T	Picloram	8.952	8.900	192.1E6	104.8E6	17.302	17.892
16) T	DCPA	0.000	8.900	0	104.8E6	N.D.	20.062



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111219\
Data File : PS007679.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2019 20:06
Operator : SM\AJ
Sample : K5760-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RBR-30

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 01:10:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

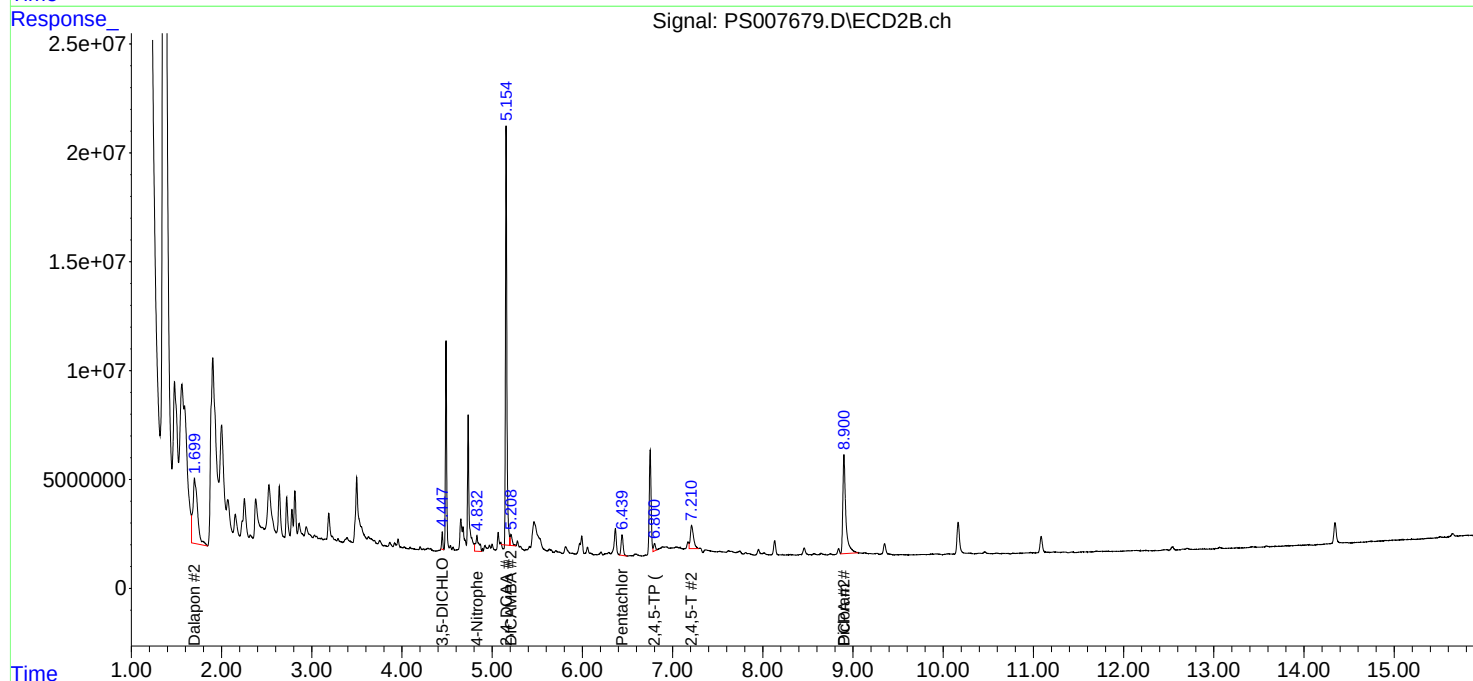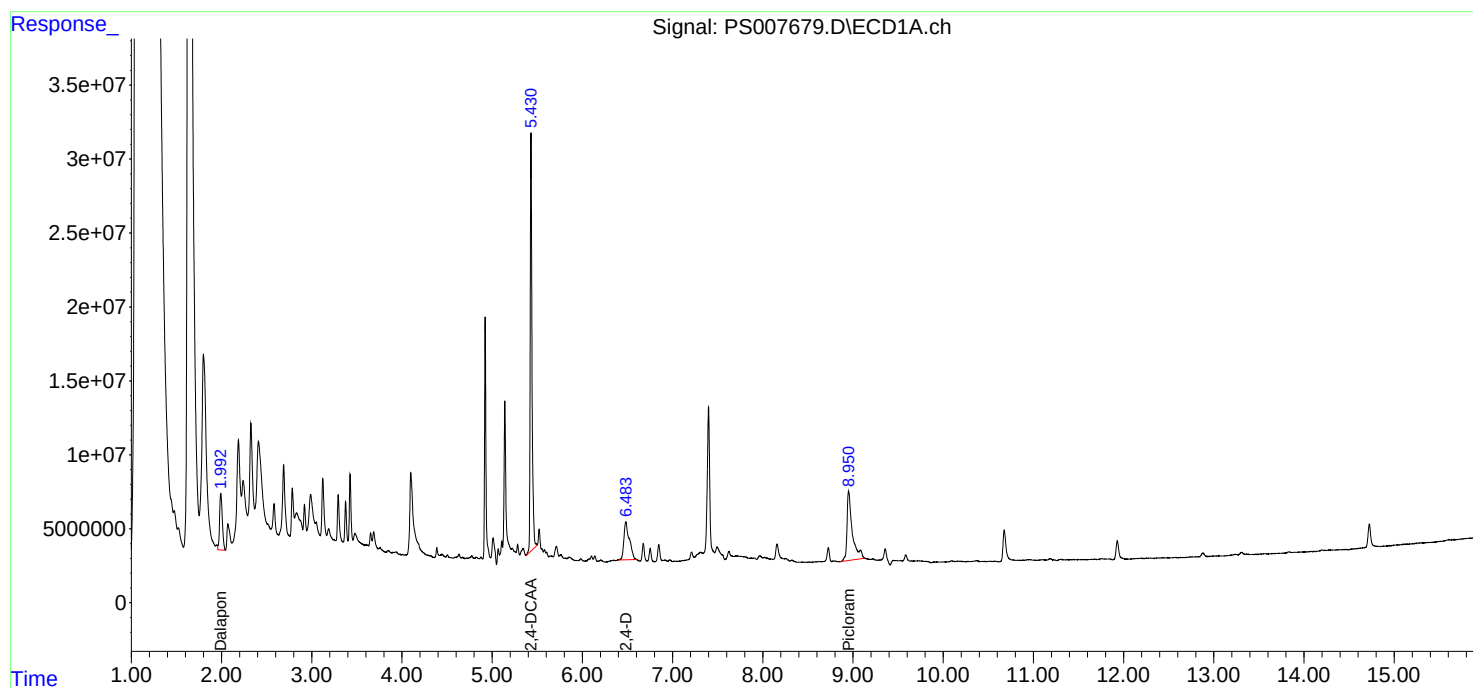


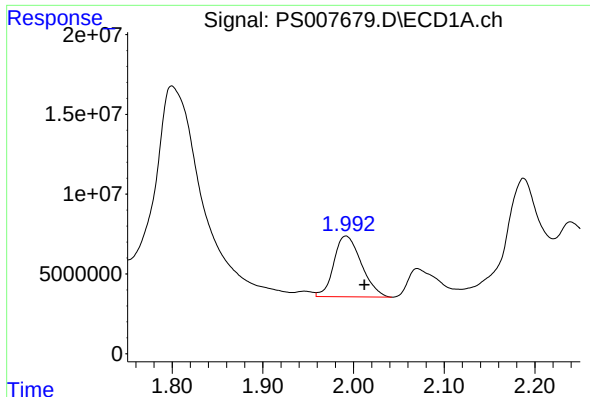

#1 Dalapon


R.T.: 1.992 min
Delta R.T.: -0.020 min
Response: 80262602
Conc: 44.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
RBR-30

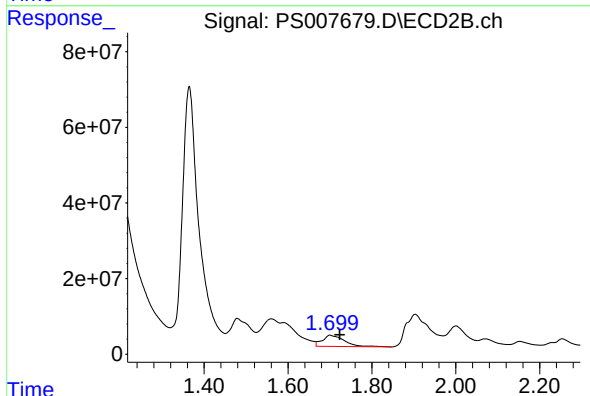


#1 Dalapon

R.T.: 1.700 min
Delta R.T.: -0.023 min
Response: 108330994
Conc: 91.23 ng/ml

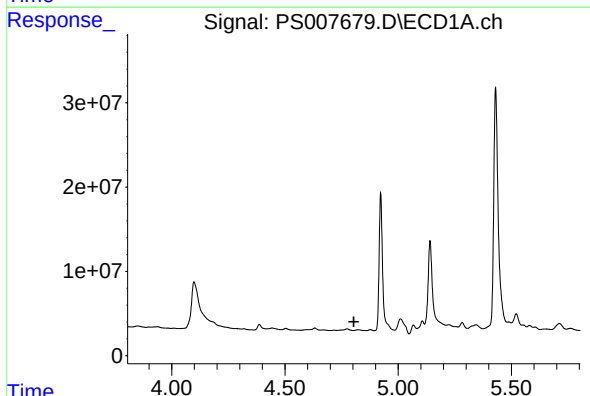


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

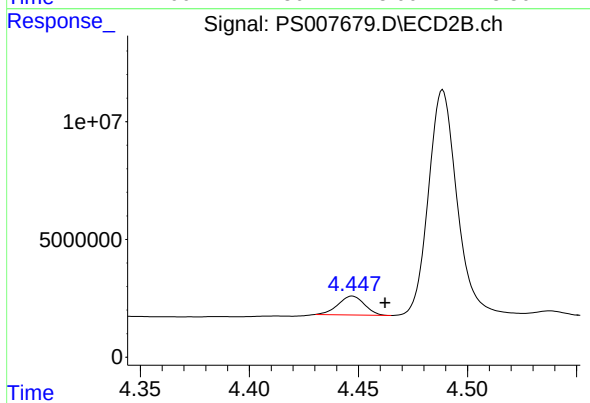

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.447 min
Delta R.T.: -0.015 min
Response: 6734789
Conc: 7.45 ng/ml

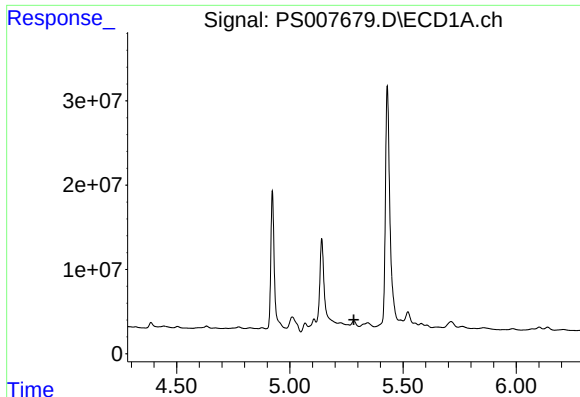

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR-30

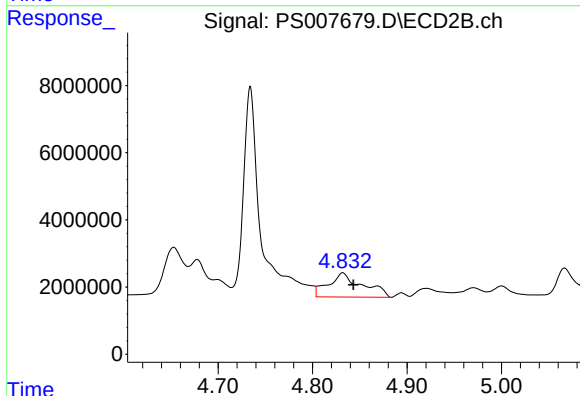


#3 4-Nitrophenol

R.T.: 4.832 min
Delta R.T.: -0.011 min
Response: 17885472
Conc: 43.46 ng/ml

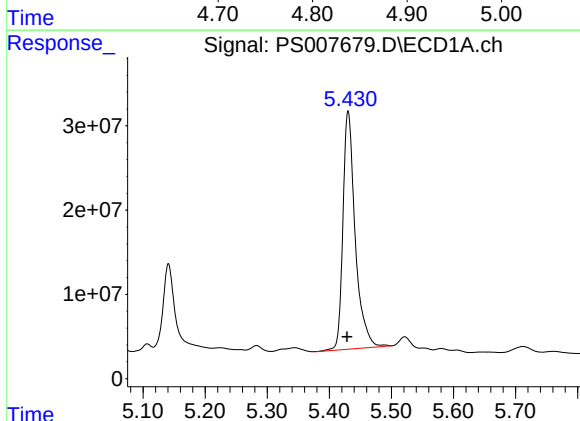


#4 2,4-DCAA

R.T.: 5.431 min
Delta R.T.: 0.002 min
Response: 387746640
Conc: 281.55 ng/ml

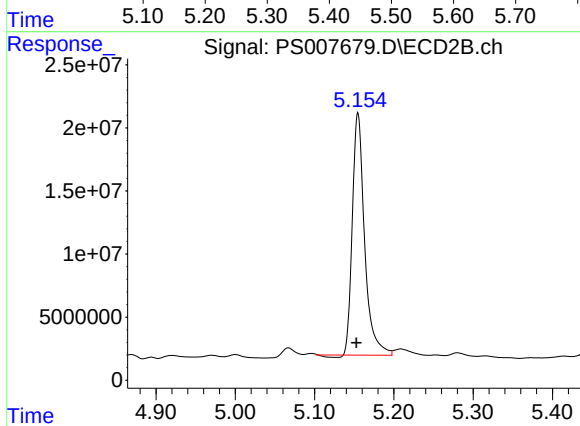

#4 2,4-DCAA


R.T.: 5.155 min
Delta R.T.: 0.002 min
Response: 205007420
Conc: 291.80 ng/ml

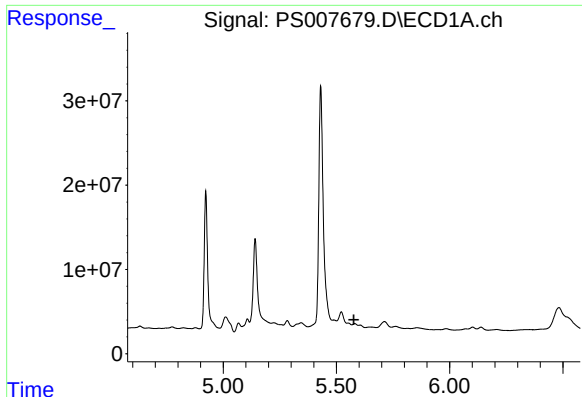

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR-30

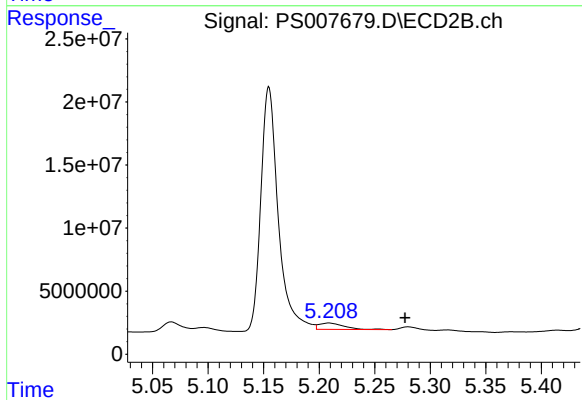


#5 DICAMBA

R.T.: 5.209 min
Delta R.T.: -0.068 min
Response: 7957423
Conc: 3.01 ng/ml

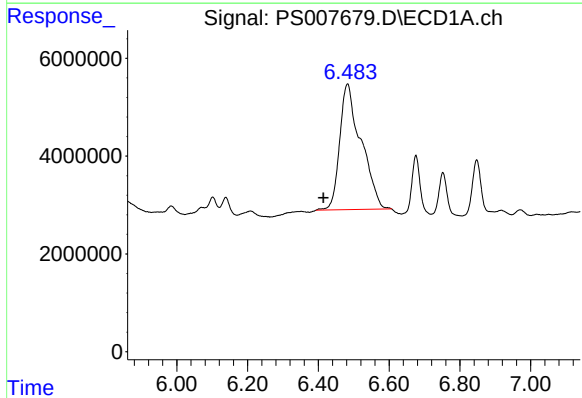


#9 2,4-D

R.T.: 6.482 min
Delta R.T.: 0.068 min
Response: 107506387
Conc: 76.65 ng/ml

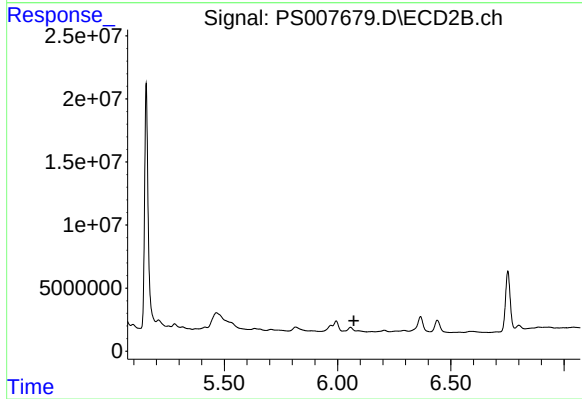

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

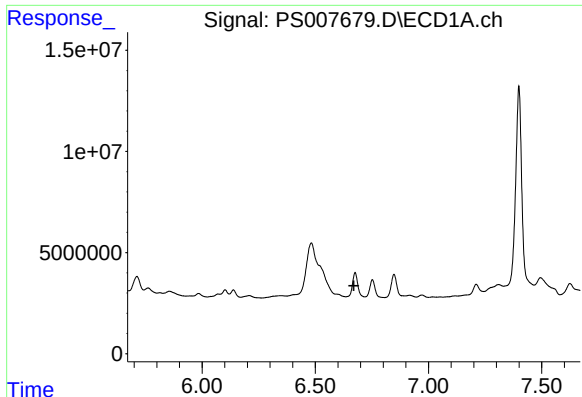

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR-30

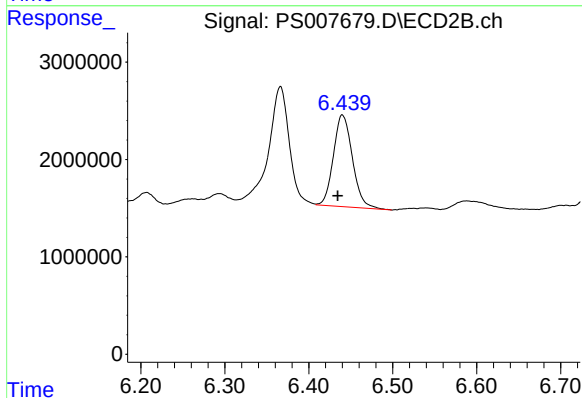


#10 Pentachlorophenol

R.T.: 6.440 min
Delta R.T.: 0.006 min
Response: 14873068
Conc: 1.52 ng/ml

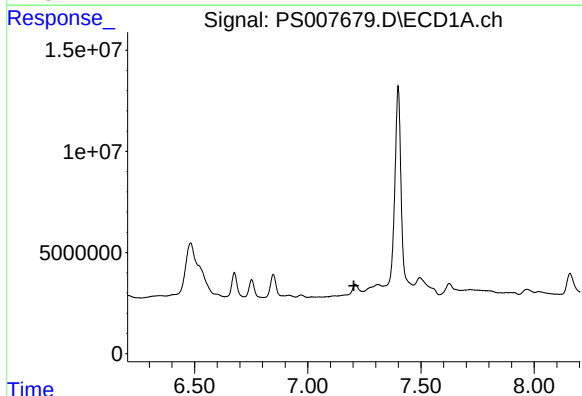


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

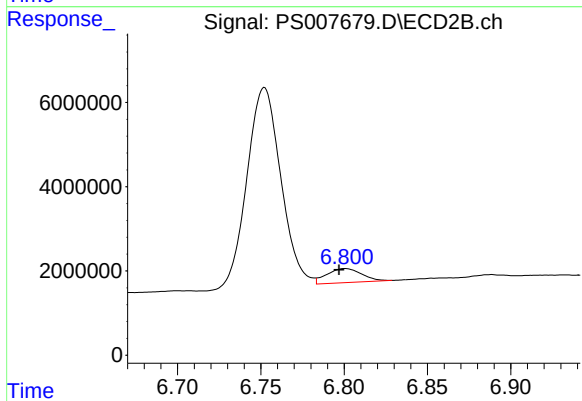

#11 2,4,5-TP (SILVEX)


R.T.: 6.801 min
Delta R.T.: 0.003 min
Response: 4892444
Conc: 1.25 ng/ml

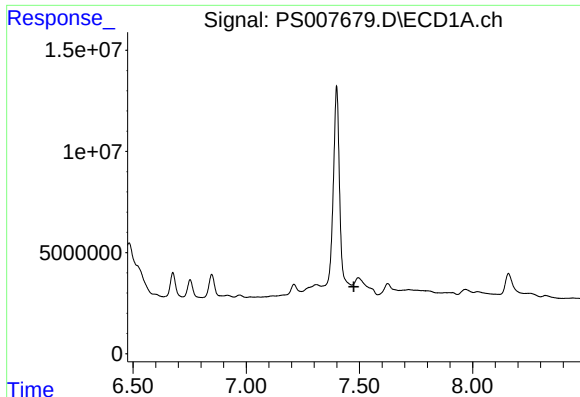

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR-30

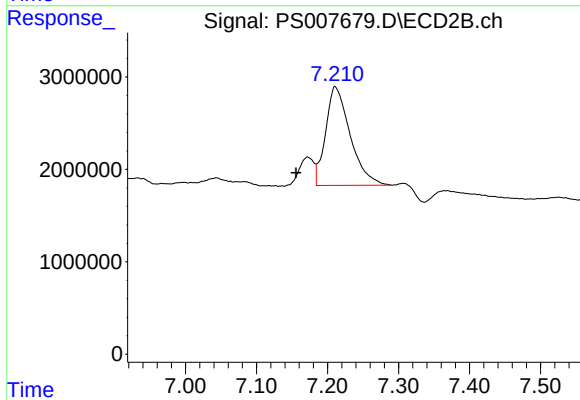


#12 2,4,5-T

R.T.: 7.211 min
Delta R.T.: 0.056 min
Response: 25681926
Conc: 6.95 ng/ml

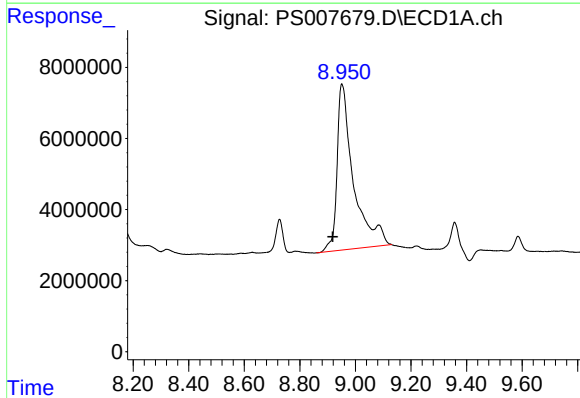


#15 Picloram

R.T.: 8.952 min
Delta R.T.: 0.034 min
Response: 192108165
Conc: 17.30 ng/ml

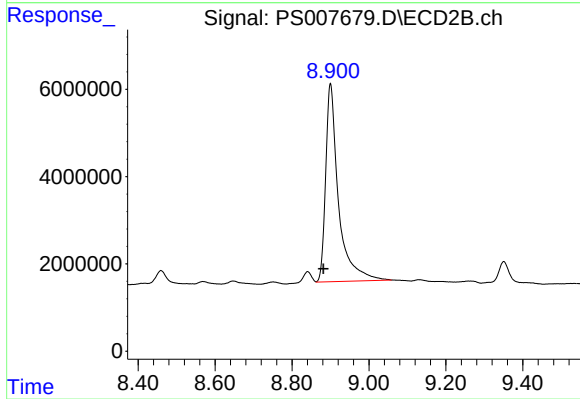

#15 Picloram


R.T.: 8.900 min
Delta R.T.: 0.018 min
Response: 104828090
Conc: 17.89 ng/ml

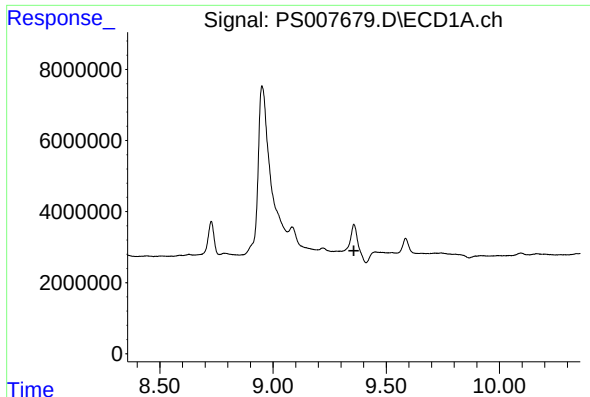

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR-30

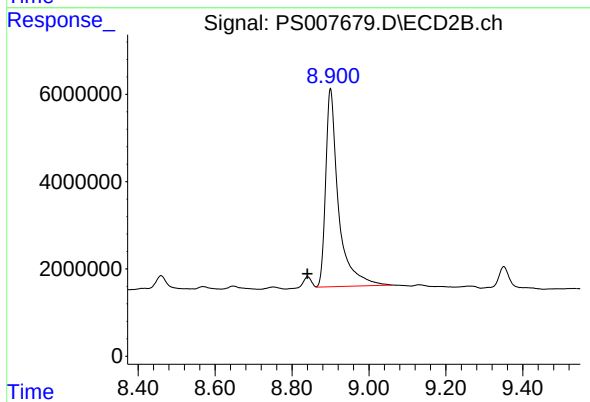

#16 DCPA

R.T.: 8.900 min
Delta R.T.: 0.060 min
Response: 104828090
Conc: 20.06 ng/ml