

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111224\
 Data File : PS028392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2024 12:36
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 23:46:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 08 17:46:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.676f	0.000	7331074	0	2.055	N.D.	#
2) T	3,5-DICHL...	6.418	0.000	446365	0	<MDL	N.D.	#
3) T	4-Nitroph...	7.032	0.000	4706373	0	2.538	N.D.	#
5) T	DICAMBA	7.435	0.000	278522	0	<MDL	N.D.	#
6) T	MCP	7.675f	0.000	20432388	0	2.498	N.D.	#
8) T	DICHLORPROP	8.197f	8.714f	6381013	7499852	2.059	4.210	#
10) T	Pentachlo...	8.680	0.000	1701450	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	0.000	9.903	0	1244376	N.D.	<MDL	#
12) T	2,4,5-T	9.555	10.319	4338210	8542309	<MDL	<MDL	#
14) T	DINOSEB	11.343	0.000	1756917	0	<MDL	N.D.	#
15) T	Picloram	11.152	12.368	83092812	31313056	2.646	2.176	#
16) T	DCPA	11.632	12.368f	2577229	31313056	<MDL	2.793	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111224\
Data File : PS028392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2024 12:36
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 23:46:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
Quant Title : 8080.M
QLast Update : Fri Nov 08 17:46:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

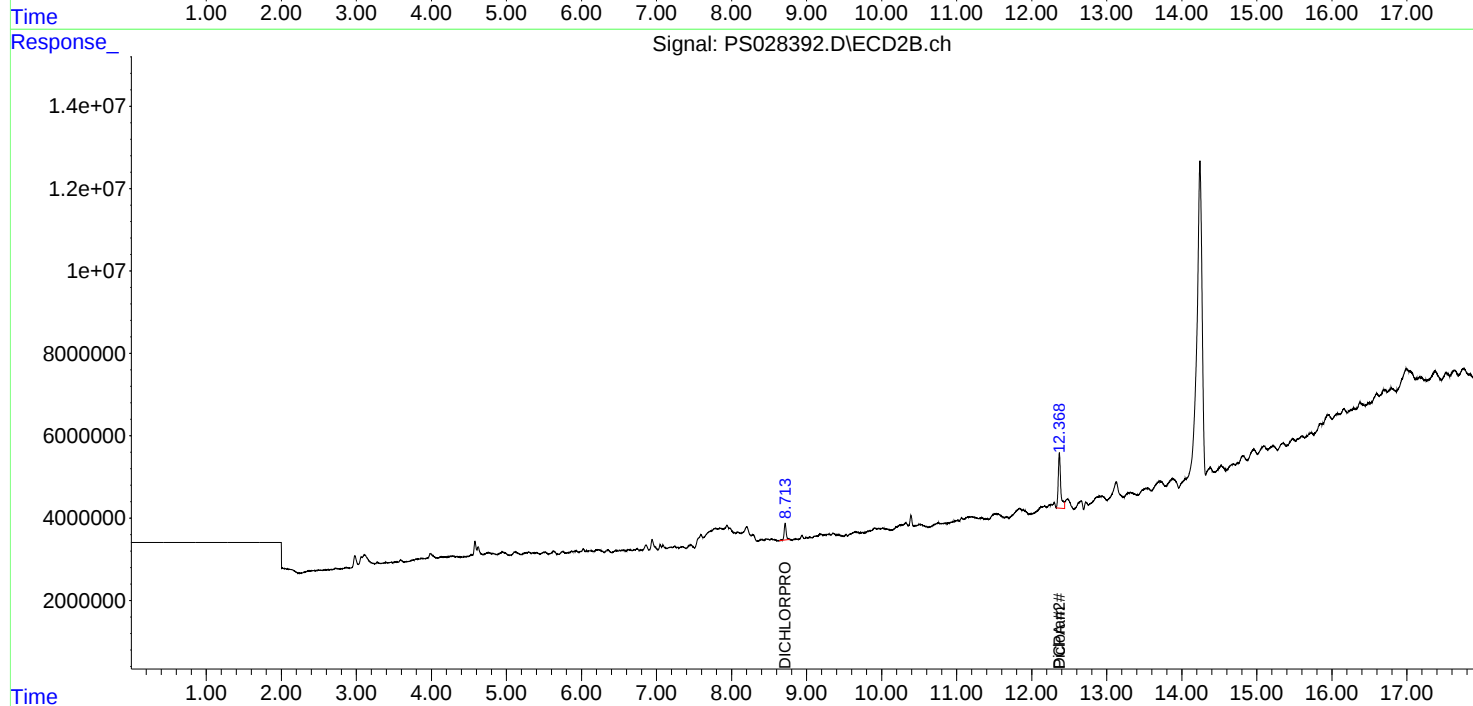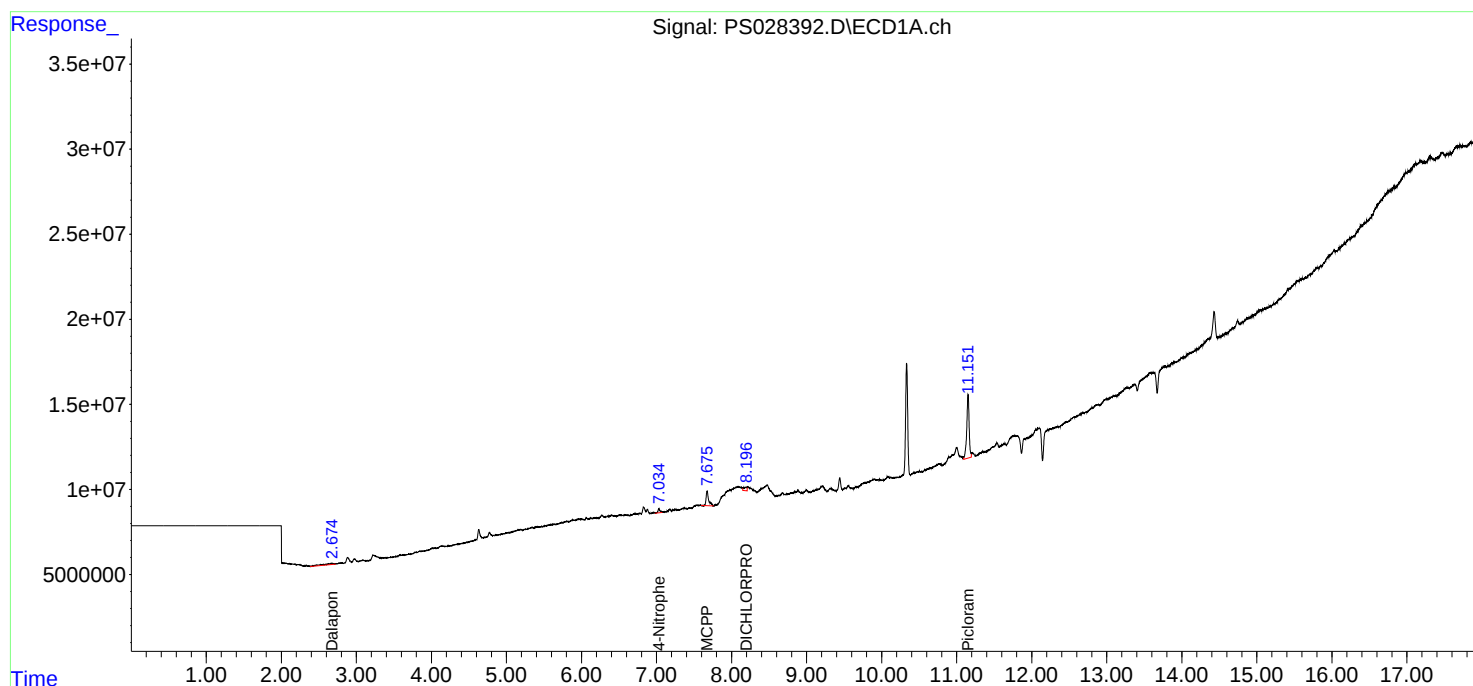


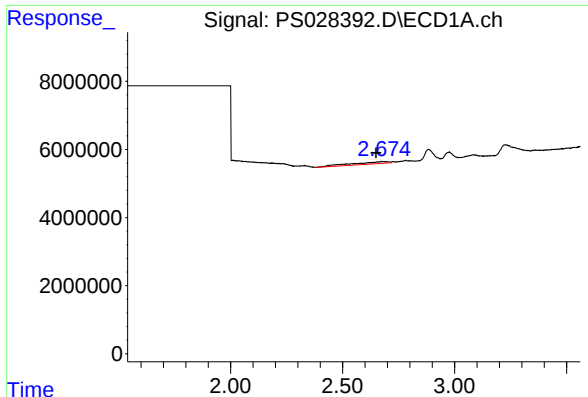

#1 Dalapon


R.T.: 2.676 min
Delta R.T.: 0.026 min
Response: 7331074
Conc: 2.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

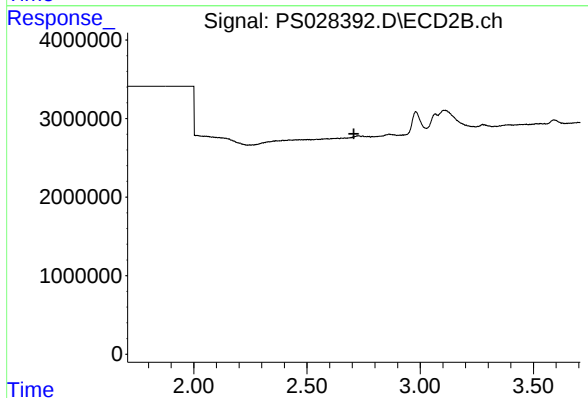


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.707 min
Response: 0
Conc: N.D.

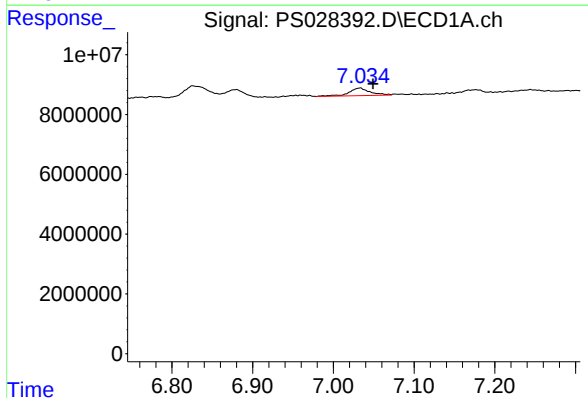


#3 4-Nitrophenol

R.T.: 7.032 min
Delta R.T.: -0.017 min
Response: 4706373
Conc: 2.54 ng/ml

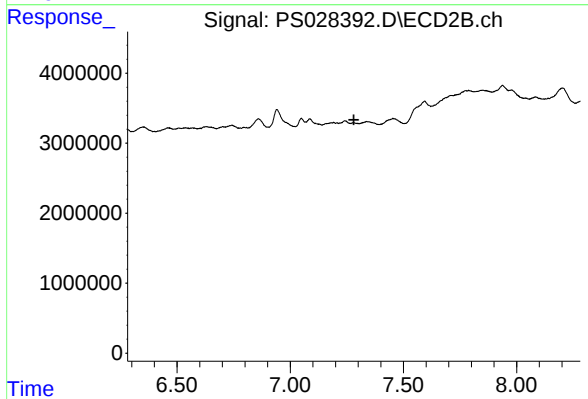

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.281 min
Response: 0
Conc: N.D.

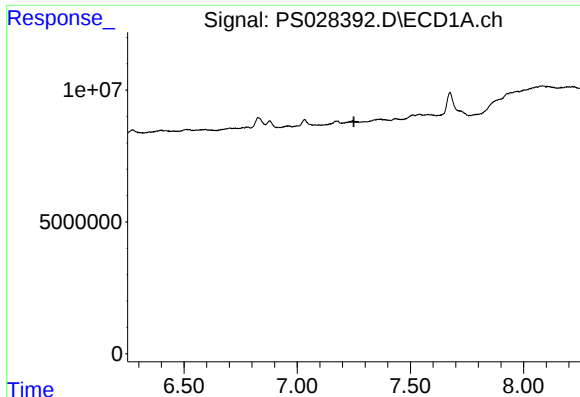

#4 2,4-DCAA


R.T.: 7.245 min
Delta R.T.: -0.005 min
Response: -799220
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

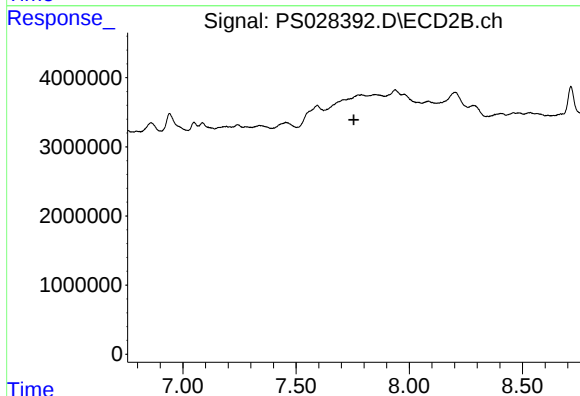


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.755 min
Response: 0
Conc: N.D.

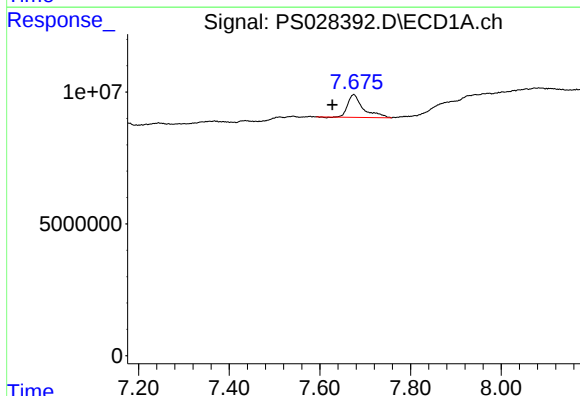


#6 MCPP

R.T.: 7.675 min
Delta R.T.: 0.047 min
Response: 20432388
Conc: 2.50 ug/ml

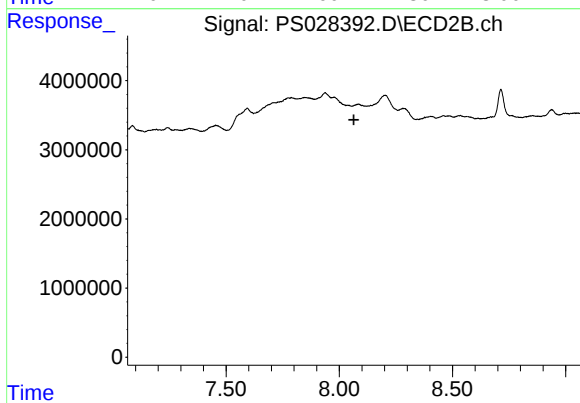

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.

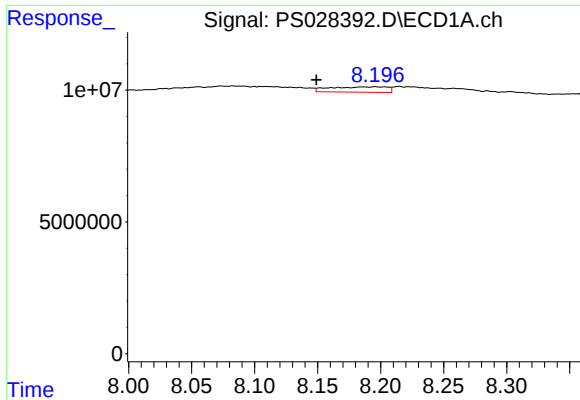

#8 DICHLORPROP


R.T.: 8.197 min
Delta R.T.: 0.048 min
Response: 6381013
Conc: 2.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

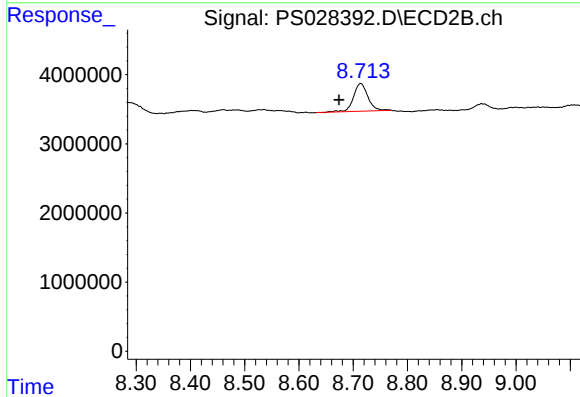


#8 DICHLORPROP

R.T.: 8.714 min
Delta R.T.: 0.040 min
Response: 7499852
Conc: 4.21 ng/ml

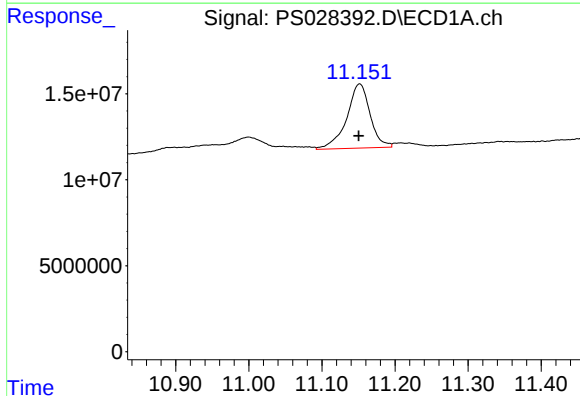


#15 Picloram

R.T.: 11.152 min
Delta R.T.: 0.001 min
Response: 83092812
Conc: 2.65 ng/ml

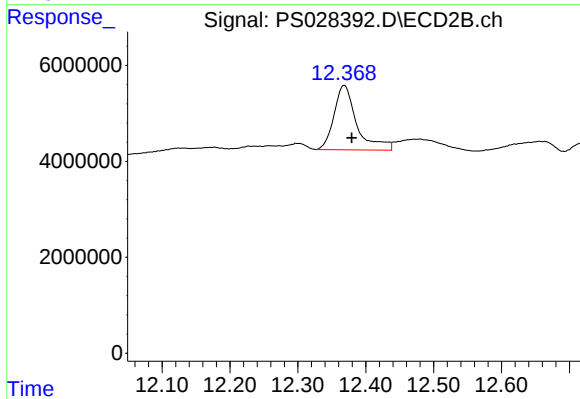

#15 Picloram


R.T.: 12.368 min
Delta R.T.: -0.011 min
Response: 31313056
Conc: 2.18 ng/ml

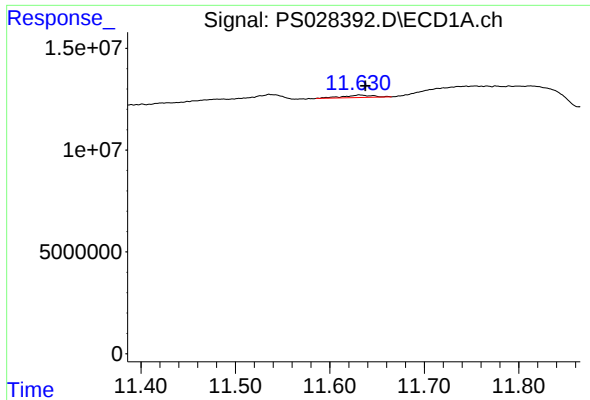

#16 DCPA

R.T.: 11.632 min
Delta R.T.: -0.006 min
Response: 2577229
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

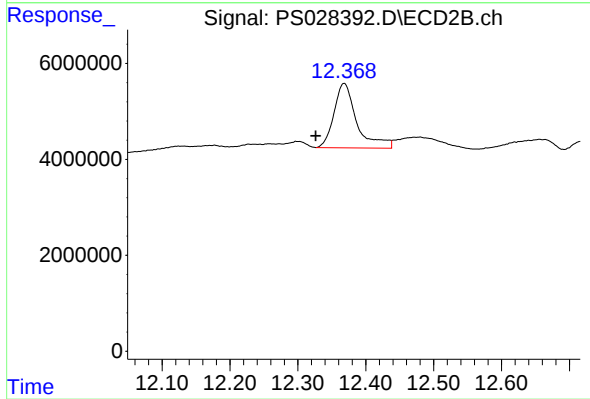

#16 DCPA

R.T.: 12.368 min
Delta R.T.: 0.042 min
Response: 31313056
Conc: 2.79 ng/ml